

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050522\
 Data File : PP047085.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2022 02:58
 Operator : YP\AJ
 Sample : N2654-01 10X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 ROOF-FLASHING-CAULK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 15:48:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 06 10:17:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.856	3.121	5695192	9436839	2.359	2.877
2) SA Decachlor...	9.924	8.429	4446261	4911852	3.022	2.059 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050522\
Data File : PP047085.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2022 02:58
Operator : YP\AJ
Sample : N2654-01 10X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
ROOF-FLASHING-CAULK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 15:48:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 06 10:17:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

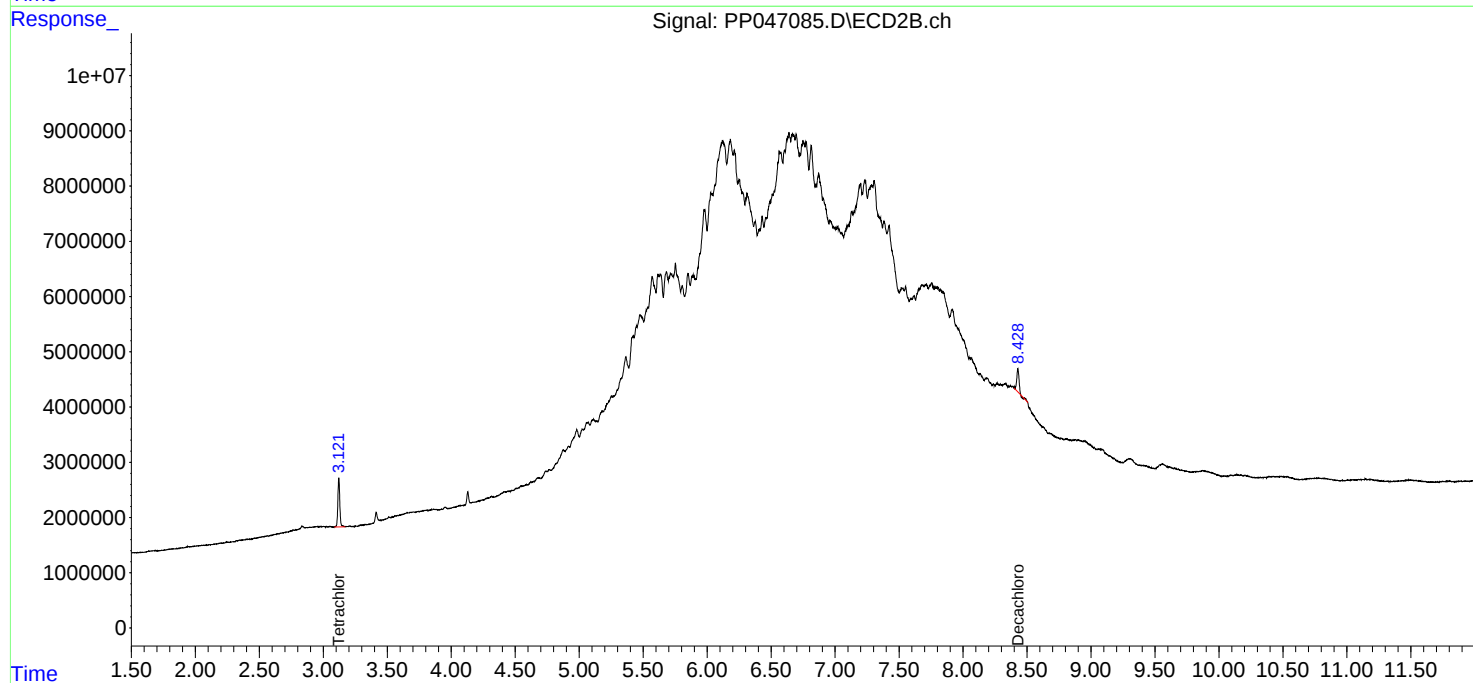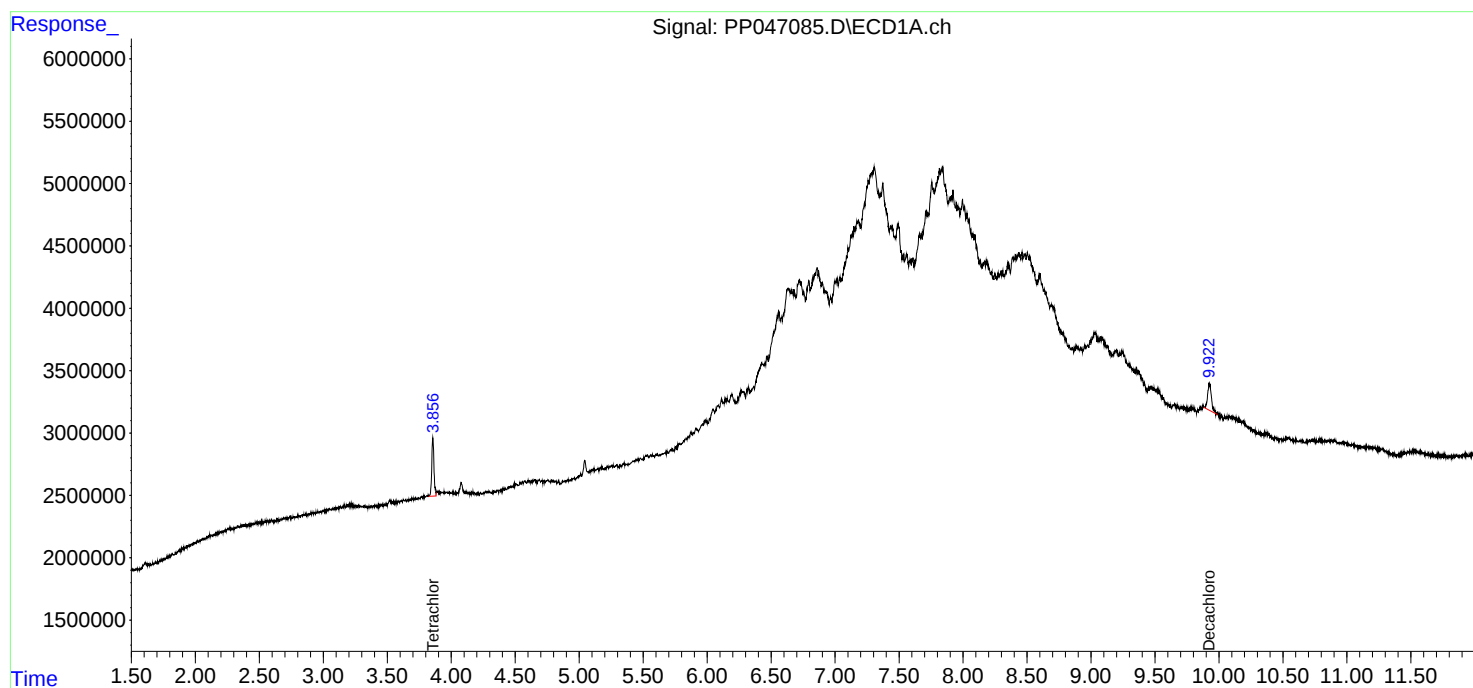


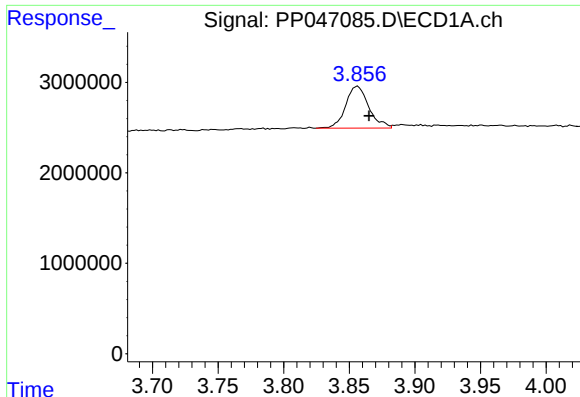

#1 Tetrachloro-m-xylene


R.T.: 3.856 min
Delta R.T.: -0.009 min
Response: 5695192
Conc: 2.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
ROOF-FLASHING-CAULK

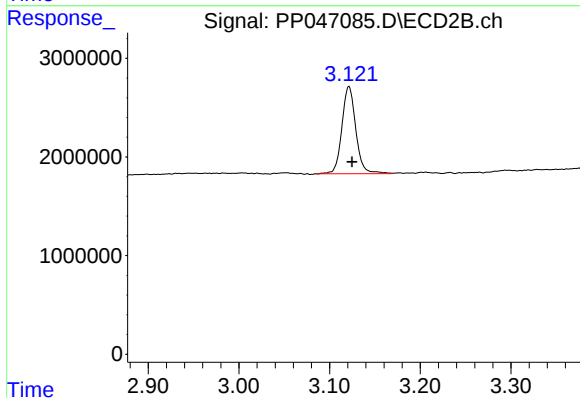


#1 Tetrachloro-m-xylene

R.T.: 3.121 min
Delta R.T.: -0.003 min
Response: 9436839
Conc: 2.88 ng/ml

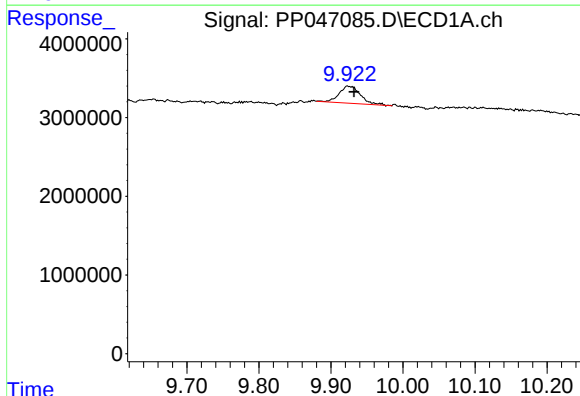

#2 Decachlorobiphenyl

R.T.: 9.924 min
Delta R.T.: -0.008 min
Response: 4446261
Conc: 3.02 ng/ml

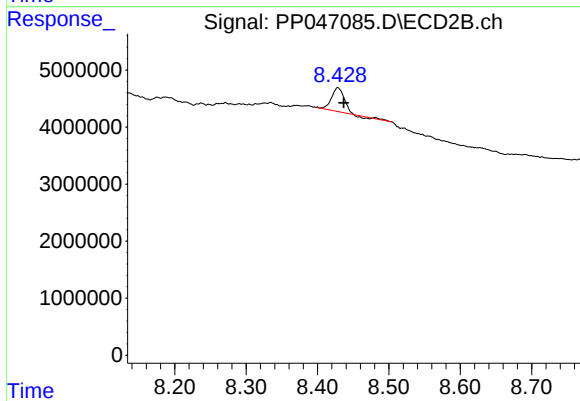

#2 Decachlorobiphenyl

R.T.: 8.429 min
Delta R.T.: -0.008 min
Response: 4911852
Conc: 2.06 ng/ml