

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050522\
 Data File : PP047086.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2022 03:14
 Operator : YP\AJ
 Sample : N2654-02 10X
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 ROOF-SOFFIT-CAULK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 15:48:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 06 10:17:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.857	3.121	6270162	9914460	2.597	3.022
2) SA Decachlor...	9.926	8.431	3621870	6988339	2.461	2.930

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050522\
Data File : PP047086.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2022 03:14
Operator : YP\AJ
Sample : N2654-02 10X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
ROOF-SOFFIT-CAULK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 15:48:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 06 10:17:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

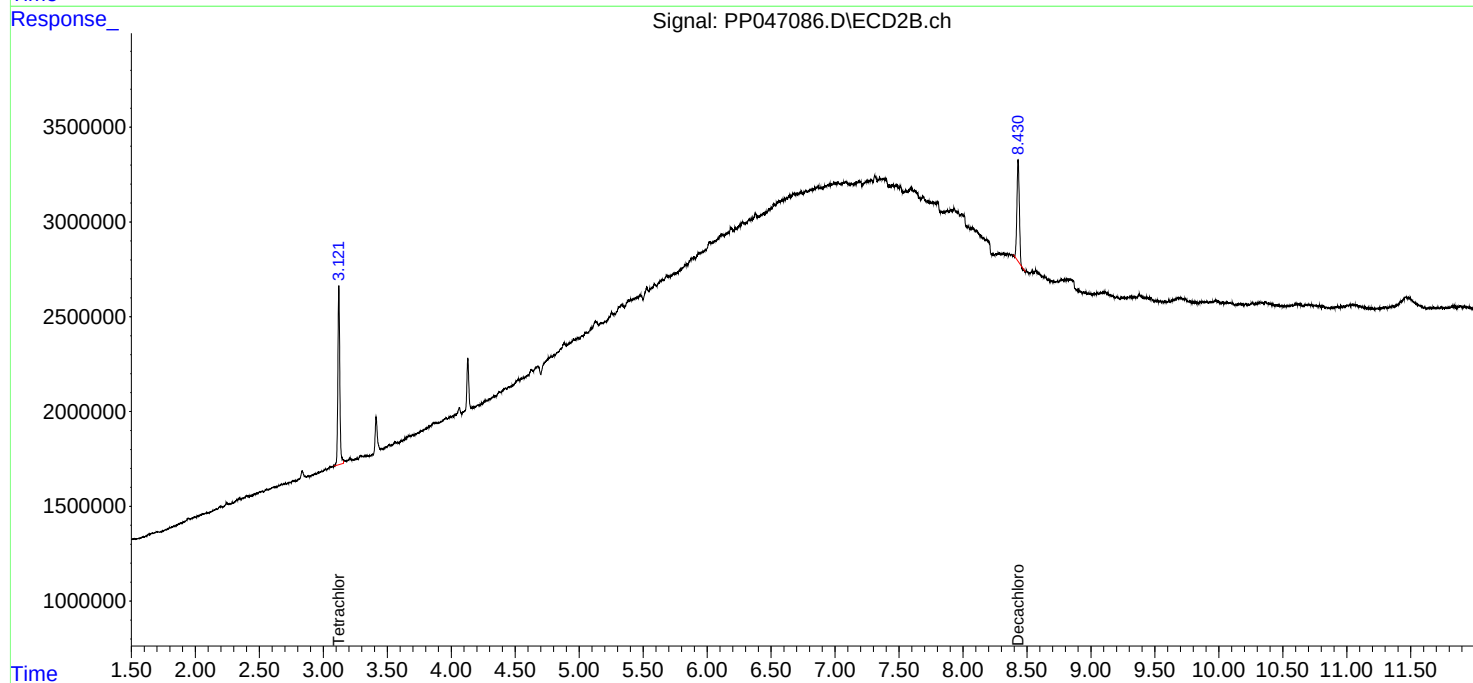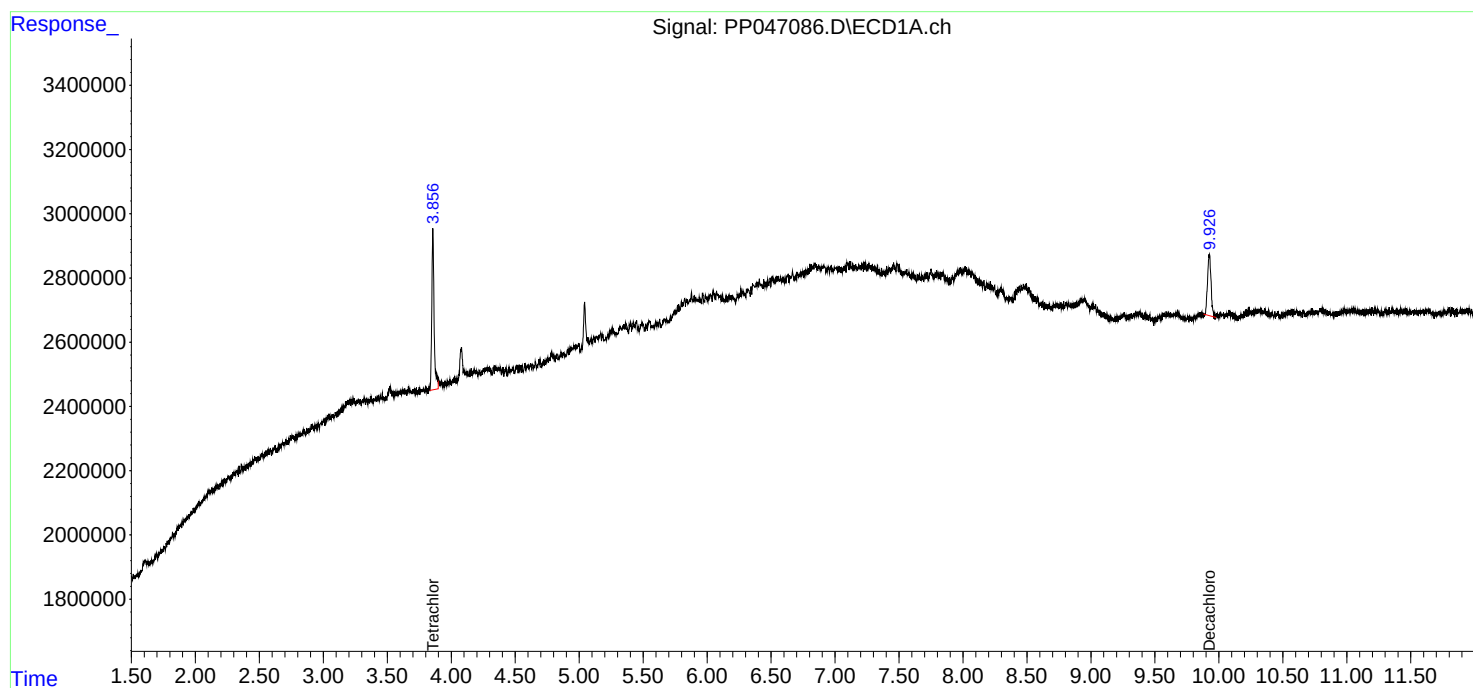


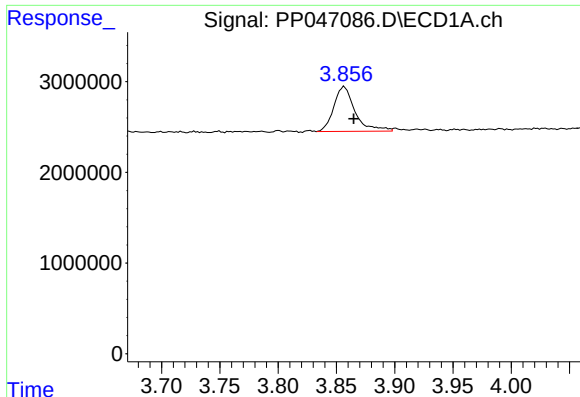

#1 Tetrachloro-m-xylene


R.T.: 3.857 min
Delta R.T.: -0.008 min
Response: 6270162
Conc: 2.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
ROOF-SOFFIT-CAULK

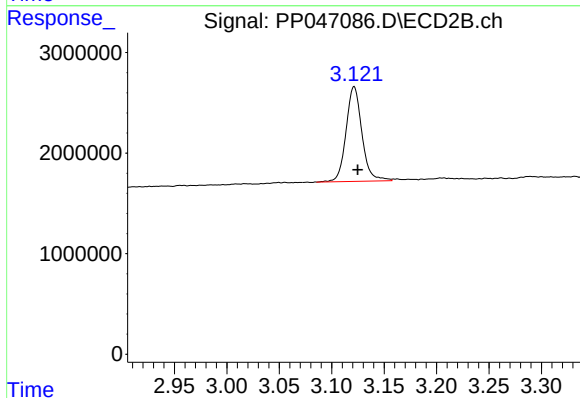


#1 Tetrachloro-m-xylene

R.T.: 3.121 min
Delta R.T.: -0.003 min
Response: 9914460
Conc: 3.02 ng/ml

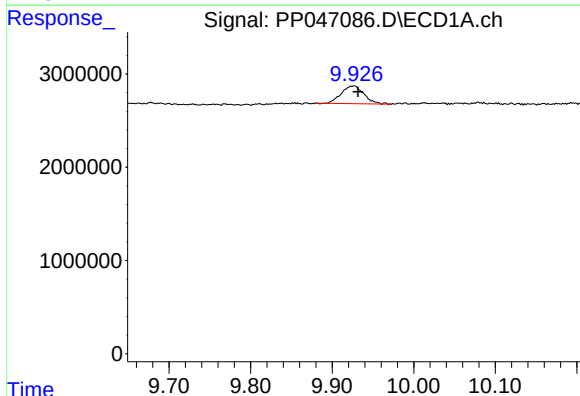

#2 Decachlorobiphenyl

R.T.: 9.926 min
Delta R.T.: -0.006 min
Response: 3621870
Conc: 2.46 ng/ml

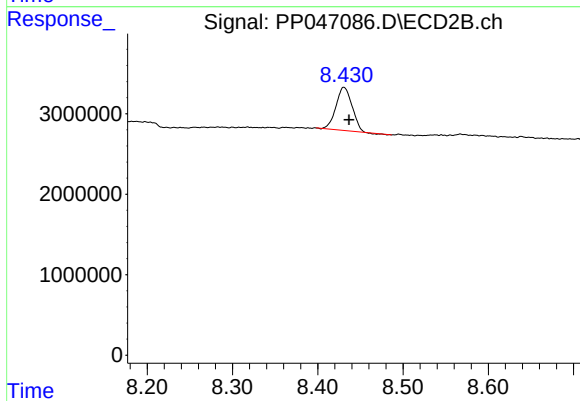

#2 Decachlorobiphenyl

R.T.: 8.431 min
Delta R.T.: -0.006 min
Response: 6988339
Conc: 2.93 ng/ml