

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050522\
 Data File : PP047092.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2022 06:10
 Operator : YP\AJ
 Sample : N2654-03 10X
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DUCT-PUTTY

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/09/2022
 Supervised By :mohammad ahmed 05/09/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 15:50:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 06 10:17:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.854	3.123	1425971	9952863	0.591m	3.034m#
2) SA Decachlor...	9.918	8.431	2280422	4860578	1.550	2.038 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050522\
Data File : PP047092.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2022 06:10
Operator : YP\AJ
Sample : N2654-03 10X
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
DUCT-PUTTY


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/09/2022
Supervised By :mohammad ahmed 05/09/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 15:50:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 06 10:17:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

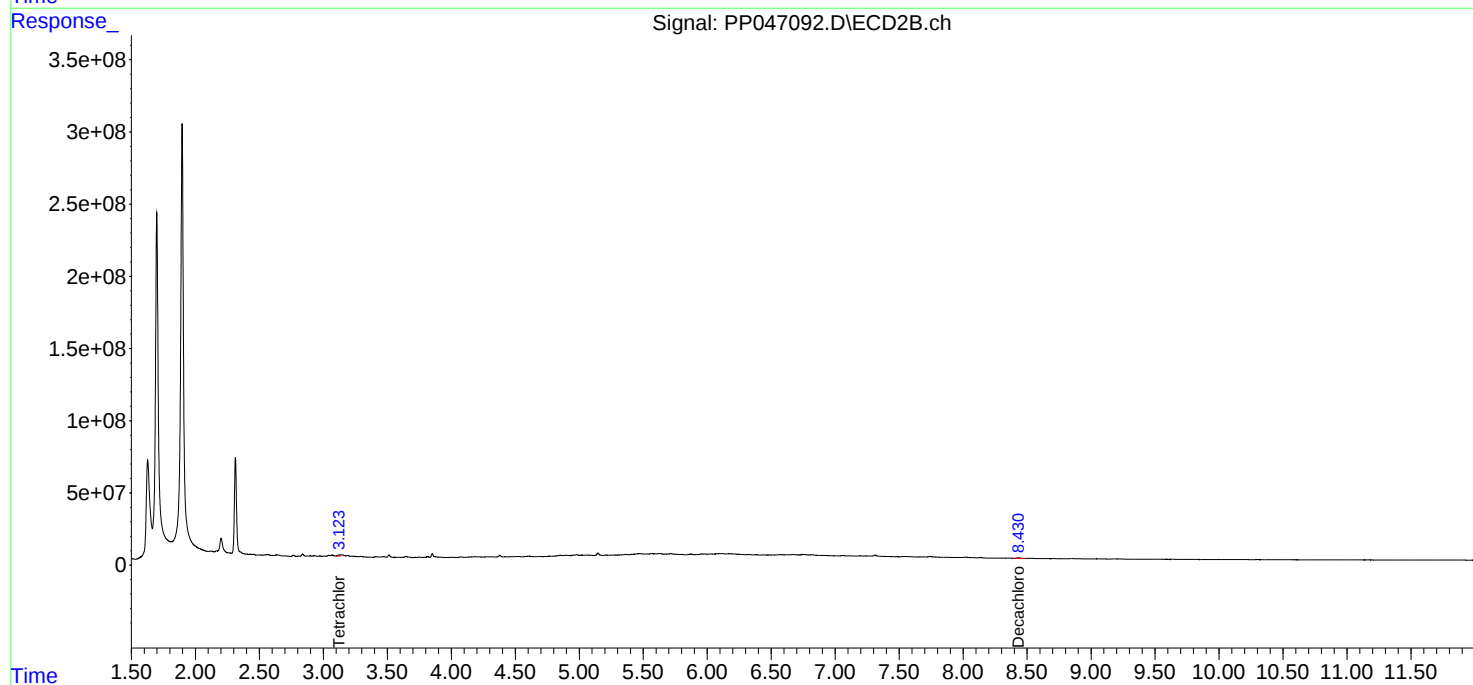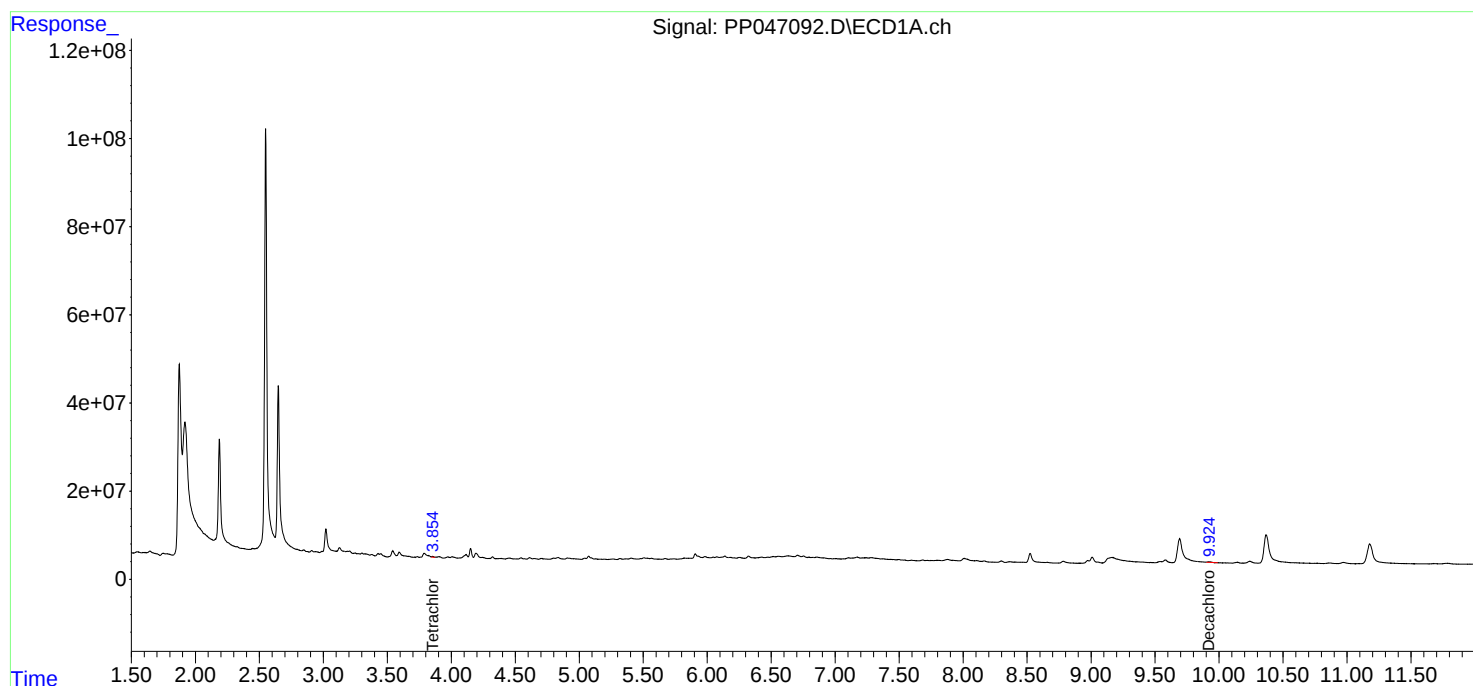

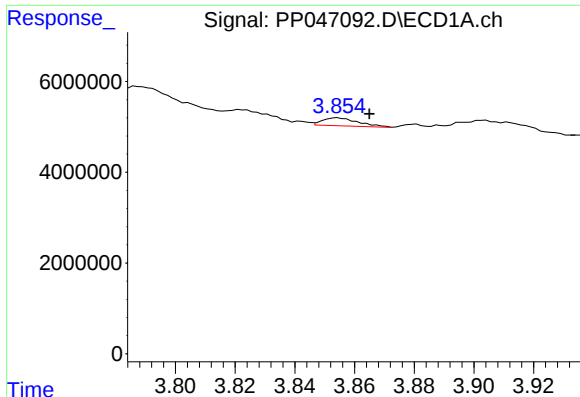


#1 Tetrachloro-m-xylene

R.T.: 3.854 min
Delta R.T.: -0.011 min
Response: 1425971
Conc: 0.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
DUCT-PUTTY


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/09/2022
Supervised By :mohammad ahmed 05/09/2022

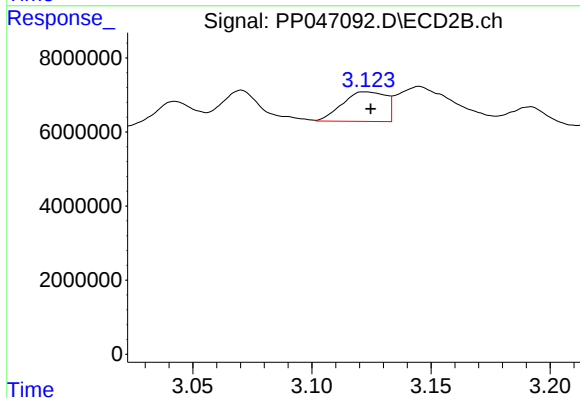


#1 Tetrachloro-m-xylene

R.T.: 3.123 min
Delta R.T.: -0.002 min
Response: 9952863
Conc: 3.03 ng/ml m

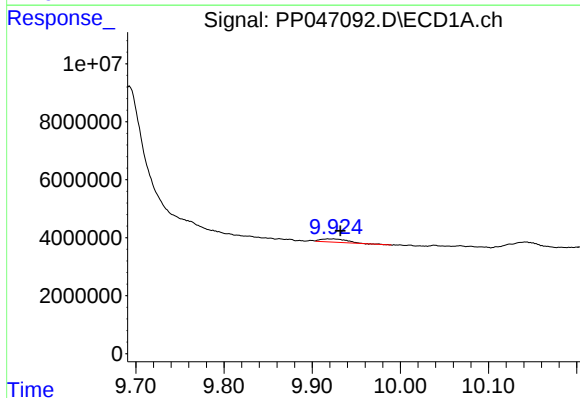

#2 Decachlorobiphenyl

R.T.: 9.918 min
Delta R.T.: -0.014 min
Response: 2280422
Conc: 1.55 ng/ml

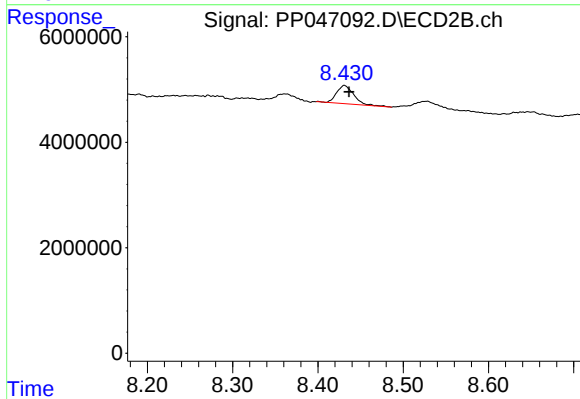

#2 Decachlorobiphenyl

R.T.: 8.431 min
Delta R.T.: -0.005 min
Response: 4860578
Conc: 2.04 ng/ml