

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051719\
 Data File : PP030197.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 May 2019 7:17
 Operator : EI/SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 23:13:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051619.M
 Quant Title : 8080.M
 QLast Update : Thu May 16 19:05:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	#
15) T Picloram	16.939	0.000	27980470	0	5.934	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051719\
Data File : PP030197.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 May 2019 7:17
Operator : EI/SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 23:13:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051619.M
Quant Title : 8080.M
QLast Update : Thu May 16 19:05:31 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

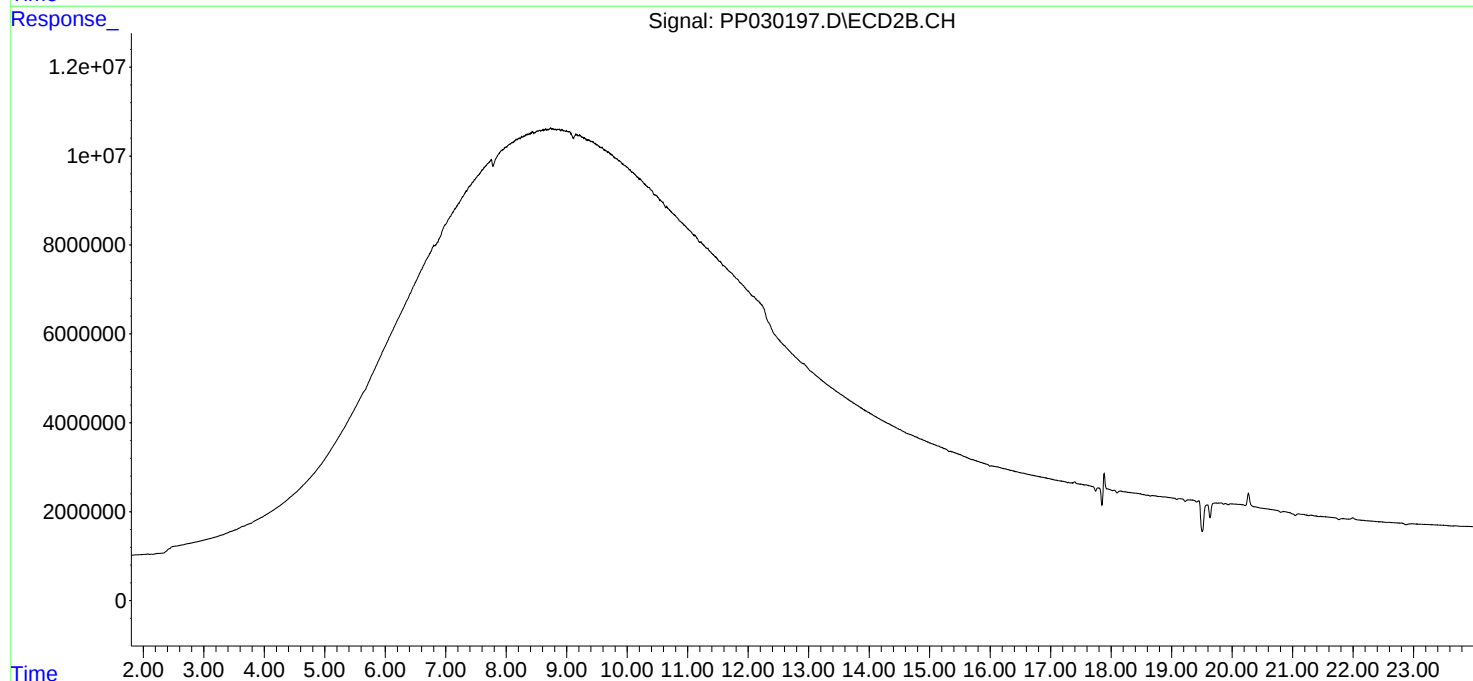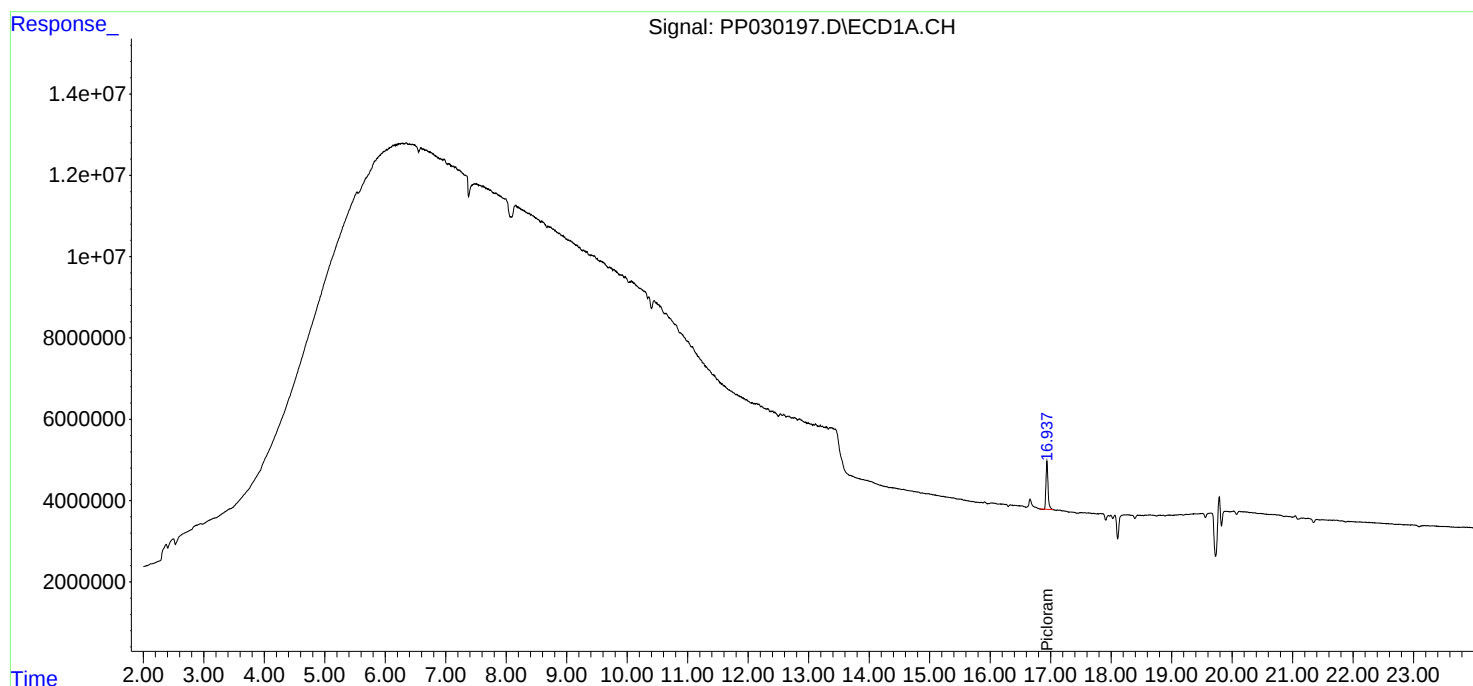


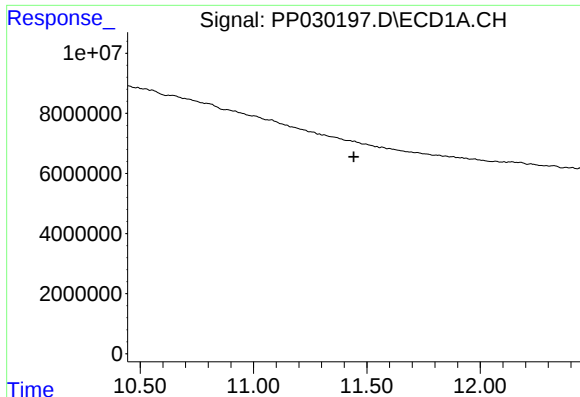

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 11.443 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

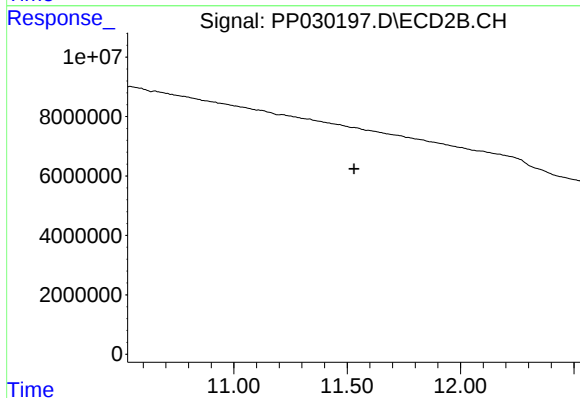


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 11.530 min
Response: 0
Conc: N.D.

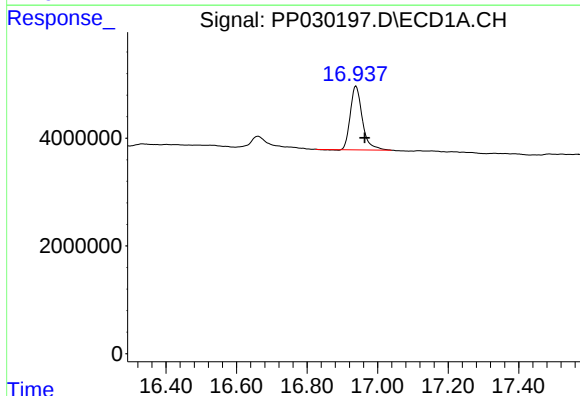

#15 Picloram

R.T.: 16.939 min
Delta R.T.: -0.024 min
Response: 27980470
Conc: 5.93 ng/ml

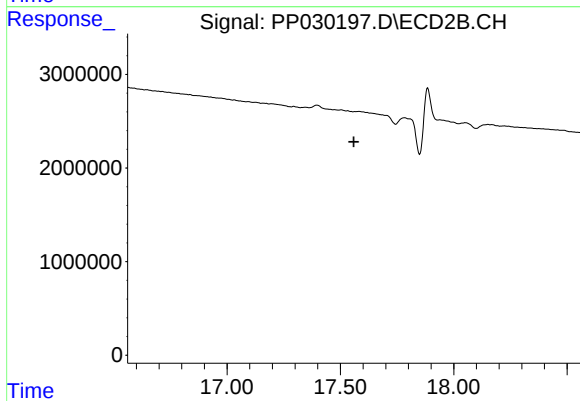

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 17.559 min
Response: 0
Conc: N.D.