

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051719\
 Data File : PP030214.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 May 2019 16:45
 Operator : EI/SJ
 Sample : K2865-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP-21-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 23:15:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051619.M
 Quant Title : 8080.M
 QLast Update : Thu May 16 19:05:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.439	11.526	225.7E6	154.0E6	387.904	347.260
Target Compounds							
8) T	DICHLORPROP	0.000	12.903	0	11087184	N.D.	25.517 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051719\
Data File : PP030214.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 May 2019 16:45
Operator : EI/SJ
Sample : K2865-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
TP-21-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 23:15:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051619.M
Quant Title : 8080.M
QLast Update : Thu May 16 19:05:31 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

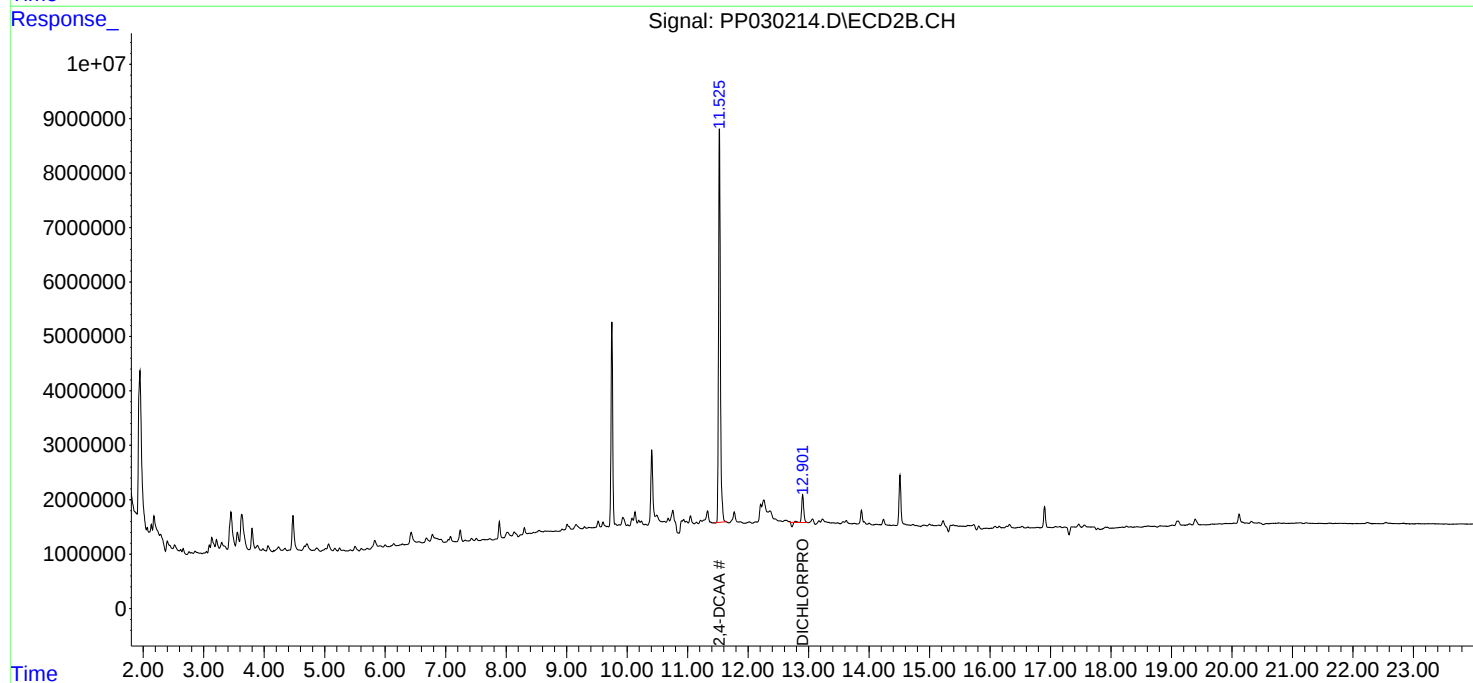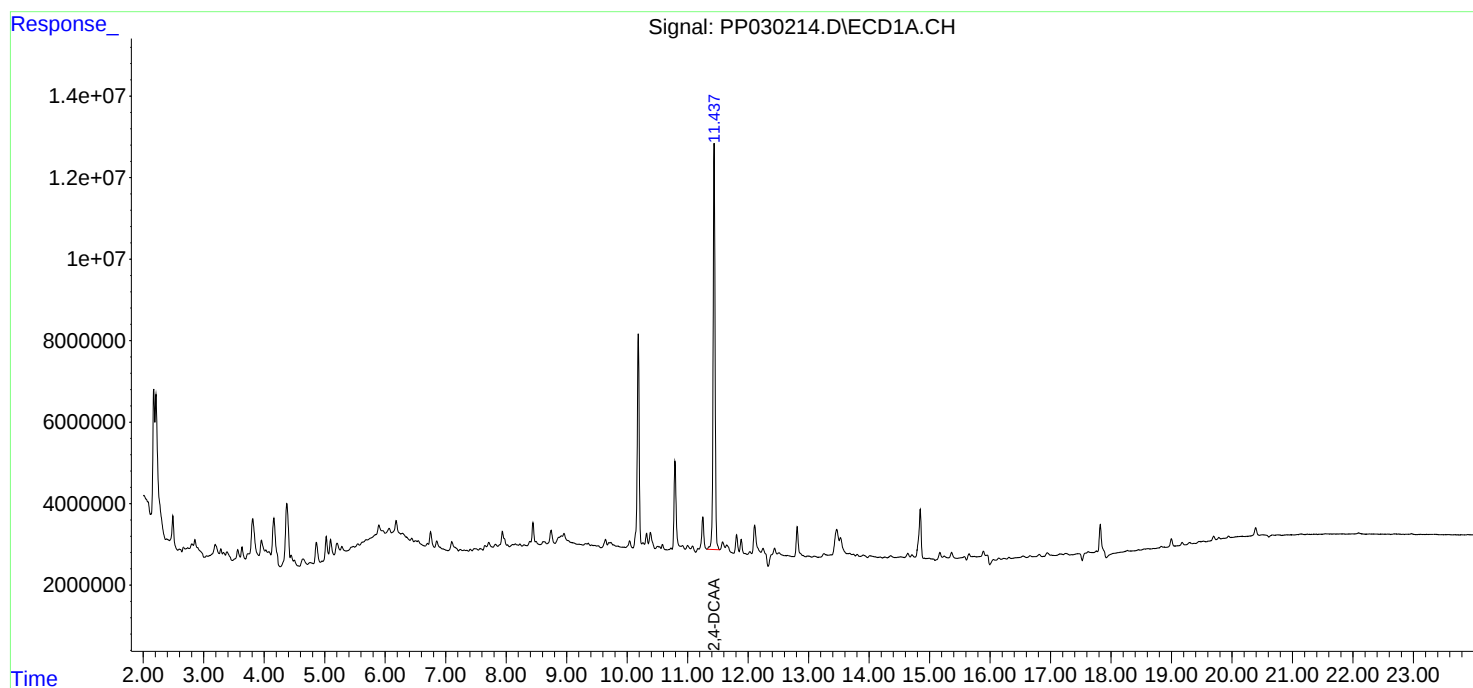


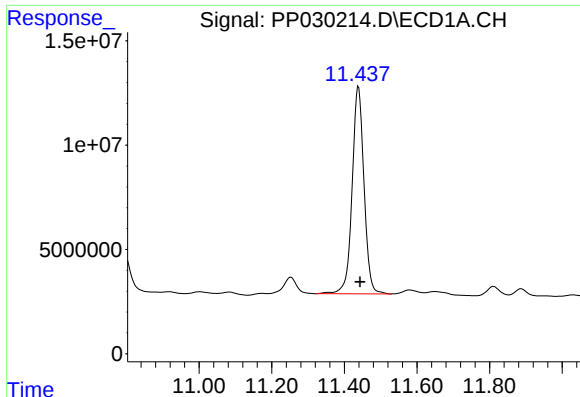

#4 2,4-DCAA


R.T.: 11.439 min
Delta R.T.: -0.004 min
Response: 225657242
Conc: 387.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-21-S

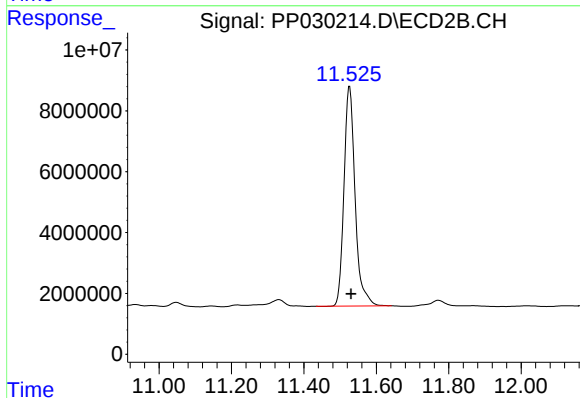


#4 2,4-DCAA

R.T.: 11.526 min
Delta R.T.: -0.004 min
Response: 153988439
Conc: 347.26 ng/ml

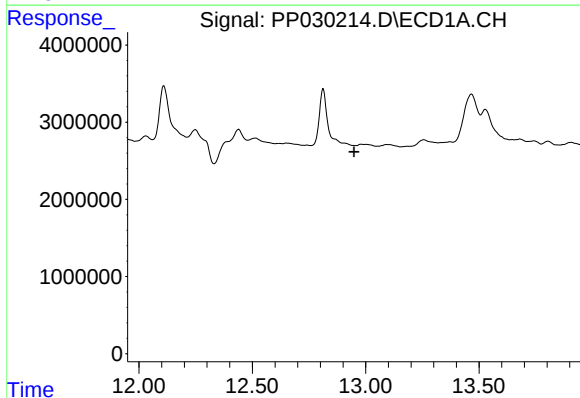

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.949 min
Response: 0
Conc: N.D.

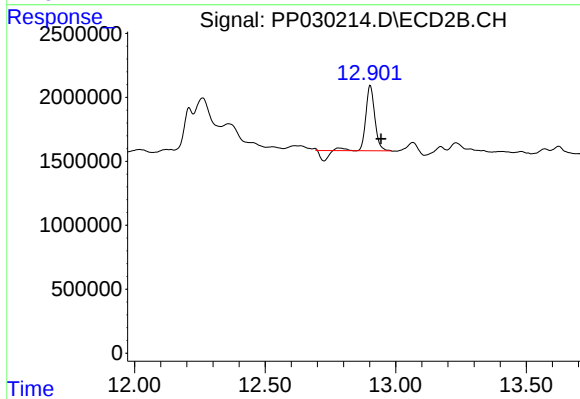

#8 DICHLORPROP

R.T.: 12.903 min
Delta R.T.: -0.041 min
Response: 11087184
Conc: 25.52 ng/ml