

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052623\
 Data File : PP057984.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2023 15:31
 Operator : YP\AJ
 Sample : 02948-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 01-A-01-B-01-C

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/30/2023
 Supervised By :Ankita Jodhani 05/30/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 21:34:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 08 19:18:05 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.380	3.619	57707944	56150639	26.305	24.754m
2) SA Decachlor...	10.204	8.677	30010881	36785919	26.482	23.434

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052623\
Data File : PP057984.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2023 15:31
Operator : YP\AJ
Sample : 02948-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
01-A-01-B-01-C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/30/2023
Supervised By :Ankita Jodhani 05/30/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 21:34:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050823.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 08 19:18:05 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

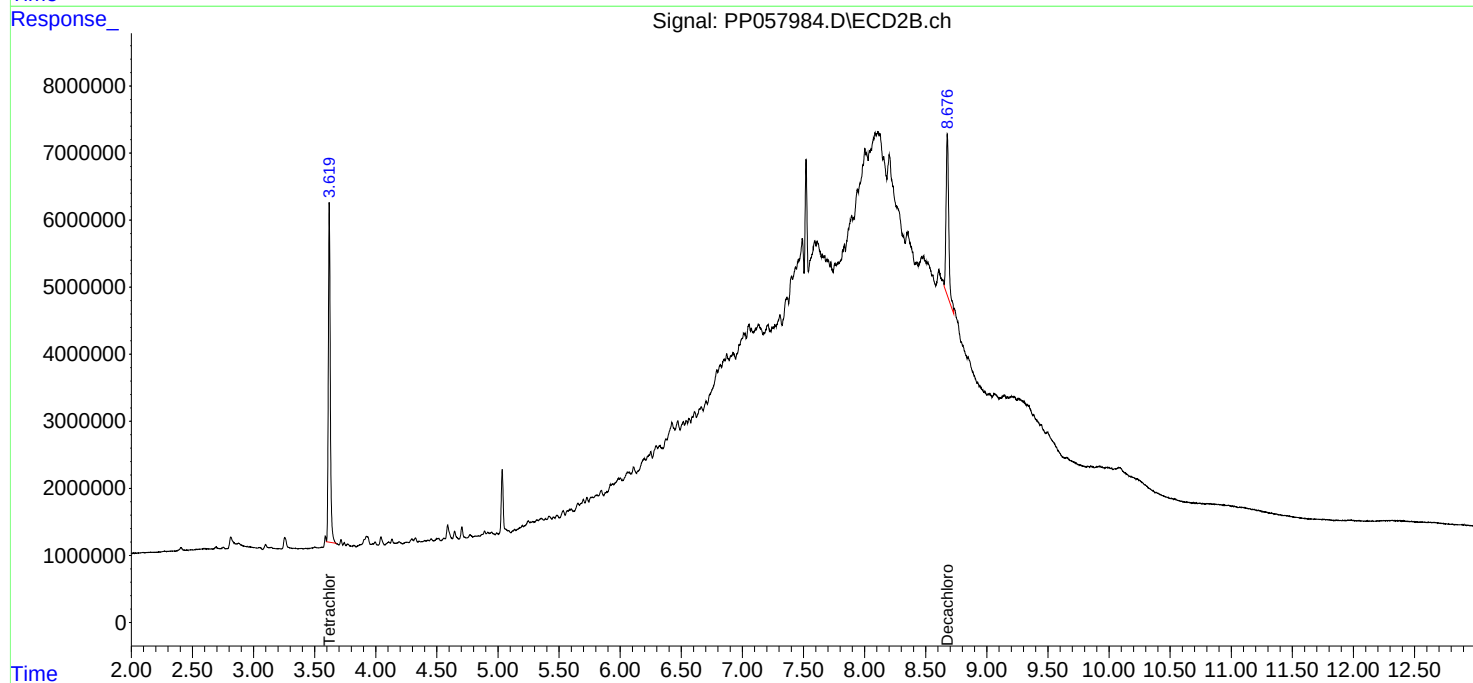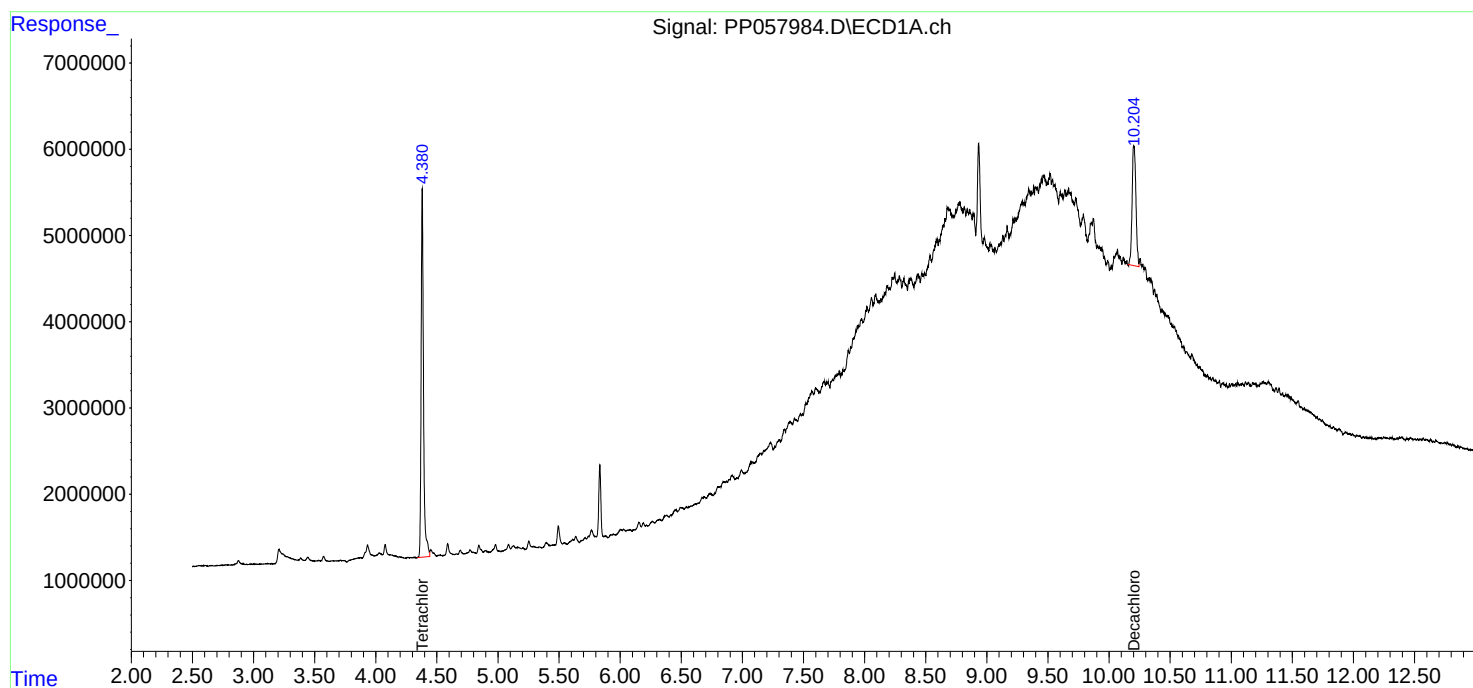

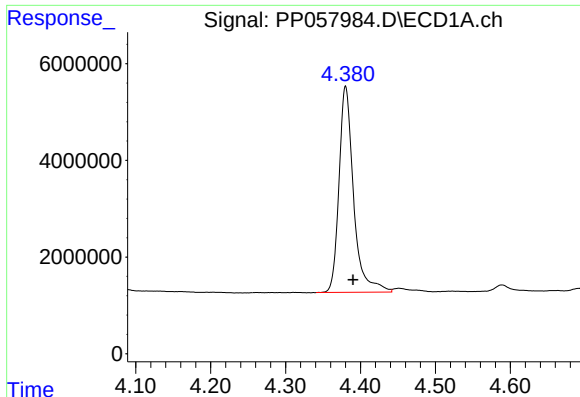


#1 Tetrachloro-m-xylene

R.T.: 4.380 min
Delta R.T.: -0.010 min
Response: 57707944
Conc: 26.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
01-A-01-B-01-C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/30/2023
Supervised By :Ankita Jodhani 05/30/2023

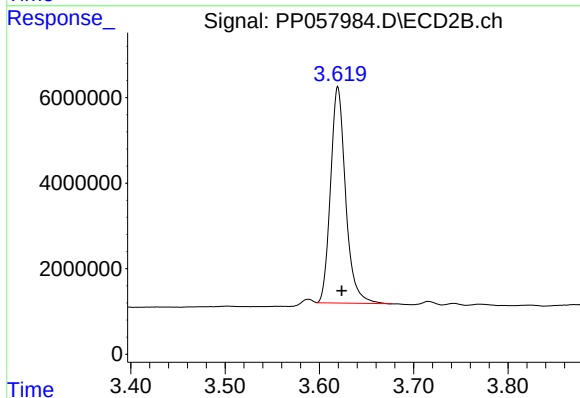


#1 Tetrachloro-m-xylene

R.T.: 3.619 min
Delta R.T.: -0.004 min
Response: 56150639
Conc: 24.75 ng/ml m

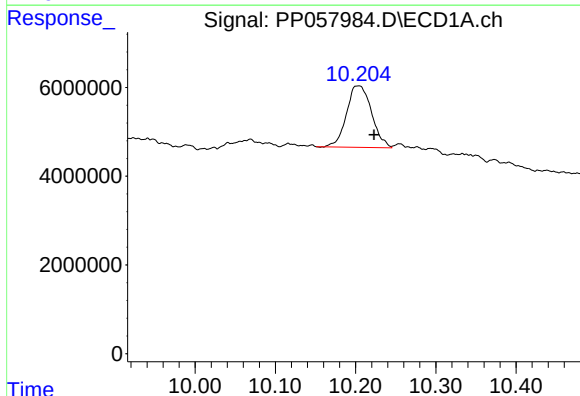

#2 Decachlorobiphenyl

R.T.: 10.204 min
Delta R.T.: -0.019 min
Response: 30010881
Conc: 26.48 ng/ml

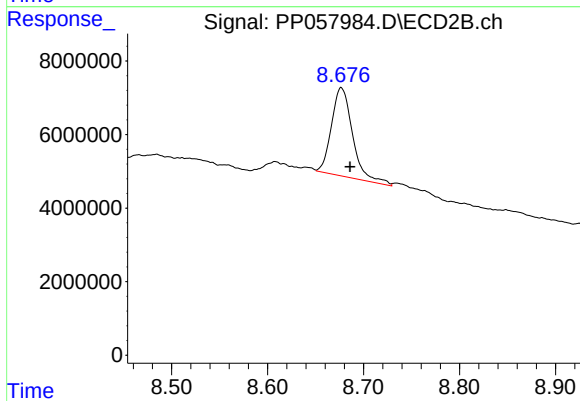

#2 Decachlorobiphenyl

R.T.: 8.677 min
Delta R.T.: -0.009 min
Response: 36785919
Conc: 23.43 ng/ml