

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP052822\  
 Data File : PP048190.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 28 May 2022 22:55  
 Operator : YP\AJ  
 Sample : N3099-03  
 Misc :  
 ALS Vial : 41 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 20220426-AMENDED-COMPOSITE-F

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 29 05:58:05 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP052722.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri May 27 23:53:39 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml  |
|-----------------------------|--------|-------|----------|----------|--------|--------|
| -----                       |        |       |          |          |        |        |
| System Monitoring Compounds |        |       |          |          |        |        |
| 1) SA Tetrachlo...          | 4.037  | 3.218 | 40224456 | 34581576 | 17.177 | 17.547 |
| 2) SA Decachlor...          | 10.390 | 8.655 | 19146325 | 16326823 | 9.851  | 10.100 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP052822\  
Data File : PP048190.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 28 May 2022 22:55  
Operator : YP\AJ  
Sample : N3099-03  
Misc :  
ALS Vial : 41 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
20220426-AMENDED-COMPOSITE-F

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: May 29 05:58:05 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP052722.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Fri May 27 23:53:39 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

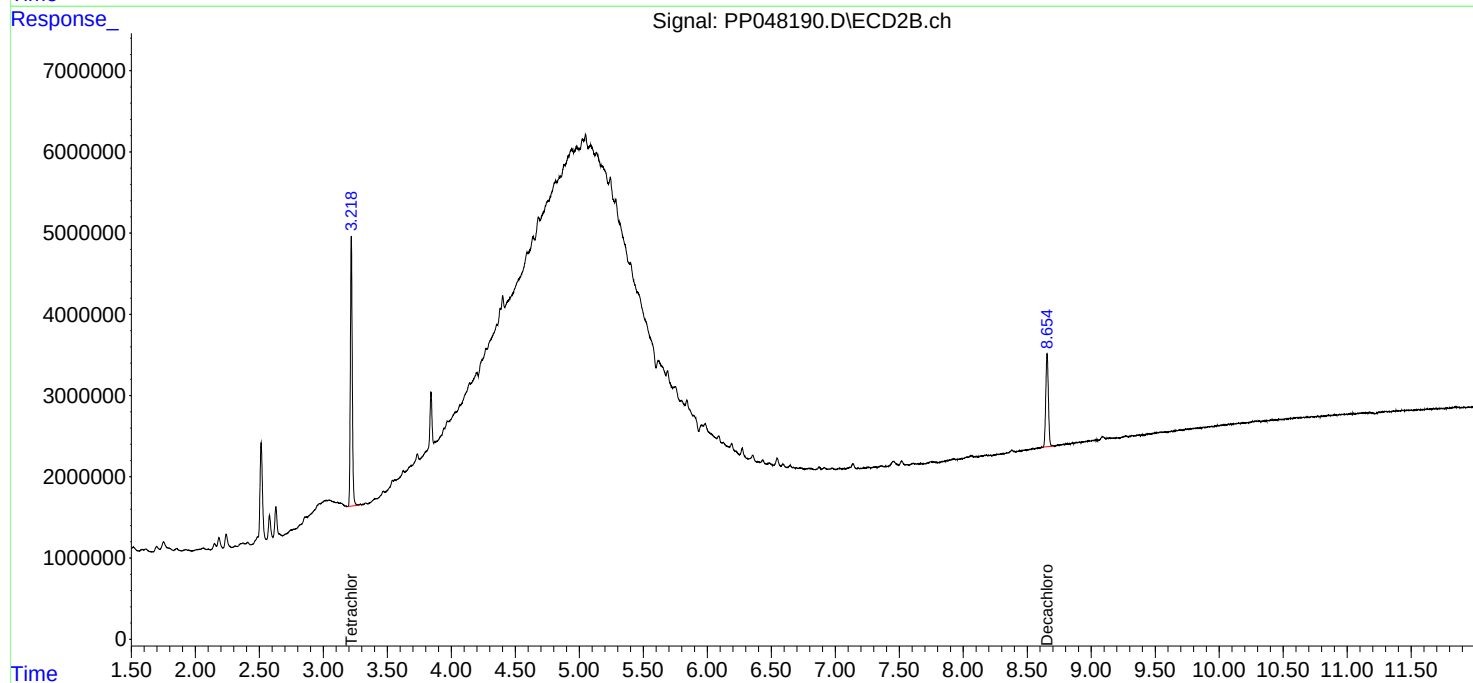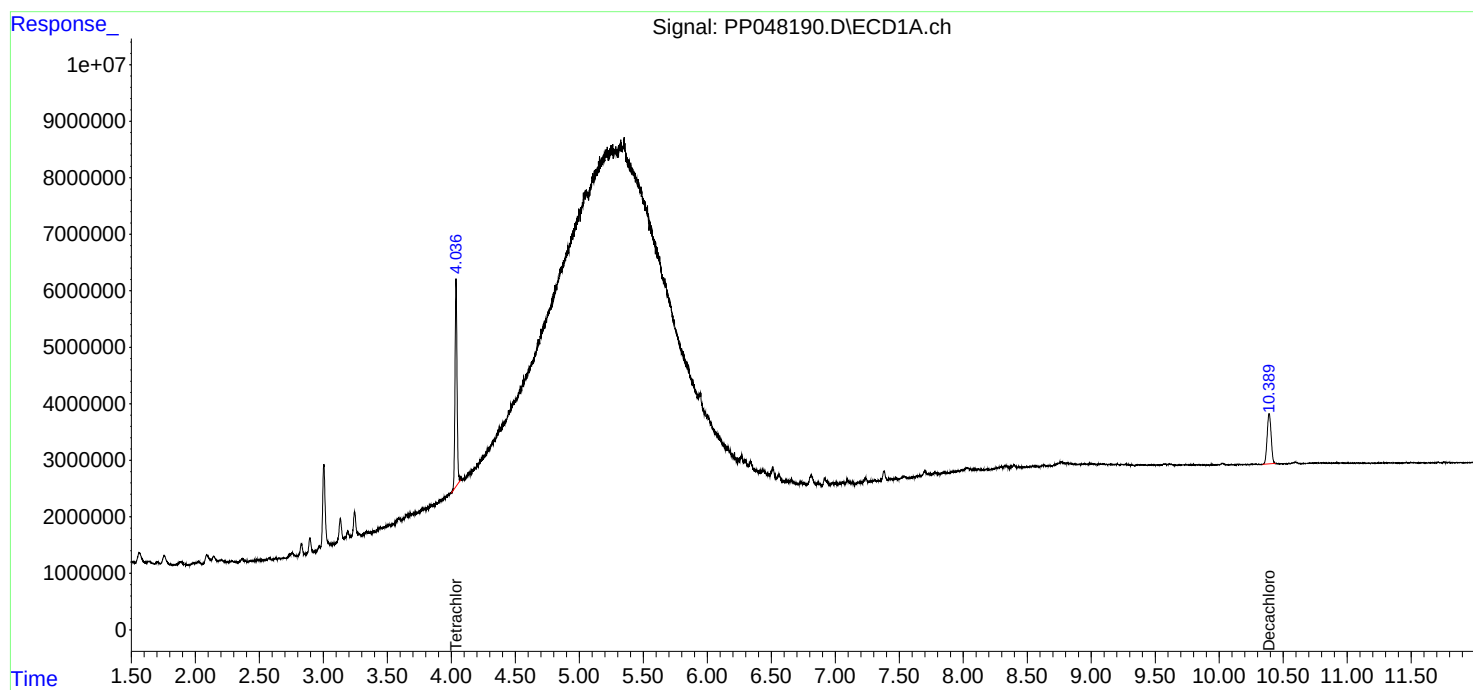


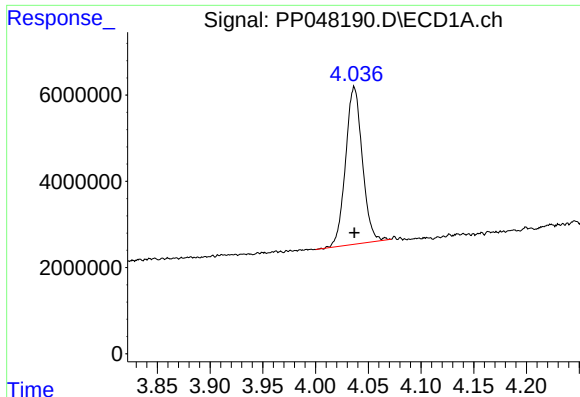

#1 Tetrachloro-m-xylene


R.T.: 4.037 min  
Delta R.T.: 0.000 min  
Response: 40224456  
Conc: 17.18 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
20220426-AMENDED-COMPOSITE-F

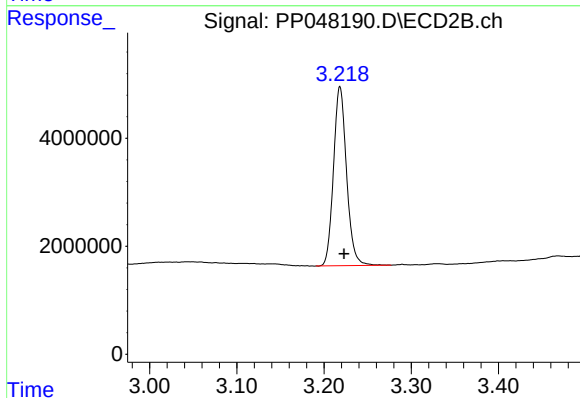


#1 Tetrachloro-m-xylene

R.T.: 3.218 min  
Delta R.T.: -0.005 min  
Response: 34581576  
Conc: 17.55 ng/ml

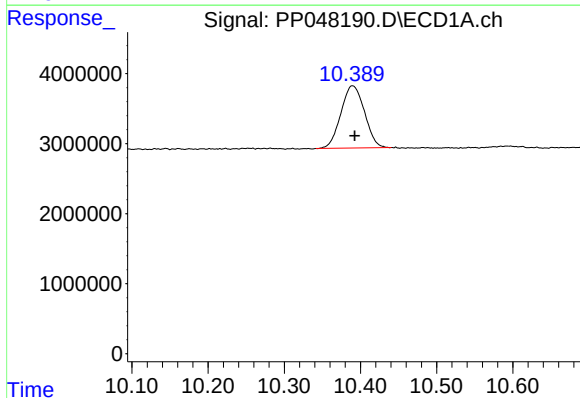

#2 Decachlorobiphenyl

R.T.: 10.390 min  
Delta R.T.: -0.003 min  
Response: 19146325  
Conc: 9.85 ng/ml

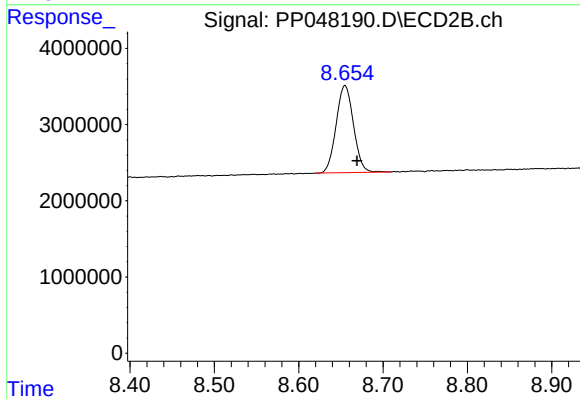

#2 Decachlorobiphenyl

R.T.: 8.655 min  
Delta R.T.: -0.014 min  
Response: 16326823  
Conc: 10.10 ng/ml