

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060822\
 Data File : PP048500.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2022 12:42
 Operator : YP\AJ
 Sample : N3162-14
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOS-B101-W1-(0-0.5)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 13:12:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 07 11:09:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.037	3.206	33169380	33049490	13.843	17.364 #
2) SA Decachlor...	10.388	8.626	27026890	17011450	14.180	13.892

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060822\
Data File : PP048500.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2022 12:42
Operator : YP\AJ
Sample : N3162-14
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOS-B101-W1-(0-0.5)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 13:12:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 07 11:09:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

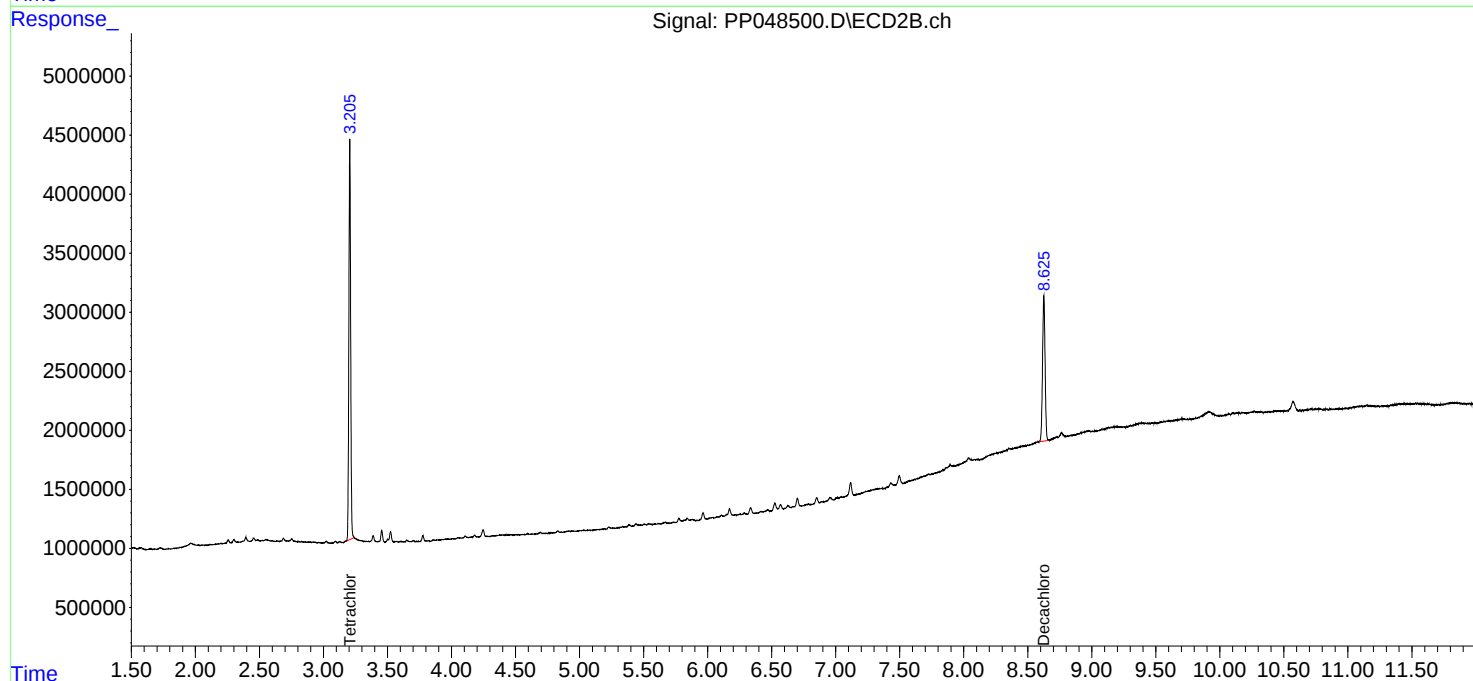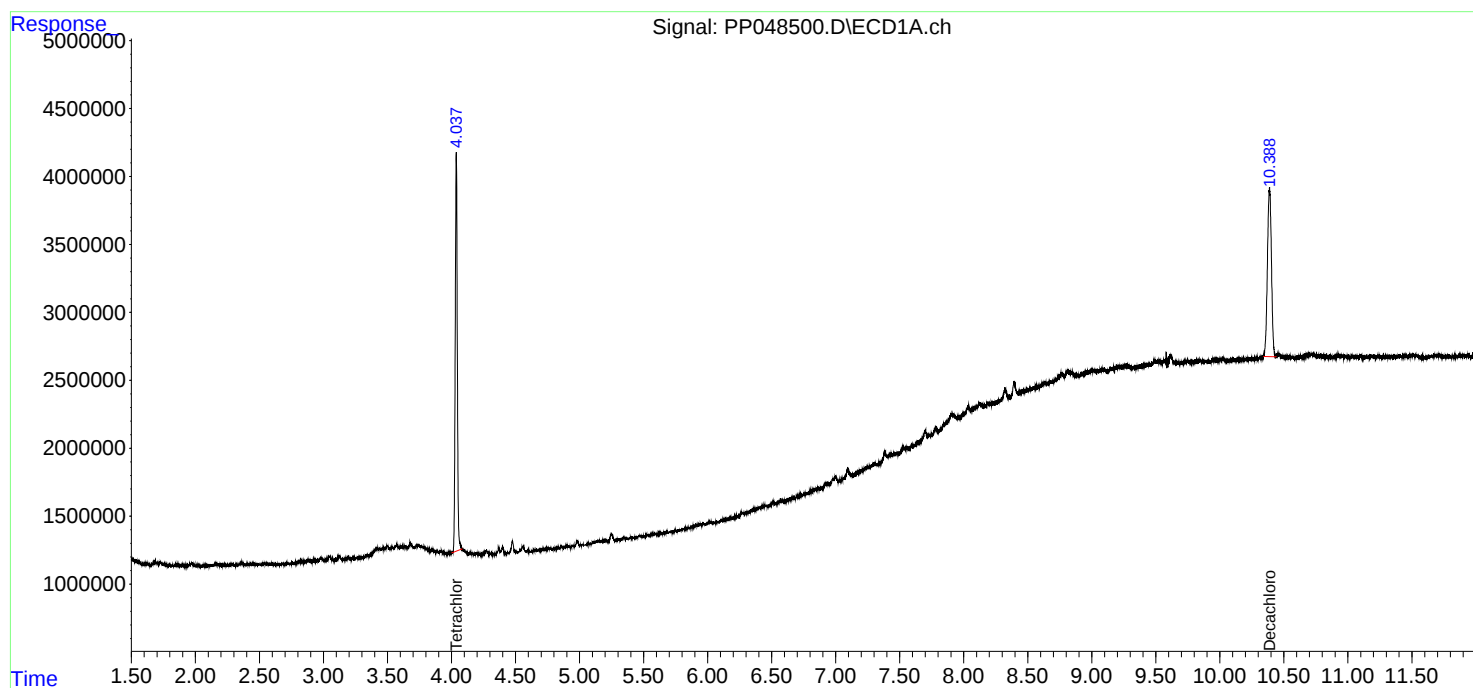


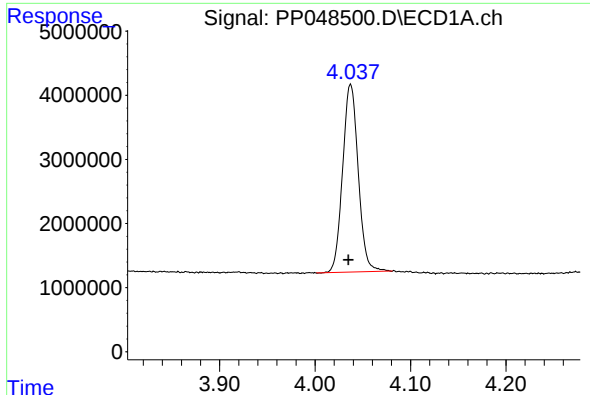

#1 Tetrachloro-m-xylene


R.T.: 4.037 min
Delta R.T.: 0.002 min
Response: 33169380
Conc: 13.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOS-B101-W1-(0-0.5)

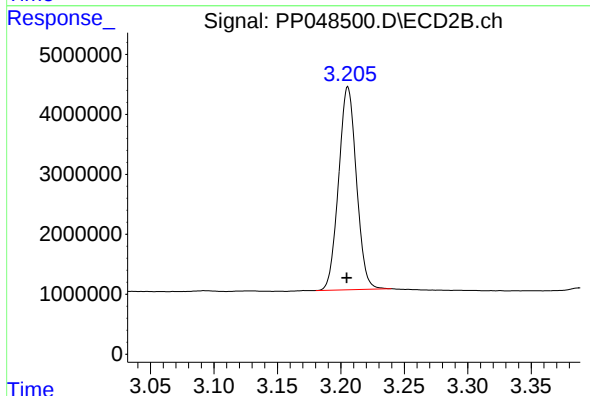


#1 Tetrachloro-m-xylene

R.T.: 3.206 min
Delta R.T.: 0.000 min
Response: 33049490
Conc: 17.36 ng/ml

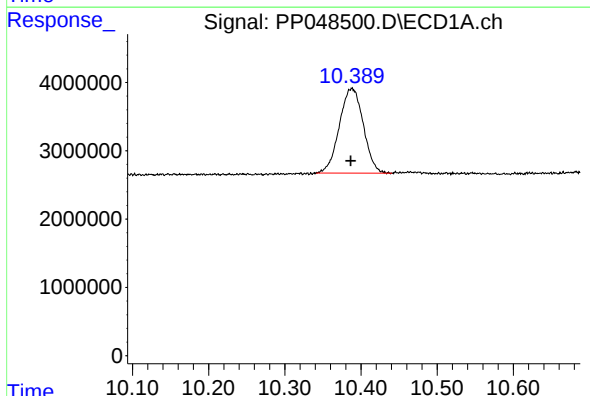

#2 Decachlorobiphenyl

R.T.: 10.388 min
Delta R.T.: 0.001 min
Response: 27026890
Conc: 14.18 ng/ml

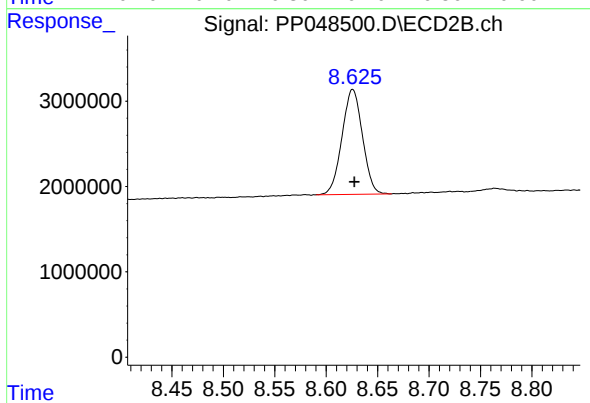

#2 Decachlorobiphenyl

R.T.: 8.626 min
Delta R.T.: -0.002 min
Response: 17011450
Conc: 13.89 ng/ml