

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060822\
 Data File : PP048547.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jun 2022 01:37
 Operator : YP\AJ
 Sample : N3175-01
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AUD-1552

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/08/2022
 Supervised By :Ankita Jodhani 06/08/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 03:21:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 07 11:09:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.034	3.203	51315029	42377954	21.415	22.265
2) SA Decachlor...	10.383	8.618	41163280	34527339	21.597	28.196m#
Target Compounds						
26) L6 AR-1254-1	6.267	5.222	4576508	5747880	49.210	56.859
27) L6 AR-1254-2	6.505	5.383	7806996	3940777	56.283	44.755
28) L6 AR-1254-3	6.913	5.818	7905705	7670386	55.603	55.179
29) L6 AR-1254-4	7.231	6.068	6239771	5595249	58.554	64.523
30) L6 AR-1254-5	7.697	6.523	5071148	10996607	42.718	89.662 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060822\
Data File : PP048547.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jun 2022 01:37
Operator : YP\AJ
Sample : N3175-01
Misc :
ALS Vial : 46 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AUD-1552


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/08/2022
Supervised By :Ankita Jodhani 06/08/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 03:21:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 07 11:09:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

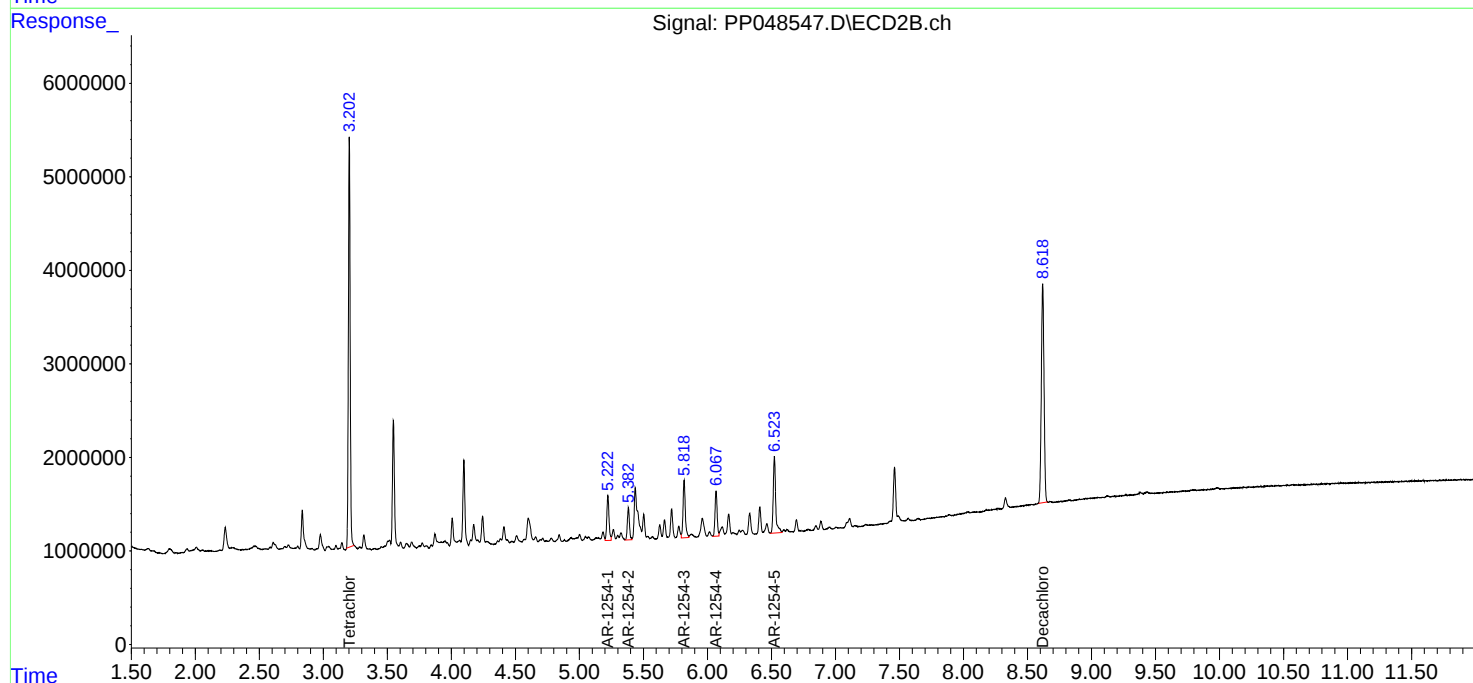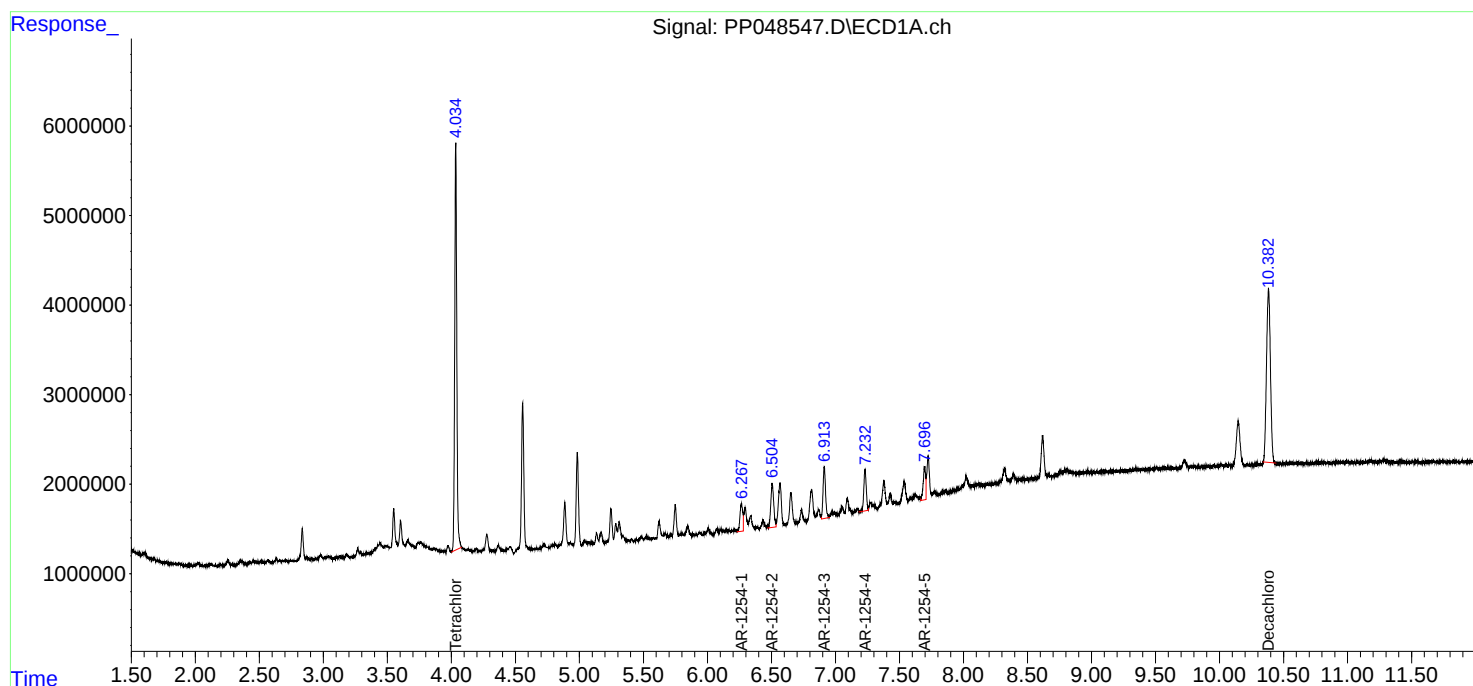

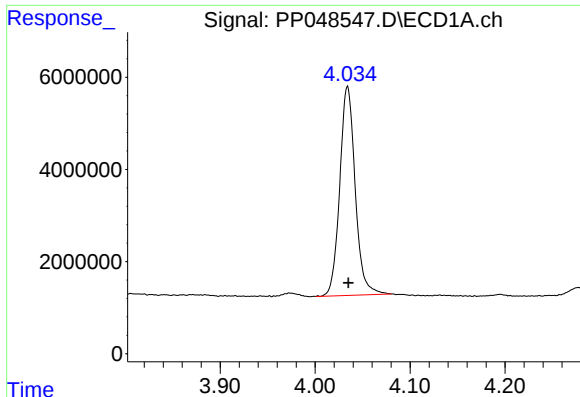


#1 Tetrachloro-m-xylene

R.T.: 4.034 min
Delta R.T.: 0.000 min
Response: 51315029
Conc: 21.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-1552


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/08/2022
Supervised By :Ankita Jodhani 06/08/2022

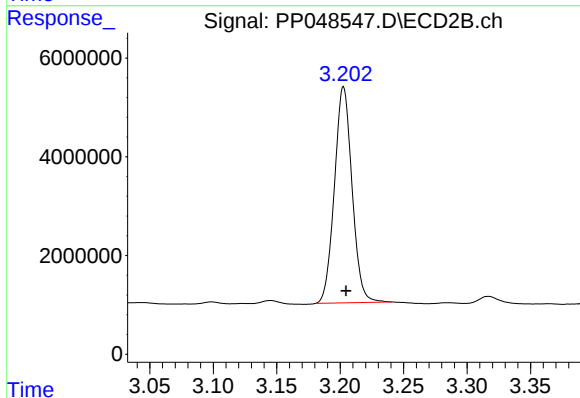


#1 Tetrachloro-m-xylene

R.T.: 3.203 min
Delta R.T.: -0.002 min
Response: 42377954
Conc: 22.26 ng/ml

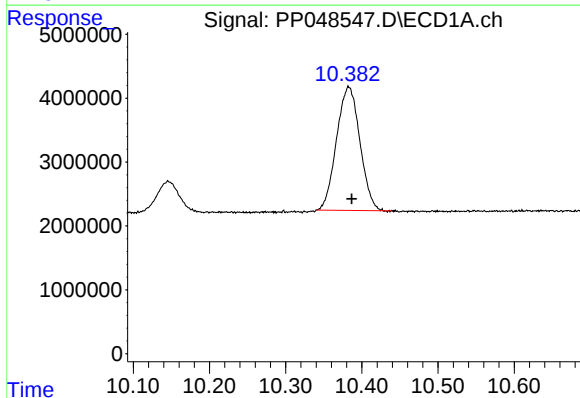


#2 Decachlorobiphenyl

R.T.: 10.383 min
Delta R.T.: -0.004 min
Response: 41163280
Conc: 21.60 ng/ml

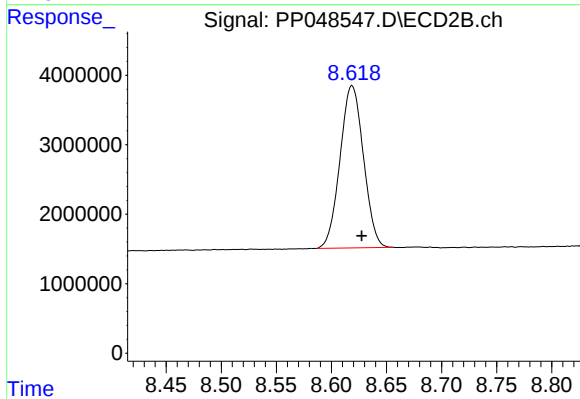

#2 Decachlorobiphenyl

R.T.: 8.618 min
Delta R.T.: -0.009 min
Response: 34527339
Conc: 28.20 ng/ml m

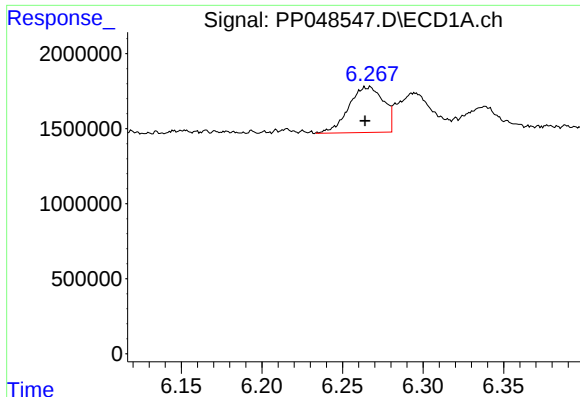


#26 AR-1254-1

R.T.: 6.267 min
Delta R.T.: 0.003 min
Response: 4576508
Conc: 49.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-1552


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/08/2022
Supervised By :Ankita Jodhani 06/08/2022

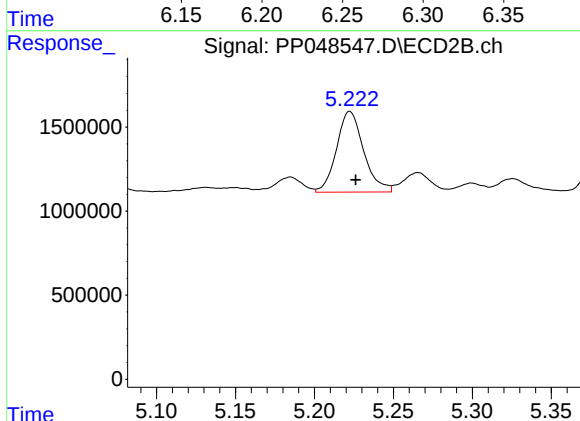


#26 AR-1254-1

R.T.: 5.222 min
Delta R.T.: -0.004 min
Response: 5747880
Conc: 56.86 ng/ml

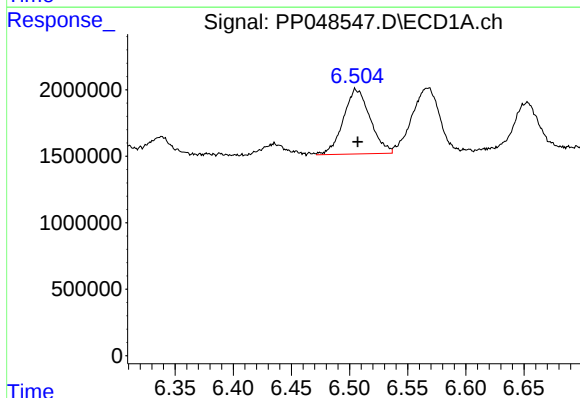


#27 AR-1254-2

R.T.: 6.505 min
Delta R.T.: -0.002 min
Response: 7806996
Conc: 56.28 ng/ml

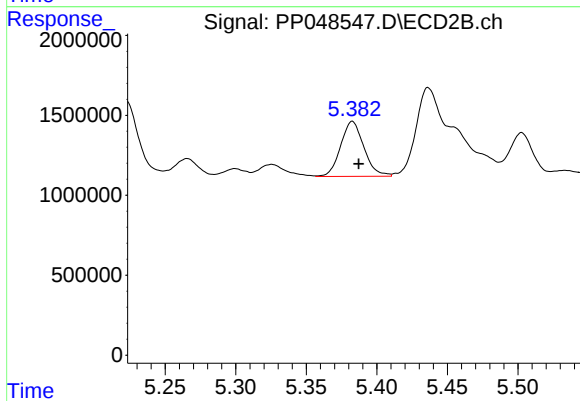

#27 AR-1254-2

R.T.: 5.383 min
Delta R.T.: -0.005 min
Response: 3940777
Conc: 44.76 ng/ml

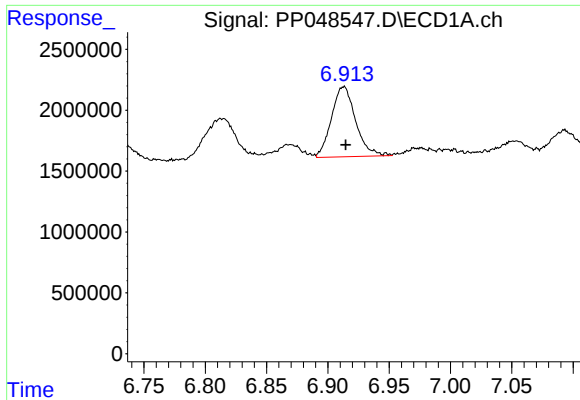


#28 AR-1254-3

R.T.: 6.913 min
Delta R.T.: -0.002 min
Response: 7905705
Conc: 55.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-1552


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/08/2022
Supervised By :Ankita Jodhani 06/08/2022

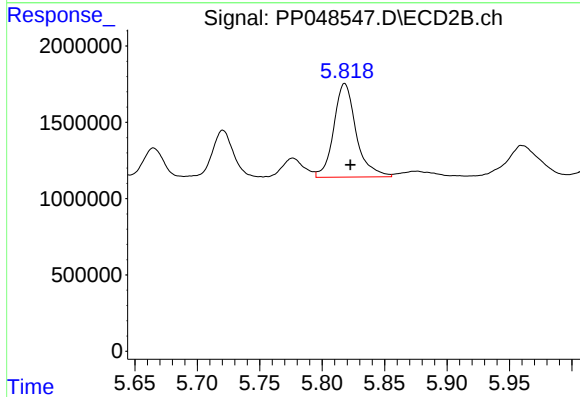


#28 AR-1254-3

R.T.: 5.818 min
Delta R.T.: -0.005 min
Response: 7670386
Conc: 55.18 ng/ml

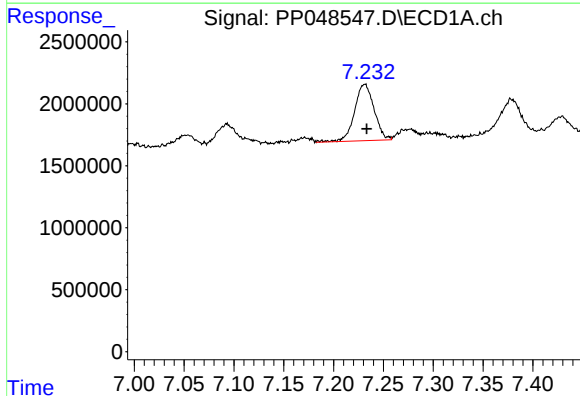


#29 AR-1254-4

R.T.: 7.231 min
Delta R.T.: -0.002 min
Response: 6239771
Conc: 58.55 ng/ml

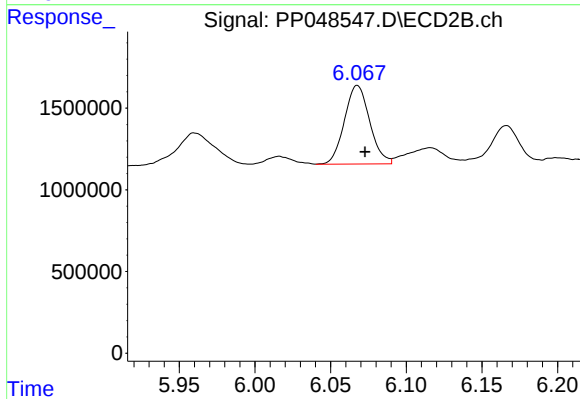

#29 AR-1254-4

R.T.: 6.068 min
Delta R.T.: -0.005 min
Response: 5595249
Conc: 64.52 ng/ml

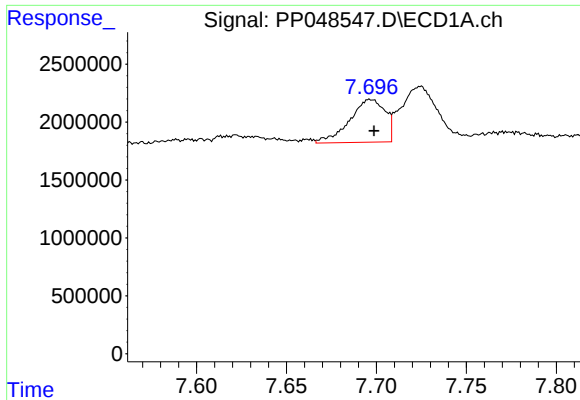


#30 AR-1254-5

R.T.: 7.697 min
Delta R.T.: -0.002 min
Response: 5071148
Conc: 42.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-1552

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/08/2022
Supervised By :Ankita Jodhani 06/08/2022

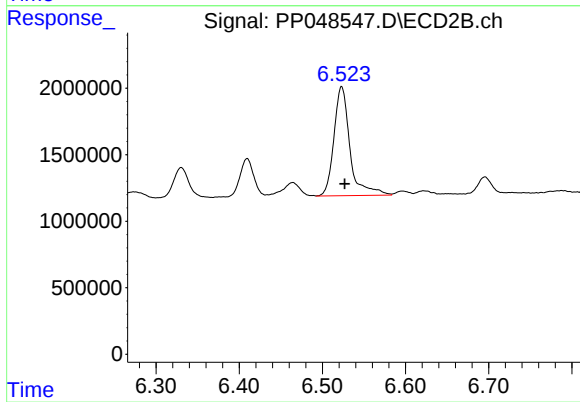

#30 AR-1254-5

R.T.: 6.523 min
Delta R.T.: -0.004 min
Response: 10996607
Conc: 89.66 ng/ml