

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060822\
 Data File : PP048565.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jun 2022 06:41
 Operator : YP\AJ
 Sample : N3175-12
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AUD-1724

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/08/2022
 Supervised By :Ankita Jodhani 06/08/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 08:55:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 07 11:09:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.035	3.202	34071917	29000744	14.219	15.237
2) SA Decachlor...	10.384	8.619	28826226	18943854	15.124	15.470
Target Compounds						
16) L4 AR-1242-1	5.322	4.361	9422877	6580049	139.575	118.267
17) L4 AR-1242-2	5.347	4.380	14203243	9910590	146.152	130.538
18) L4 AR-1242-3	5.413	4.567	10195399	7421921	168.170	175.827
19) L4 AR-1242-4	5.523	4.659	10199510	8437512	200.512	209.668
20) L4 AR-1242-5	6.338	5.221	13131243	7942072	245.907	160.796m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060822\
Data File : PP048565.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jun 2022 06:41
Operator : YP\AJ
Sample : N3175-12
Misc :
ALS Vial : 59 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AUD-1724


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/08/2022
Supervised By :Ankita Jodhani 06/08/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 08:55:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 07 11:09:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

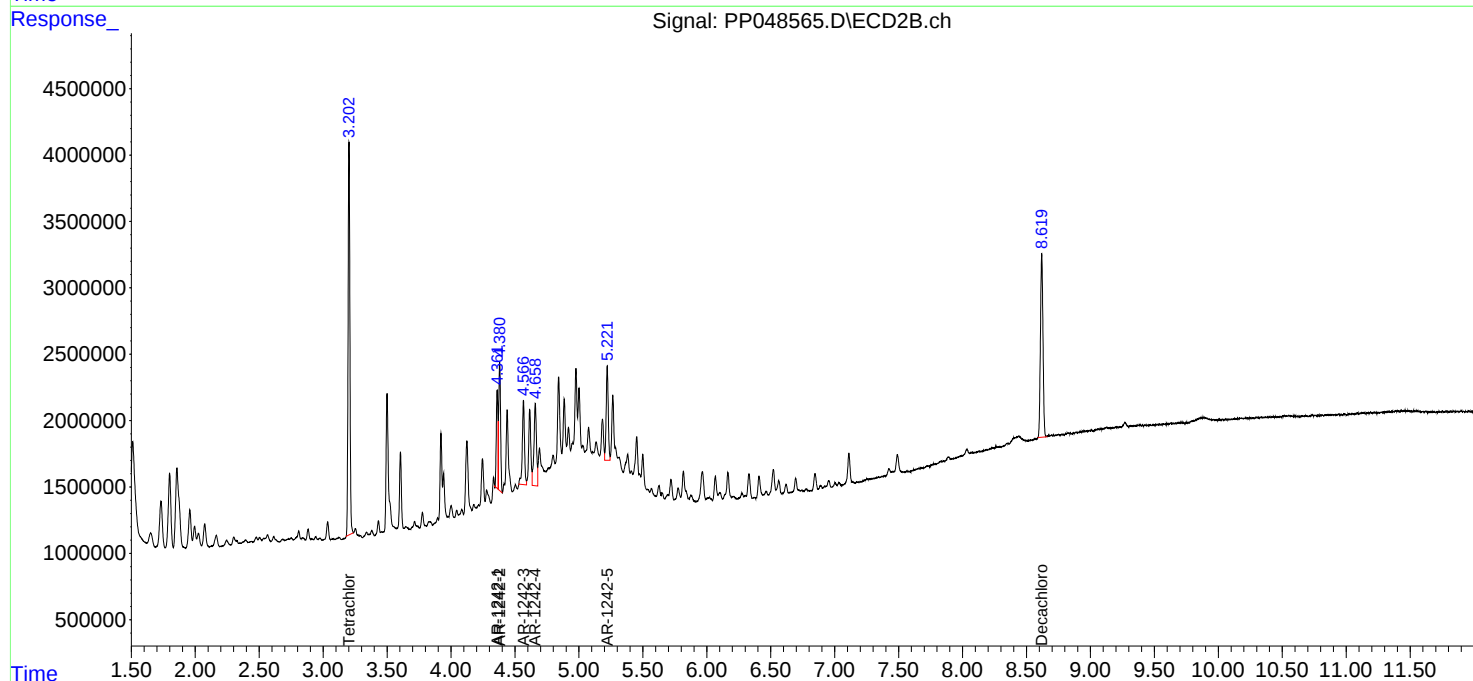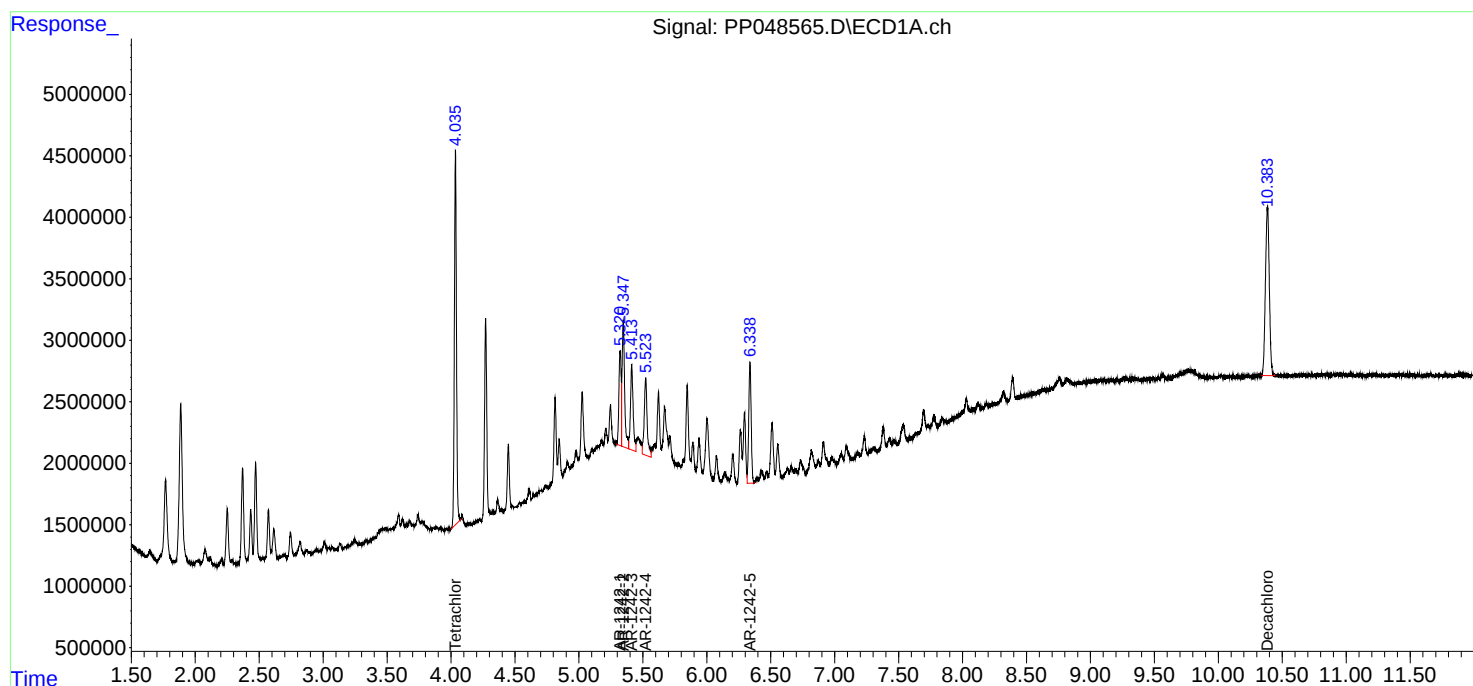

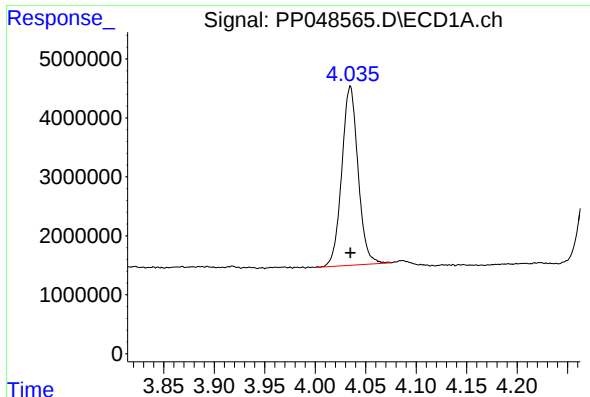


#1 Tetrachloro-m-xylene

R.T.: 4.035 min
Delta R.T.: 0.000 min
Response: 34071917
Conc: 14.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-1724


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/08/2022
Supervised By :Ankita Jodhani 06/08/2022

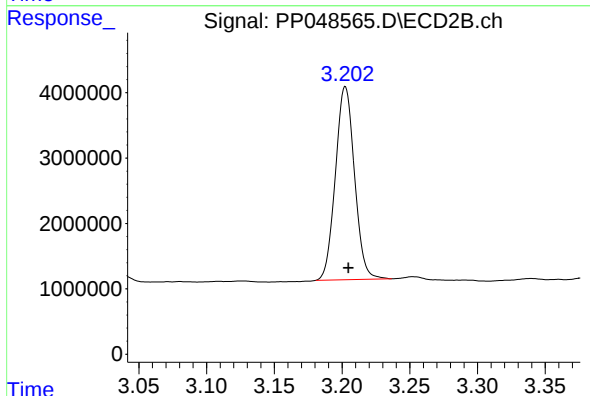


#1 Tetrachloro-m-xylene

R.T.: 3.202 min
Delta R.T.: -0.002 min
Response: 29000744
Conc: 15.24 ng/ml

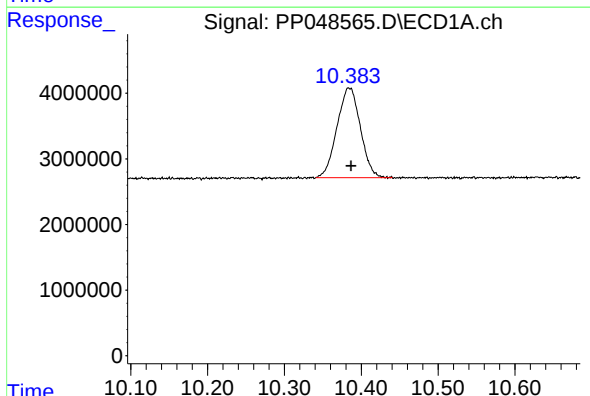


#2 Decachlorobiphenyl

R.T.: 10.384 min
Delta R.T.: -0.002 min
Response: 28826226
Conc: 15.12 ng/ml

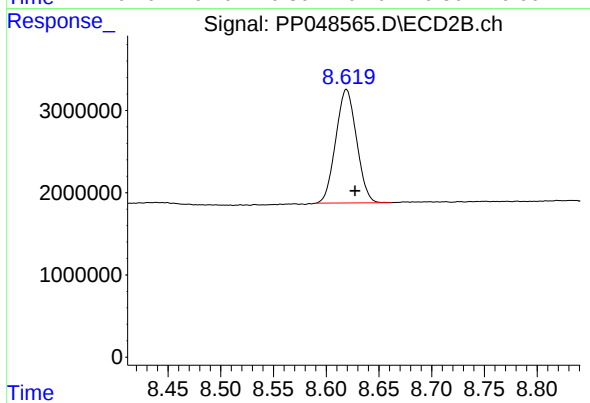

#2 Decachlorobiphenyl

R.T.: 8.619 min
Delta R.T.: -0.008 min
Response: 18943854
Conc: 15.47 ng/ml

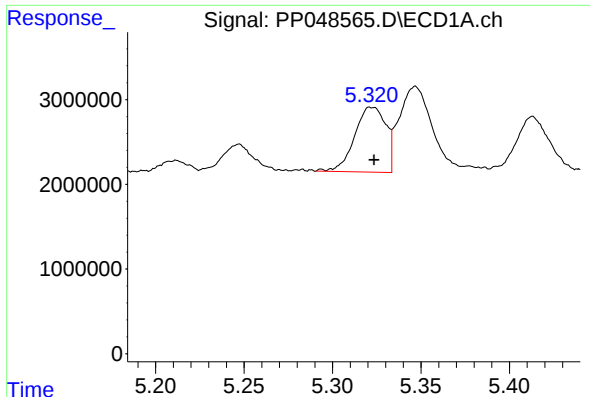


#16 AR-1242-1

R.T.: 5.322 min
Delta R.T.: -0.001 min
Response: 9422877
Conc: 139.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-1724


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/08/2022
Supervised By :Ankita Jodhani 06/08/2022

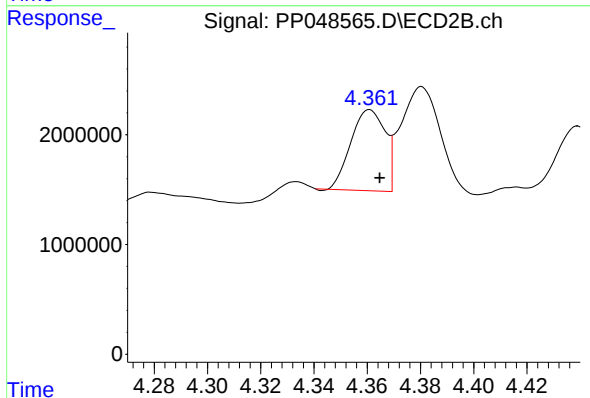


#16 AR-1242-1

R.T.: 4.361 min
Delta R.T.: -0.004 min
Response: 6580049
Conc: 118.27 ng/ml

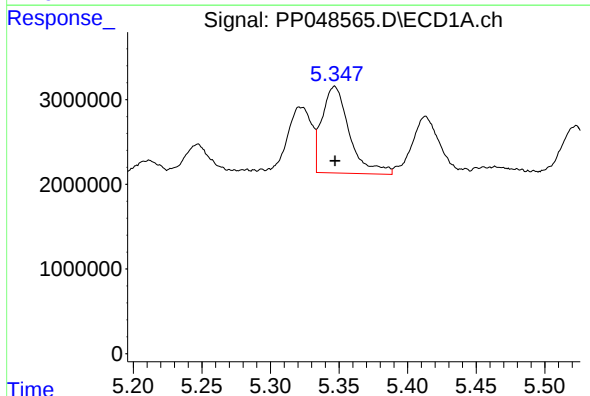


#17 AR-1242-2

R.T.: 5.347 min
Delta R.T.: 0.000 min
Response: 14203243
Conc: 146.15 ng/ml

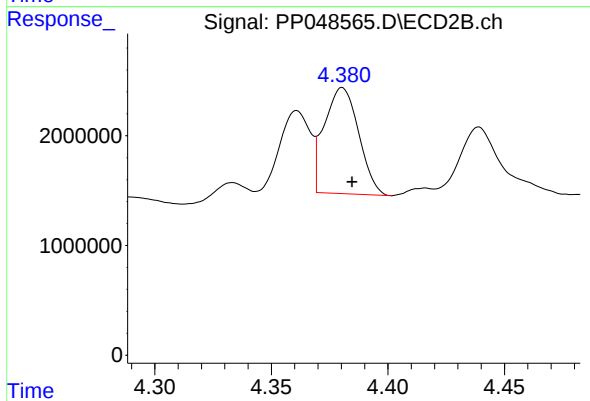

#17 AR-1242-2

R.T.: 4.380 min
Delta R.T.: -0.004 min
Response: 9910590
Conc: 130.54 ng/ml

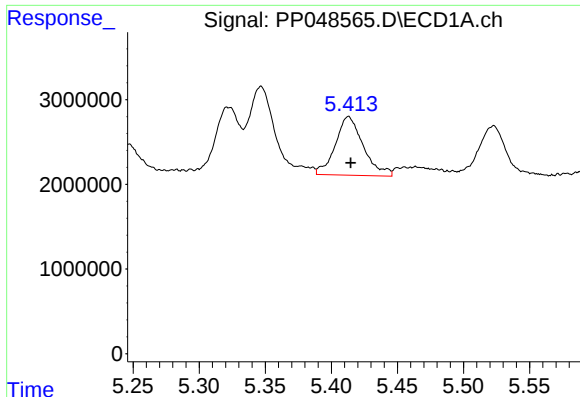


#18 AR-1242-3

R.T.: 5.413 min
Delta R.T.: -0.002 min
Response: 10195399
Conc: 168.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-1724


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/08/2022
Supervised By :Ankita Jodhani 06/08/2022

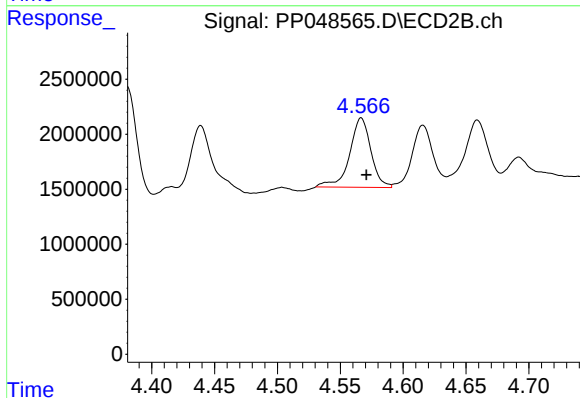


#18 AR-1242-3

R.T.: 4.567 min
Delta R.T.: -0.004 min
Response: 7421921
Conc: 175.83 ng/ml

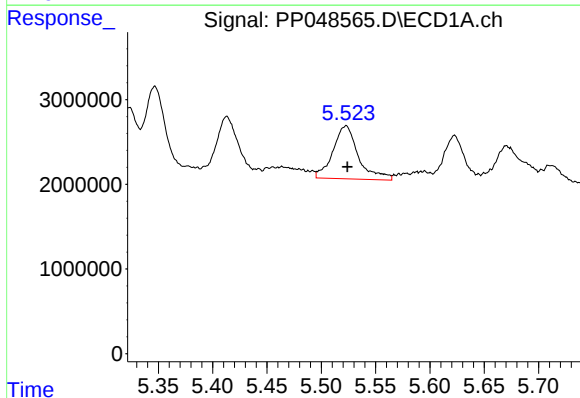


#19 AR-1242-4

R.T.: 5.523 min
Delta R.T.: -0.001 min
Response: 10199510
Conc: 200.51 ng/ml

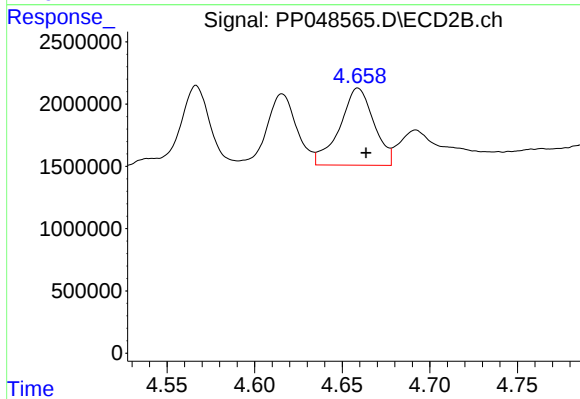

#19 AR-1242-4

R.T.: 4.659 min
Delta R.T.: -0.005 min
Response: 8437512
Conc: 209.67 ng/ml

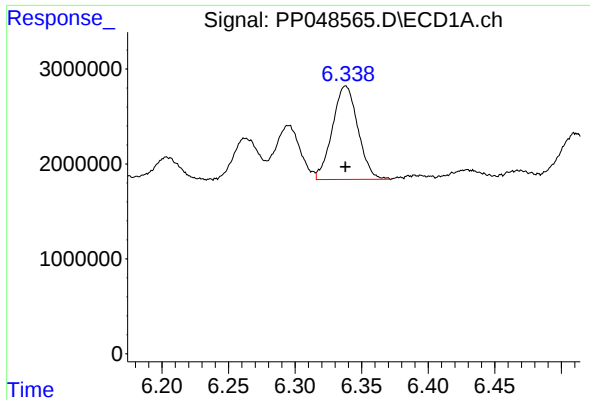


#20 AR-1242-5

R.T.: 6.338 min
Delta R.T.: 0.000 min
Response: 13131243
Conc: 245.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-1724

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/08/2022
Supervised By :Ankita Jodhani 06/08/2022

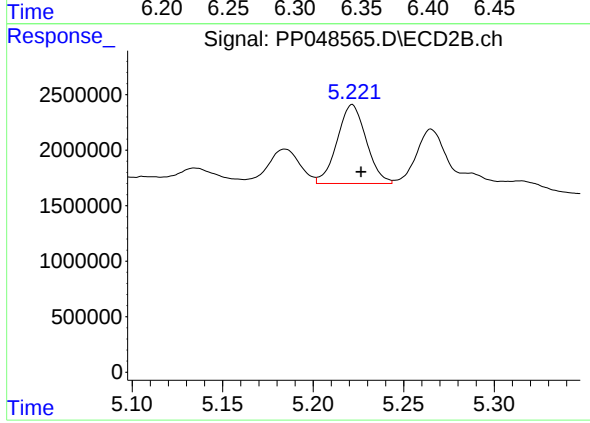

#20 AR-1242-5

R.T.: 5.221 min
Delta R.T.: -0.005 min
Response: 7942072
Conc: 160.80 ng/ml m