

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062118\
 Data File : PP026592.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2018 14:56
 Operator : UA/AJ
 Sample : AR1660ICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1660ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 16:04:05 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 21 16:04:02 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.062	4.276	391148	1055203	4.117	4.529
2)	SA Decachlor...	8.334	9.188	585656	688562	4.157	4.832
Target Compounds							
3)	L1 Aroclor-1...	0.000	4.927	0	344567	N.D.	45.834 #
4)	L1 Aroclor-1...	0.000	5.085	0	140182	N.D.	50.565 #
5)	L1 Aroclor-1...	0.000	5.244	0	319258	N.D.	52.542 #
6)	L1 Aroclor-1...	0.000	5.259	0	476194	N.D.	48.865 #
7)	L1 Aroclor-1...	0.000	5.496	0	174588	N.D.	54.695 #
31)	L7 Aroclor-1...	0.000	6.552	0	202470	N.D.	51.422 #
32)	L7 Aroclor-1...	0.000	6.681	0	416913	N.D.	50.718 #
33)	L7 Aroclor-1...	0.000	6.973	0	408440	N.D.	60.563 #
34)	L7 Aroclor-1...	0.000	7.454	0	354687	N.D.	49.043 #
35)	L7 Aroclor-1...	7.161	7.645	687197	715129	38.869	45.655



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062118\
Data File : PP026592.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2018 14:56
Operator : UA/AJ
Sample : AR1660ICC050
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660ICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 16:04:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062118.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 21 16:04:02 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

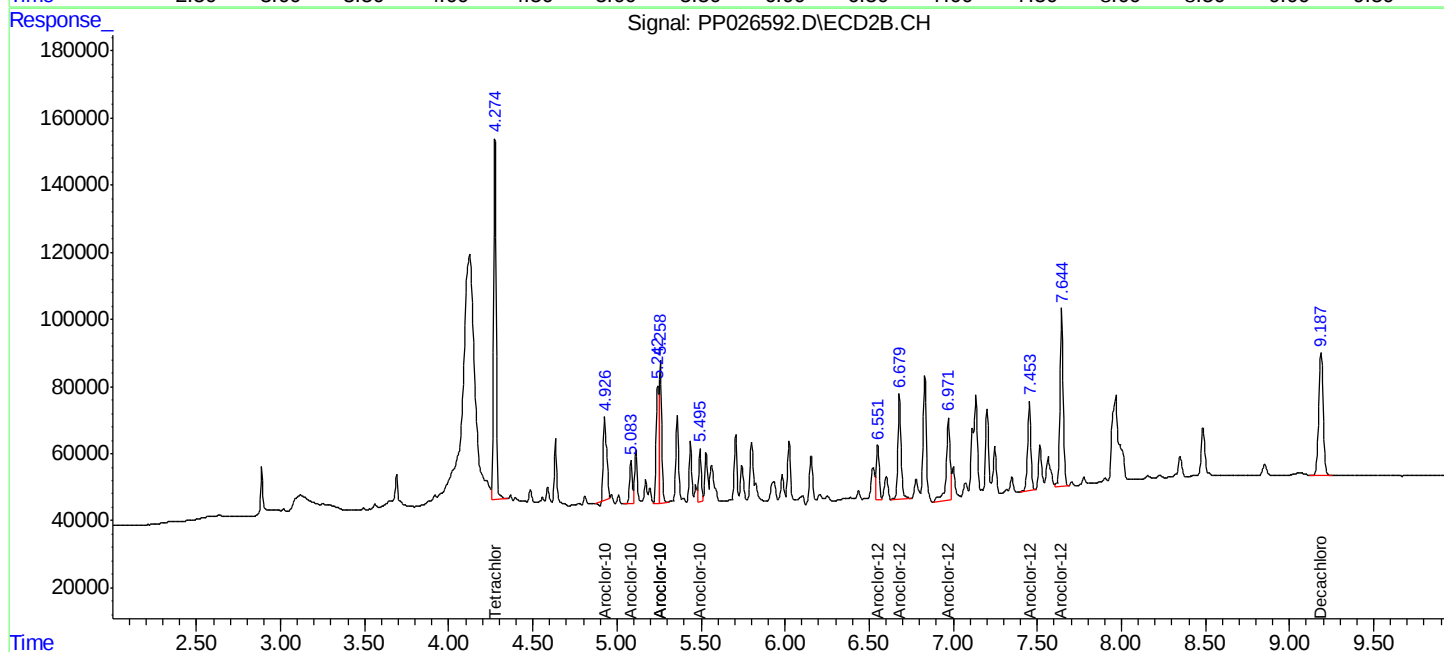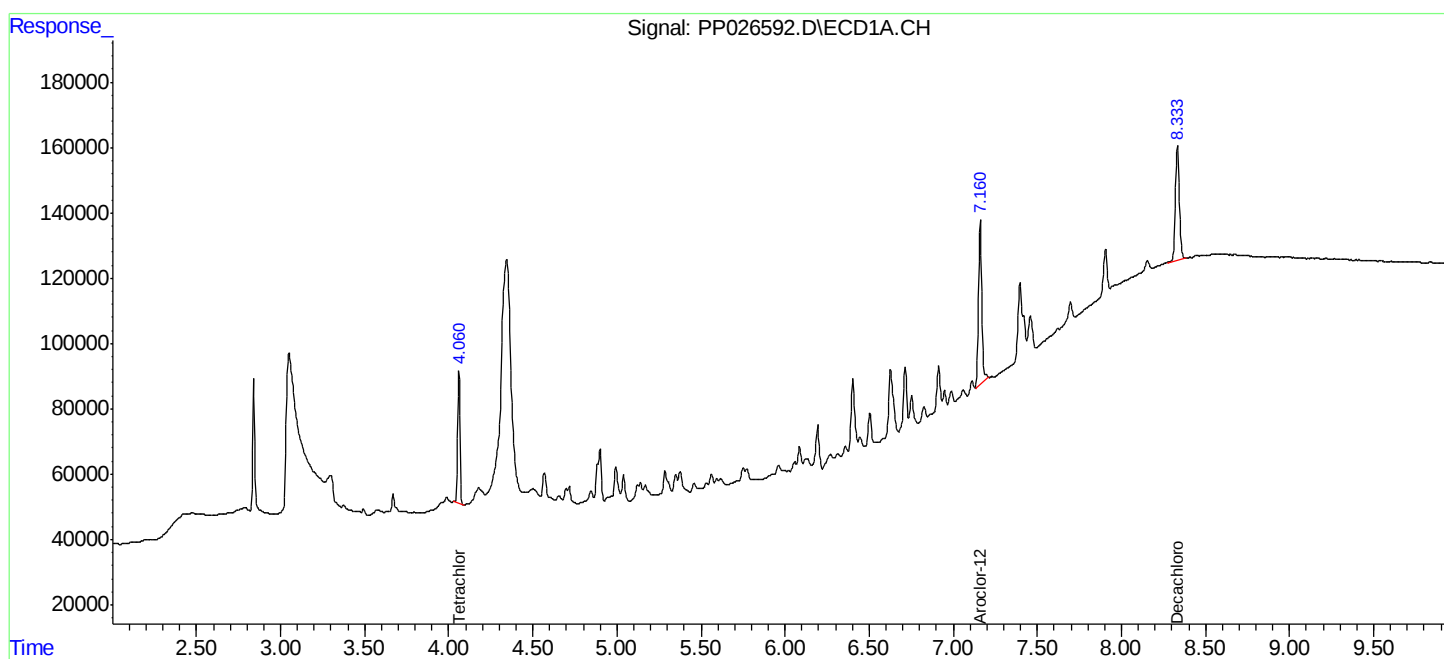


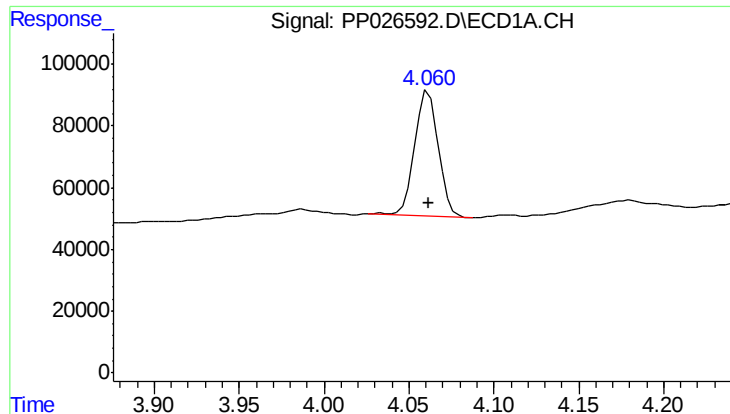

#1 Tetrachloro-m-xylene


R.T.: 4.062 min
Delta R.T.: 0.000 min
Response: 391148
Conc: 4.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1660ICC050

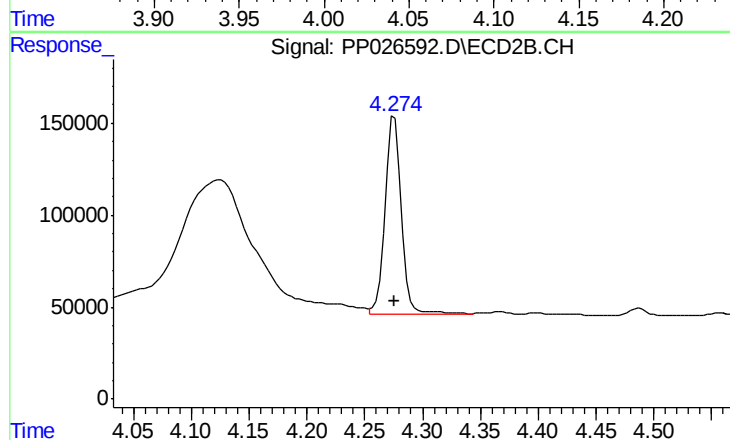


#1 Tetrachloro-m-xylene

R.T.: 4.276 min
Delta R.T.: 0.000 min
Response: 1055203
Conc: 4.53 ng/ml

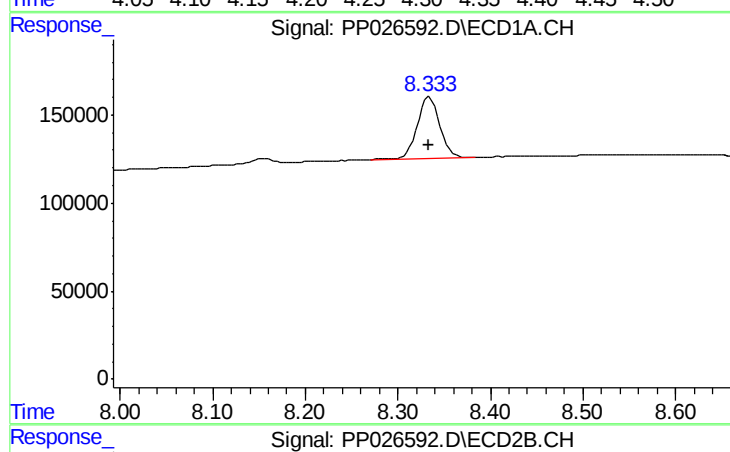


#2 Decachlorobiphenyl

R.T.: 8.334 min
Delta R.T.: 0.000 min
Response: 585656
Conc: 4.16 ng/ml

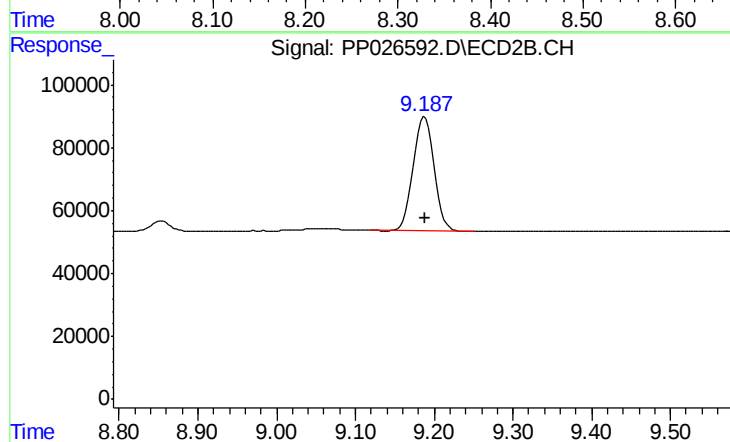

#2 Decachlorobiphenyl


R.T.: 9.188 min
Delta R.T.: 0.000 min
Response: 688562
Conc: 4.83 ng/ml

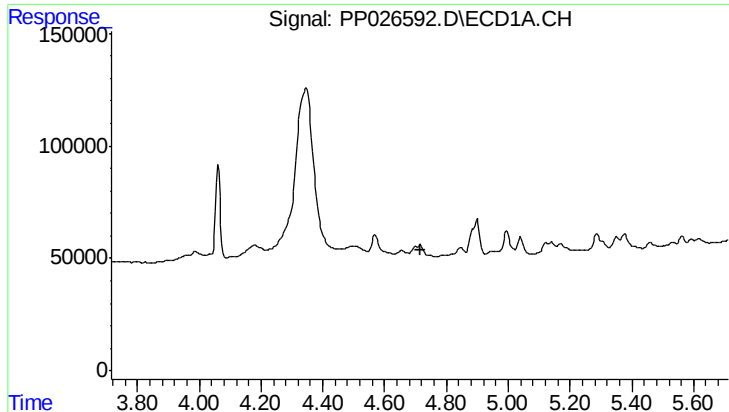

#3 Aroclor-1016-1


R.T.: 0.000 min
Exp R.T.: 4.715 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
AR1660ICC050

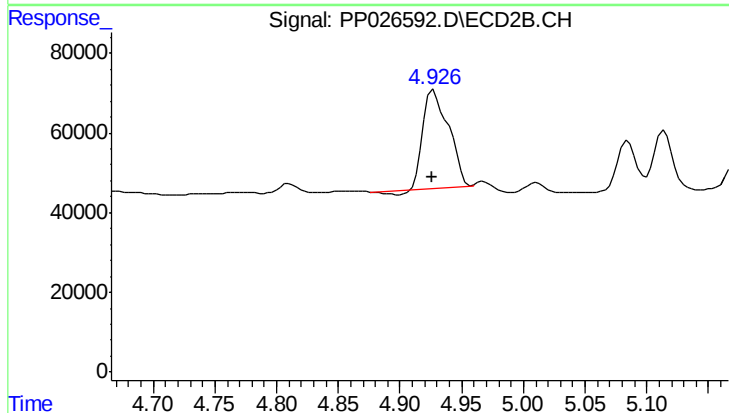


#3 Aroclor-1016-1

R.T.: 4.927 min
Delta R.T.: 0.001 min
Response: 344567
Conc: 45.83 ng/ml

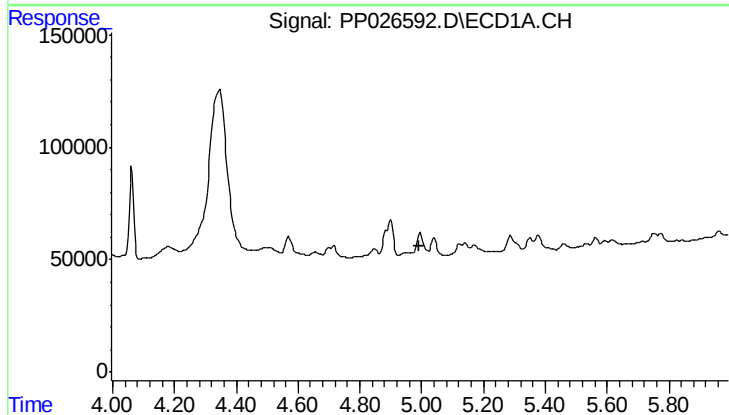


#4 Aroclor-1016-2

R.T.: 0.000 min
Exp R.T.: 4.994 min
Response: 0
Conc: N.D.

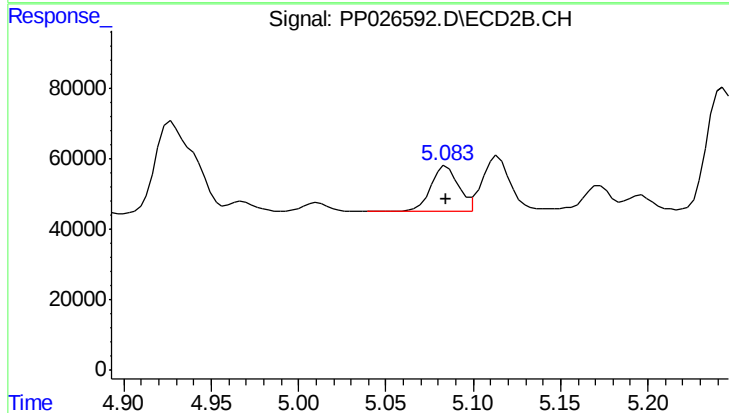

#4 Aroclor-1016-2


R.T.: 5.085 min
Delta R.T.: 0.000 min
Response: 140182
Conc: 50.57 ng/ml

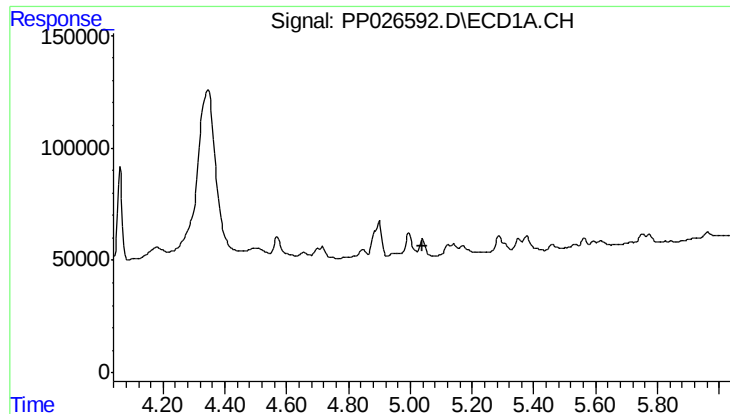

#5 Aroclor-1016-3


R.T.: 0.000 min
Exp R.T.: 5.039 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
AR1660ICC050

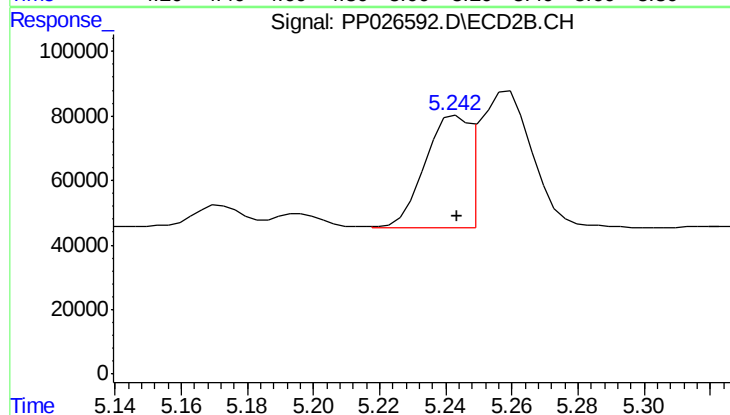


#5 Aroclor-1016-3

R.T.: 5.244 min
Delta R.T.: 0.000 min
Response: 319258
Conc: 52.54 ng/ml

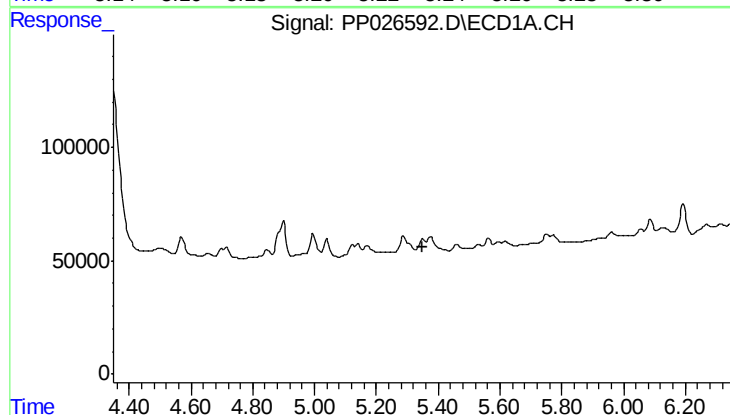


#6 Aroclor-1016-4

R.T.: 0.000 min
Exp R.T.: 5.349 min
Response: 0
Conc: N.D.

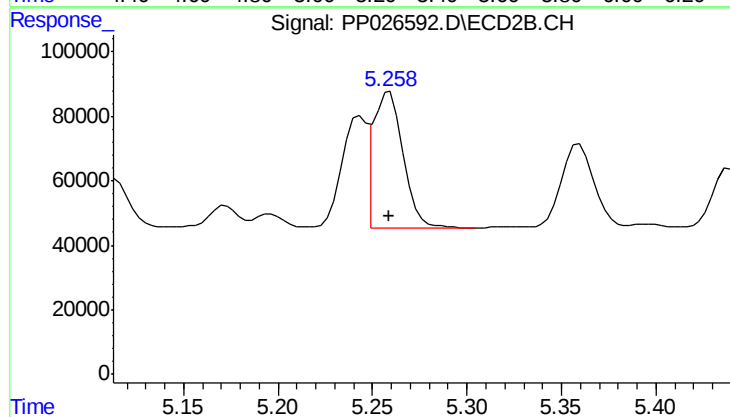

#6 Aroclor-1016-4


R.T.: 5.259 min
Delta R.T.: 0.000 min
Response: 476194
Conc: 48.87 ng/ml

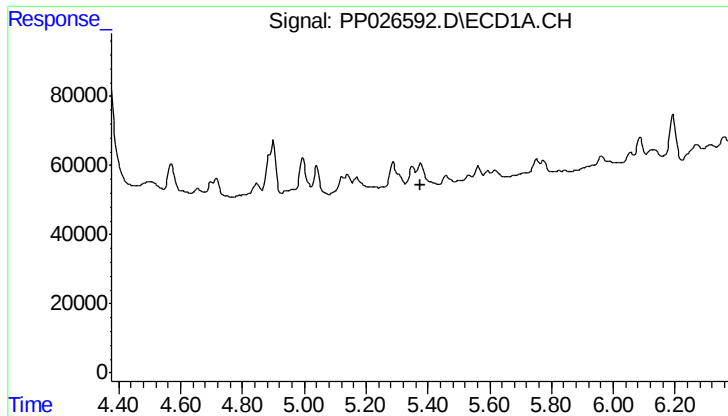

#7 Aroclor-1016-5


R.T.: 0.000 min
Exp R.T.: 5.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
AR1660ICC050

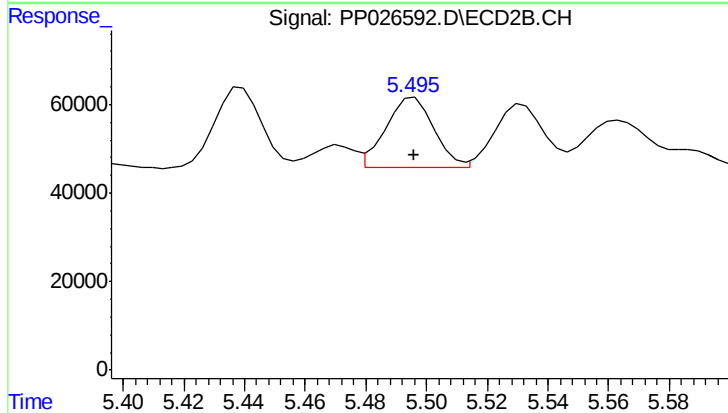


#7 Aroclor-1016-5

R.T.: 5.496 min
Delta R.T.: 0.000 min
Response: 174588
Conc: 54.69 ng/ml

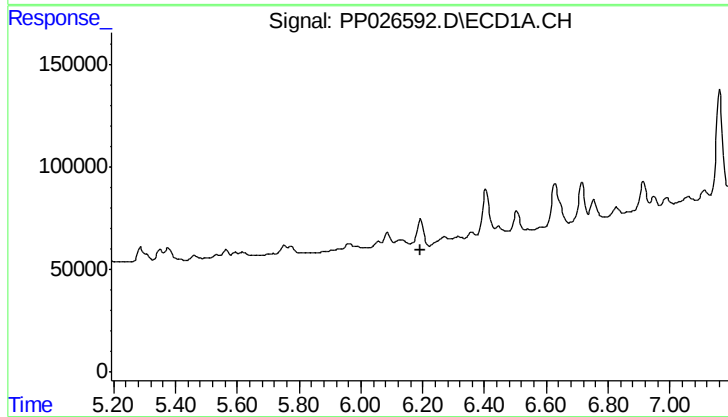


#31 Aroclor-1260-1

R.T.: 0.000 min
Exp R.T.: 6.192 min
Response: 0
Conc: N.D.

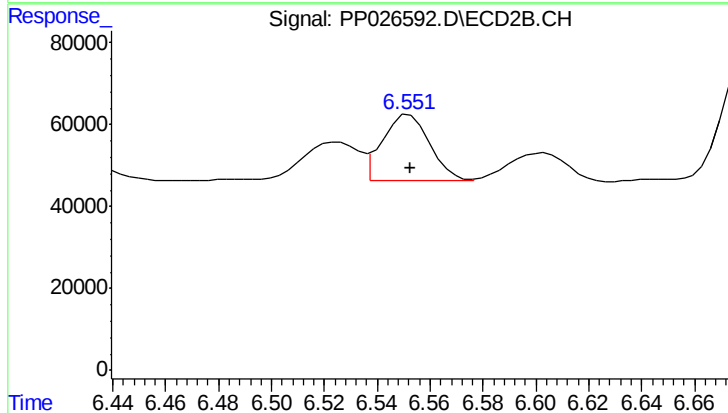

#31 Aroclor-1260-1


R.T.: 6.552 min
Delta R.T.: 0.000 min
Response: 202470
Conc: 51.42 ng/ml

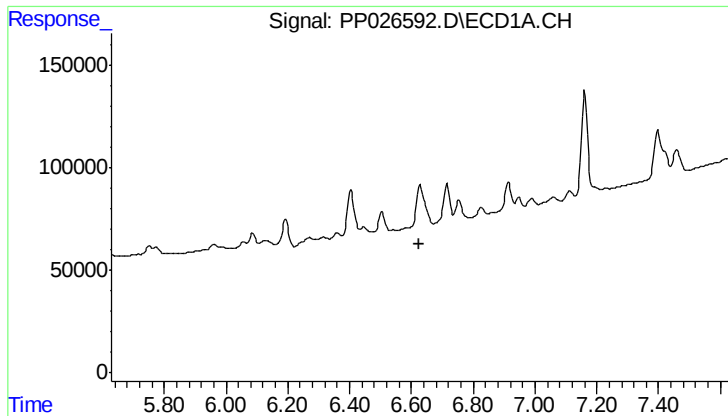

#32 Aroclor-1260-2


R.T.: 0.000 min
Exp R.T.: 6.627 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
AR1660ICC050

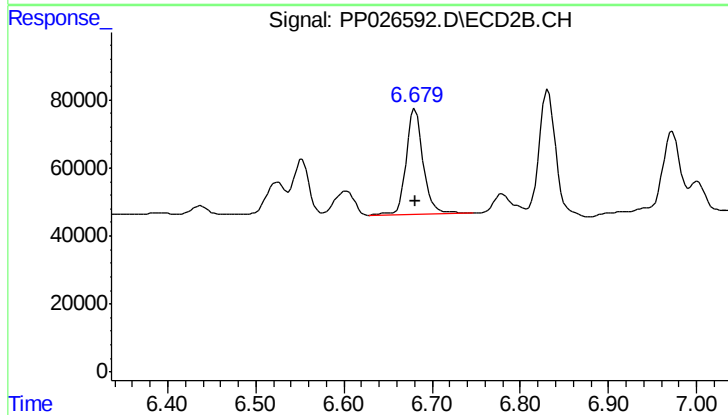


#32 Aroclor-1260-2

R.T.: 6.681 min
Delta R.T.: 0.000 min
Response: 416913
Conc: 50.72 ng/ml

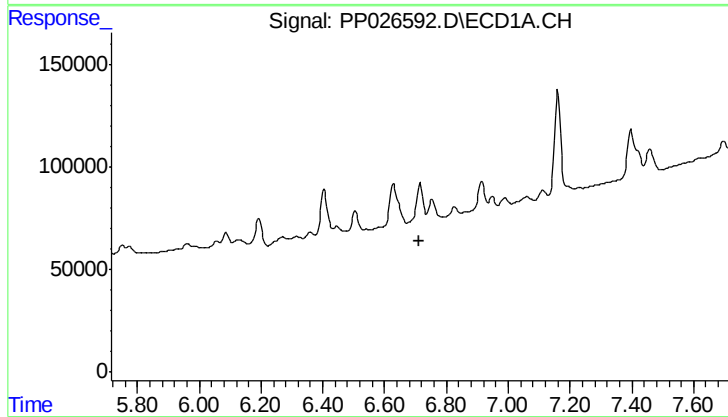


#33 Aroclor-1260-3

R.T.: 0.000 min
Exp R.T.: 6.714 min
Response: 0
Conc: N.D.

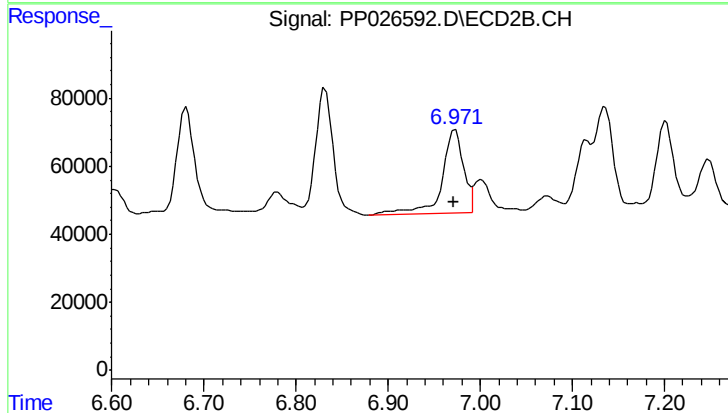

#33 Aroclor-1260-3


R.T.: 6.973 min
Delta R.T.: 0.001 min
Response: 408440
Conc: 60.56 ng/ml

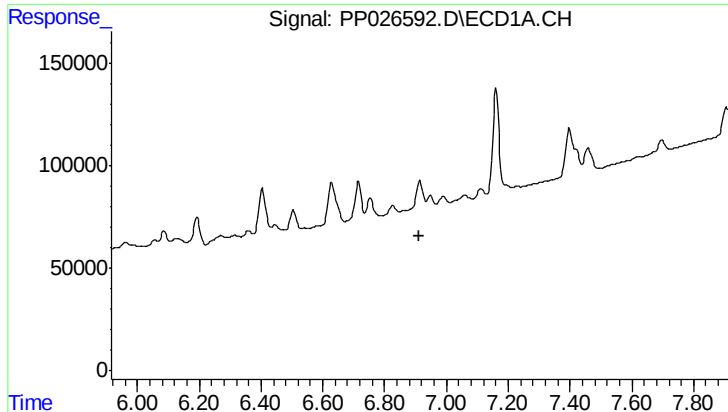

#34 Aroclor-1260-4


R.T.: 0.000 min
Exp R.T.: 6.913 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
AR1660ICC050

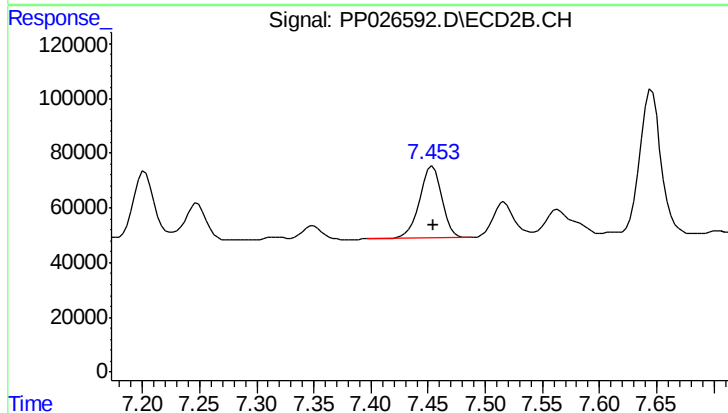


#34 Aroclor-1260-4

R.T.: 7.454 min
Delta R.T.: 0.000 min
Response: 354687
Conc: 49.04 ng/ml

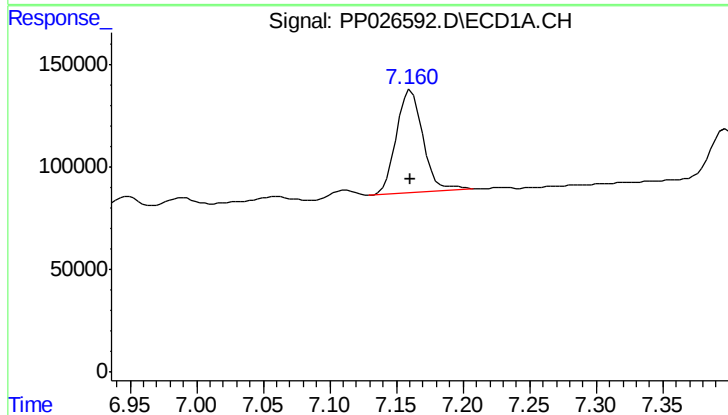

#35 Aroclor-1260-5

R.T.: 7.161 min
Delta R.T.: 0.000 min
Response: 687197
Conc: 38.87 ng/ml

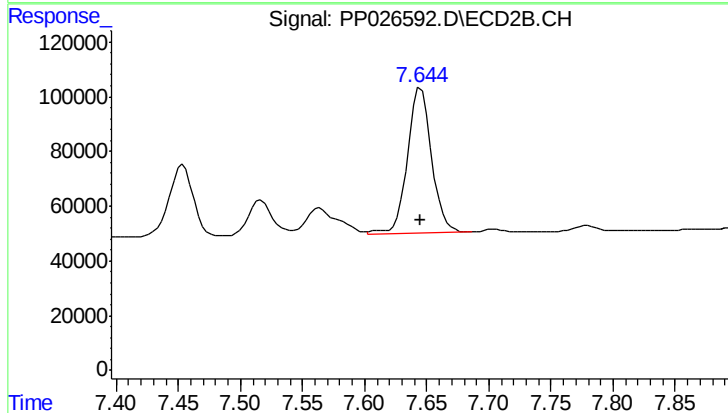

#35 Aroclor-1260-5

R.T.: 7.645 min
Delta R.T.: 0.000 min
Response: 715129
Conc: 45.66 ng/ml