

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062118\
 Data File : PP026593.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2018 15:16
 Operator : UA/AJ
 Sample : AR1221ICC500
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1221ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 16:38:31 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 21 16:28:30 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.064	4.278	4410769	10811646	47.030	47.242
2) SA Decachlor...	8.340	9.191	6619301	6897916	47.422	48.062
Target Compounds						
3) L1 Aroclor-1...	0.000	4.924	0	659008	N.D.	104.788 #
4) L1 Aroclor-1...	0.000	5.086	0	193598	N.D.	85.594 #
5) L1 Aroclor-1...	0.000	5.260	0	676666	N.D.	132.326 #
6) L1 Aroclor-1...	0.000	5.260	0	676666	N.D.	83.919 #
7) L1 Aroclor-1...	0.000	5.440	0	178840	N.D.	67.308 #
8) L2 Aroclor-1...	4.183	4.490	565558	1322702	500.000	500.000
9) L2 Aroclor-1...	4.289	4.592	3103278	870884	500.000	500.000
10) L2 Aroclor-1...	4.319	4.638	4784543	3104158	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062118\
Data File : PP026593.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2018 15:16
Operator : UA/AJ
Sample : AR1221ICC500
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1221ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 16:38:31 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062118.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 21 16:28:30 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

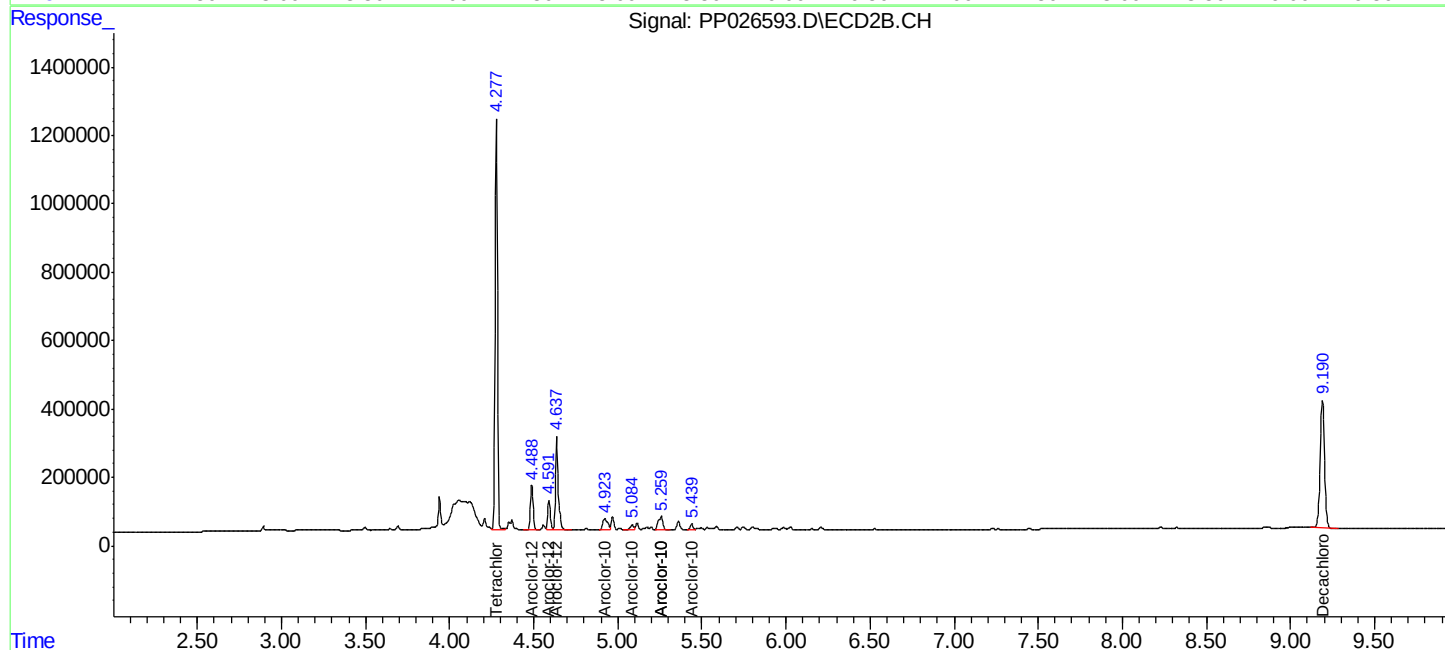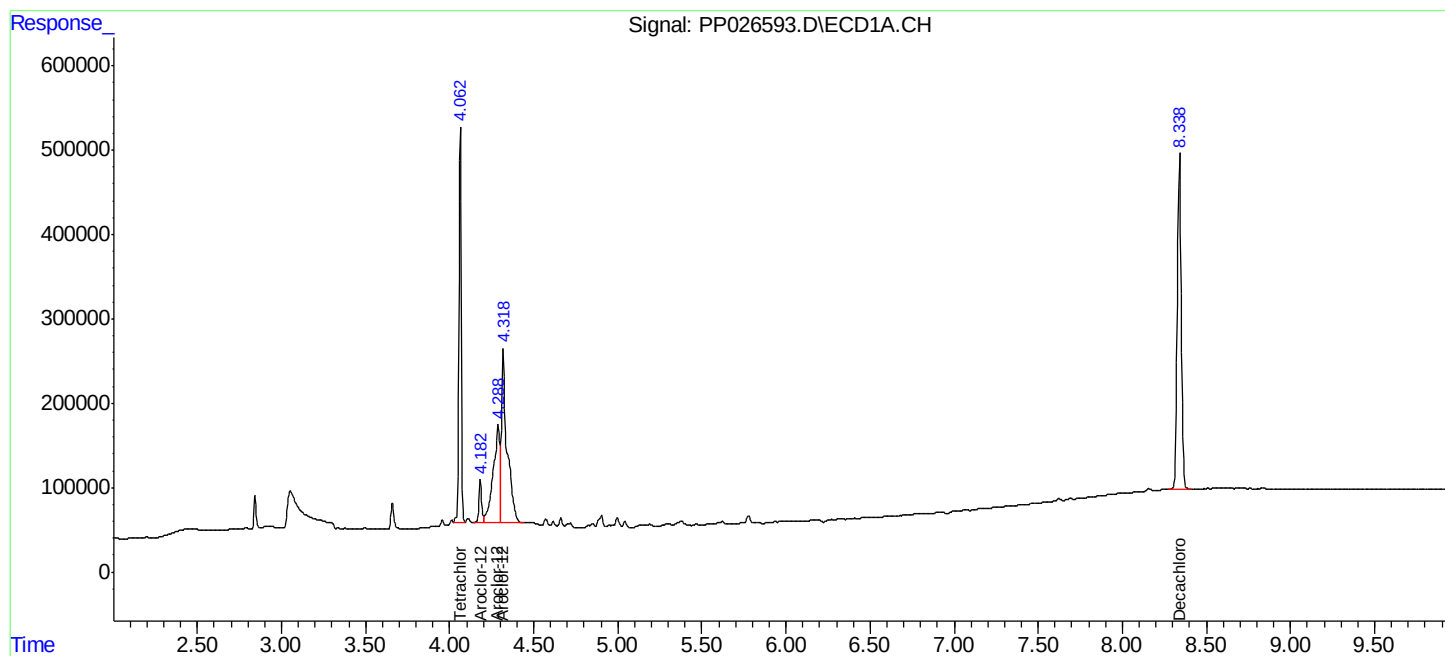


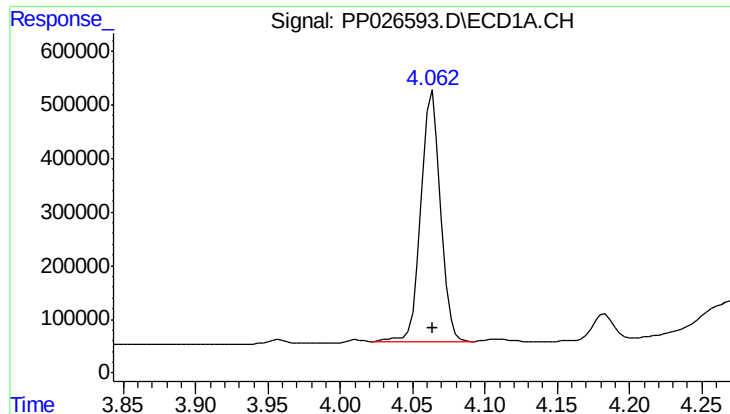

#1 Tetrachloro-m-xylene


R.T.: 4.064 min
Delta R.T.: 0.000 min
Response: 4410769
Conc: 47.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1221ICC500

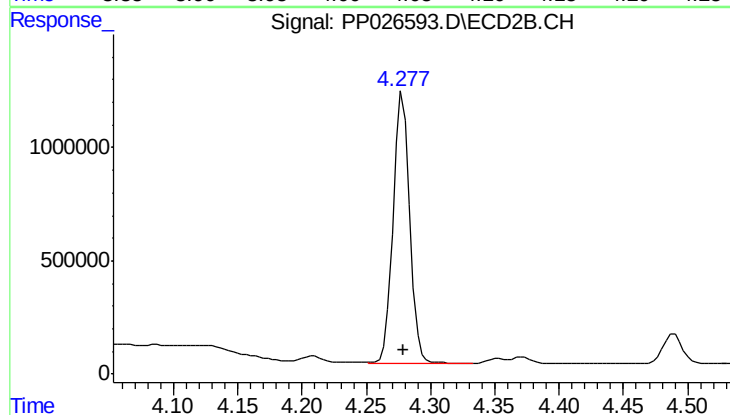


#1 Tetrachloro-m-xylene

R.T.: 4.278 min
Delta R.T.: 0.000 min
Response: 10811646
Conc: 47.24 ng/ml

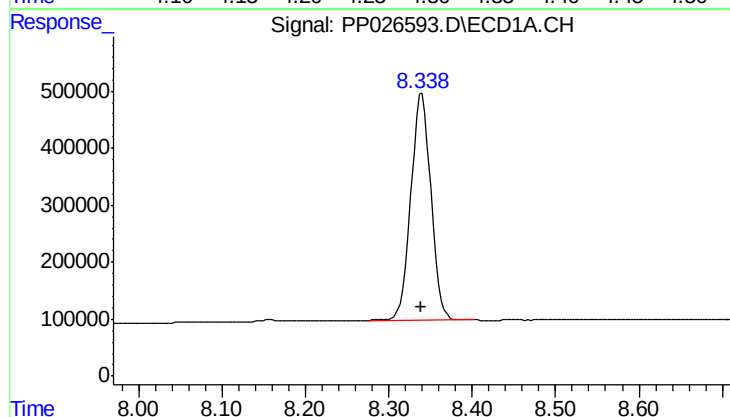


#2 Decachlorobiphenyl

R.T.: 8.340 min
Delta R.T.: 0.000 min
Response: 6619301
Conc: 47.42 ng/ml

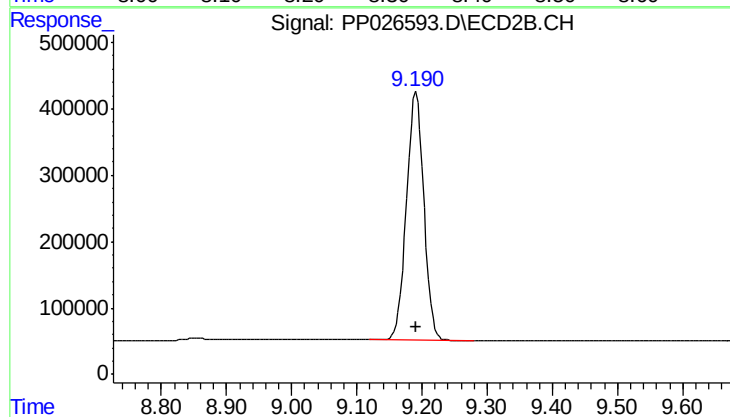

#2 Decachlorobiphenyl


R.T.: 9.191 min
Delta R.T.: 0.000 min
Response: 6897916
Conc: 48.06 ng/ml

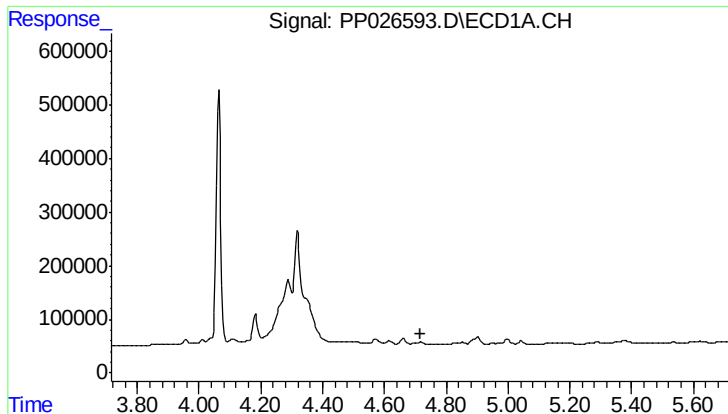

#3 Aroclor-1016-1


R.T.: 0.000 min
Exp R.T.: 4.715 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
AR1221ICC500

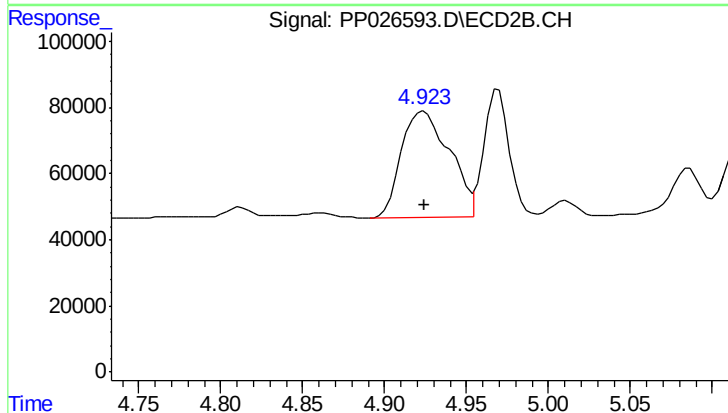


#3 Aroclor-1016-1

R.T.: 4.924 min
Delta R.T.: 0.000 min
Response: 659008
Conc: 104.79 ng/ml

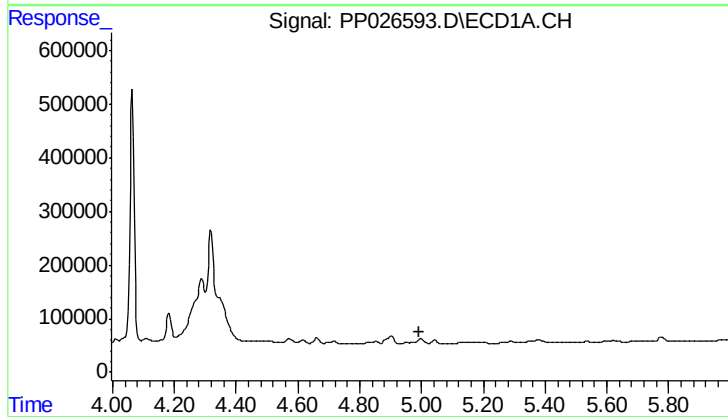


#4 Aroclor-1016-2

R.T.: 0.000 min
Exp R.T.: 4.994 min
Response: 0
Conc: N.D.

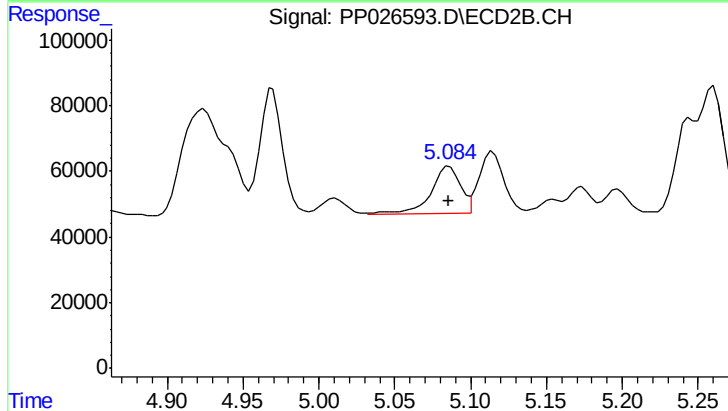

#4 Aroclor-1016-2


R.T.: 5.086 min
Delta R.T.: 0.000 min
Response: 193598
Conc: 85.59 ng/ml

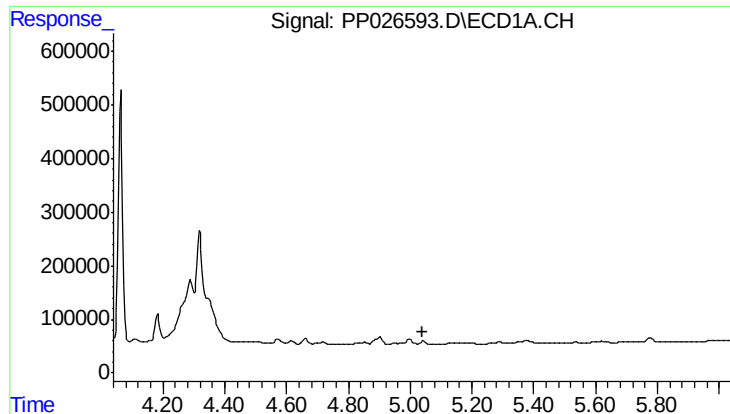

#5 Aroclor-1016-3


R.T.: 0.000 min
Exp R.T.: 5.039 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
AR1221ICC500

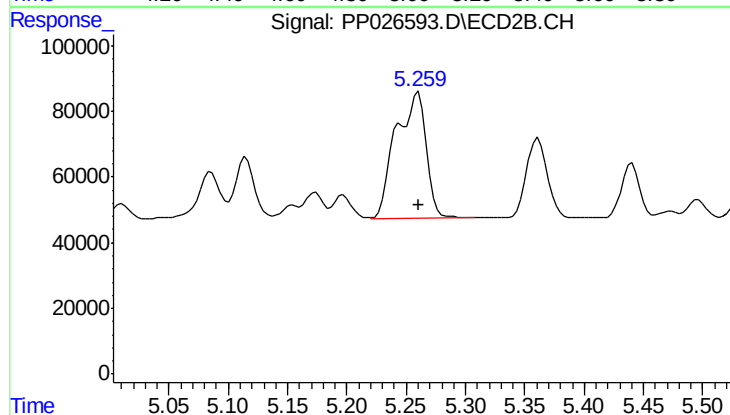


#5 Aroclor-1016-3

R.T.: 5.260 min
Delta R.T.: 0.000 min
Response: 676666
Conc: 132.33 ng/ml

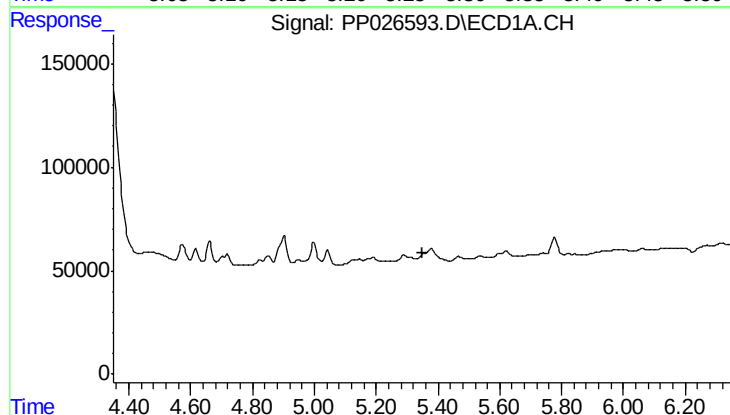


#6 Aroclor-1016-4

R.T.: 0.000 min
Exp R.T.: 5.349 min
Response: 0
Conc: N.D.

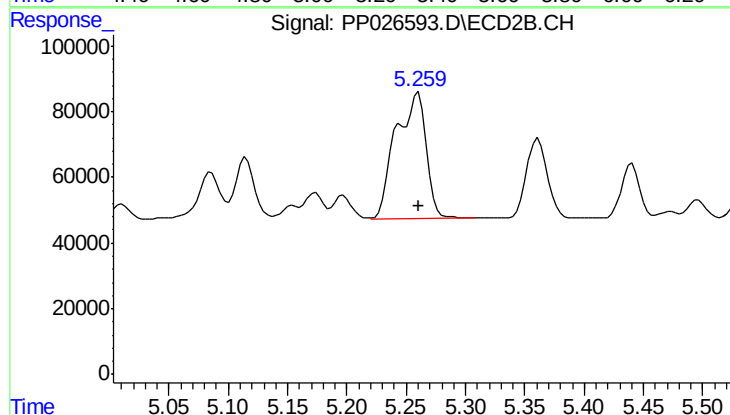

#6 Aroclor-1016-4


R.T.: 5.260 min
Delta R.T.: 0.000 min
Response: 676666
Conc: 83.92 ng/ml

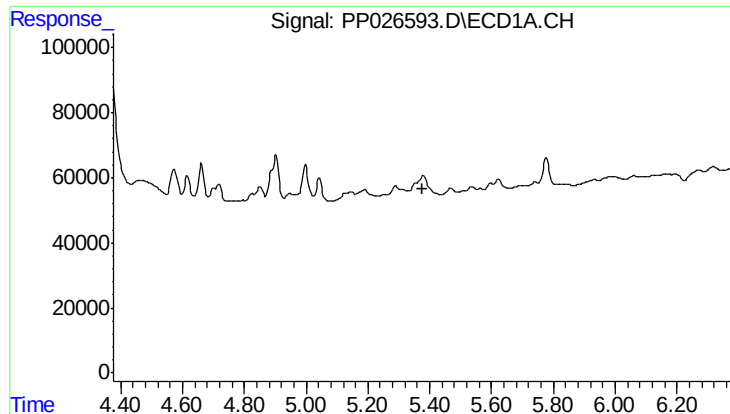

#7 Aroclor-1016-5


R.T.: 0.000 min
Exp R.T.: 5.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
AR1221ICC500

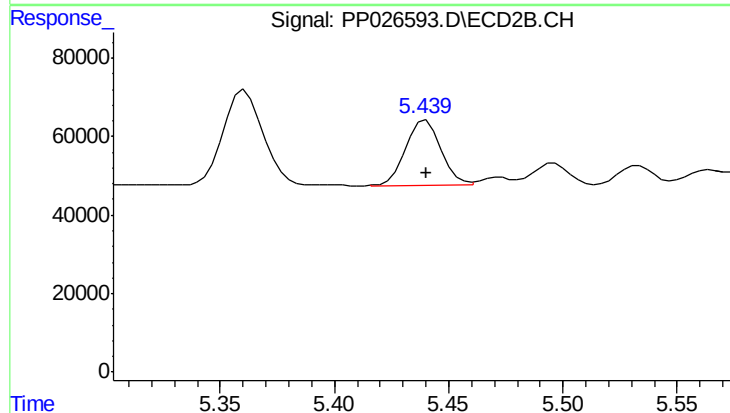


#7 Aroclor-1016-5

R.T.: 5.440 min
Delta R.T.: 0.000 min
Response: 178840
Conc: 67.31 ng/ml

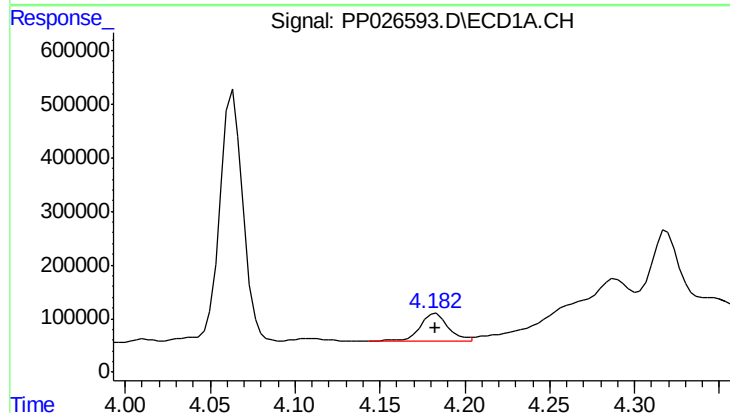


#8 Aroclor-1221-1

R.T.: 4.183 min
Delta R.T.: 0.000 min
Response: 565558
Conc: 500.00 ng/ml

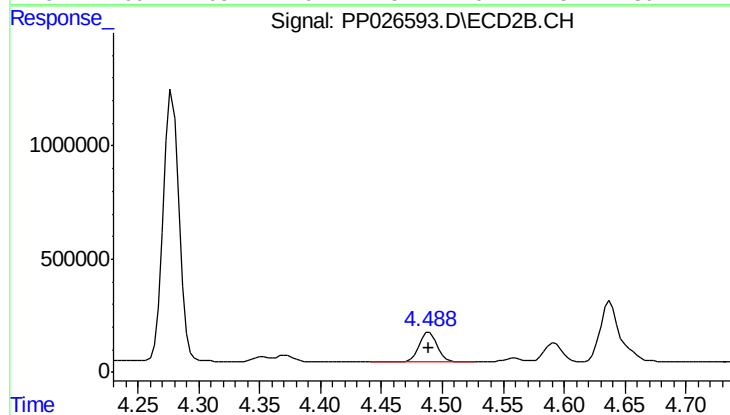

#8 Aroclor-1221-1


R.T.: 4.490 min
Delta R.T.: 0.000 min
Response: 1322702
Conc: 500.00 ng/ml

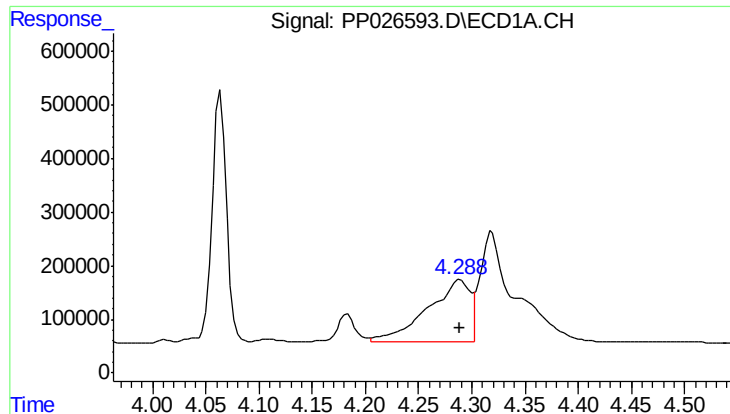

#9 Aroclor-1221-2


R.T.: 4.289 min
Delta R.T.: 0.000 min
Response: 3103278
Conc: 500.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1221ICC500

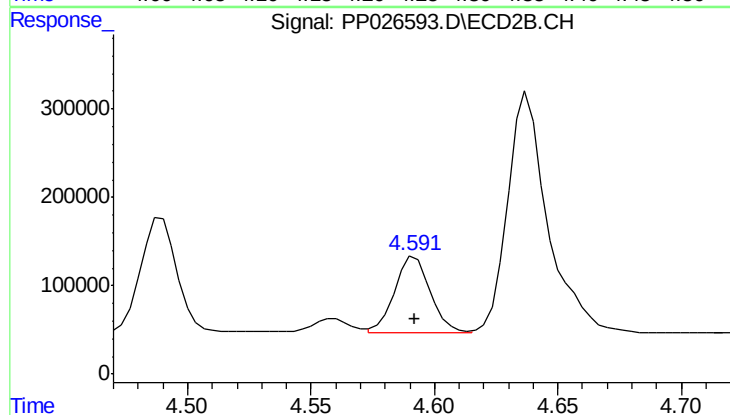


#9 Aroclor-1221-2

R.T.: 4.592 min
Delta R.T.: 0.000 min
Response: 870884
Conc: 500.00 ng/ml

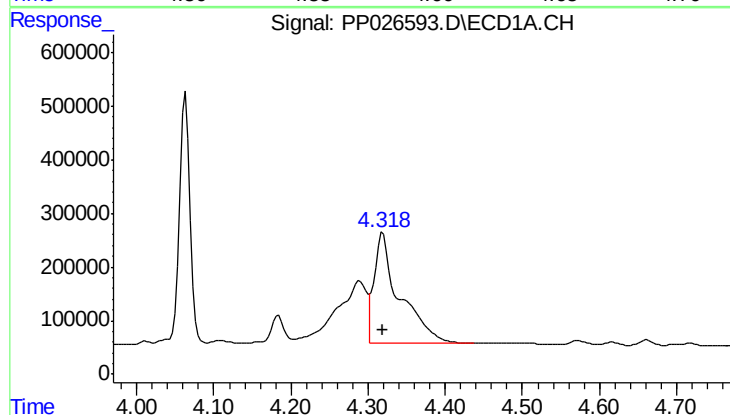

#10 Aroclor-1221-3

R.T.: 4.319 min
Delta R.T.: 0.000 min
Response: 4784543
Conc: 500.00 ng/ml

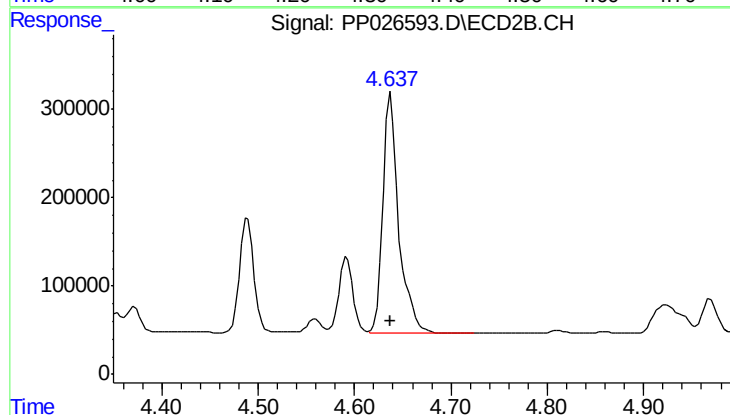

#10 Aroclor-1221-3

R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 3104158
Conc: 500.00 ng/ml