

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062118\
 Data File : PP026586.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2018 13:04
 Operator : UA/AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 05:11:23 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 22 02:45:20 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

7) L1 Aroclor-1...	0.000	5.551	0	92398	N.D.	28.947 #
14) L3 Aroclor-1...	0.000	5.551	0	92398	N.D.	80.001 #
21) L5 Aroclor-1...	0.000	5.551	0	92398	N.D.	19.594 #
22) L5 Aroclor-1...	0.000	5.551	0	92398	N.D.	24.913 #
24) L5 Aroclor-1...	0.000	5.954	0	131192	N.D.	20.488 #
41) L9 Aroclor-1...	7.393	7.908	933186	388726	42.489	21.463 #
42) L9 Aroclor-1...	7.393	0.000	933186	0	49.542	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062118\
Data File : PP026586.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2018 13:04
Operator : UA/AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 05:11:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062118.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 22 02:45:20 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

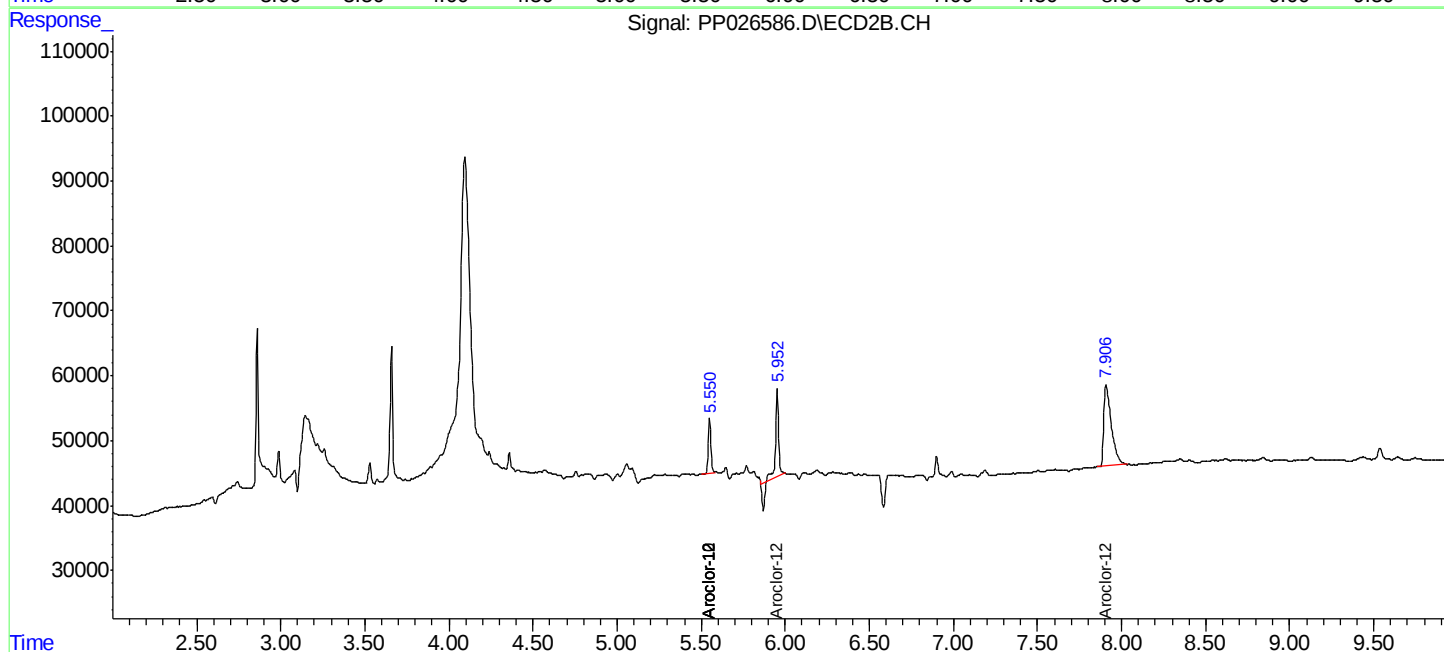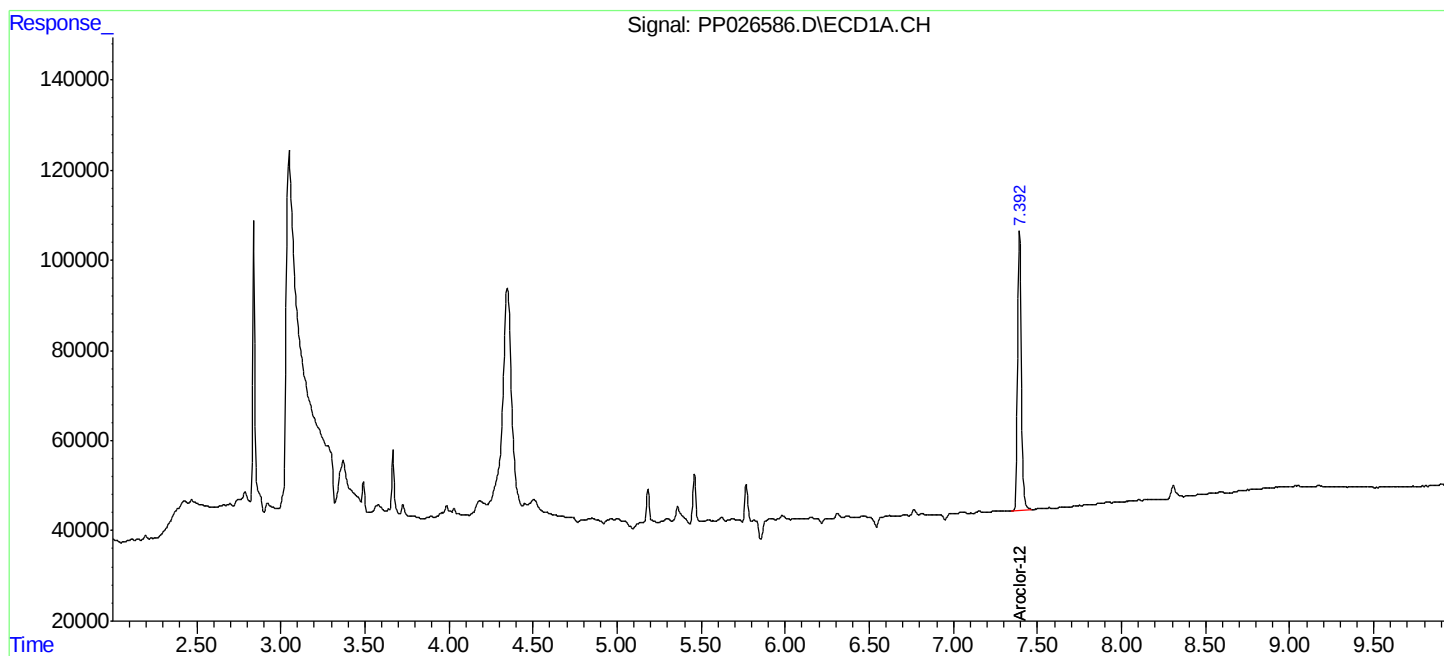


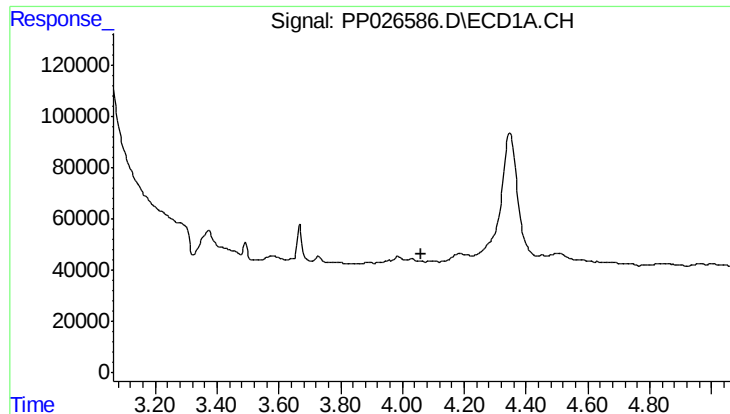

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 4.062 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

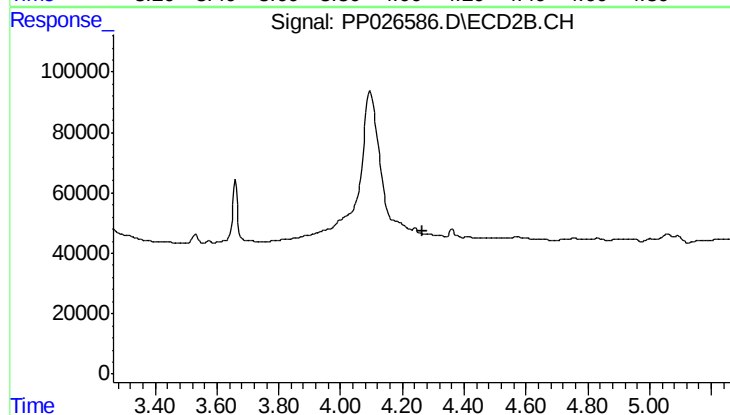


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.263 min
Response: 0
Conc: N.D.

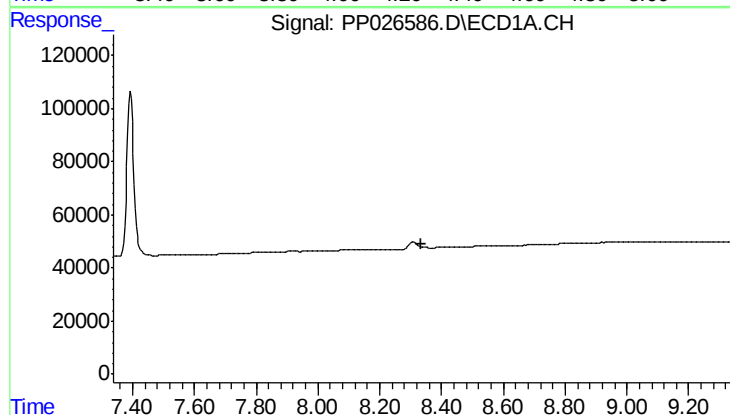


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.336 min
Response: 0
Conc: N.D.

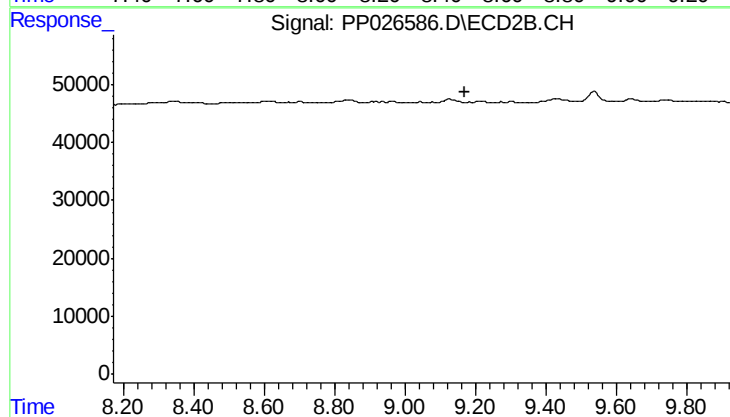

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T.: 9.169 min
Response: 0
Conc: N.D.

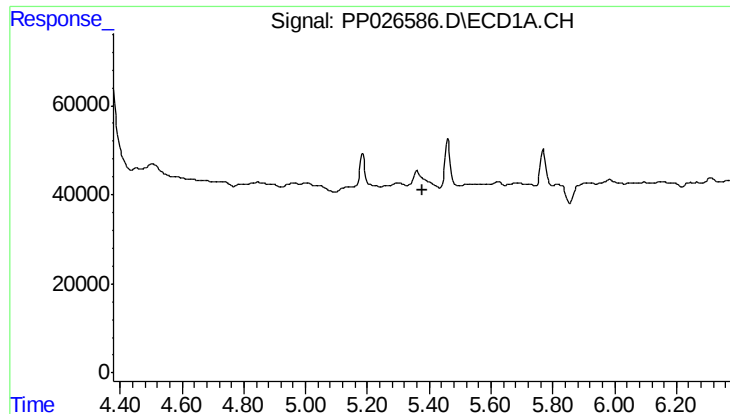

#7 Aroclor-1016-5


R.T.: 0.000 min
Exp R.T.: 5.377 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

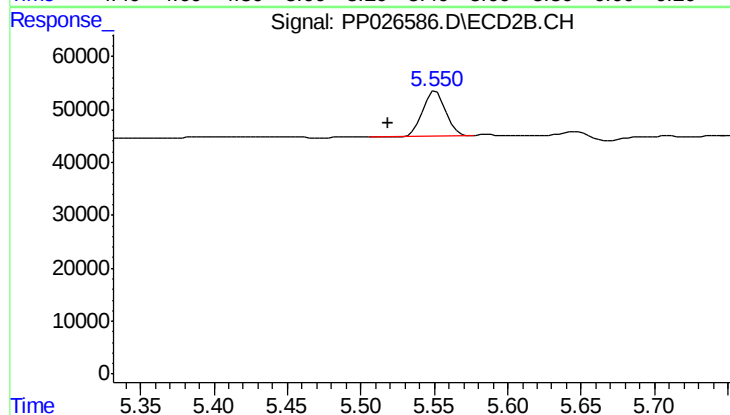


#7 Aroclor-1016-5

R.T.: 5.551 min
Delta R.T.: 0.033 min
Response: 92398
Conc: 28.95 ng/ml

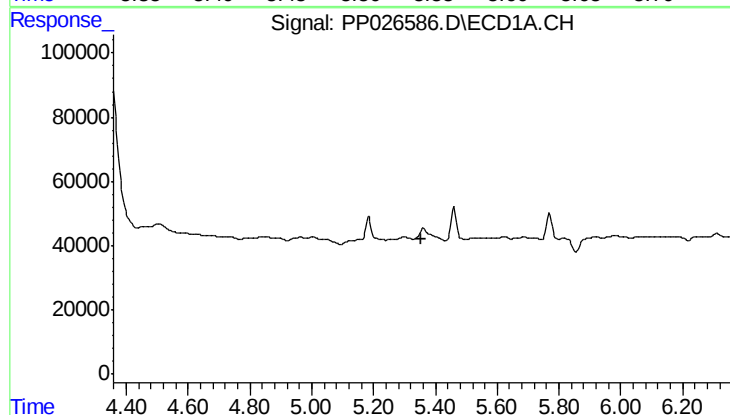


#14 Aroclor-1232-4

R.T.: 0.000 min
Exp R.T.: 5.355 min
Response: 0
Conc: N.D.

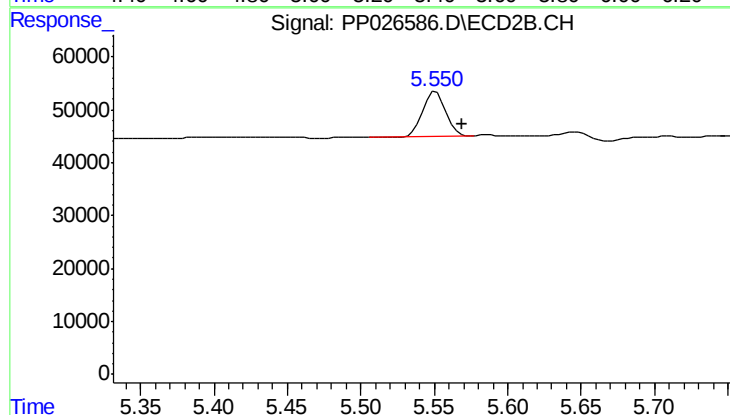

#14 Aroclor-1232-4


R.T.: 5.551 min
Delta R.T.: -0.018 min
Response: 92398
Conc: 80.00 ng/ml

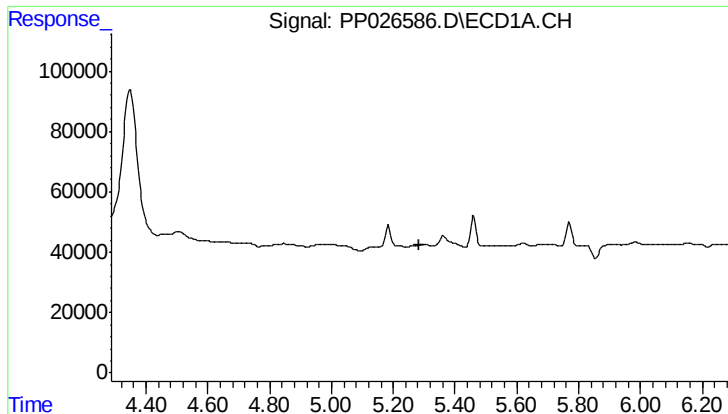

#21 Aroclor-1248-1


R.T.: 0.000 min
Exp R.T.: 5.286 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

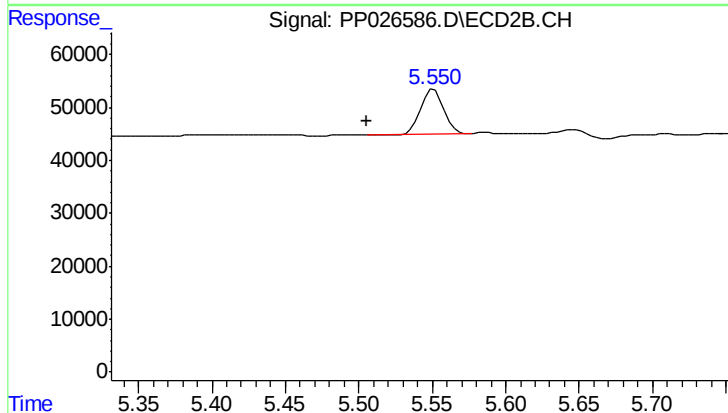


#21 Aroclor-1248-1

R.T.: 5.551 min
Delta R.T.: 0.046 min
Response: 92398
Conc: 19.59 ng/ml

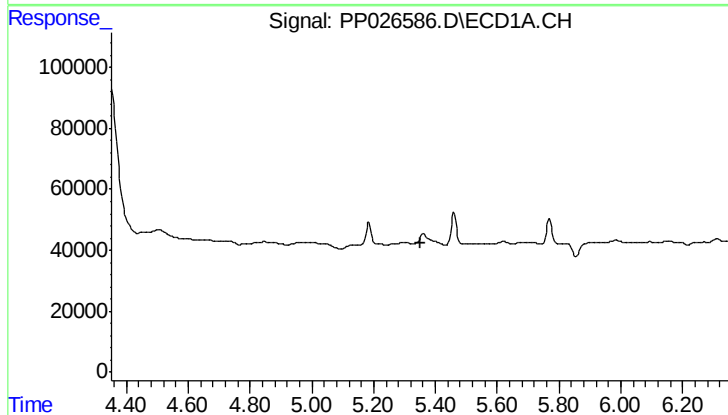


#22 Aroclor-1248-2

R.T.: 0.000 min
Exp R.T.: 5.350 min
Response: 0
Conc: N.D.

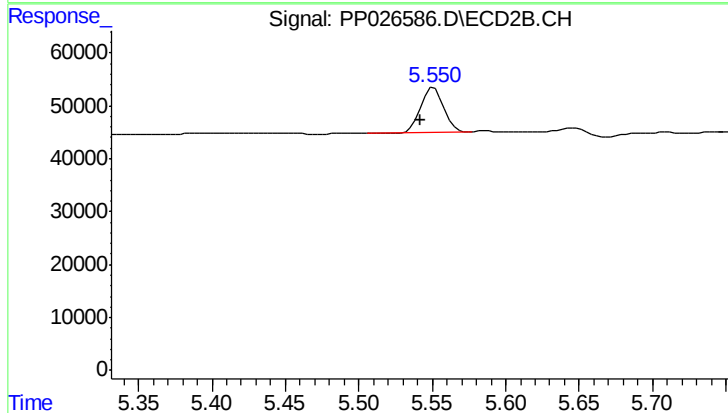

#22 Aroclor-1248-2


R.T.: 5.551 min
Delta R.T.: 0.009 min
Response: 92398
Conc: 24.91 ng/ml

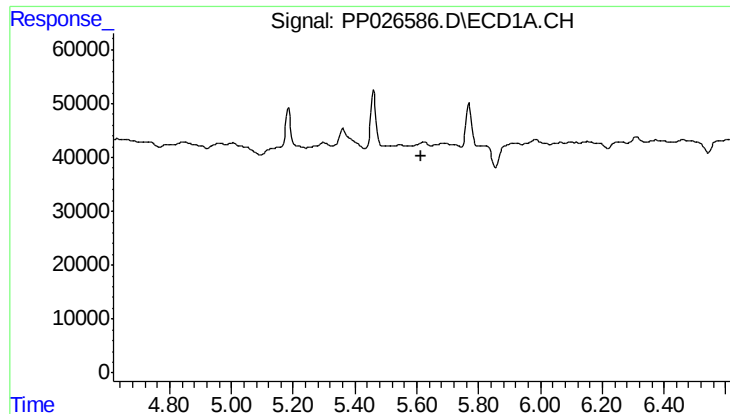

#24 Aroclor-1248-4


R.T.: 0.000 min
Exp R.T.: 5.616 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

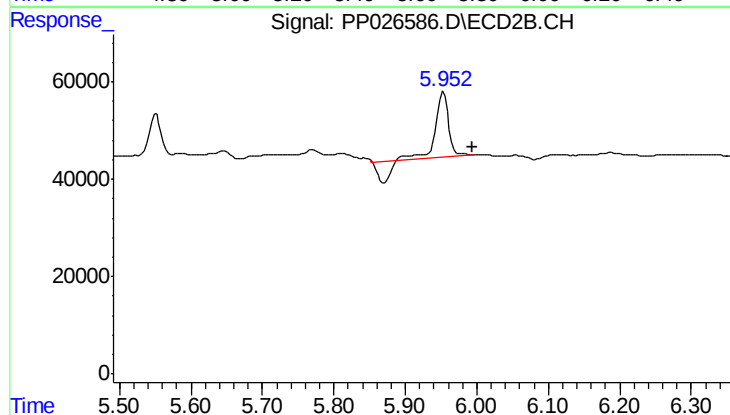


#24 Aroclor-1248-4

R.T.: 5.954 min
Delta R.T.: -0.040 min
Response: 131192
Conc: 20.49 ng/ml

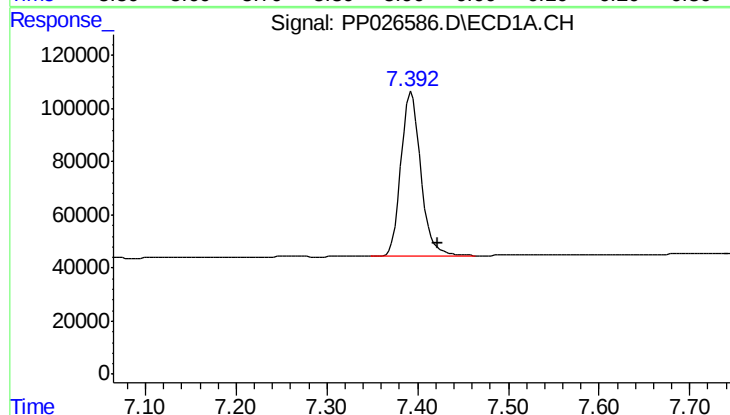


#41 Aroclor-1268-1

R.T.: 7.393 min
Delta R.T.: -0.028 min
Response: 933186
Conc: 42.49 ng/ml

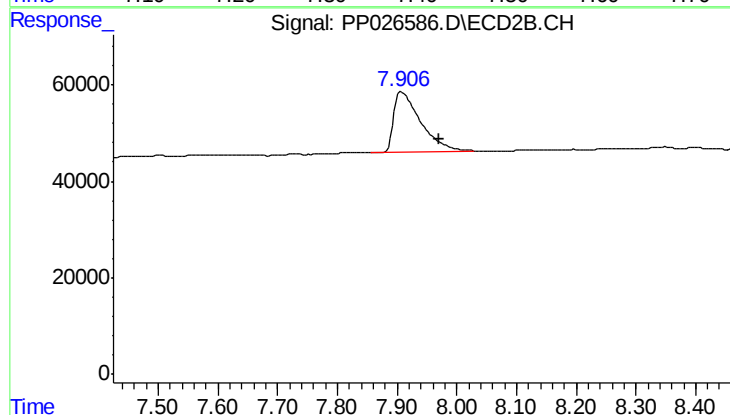

#41 Aroclor-1268-1


R.T.: 7.908 min
Delta R.T.: -0.063 min
Response: 388726
Conc: 21.46 ng/ml

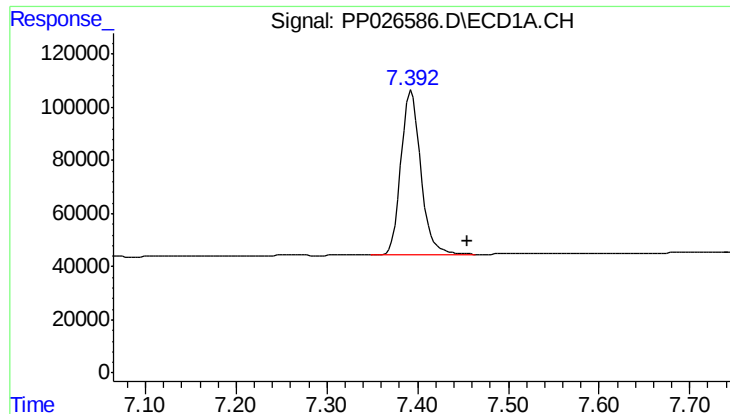

#42 Aroclor-1268-2

R.T.: 7.393 min
Delta R.T.: -0.062 min
Response: 933186
Conc: 49.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

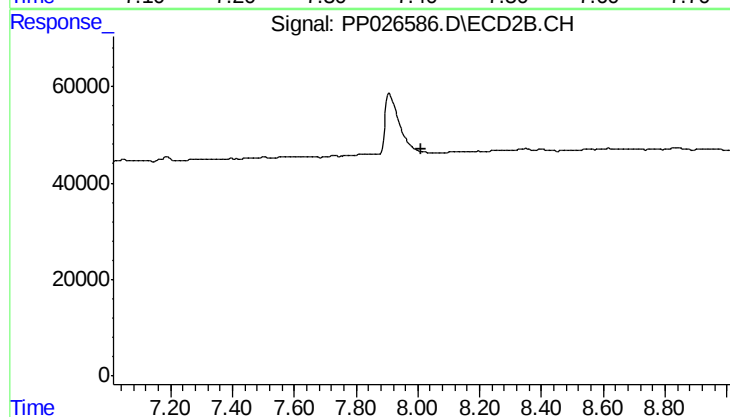

#42 Aroclor-1268-2

R.T.: 0.000 min
Exp R.T. : 8.012 min
Response: 0
Conc: N.D.