

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062118\
 Data File : PP026587.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2018 10:27
 Operator : UA/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

ugo
 6/27/2018 2:35:19 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 05:12:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 22 02:45:20 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.062	4.227	2370315	5865060	24.950	25.174
2) SA Decachlor...	8.331	9.110	4166048	3835841	29.240	26.917m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062118\
Data File : PP026587.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2018 10:27
Operator : UA/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

ugo
6/27/2018 2:35:19 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 05:12:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062118.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 22 02:45:20 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

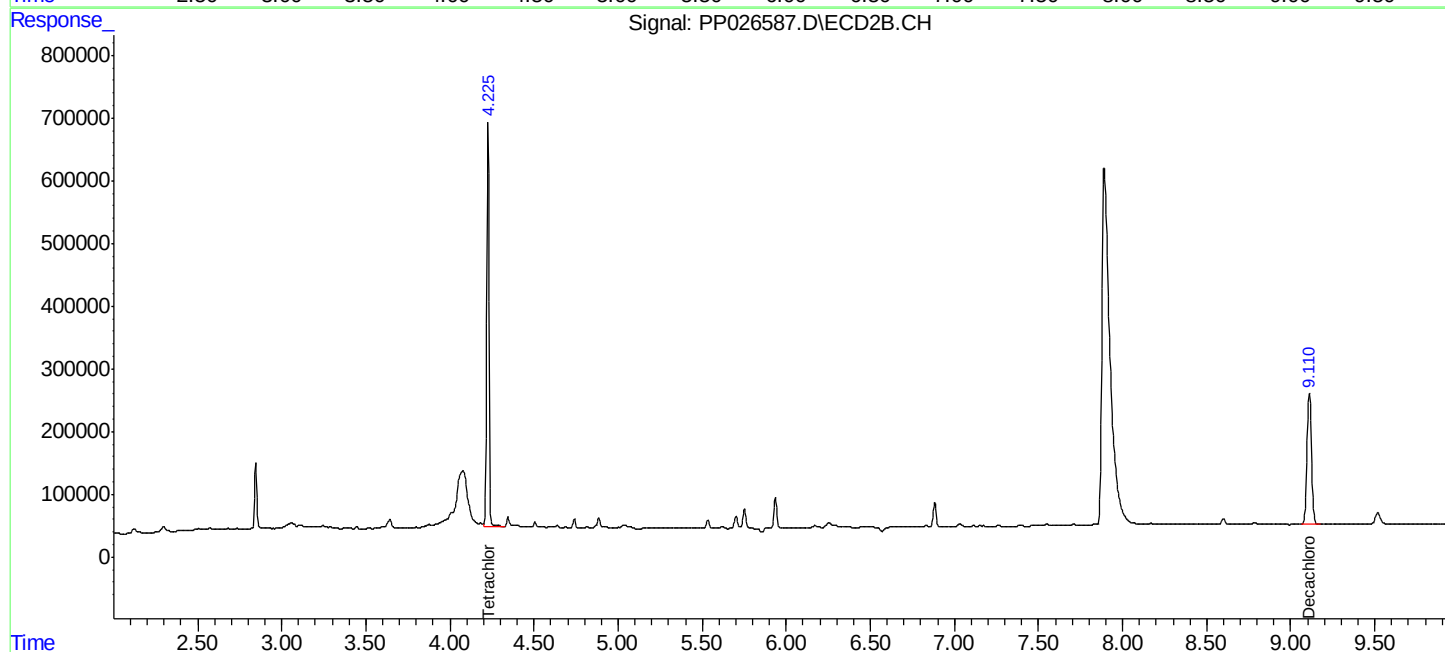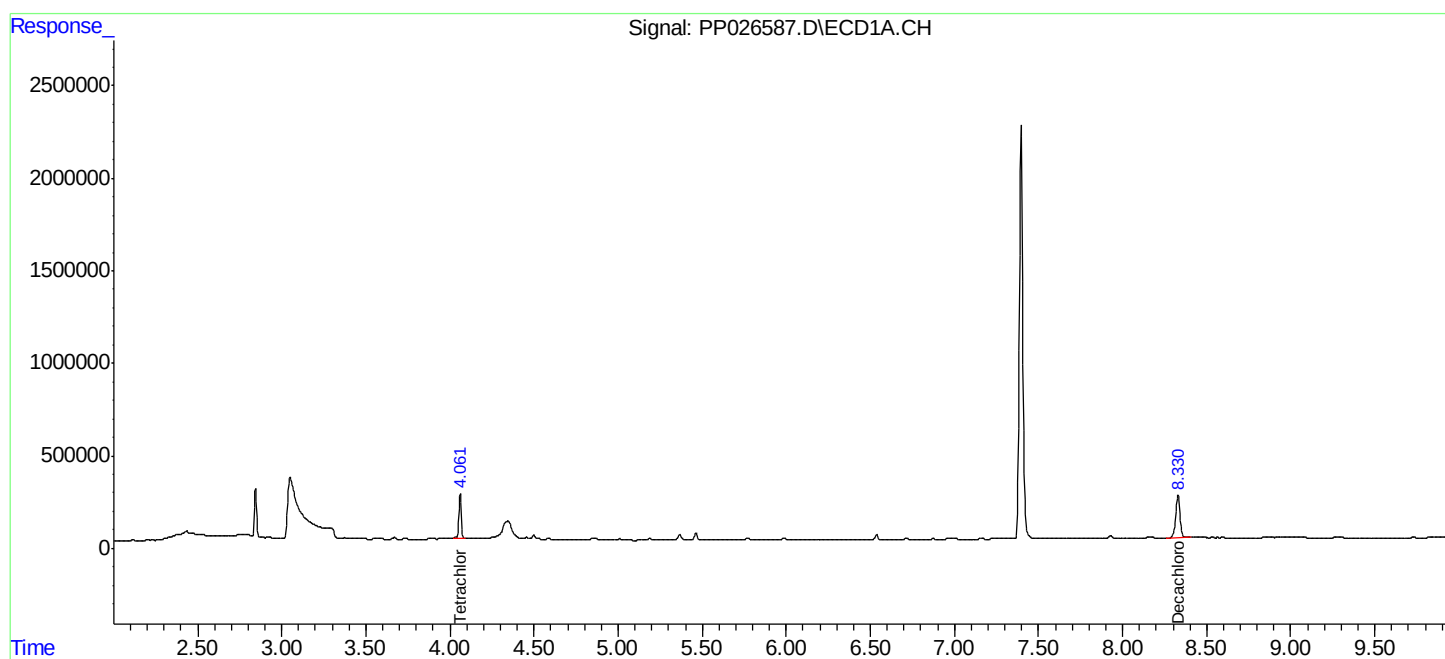

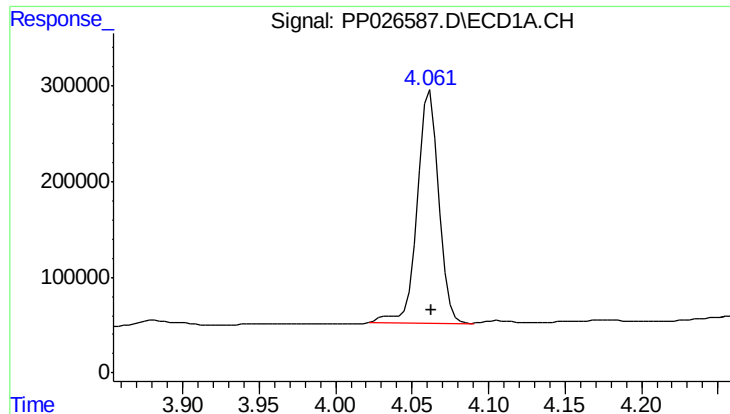


#1 Tetrachloro-m-xylene

R.T.: 4.062 min
Delta R.T.: 0.000 min
Response: 2370315
Conc: 24.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

ugo
6/27/2018 2:35:19 PM

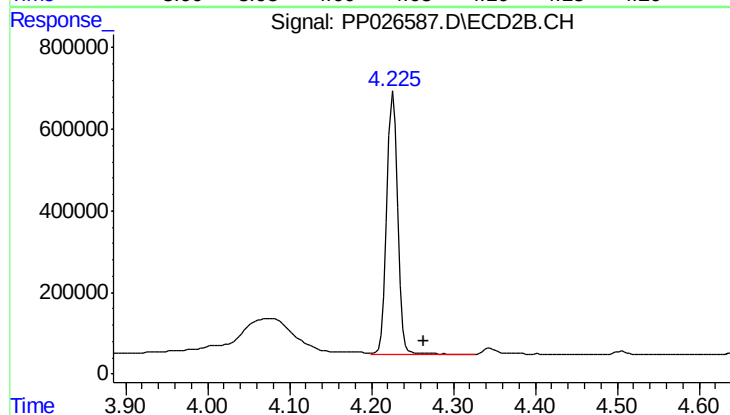


#1 Tetrachloro-m-xylene

R.T.: 4.227 min
Delta R.T.: -0.037 min
Response: 5865060
Conc: 25.17 ng/ml

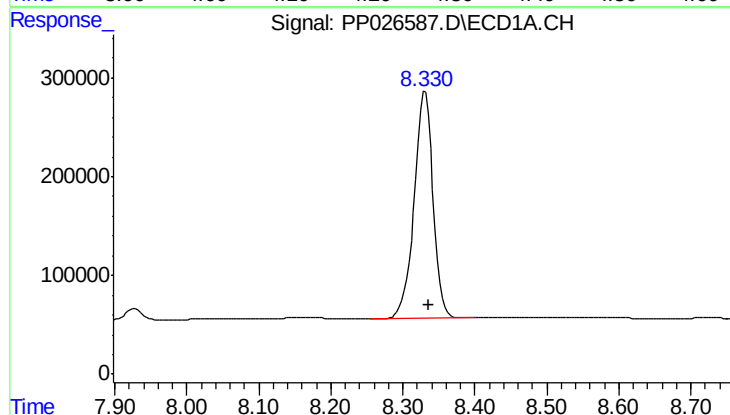

#2 Decachlorobiphenyl

R.T.: 8.331 min
Delta R.T.: -0.005 min
Response: 4166048
Conc: 29.24 ng/ml

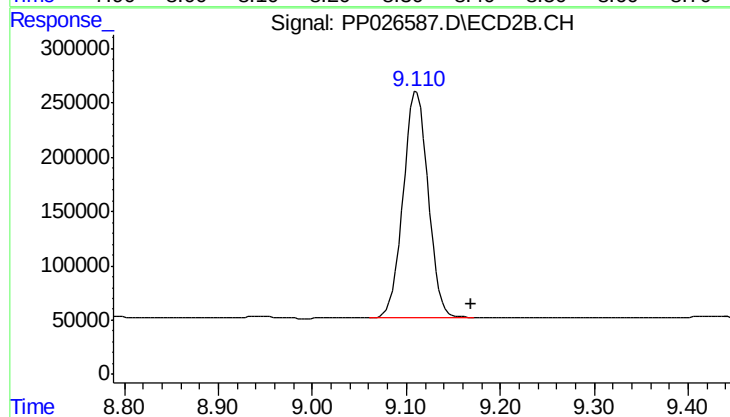

#2 Decachlorobiphenyl

R.T.: 9.110 min
Delta R.T.: -0.059 min
Response: 3835841
Conc: 26.92 ng/ml m