

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062118\
 Data File : PP026600.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2018 17:06
 Operator : UA/AJ
 Sample : PP062118ICV500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 ICVPP062118

Manual Integrations
 APPROVED

ugo
 6/27/2018 2:35:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 02:48:54 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 22 02:45:20 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.061	4.299	4837222	12195030	50.916	52.343
2)	SA Decachlor...	8.334	9.227	7437867	7525181	52.204	52.807
Target Compounds							
3)	L1 Aroclor-1...	4.716	4.952	578542	3944560	525.271	526.022
4)	L1 Aroclor-1...	4.995	5.110	1395732	1204527	515.028	418.135
5)	L1 Aroclor-1...	5.040	5.268	986939	3480930	527.920	565.898m
6)	L1 Aroclor-1...	5.350	5.283	672408	4923343	517.165	504.332m
7)	L1 Aroclor-1...	5.377	5.521	779908	1739163	499.128	544.845
31)	L7 Aroclor-1...	6.193	6.578	1777884	2121723	493.929	538.858m
32)	L7 Aroclor-1...	6.628	6.706	4621934	3980512	515.840	491.960m
33)	L7 Aroclor-1...	6.715	6.998	3305421	3343259	522.056	500.992m
34)	L7 Aroclor-1...	6.915	7.481	2599646	3746697	518.582	518.063
35)	L7 Aroclor-1...	7.160	7.672	9437142	8203536	525.042	528.246

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062118\
Data File : PP026600.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2018 17:06
Operator : UA/AJ
Sample : PP062118ICV500
Misc :
ALS Vial : 3 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
ICVPP062118


Manual Integrations
APPROVED

ugo
6/27/2018 2:35:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 02:48:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062118.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 22 02:45:20 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

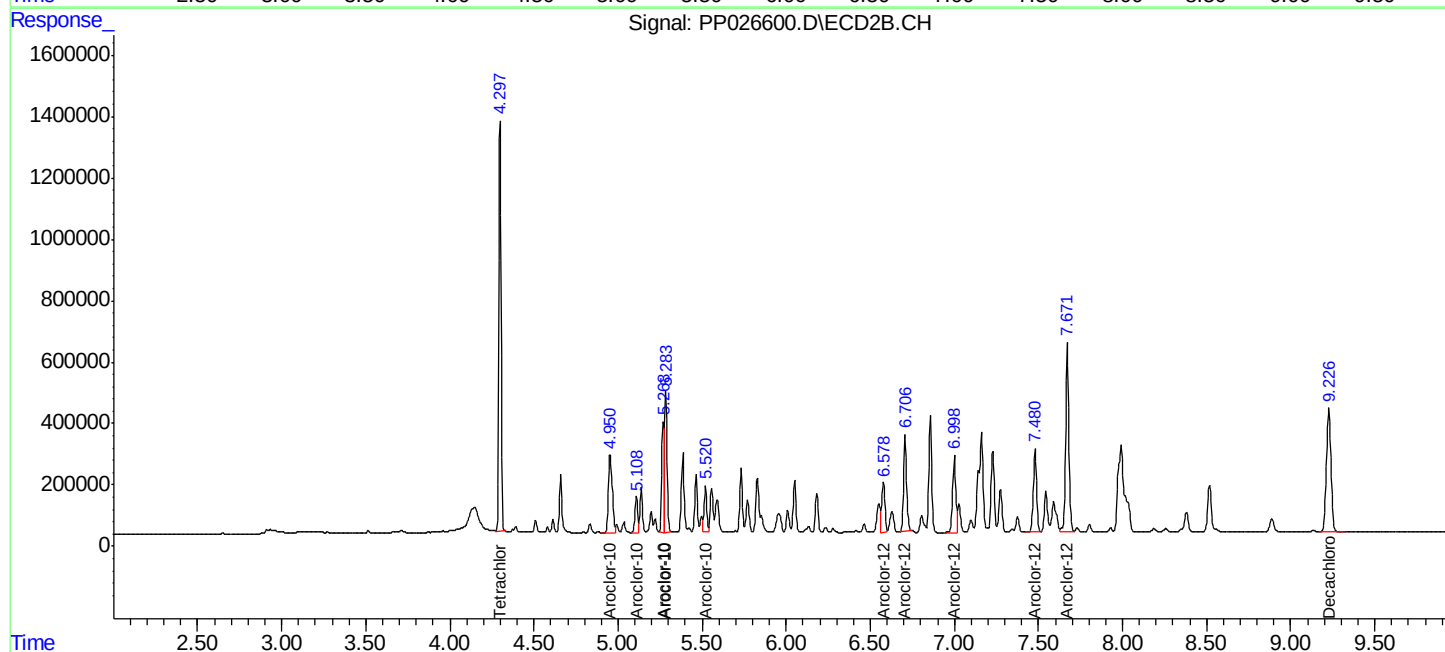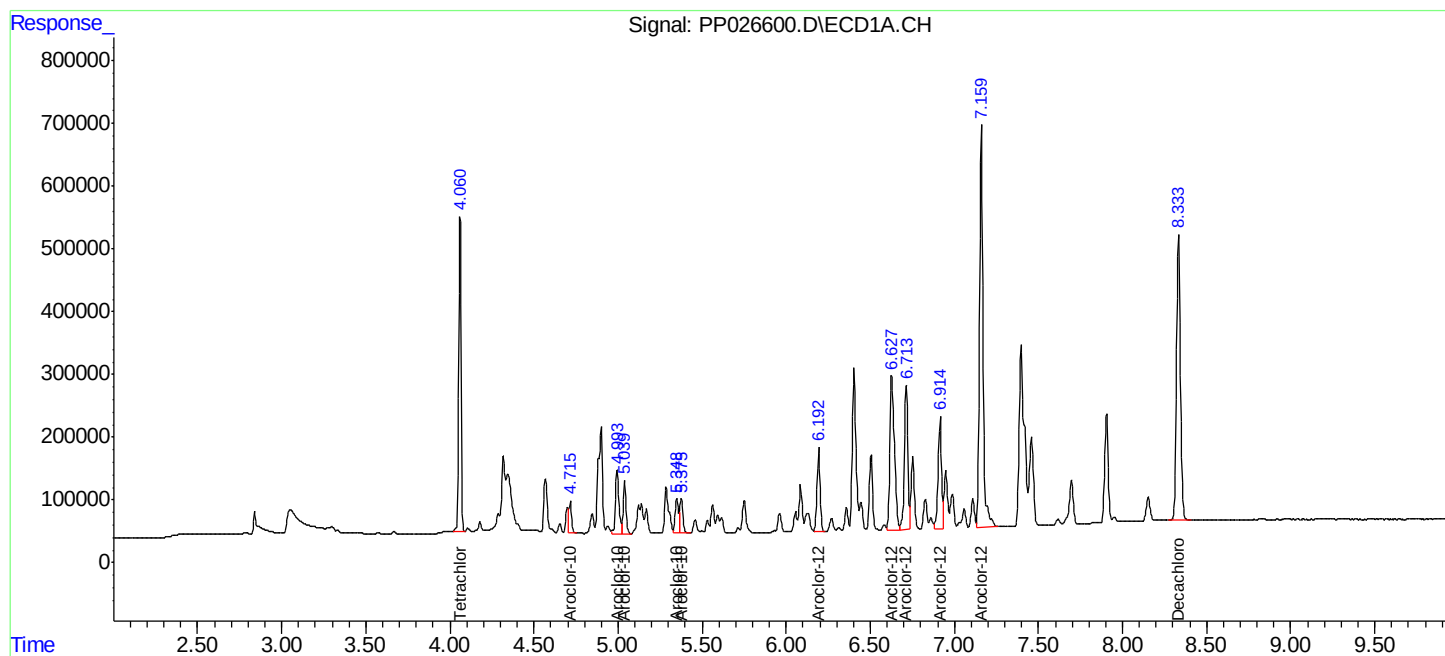

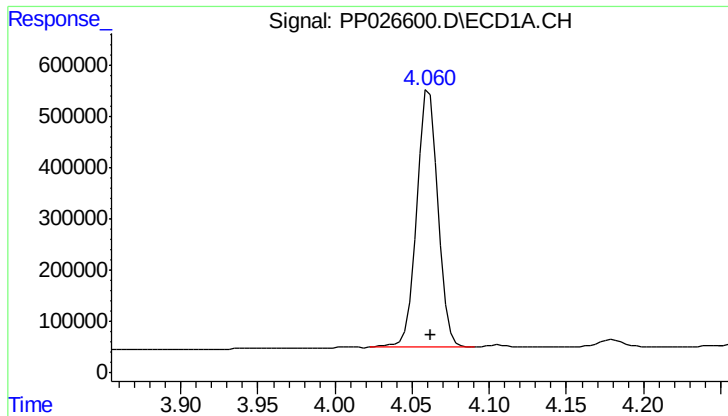


#1 Tetrachloro-m-xylene

R.T.: 4.061 min
Delta R.T.: -0.001 min
Response: 4837222
Conc: 50.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
ICVPP062118


Manual Integrations
APPROVED

ugo
6/27/2018 2:35:41 PM

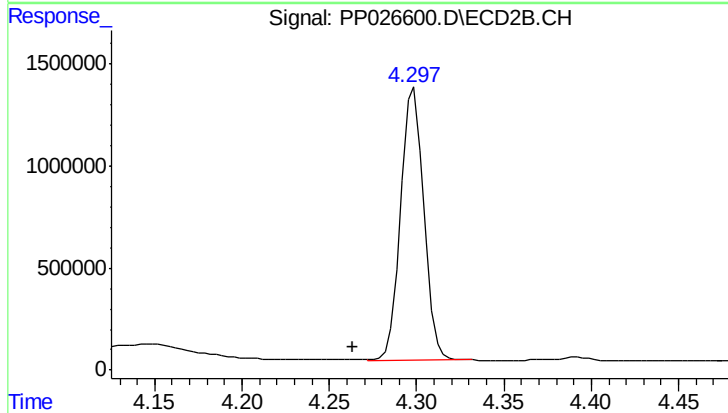


#1 Tetrachloro-m-xylene

R.T.: 4.299 min
Delta R.T.: 0.036 min
Response: 12195030
Conc: 52.34 ng/ml

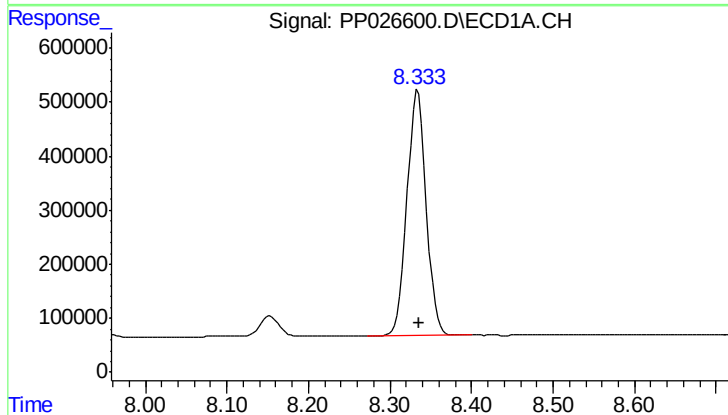


#2 Decachlorobiphenyl

R.T.: 8.334 min
Delta R.T.: -0.002 min
Response: 7437867
Conc: 52.20 ng/ml

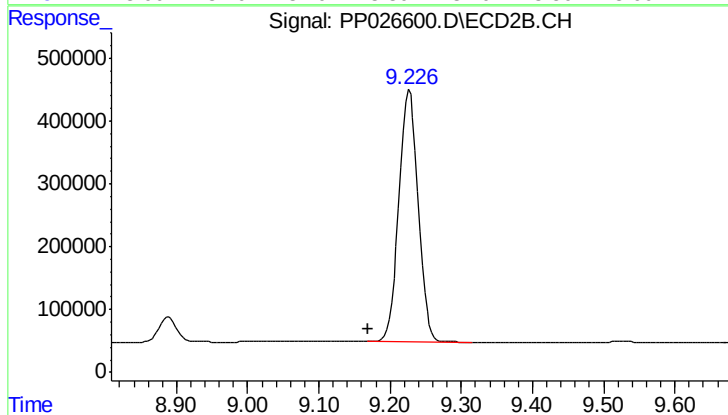

#2 Decachlorobiphenyl

R.T.: 9.227 min
Delta R.T.: 0.058 min
Response: 7525181
Conc: 52.81 ng/ml

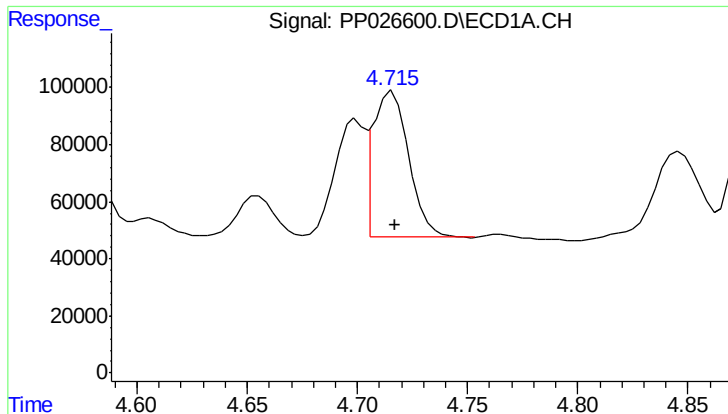


#3 Aroclor-1016-1

R.T.: 4.716 min
Delta R.T.: -0.001 min
Response: 578542
Conc: 525.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
ICVPP062118


Manual Integrations
APPROVED

ugo
6/27/2018 2:35:41 PM

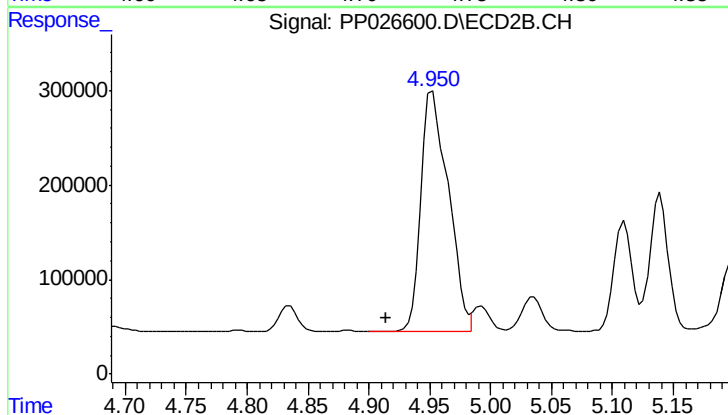


#3 Aroclor-1016-1

R.T.: 4.952 min
Delta R.T.: 0.038 min
Response: 3944560
Conc: 526.02 ng/ml

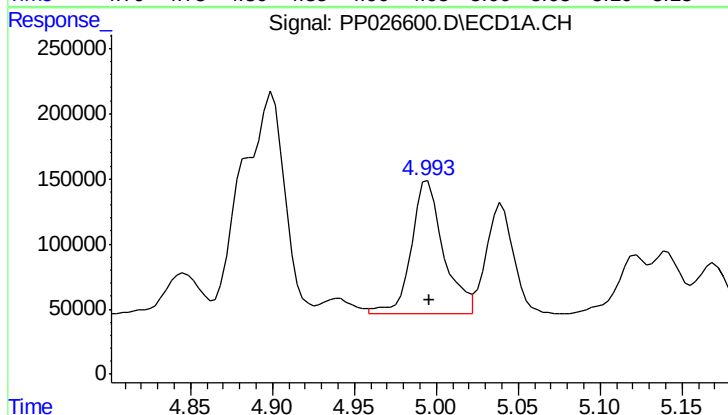


#4 Aroclor-1016-2

R.T.: 4.995 min
Delta R.T.: -0.001 min
Response: 1395732
Conc: 515.03 ng/ml

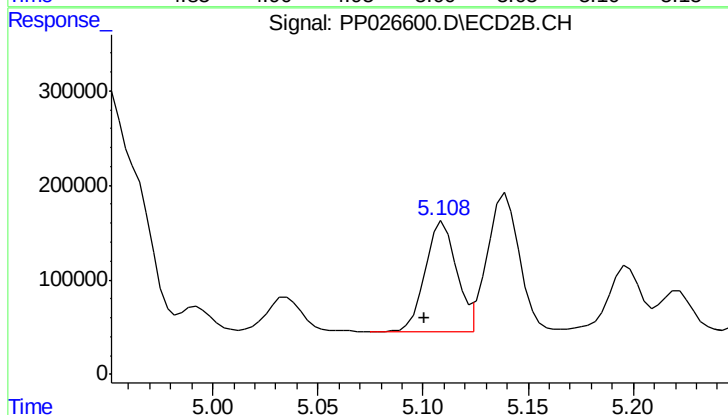

#4 Aroclor-1016-2

R.T.: 5.110 min
Delta R.T.: 0.009 min
Response: 1204527
Conc: 418.14 ng/ml

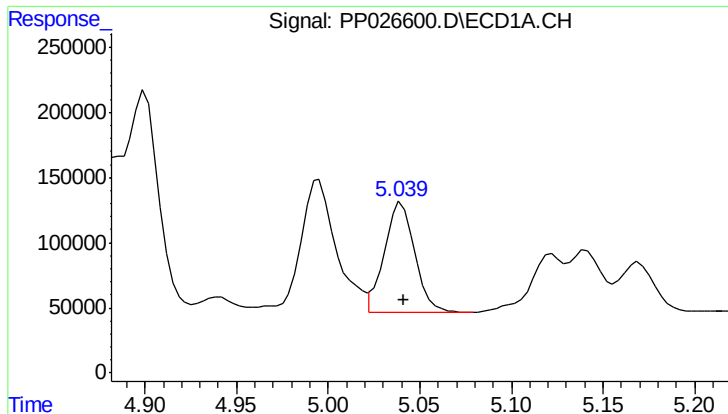


#5 Aroclor-1016-3

R.T.: 5.040 min
Delta R.T.: -0.001 min
Response: 986939
Conc: 527.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
ICVPP062118


Manual Integrations
APPROVED

ugo
6/27/2018 2:35:41 PM

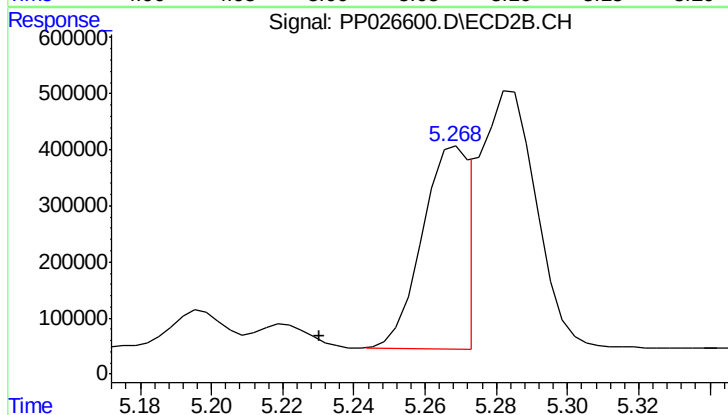


#5 Aroclor-1016-3

R.T.: 5.268 min
Delta R.T.: 0.037 min
Response: 3480930
Conc: 565.90 ng/ml m

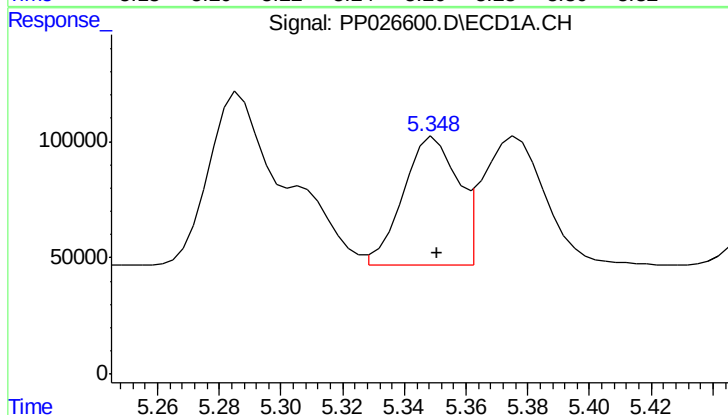


#6 Aroclor-1016-4

R.T.: 5.350 min
Delta R.T.: 0.000 min
Response: 672408
Conc: 517.17 ng/ml

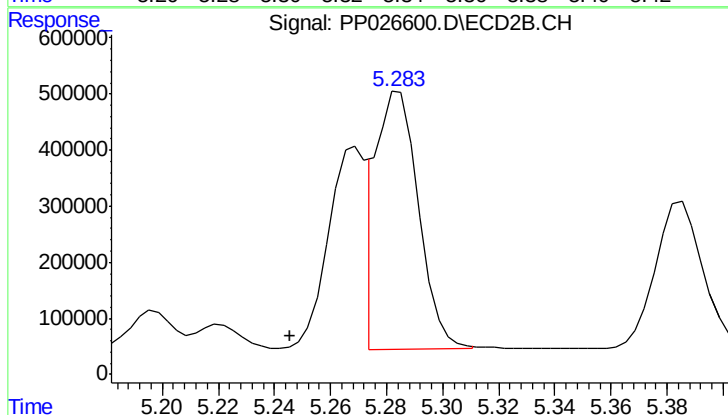

#6 Aroclor-1016-4

R.T.: 5.283 min
Delta R.T.: 0.038 min
Response: 4923343
Conc: 504.33 ng/ml m

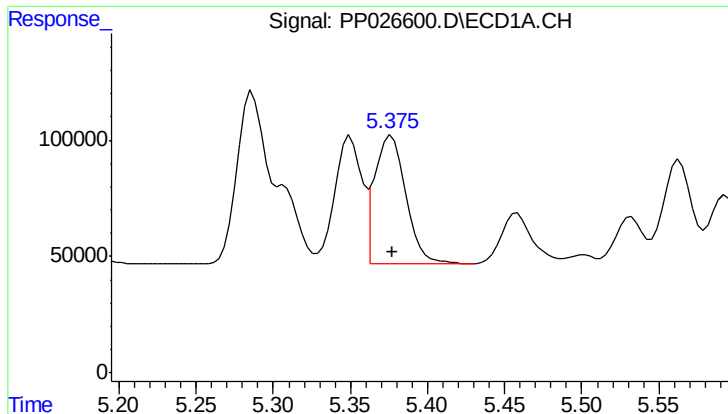


#7 Aroclor-1016-5

R.T.: 5.377 min
Delta R.T.: 0.000 min
Response: 779908
Conc: 499.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
ICVPP062118


Manual Integrations
APPROVED

ugo
6/27/2018 2:35:41 PM

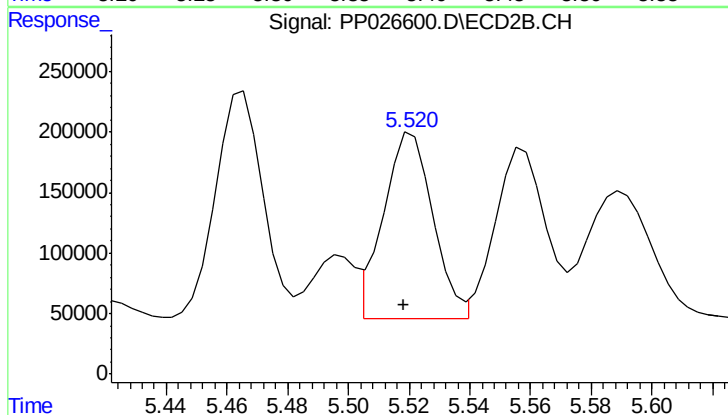


#7 Aroclor-1016-5

R.T.: 5.521 min
Delta R.T.: 0.003 min
Response: 1739163
Conc: 544.85 ng/ml

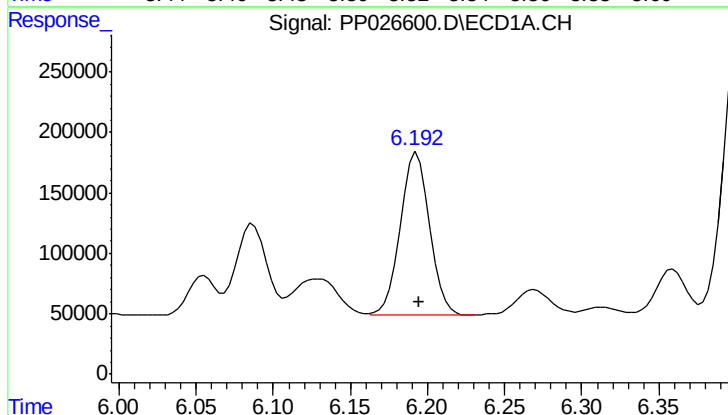


#31 Aroclor-1260-1

R.T.: 6.193 min
Delta R.T.: -0.001 min
Response: 1777884
Conc: 493.93 ng/ml

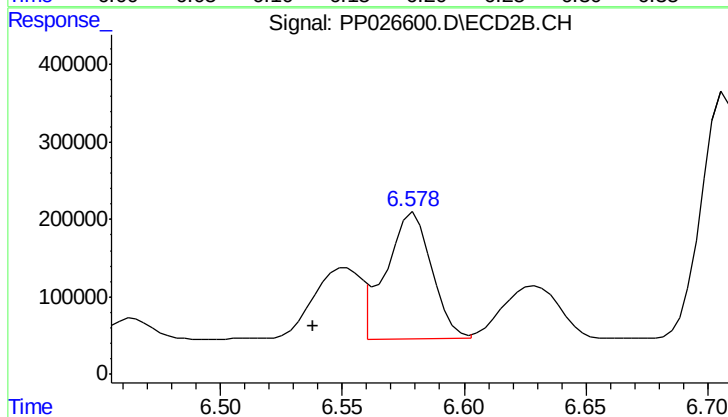

#31 Aroclor-1260-1

R.T.: 6.578 min
Delta R.T.: 0.040 min
Response: 2121723
Conc: 538.86 ng/ml m

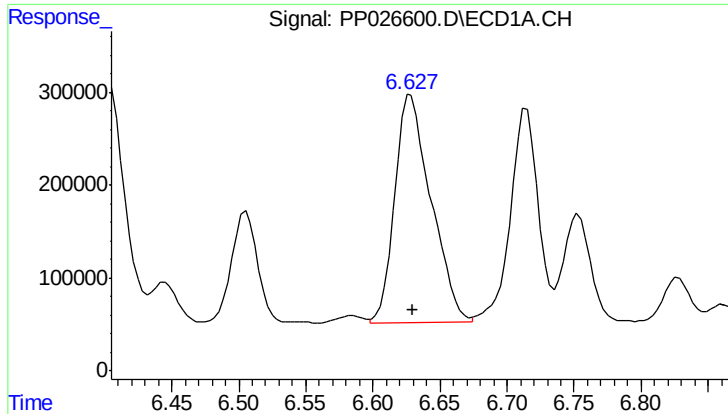


#32 Aroclor-1260-2

R.T.: 6.628 min
Delta R.T.: -0.001 min
Response: 4621934
Conc: 515.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
ICVPP062118


Manual Integrations
APPROVED

ugo
6/27/2018 2:35:41 PM

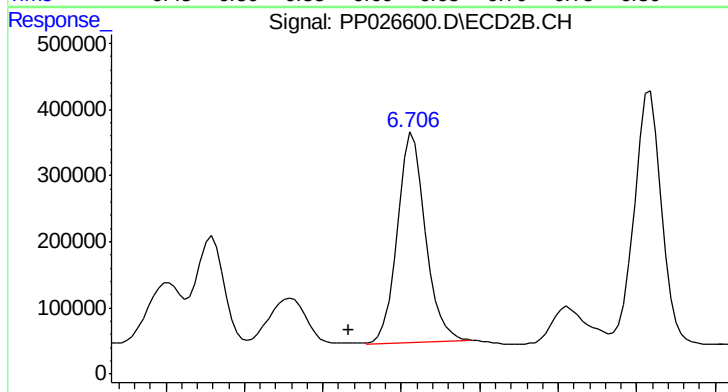


#32 Aroclor-1260-2

R.T.: 6.706 min
Delta R.T.: 0.039 min
Response: 3980512
Conc: 491.96 ng/ml m

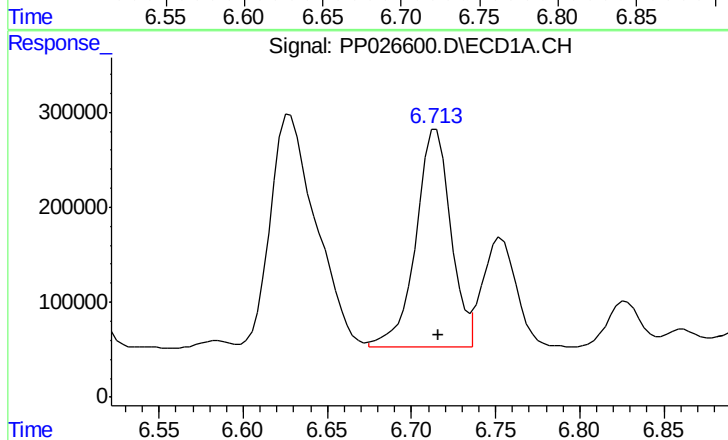


#33 Aroclor-1260-3

R.T.: 6.715 min
Delta R.T.: -0.001 min
Response: 3305421
Conc: 522.06 ng/ml

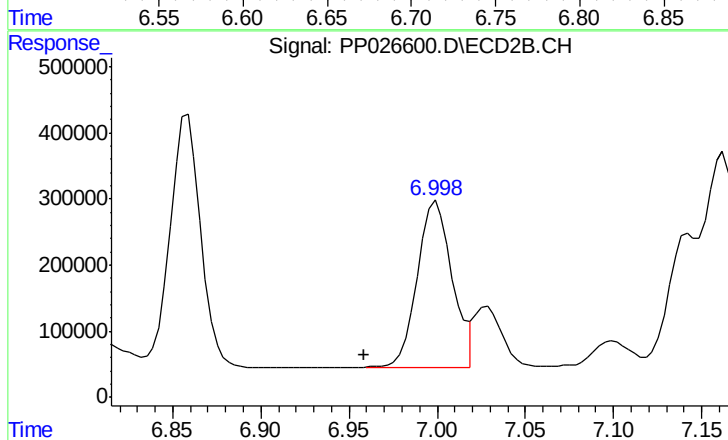

#33 Aroclor-1260-3

R.T.: 6.998 min
Delta R.T.: 0.040 min
Response: 3343259
Conc: 500.99 ng/ml m

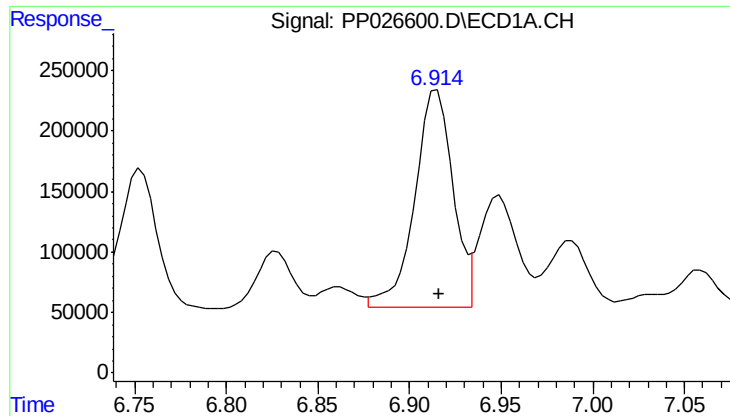


#34 Aroclor-1260-4

R.T.: 6.915 min
Delta R.T.: -0.001 min
Response: 2599646
Conc: 518.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
ICVPP062118


Manual Integrations
APPROVED

ugo
6/27/2018 2:35:41 PM

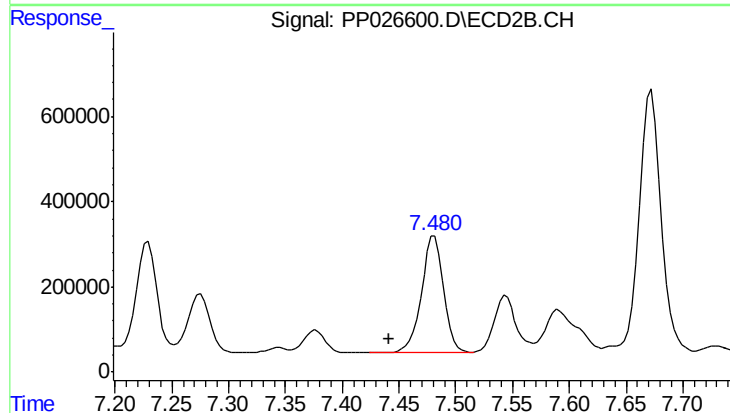


#34 Aroclor-1260-4

R.T.: 7.481 min
Delta R.T.: 0.040 min
Response: 3746697
Conc: 518.06 ng/ml

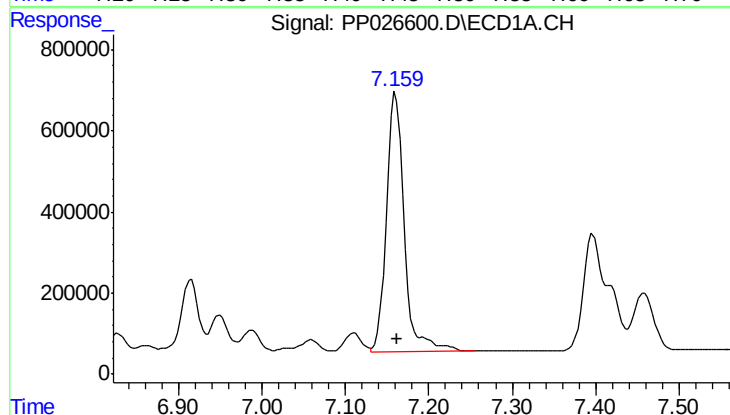

#35 Aroclor-1260-5

R.T.: 7.160 min
Delta R.T.: -0.002 min
Response: 9437142
Conc: 525.04 ng/ml

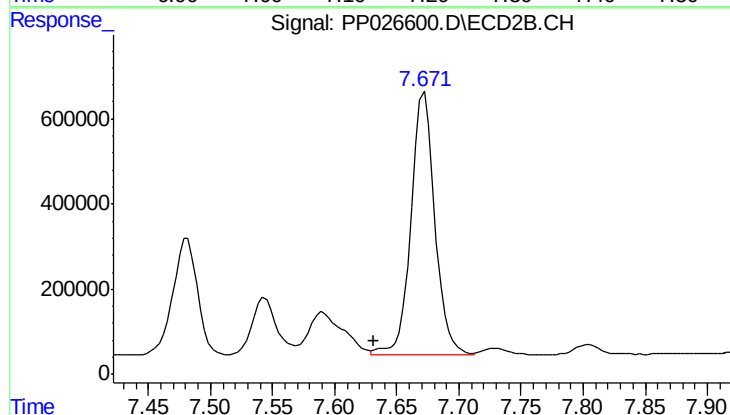

#35 Aroclor-1260-5

R.T.: 7.672 min
Delta R.T.: 0.040 min
Response: 8203536
Conc: 528.25 ng/ml