

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080622\
 Data File : PP050246.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2022 12:24
 Operator : YP\AJ
 Sample : N3980-07
 Misc : AR1660 LOD 25 PPB
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 00:19:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Aug 07 23:52:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.346	3.592	39453110	81914622	24.510	26.152
2)	SA Decachlor...	10.093	8.557	45849224	39293637	26.037	25.531
Target Compounds							
3)	L1 AR-1016-1	5.524	4.665	2251728	4211565	35.961	41.434
4)	L1 AR-1016-2	5.545	4.684	3223272	5715951	36.399	39.518
5)	L1 AR-1016-3	5.607	4.859	1915036	3103372	35.040	40.897
6)	L1 AR-1016-4	5.708	4.900	1673928	2517947	36.300	43.215
7)	L1 AR-1016-5	6.002	5.112	1722824	3645699	38.559	47.715
8)	L2 AR-1221-1	0.000	3.800	0	392158	N.D.	10.260 #
9)	L2 AR-1221-2	0.000	3.888	0	1792377	N.D.	62.768 #
10)	L2 AR-1221-3	0.000	3.963	0	3055549	N.D.	35.691 #
11)	L3 AR-1232-1	0.000	3.963	0	3055549	N.D.	43.770 #
12)	L3 AR-1232-2	5.254	4.684	1677615	5715951	92.631	88.908
13)	L3 AR-1232-3	5.545	4.859	3223272	3103372	81.860	92.527
14)	L3 AR-1232-4	5.708	4.941	1673928	3440640	82.733	116.791 #
15)	L3 AR-1232-5	5.796	5.112	1273199	3645699	81.440	110.709 #
16)	L4 AR-1242-1	5.524	4.665	2251728	4211565	44.429	50.803
17)	L4 AR-1242-2	5.545	4.684	3223272	5715951	44.619	48.946
18)	L4 AR-1242-3	5.607	4.859	1915036	3103372	43.304	50.609
19)	L4 AR-1242-4	5.708	4.941	1673928	3440640	44.921	58.775 #
20)	L4 AR-1242-5	0.000	5.461	0	3783585	N.D.	54.432 #
21)	L5 AR-1248-1	5.524	4.665	2251728	4211565	55.767	63.015
22)	L5 AR-1248-2	5.796	4.900	1273199	2517947	22.790	29.148 #
23)	L5 AR-1248-3	6.002	4.941	1722824	3440640	26.932	37.953 #
24)	L5 AR-1248-4	6.381f	5.112	1237936	3645699	15.650	34.590 #
25)	L5 AR-1248-5	0.000	5.503	0	1260303	N.D.	12.693 #
26)	L6 AR-1254-1	6.381	5.461	1237936	3783585	17.857	28.632 #
27)	L6 AR-1254-2	6.597	5.607	3832579	3539039	36.345	32.476
28)	L6 AR-1254-3	6.973	6.024f	5151581	4514678	45.411	28.366 #
29)	L6 AR-1254-4	0.000	6.266f	0	1626784	N.D.	16.732 #
30)	L6 AR-1254-5	7.675	6.652	19416234	5443639	205.423	44.163 #
31)	L7 AR-1260-1	7.130	6.138	9870747	7521162	108.076	66.373 #
32)	L7 AR-1260-2	7.389	6.325	7911211	8106633	69.245	60.344
33)	L7 AR-1260-3	7.746	6.478	7527531	5152045	88.396	42.768 #
34)	L7 AR-1260-4	7.975	6.948	8773306	2650331	92.169	29.897 #
35)	L7 AR-1260-5	8.294	7.189	7417718	9854475	39.682	50.551 #
36)	L8 AR-1262-1	7.746	6.689	7527531	4356436	62.857	32.236 #
37)	L8 AR-1262-2	8.294	6.948	7417718	2650331	34.330	24.391 #
38)	L8 AR-1262-3	8.624f	7.472	4736492	1711594	48.201	23.585 #
39)	L8 AR-1262-4	8.672f	7.535	4374436	4963691	68.044	36.002 #
40)	L8 AR-1262-5	9.353	8.028	1960424	1661284	24.835	25.794
41)	L9 AR-1268-1	8.624f	7.472	4736492	1711594	18.654	7.789 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080622\
Data File : PP050246.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2022 12:24
Operator : YP\AJ
Sample : N3980-07
Misc : AR1660 LOD 25 PPB
ALS Vial : 46 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 00:19:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Aug 07 23:52:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.672f	7.535	4374436	4963691	17.933	24.921 #
44) L9	AR-1268-4	9.353	8.028	1960424	1661284	22.746	23.381
45) L9	AR-1268-5	9.783f	8.311	1963810	769196	2.944	1.397 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080622\
Data File : PP050246.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2022 12:24
Operator : YP\AJ
Sample : N3980-07
Misc : AR1660 LOD 25 PPB
ALS Vial : 46 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 00:19:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Aug 07 23:52:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

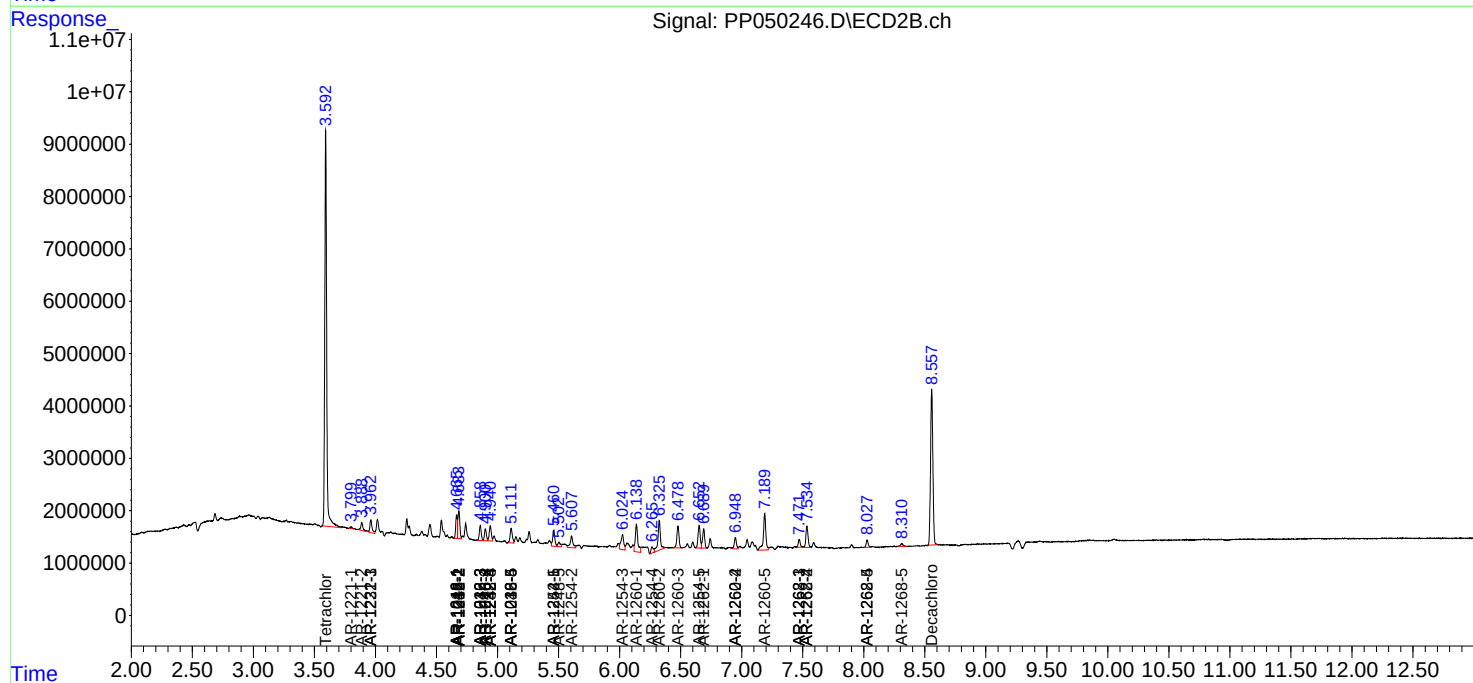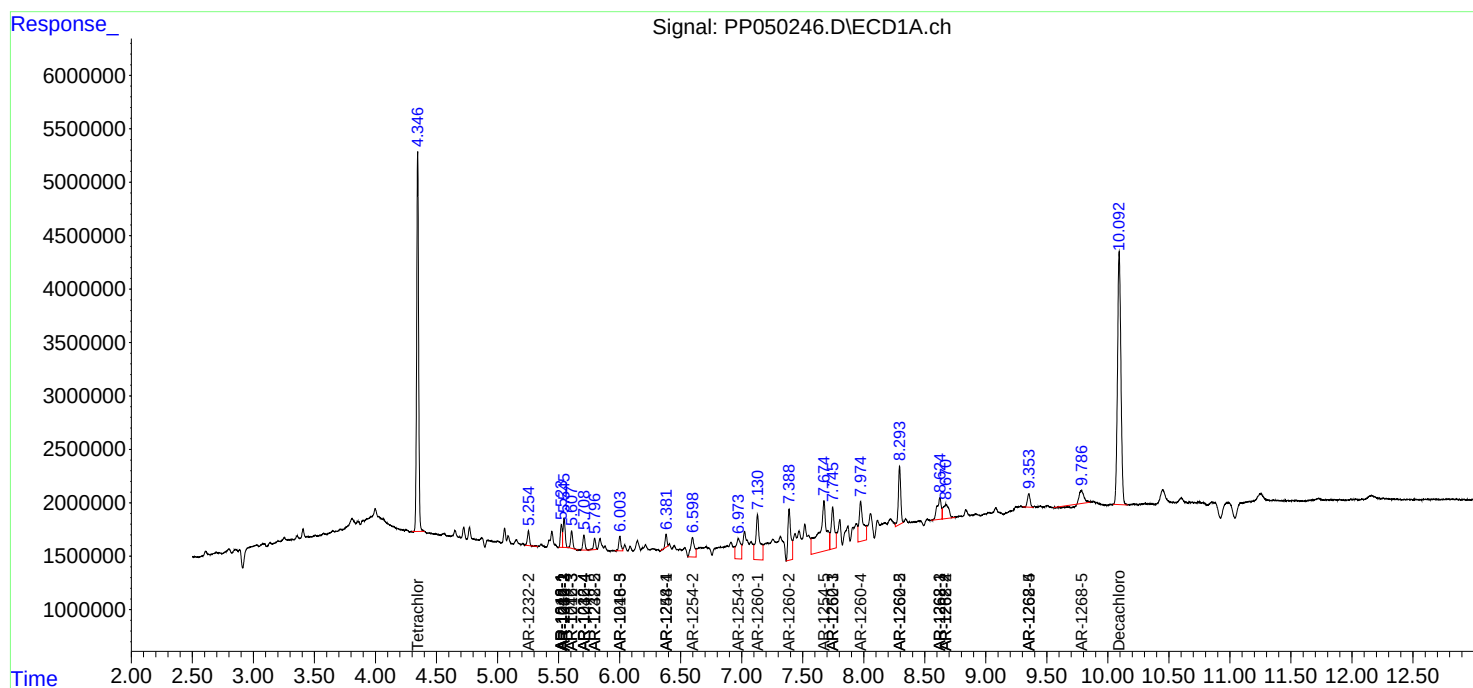


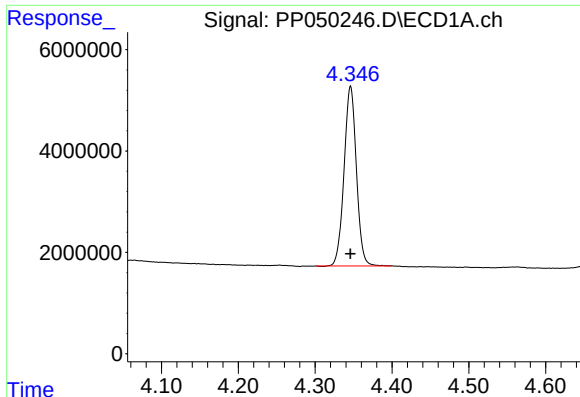

#1 Tetrachloro-m-xylene


R.T.: 4.346 min
Delta R.T.: 0.000 min
Response: 39453110
Conc: 24.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

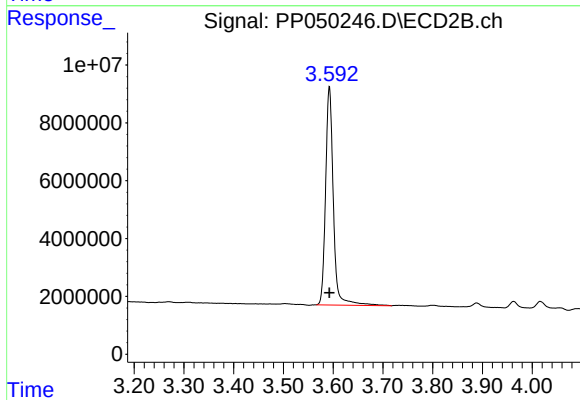


#1 Tetrachloro-m-xylene

R.T.: 3.592 min
Delta R.T.: 0.000 min
Response: 81914622
Conc: 26.15 ng/ml

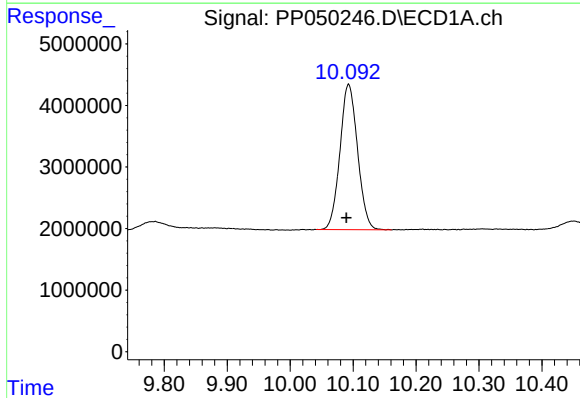


#2 Decachlorobiphenyl

R.T.: 10.093 min
Delta R.T.: 0.003 min
Response: 45849224
Conc: 26.04 ng/ml

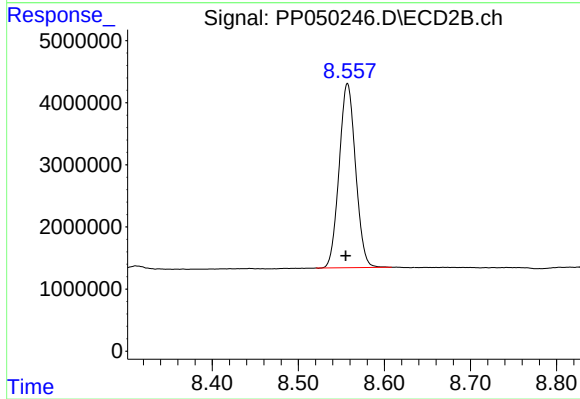

#2 Decachlorobiphenyl


R.T.: 8.557 min
Delta R.T.: 0.002 min
Response: 39293637
Conc: 25.53 ng/ml

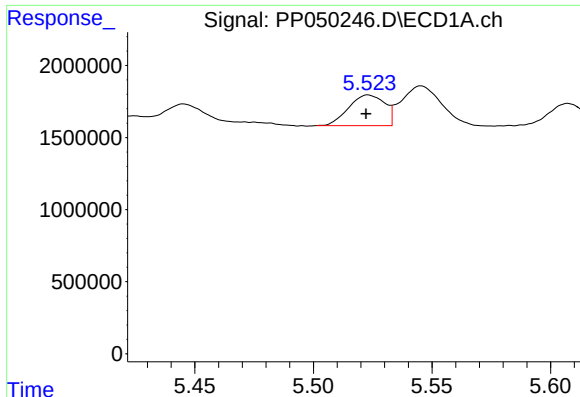

#3 AR-1016-1


R.T.: 5.524 min
Delta R.T.: 0.001 min
Response: 2251728
Conc: 35.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

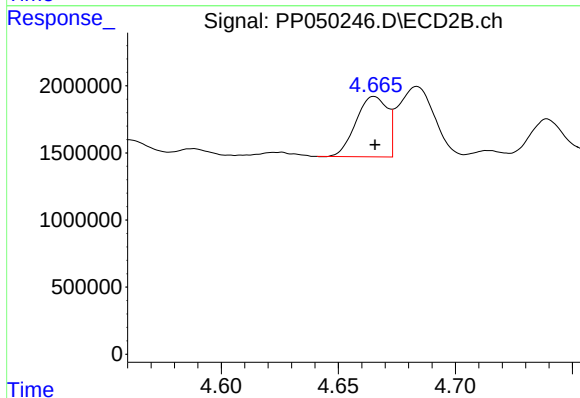


#3 AR-1016-1

R.T.: 4.665 min
Delta R.T.: 0.000 min
Response: 4211565
Conc: 41.43 ng/ml

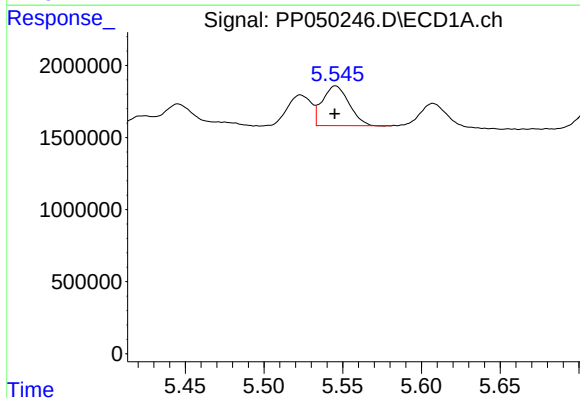


#4 AR-1016-2

R.T.: 5.545 min
Delta R.T.: 0.000 min
Response: 3223272
Conc: 36.40 ng/ml

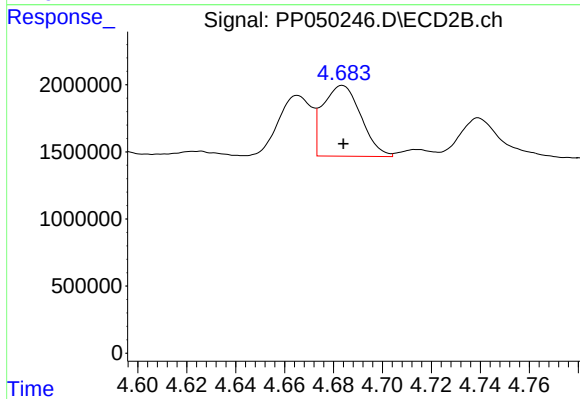

#4 AR-1016-2


R.T.: 4.684 min
Delta R.T.: 0.000 min
Response: 5715951
Conc: 39.52 ng/ml

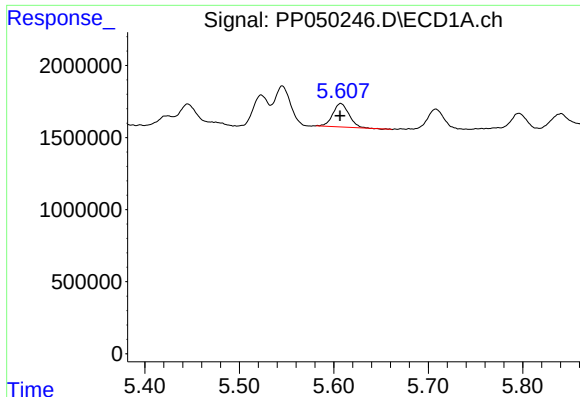

#5 AR-1016-3


R.T.: 5.607 min
Delta R.T.: 0.001 min
Response: 1915036
Conc: 35.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

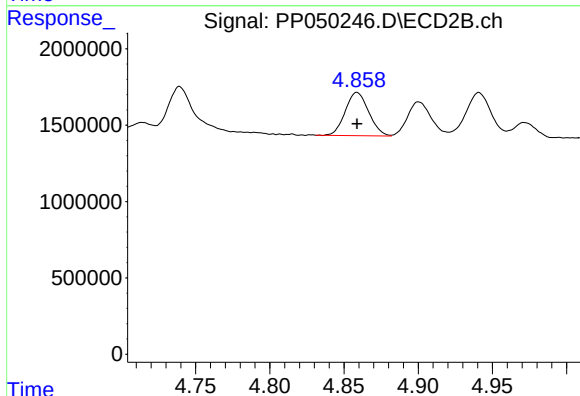


#5 AR-1016-3

R.T.: 4.859 min
Delta R.T.: 0.000 min
Response: 3103372
Conc: 40.90 ng/ml

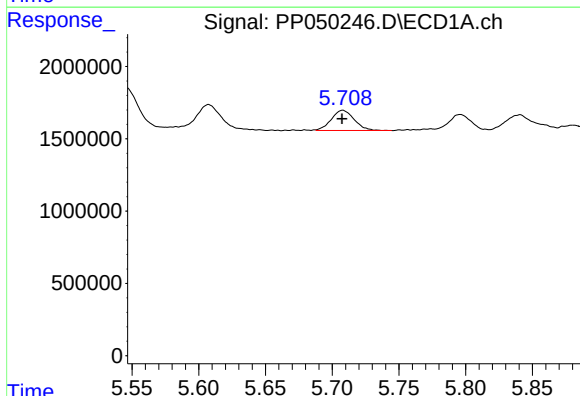


#6 AR-1016-4

R.T.: 5.708 min
Delta R.T.: 0.000 min
Response: 1673928
Conc: 36.30 ng/ml

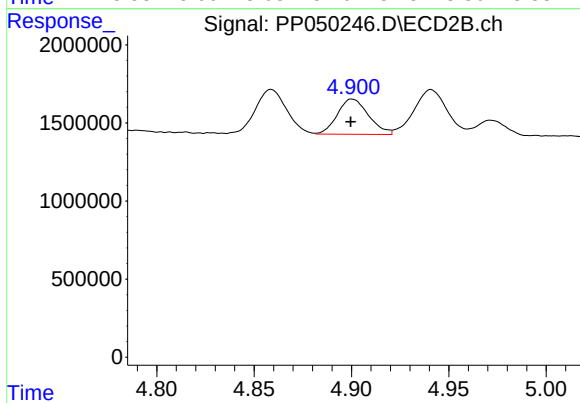

#6 AR-1016-4


R.T.: 4.900 min
Delta R.T.: 0.000 min
Response: 2517947
Conc: 43.21 ng/ml

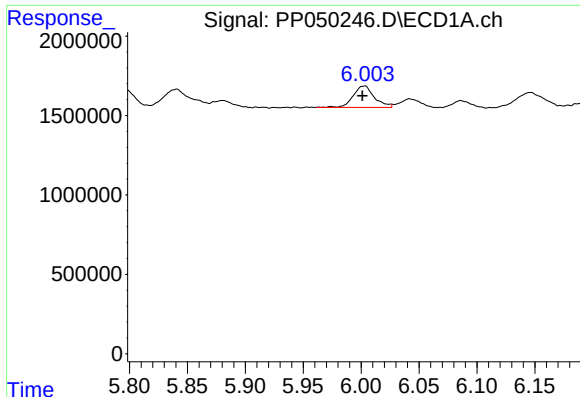

#7 AR-1016-5


R.T.: 6.002 min
Delta R.T.: 0.001 min
Response: 1722824
Conc: 38.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

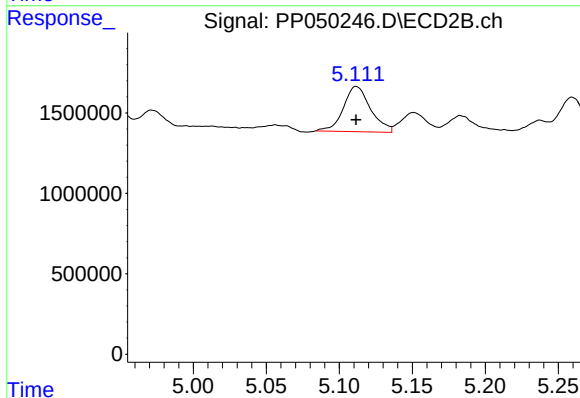


#7 AR-1016-5

R.T.: 5.112 min
Delta R.T.: 0.000 min
Response: 3645699
Conc: 47.71 ng/ml

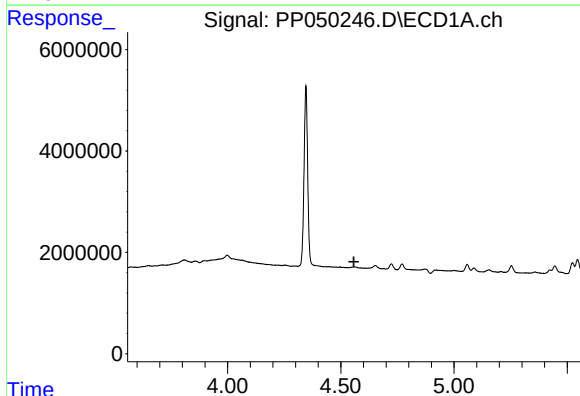


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.558 min
Response: 0
Conc: N.D.

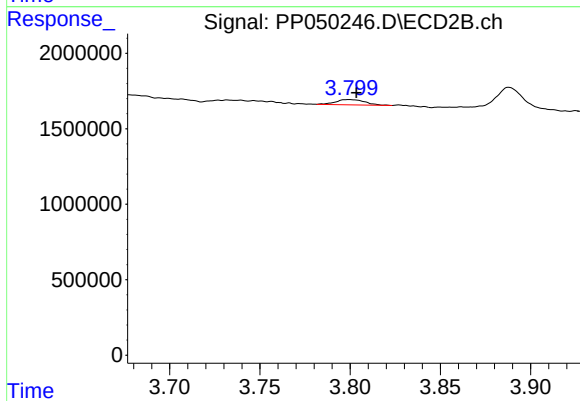

#8 AR-1221-1


R.T.: 3.800 min
Delta R.T.: -0.004 min
Response: 392158
Conc: 10.26 ng/ml

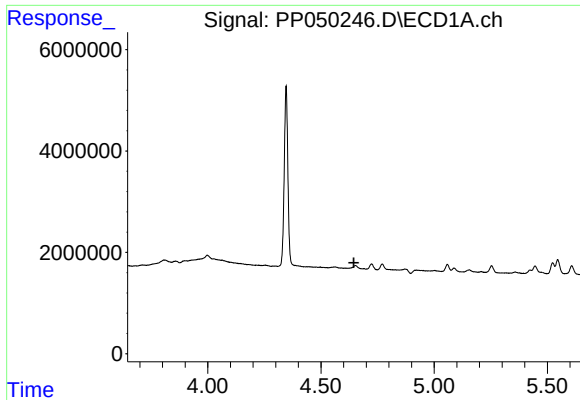

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.646 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

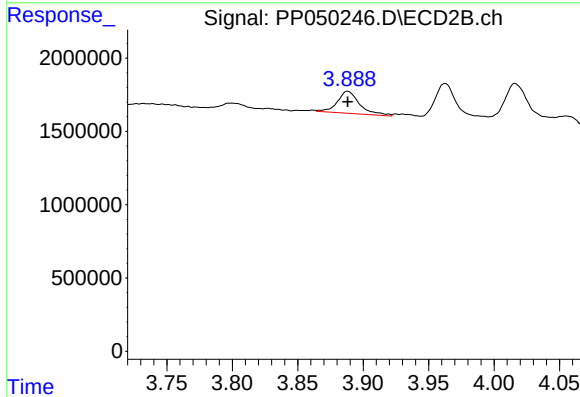


#9 AR-1221-2

R.T.: 3.888 min
Delta R.T.: 0.000 min
Response: 1792377
Conc: 62.77 ng/ml

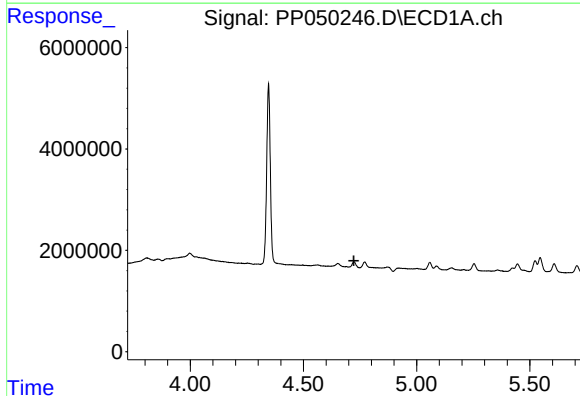


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

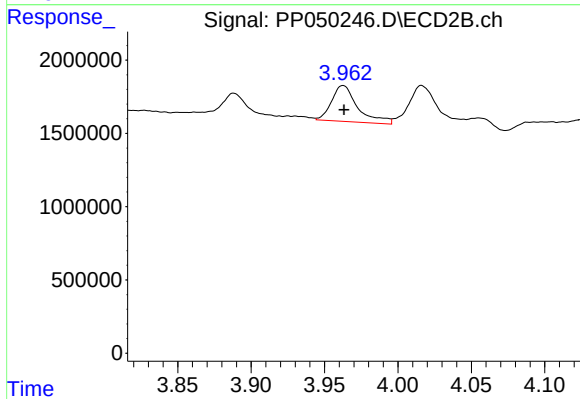

#10 AR-1221-3


R.T.: 3.963 min
Delta R.T.: 0.000 min
Response: 3055549
Conc: 35.69 ng/ml

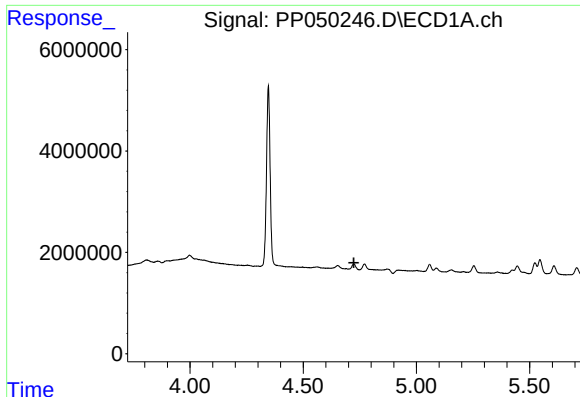

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T.: 4.723 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

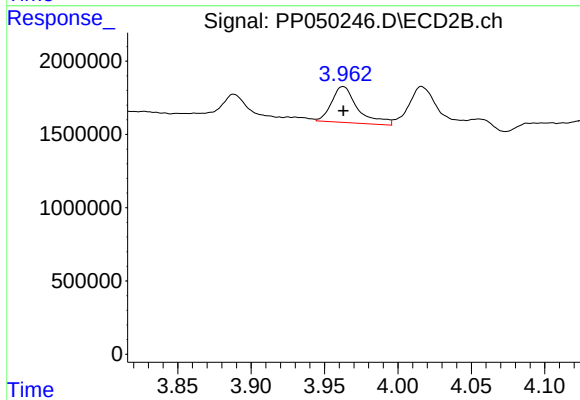


#11 AR-1232-1

R.T.: 3.963 min
Delta R.T.: 0.000 min
Response: 3055549
Conc: 43.77 ng/ml

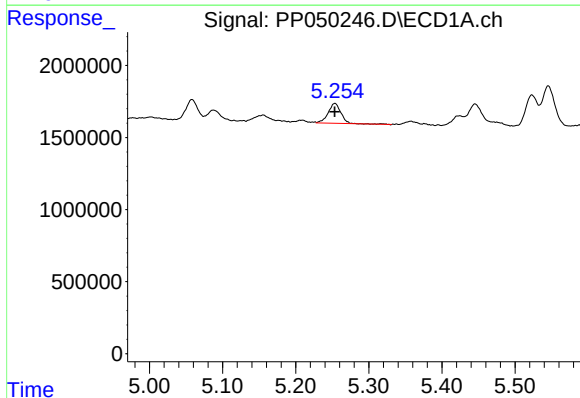


#12 AR-1232-2

R.T.: 5.254 min
Delta R.T.: 0.000 min
Response: 1677615
Conc: 92.63 ng/ml

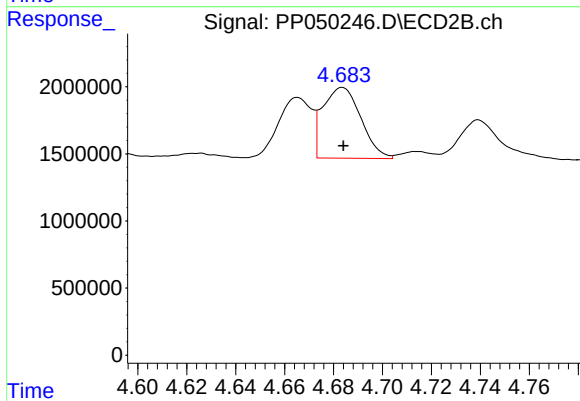

#12 AR-1232-2


R.T.: 4.684 min
Delta R.T.: 0.000 min
Response: 5715951
Conc: 88.91 ng/ml

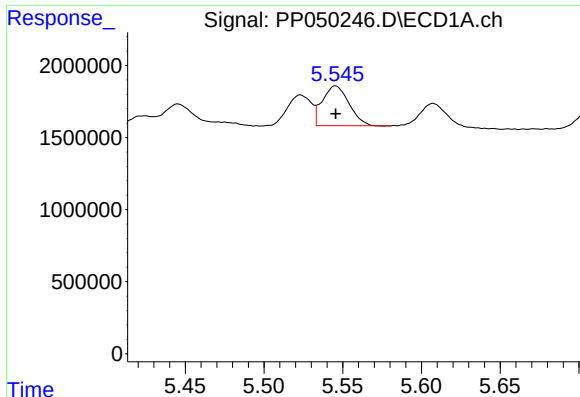

#13 AR-1232-3


R.T.: 5.545 min
Delta R.T.: 0.000 min
Response: 3223272
Conc: 81.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

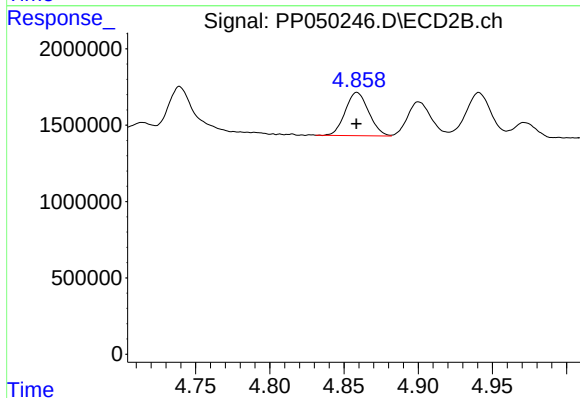


#13 AR-1232-3

R.T.: 4.859 min
Delta R.T.: 0.000 min
Response: 3103372
Conc: 92.53 ng/ml

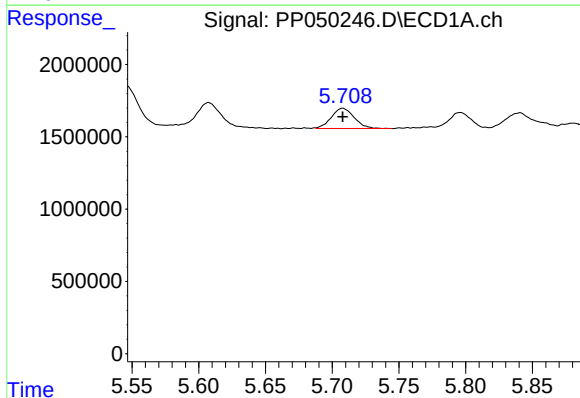


#14 AR-1232-4

R.T.: 5.708 min
Delta R.T.: 0.000 min
Response: 1673928
Conc: 82.73 ng/ml

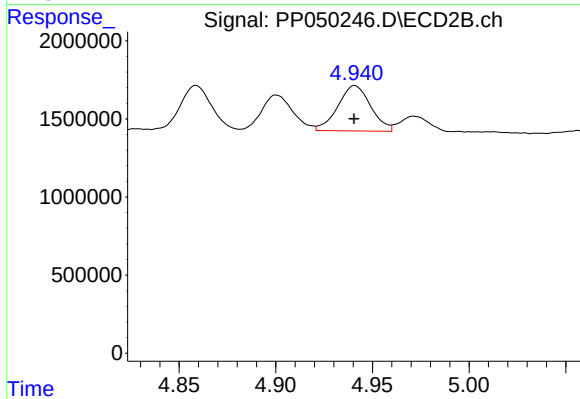

#14 AR-1232-4


R.T.: 4.941 min
Delta R.T.: 0.000 min
Response: 3440640
Conc: 116.79 ng/ml

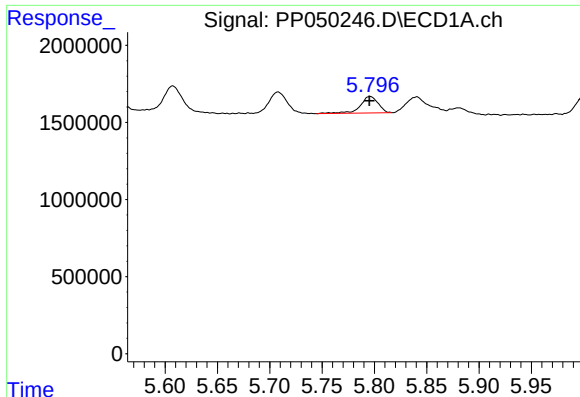

#15 AR-1232-5


R.T.: 5.796 min
Delta R.T.: 0.000 min
Response: 1273199
Conc: 81.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

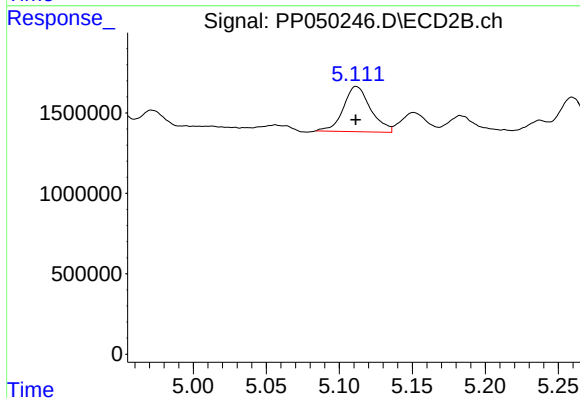


#15 AR-1232-5

R.T.: 5.112 min
Delta R.T.: 0.000 min
Response: 3645699
Conc: 110.71 ng/ml

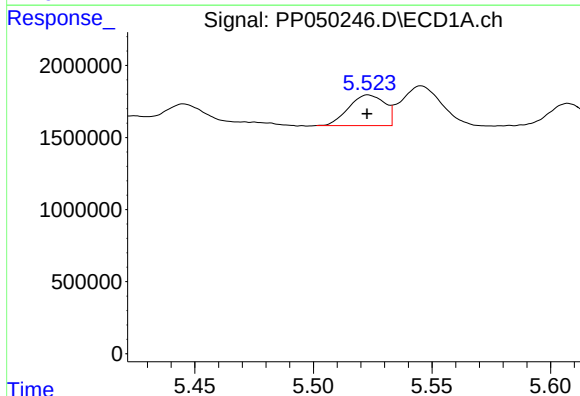


#16 AR-1242-1

R.T.: 5.524 min
Delta R.T.: 0.000 min
Response: 2251728
Conc: 44.43 ng/ml

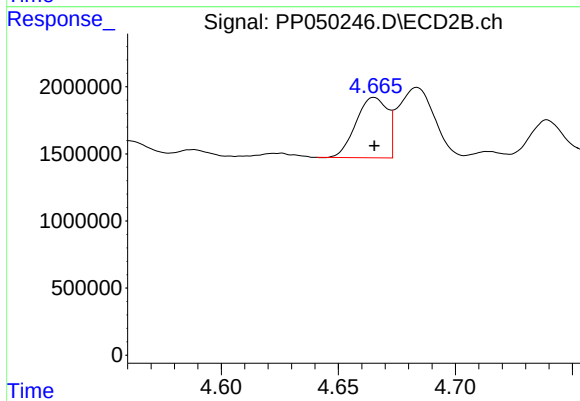

#16 AR-1242-1


R.T.: 4.665 min
Delta R.T.: 0.000 min
Response: 4211565
Conc: 50.80 ng/ml

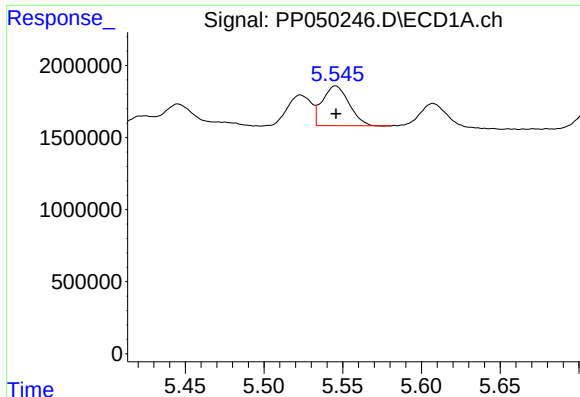

#17 AR-1242-2


R.T.: 5.545 min
Delta R.T.: 0.000 min
Response: 3223272
Conc: 44.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

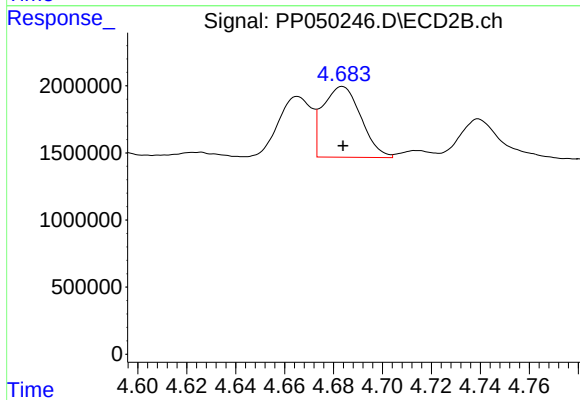


#17 AR-1242-2

R.T.: 4.684 min
Delta R.T.: 0.000 min
Response: 5715951
Conc: 48.95 ng/ml

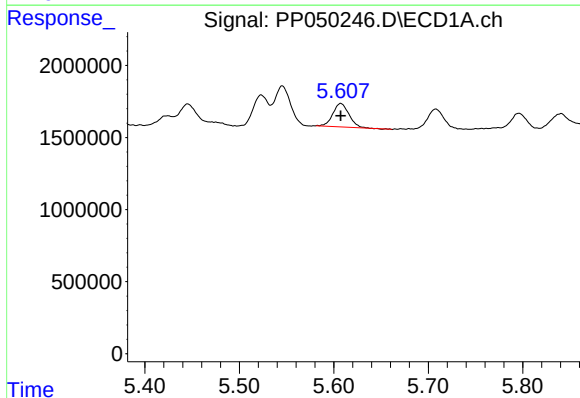


#18 AR-1242-3

R.T.: 5.607 min
Delta R.T.: 0.000 min
Response: 1915036
Conc: 43.30 ng/ml

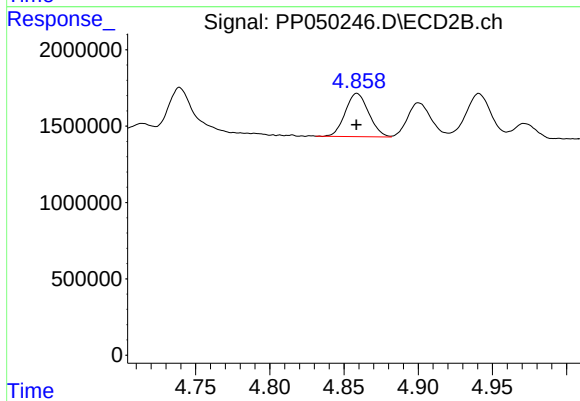

#18 AR-1242-3


R.T.: 4.859 min
Delta R.T.: 0.000 min
Response: 3103372
Conc: 50.61 ng/ml

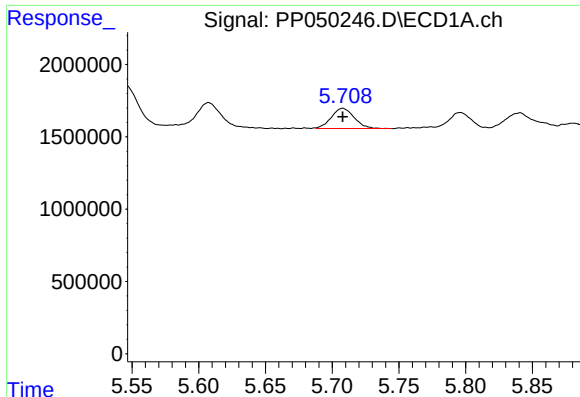

#19 AR-1242-4


R.T.: 5.708 min
Delta R.T.: 0.000 min
Response: 1673928
Conc: 44.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

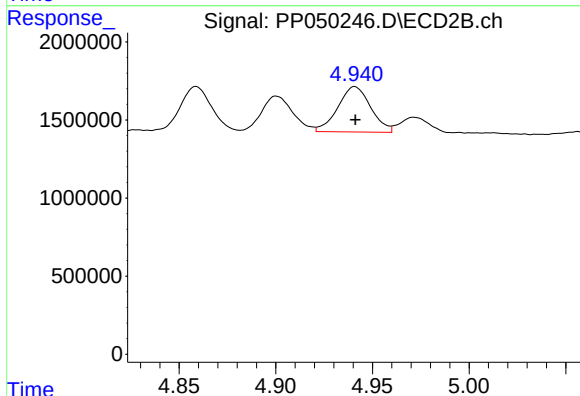


#19 AR-1242-4

R.T.: 4.941 min
Delta R.T.: 0.000 min
Response: 3440640
Conc: 58.77 ng/ml

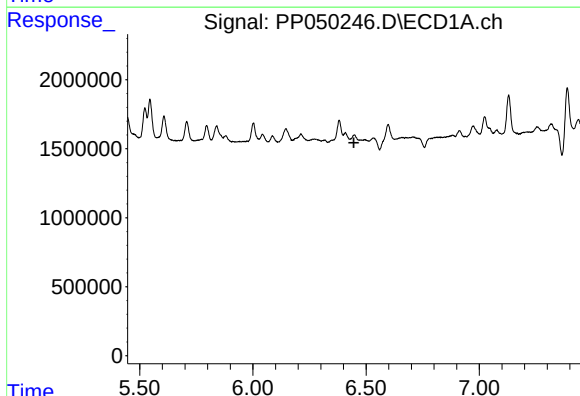


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 6.446 min
Response: 0
Conc: N.D.

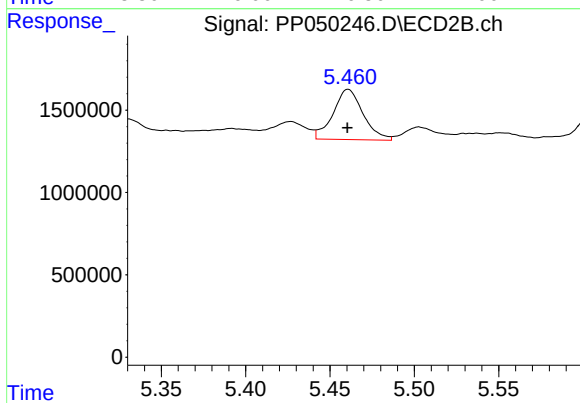

#20 AR-1242-5


R.T.: 5.461 min
Delta R.T.: 0.000 min
Response: 3783585
Conc: 54.43 ng/ml

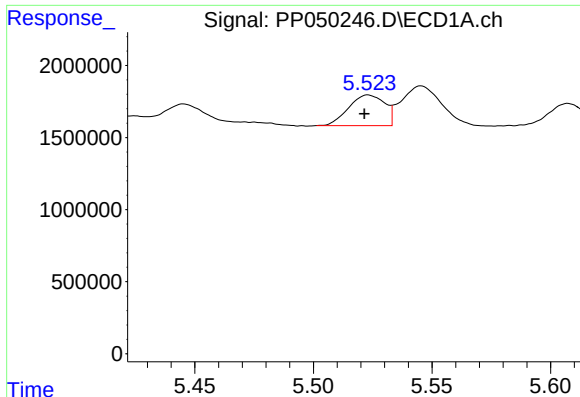

#21 AR-1248-1


R.T.: 5.524 min
Delta R.T.: 0.002 min
Response: 2251728
Conc: 55.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

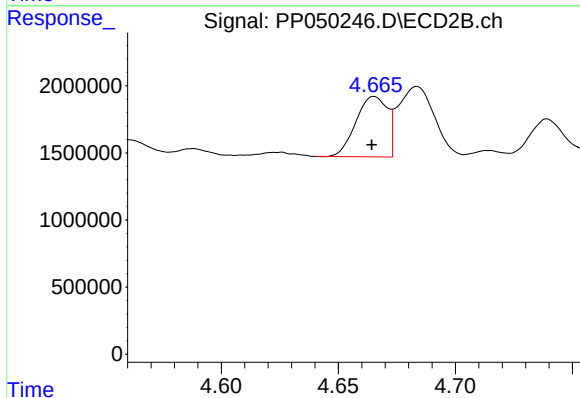


#21 AR-1248-1

R.T.: 4.665 min
Delta R.T.: 0.001 min
Response: 4211565
Conc: 63.01 ng/ml

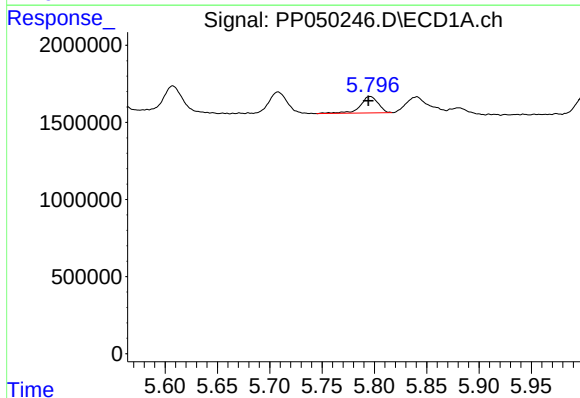


#22 AR-1248-2

R.T.: 5.796 min
Delta R.T.: 0.002 min
Response: 1273199
Conc: 22.79 ng/ml

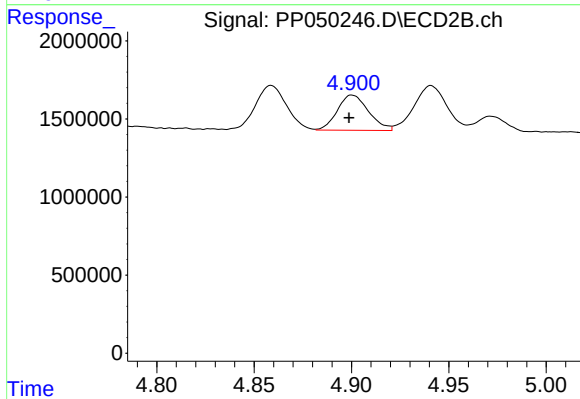

#22 AR-1248-2


R.T.: 4.900 min
Delta R.T.: 0.002 min
Response: 2517947
Conc: 29.15 ng/ml

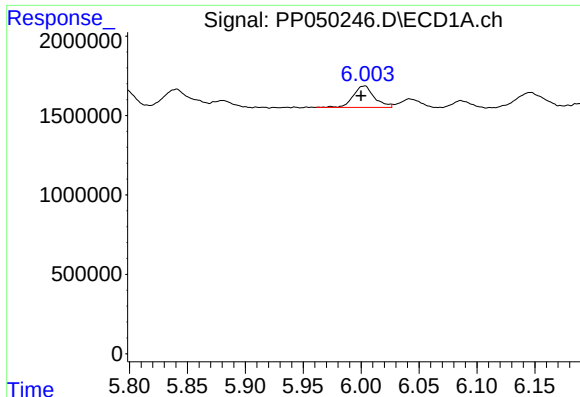

#23 AR-1248-3


R.T.: 6.002 min
Delta R.T.: 0.002 min
Response: 1722824
Conc: 26.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

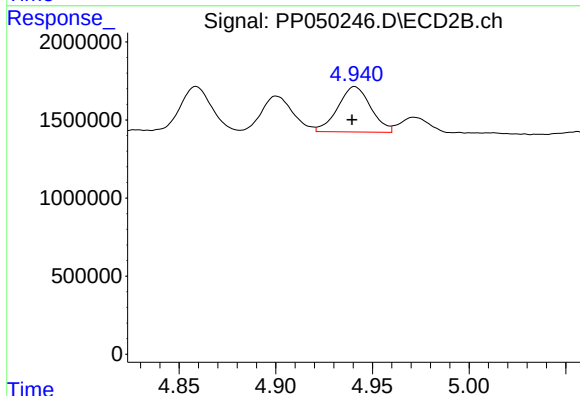


#23 AR-1248-3

R.T.: 4.941 min
Delta R.T.: 0.001 min
Response: 3440640
Conc: 37.95 ng/ml

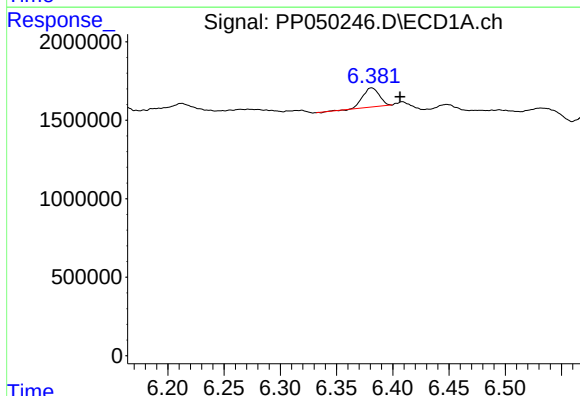


#24 AR-1248-4

R.T.: 6.381 min
Delta R.T.: -0.025 min
Response: 1237936
Conc: 15.65 ng/ml

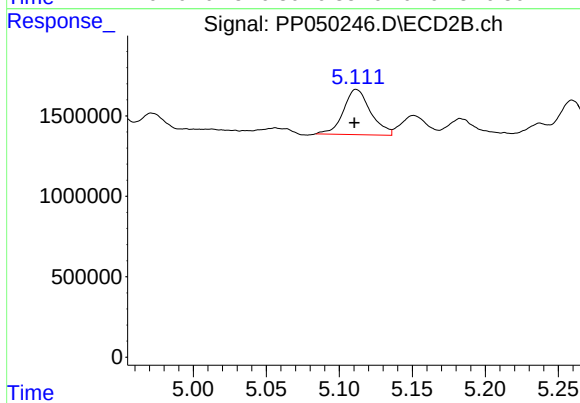

#24 AR-1248-4


R.T.: 5.112 min
Delta R.T.: 0.001 min
Response: 3645699
Conc: 34.59 ng/ml

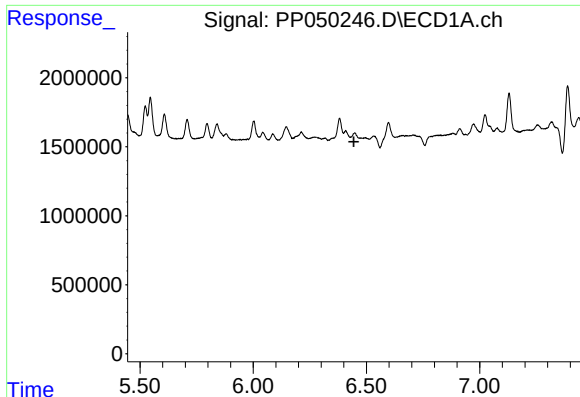

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.445 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

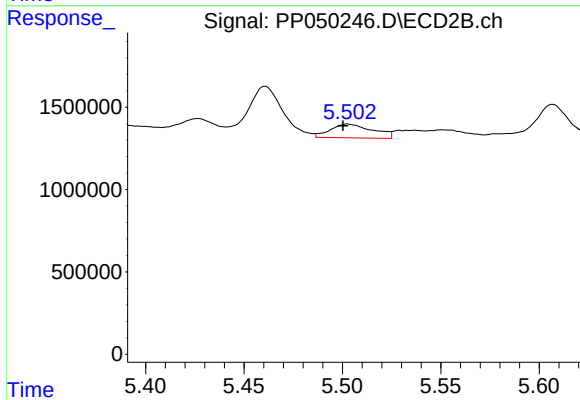


#25 AR-1248-5

R.T.: 5.503 min
Delta R.T.: 0.003 min
Response: 1260303
Conc: 12.69 ng/ml

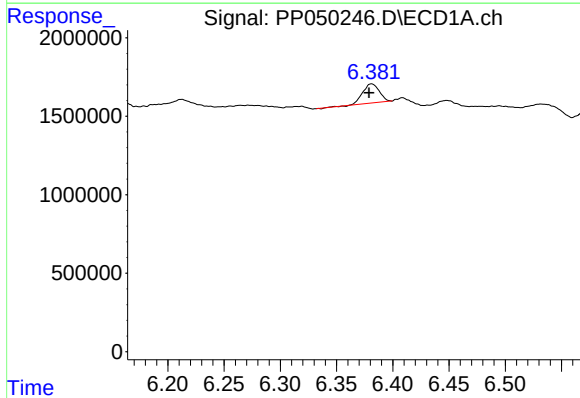


#26 AR-1254-1

R.T.: 6.381 min
Delta R.T.: 0.002 min
Response: 1237936
Conc: 17.86 ng/ml

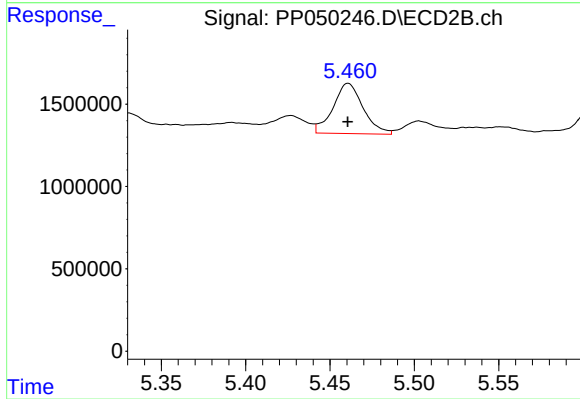

#26 AR-1254-1


R.T.: 5.461 min
Delta R.T.: 0.000 min
Response: 3783585
Conc: 28.63 ng/ml

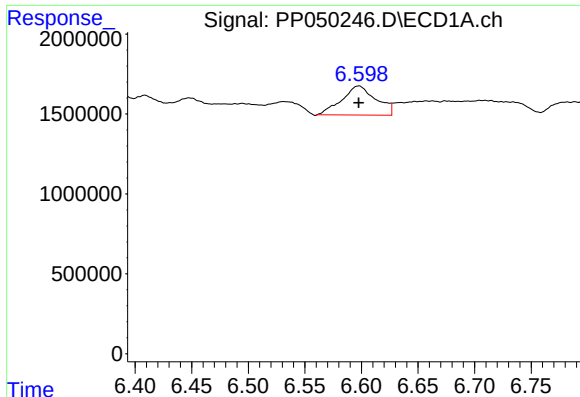

#27 AR-1254-2


R.T.: 6.597 min
Delta R.T.: 0.000 min
Response: 3832579
Conc: 36.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

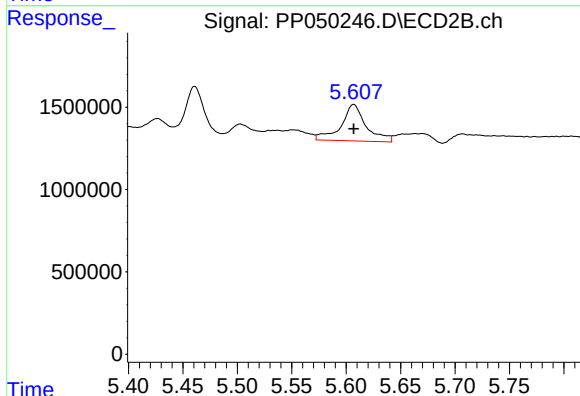


#27 AR-1254-2

R.T.: 5.607 min
Delta R.T.: 0.000 min
Response: 3539039
Conc: 32.48 ng/ml

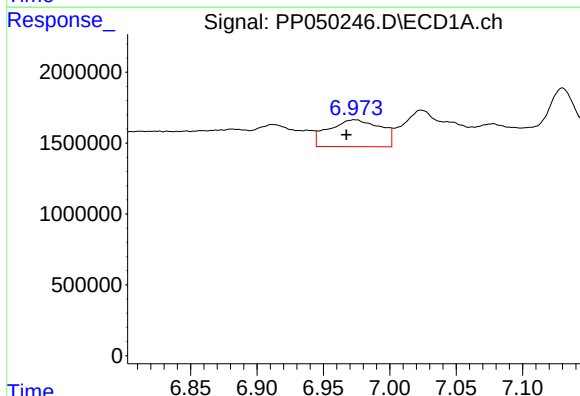


#28 AR-1254-3

R.T.: 6.973 min
Delta R.T.: 0.006 min
Response: 5151581
Conc: 45.41 ng/ml

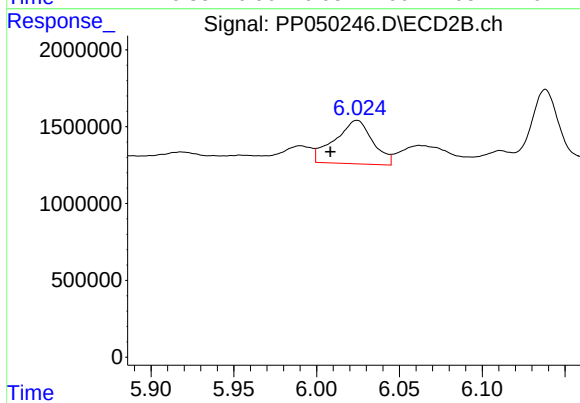

#28 AR-1254-3


R.T.: 6.024 min
Delta R.T.: 0.016 min
Response: 4514678
Conc: 28.37 ng/ml

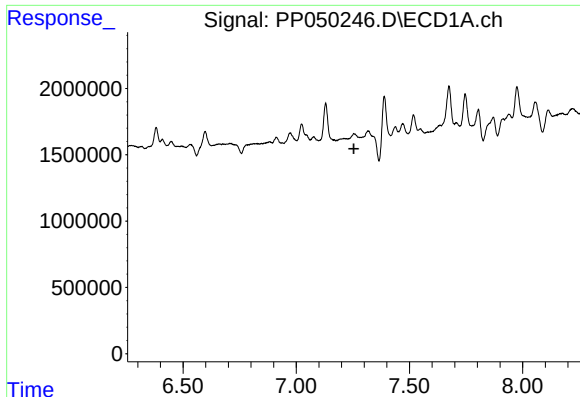

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.255 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

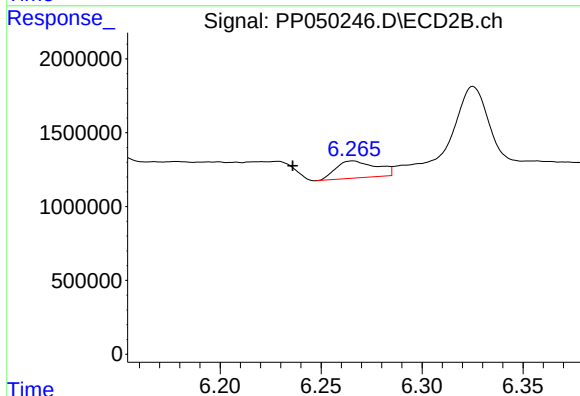


#29 AR-1254-4

R.T.: 6.266 min
Delta R.T.: 0.030 min
Response: 1626784
Conc: 16.73 ng/ml

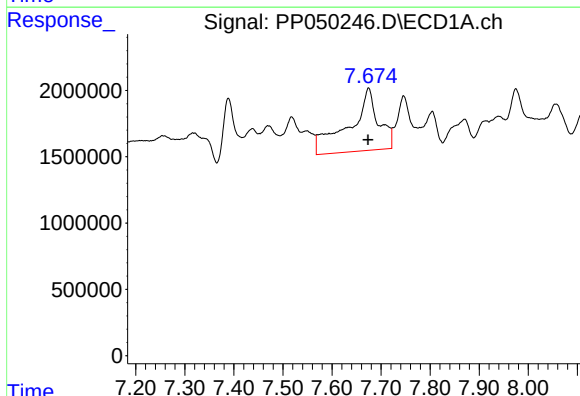


#30 AR-1254-5

R.T.: 7.675 min
Delta R.T.: 0.000 min
Response: 19416234
Conc: 205.42 ng/ml

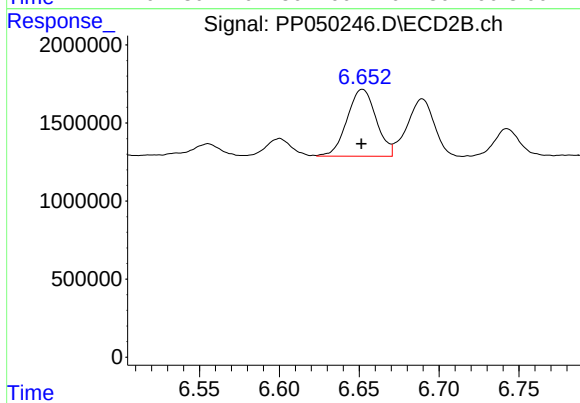

#30 AR-1254-5


R.T.: 6.652 min
Delta R.T.: 0.000 min
Response: 5443639
Conc: 44.16 ng/ml

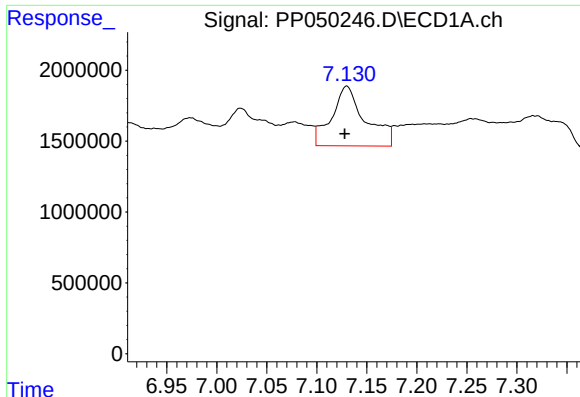

#31 AR-1260-1


R.T.: 7.130 min
Delta R.T.: 0.002 min
Response: 9870747
Conc: 108.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

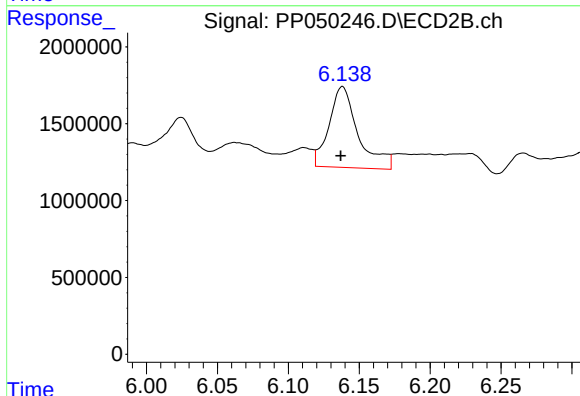


#31 AR-1260-1

R.T.: 6.138 min
Delta R.T.: 0.001 min
Response: 7521162
Conc: 66.37 ng/ml

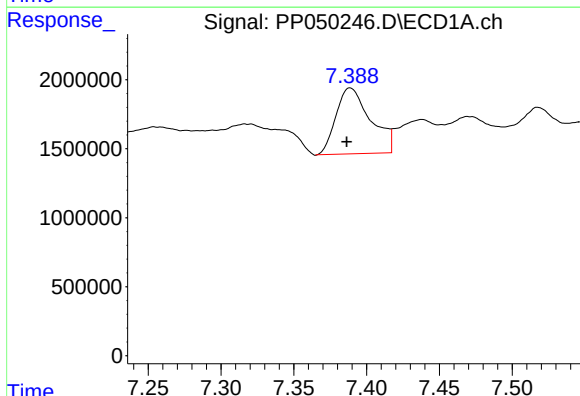


#32 AR-1260-2

R.T.: 7.389 min
Delta R.T.: 0.003 min
Response: 7911211
Conc: 69.24 ng/ml

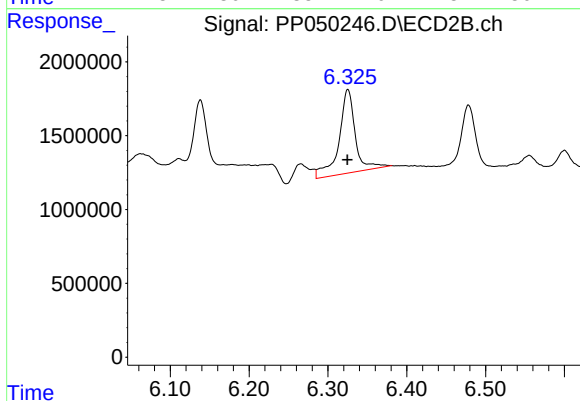

#32 AR-1260-2


R.T.: 6.325 min
Delta R.T.: 0.000 min
Response: 8106633
Conc: 60.34 ng/ml

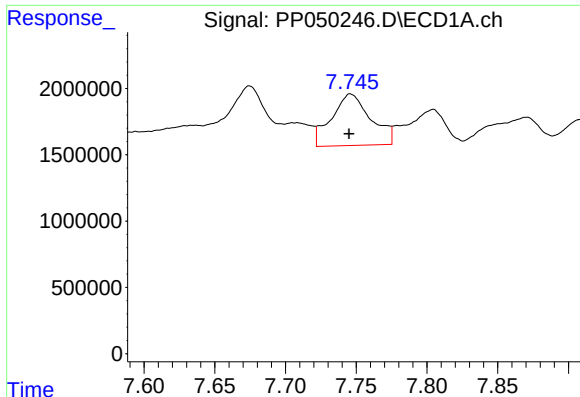

#33 AR-1260-3


R.T.: 7.746 min
Delta R.T.: 0.001 min
Response: 7527531
Conc: 88.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

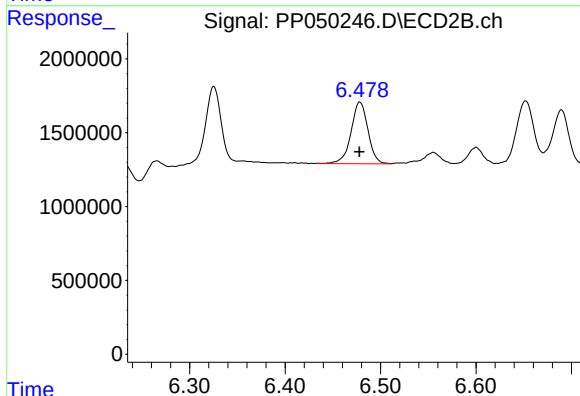


#33 AR-1260-3

R.T.: 6.478 min
Delta R.T.: 0.000 min
Response: 5152045
Conc: 42.77 ng/ml

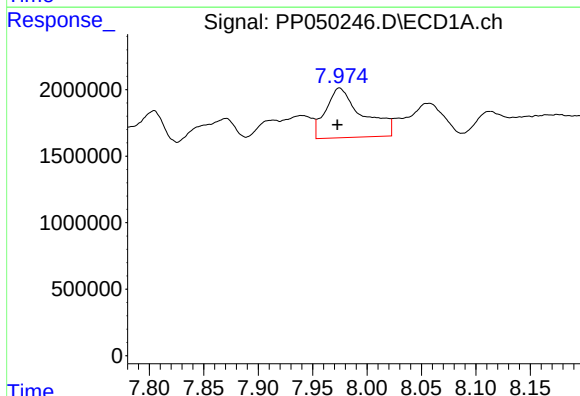


#34 AR-1260-4

R.T.: 7.975 min
Delta R.T.: 0.002 min
Response: 8773306
Conc: 92.17 ng/ml

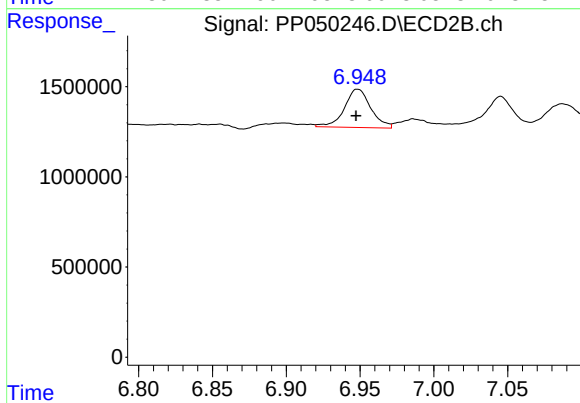

#34 AR-1260-4


R.T.: 6.948 min
Delta R.T.: 0.001 min
Response: 2650331
Conc: 29.90 ng/ml

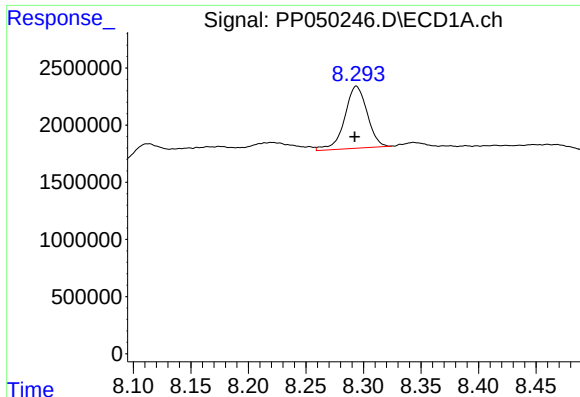

#35 AR-1260-5


R.T.: 8.294 min
Delta R.T.: 0.002 min
Response: 7417718
Conc: 39.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

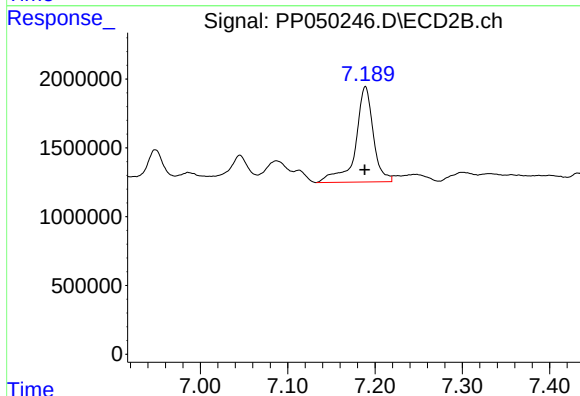


#35 AR-1260-5

R.T.: 7.189 min
Delta R.T.: 0.000 min
Response: 9854475
Conc: 50.55 ng/ml

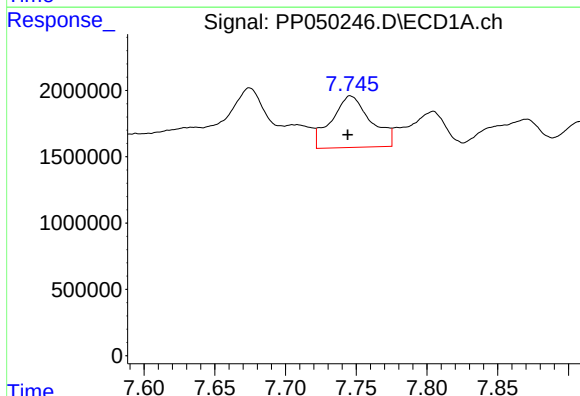


#36 AR-1262-1

R.T.: 7.746 min
Delta R.T.: 0.002 min
Response: 7527531
Conc: 62.86 ng/ml

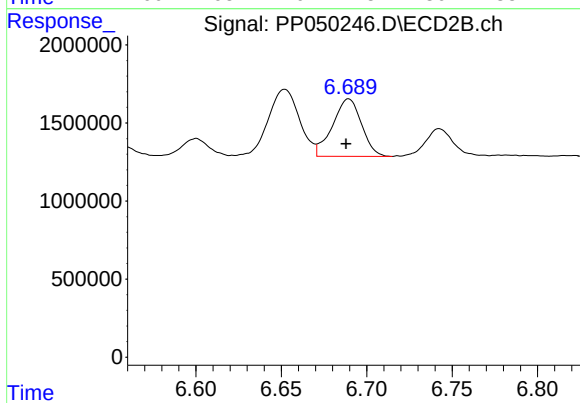

#36 AR-1262-1


R.T.: 6.689 min
Delta R.T.: 0.002 min
Response: 4356436
Conc: 32.24 ng/ml

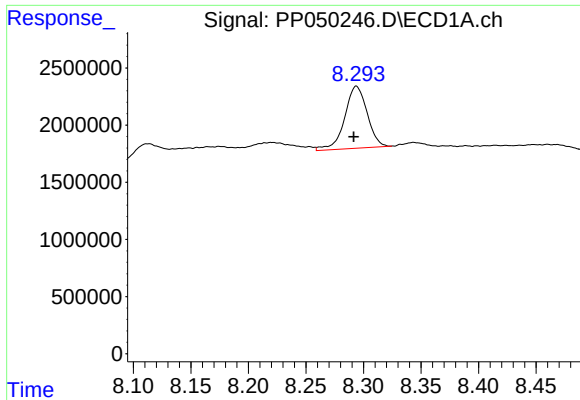

#37 AR-1262-2


R.T.: 8.294 min
Delta R.T.: 0.003 min
Response: 7417718
Conc: 34.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

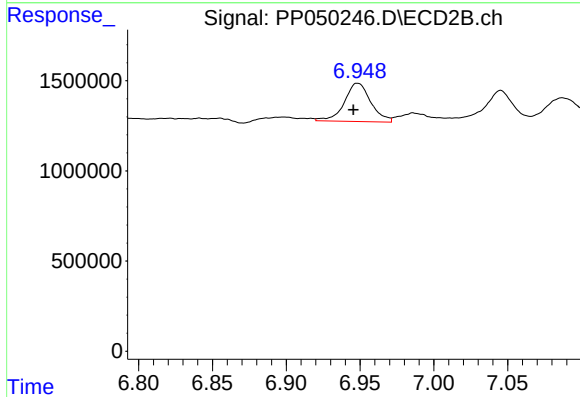


#37 AR-1262-2

R.T.: 6.948 min
Delta R.T.: 0.003 min
Response: 2650331
Conc: 24.39 ng/ml

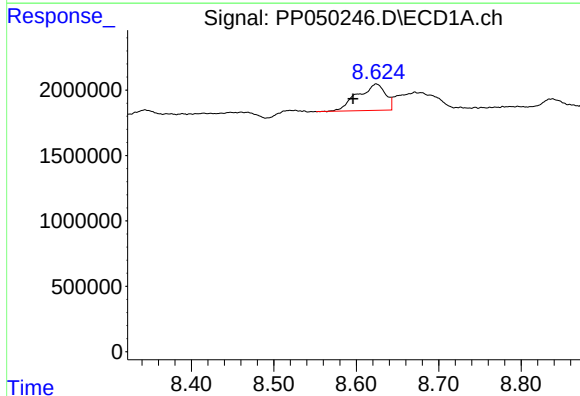


#38 AR-1262-3

R.T.: 8.624 min
Delta R.T.: 0.029 min
Response: 4736492
Conc: 48.20 ng/ml

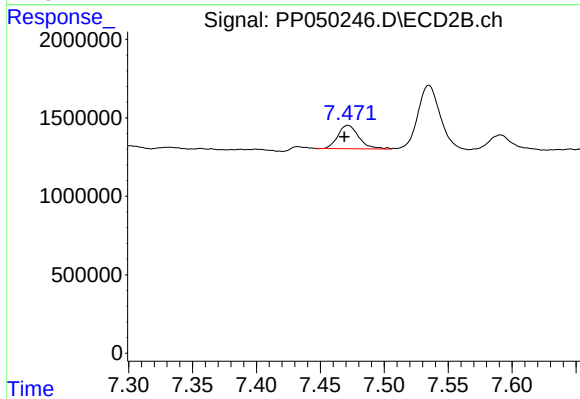

#38 AR-1262-3


R.T.: 7.472 min
Delta R.T.: 0.003 min
Response: 1711594
Conc: 23.58 ng/ml

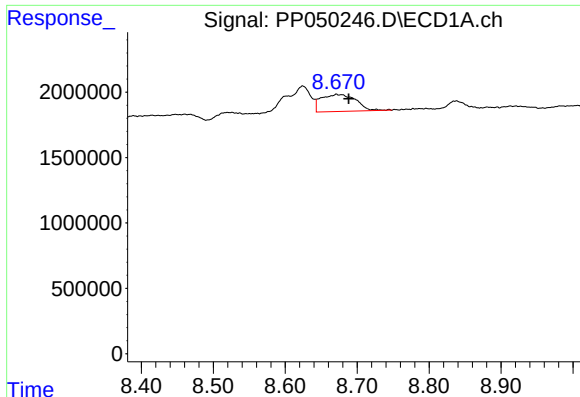

#39 AR-1262-4


R.T.: 8.672 min
Delta R.T.: -0.016 min
Response: 4374436
Conc: 68.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

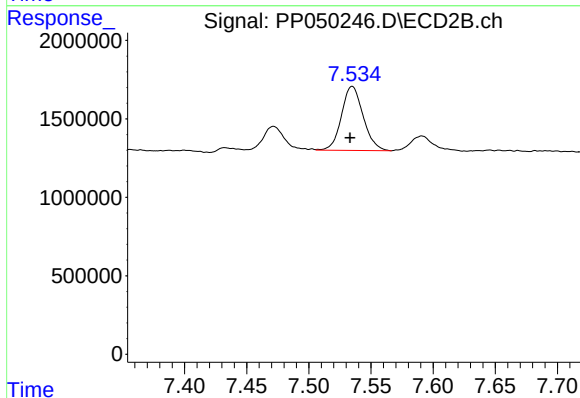


#39 AR-1262-4

R.T.: 7.535 min
Delta R.T.: 0.002 min
Response: 4963691
Conc: 36.00 ng/ml

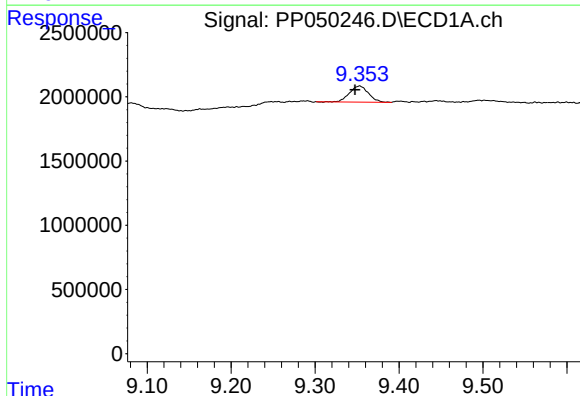


#40 AR-1262-5

R.T.: 9.353 min
Delta R.T.: 0.005 min
Response: 1960424
Conc: 24.84 ng/ml

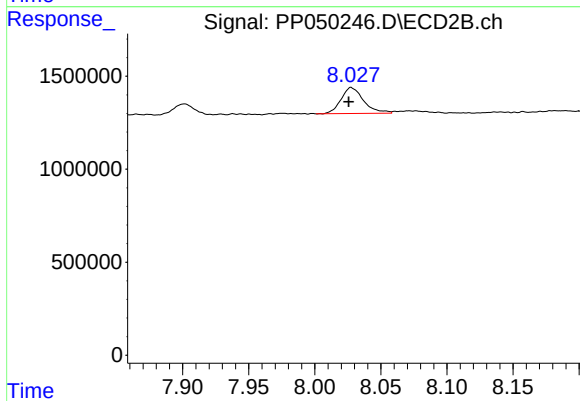

#40 AR-1262-5


R.T.: 8.028 min
Delta R.T.: 0.002 min
Response: 1661284
Conc: 25.79 ng/ml

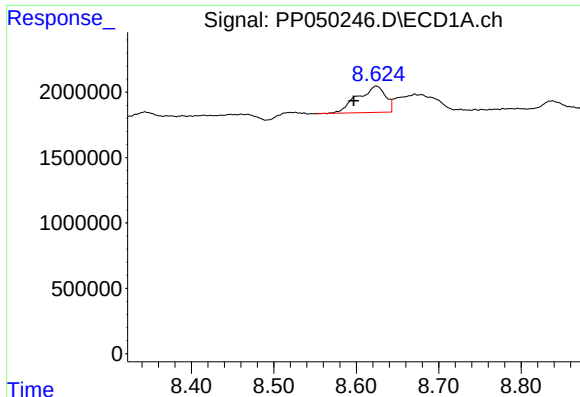

#41 AR-1268-1


R.T.: 8.624 min
Delta R.T.: 0.027 min
Response: 4736492
Conc: 18.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

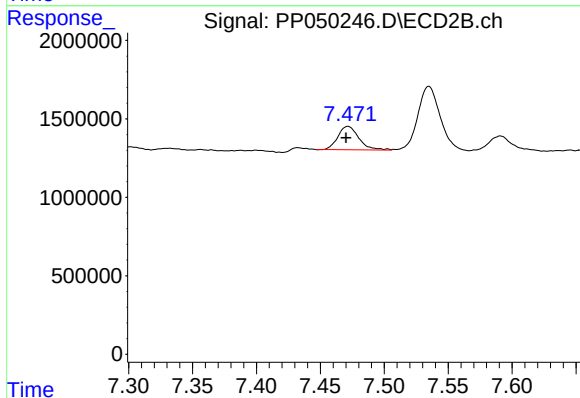


#41 AR-1268-1

R.T.: 7.472 min
Delta R.T.: 0.002 min
Response: 1711594
Conc: 7.79 ng/ml

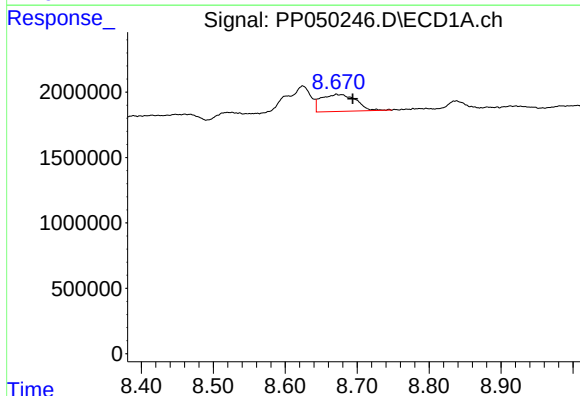


#42 AR-1268-2

R.T.: 8.672 min
Delta R.T.: -0.021 min
Response: 4374436
Conc: 17.93 ng/ml

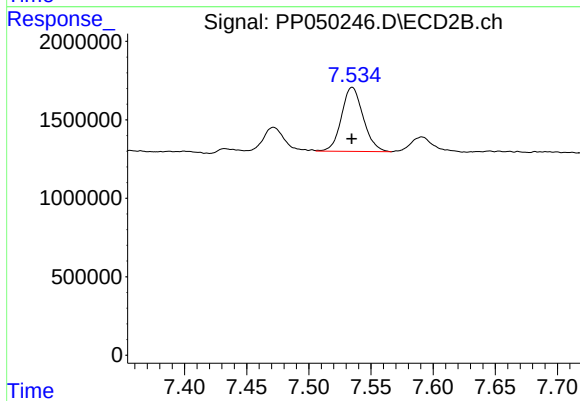

#42 AR-1268-2


R.T.: 7.535 min
Delta R.T.: 0.000 min
Response: 4963691
Conc: 24.92 ng/ml

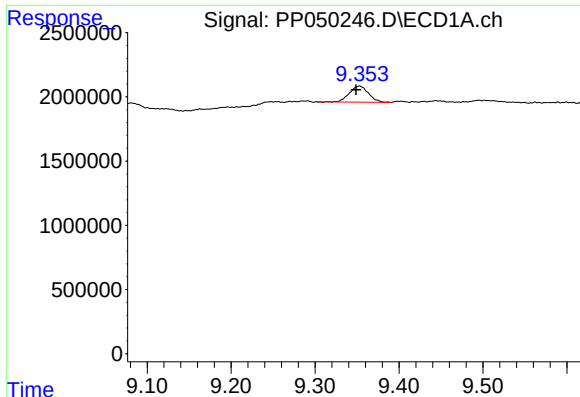

#44 AR-1268-4


R.T.: 9.353 min
Delta R.T.: 0.004 min
Response: 1960424
Conc: 22.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

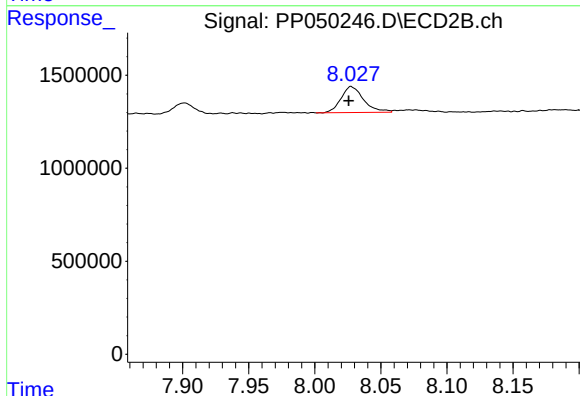


#44 AR-1268-4

R.T.: 8.028 min
Delta R.T.: 0.002 min
Response: 1661284
Conc: 23.38 ng/ml

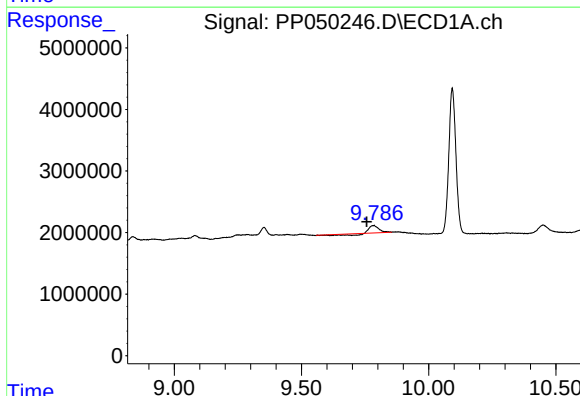

#45 AR-1268-5

R.T.: 9.783 min
Delta R.T.: 0.026 min
Response: 1963810
Conc: 2.94 ng/ml

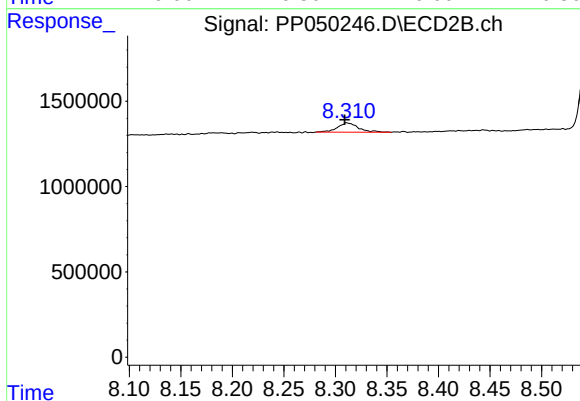

#45 AR-1268-5

R.T.: 8.311 min
Delta R.T.: 0.002 min
Response: 769196
Conc: 1.40 ng/ml