

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080622\
 Data File : PP050266.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2022 18:13
 Operator : YP\AJ
 Sample : N3980-07
 Misc : AR1660 LOD 40 PPB
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 00:33:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Aug 07 23:52:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.345	3.591	40246908	81776793	25.003	26.108
2)	SA Decachlor...	10.089	8.555	46229662	39543254	26.253	25.693
Target Compounds							
3)	L1 AR-1016-1	5.522	4.664	3607569	6544221	57.615	64.383
4)	L1 AR-1016-2	5.545	4.683	5044863	8967187	56.969	61.995
5)	L1 AR-1016-3	5.606	4.857	2930772	4653773	53.625	61.328
6)	L1 AR-1016-4	5.707	4.899	2663936	3722072	57.768	63.881
7)	L1 AR-1016-5	6.001	5.110	2536541	4955186	56.771	64.853
8)	L2 AR-1221-1	0.000	3.800	0	691913	N.D.	18.102 #
9)	L2 AR-1221-2	0.000	3.887	0	1790261	N.D.	62.694 #
10)	L2 AR-1221-3	4.722	3.962	1790288	3651172	39.792	42.649
11)	L3 AR-1232-1	4.722	3.962	1790288	3651172	47.892	52.302
12)	L3 AR-1232-2	5.252	4.683	2524572	8967187	139.397	139.478
13)	L3 AR-1232-3	5.545	4.857	5044863	4653773	128.122	138.752
14)	L3 AR-1232-4	5.707	4.939	2663936	4482882	131.664	152.169
15)	L3 AR-1232-5	5.794	5.110	2096219	4955186	134.084	150.474
16)	L4 AR-1242-1	5.522	4.664	3607569	6544221	71.181	78.941
17)	L4 AR-1242-2	5.545	4.683	5044863	8967187	69.835	76.787
18)	L4 AR-1242-3	5.606	4.857	2930772	4653773	66.272	75.892
19)	L4 AR-1242-4	5.707	4.939	2663936	4482882	71.488	76.579
20)	L4 AR-1242-5	0.000	5.460	0	4679635	N.D.	67.323 #
21)	L5 AR-1248-1	5.522	4.664	3607569	6544221	89.346	97.917
22)	L5 AR-1248-2	5.794	4.899	2096219	3722072	37.522	43.087
23)	L5 AR-1248-3	6.001	4.939	2536541	4482882	39.652	49.450
24)	L5 AR-1248-4	6.379f	5.110	2038115	4955186	25.765	47.014 #
25)	L5 AR-1248-5	0.000	5.499	0	1954567	N.D.	19.686 #
26)	L6 AR-1254-1	6.379	5.460	2038115	4679635	29.399	35.413
27)	L6 AR-1254-2	6.596	5.606	2163644	3170819	20.518	29.097 #
28)	L6 AR-1254-3	0.000	6.022	0	5328754	N.D.	33.481 #
29)	L6 AR-1254-4	0.000	6.236	0	368892	N.D.	3.794 #
30)	L6 AR-1254-5	7.673	6.650	8433564	8223272	89.227	66.714 #
31)	L7 AR-1260-1	7.128	6.136	5771330	7297106	63.191	64.395
32)	L7 AR-1260-2	7.387	6.323	6684779	8960635	58.510	66.701
33)	L7 AR-1260-3	7.744	6.477	4942313	7702391	58.038	63.939
34)	L7 AR-1260-4	7.973	6.946	6251589	5554037	65.677	62.652
35)	L7 AR-1260-5	8.292	7.187	10534440	12158100	56.355	62.368
36)	L8 AR-1262-1	7.744	6.688	4942313	6686490	41.269	49.477
37)	L8 AR-1262-2	8.292	6.946	10534440	5554037	48.755	51.114
38)	L8 AR-1262-3	8.621f	7.469	7345966	2431412	74.756	33.504 #
39)	L8 AR-1262-4	8.672f	7.533	5131034	7637401	79.813	55.395 #
40)	L8 AR-1262-5	9.349	8.026	3013912	2479899	38.181	38.505
41)	L9 AR-1268-1	8.621f	7.469	7345966	2431412	28.932	11.065 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080622\
 Data File : PP050266.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2022 18:13
 Operator : YP\AJ
 Sample : N3980-07
 Misc : AR1660 LOD 40 PPB
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 00:33:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Aug 07 23:52:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.672f	7.533	5131034	7637401	21.035	38.346 #
43) L9	AR-1268-3	0.000	7.737	0	150860	N.D.	0.891 #
44) L9	AR-1268-4	9.349	8.026	3013912	2479899	34.968	34.903
45) L9	AR-1268-5	9.772f	8.308	3274093	819464	4.909	1.488 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080622\
Data File : PP050266.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2022 18:13
Operator : YP\AJ
Sample : N3980-07
Misc : AR1660 LOD 40 PPB
ALS Vial : 62 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 00:33:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Aug 07 23:52:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

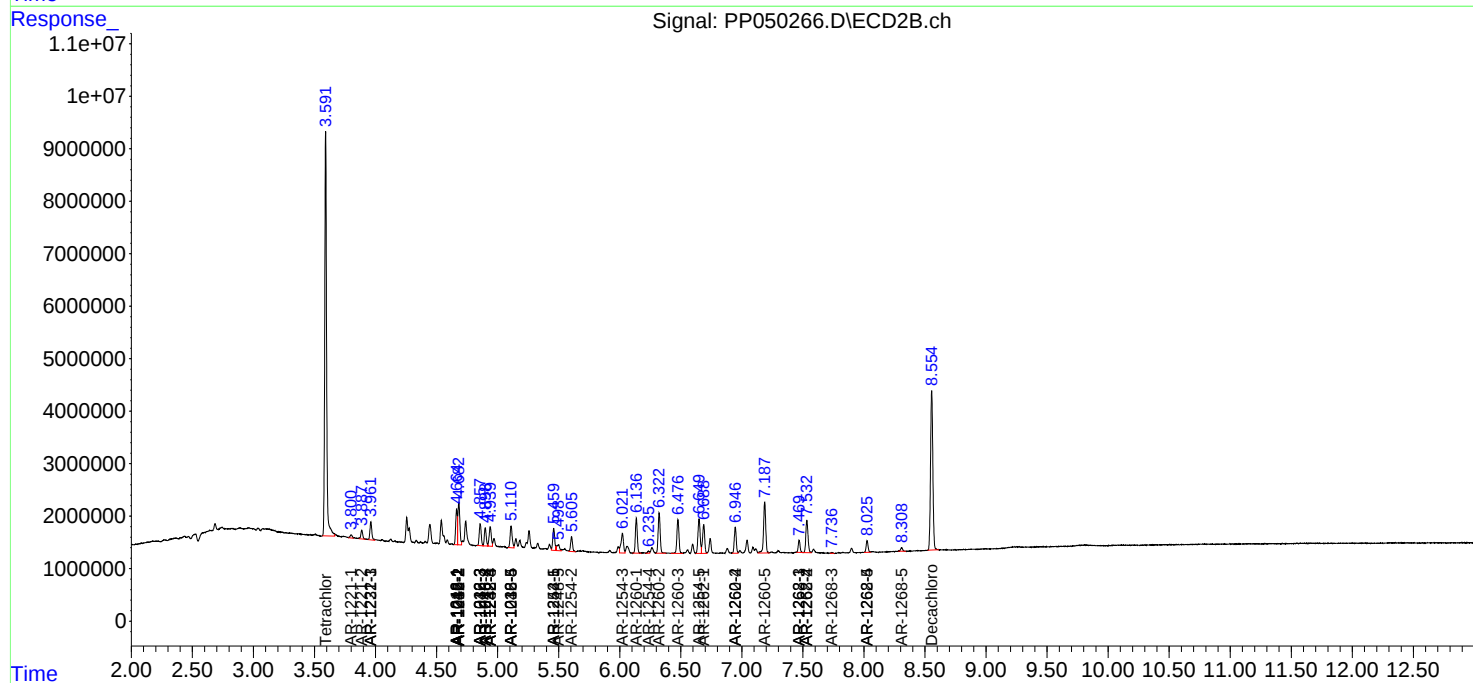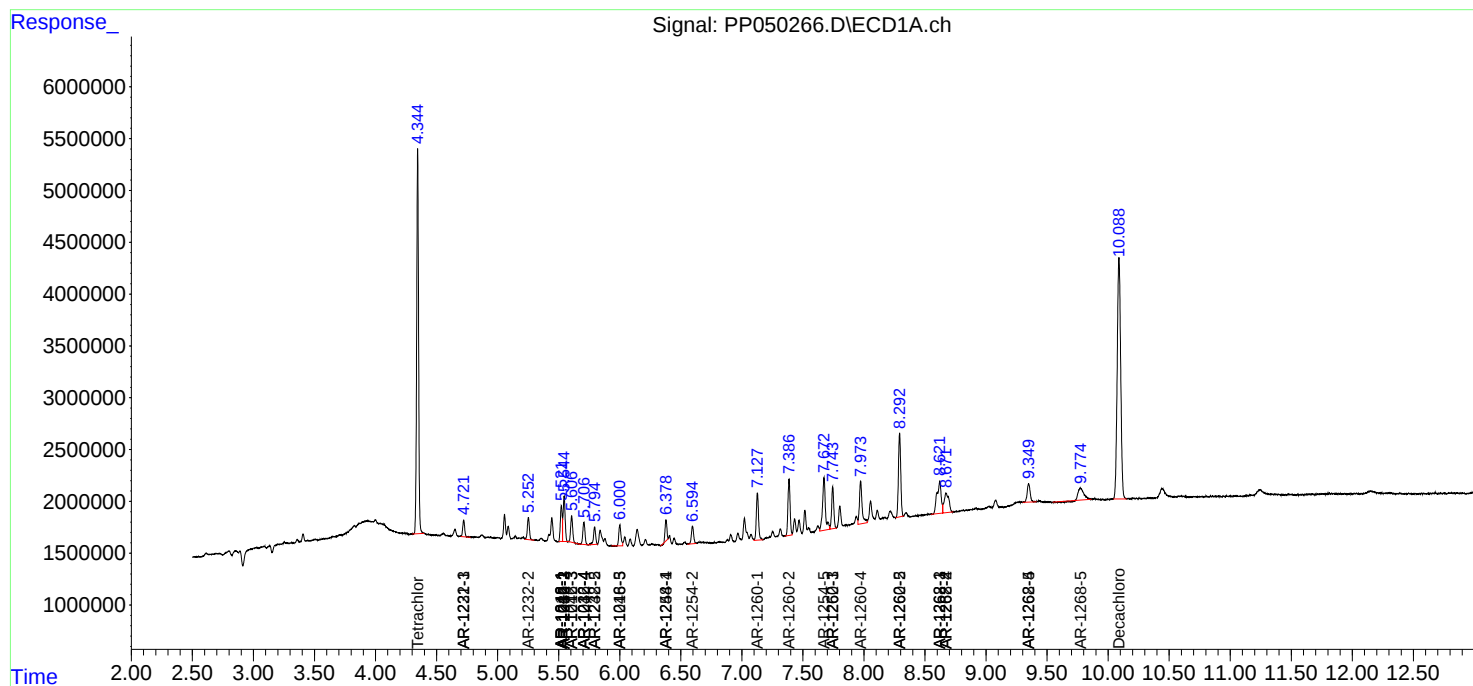


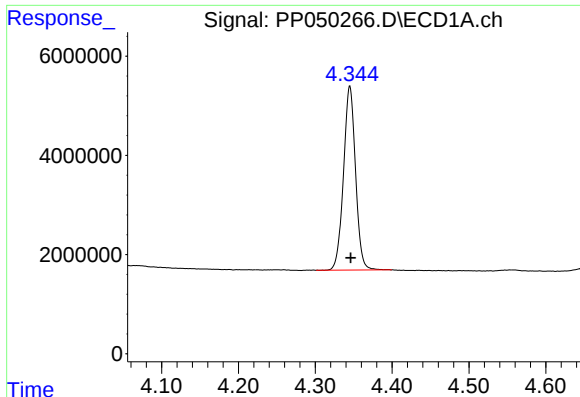

#1 Tetrachloro-m-xylene


R.T.: 4.345 min
Delta R.T.: -0.001 min
Response: 40246908
Conc: 25.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

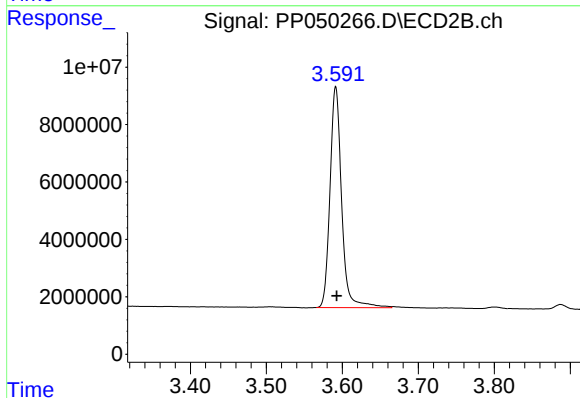


#1 Tetrachloro-m-xylene

R.T.: 3.591 min
Delta R.T.: -0.001 min
Response: 81776793
Conc: 26.11 ng/ml

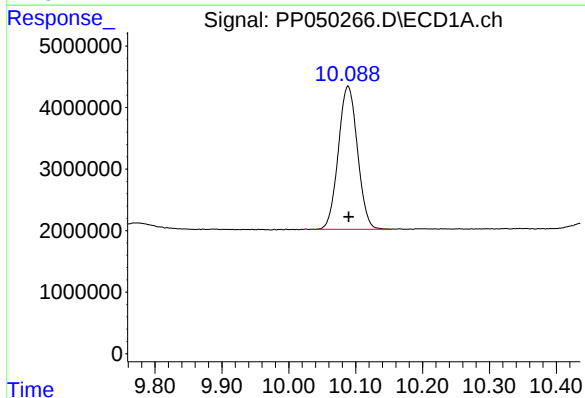


#2 Decachlorobiphenyl

R.T.: 10.089 min
Delta R.T.: -0.001 min
Response: 46229662
Conc: 26.25 ng/ml

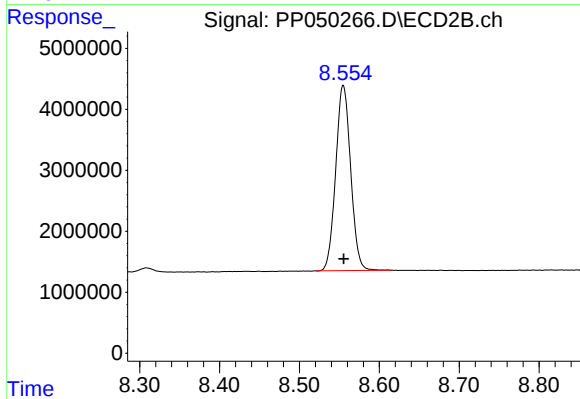

#2 Decachlorobiphenyl


R.T.: 8.555 min
Delta R.T.: 0.000 min
Response: 39543254
Conc: 25.69 ng/ml

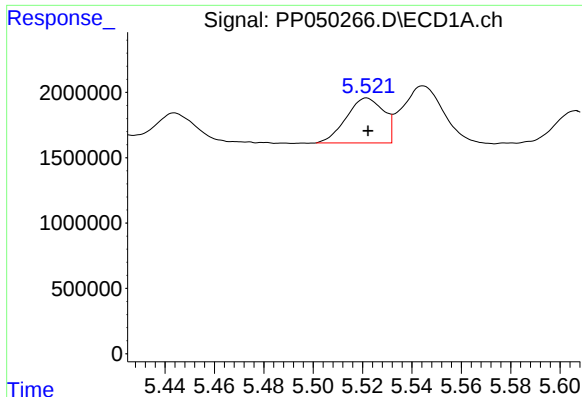

#3 AR-1016-1


R.T.: 5.522 min
Delta R.T.: 0.000 min
Response: 3607569
Conc: 57.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

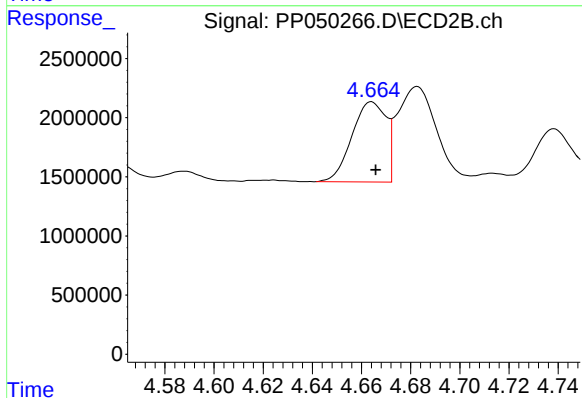


#3 AR-1016-1

R.T.: 4.664 min
Delta R.T.: -0.002 min
Response: 6544221
Conc: 64.38 ng/ml

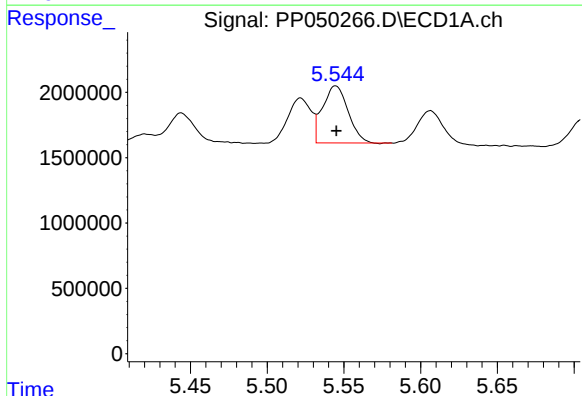


#4 AR-1016-2

R.T.: 5.545 min
Delta R.T.: 0.000 min
Response: 5044863
Conc: 56.97 ng/ml

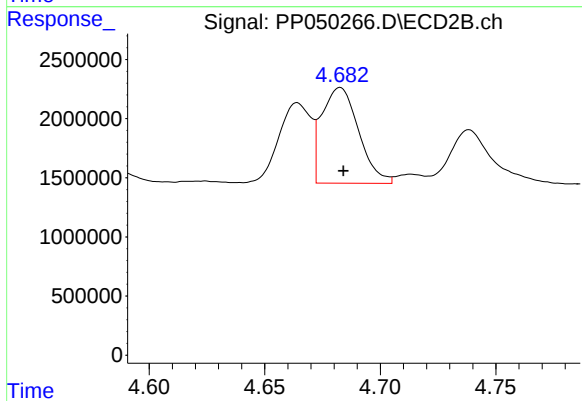

#4 AR-1016-2


R.T.: 4.683 min
Delta R.T.: -0.001 min
Response: 8967187
Conc: 62.00 ng/ml

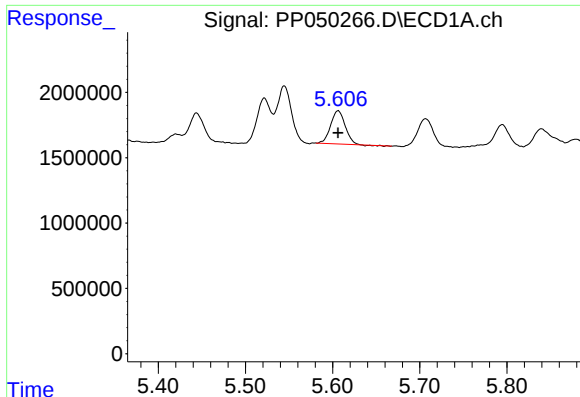

#5 AR-1016-3


R.T.: 5.606 min
Delta R.T.: 0.000 min
Response: 2930772
Conc: 53.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

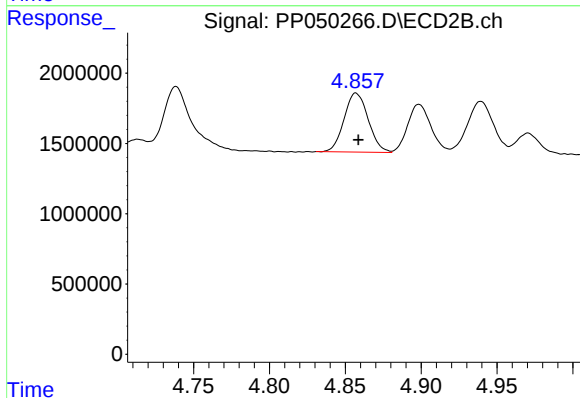


#5 AR-1016-3

R.T.: 4.857 min
Delta R.T.: -0.002 min
Response: 4653773
Conc: 61.33 ng/ml

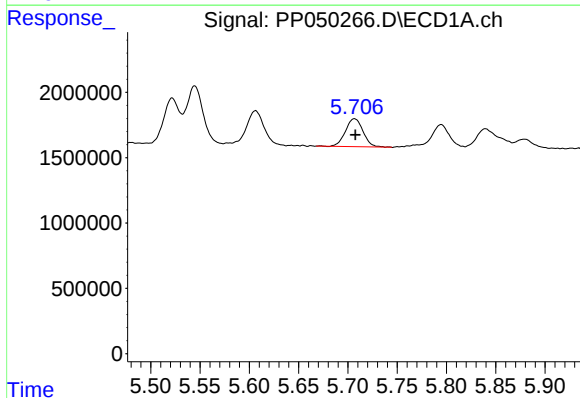


#6 AR-1016-4

R.T.: 5.707 min
Delta R.T.: 0.000 min
Response: 2663936
Conc: 57.77 ng/ml

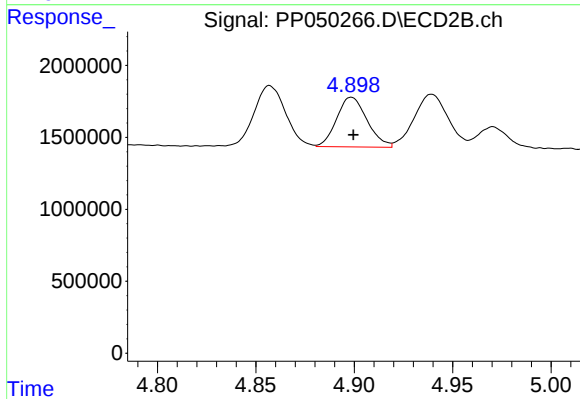

#6 AR-1016-4


R.T.: 4.899 min
Delta R.T.: 0.000 min
Response: 3722072
Conc: 63.88 ng/ml

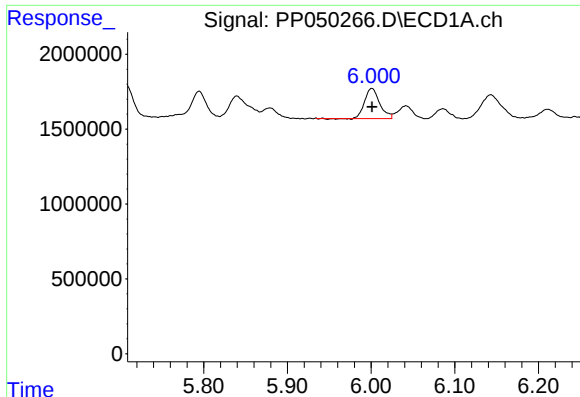

#7 AR-1016-5


R.T.: 6.001 min
Delta R.T.: 0.000 min
Response: 2536541
Conc: 56.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

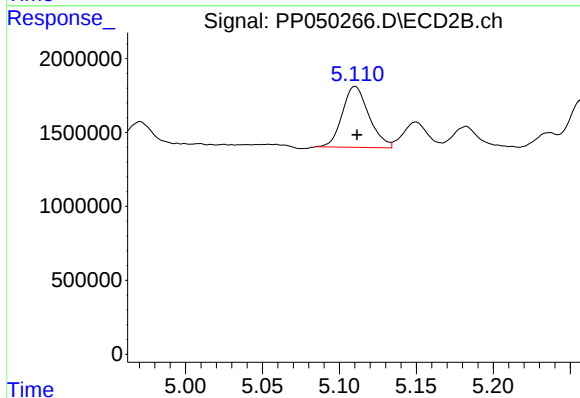


#7 AR-1016-5

R.T.: 5.110 min
Delta R.T.: -0.001 min
Response: 4955186
Conc: 64.85 ng/ml

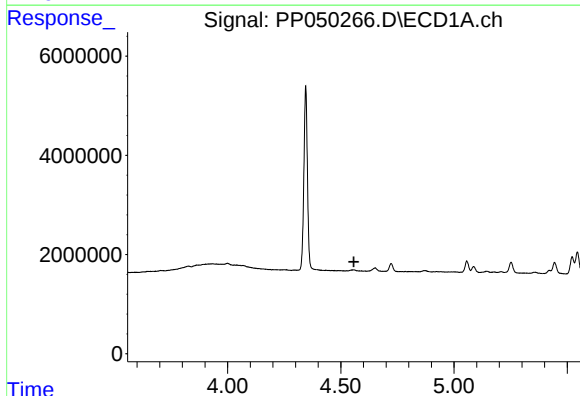


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.558 min
Response: 0
Conc: N.D.

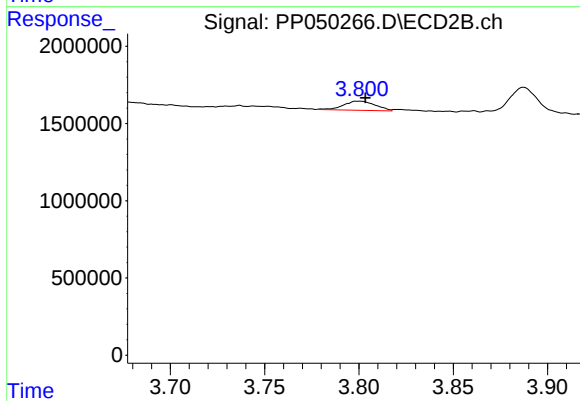

#8 AR-1221-1


R.T.: 3.800 min
Delta R.T.: -0.003 min
Response: 691913
Conc: 18.10 ng/ml

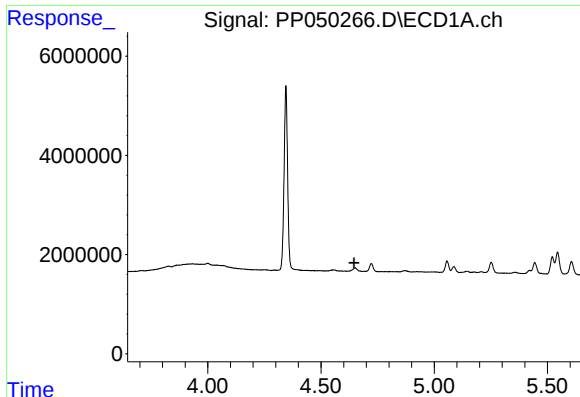

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 4.646 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

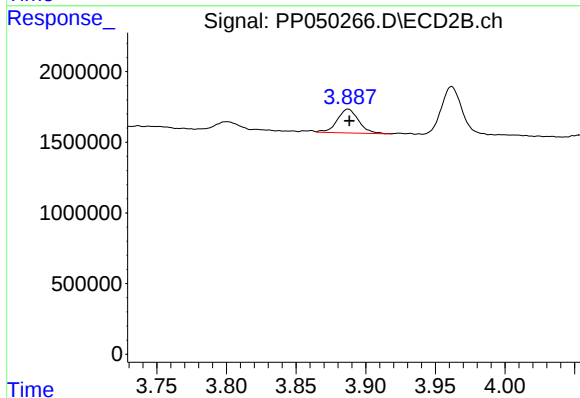


#9 AR-1221-2

R.T.: 3.887 min
Delta R.T.: 0.000 min
Response: 1790261
Conc: 62.69 ng/ml

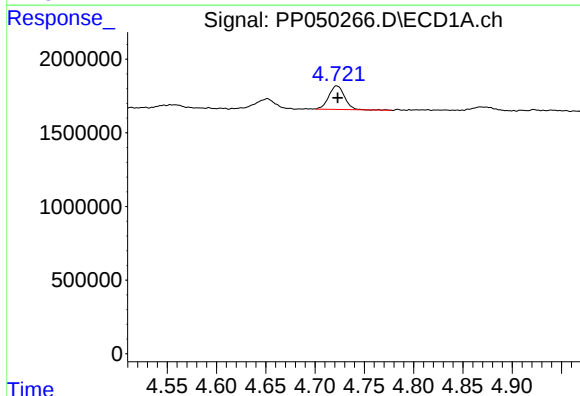


#10 AR-1221-3

R.T.: 4.722 min
Delta R.T.: -0.001 min
Response: 1790288
Conc: 39.79 ng/ml

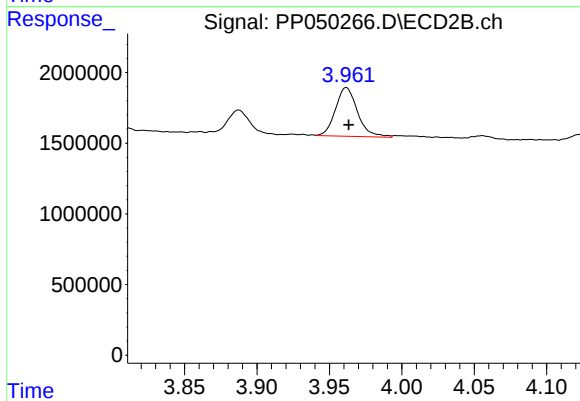

#10 AR-1221-3


R.T.: 3.962 min
Delta R.T.: -0.002 min
Response: 3651172
Conc: 42.65 ng/ml

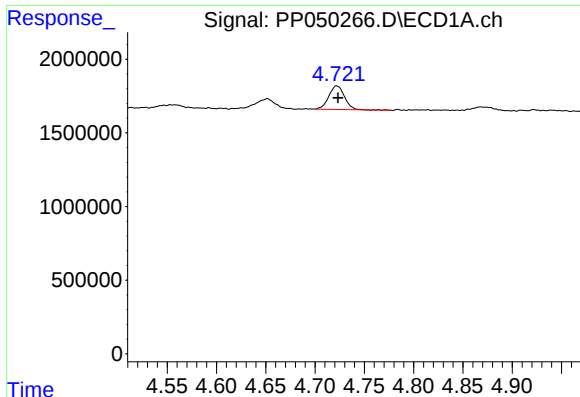

#11 AR-1232-1


R.T.: 4.722 min
Delta R.T.: -0.001 min
Response: 1790288
Conc: 47.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

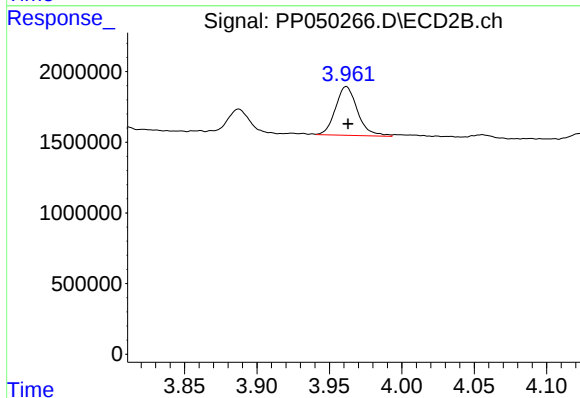


#11 AR-1232-1

R.T.: 3.962 min
Delta R.T.: -0.001 min
Response: 3651172
Conc: 52.30 ng/ml

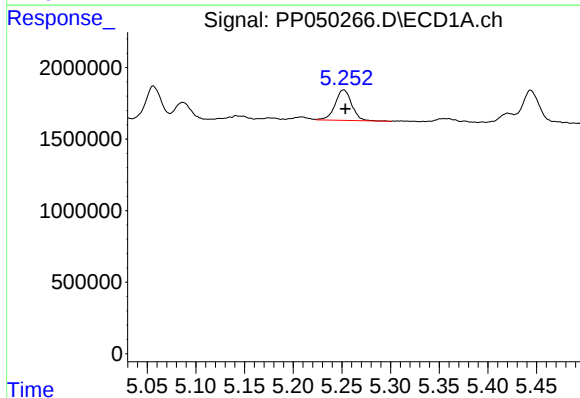


#12 AR-1232-2

R.T.: 5.252 min
Delta R.T.: -0.002 min
Response: 2524572
Conc: 139.40 ng/ml

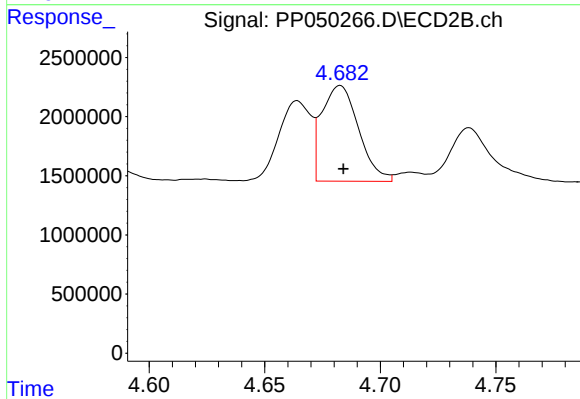

#12 AR-1232-2


R.T.: 4.683 min
Delta R.T.: -0.001 min
Response: 8967187
Conc: 139.48 ng/ml

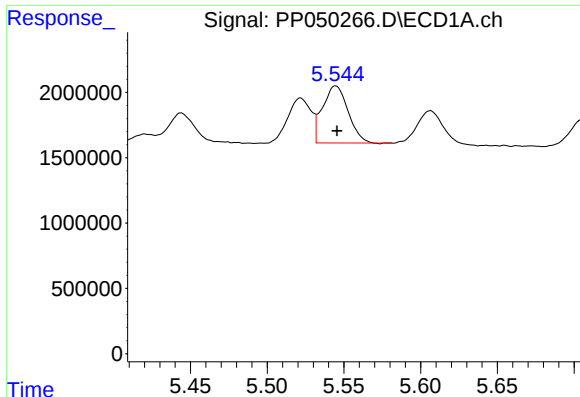

#13 AR-1232-3


R.T.: 5.545 min
Delta R.T.: 0.000 min
Response: 5044863
Conc: 128.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

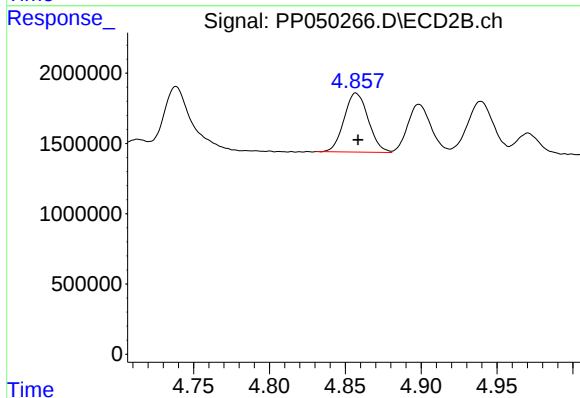


#13 AR-1232-3

R.T.: 4.857 min
Delta R.T.: -0.001 min
Response: 4653773
Conc: 138.75 ng/ml

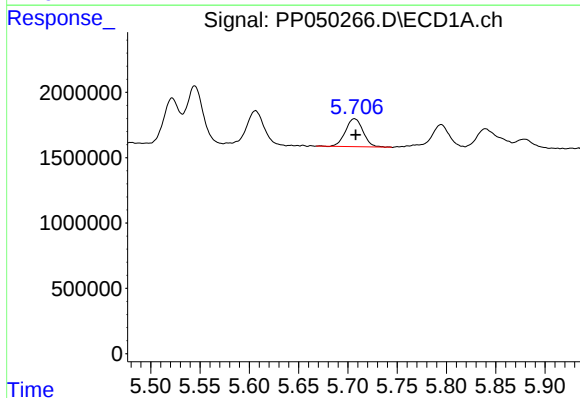


#14 AR-1232-4

R.T.: 5.707 min
Delta R.T.: -0.001 min
Response: 2663936
Conc: 131.66 ng/ml

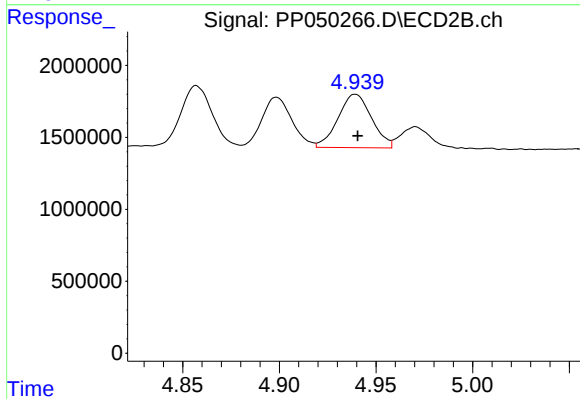

#14 AR-1232-4


R.T.: 4.939 min
Delta R.T.: -0.001 min
Response: 4482882
Conc: 152.17 ng/ml

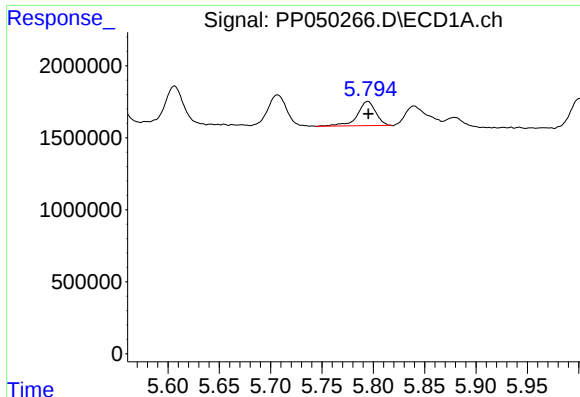

#15 AR-1232-5


R.T.: 5.794 min
Delta R.T.: 0.000 min
Response: 2096219
Conc: 134.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

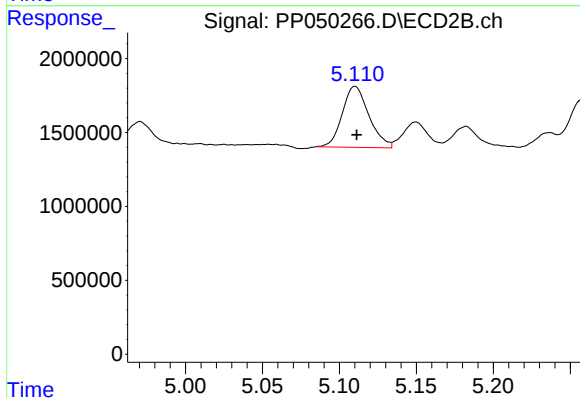


#15 AR-1232-5

R.T.: 5.110 min
Delta R.T.: -0.001 min
Response: 4955186
Conc: 150.47 ng/ml

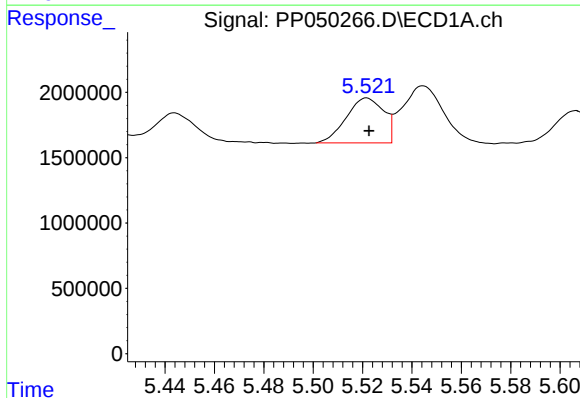


#16 AR-1242-1

R.T.: 5.522 min
Delta R.T.: 0.000 min
Response: 3607569
Conc: 71.18 ng/ml

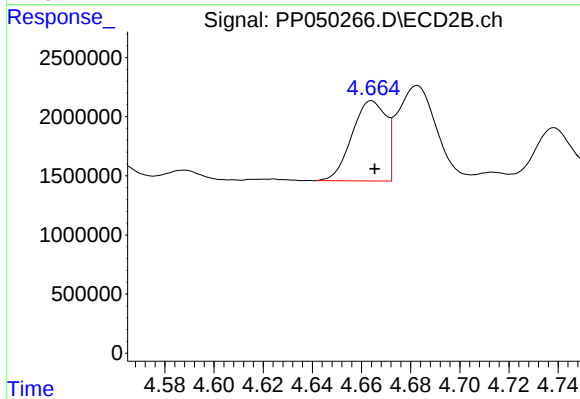

#16 AR-1242-1


R.T.: 4.664 min
Delta R.T.: -0.001 min
Response: 6544221
Conc: 78.94 ng/ml

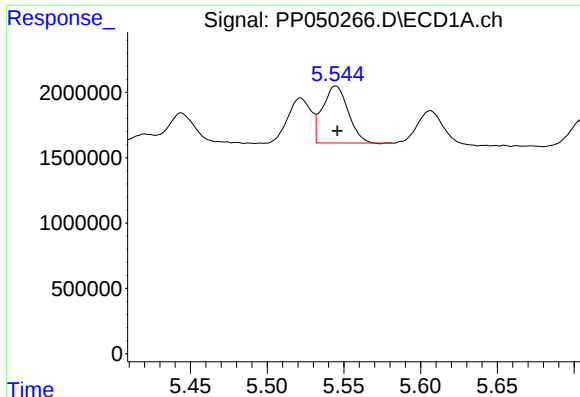

#17 AR-1242-2


R.T.: 5.545 min
Delta R.T.: -0.001 min
Response: 5044863
Conc: 69.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

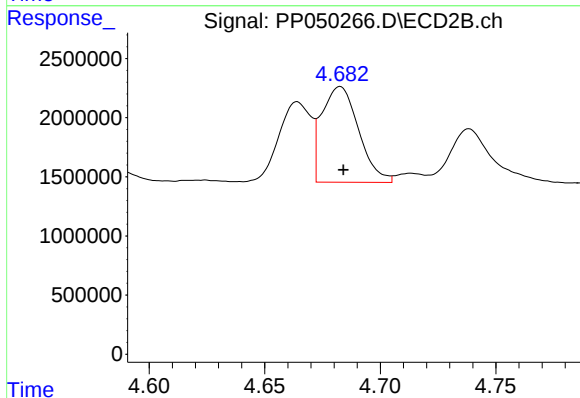


#17 AR-1242-2

R.T.: 4.683 min
Delta R.T.: -0.001 min
Response: 8967187
Conc: 76.79 ng/ml

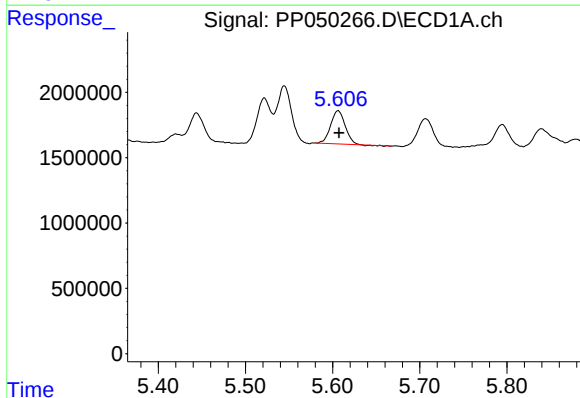


#18 AR-1242-3

R.T.: 5.606 min
Delta R.T.: -0.001 min
Response: 2930772
Conc: 66.27 ng/ml

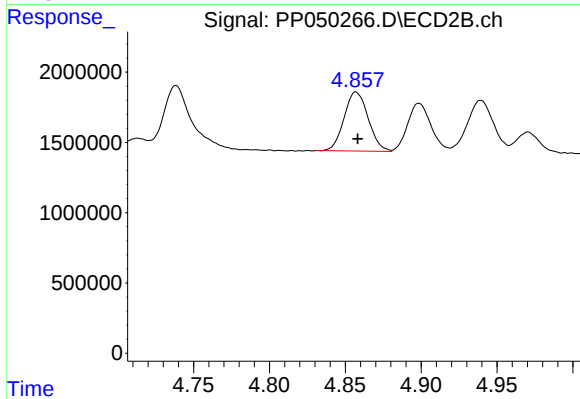

#18 AR-1242-3


R.T.: 4.857 min
Delta R.T.: -0.001 min
Response: 4653773
Conc: 75.89 ng/ml

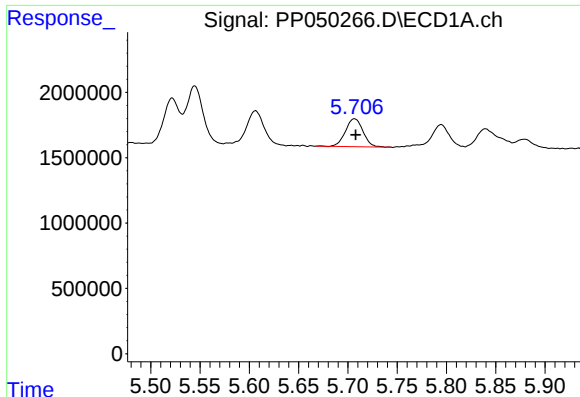

#19 AR-1242-4


R.T.: 5.707 min
Delta R.T.: -0.001 min
Response: 2663936
Conc: 71.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

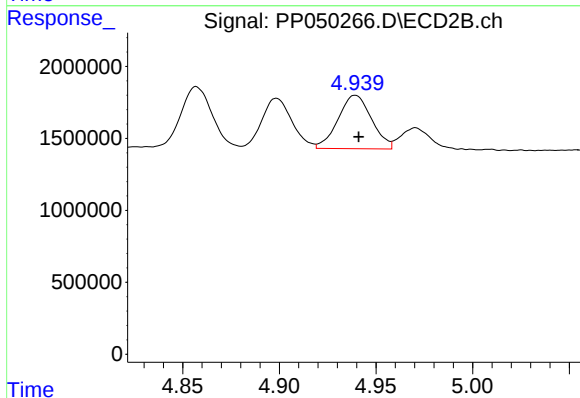


#19 AR-1242-4

R.T.: 4.939 min
Delta R.T.: -0.002 min
Response: 4482882
Conc: 76.58 ng/ml

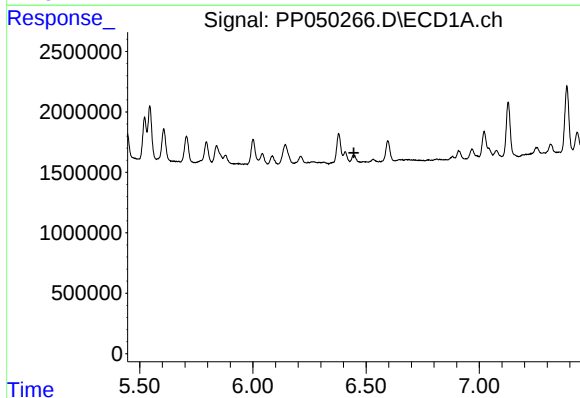


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 6.446 min
Response: 0
Conc: N.D.

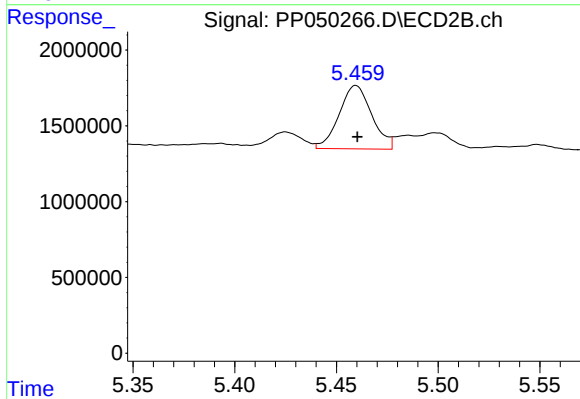

#20 AR-1242-5


R.T.: 5.460 min
Delta R.T.: 0.000 min
Response: 4679635
Conc: 67.32 ng/ml

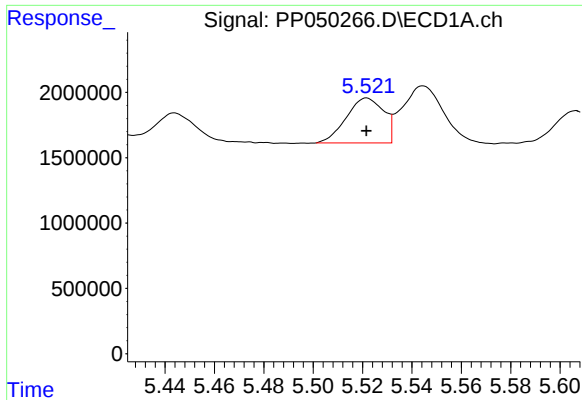

#21 AR-1248-1


R.T.: 5.522 min
Delta R.T.: 0.000 min
Response: 3607569
Conc: 89.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

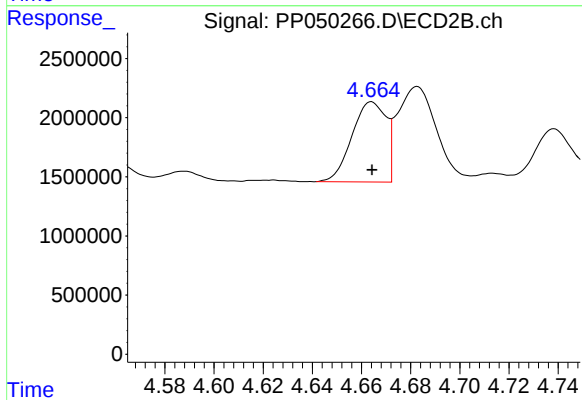


#21 AR-1248-1

R.T.: 4.664 min
Delta R.T.: 0.000 min
Response: 6544221
Conc: 97.92 ng/ml

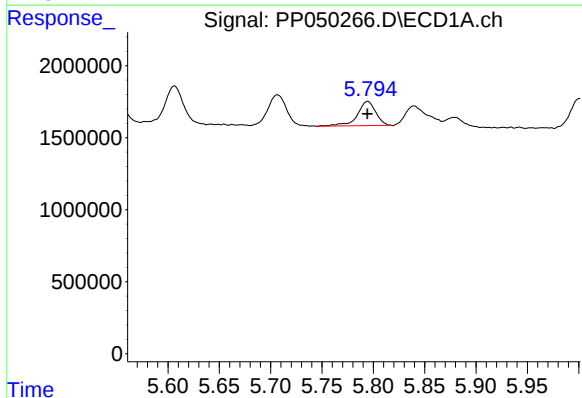


#22 AR-1248-2

R.T.: 5.794 min
Delta R.T.: 0.000 min
Response: 2096219
Conc: 37.52 ng/ml

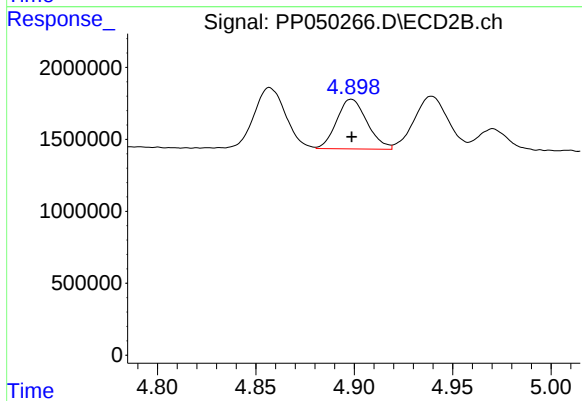

#22 AR-1248-2


R.T.: 4.899 min
Delta R.T.: 0.000 min
Response: 3722072
Conc: 43.09 ng/ml

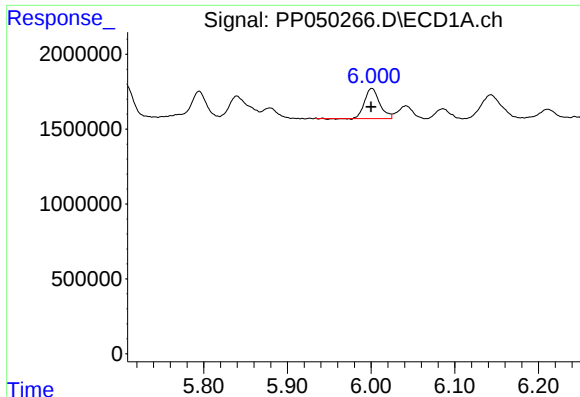

#23 AR-1248-3


R.T.: 6.001 min
Delta R.T.: 0.000 min
Response: 2536541
Conc: 39.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

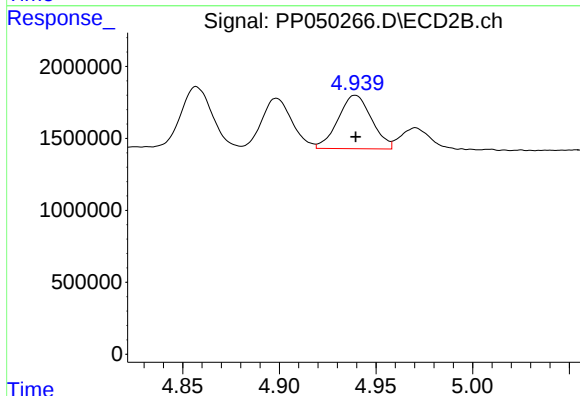


#23 AR-1248-3

R.T.: 4.939 min
Delta R.T.: 0.000 min
Response: 4482882
Conc: 49.45 ng/ml

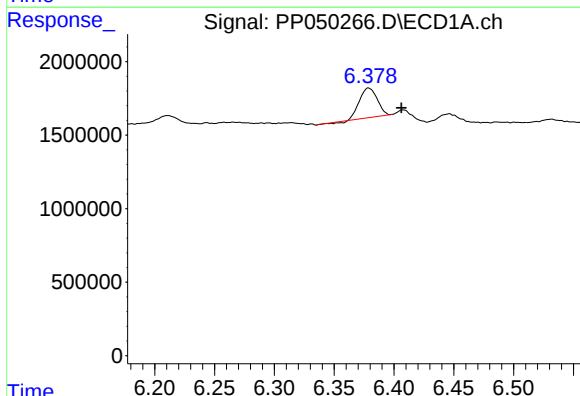


#24 AR-1248-4

R.T.: 6.379 min
Delta R.T.: -0.027 min
Response: 2038115
Conc: 25.77 ng/ml

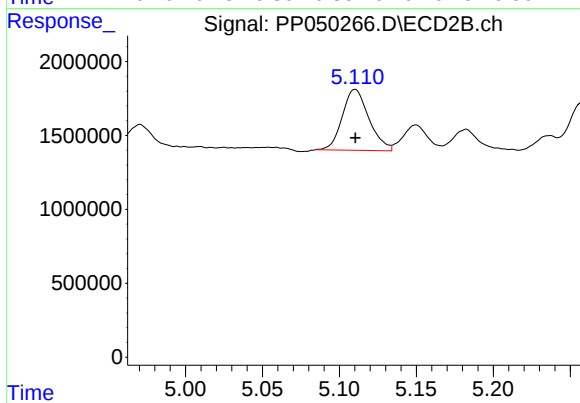

#24 AR-1248-4


R.T.: 5.110 min
Delta R.T.: 0.000 min
Response: 4955186
Conc: 47.01 ng/ml

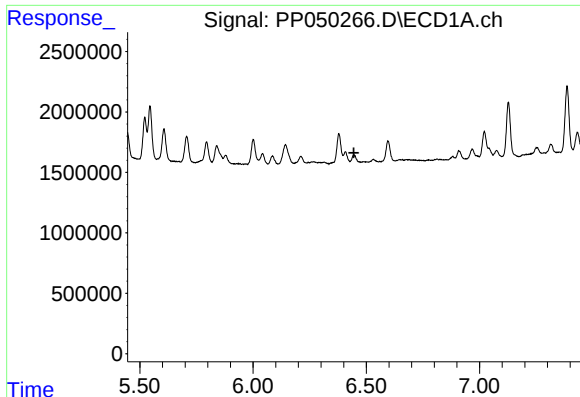

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.445 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

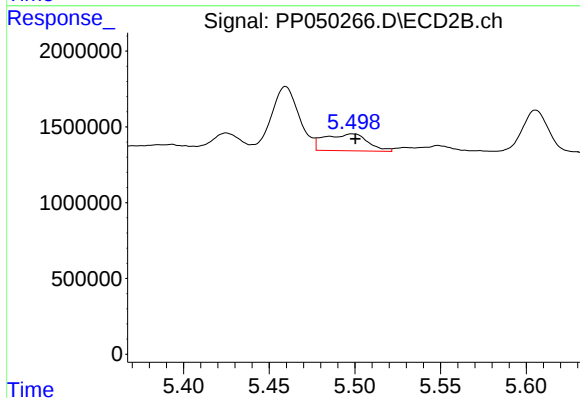


#25 AR-1248-5

R.T.: 5.499 min
Delta R.T.: -0.002 min
Response: 1954567
Conc: 19.69 ng/ml

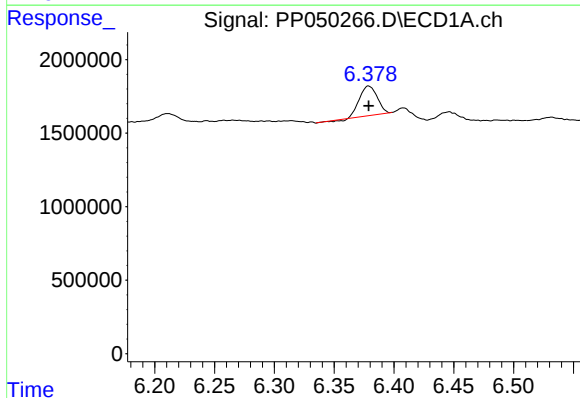


#26 AR-1254-1

R.T.: 6.379 min
Delta R.T.: 0.000 min
Response: 2038115
Conc: 29.40 ng/ml

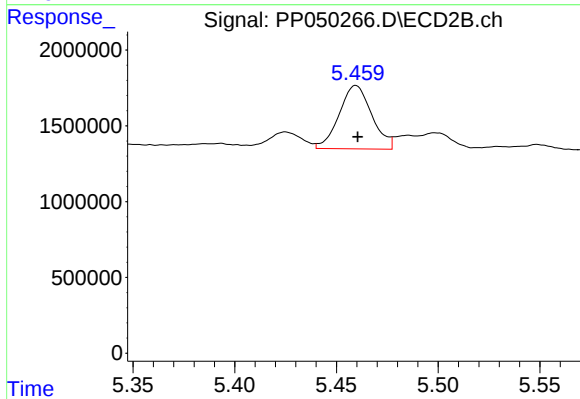

#26 AR-1254-1


R.T.: 5.460 min
Delta R.T.: 0.000 min
Response: 4679635
Conc: 35.41 ng/ml

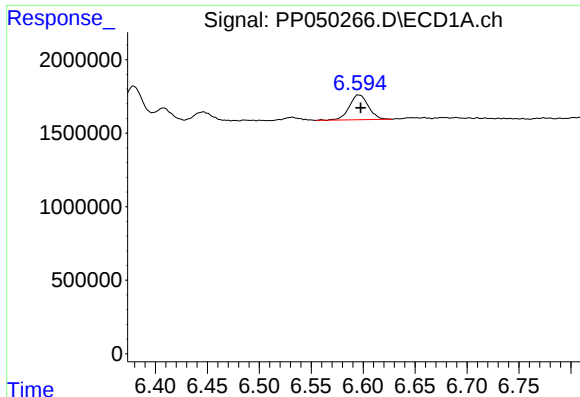

#27 AR-1254-2


R.T.: 6.596 min
Delta R.T.: -0.001 min
Response: 2163644
Conc: 20.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

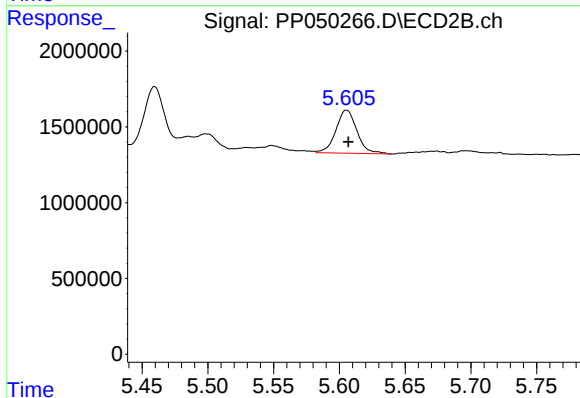


#27 AR-1254-2

R.T.: 5.606 min
Delta R.T.: -0.001 min
Response: 3170819
Conc: 29.10 ng/ml

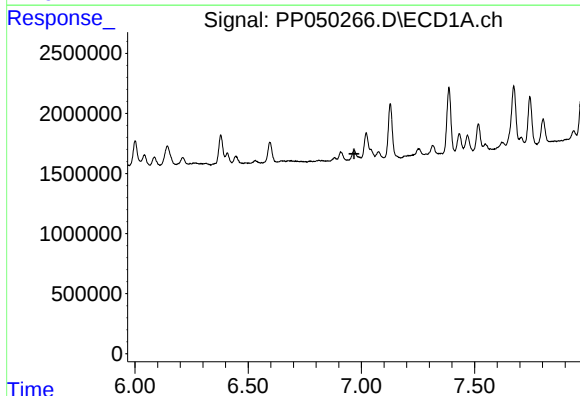


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.967 min
Response: 0
Conc: N.D.

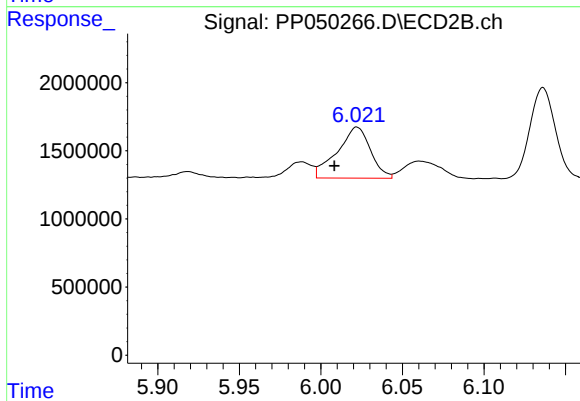

#28 AR-1254-3


R.T.: 6.022 min
Delta R.T.: 0.014 min
Response: 5328754
Conc: 33.48 ng/ml

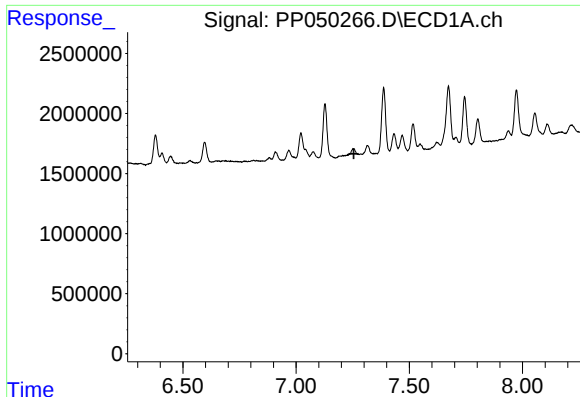

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.255 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

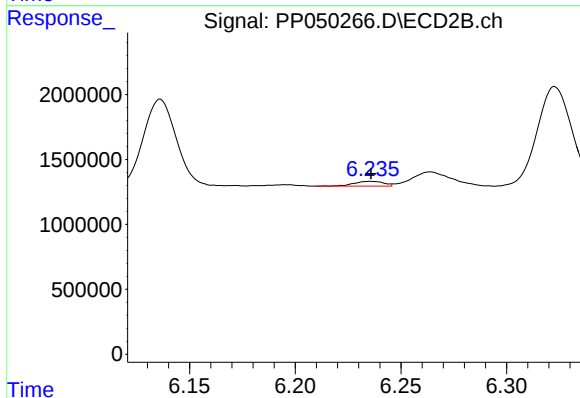


#29 AR-1254-4

R.T.: 6.236 min
Delta R.T.: 0.000 min
Response: 368892
Conc: 3.79 ng/ml

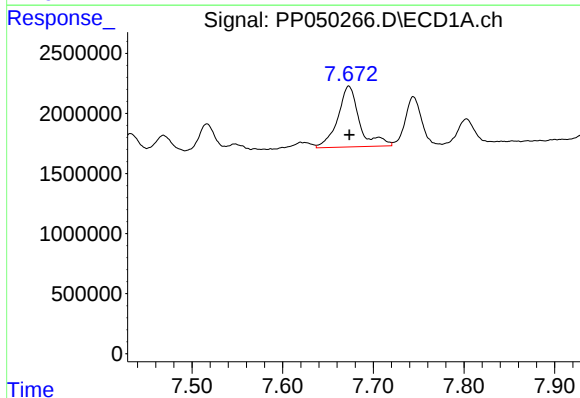


#30 AR-1254-5

R.T.: 7.673 min
Delta R.T.: 0.000 min
Response: 8433564
Conc: 89.23 ng/ml

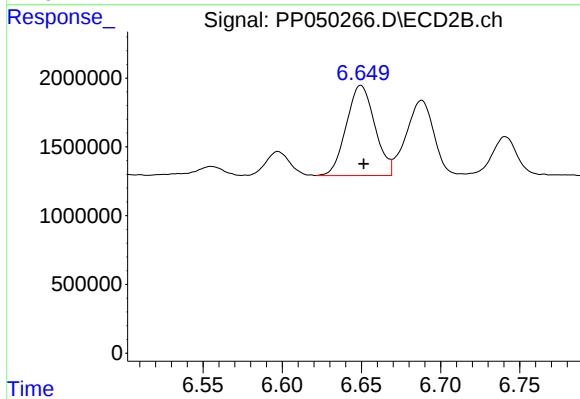

#30 AR-1254-5


R.T.: 6.650 min
Delta R.T.: -0.002 min
Response: 8223272
Conc: 66.71 ng/ml

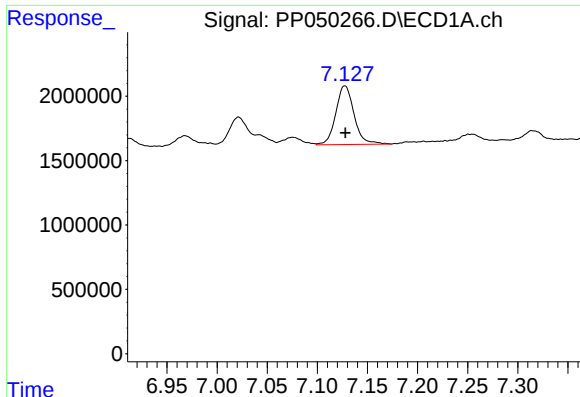

#31 AR-1260-1


R.T.: 7.128 min
Delta R.T.: 0.000 min
Response: 5771330
Conc: 63.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

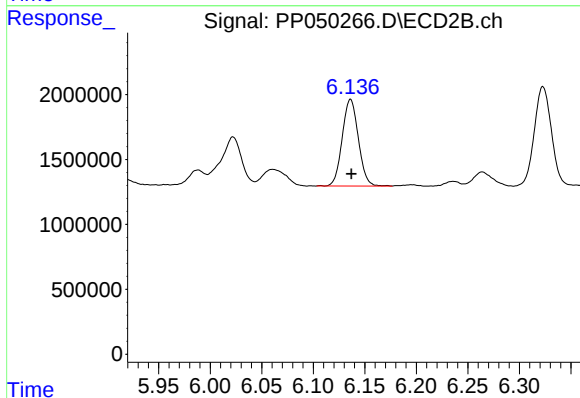


#31 AR-1260-1

R.T.: 6.136 min
Delta R.T.: 0.000 min
Response: 7297106
Conc: 64.40 ng/ml

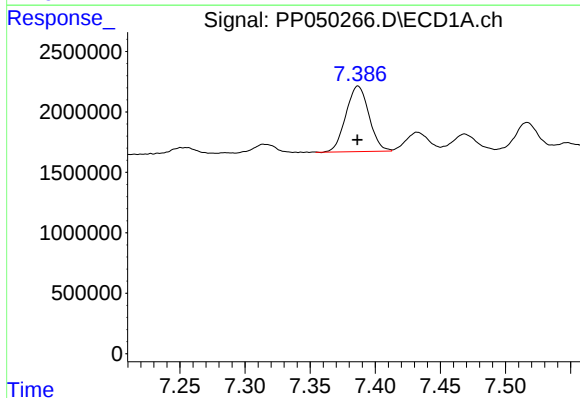


#32 AR-1260-2

R.T.: 7.387 min
Delta R.T.: 0.000 min
Response: 6684779
Conc: 58.51 ng/ml

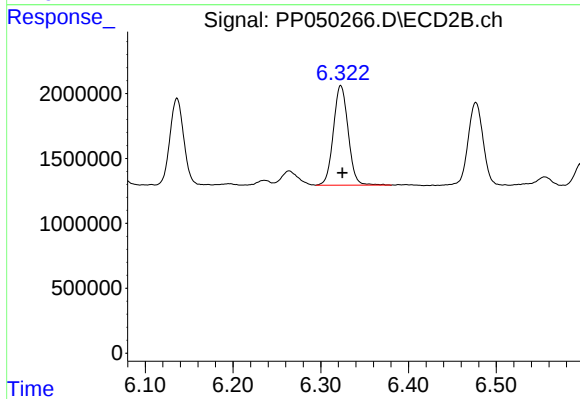

#32 AR-1260-2


R.T.: 6.323 min
Delta R.T.: -0.002 min
Response: 8960635
Conc: 66.70 ng/ml

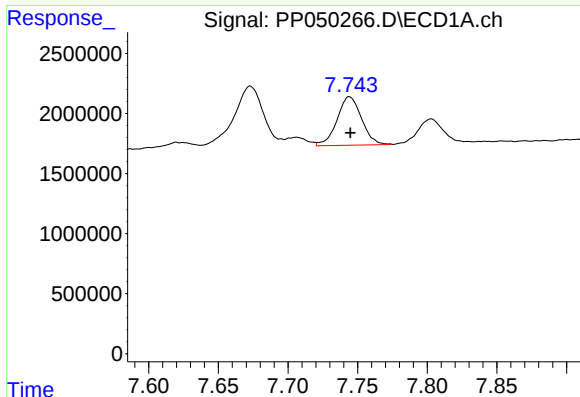

#33 AR-1260-3


R.T.: 7.744 min
Delta R.T.: 0.000 min
Response: 4942313
Conc: 58.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

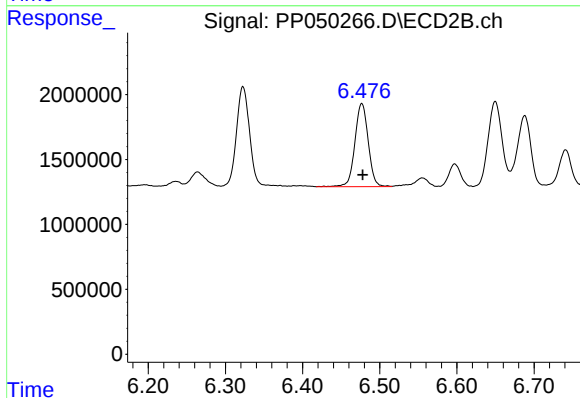


#33 AR-1260-3

R.T.: 6.477 min
Delta R.T.: -0.001 min
Response: 7702391
Conc: 63.94 ng/ml

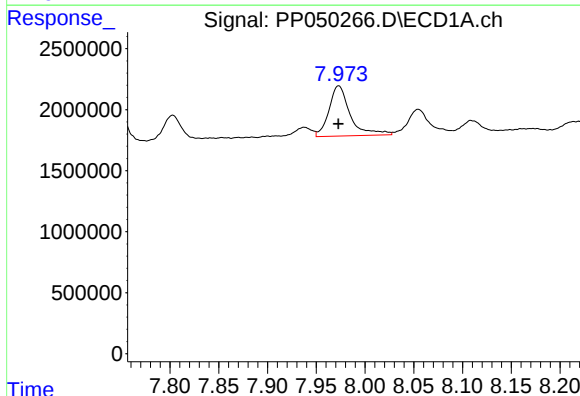


#34 AR-1260-4

R.T.: 7.973 min
Delta R.T.: 0.000 min
Response: 6251589
Conc: 65.68 ng/ml

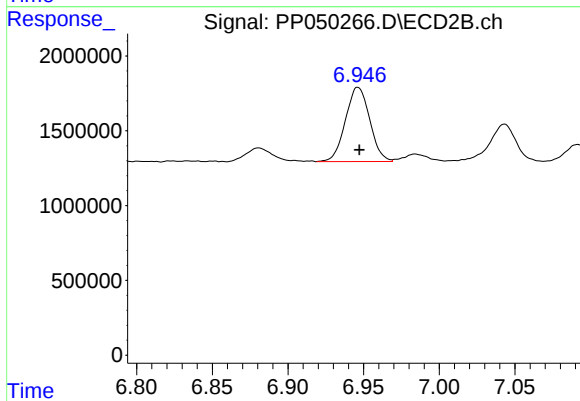

#34 AR-1260-4


R.T.: 6.946 min
Delta R.T.: 0.000 min
Response: 5554037
Conc: 62.65 ng/ml

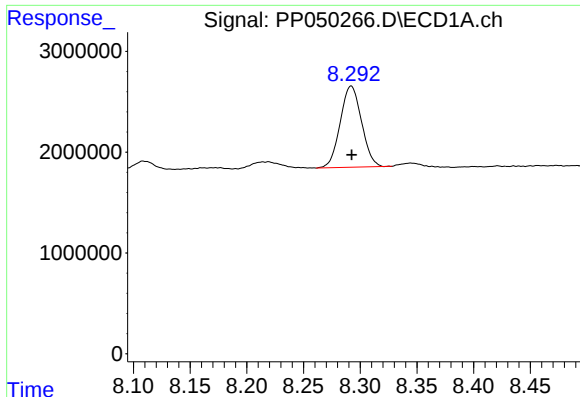

#35 AR-1260-5


R.T.: 8.292 min
Delta R.T.: 0.000 min
Response: 10534440
Conc: 56.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

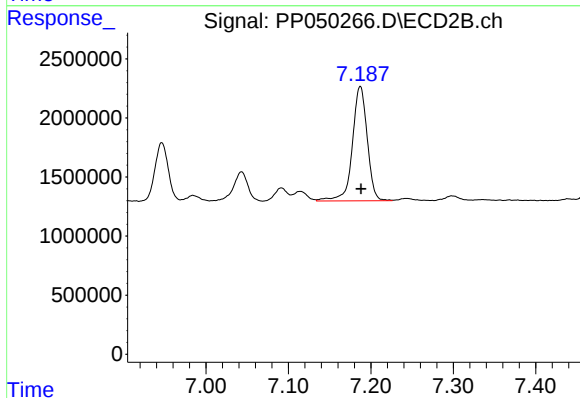


#35 AR-1260-5

R.T.: 7.187 min
Delta R.T.: -0.001 min
Response: 12158100
Conc: 62.37 ng/ml

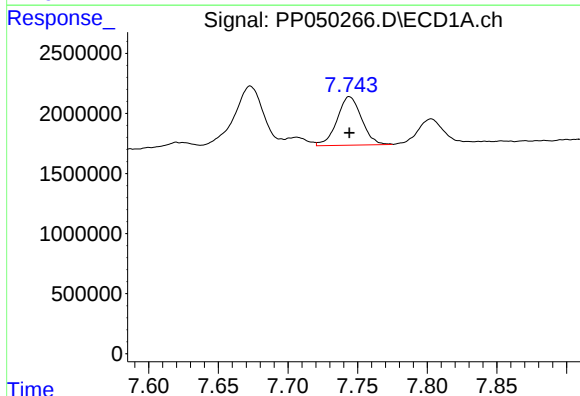


#36 AR-1262-1

R.T.: 7.744 min
Delta R.T.: 0.000 min
Response: 4942313
Conc: 41.27 ng/ml

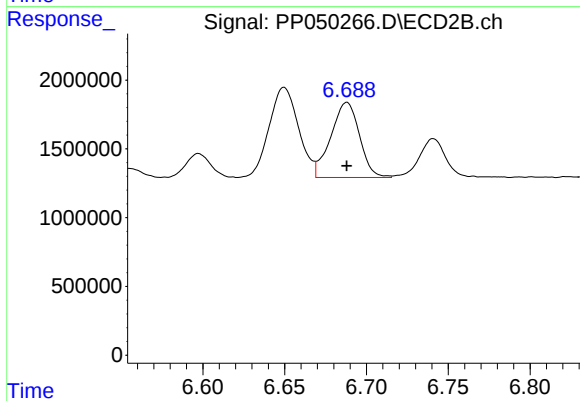

#36 AR-1262-1


R.T.: 6.688 min
Delta R.T.: 0.000 min
Response: 6686490
Conc: 49.48 ng/ml

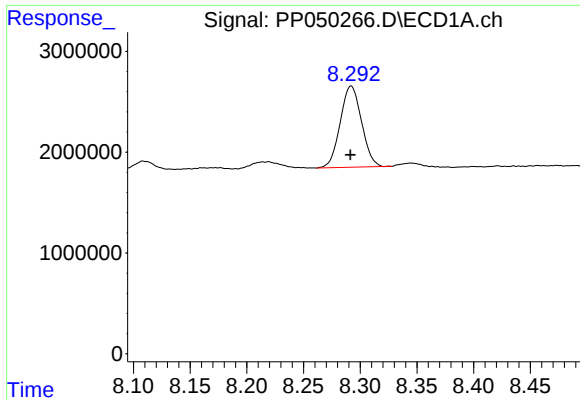

#37 AR-1262-2


R.T.: 8.292 min
Delta R.T.: 0.000 min
Response: 10534440
Conc: 48.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

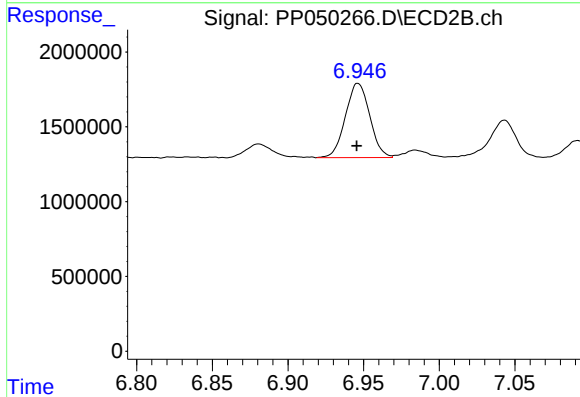


#37 AR-1262-2

R.T.: 6.946 min
Delta R.T.: 0.000 min
Response: 5554037
Conc: 51.11 ng/ml

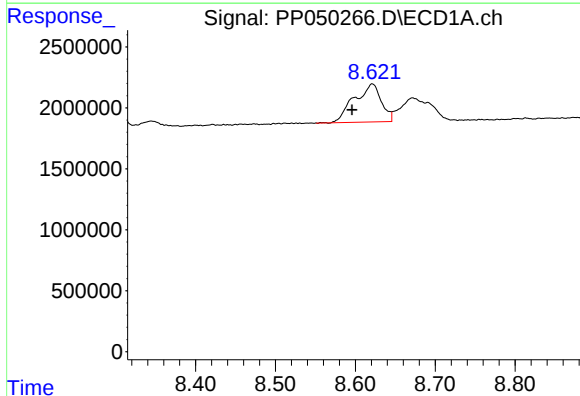


#38 AR-1262-3

R.T.: 8.621 min
Delta R.T.: 0.025 min
Response: 7345966
Conc: 74.76 ng/ml

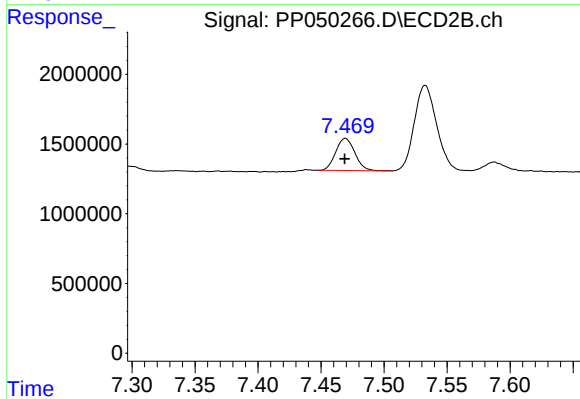

#38 AR-1262-3


R.T.: 7.469 min
Delta R.T.: 0.000 min
Response: 2431412
Conc: 33.50 ng/ml

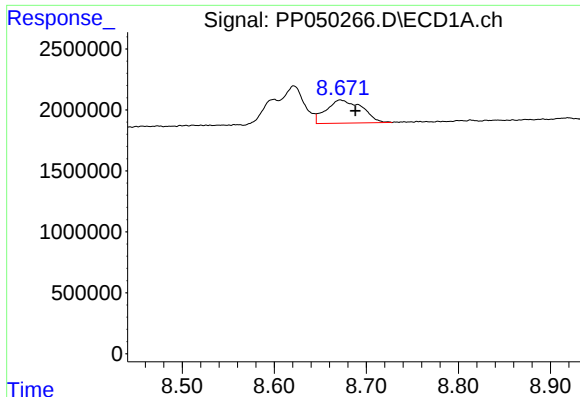

#39 AR-1262-4


R.T.: 8.672 min
Delta R.T.: -0.016 min
Response: 5131034
Conc: 79.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

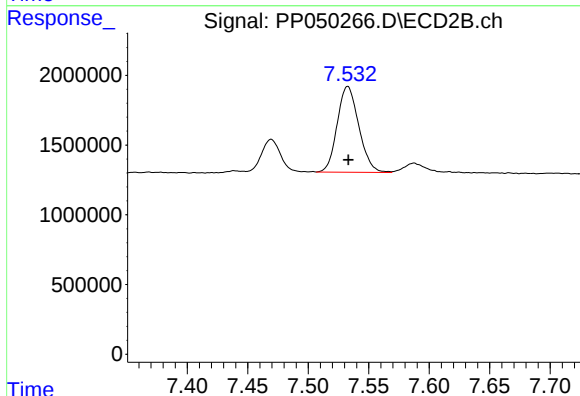


#39 AR-1262-4

R.T.: 7.533 min
Delta R.T.: 0.000 min
Response: 7637401
Conc: 55.39 ng/ml

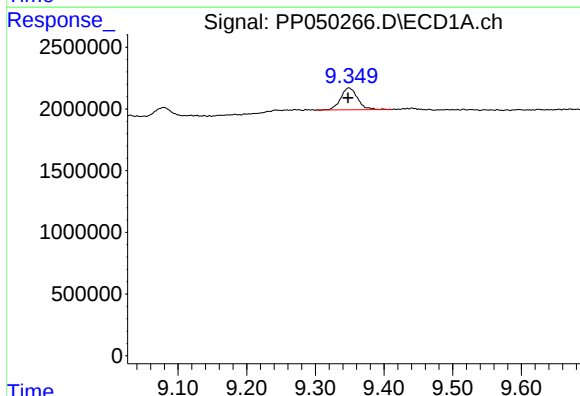


#40 AR-1262-5

R.T.: 9.349 min
Delta R.T.: 0.001 min
Response: 3013912
Conc: 38.18 ng/ml

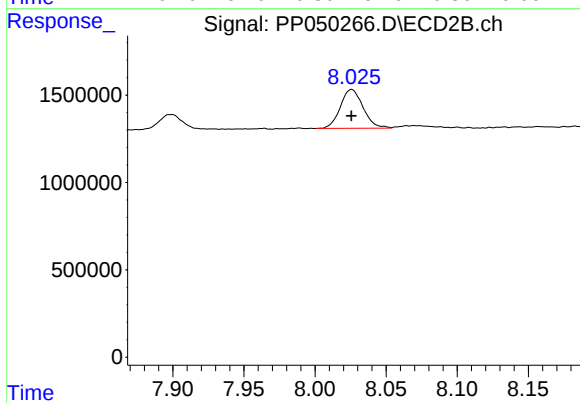

#40 AR-1262-5


R.T.: 8.026 min
Delta R.T.: 0.000 min
Response: 2479899
Conc: 38.50 ng/ml

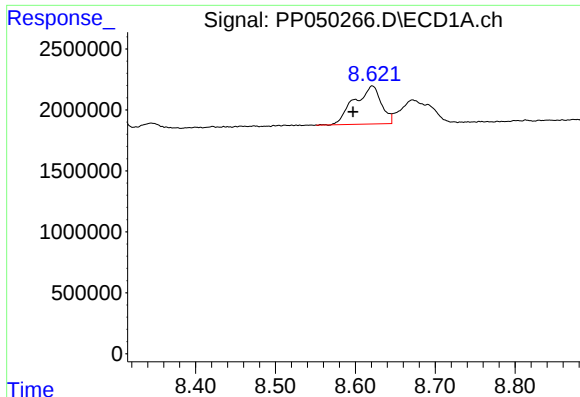

#41 AR-1268-1


R.T.: 8.621 min
Delta R.T.: 0.024 min
Response: 7345966
Conc: 28.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

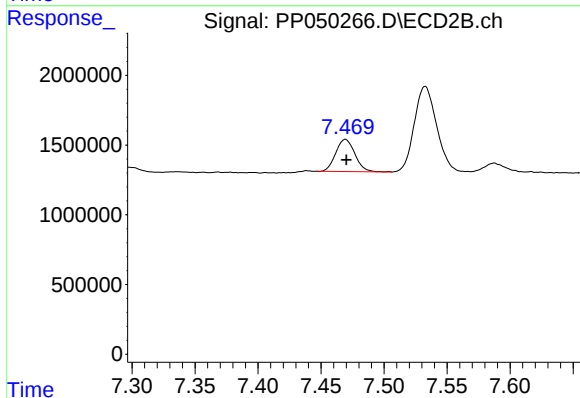


#41 AR-1268-1

R.T.: 7.469 min
Delta R.T.: 0.000 min
Response: 2431412
Conc: 11.07 ng/ml

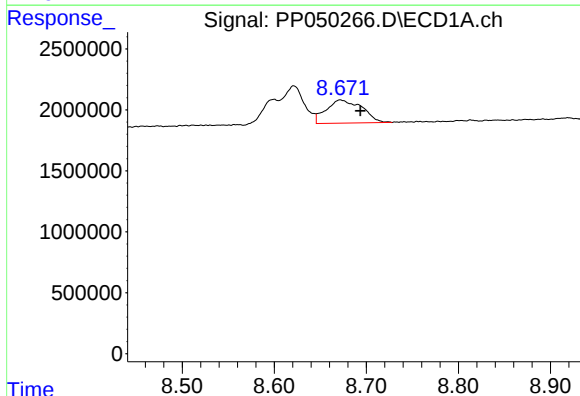


#42 AR-1268-2

R.T.: 8.672 min
Delta R.T.: -0.021 min
Response: 5131034
Conc: 21.04 ng/ml

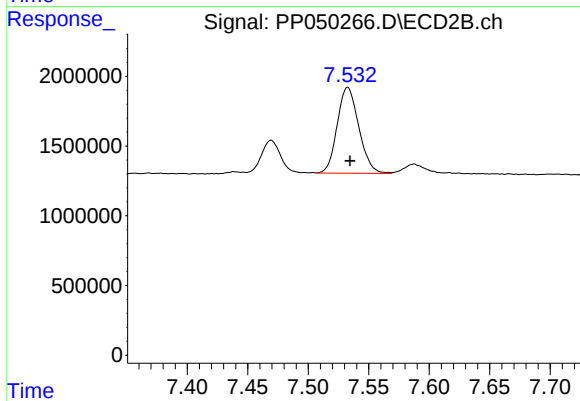

#42 AR-1268-2


R.T.: 7.533 min
Delta R.T.: -0.002 min
Response: 7637401
Conc: 38.35 ng/ml

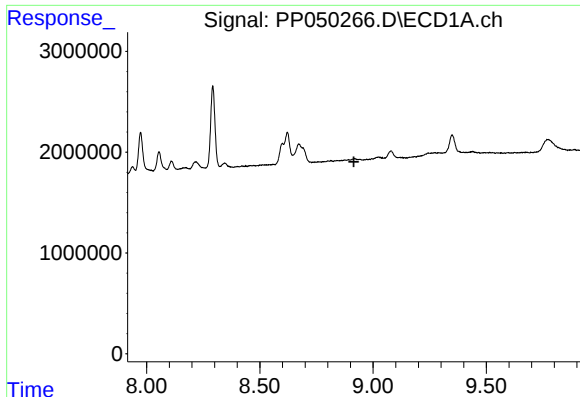

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.915 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

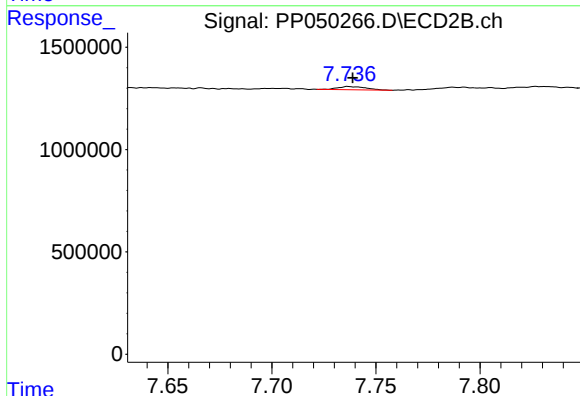


#43 AR-1268-3

R.T.: 7.737 min
Delta R.T.: -0.002 min
Response: 150860
Conc: 0.89 ng/ml

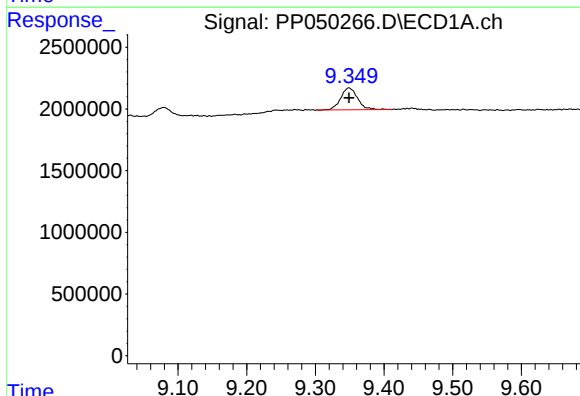


#44 AR-1268-4

R.T.: 9.349 min
Delta R.T.: 0.000 min
Response: 3013912
Conc: 34.97 ng/ml

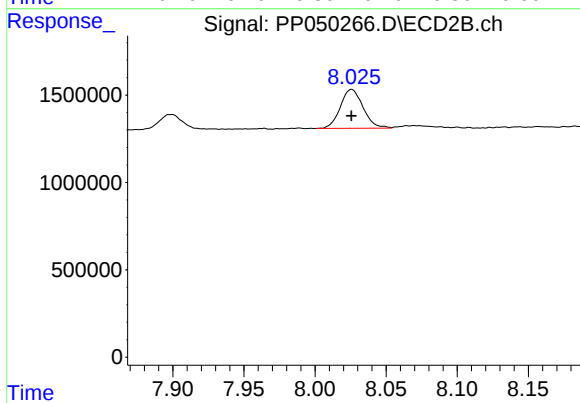

#44 AR-1268-4


R.T.: 8.026 min
Delta R.T.: 0.000 min
Response: 2479899
Conc: 34.90 ng/ml

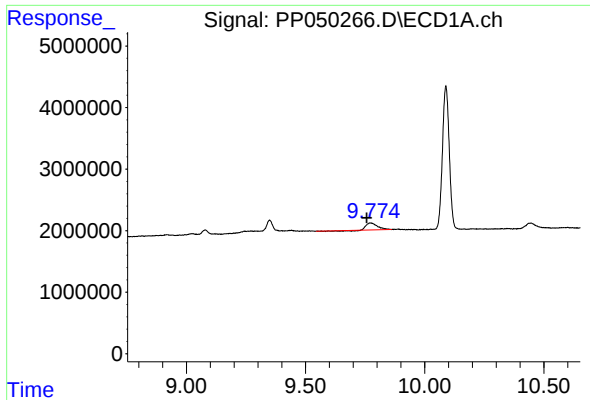

#45 AR-1268-5

R.T.: 9.772 min
Delta R.T.: 0.015 min
Response: 3274093
Conc: 4.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

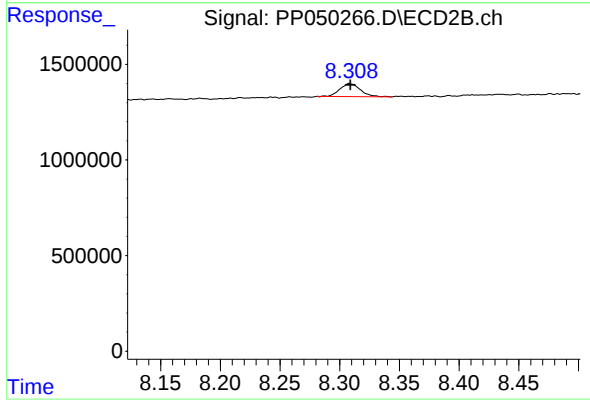

#45 AR-1268-5

R.T.: 8.308 min
Delta R.T.: 0.000 min
Response: 819464
Conc: 1.49 ng/ml