

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP080622\  
 Data File : PP050268.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 06 Aug 2022 18:46  
 Operator : YP\AJ  
 Sample : N3980-07  
 Misc : AR1232 LOD 40 PPB  
 ALS Vial : 64 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 LOD-MDL-WATER-01-QT3-2022

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Aug 08 00:34:52 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP080622.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Sun Aug 07 23:52:23 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound        | RT#1   | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml    |
|-----------------------------|-----------------|--------|-------|----------|----------|--------|----------|
| -----                       |                 |        |       |          |          |        |          |
| System Monitoring Compounds |                 |        |       |          |          |        |          |
| 1)                          | SA Tetrachlo... | 4.345  | 3.591 | 38807680 | 78347662 | 24.109 | 25.013   |
| 2)                          | SA Decachlor... | 10.090 | 8.555 | 44296821 | 38086821 | 25.156 | 24.746   |
| Target Compounds            |                 |        |       |          |          |        |          |
| 3)                          | L1 AR-1016-1    | 5.523  | 4.665 | 1278144  | 2510669  | 20.413 | 24.700   |
| 4)                          | L1 AR-1016-2    | 5.545  | 4.682 | 1750520  | 3574046  | 19.768 | 24.710   |
| 5)                          | L1 AR-1016-3    | 0.000  | 4.857 | 0        | 1690769  | N.D.   | 22.281 # |
| 6)                          | L1 AR-1016-4    | 0.000  | 4.899 | 0        | 1298397  | N.D.   | 22.284 # |
| 7)                          | L1 AR-1016-5    | 0.000  | 5.110 | 0        | 1893895  | N.D.   | 24.787 # |
| 8)                          | L2 AR-1221-1    | 0.000  | 3.802 | 0        | 1173906  | N.D.   | 30.713 # |
| 9)                          | L2 AR-1221-2    | 0.000  | 3.888 | 0        | 1816838  | N.D.   | 63.625 # |
| 10)                         | L2 AR-1221-3    | 4.722  | 3.962 | 1871981  | 3726046  | 41.608 | 43.523   |
| 11)                         | L3 AR-1232-1    | 4.722  | 3.962 | 1871981  | 3726046  | 50.077 | 53.375   |
| 12)                         | L3 AR-1232-2    | 0.000  | 4.682 | 0        | 3574046  | N.D.   | 55.592 # |
| 13)                         | L3 AR-1232-3    | 5.545  | 4.857 | 1750520  | 1690769  | 44.457 | 50.410   |
| 14)                         | L3 AR-1232-4    | 0.000  | 4.939 | 0        | 1522299  | N.D.   | 51.674 # |
| 15)                         | L3 AR-1232-5    | 0.000  | 5.110 | 0        | 1893895  | N.D.   | 57.512 # |
| 16)                         | L4 AR-1242-1    | 5.523  | 4.665 | 1278144  | 2510669  | 25.219 | 30.286   |
| 17)                         | L4 AR-1242-2    | 5.545  | 4.682 | 1750520  | 3574046  | 24.232 | 30.605 # |
| 18)                         | L4 AR-1242-3    | 0.000  | 4.857 | 0        | 1690769  | N.D.   | 27.573 # |
| 19)                         | L4 AR-1242-4    | 0.000  | 4.939 | 0        | 1522299  | N.D.   | 26.005 # |
| 20)                         | L4 AR-1242-5    | 0.000  | 5.459 | 0        | 1845650  | N.D.   | 26.552 # |
| 21)                         | L5 AR-1248-1    | 5.523  | 4.665 | 1278144  | 2510669  | 31.655 | 37.565   |
| 22)                         | L5 AR-1248-2    | 0.000  | 4.899 | 0        | 1298397  | N.D.   | 15.030 # |
| 23)                         | L5 AR-1248-3    | 0.000  | 4.939 | 0        | 1522299  | N.D.   | 16.792 # |
| 24)                         | L5 AR-1248-4    | 6.382f | 5.110 | 621538   | 1893895  | 7.857  | 17.969 # |
| 25)                         | L5 AR-1248-5    | 0.000  | 5.500 | 0        | 1940971  | N.D.   | 19.549 # |
| 26)                         | L6 AR-1254-1    | 6.382  | 5.459 | 621538   | 1845650  | 8.965  | 13.967 # |
| 27)                         | L6 AR-1254-2    | 0.000  | 5.605 | 0        | 539255   | N.D.   | 4.948 #  |
| 28)                         | L6 AR-1254-3    | 0.000  | 6.008 | 0        | 870507   | N.D.   | 5.469 #  |
| 29)                         | L6 AR-1254-4    | 0.000  | 6.236 | 0        | 367333   | N.D.   | 3.778 #  |
| 30)                         | L6 AR-1254-5    | 0.000  | 6.653 | 0        | 248532   | N.D.   | 2.016 #  |
| 31)                         | L7 AR-1260-1    | 0.000  | 6.136 | 0        | 256117   | N.D.   | 2.260 #  |
| 32)                         | L7 AR-1260-2    | 0.000  | 6.314 | 0        | 587200   | N.D.   | 4.371 #  |
| 33)                         | L7 AR-1260-3    | 0.000  | 6.475 | 0        | 338455   | N.D.   | 2.810 #  |
| 35)                         | L7 AR-1260-5    | 8.294  | 7.187 | 2463719  | 206770   | 13.180 | 1.061 #  |
| 36)                         | L8 AR-1262-1    | 0.000  | 6.686 | 0        | 195700   | N.D.   | 1.448 #  |
| 37)                         | L8 AR-1262-2    | 8.294  | 0.000 | 2463719  | 0        | 11.402 | N.D. #   |
| 38)                         | L8 AR-1262-3    | 0.000  | 7.469 | 0        | 596137   | N.D.   | 8.214 #  |
| 39)                         | L8 AR-1262-4    | 0.000  | 7.532 | 0        | 410752   | N.D.   | 2.979 #  |
| 41)                         | L9 AR-1268-1    | 0.000  | 7.469 | 0        | 596137   | N.D.   | 2.713 #  |
| 42)                         | L9 AR-1268-2    | 0.000  | 7.532 | 0        | 410752   | N.D.   | 2.062 #  |
| 45)                         | L9 AR-1268-5    | 9.781f | 8.309 | 3425272  | 318800   | 5.136  | 0.579 #  |

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP080622\  
Data File : PP050268.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 06 Aug 2022 18:46  
Operator : YP\AJ  
Sample : N3980-07  
Misc : AR1232 LOD 40 PPB  
ALS Vial : 64 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
LOD-MDL-WATER-01-QT3-2022

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Aug 08 00:34:52 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP080622.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Sun Aug 07 23:52:23 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
| -----    |      |      |        |        |       |       |
| -----    |      |      |        |        |       |       |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP080622\  
Data File : PP050268.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 06 Aug 2022 18:46  
Operator : YP\AJ  
Sample : N3980-07  
Misc : AR1232 LOD 40 PPB  
ALS Vial : 64 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
LOD-MDL-WATER-01-QT3-2022

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Aug 08 00:34:52 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP080622.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Sun Aug 07 23:52:23 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

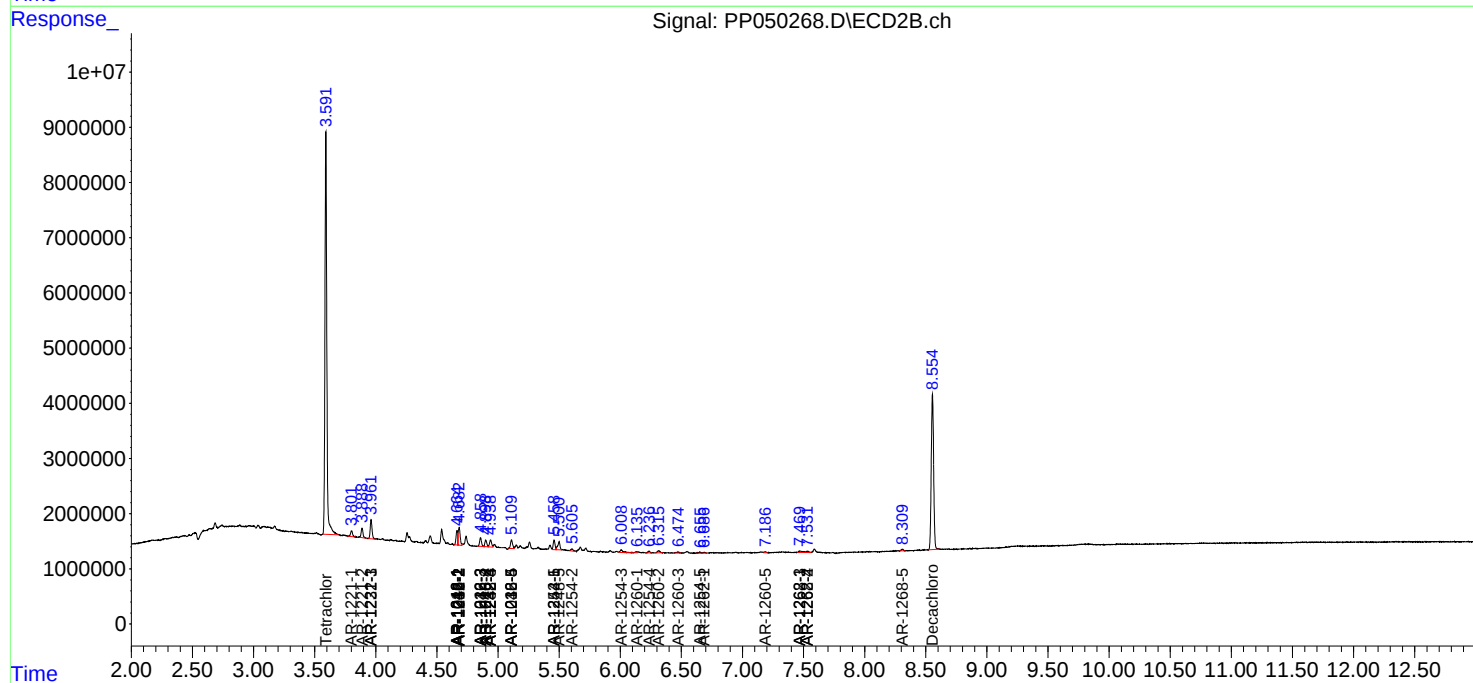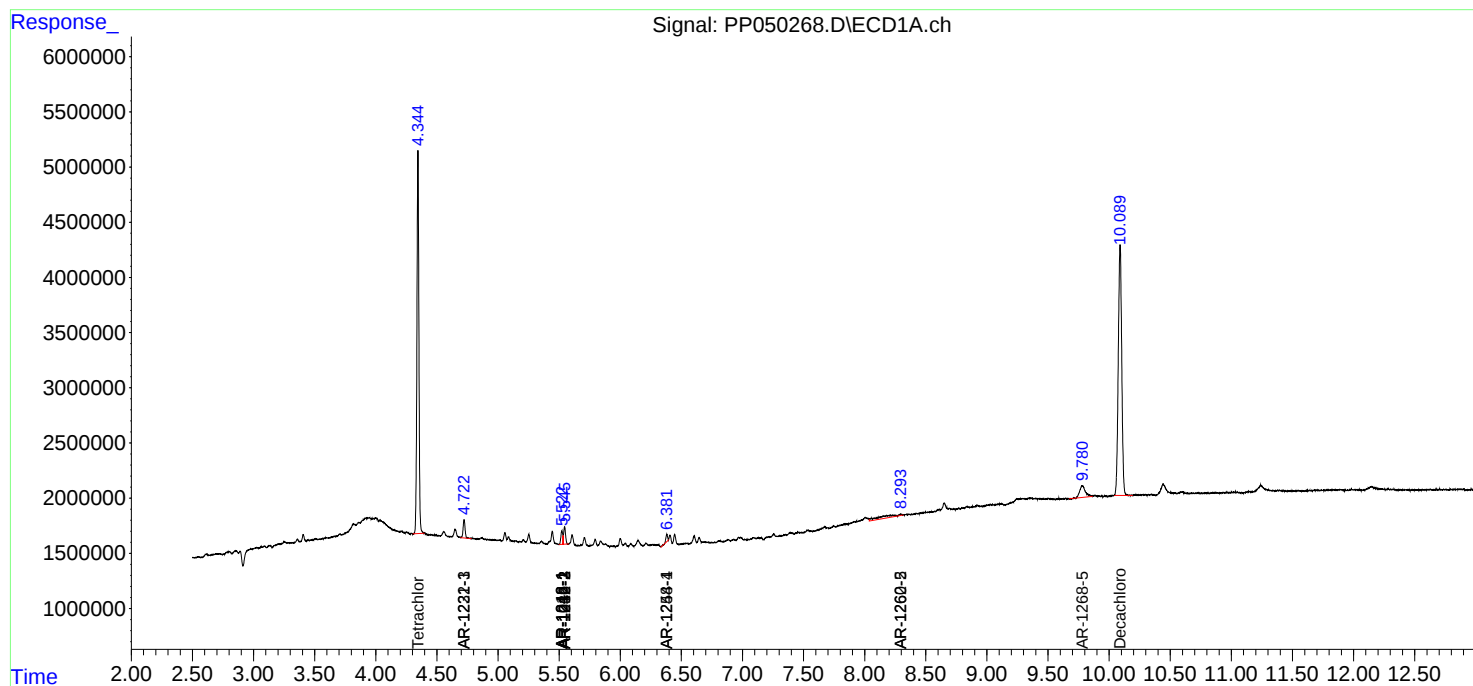


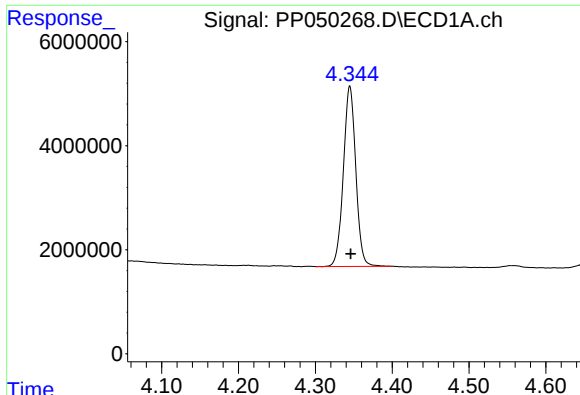

#1 Tetrachloro-m-xylene


R.T.: 4.345 min  
Delta R.T.: -0.001 min  
Response: 38807680  
Conc: 24.11 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
LOD-MDL-WATER-01-QT3-2022

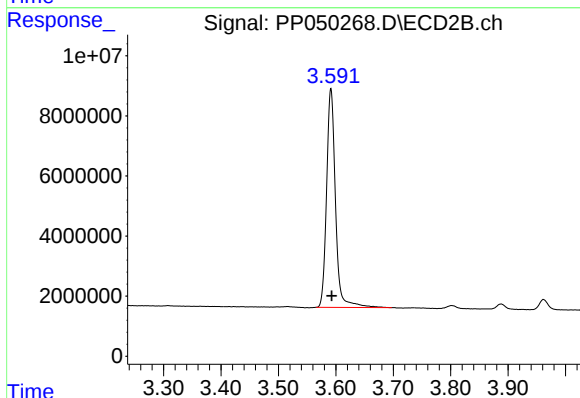


#1 Tetrachloro-m-xylene

R.T.: 3.591 min  
Delta R.T.: -0.001 min  
Response: 78347662  
Conc: 25.01 ng/ml

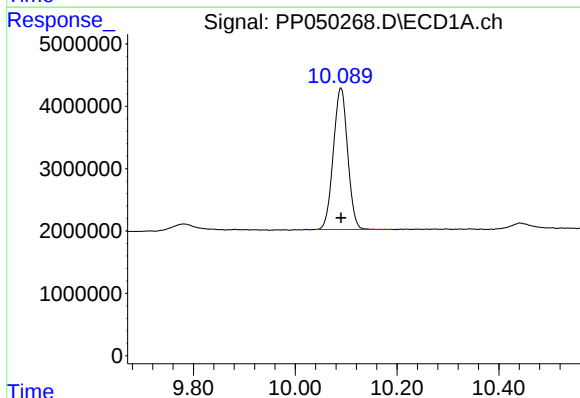


#2 Decachlorobiphenyl

R.T.: 10.090 min  
Delta R.T.: 0.000 min  
Response: 44296821  
Conc: 25.16 ng/ml

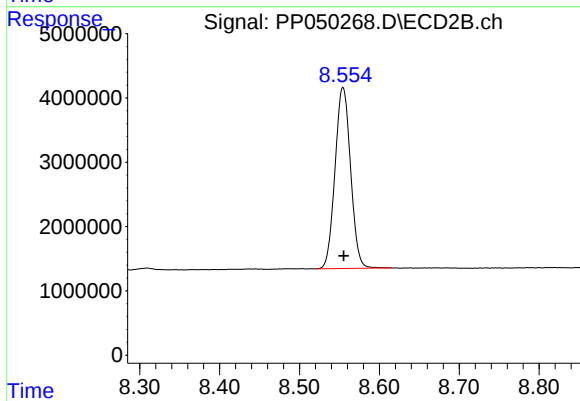

#2 Decachlorobiphenyl


R.T.: 8.555 min  
Delta R.T.: 0.000 min  
Response: 38086821  
Conc: 24.75 ng/ml

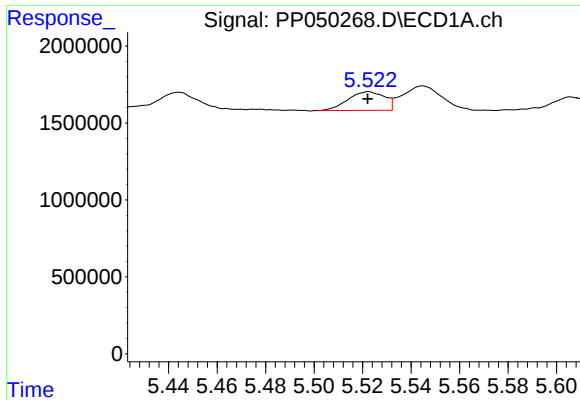

#3 AR-1016-1


R.T.: 5.523 min  
Delta R.T.: 0.000 min  
Response: 1278144  
Conc: 20.41 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
LOD-MDL-WATER-01-QT3-2022

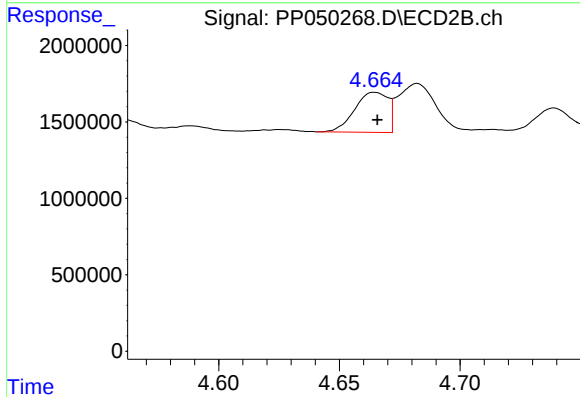


#3 AR-1016-1

R.T.: 4.665 min  
Delta R.T.: -0.001 min  
Response: 2510669  
Conc: 24.70 ng/ml

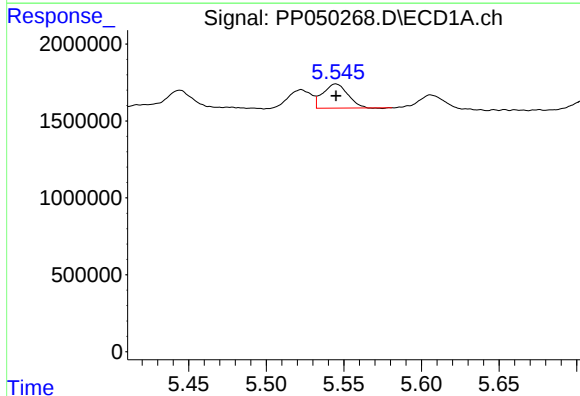


#4 AR-1016-2

R.T.: 5.545 min  
Delta R.T.: 0.000 min  
Response: 1750520  
Conc: 19.77 ng/ml

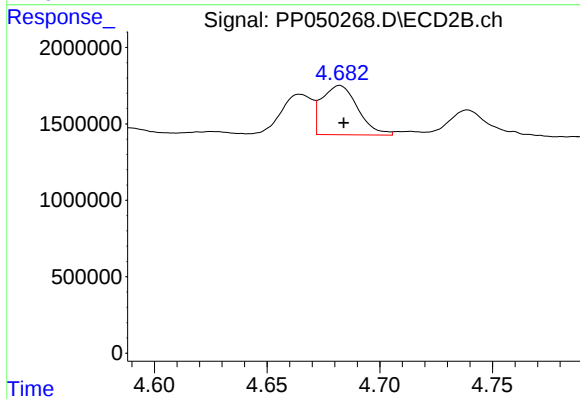

#4 AR-1016-2


R.T.: 4.682 min  
Delta R.T.: -0.002 min  
Response: 3574046  
Conc: 24.71 ng/ml

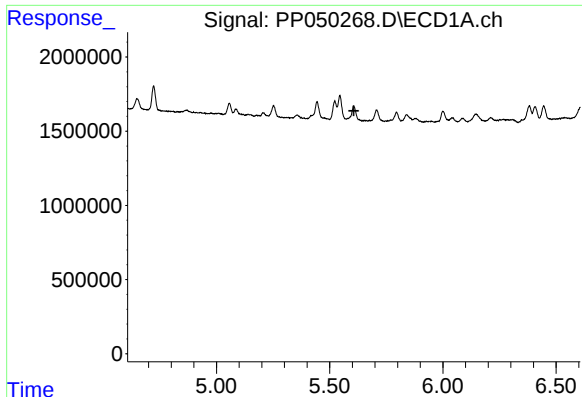

#5 AR-1016-3


R.T.: 0.000 min  
Exp R.T.: 5.606 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_P  
ClientSampleId :  
LOD-MDL-WATER-01-QT3-2022

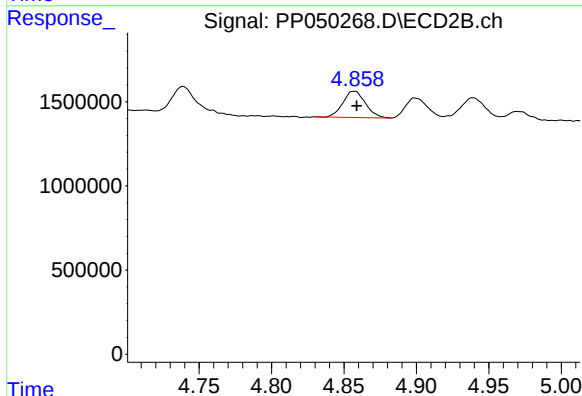


#5 AR-1016-3

R.T.: 4.857 min  
Delta R.T.: -0.002 min  
Response: 1690769  
Conc: 22.28 ng/ml

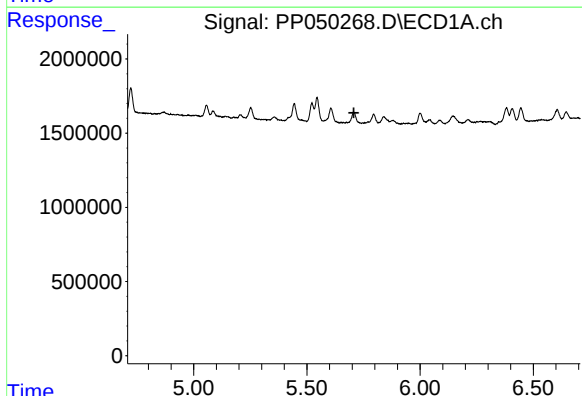


#6 AR-1016-4

R.T.: 0.000 min  
Exp R.T.: 5.707 min  
Response: 0  
Conc: N.D.

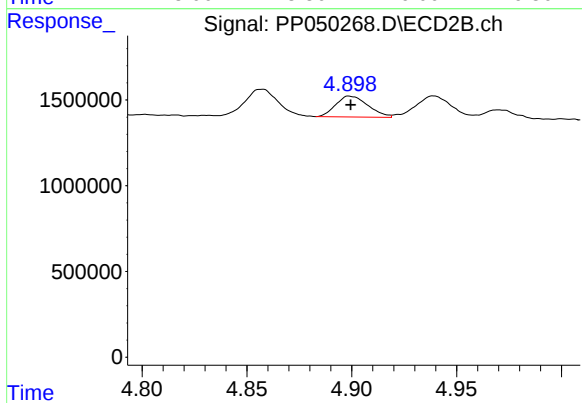

#6 AR-1016-4


R.T.: 4.899 min  
Delta R.T.: 0.000 min  
Response: 1298397  
Conc: 22.28 ng/ml

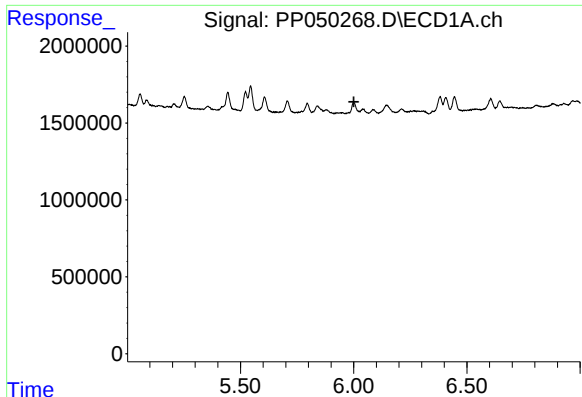

#7 AR-1016-5


R.T.: 0.000 min  
Exp R.T.: 6.001 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_P  
ClientSampleId :  
LOD-MDL-WATER-01-QT3-2022

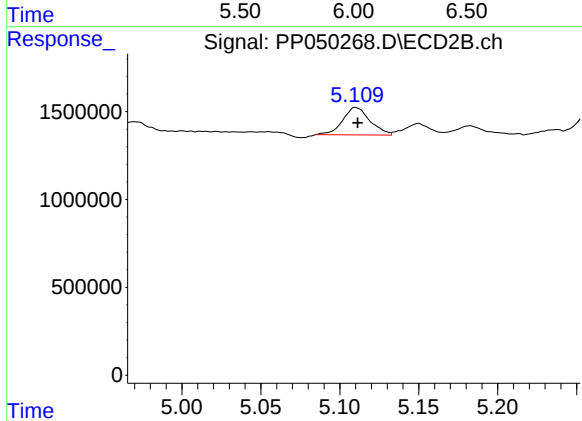


#7 AR-1016-5

R.T.: 5.110 min  
Delta R.T.: -0.001 min  
Response: 1893895  
Conc: 24.79 ng/ml

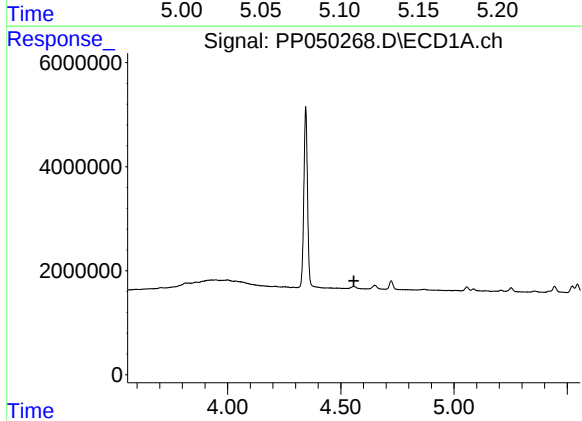


#8 AR-1221-1

R.T.: 0.000 min  
Exp R.T.: 4.558 min  
Response: 0  
Conc: N.D.

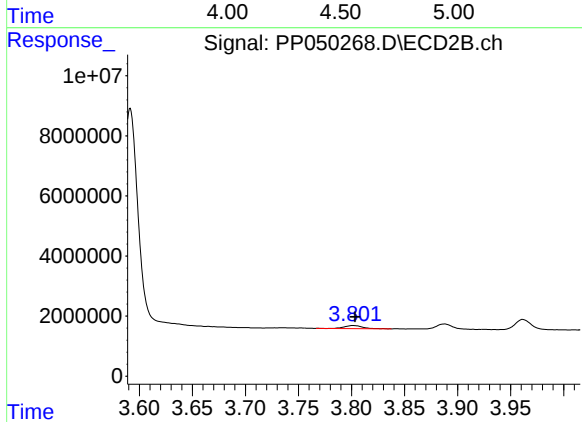

#8 AR-1221-1


R.T.: 3.802 min  
Delta R.T.: -0.002 min  
Response: 1173906  
Conc: 30.71 ng/ml

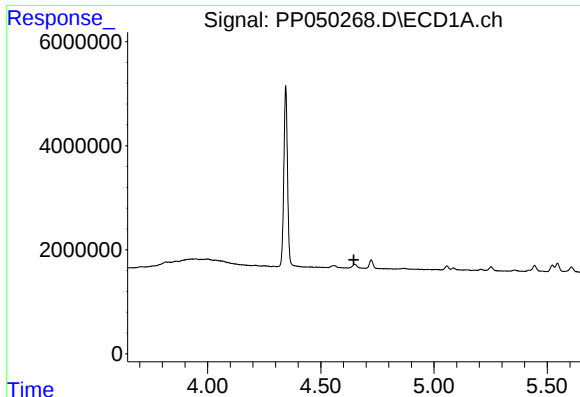

#9 AR-1221-2


R.T.: 0.000 min  
Exp R.T.: 4.646 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_P  
ClientSampleId :  
LOD-MDL-WATER-01-QT3-2022

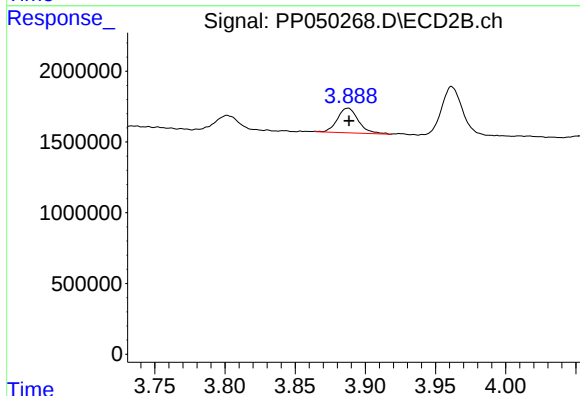


#9 AR-1221-2

R.T.: 3.888 min  
Delta R.T.: 0.000 min  
Response: 1816838  
Conc: 63.62 ng/ml

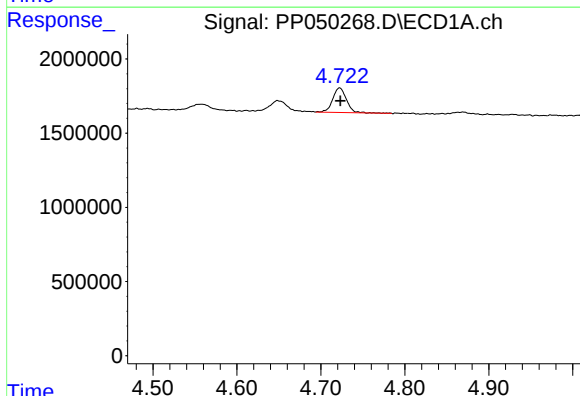


#10 AR-1221-3

R.T.: 4.722 min  
Delta R.T.: 0.000 min  
Response: 1871981  
Conc: 41.61 ng/ml

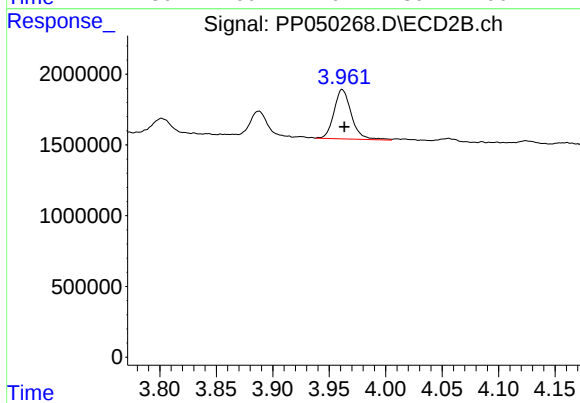

#10 AR-1221-3


R.T.: 3.962 min  
Delta R.T.: -0.002 min  
Response: 3726046  
Conc: 43.52 ng/ml

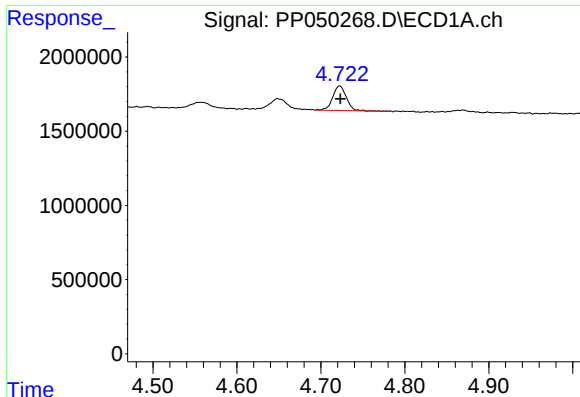

#11 AR-1232-1


R.T.: 4.722 min  
Delta R.T.: -0.001 min  
Response: 1871981  
Conc: 50.08 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
LOD-MDL-WATER-01-QT3-2022

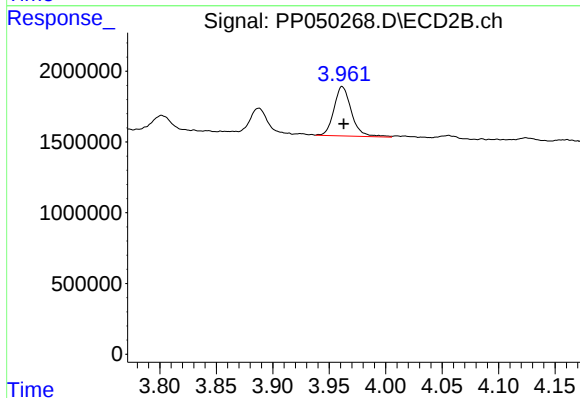


#11 AR-1232-1

R.T.: 3.962 min  
Delta R.T.: -0.001 min  
Response: 3726046  
Conc: 53.37 ng/ml

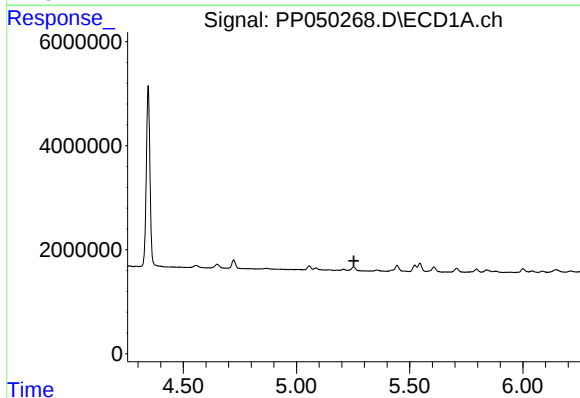


#12 AR-1232-2

R.T.: 0.000 min  
Exp R.T. : 5.254 min  
Response: 0  
Conc: N.D.

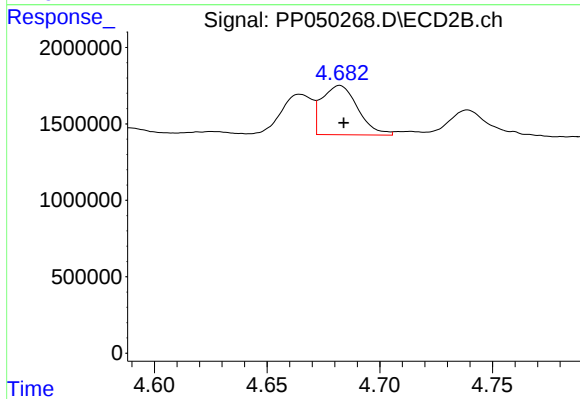

#12 AR-1232-2


R.T.: 4.682 min  
Delta R.T.: -0.002 min  
Response: 3574046  
Conc: 55.59 ng/ml

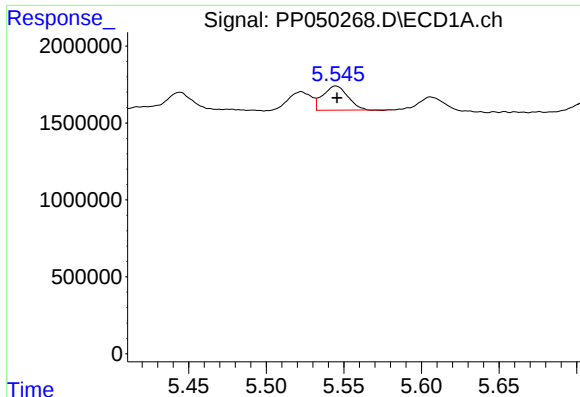

#13 AR-1232-3


R.T.: 5.545 min  
Delta R.T.: 0.000 min  
Response: 1750520  
Conc: 44.46 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
LOD-MDL-WATER-01-QT3-2022

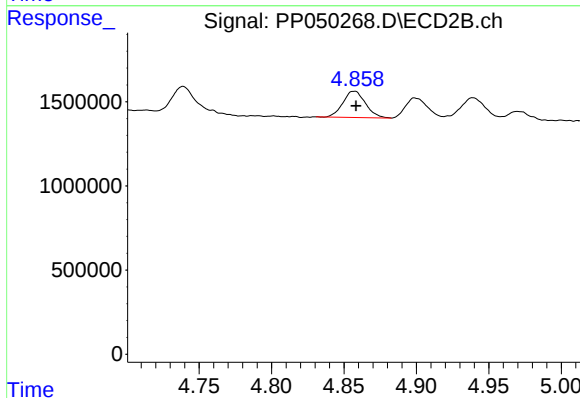


#13 AR-1232-3

R.T.: 4.857 min  
Delta R.T.: -0.001 min  
Response: 1690769  
Conc: 50.41 ng/ml

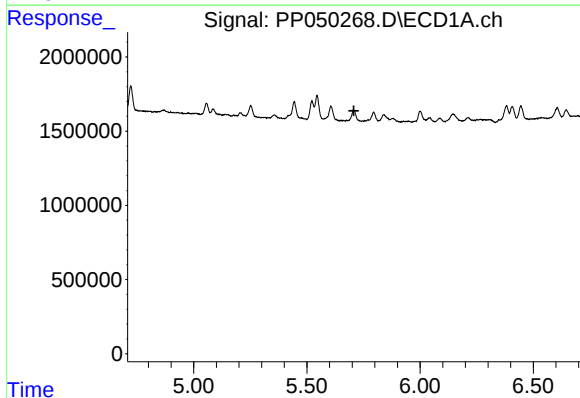


#14 AR-1232-4

R.T.: 0.000 min  
Exp R.T. : 5.708 min  
Response: 0  
Conc: N.D.

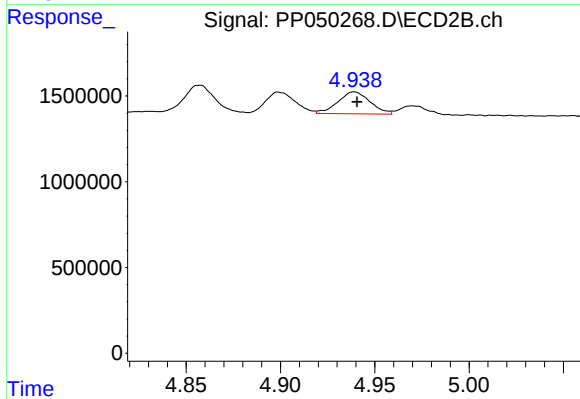

#14 AR-1232-4


R.T.: 4.939 min  
Delta R.T.: -0.001 min  
Response: 1522299  
Conc: 51.67 ng/ml

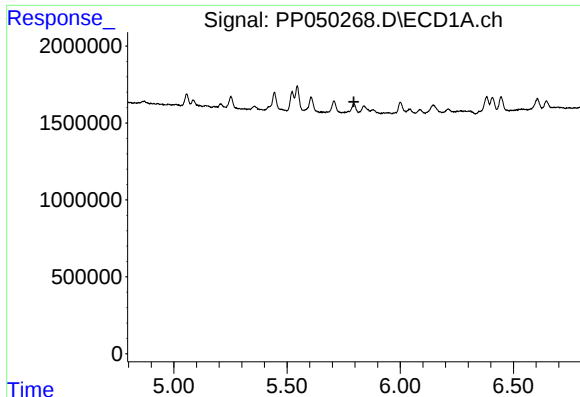

#15 AR-1232-5


R.T.: 0.000 min  
Exp R.T.: 5.795 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_P  
ClientSampleId :  
LOD-MDL-WATER-01-QT3-2022

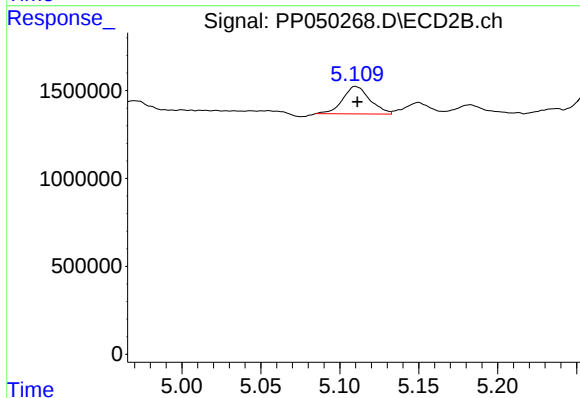


#15 AR-1232-5

R.T.: 5.110 min  
Delta R.T.: -0.001 min  
Response: 1893895  
Conc: 57.51 ng/ml

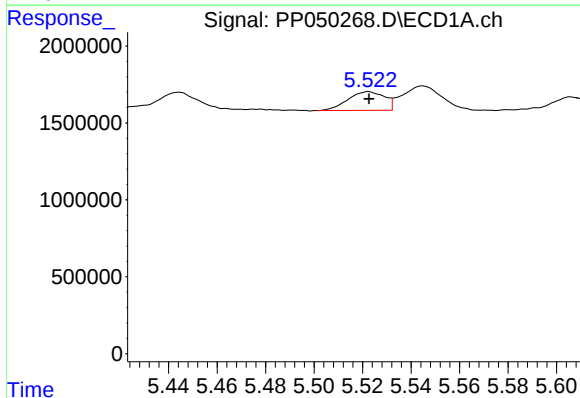


#16 AR-1242-1

R.T.: 5.523 min  
Delta R.T.: 0.000 min  
Response: 1278144  
Conc: 25.22 ng/ml

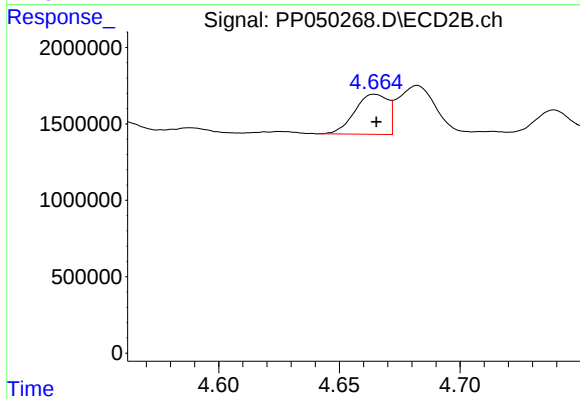

#16 AR-1242-1


R.T.: 4.665 min  
Delta R.T.: 0.000 min  
Response: 2510669  
Conc: 30.29 ng/ml

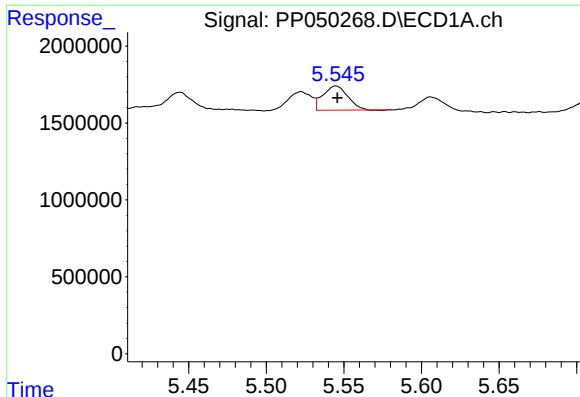

#17 AR-1242-2


R.T.: 5.545 min  
Delta R.T.: 0.000 min  
Response: 1750520  
Conc: 24.23 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
LOD-MDL-WATER-01-QT3-2022

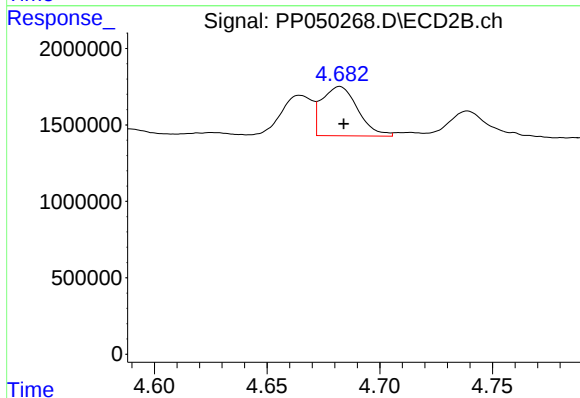


#17 AR-1242-2

R.T.: 4.682 min  
Delta R.T.: -0.002 min  
Response: 3574046  
Conc: 30.61 ng/ml

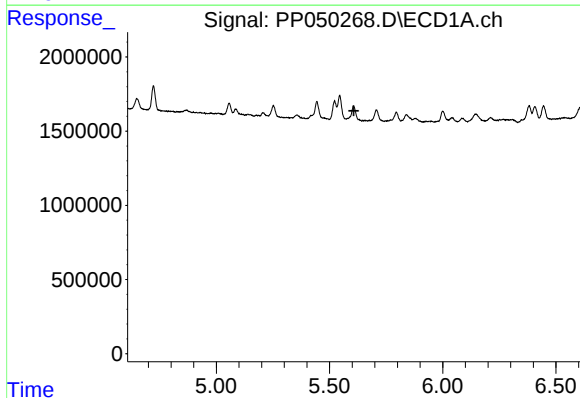


#18 AR-1242-3

R.T.: 0.000 min  
Exp R.T. : 5.607 min  
Response: 0  
Conc: N.D.

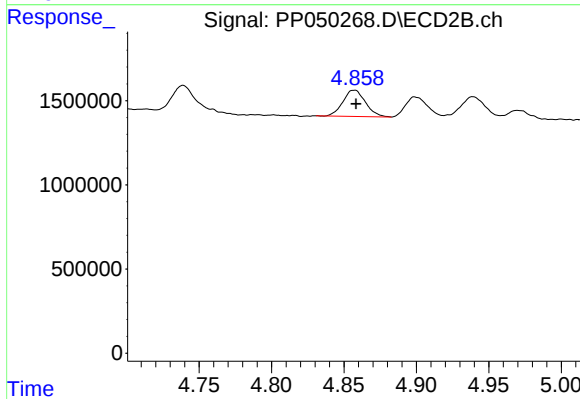

#18 AR-1242-3


R.T.: 4.857 min  
Delta R.T.: -0.001 min  
Response: 1690769  
Conc: 27.57 ng/ml

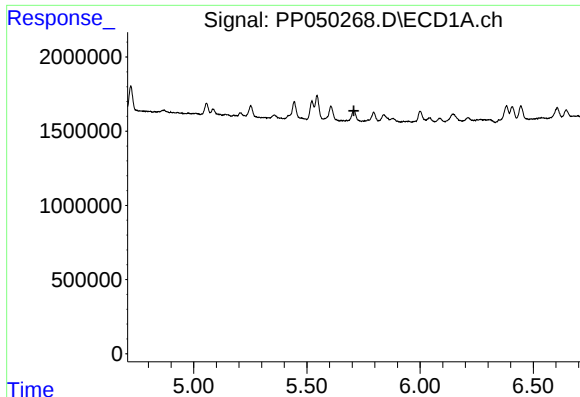

#19 AR-1242-4


R.T.: 0.000 min  
Exp R.T.: 5.708 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_P  
ClientSampleId :  
LOD-MDL-WATER-01-QT3-2022

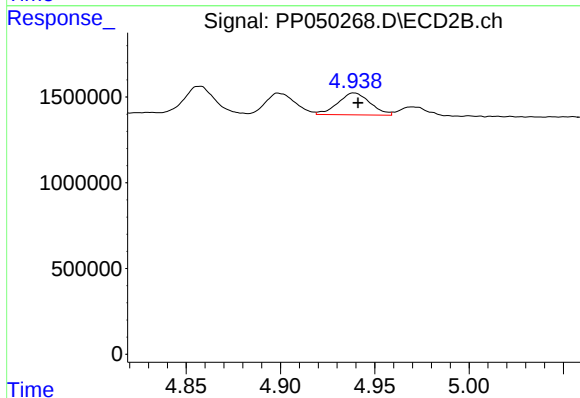


#19 AR-1242-4

R.T.: 4.939 min  
Delta R.T.: -0.002 min  
Response: 1522299  
Conc: 26.00 ng/ml

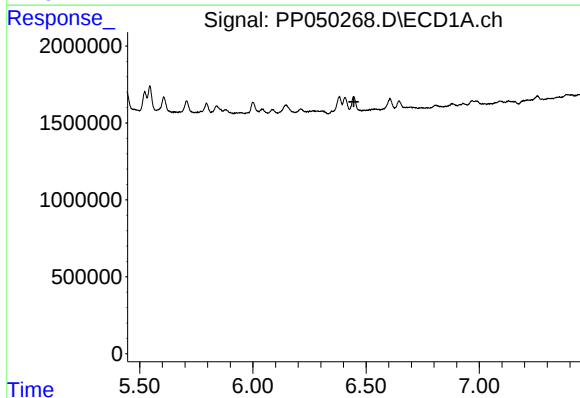


#20 AR-1242-5

R.T.: 0.000 min  
Exp R.T.: 6.446 min  
Response: 0  
Conc: N.D.

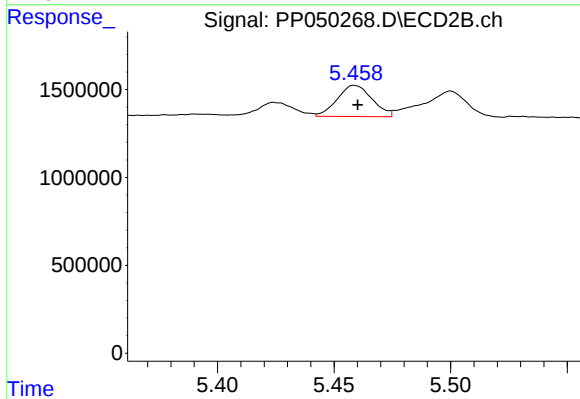

#20 AR-1242-5


R.T.: 5.459 min  
Delta R.T.: -0.001 min  
Response: 1845650  
Conc: 26.55 ng/ml

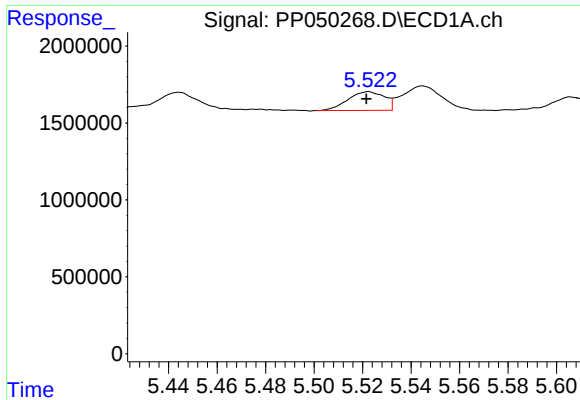

#21 AR-1248-1


R.T.: 5.523 min  
Delta R.T.: 0.000 min  
Response: 1278144  
Conc: 31.66 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
LOD-MDL-WATER-01-QT3-2022

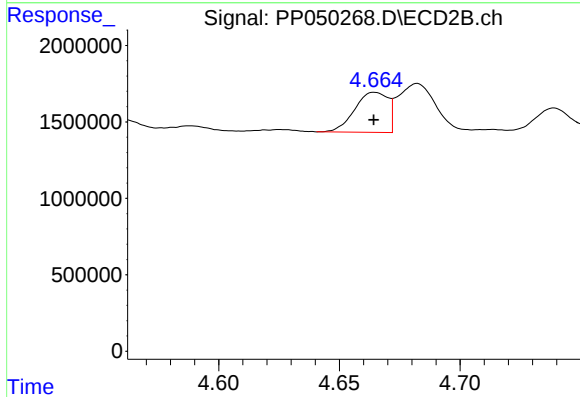


#21 AR-1248-1

R.T.: 4.665 min  
Delta R.T.: 0.000 min  
Response: 2510669  
Conc: 37.57 ng/ml

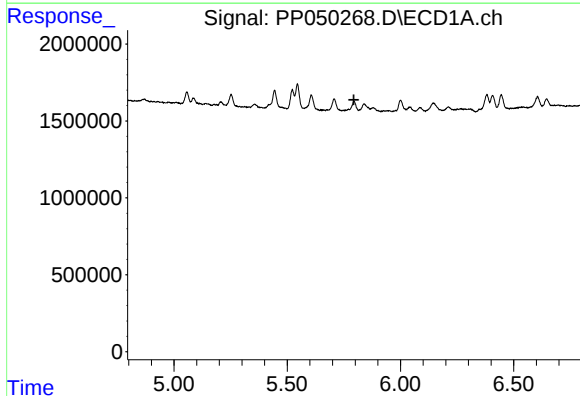


#22 AR-1248-2

R.T.: 0.000 min  
Exp R.T. : 5.794 min  
Response: 0  
Conc: N.D.

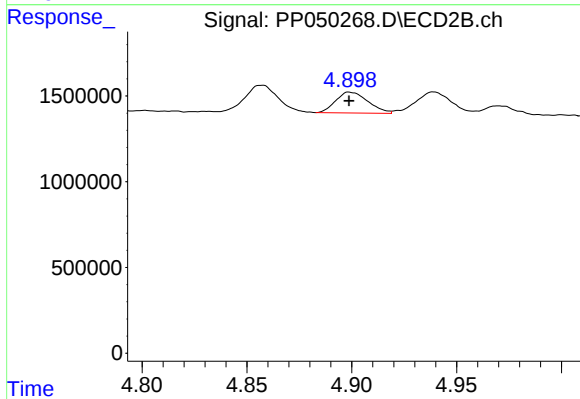

#22 AR-1248-2


R.T.: 4.899 min  
Delta R.T.: 0.000 min  
Response: 1298397  
Conc: 15.03 ng/ml

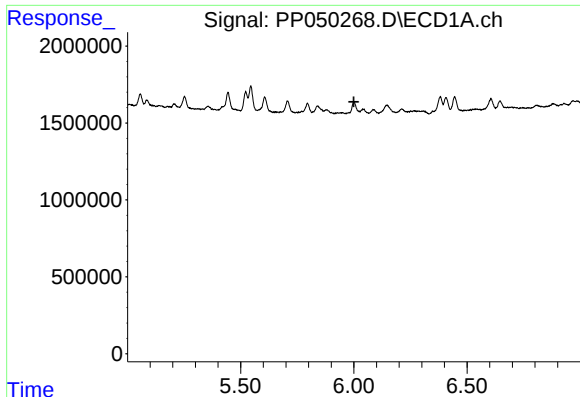

#23 AR-1248-3


R.T.: 0.000 min  
Exp R.T.: 6.000 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_P  
ClientSampleId :  
LOD-MDL-WATER-01-QT3-2022

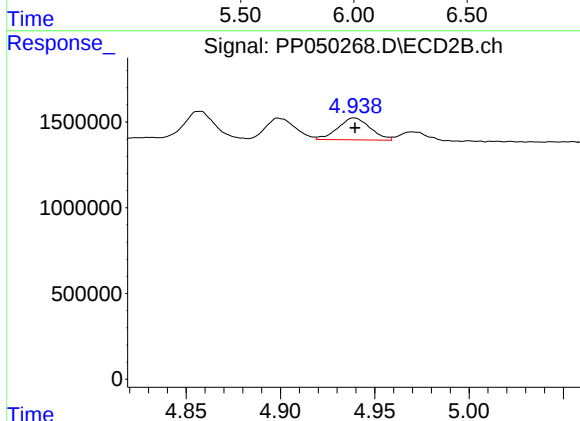


#23 AR-1248-3

R.T.: 4.939 min  
Delta R.T.: 0.000 min  
Response: 1522299  
Conc: 16.79 ng/ml

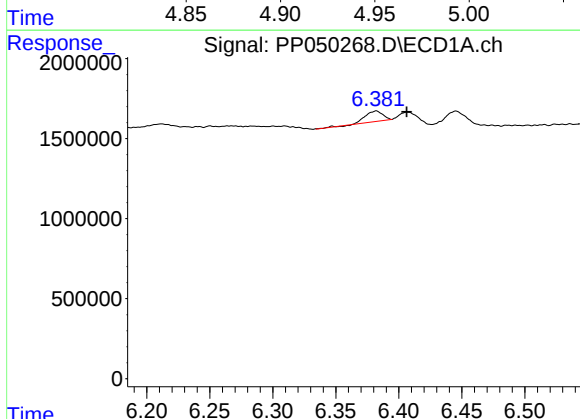


#24 AR-1248-4

R.T.: 6.382 min  
Delta R.T.: -0.025 min  
Response: 621538  
Conc: 7.86 ng/ml

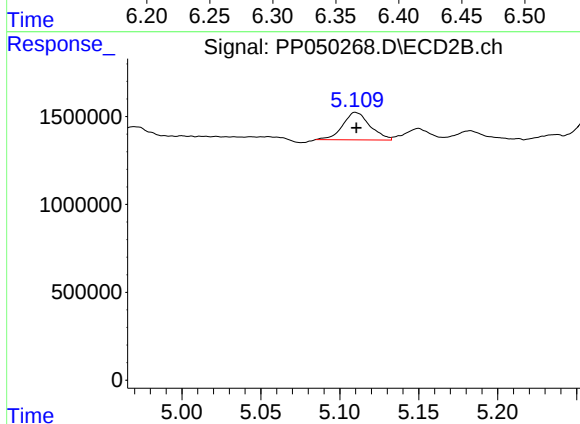

#24 AR-1248-4


R.T.: 5.110 min  
Delta R.T.: 0.000 min  
Response: 1893895  
Conc: 17.97 ng/ml

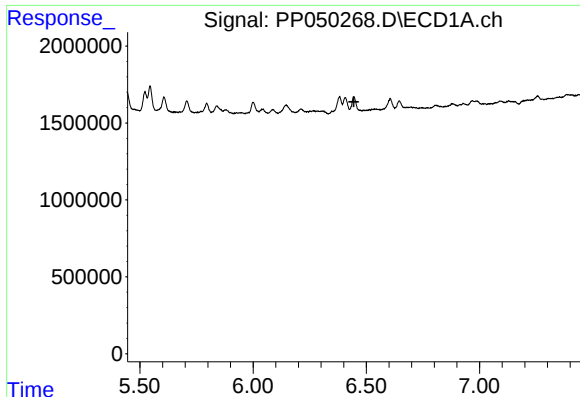

#25 AR-1248-5


R.T.: 0.000 min  
Exp R.T.: 6.445 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_P  
ClientSampleId :  
LOD-MDL-WATER-01-QT3-2022

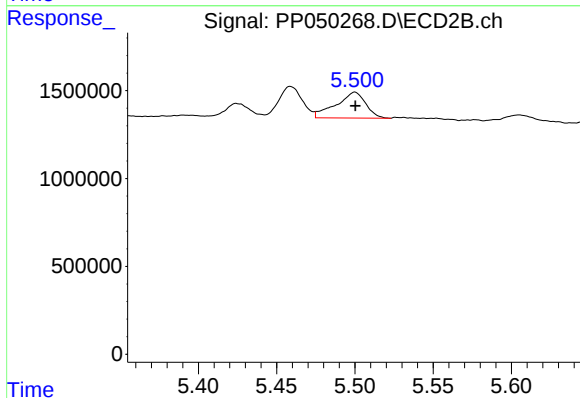


#25 AR-1248-5

R.T.: 5.500 min  
Delta R.T.: 0.000 min  
Response: 1940971  
Conc: 19.55 ng/ml

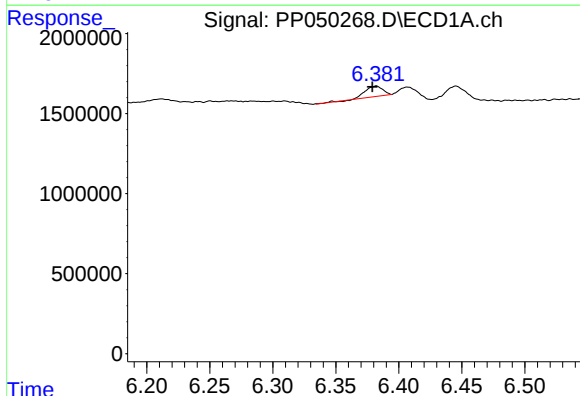


#26 AR-1254-1

R.T.: 6.382 min  
Delta R.T.: 0.003 min  
Response: 621538  
Conc: 8.97 ng/ml

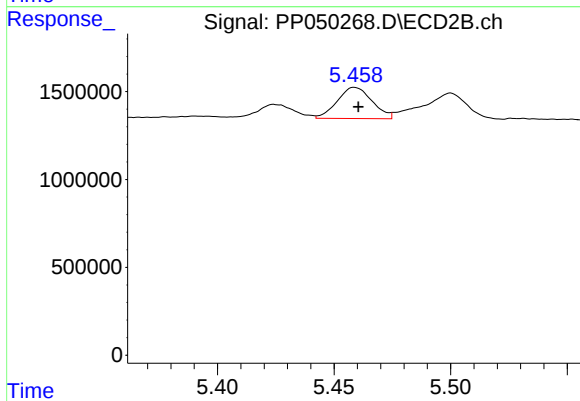

#26 AR-1254-1


R.T.: 5.459 min  
Delta R.T.: -0.002 min  
Response: 1845650  
Conc: 13.97 ng/ml

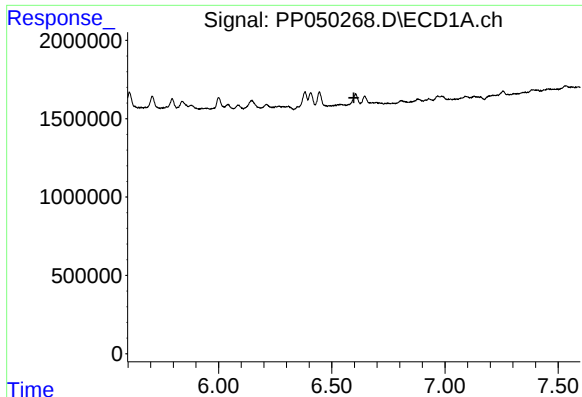

#27 AR-1254-2


R.T.: 0.000 min  
Exp R.T.: 6.598 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_P  
ClientSampleId :  
LOD-MDL-WATER-01-QT3-2022

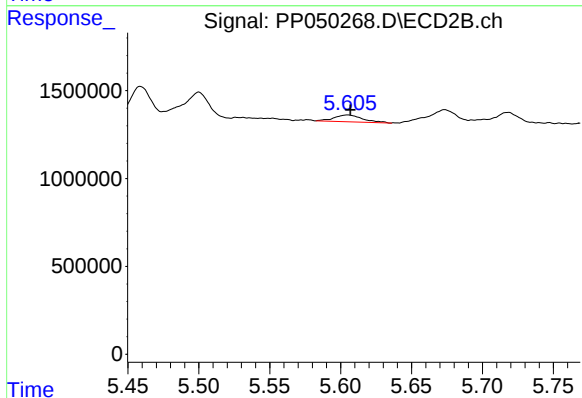


#27 AR-1254-2

R.T.: 5.605 min  
Delta R.T.: -0.002 min  
Response: 539255  
Conc: 4.95 ng/ml

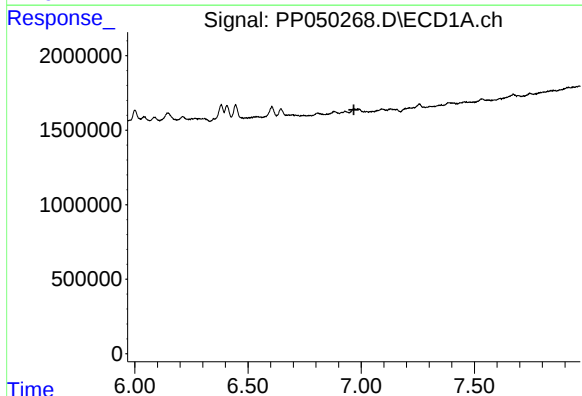


#28 AR-1254-3

R.T.: 0.000 min  
Exp R.T.: 6.967 min  
Response: 0  
Conc: N.D.

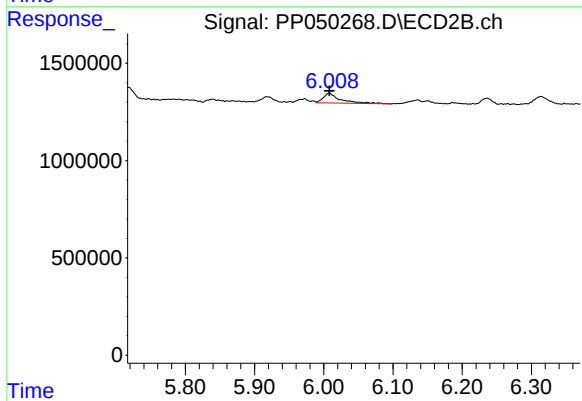

#28 AR-1254-3


R.T.: 6.008 min  
Delta R.T.: 0.000 min  
Response: 870507  
Conc: 5.47 ng/ml

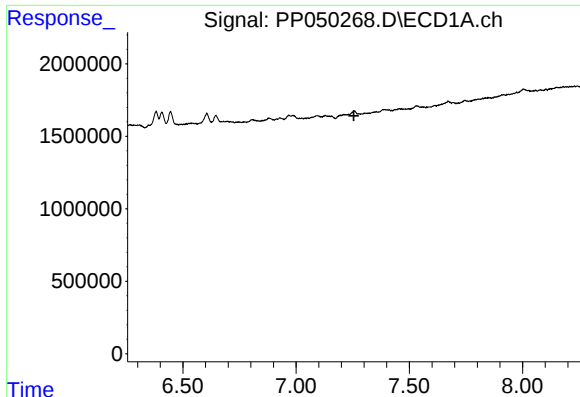

#29 AR-1254-4


R.T.: 0.000 min  
Exp R.T.: 7.255 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_P  
ClientSampleId :  
LOD-MDL-WATER-01-QT3-2022

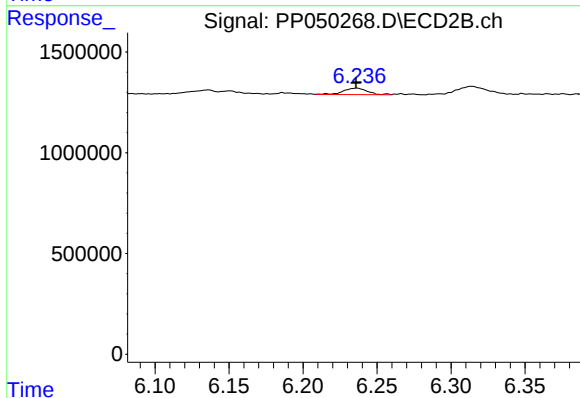


#29 AR-1254-4

R.T.: 6.236 min  
Delta R.T.: 0.000 min  
Response: 367333  
Conc: 3.78 ng/ml

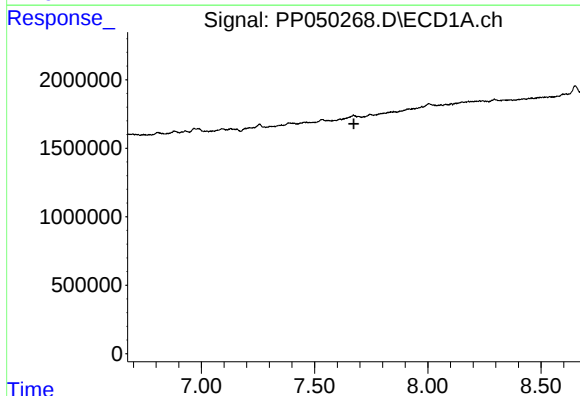


#30 AR-1254-5

R.T.: 0.000 min  
Exp R.T.: 7.674 min  
Response: 0  
Conc: N.D.

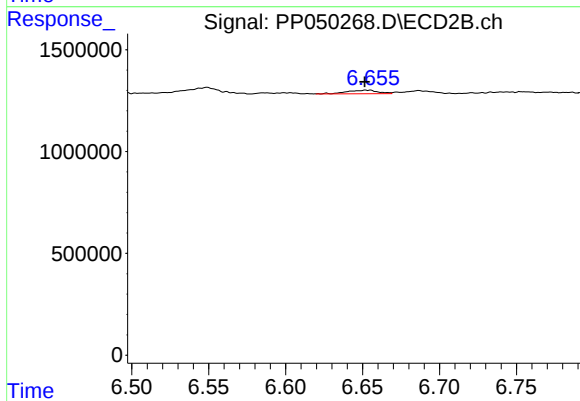

#30 AR-1254-5


R.T.: 6.653 min  
Delta R.T.: 0.002 min  
Response: 248532  
Conc: 2.02 ng/ml

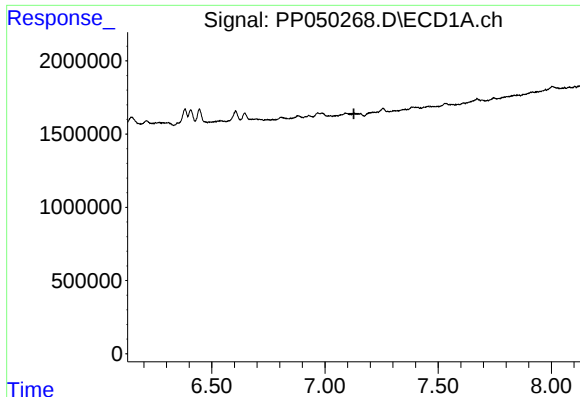

#31 AR-1260-1


R.T.: 0.000 min  
Exp R.T.: 7.128 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_P  
ClientSampleId :  
LOD-MDL-WATER-01-QT3-2022

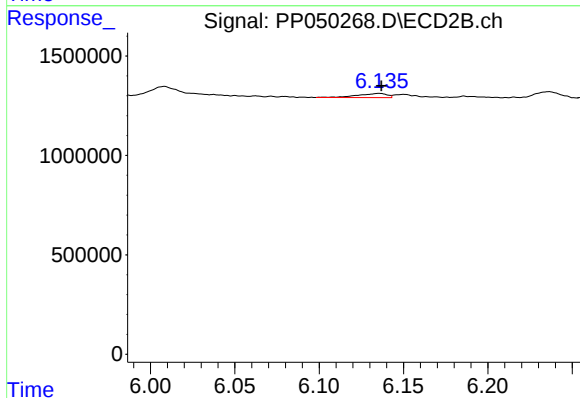


#31 AR-1260-1

R.T.: 6.136 min  
Delta R.T.: -0.001 min  
Response: 256117  
Conc: 2.26 ng/ml

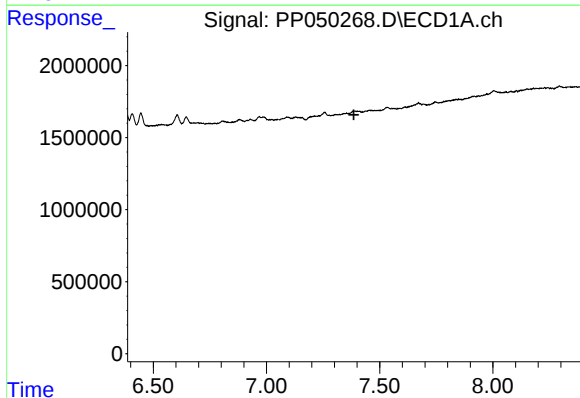


#32 AR-1260-2

R.T.: 0.000 min  
Exp R.T.: 7.386 min  
Response: 0  
Conc: N.D.

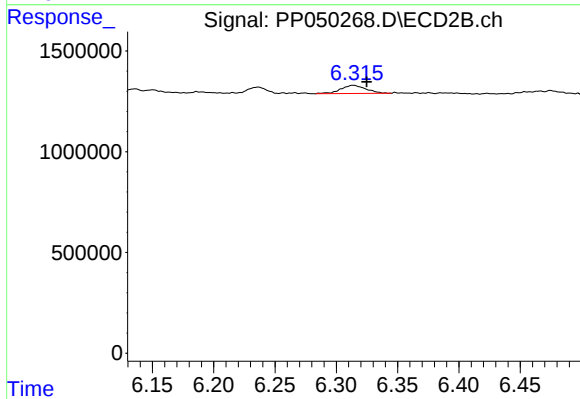

#32 AR-1260-2


R.T.: 6.314 min  
Delta R.T.: -0.011 min  
Response: 587200  
Conc: 4.37 ng/ml

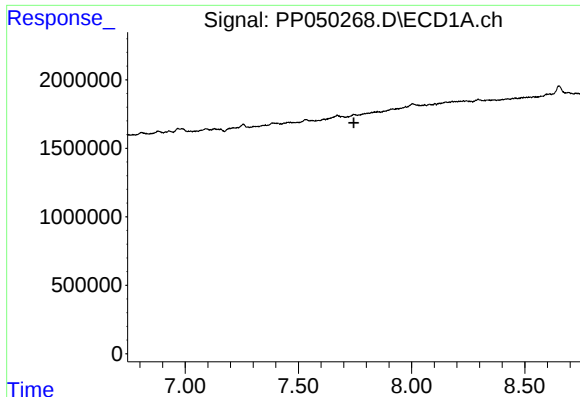

#33 AR-1260-3


R.T.: 0.000 min  
Exp R.T.: 7.745 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_P  
ClientSampleId :  
LOD-MDL-WATER-01-QT3-2022

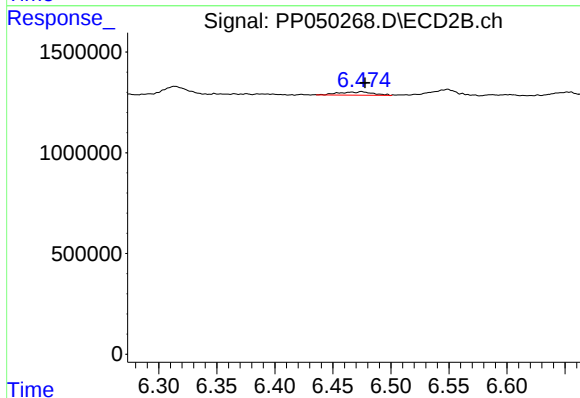


#33 AR-1260-3

R.T.: 6.475 min  
Delta R.T.: -0.003 min  
Response: 338455  
Conc: 2.81 ng/ml

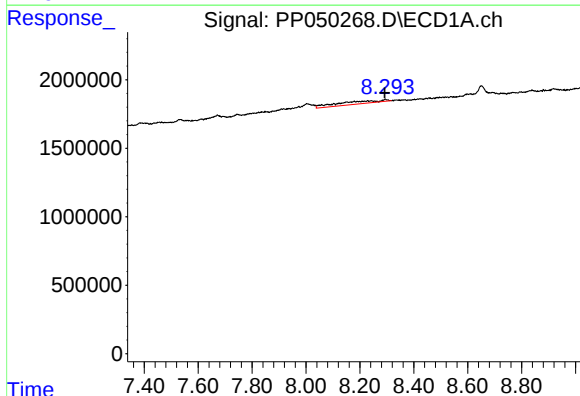


#35 AR-1260-5

R.T.: 8.294 min  
Delta R.T.: 0.002 min  
Response: 2463719  
Conc: 13.18 ng/ml

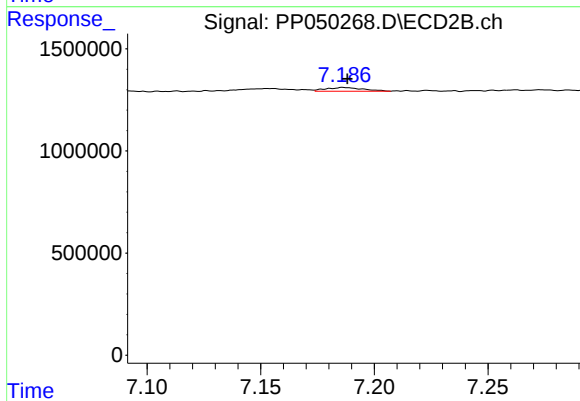

#35 AR-1260-5


R.T.: 7.187 min  
Delta R.T.: -0.002 min  
Response: 206770  
Conc: 1.06 ng/ml

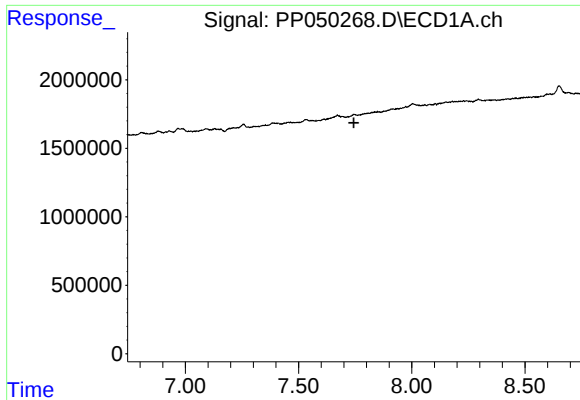

#36 AR-1262-1


R.T.: 0.000 min  
Exp R.T.: 7.744 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_P  
ClientSampleId :  
LOD-MDL-WATER-01-QT3-2022

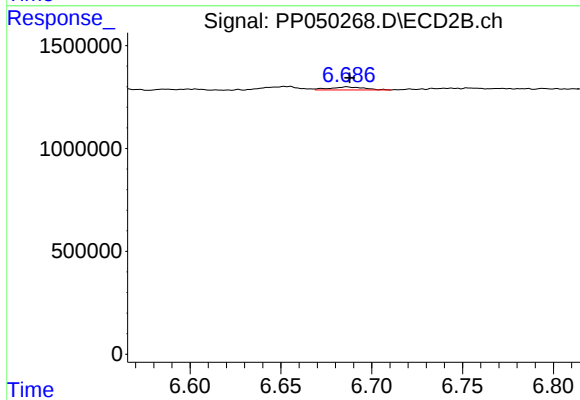


#36 AR-1262-1

R.T.: 6.686 min  
Delta R.T.: -0.001 min  
Response: 195700  
Conc: 1.45 ng/ml

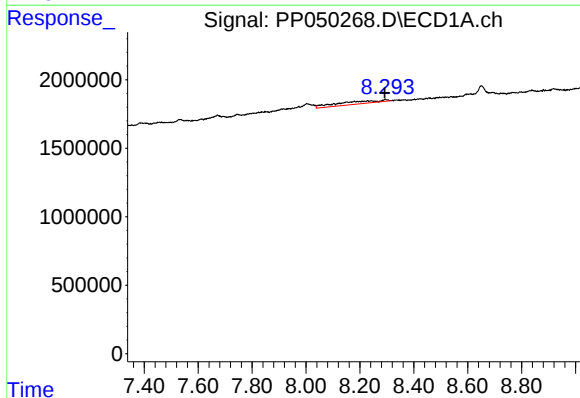


#37 AR-1262-2

R.T.: 8.294 min  
Delta R.T.: 0.003 min  
Response: 2463719  
Conc: 11.40 ng/ml

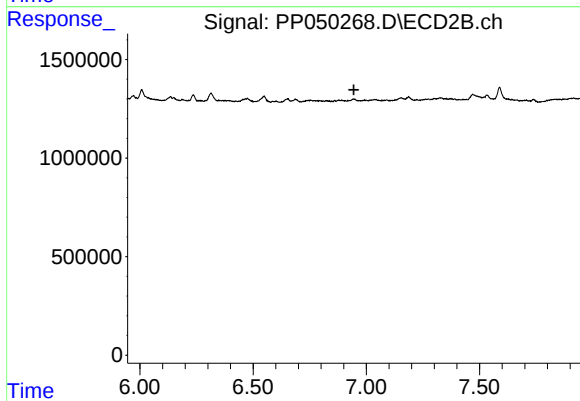

#37 AR-1262-2


R.T.: 0.000 min  
Exp R.T.: 6.945 min  
Response: 0  
Conc: N.D.

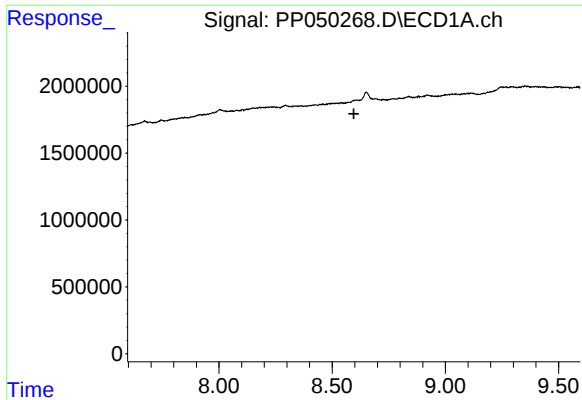

#38 AR-1262-3


R.T.: 0.000 min  
Exp R.T.: 8.596 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_P  
ClientSampleId :  
LOD-MDL-WATER-01-QT3-2022

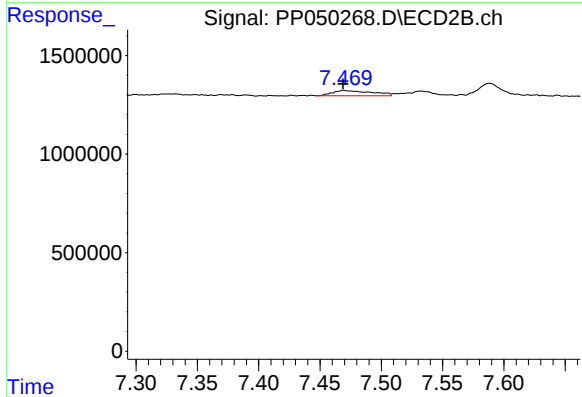


#38 AR-1262-3

R.T.: 7.469 min  
Delta R.T.: 0.000 min  
Response: 596137  
Conc: 8.21 ng/ml

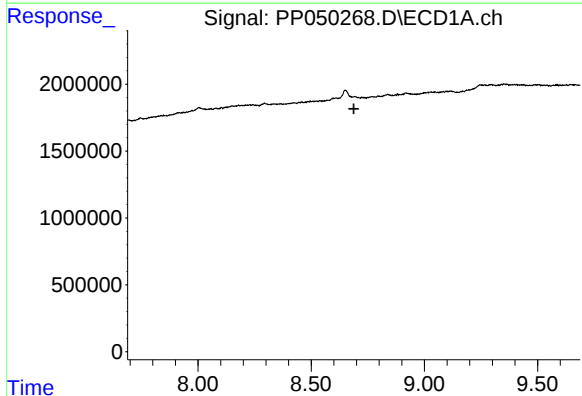


#39 AR-1262-4

R.T.: 0.000 min  
Exp R.T.: 8.688 min  
Response: 0  
Conc: N.D.

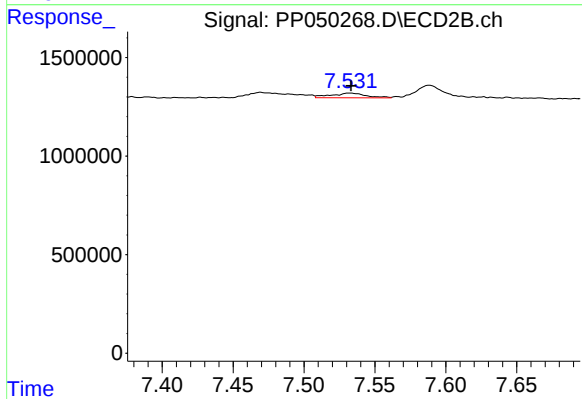

#39 AR-1262-4


R.T.: 7.532 min  
Delta R.T.: -0.001 min  
Response: 410752  
Conc: 2.98 ng/ml

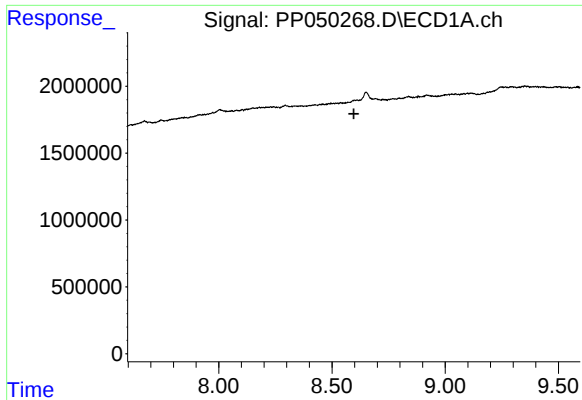

#41 AR-1268-1


R.T.: 0.000 min  
Exp R.T.: 8.597 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_P  
ClientSampleId :  
LOD-MDL-WATER-01-QT3-2022

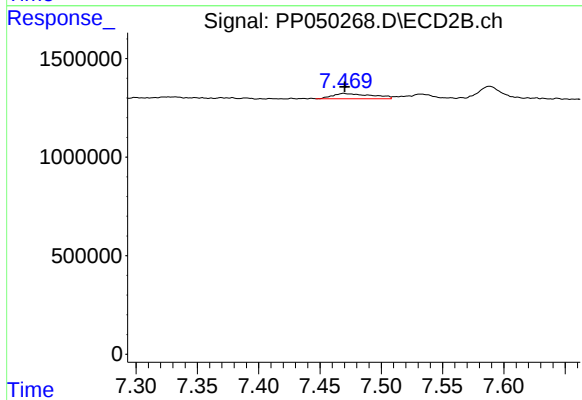


#41 AR-1268-1

R.T.: 7.469 min  
Delta R.T.: 0.000 min  
Response: 596137  
Conc: 2.71 ng/ml

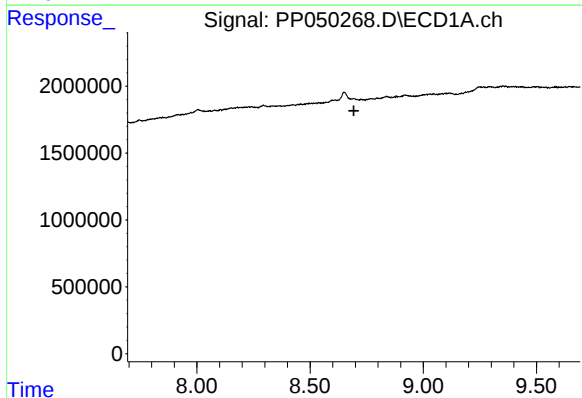


#42 AR-1268-2

R.T.: 0.000 min  
Exp R.T.: 8.694 min  
Response: 0  
Conc: N.D.

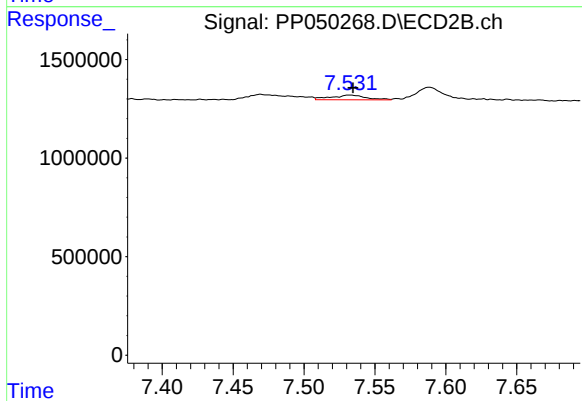

#42 AR-1268-2


R.T.: 7.532 min  
Delta R.T.: -0.003 min  
Response: 410752  
Conc: 2.06 ng/ml

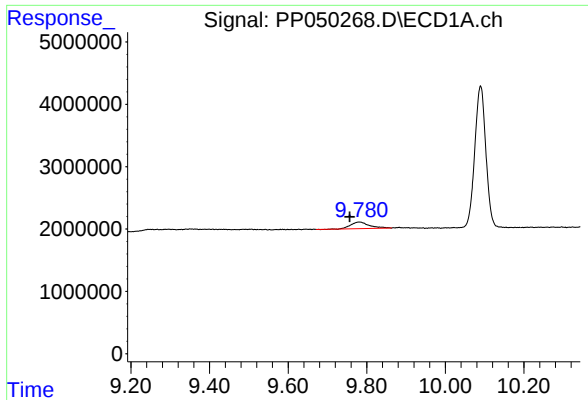

#45 AR-1268-5

R.T.: 9.781 min  
Delta R.T.: 0.024 min  
Response: 3425272  
Conc: 5.14 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
LOD-MDL-WATER-01-QT3-2022

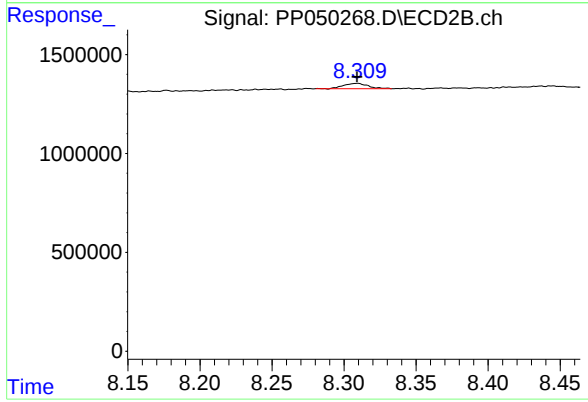

#45 AR-1268-5

R.T.: 8.309 min  
Delta R.T.: 0.000 min  
Response: 318800  
Conc: 0.58 ng/ml