

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080622\
 Data File : PP050269.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2022 19:03
 Operator : YP\AJ
 Sample : N3980-07
 Misc : AR1242 LOD 40 PPB
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 00:35:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Aug 07 23:52:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.345	3.591	40485728	82073304	25.152	26.203
2)	SA Decachlor...	10.090	8.554	46599108	39726084	26.463	25.811
Target Compounds							
16)	L4 AR-1242-1	5.522	4.664	2469174	4766860	48.719	57.501
17)	L4 AR-1242-2	5.544	4.682	3462154	6486463	47.926	55.544
18)	L4 AR-1242-3	5.606	4.857	1988288	3363325	44.960	54.848
19)	L4 AR-1242-4	5.707	4.939	1863092	3308102	49.997	56.511
20)	L4 AR-1242-5	6.446	5.459	2065277	3664699	48.939	52.722



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080622\
Data File : PP050269.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2022 19:03
Operator : YP\AJ
Sample : N3980-07
Misc : AR1242 LOD 40 PPB
ALS Vial : 65 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 00:35:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Aug 07 23:52:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

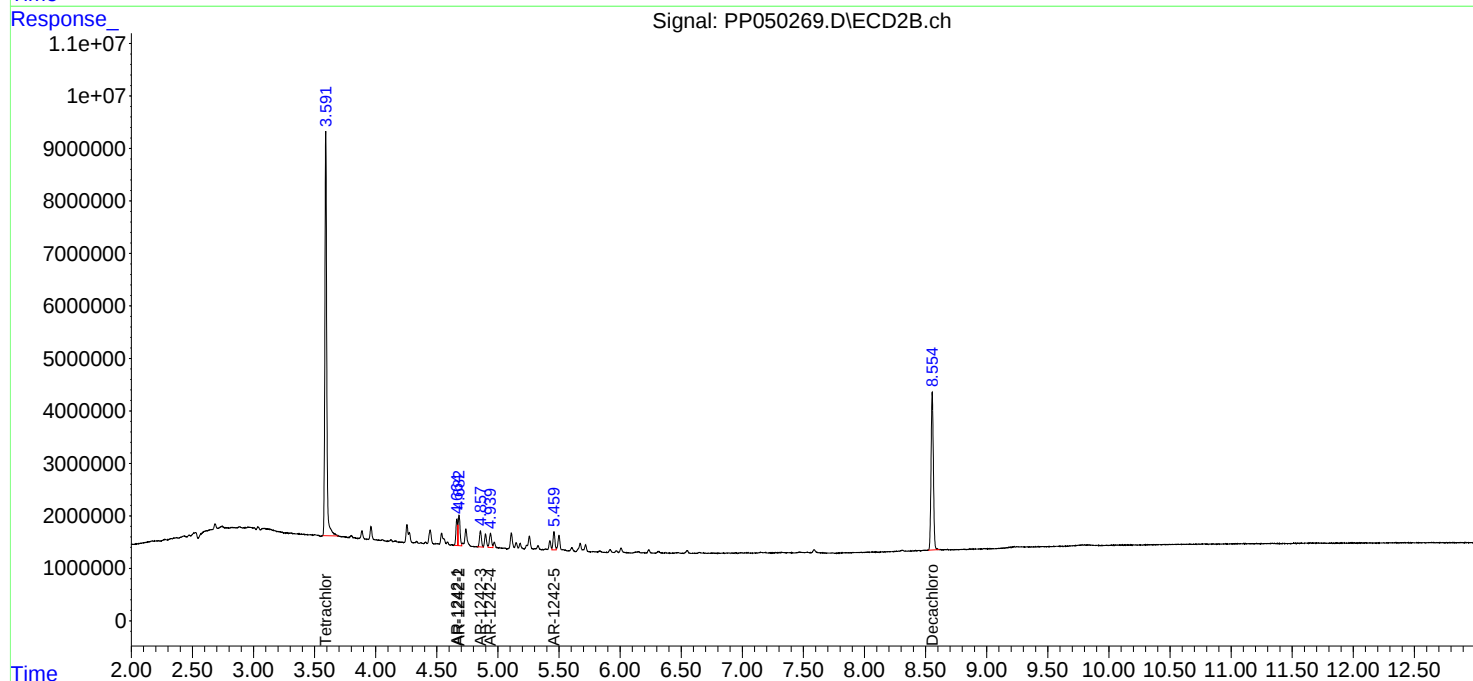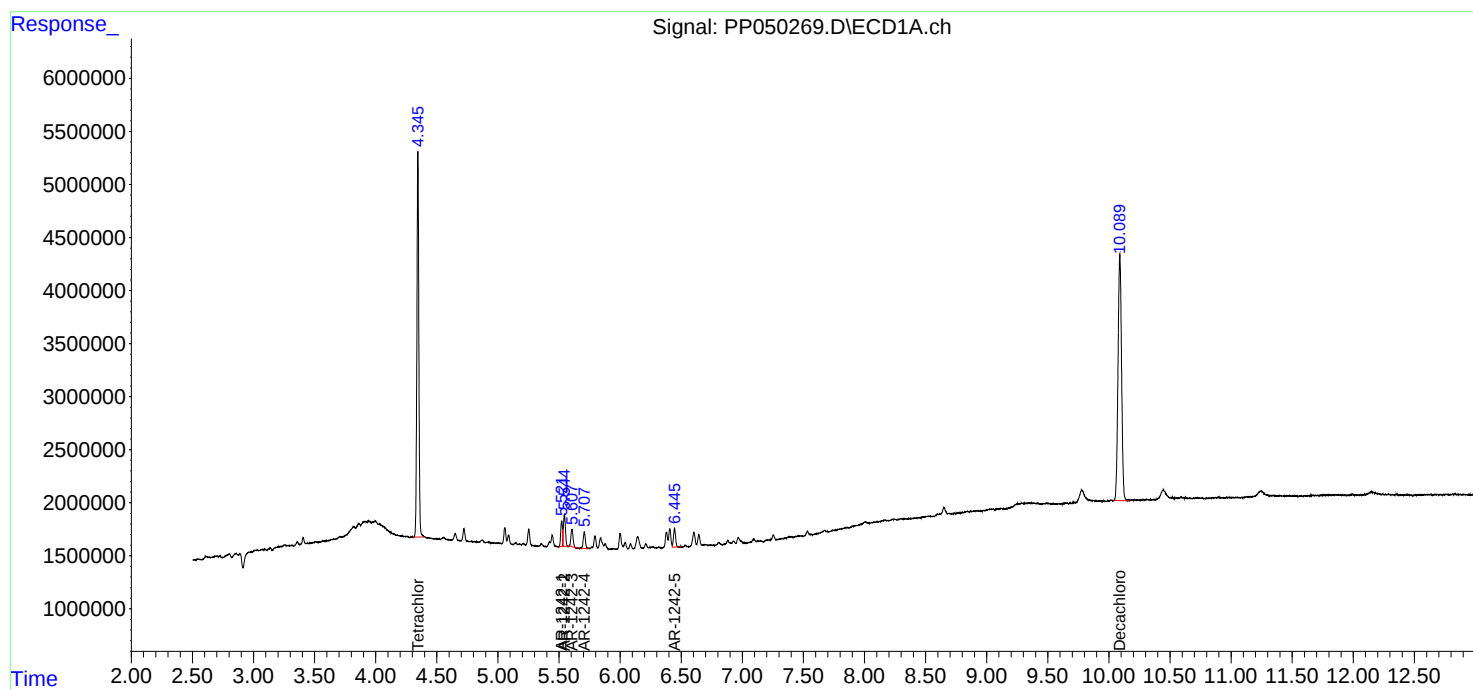


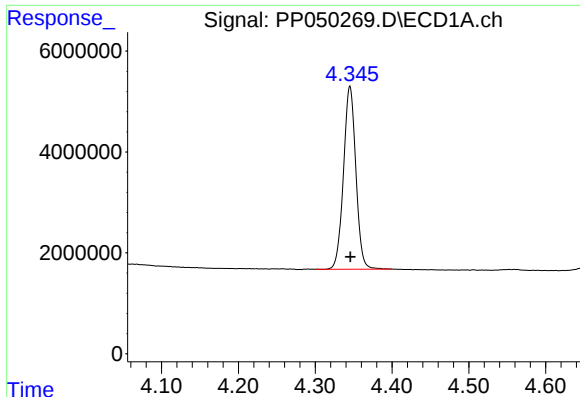

#1 Tetrachloro-m-xylene


R.T.: 4.345 min
Delta R.T.: 0.000 min
Response: 40485728
Conc: 25.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

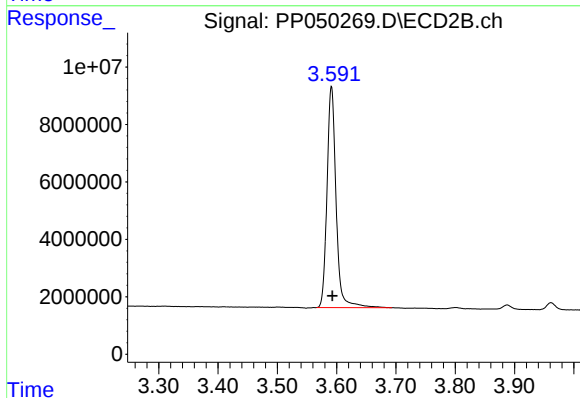


#1 Tetrachloro-m-xylene

R.T.: 3.591 min
Delta R.T.: -0.001 min
Response: 82073304
Conc: 26.20 ng/ml

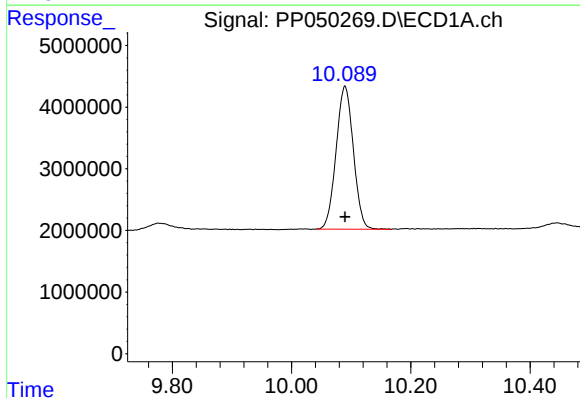


#2 Decachlorobiphenyl

R.T.: 10.090 min
Delta R.T.: 0.000 min
Response: 46599108
Conc: 26.46 ng/ml

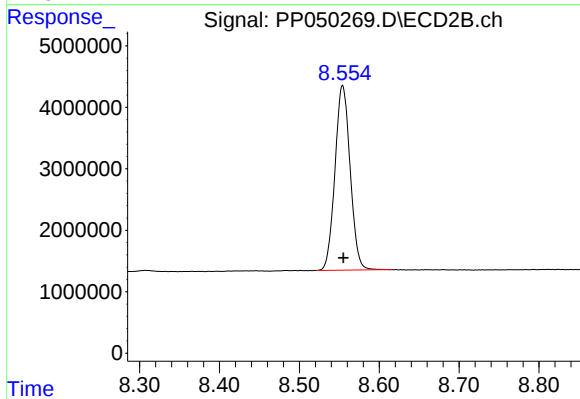

#2 Decachlorobiphenyl


R.T.: 8.554 min
Delta R.T.: -0.001 min
Response: 39726084
Conc: 25.81 ng/ml

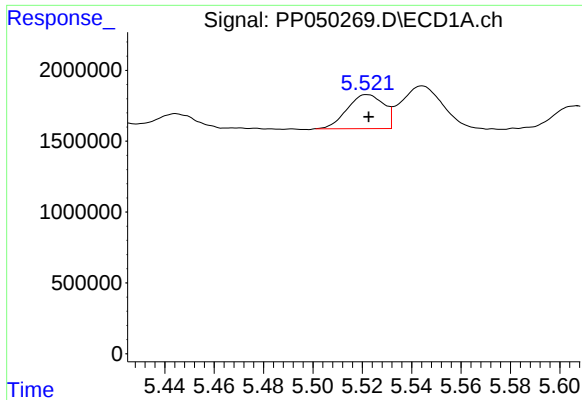

#16 AR-1242-1


R.T.: 5.522 min
Delta R.T.: 0.000 min
Response: 2469174
Conc: 48.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

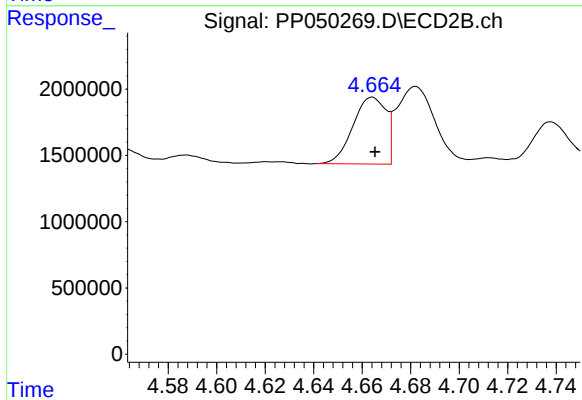


#16 AR-1242-1

R.T.: 4.664 min
Delta R.T.: -0.001 min
Response: 4766860
Conc: 57.50 ng/ml

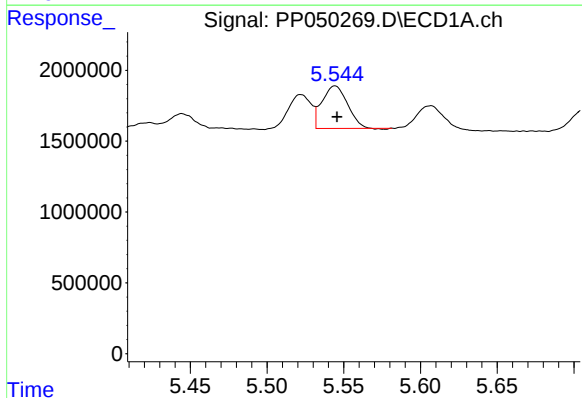


#17 AR-1242-2

R.T.: 5.544 min
Delta R.T.: -0.001 min
Response: 3462154
Conc: 47.93 ng/ml

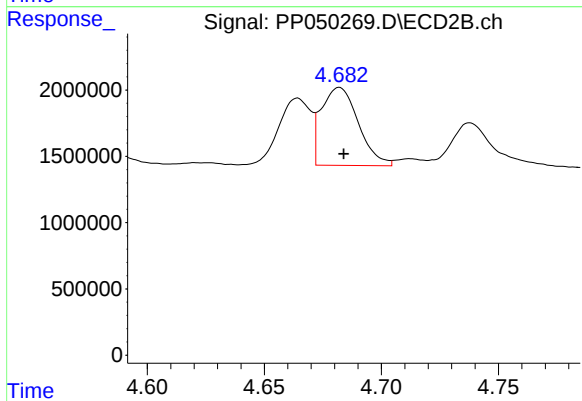

#17 AR-1242-2


R.T.: 4.682 min
Delta R.T.: -0.002 min
Response: 6486463
Conc: 55.54 ng/ml

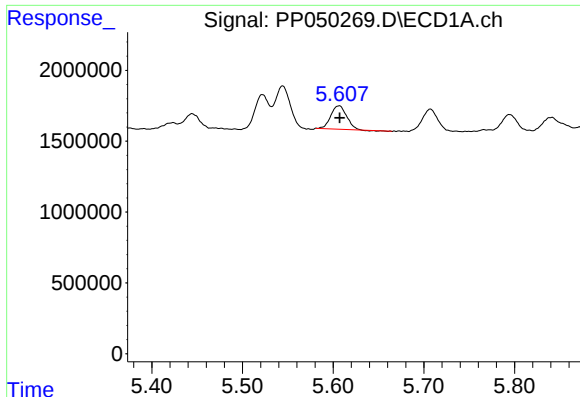

#18 AR-1242-3


R.T.: 5.606 min
Delta R.T.: -0.001 min
Response: 1988288
Conc: 44.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

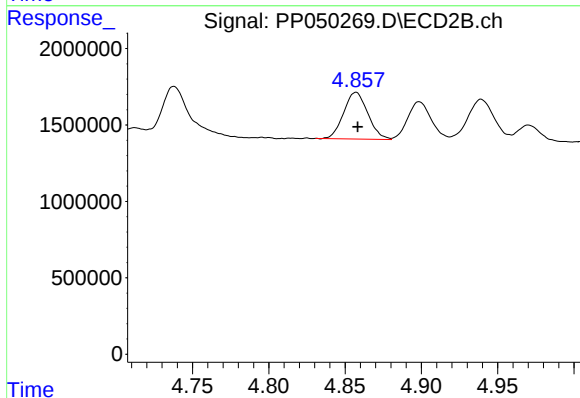


#18 AR-1242-3

R.T.: 4.857 min
Delta R.T.: 0.000 min
Response: 3363325
Conc: 54.85 ng/ml

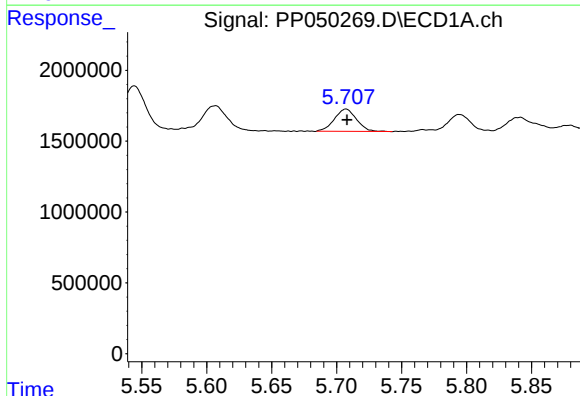


#19 AR-1242-4

R.T.: 5.707 min
Delta R.T.: 0.000 min
Response: 1863092
Conc: 50.00 ng/ml

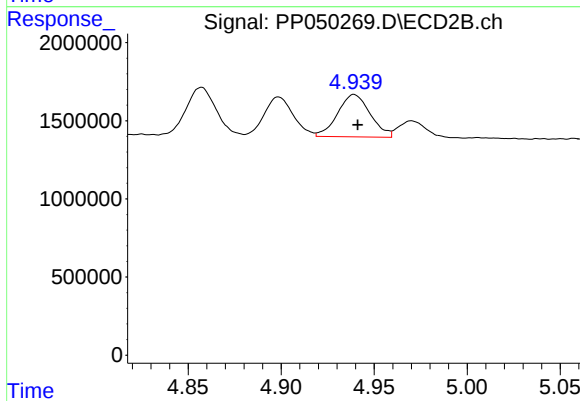

#19 AR-1242-4


R.T.: 4.939 min
Delta R.T.: -0.002 min
Response: 3308102
Conc: 56.51 ng/ml

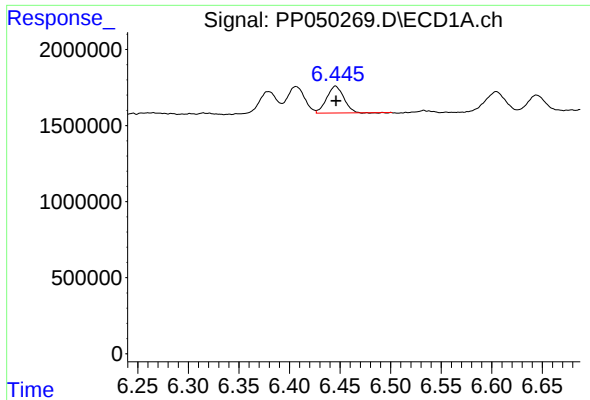

#20 AR-1242-5

R.T.: 6.446 min
Delta R.T.: 0.000 min
Response: 2065277
Conc: 48.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

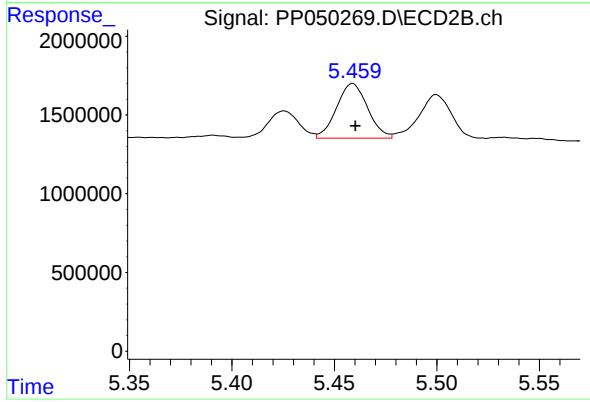

#20 AR-1242-5

R.T.: 5.459 min
Delta R.T.: -0.001 min
Response: 3664699
Conc: 52.72 ng/ml