

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080622\
 Data File : PP050270.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2022 19:20
 Operator : YP\AJ
 Sample : N3980-07
 Misc : AR1248 LOD 40 PPB
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 00:36:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Aug 07 23:52:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.345	3.591	43299777	88048160	26.900	28.110
2)	SA Decachlor...	10.087	8.554	49860428	42981462	28.315	27.927
Target Compounds							
21)	L5 AR-1248-1	5.521	4.664	2056562	4000525	50.934	59.857
22)	L5 AR-1248-2	5.794	4.898	2899757	5336625	51.905	61.778
23)	L5 AR-1248-3	6.000	4.939	3424769	5291904	53.537	58.374
24)	L5 AR-1248-4	6.407	5.110	4364644	6169142	55.177	58.531
25)	L5 AR-1248-5	6.445	5.500	4067186	5956152	53.576	59.988



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080622\
Data File : PP050270.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2022 19:20
Operator : YP\AJ
Sample : N3980-07
Misc : AR1248 LOD 40 PPB
ALS Vial : 66 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 00:36:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Aug 07 23:52:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

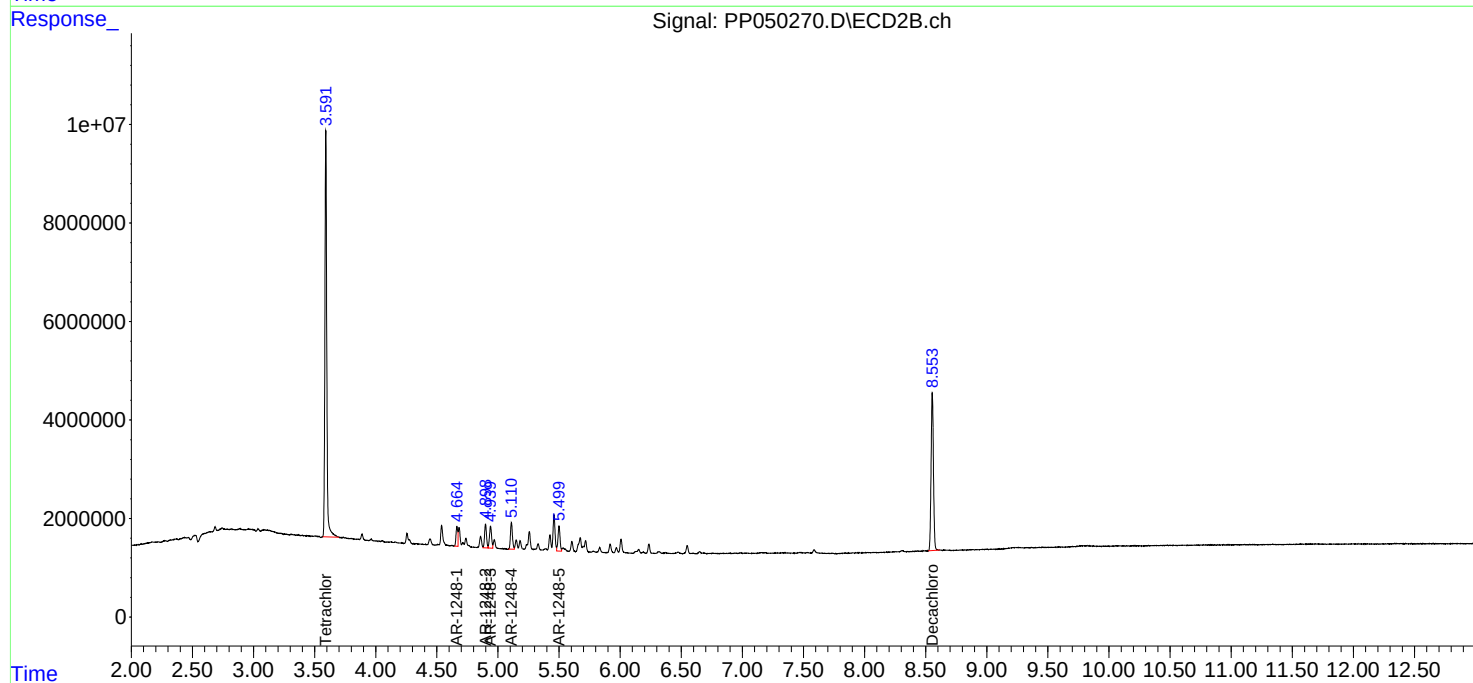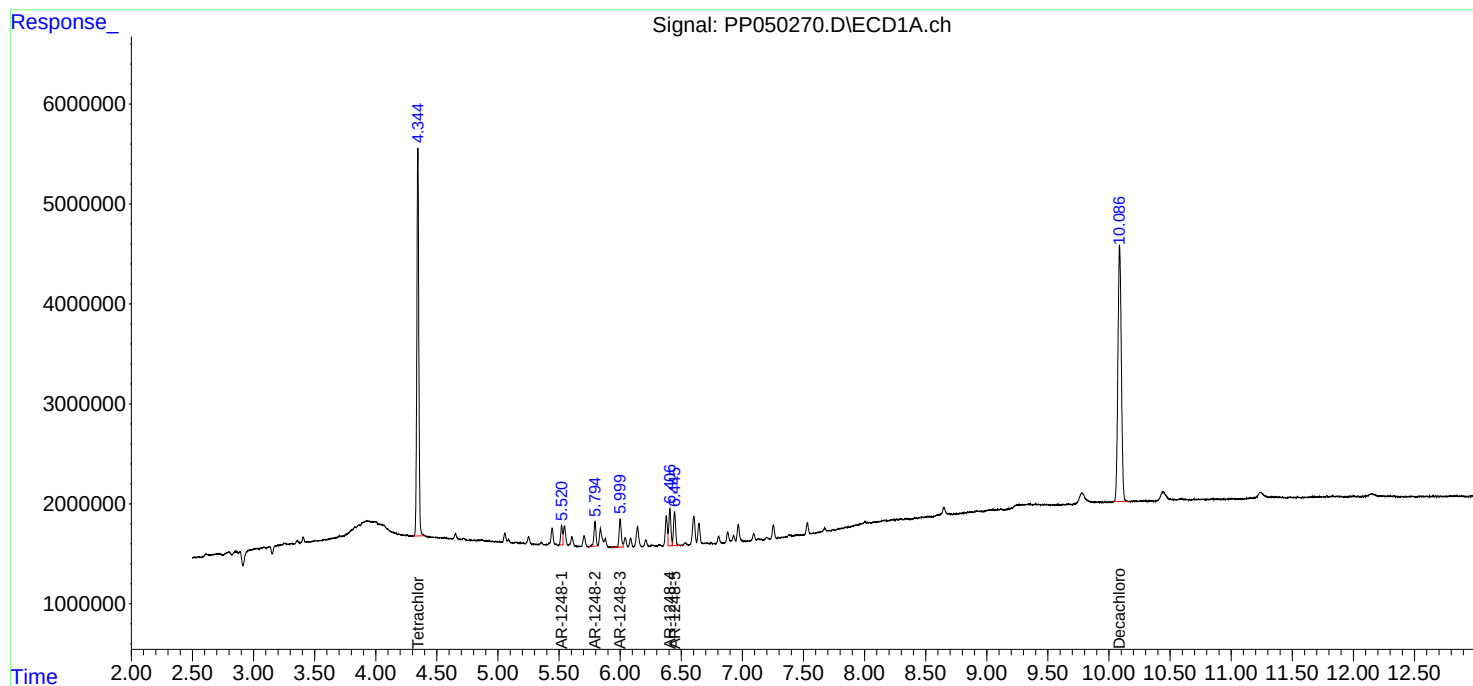


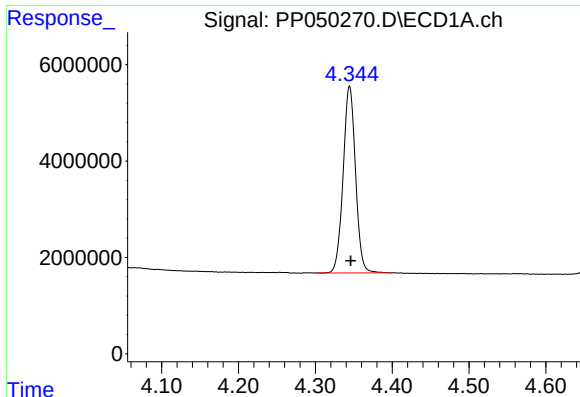

#1 Tetrachloro-m-xylene


R.T.: 4.345 min
Delta R.T.: -0.001 min
Response: 43299777
Conc: 26.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

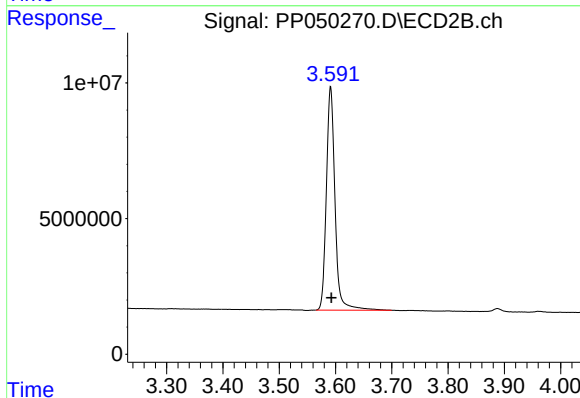


#1 Tetrachloro-m-xylene

R.T.: 3.591 min
Delta R.T.: -0.001 min
Response: 88048160
Conc: 28.11 ng/ml

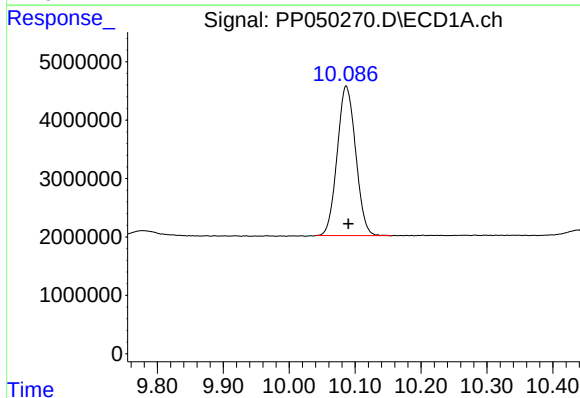


#2 Decachlorobiphenyl

R.T.: 10.087 min
Delta R.T.: -0.003 min
Response: 49860428
Conc: 28.32 ng/ml

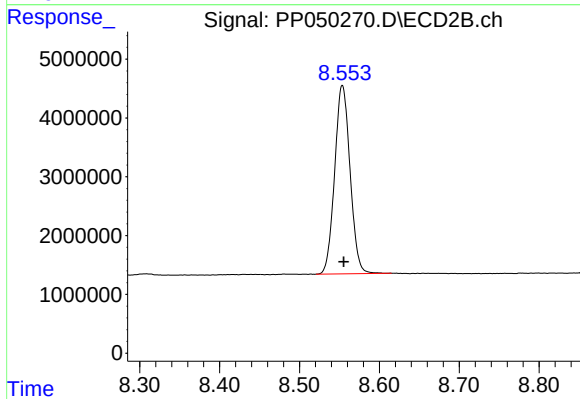

#2 Decachlorobiphenyl


R.T.: 8.554 min
Delta R.T.: -0.002 min
Response: 42981462
Conc: 27.93 ng/ml

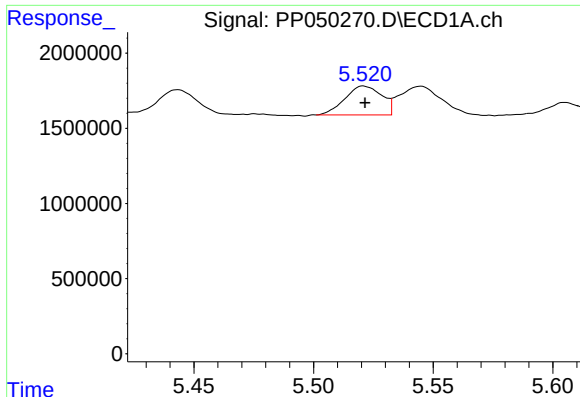

#21 AR-1248-1


R.T.: 5.521 min
Delta R.T.: 0.000 min
Response: 2056562
Conc: 50.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

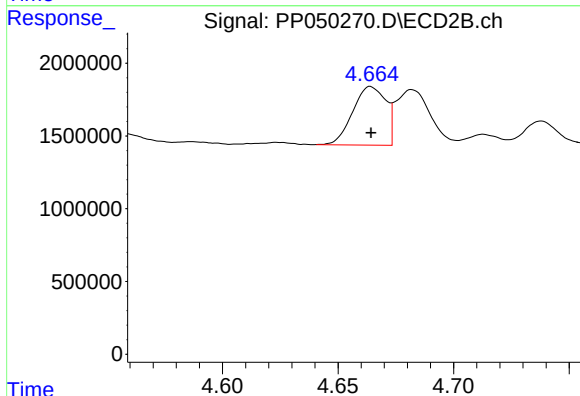


#21 AR-1248-1

R.T.: 4.664 min
Delta R.T.: 0.000 min
Response: 4000525
Conc: 59.86 ng/ml

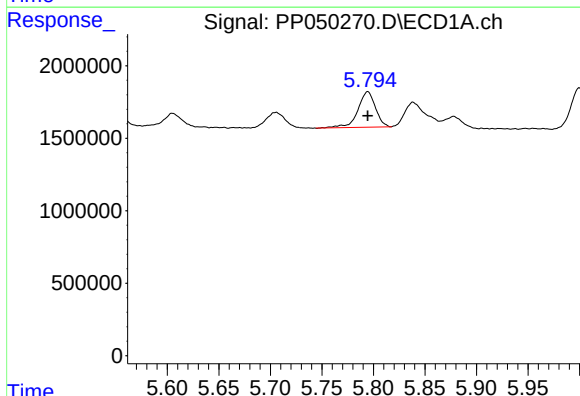


#22 AR-1248-2

R.T.: 5.794 min
Delta R.T.: 0.000 min
Response: 2899757
Conc: 51.91 ng/ml

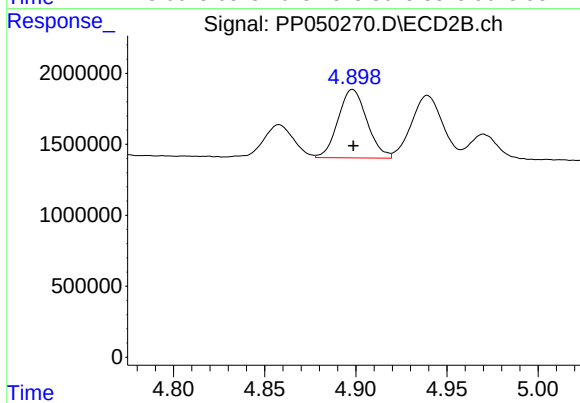

#22 AR-1248-2


R.T.: 4.898 min
Delta R.T.: 0.000 min
Response: 5336625
Conc: 61.78 ng/ml

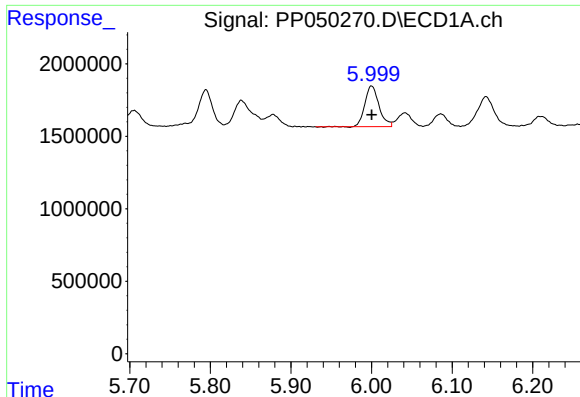

#23 AR-1248-3


R.T.: 6.000 min
Delta R.T.: 0.000 min
Response: 3424769
Conc: 53.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

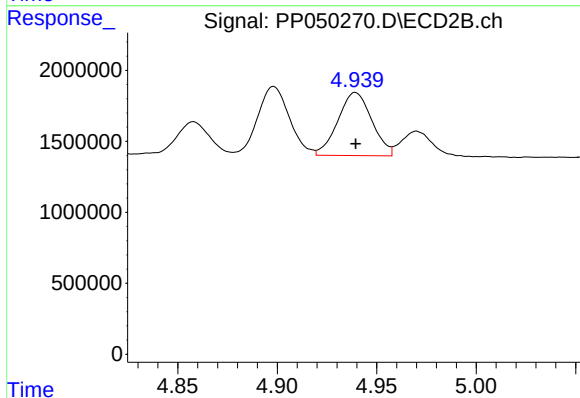


#23 AR-1248-3

R.T.: 4.939 min
Delta R.T.: 0.000 min
Response: 5291904
Conc: 58.37 ng/ml

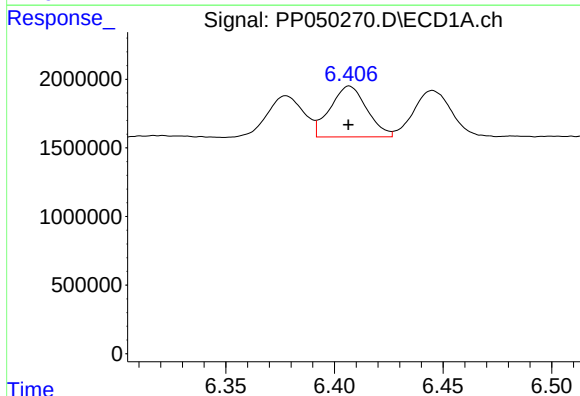


#24 AR-1248-4

R.T.: 6.407 min
Delta R.T.: 0.000 min
Response: 4364644
Conc: 55.18 ng/ml

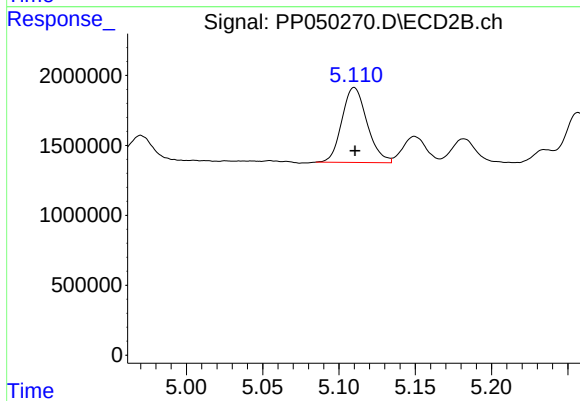

#24 AR-1248-4


R.T.: 5.110 min
Delta R.T.: 0.000 min
Response: 6169142
Conc: 58.53 ng/ml

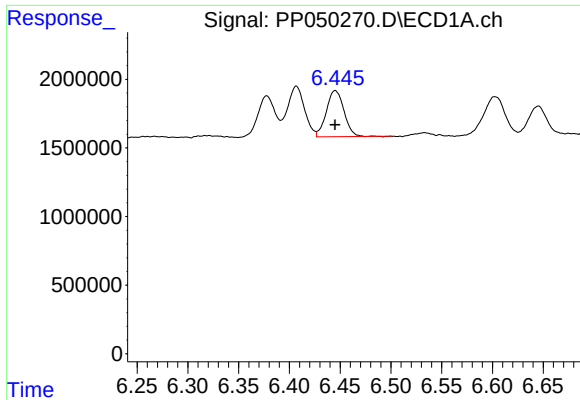

#25 AR-1248-5

R.T.: 6.445 min
Delta R.T.: 0.000 min
Response: 4067186
Conc: 53.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

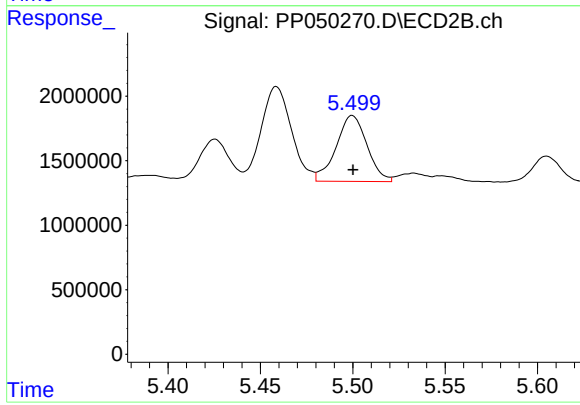

#25 AR-1248-5

R.T.: 5.500 min
Delta R.T.: 0.000 min
Response: 5956152
Conc: 59.99 ng/ml