

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081123\
 Data File : PP059322.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Aug 2023 10:52
 Operator : YP\AJ
 Sample : 03572-09
 Misc : AR1221 MDL 25 PPB
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT3-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 17:24:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 02:30:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.414	3.645	19487633	34584393	15.882	17.069
2) SA Decachlor...	10.204	8.680	16086211	29648962	21.076	21.075
Target Compounds						
8) L2 AR-1221-1	4.624	3.861	363705	628184	23.086	23.141m
9) L2 AR-1221-2	4.722	3.946	570759	729739	48.333	36.652
10) L2 AR-1221-3	4.787	4.022	744485	1235066	21.142	20.746



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081123\
Data File : PP059322.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Aug 2023 10:52
Operator : YP\AJ
Sample : 03572-09
Misc : AR1221 MDL 25 PPB
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 17:24:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 09 02:30:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

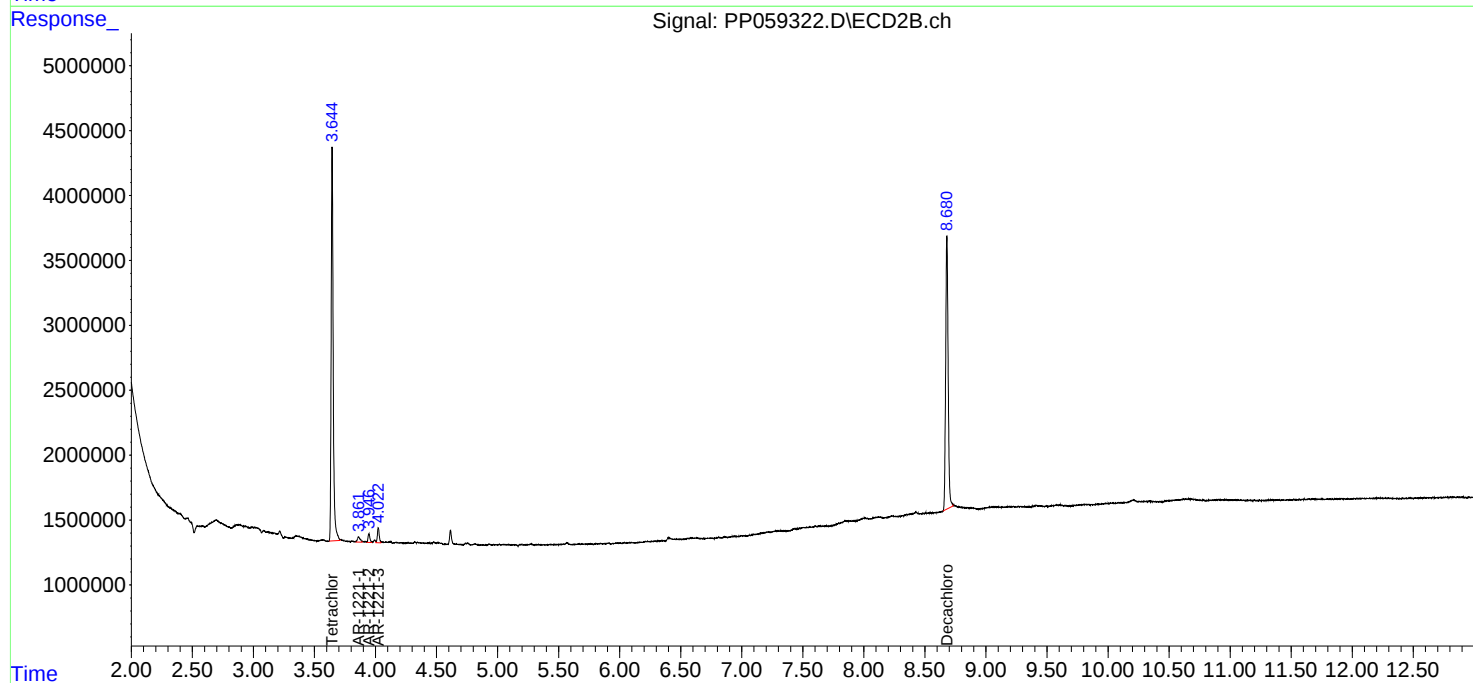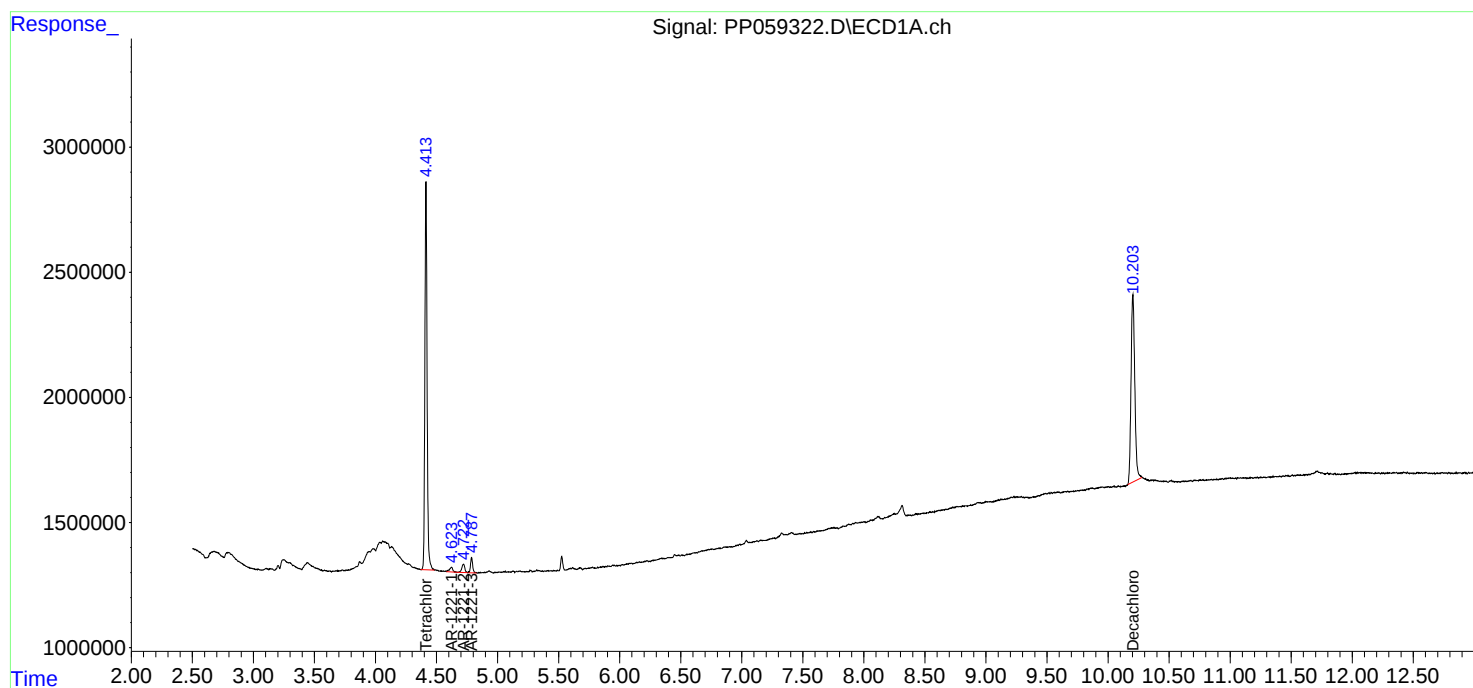


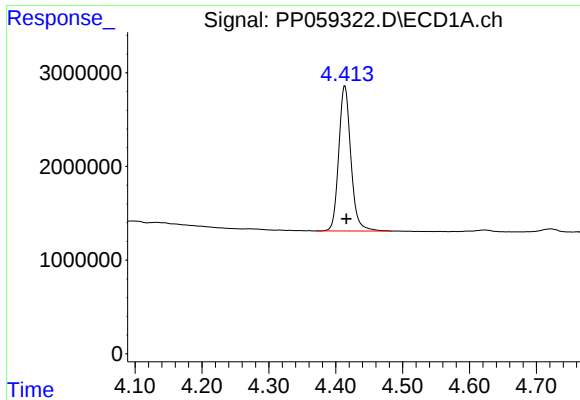

#1 Tetrachloro-m-xylene


R.T.: 4.414 min
Delta R.T.: -0.002 min
Response: 19487633
Conc: 15.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

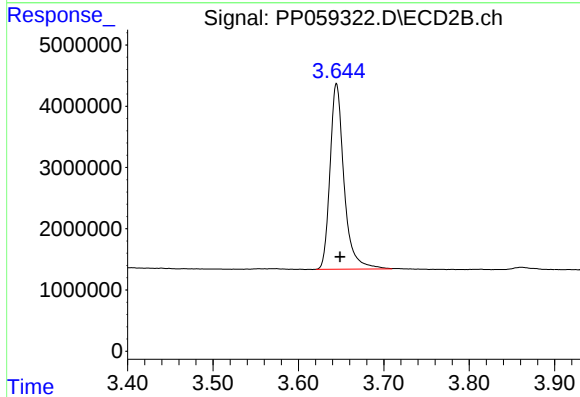


#1 Tetrachloro-m-xylene

R.T.: 3.645 min
Delta R.T.: -0.004 min
Response: 34584393
Conc: 17.07 ng/ml

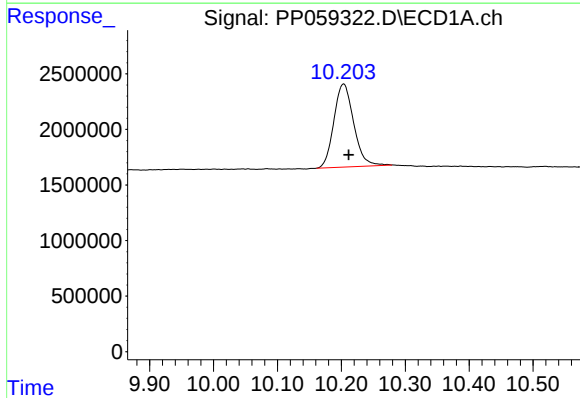


#2 Decachlorobiphenyl

R.T.: 10.204 min
Delta R.T.: -0.008 min
Response: 16086211
Conc: 21.08 ng/ml

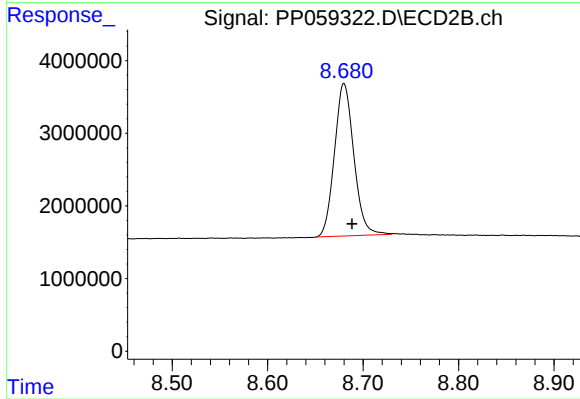

#2 Decachlorobiphenyl


R.T.: 8.680 min
Delta R.T.: -0.009 min
Response: 29648962
Conc: 21.08 ng/ml

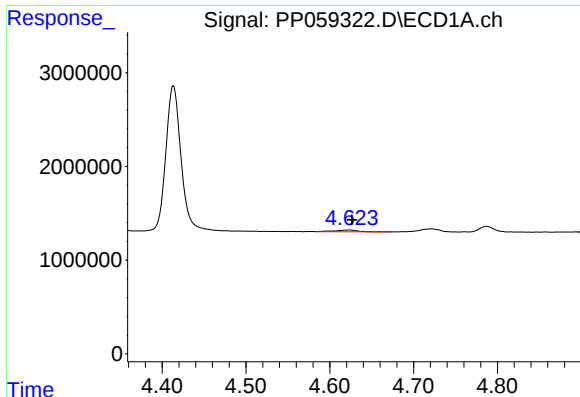

#8 AR-1221-1


R.T.: 4.624 min
Delta R.T.: -0.003 min
Response: 363705
Conc: 23.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

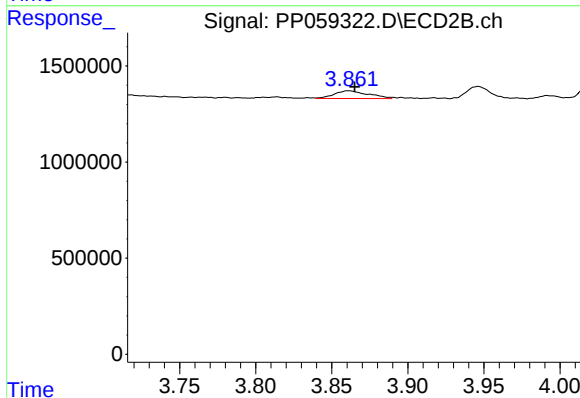


#8 AR-1221-1

R.T.: 3.861 min
Delta R.T.: -0.004 min
Response: 628184
Conc: 23.14 ng/ml m

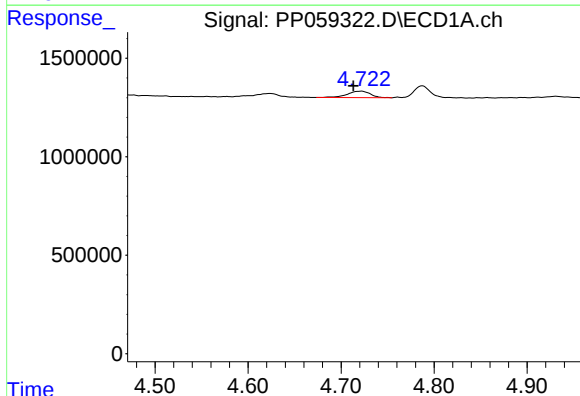


#9 AR-1221-2

R.T.: 4.722 min
Delta R.T.: 0.008 min
Response: 570759
Conc: 48.33 ng/ml

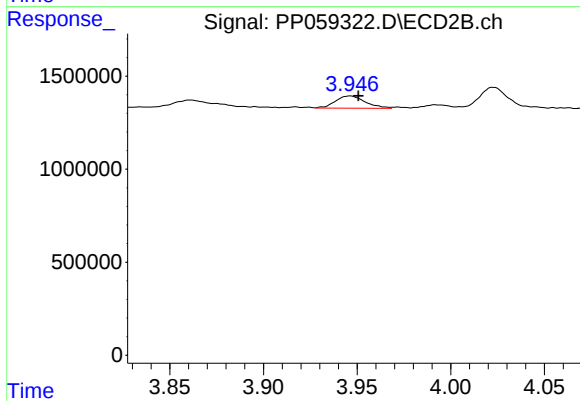

#9 AR-1221-2


R.T.: 3.946 min
Delta R.T.: -0.004 min
Response: 729739
Conc: 36.65 ng/ml

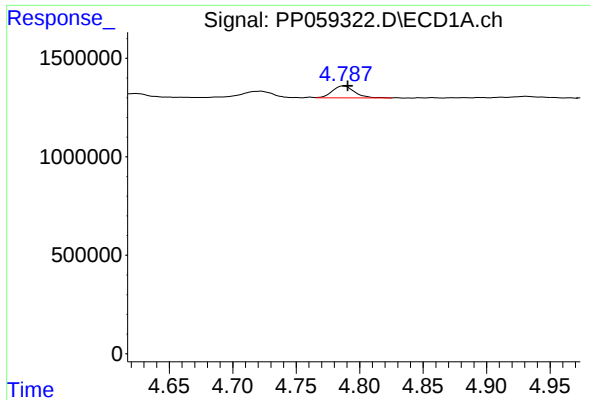

#10 AR-1221-3

R.T.: 4.787 min
Delta R.T.: -0.003 min
Response: 744485
Conc: 21.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

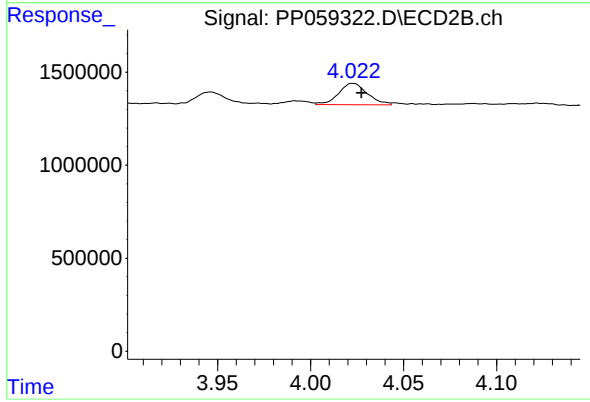

#10 AR-1221-3

R.T.: 4.022 min
Delta R.T.: -0.005 min
Response: 1235066
Conc: 20.75 ng/ml