

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081123\
 Data File : PP059323.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Aug 2023 11:09
 Operator : YP\AJ
 Sample : 03572-09
 Misc : AR1232 MDL 25 PPB
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT3-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 17:24:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 02:30:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.413	3.661	21282822	37630370	17.345	18.572
2) SA Decachlor...	10.203	8.696	17915555	32571036	23.473	23.152
Target Compounds						
11) L3 AR-1232-1	4.787	4.037	781369	1115453	26.580m	23.509m
12) L3 AR-1232-2	5.322	4.754	403313	824367	25.875	19.434
13) L3 AR-1232-3	5.612	4.949	630717	632204	23.886	28.493m
14) L3 AR-1232-4	5.774	5.032	300854	618788	22.733	29.307m#
15) L3 AR-1232-5	5.865	5.203	254197	655469	22.270	28.595m#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081123\
Data File : PP059323.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Aug 2023 11:09
Operator : YP\AJ
Sample : 03572-09
Misc : AR1232 MDL 25 PPB
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 17:24:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 09 02:30:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

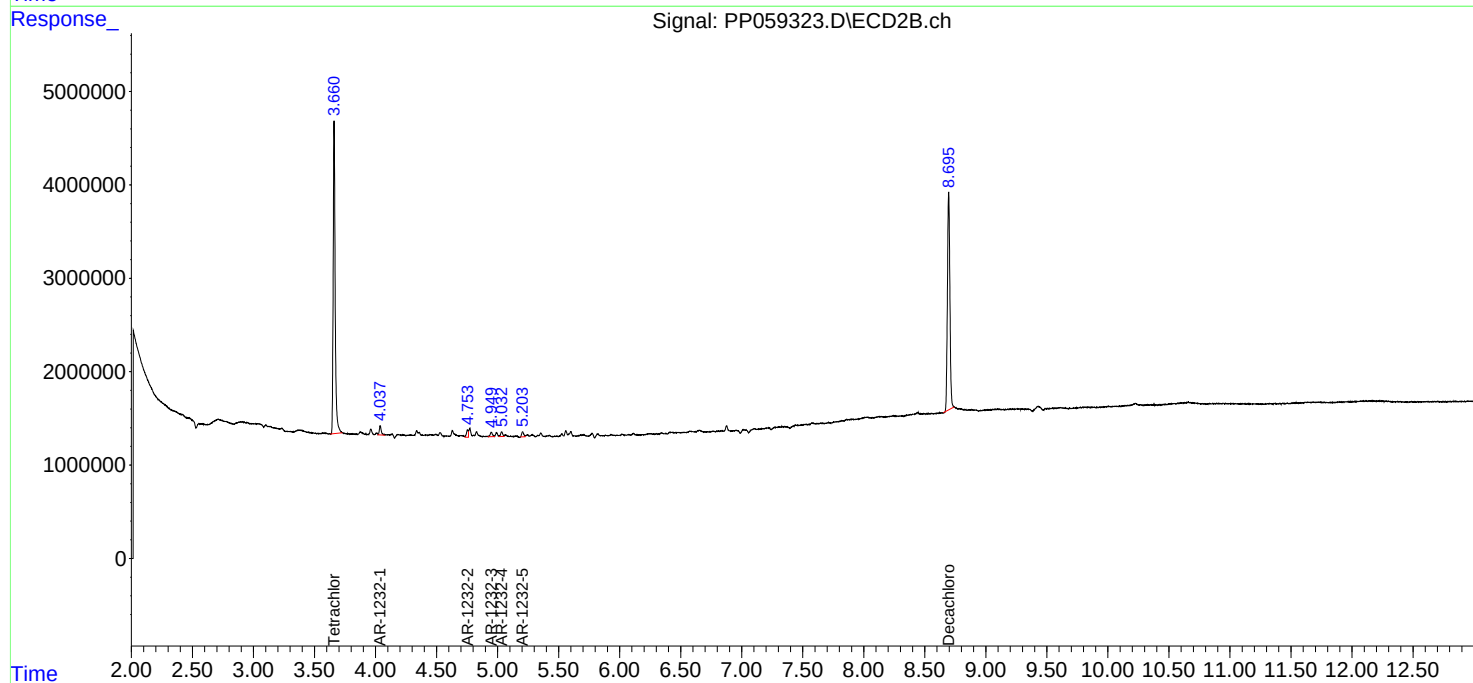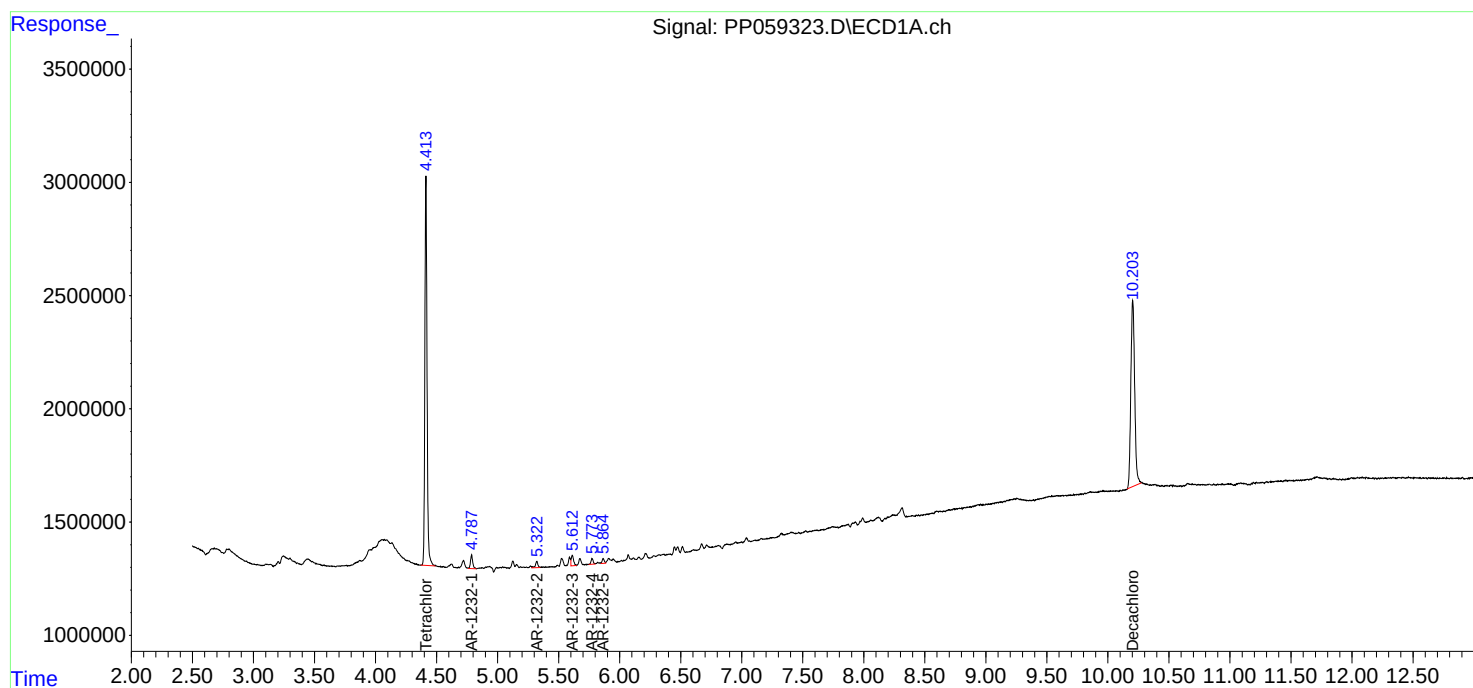


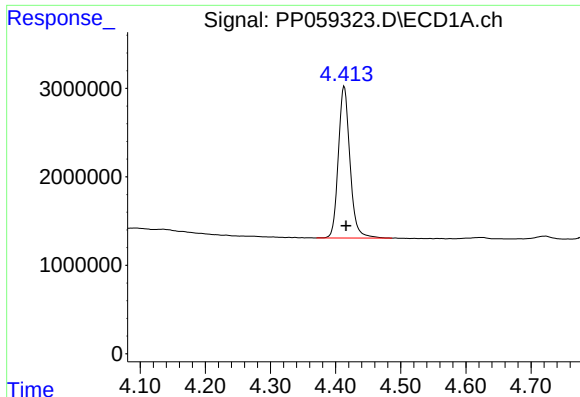

#1 Tetrachloro-m-xylene


R.T.: 4.413 min
Delta R.T.: -0.003 min
Response: 21282822
Conc: 17.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

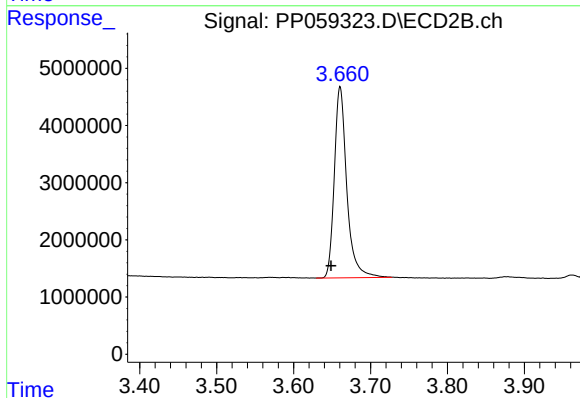


#1 Tetrachloro-m-xylene

R.T.: 3.661 min
Delta R.T.: 0.012 min
Response: 37630370
Conc: 18.57 ng/ml

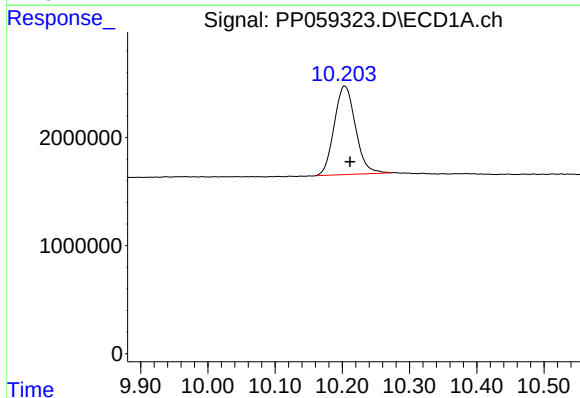


#2 Decachlorobiphenyl

R.T.: 10.203 min
Delta R.T.: -0.008 min
Response: 17915555
Conc: 23.47 ng/ml

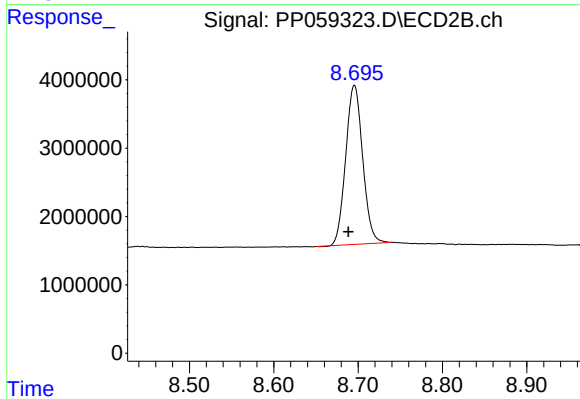

#2 Decachlorobiphenyl


R.T.: 8.696 min
Delta R.T.: 0.007 min
Response: 32571036
Conc: 23.15 ng/ml

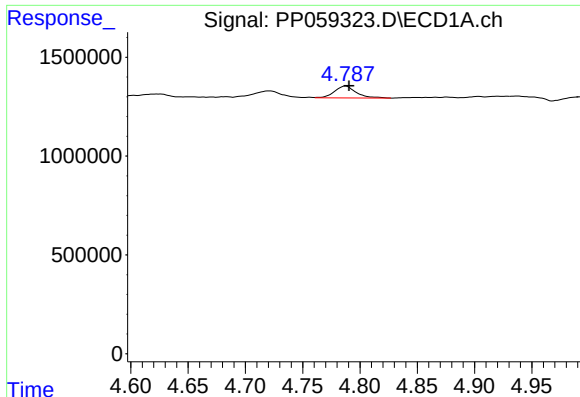

#11 AR-1232-1


R.T.: 4.787 min
Delta R.T.: -0.003 min
Response: 781369
Conc: 26.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

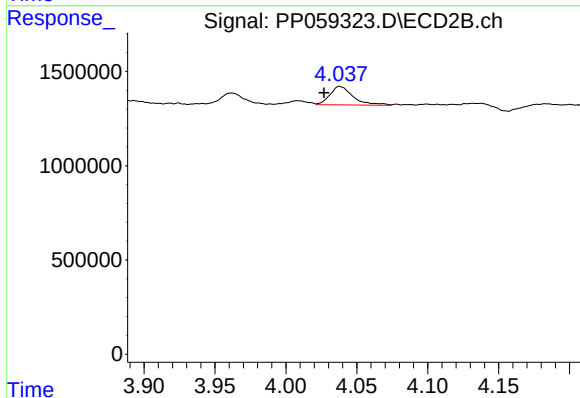


#11 AR-1232-1

R.T.: 4.037 min
Delta R.T.: 0.010 min
Response: 1115453
Conc: 23.51 ng/ml m

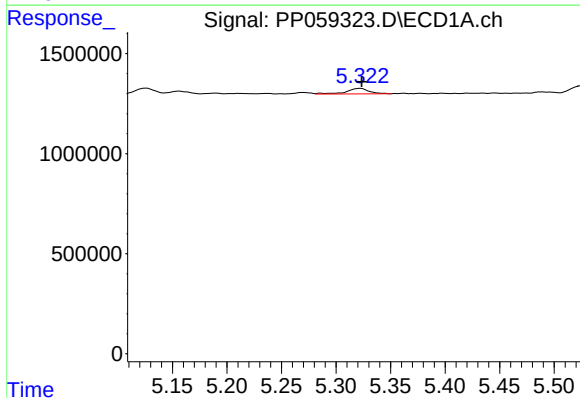


#12 AR-1232-2

R.T.: 5.322 min
Delta R.T.: -0.002 min
Response: 403313
Conc: 25.87 ng/ml

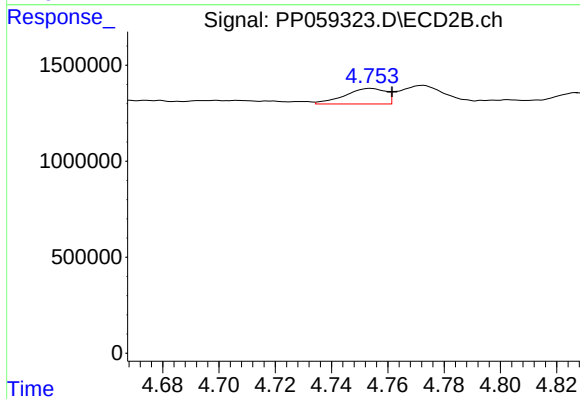

#12 AR-1232-2


R.T.: 4.754 min
Delta R.T.: -0.008 min
Response: 824367
Conc: 19.43 ng/ml

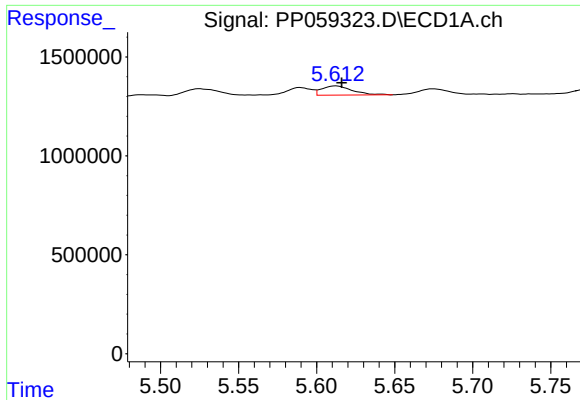

#13 AR-1232-3


R.T.: 5.612 min
Delta R.T.: -0.004 min
Response: 630717
Conc: 23.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

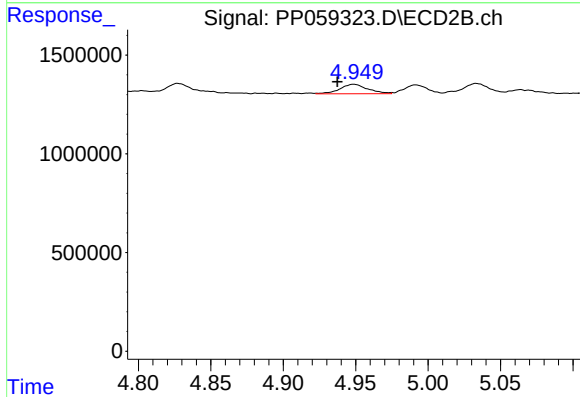


#13 AR-1232-3

R.T.: 4.949 min
Delta R.T.: 0.011 min
Response: 632204
Conc: 28.49 ng/ml m

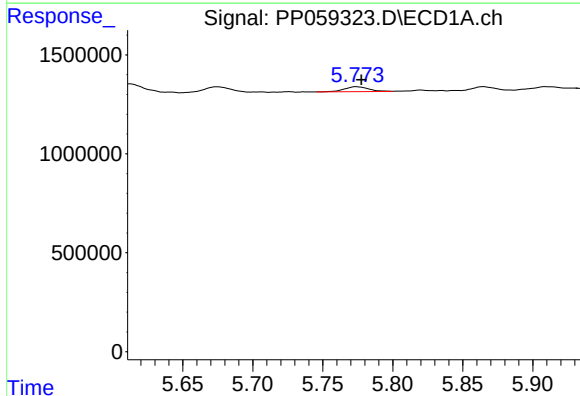


#14 AR-1232-4

R.T.: 5.774 min
Delta R.T.: -0.004 min
Response: 300854
Conc: 22.73 ng/ml

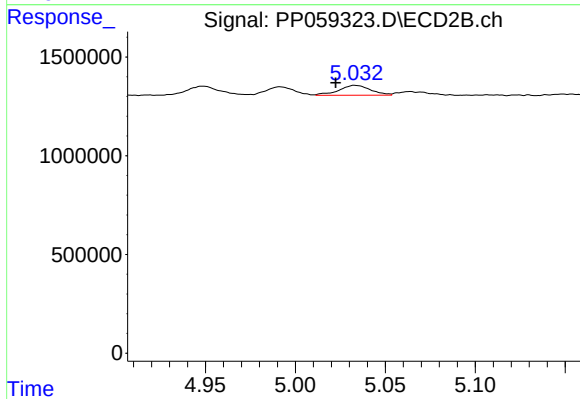

#14 AR-1232-4


R.T.: 5.032 min
Delta R.T.: 0.010 min
Response: 618788
Conc: 29.31 ng/ml m

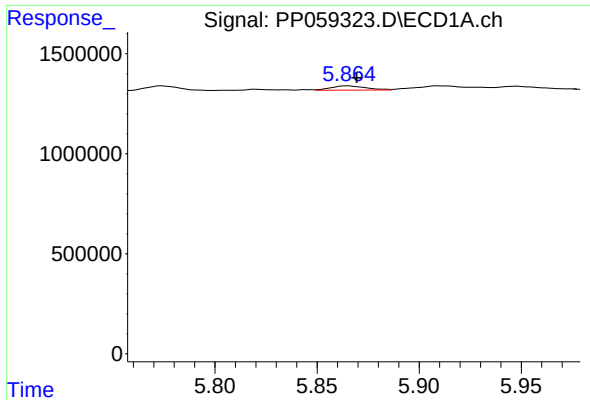

#15 AR-1232-5

R.T.: 5.865 min
Delta R.T.: -0.005 min
Response: 254197
Conc: 22.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

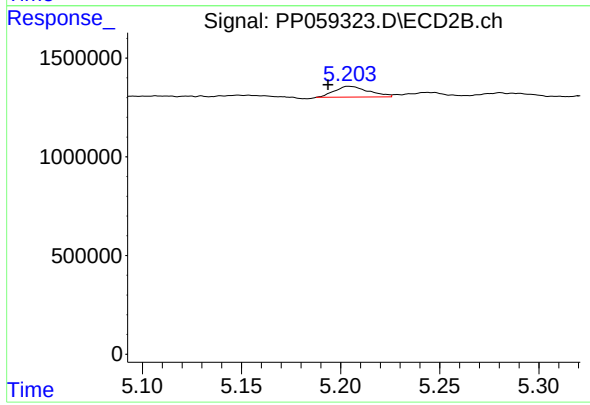

#15 AR-1232-5

R.T.: 5.203 min
Delta R.T.: 0.010 min
Response: 655469
Conc: 28.59 ng/ml m