

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081123\
 Data File : PP059325.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Aug 2023 11:41
 Operator : YP\AJ
 Sample : 03572-09
 Misc : AR1248 MDL 25 PPB
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT3-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 17:25:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 02:30:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.414	3.645	19543375	34192635	15.927	16.876
2) SA Decachlor...	10.205	8.680	16510077	30609992	21.632	21.758
Target Compounds						
21) L5 AR-1248-1	5.591	4.737	559289	976345	22.036	23.733m
22) L5 AR-1248-2	5.866	4.975	814905	1659364	21.054	27.556 #
23) L5 AR-1248-3	6.072	5.017	947122	1787658	22.419	29.016 #
24) L5 AR-1248-4	6.477	5.189	1018903	1698643	24.472	23.594
25) L5 AR-1248-5	6.515	5.584	974221	1584084	23.883	24.007m



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081123\
Data File : PP059325.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Aug 2023 11:41
Operator : YP\AJ
Sample : 03572-09
Misc : AR1248 MDL 25 PPB
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 17:25:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 09 02:30:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

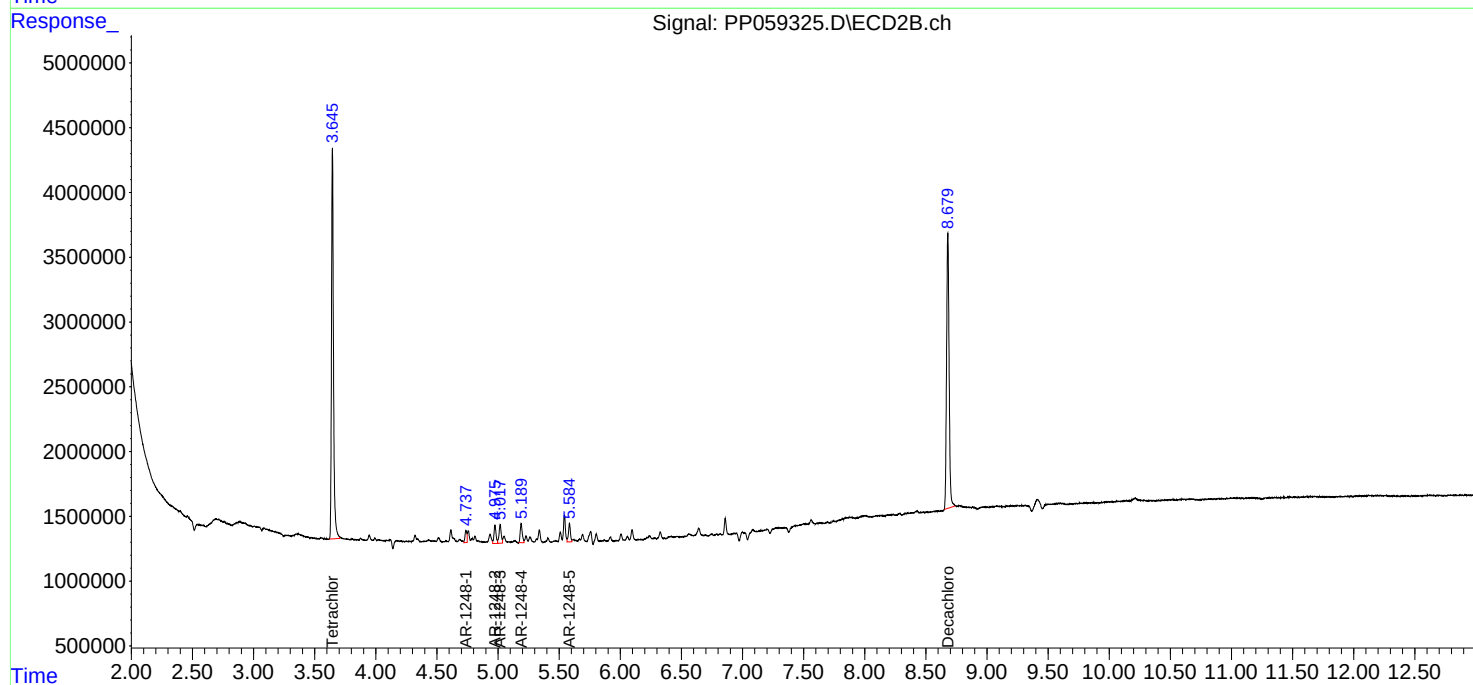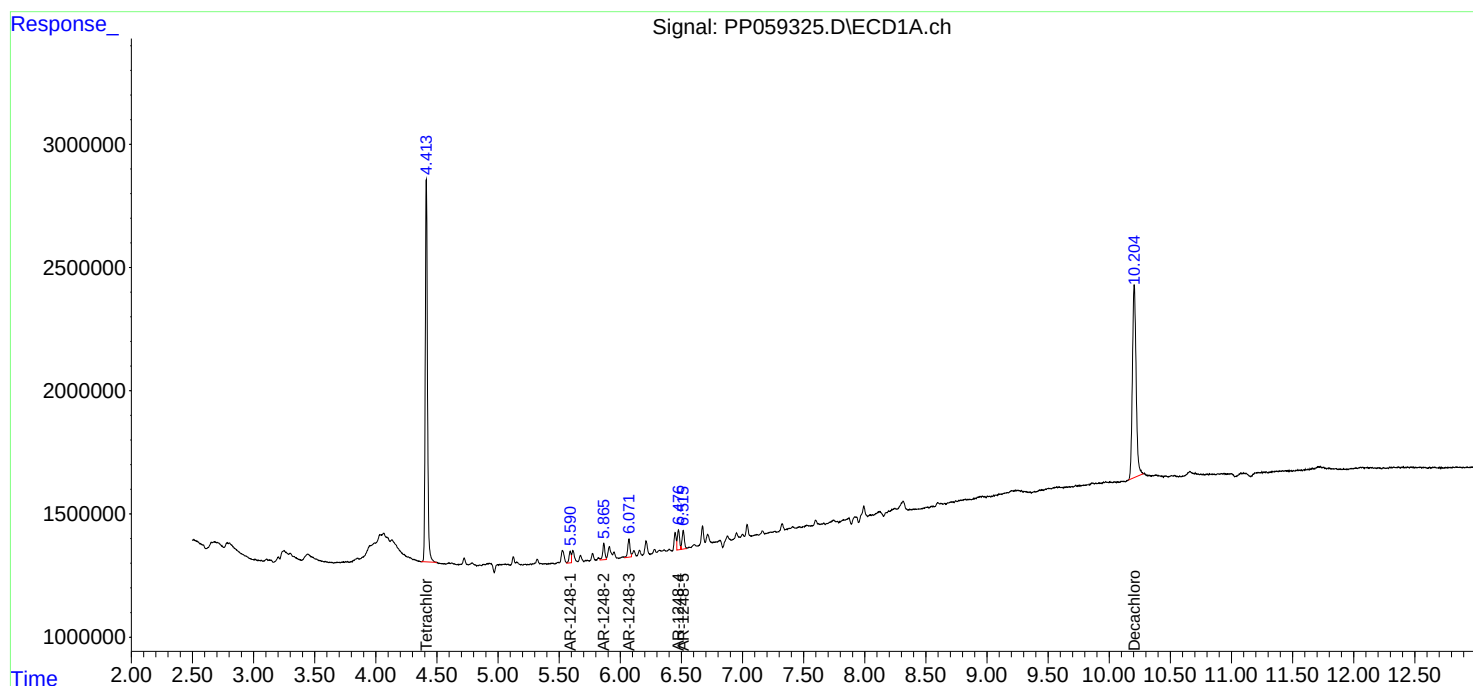


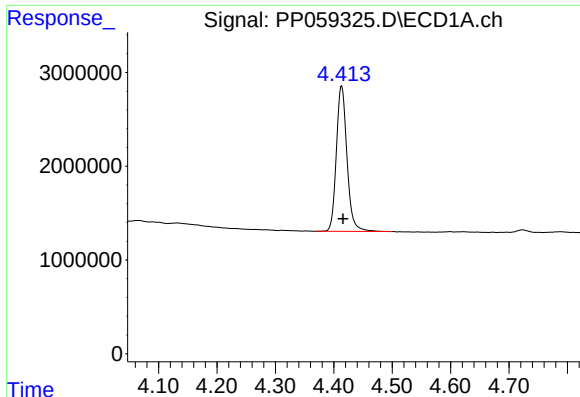

#1 Tetrachloro-m-xylene


R.T.: 4.414 min
Delta R.T.: -0.002 min
Response: 19543375
Conc: 15.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

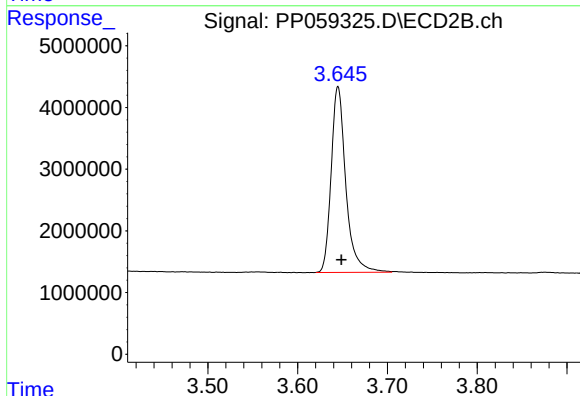


#1 Tetrachloro-m-xylene

R.T.: 3.645 min
Delta R.T.: -0.004 min
Response: 34192635
Conc: 16.88 ng/ml

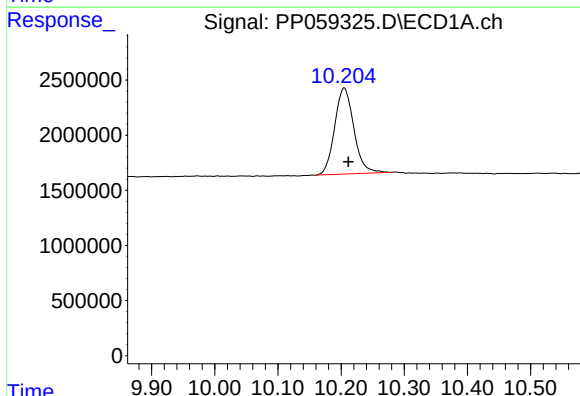


#2 Decachlorobiphenyl

R.T.: 10.205 min
Delta R.T.: -0.006 min
Response: 16510077
Conc: 21.63 ng/ml

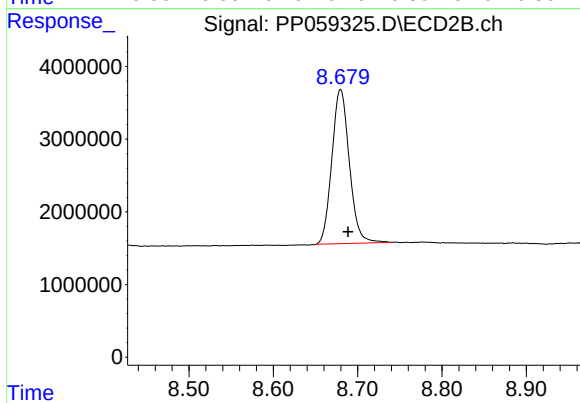

#2 Decachlorobiphenyl


R.T.: 8.680 min
Delta R.T.: -0.009 min
Response: 30609992
Conc: 21.76 ng/ml

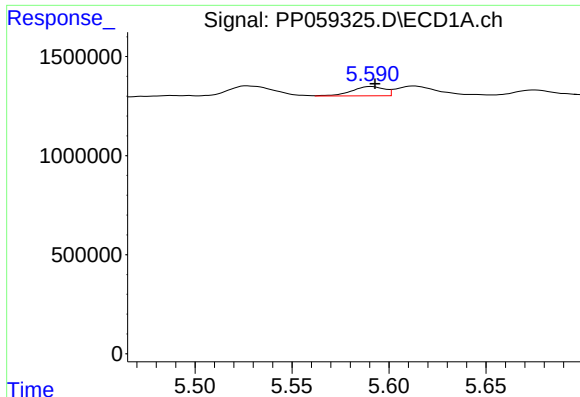

#21 AR-1248-1


R.T.: 5.591 min
Delta R.T.: -0.002 min
Response: 559289
Conc: 22.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

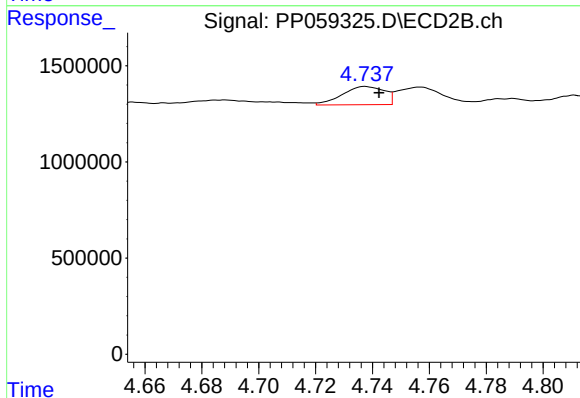


#21 AR-1248-1

R.T.: 4.737 min
Delta R.T.: -0.005 min
Response: 976345
Conc: 23.73 ng/ml m

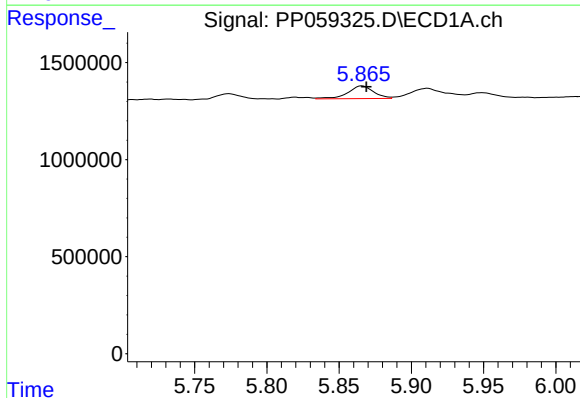


#22 AR-1248-2

R.T.: 5.866 min
Delta R.T.: -0.003 min
Response: 814905
Conc: 21.05 ng/ml

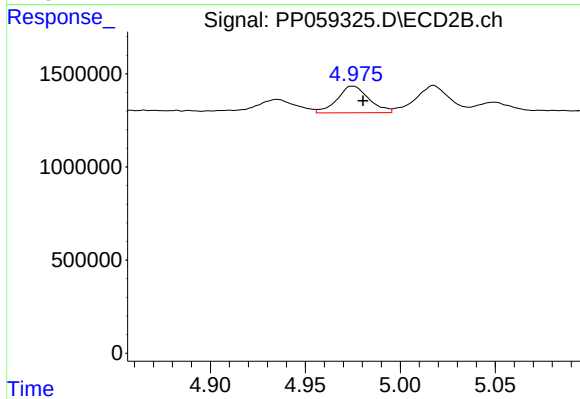

#22 AR-1248-2


R.T.: 4.975 min
Delta R.T.: -0.005 min
Response: 1659364
Conc: 27.56 ng/ml

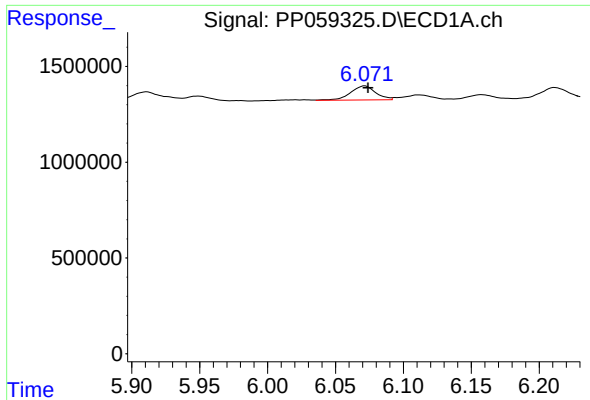

#23 AR-1248-3


R.T.: 6.072 min
Delta R.T.: -0.002 min
Response: 947122
Conc: 22.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

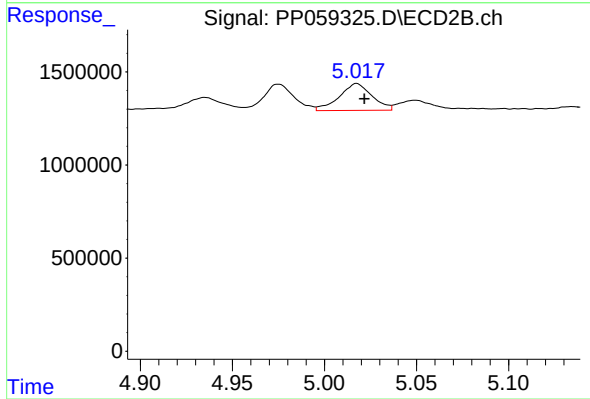


#23 AR-1248-3

R.T.: 5.017 min
Delta R.T.: -0.004 min
Response: 1787658
Conc: 29.02 ng/ml

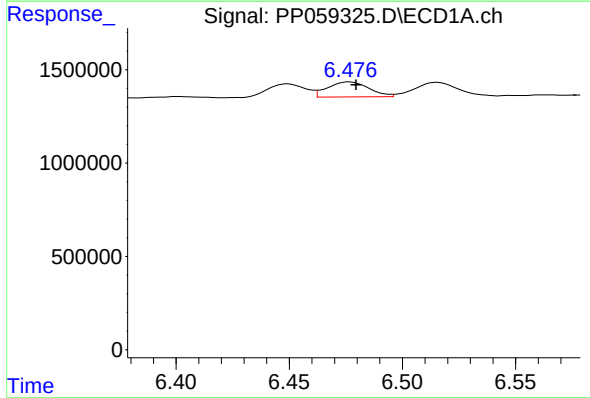


#24 AR-1248-4

R.T.: 6.477 min
Delta R.T.: -0.003 min
Response: 1018903
Conc: 24.47 ng/ml

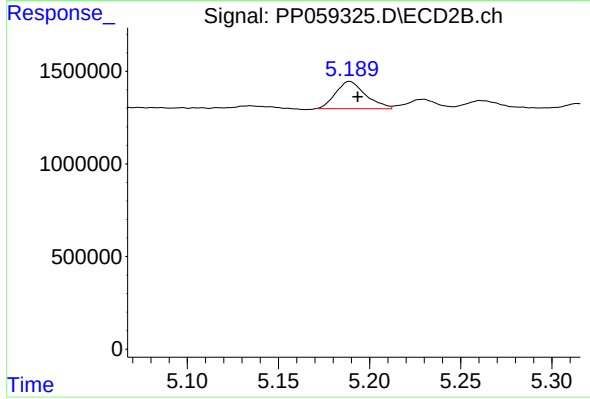

#24 AR-1248-4


R.T.: 5.189 min
Delta R.T.: -0.004 min
Response: 1698643
Conc: 23.59 ng/ml

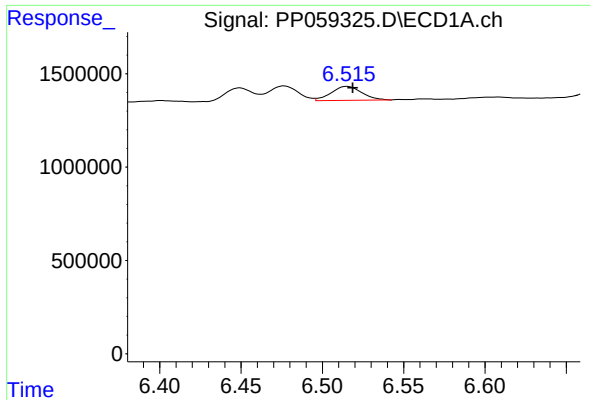

#25 AR-1248-5

R.T.: 6.515 min
Delta R.T.: -0.003 min
Response: 974221
Conc: 23.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

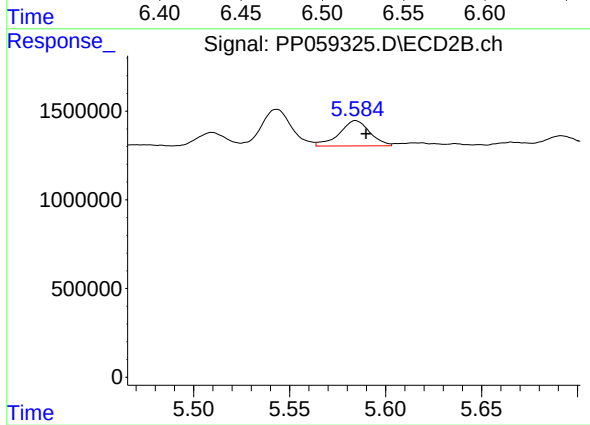

#25 AR-1248-5

R.T.: 5.584 min
Delta R.T.: -0.006 min
Response: 1584084
Conc: 24.01 ng/ml m