

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081123\
 Data File : PP059326.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Aug 2023 11:57
 Operator : YP\AJ
 Sample : 03572-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT3-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 17:26:09 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 02:30:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.413	3.645	20861728	35981227	17.002	17.758
2) SA Decachlor...	10.206	8.680	17768790	31382671	23.281	22.308
Target Compounds						
26) L6 AR-1254-1	6.450	5.543	1365729	2762184	29.235	27.263m
27) L6 AR-1254-2	6.671	5.692	2129404	2320608	30.947	26.287m
28) L6 AR-1254-3	7.037	6.097	2004593	3763165	29.044m	27.221
29) L6 AR-1254-4	7.325	6.328	1244023	2253193	27.635	28.031
30) L6 AR-1254-5	7.745	6.746	1263176	2939747	26.884m	24.583



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081123\
Data File : PP059326.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Aug 2023 11:57
Operator : YP\AJ
Sample : 03572-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 17:26:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 09 02:30:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

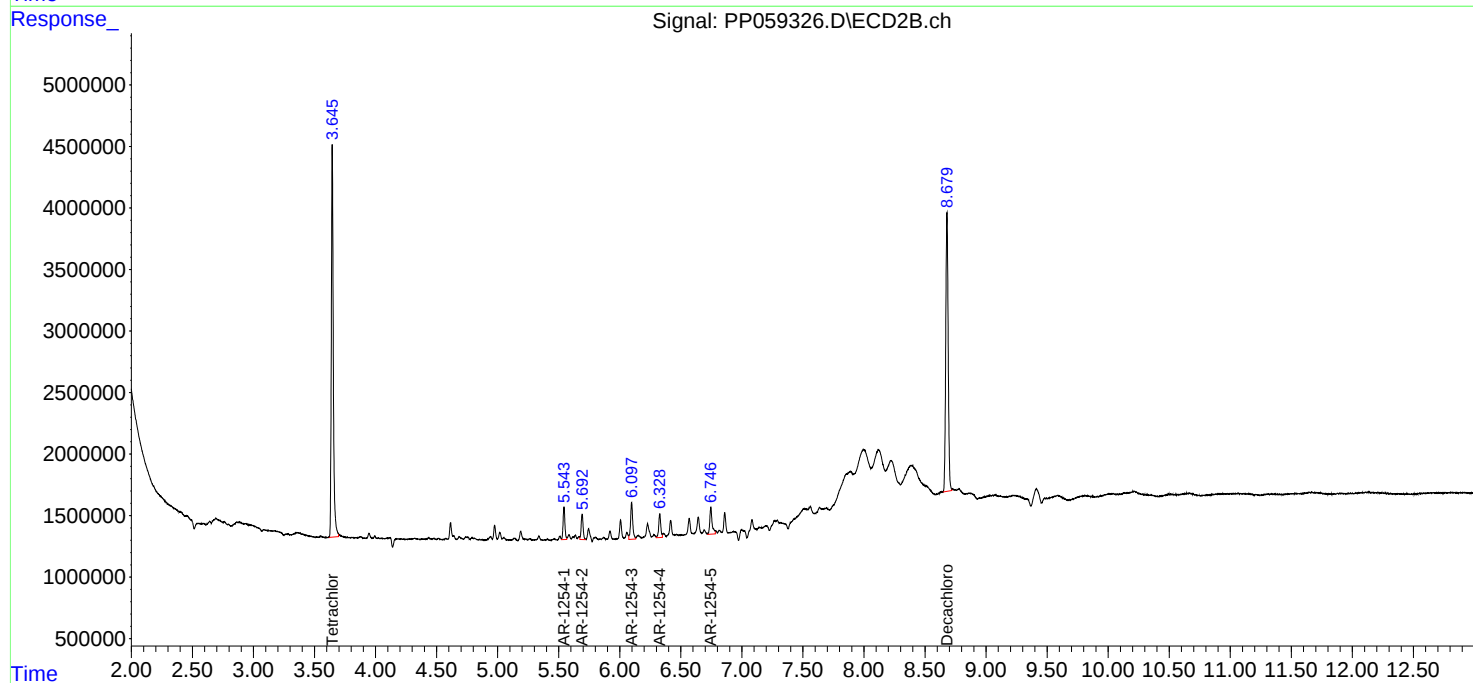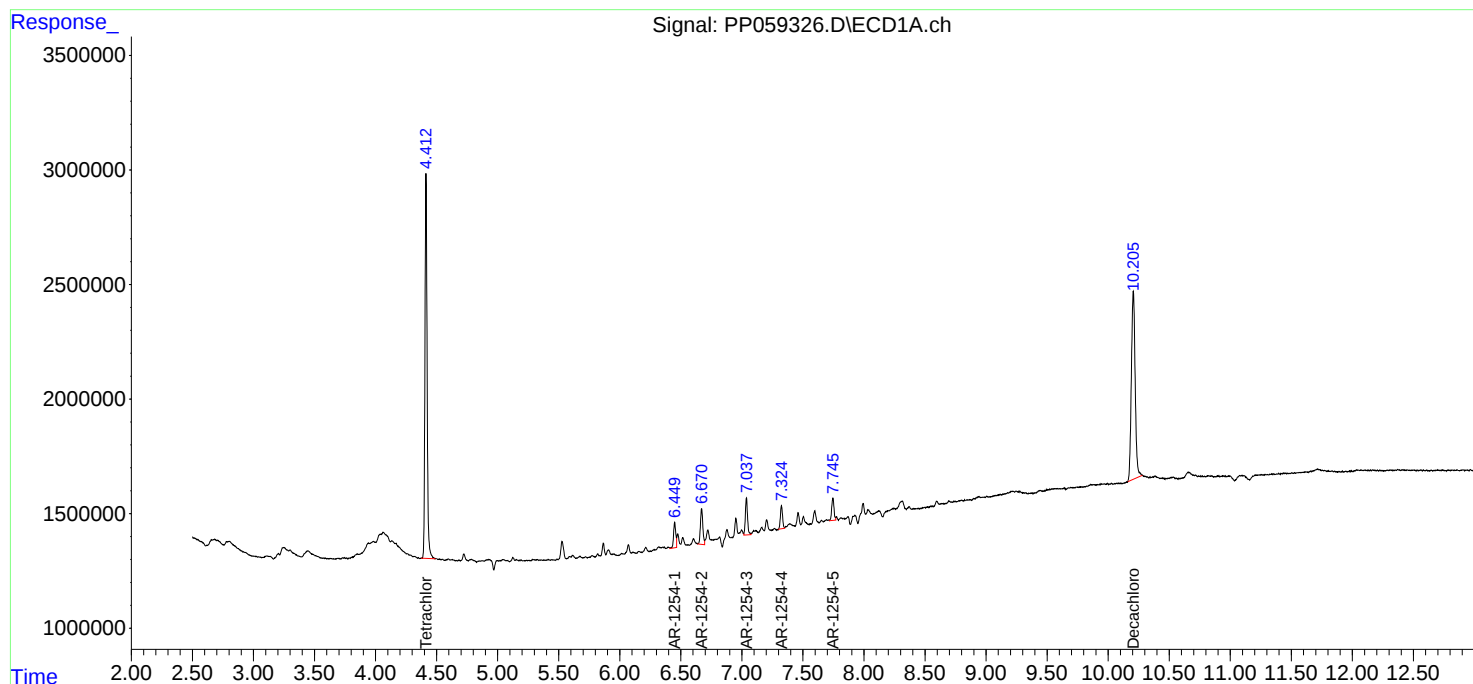


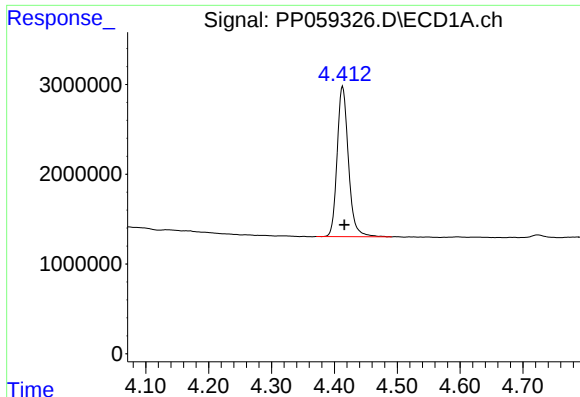

#1 Tetrachloro-m-xylene


R.T.: 4.413 min
Delta R.T.: -0.003 min
Response: 20861728
Conc: 17.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

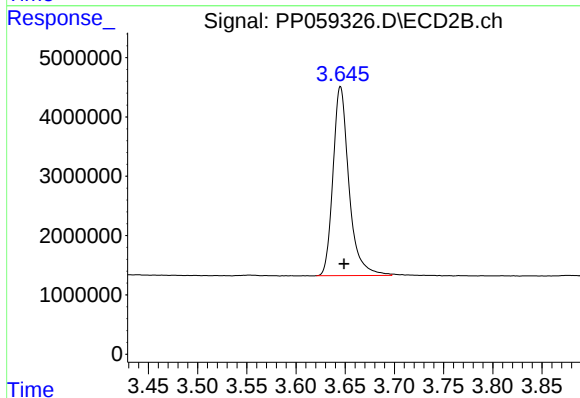


#1 Tetrachloro-m-xylene

R.T.: 3.645 min
Delta R.T.: -0.004 min
Response: 35981227
Conc: 17.76 ng/ml

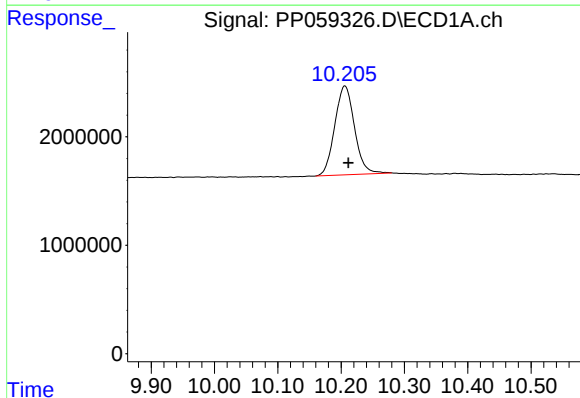


#2 Decachlorobiphenyl

R.T.: 10.206 min
Delta R.T.: -0.005 min
Response: 17768790
Conc: 23.28 ng/ml

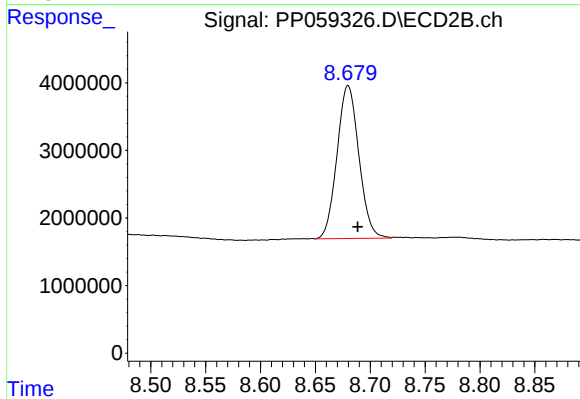

#2 Decachlorobiphenyl


R.T.: 8.680 min
Delta R.T.: -0.009 min
Response: 31382671
Conc: 22.31 ng/ml

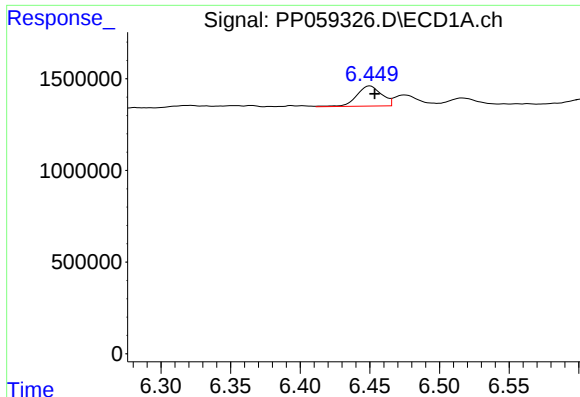

#26 AR-1254-1


R.T.: 6.450 min
Delta R.T.: -0.003 min
Response: 1365729
Conc: 29.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

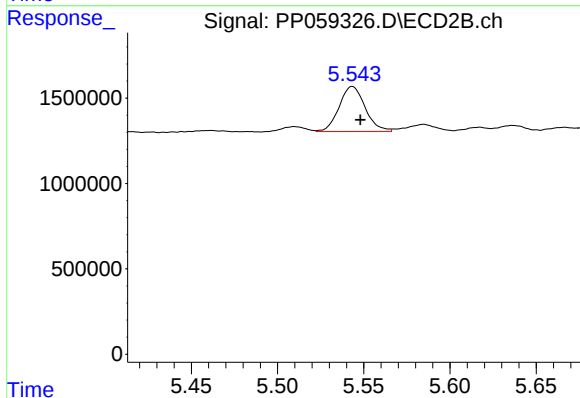


#26 AR-1254-1

R.T.: 5.543 min
Delta R.T.: -0.005 min
Response: 2762184
Conc: 27.26 ng/ml m

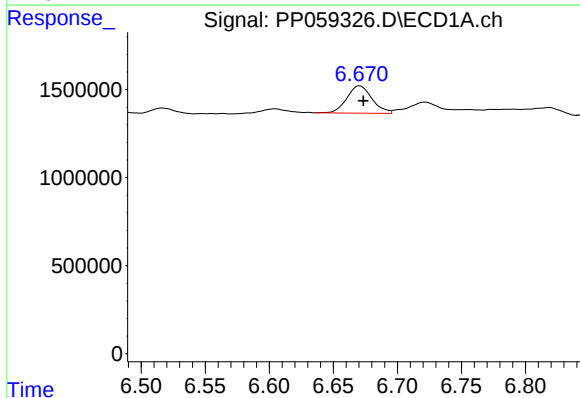


#27 AR-1254-2

R.T.: 6.671 min
Delta R.T.: -0.003 min
Response: 2129404
Conc: 30.95 ng/ml

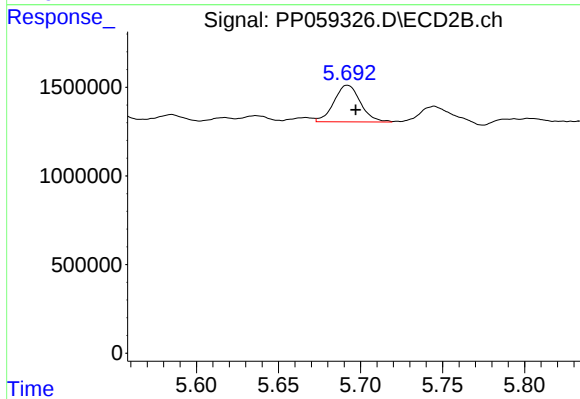

#27 AR-1254-2


R.T.: 5.692 min
Delta R.T.: -0.005 min
Response: 2320608
Conc: 26.29 ng/ml m

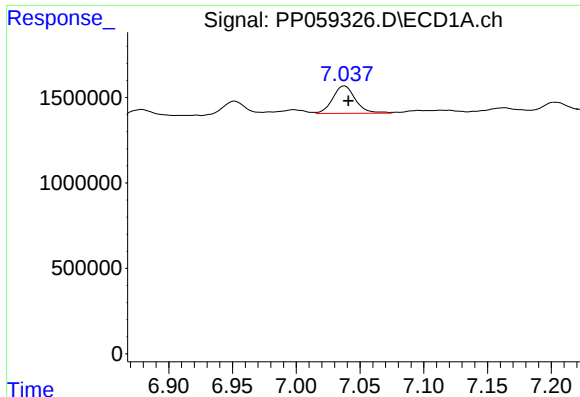

#28 AR-1254-3


R.T.: 7.037 min
Delta R.T.: -0.003 min
Response: 2004593
Conc: 29.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

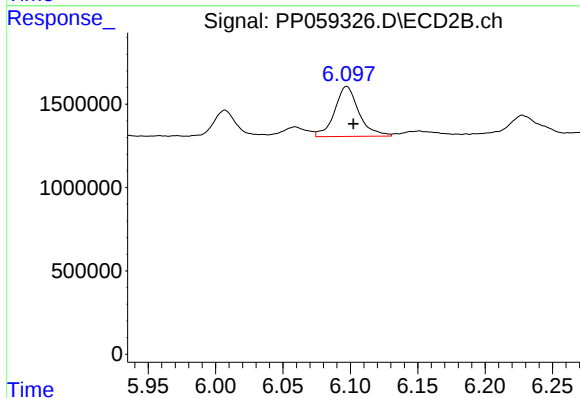


#28 AR-1254-3

R.T.: 6.097 min
Delta R.T.: -0.005 min
Response: 3763165
Conc: 27.22 ng/ml

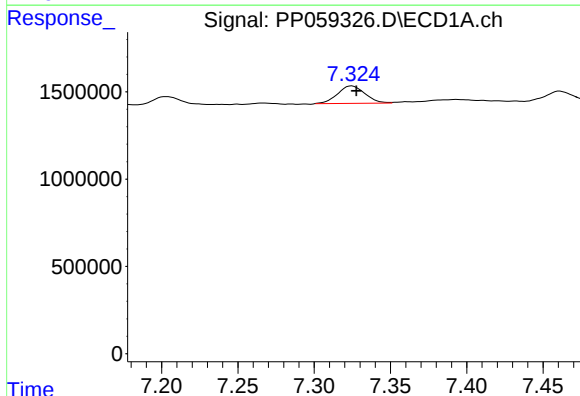


#29 AR-1254-4

R.T.: 7.325 min
Delta R.T.: -0.003 min
Response: 1244023
Conc: 27.64 ng/ml

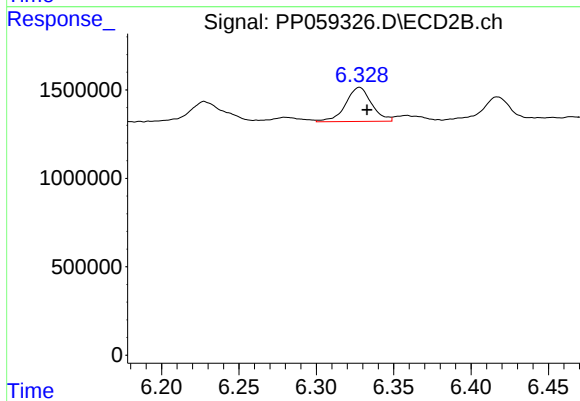

#29 AR-1254-4


R.T.: 6.328 min
Delta R.T.: -0.005 min
Response: 2253193
Conc: 28.03 ng/ml

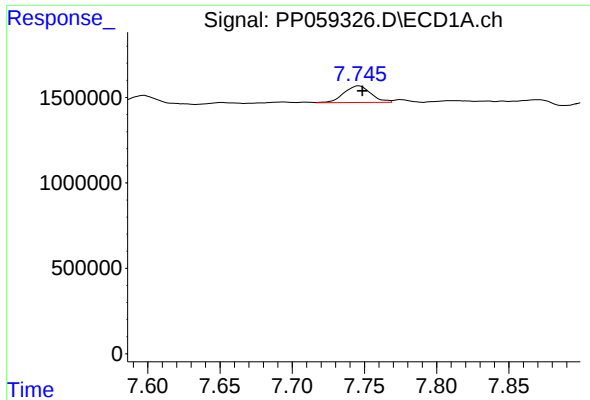

#30 AR-1254-5

R.T.: 7.745 min
Delta R.T.: -0.003 min
Response: 1263176
Conc: 26.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

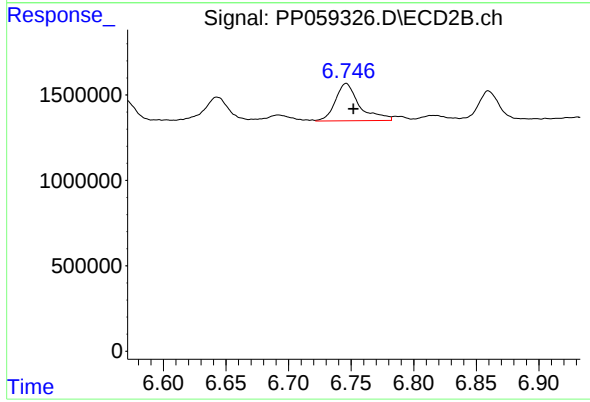

#30 AR-1254-5

R.T.: 6.746 min
Delta R.T.: -0.006 min
Response: 2939747
Conc: 24.58 ng/ml