

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081123\
 Data File : PP059327.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Aug 2023 12:14
 Operator : YP\AJ
 Sample : 03572-09
 Misc : AR1262 MDL 25 PPB
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT3-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 17:26:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 02:30:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.413	3.645	20403364	35551718	16.628	17.547
2) SA Decachlor...	10.204	8.679	16823436	31140298	22.042	22.135
Target Compounds						
36) L8 AR-1262-1	7.821	6.838	1651977	1172411	25.937	20.377
37) L8 AR-1262-2	8.368	7.044	2144730	2493060	23.354	21.128
38) L8 AR-1262-3	8.683	7.571	1539848	2186365	23.928m	25.692
39) L8 AR-1262-4	8.773	7.636	782590	3555582	23.567m	23.537
40) L8 AR-1262-5	9.437	8.133	667475	1712929	22.367	26.859



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081123\
Data File : PP059327.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Aug 2023 12:14
Operator : YP\AJ
Sample : 03572-09
Misc : AR1262 MDL 25 PPB
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 17:26:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 09 02:30:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

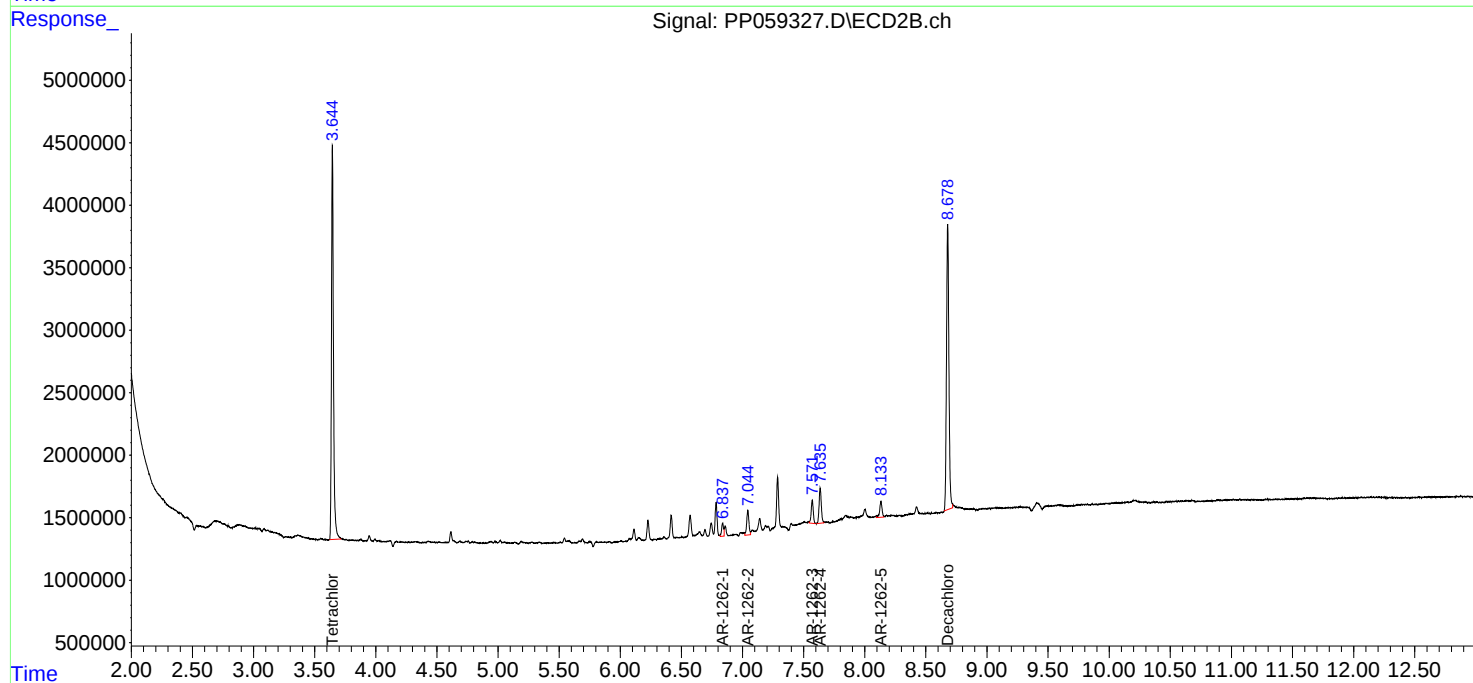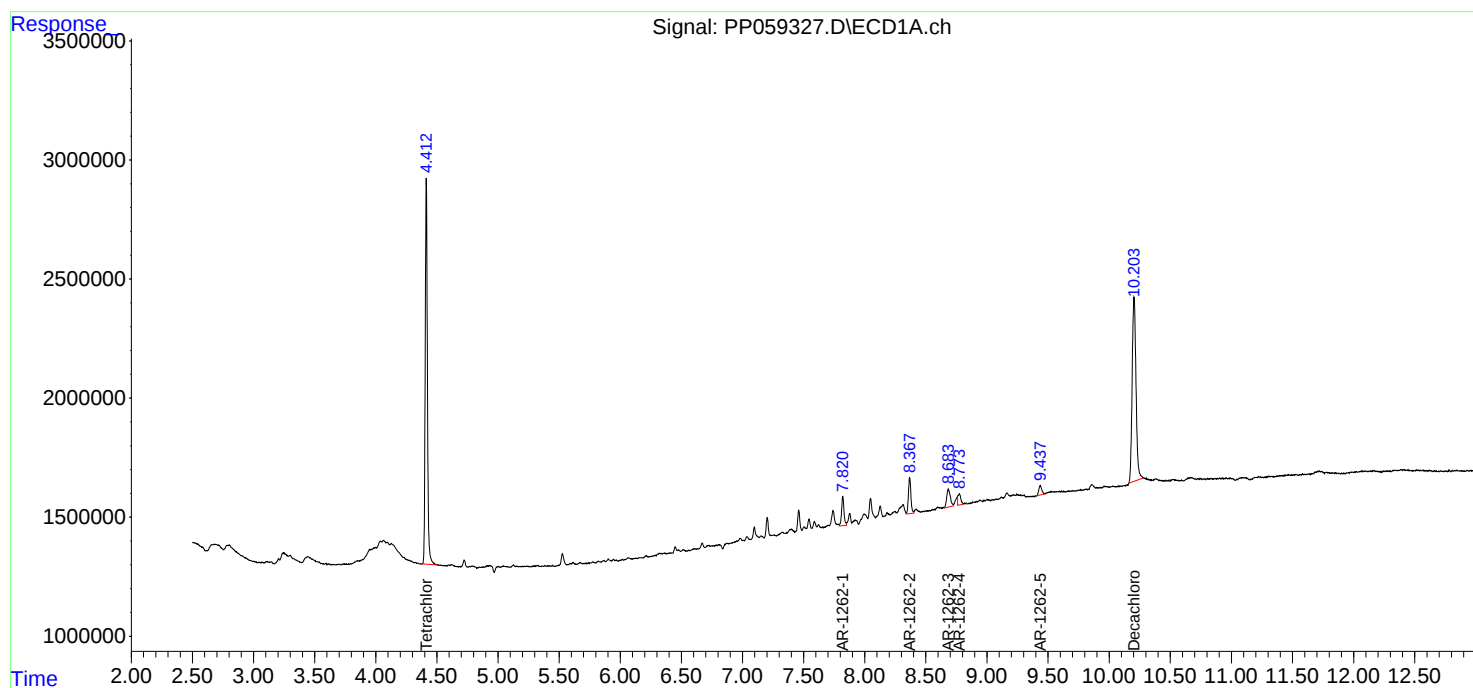


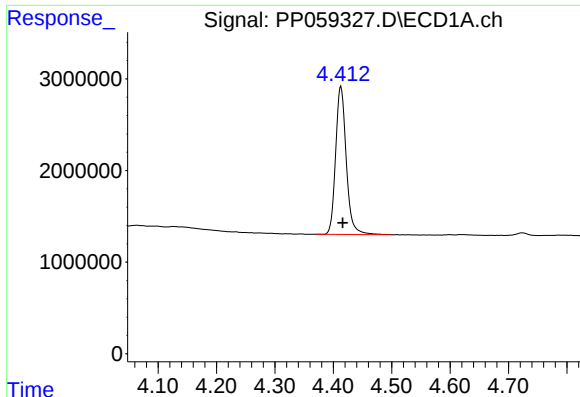

#1 Tetrachloro-m-xylene


R.T.: 4.413 min
Delta R.T.: -0.003 min
Response: 20403364
Conc: 16.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

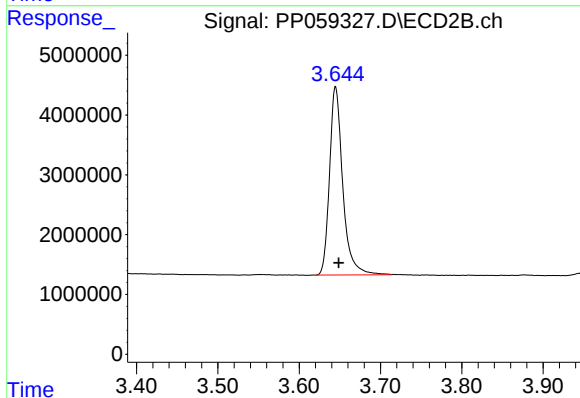


#1 Tetrachloro-m-xylene

R.T.: 3.645 min
Delta R.T.: -0.004 min
Response: 35551718
Conc: 17.55 ng/ml

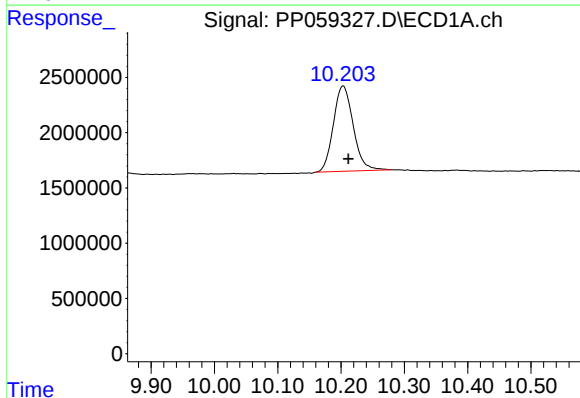


#2 Decachlorobiphenyl

R.T.: 10.204 min
Delta R.T.: -0.008 min
Response: 16823436
Conc: 22.04 ng/ml

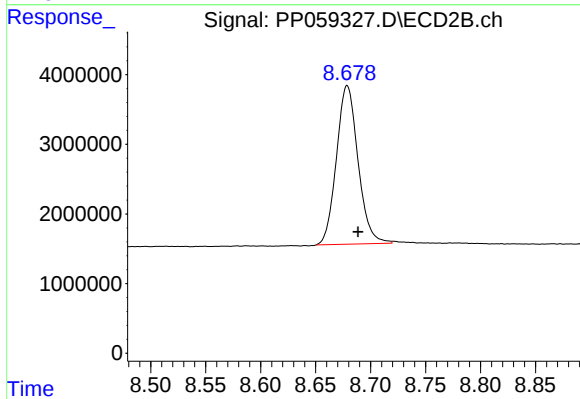

#2 Decachlorobiphenyl


R.T.: 8.679 min
Delta R.T.: -0.010 min
Response: 31140298
Conc: 22.14 ng/ml

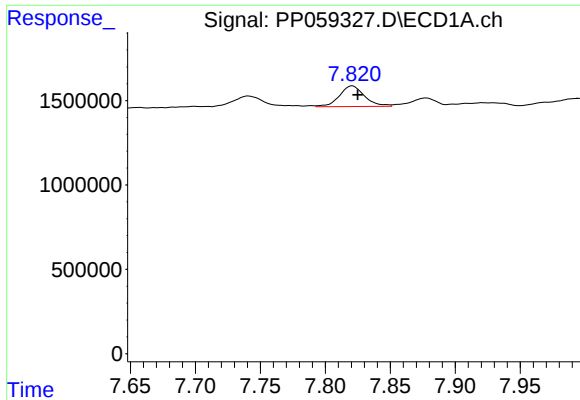

#36 AR-1262-1


R.T.: 7.821 min
Delta R.T.: -0.004 min
Response: 1651977
Conc: 25.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

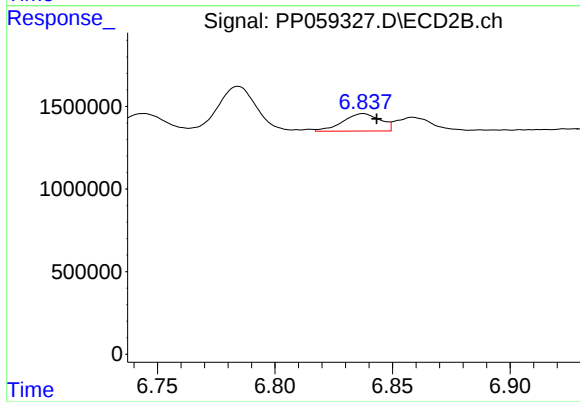


#36 AR-1262-1

R.T.: 6.838 min
Delta R.T.: -0.006 min
Response: 1172411
Conc: 20.38 ng/ml

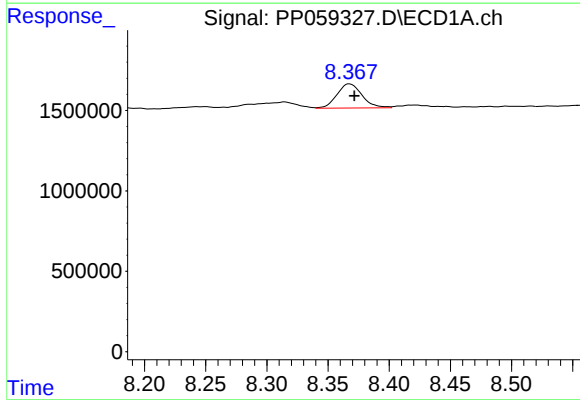


#37 AR-1262-2

R.T.: 8.368 min
Delta R.T.: -0.004 min
Response: 2144730
Conc: 23.35 ng/ml

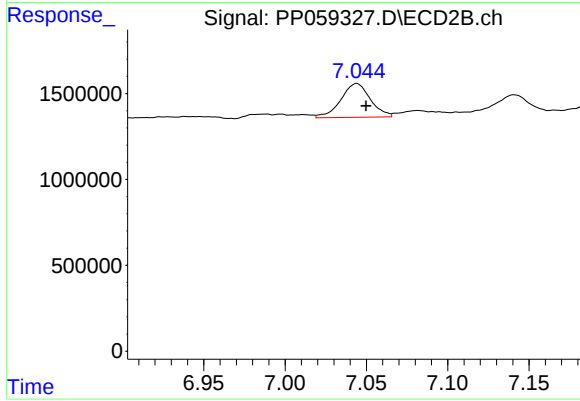

#37 AR-1262-2


R.T.: 7.044 min
Delta R.T.: -0.006 min
Response: 2493060
Conc: 21.13 ng/ml

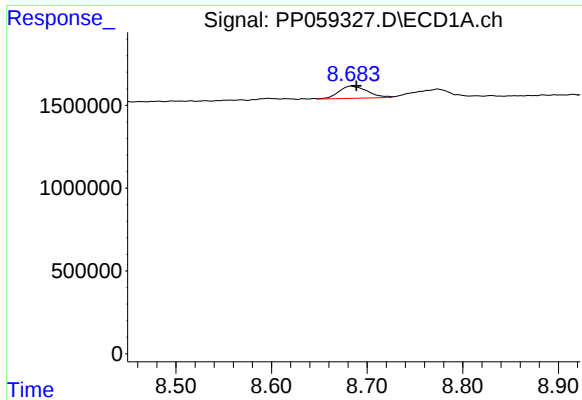

#38 AR-1262-3


R.T.: 8.683 min
Delta R.T.: -0.006 min
Response: 1539848
Conc: 23.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

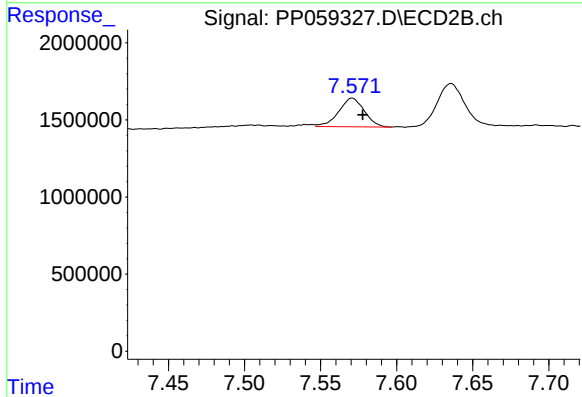


#38 AR-1262-3

R.T.: 7.571 min
Delta R.T.: -0.007 min
Response: 2186365
Conc: 25.69 ng/ml

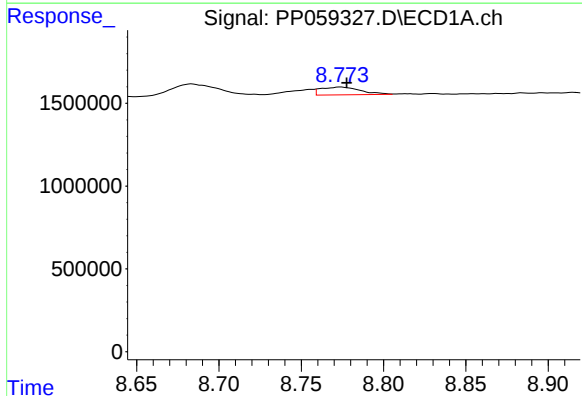


#39 AR-1262-4

R.T.: 8.773 min
Delta R.T.: -0.005 min
Response: 782590
Conc: 23.57 ng/ml m

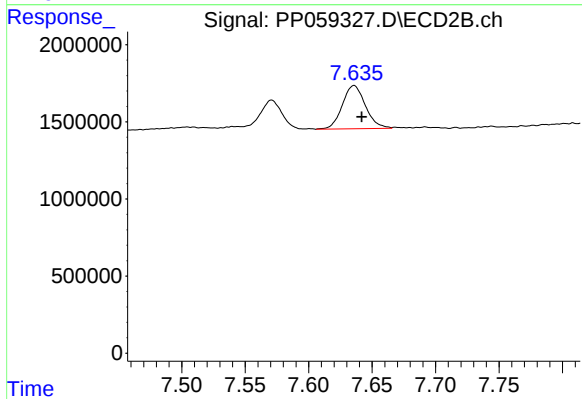

#39 AR-1262-4


R.T.: 7.636 min
Delta R.T.: -0.006 min
Response: 3555582
Conc: 23.54 ng/ml

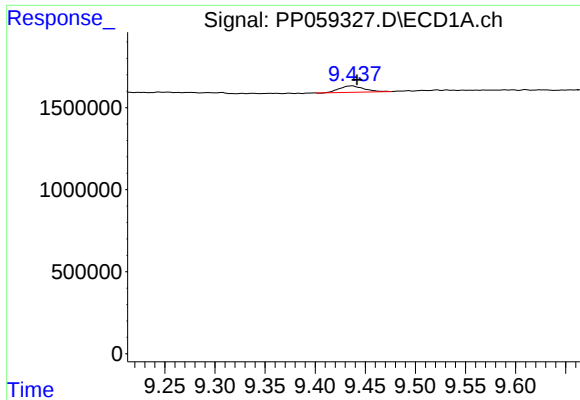

#40 AR-1262-5

R.T.: 9.437 min
Delta R.T.: -0.005 min
Response: 667475
Conc: 22.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

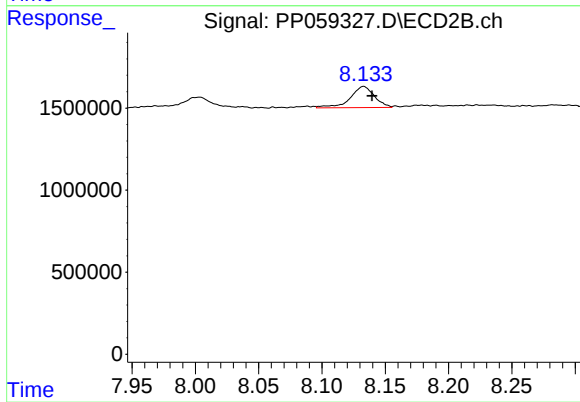

#40 AR-1262-5

R.T.: 8.133 min
Delta R.T.: -0.006 min
Response: 1712929
Conc: 26.86 ng/ml