

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081123\
 Data File : PP059328.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Aug 2023 12:30
 Operator : YP\AJ
 Sample : 03572-09
 Misc : AR1268 MDL 25 PPB
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT3-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 17:27:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 02:30:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.414	3.662	20256189	35327886	16.508	17.436
2) SA Decachlor...	10.203	8.696	17946543	32914036	23.514	23.396
Target Compounds						
41) L9 AR-1268-1	8.682	7.589	2607015	6108186	22.956	25.049
42) L9 AR-1268-2	8.776	7.653	2349583	5063126	23.874	23.117
43) L9 AR-1268-3	9.007	7.860	2177570	4637970	23.489	23.720
44) L9 AR-1268-4	9.436	8.149	785378	1739896	24.619	25.002
45) L9 AR-1268-5	9.860	8.441	6353069	12096609	23.403	23.334



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081123\
Data File : PP059328.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Aug 2023 12:30
Operator : YP\AJ
Sample : 03572-09
Misc : AR1268 MDL 25 PPB
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 17:27:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 09 02:30:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

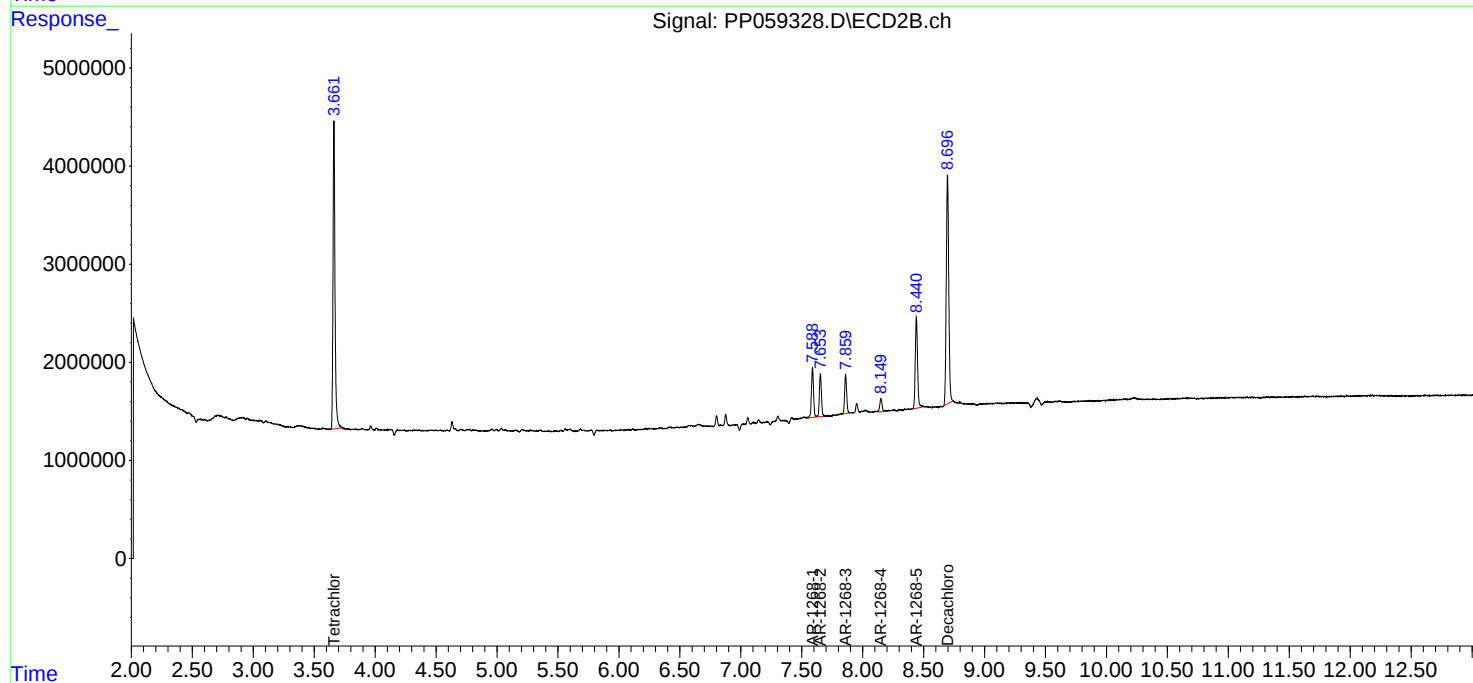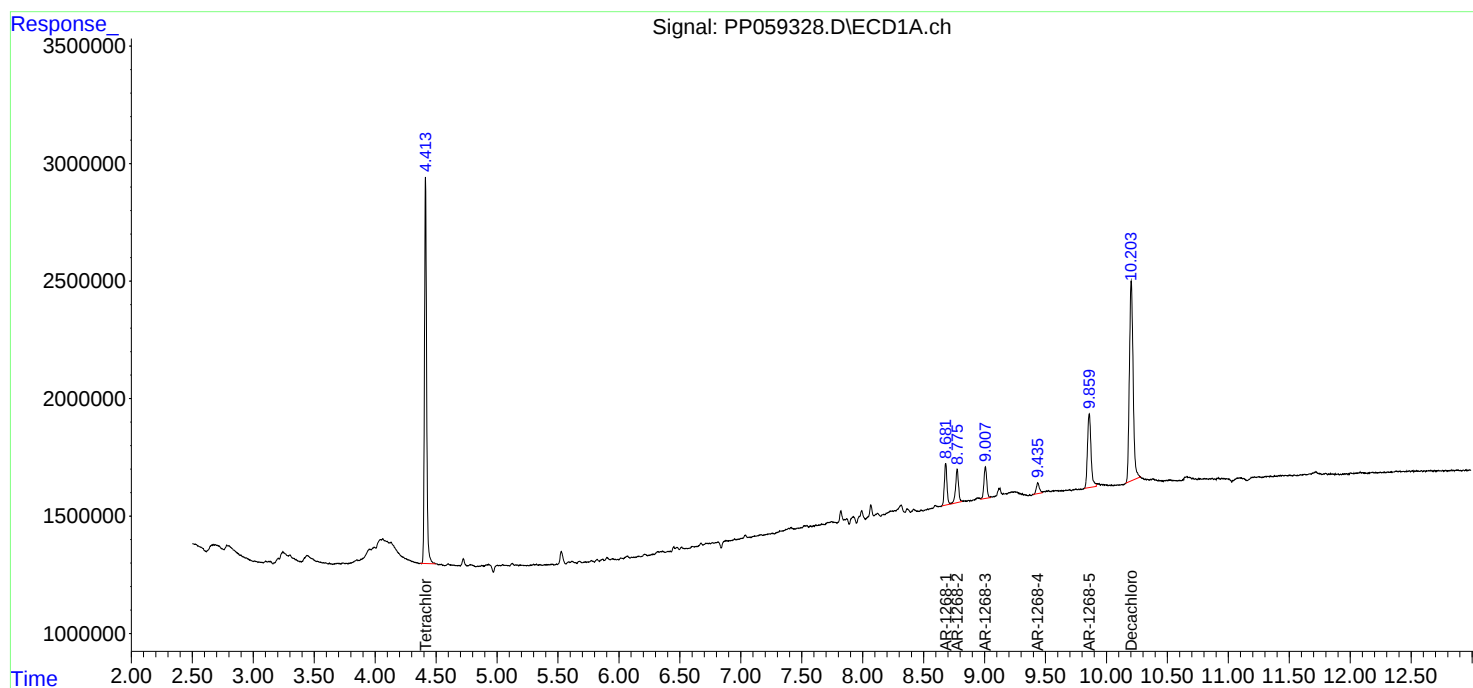


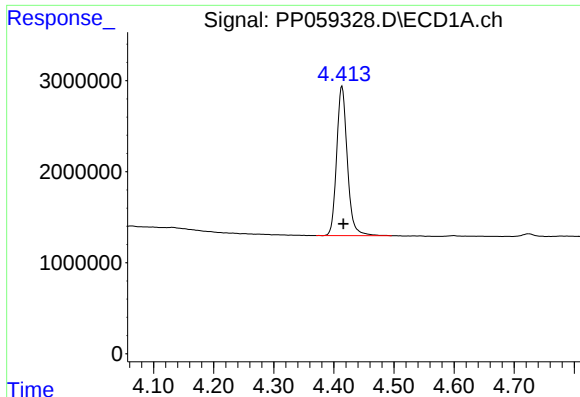

#1 Tetrachloro-m-xylene


R.T.: 4.414 min
Delta R.T.: -0.002 min
Response: 20256189
Conc: 16.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

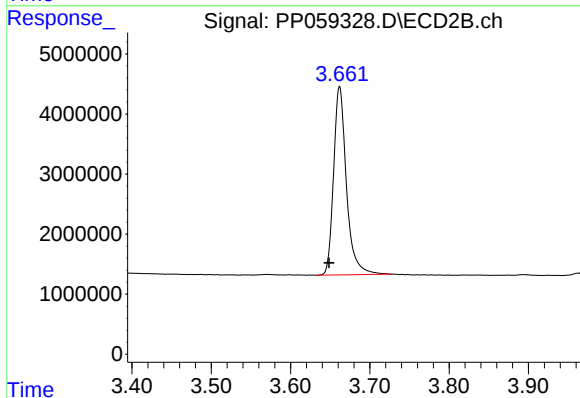


#1 Tetrachloro-m-xylene

R.T.: 3.662 min
Delta R.T.: 0.013 min
Response: 35327886
Conc: 17.44 ng/ml

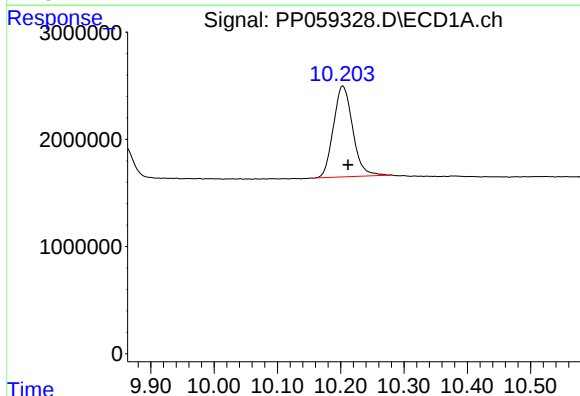


#2 Decachlorobiphenyl

R.T.: 10.203 min
Delta R.T.: -0.008 min
Response: 17946543
Conc: 23.51 ng/ml

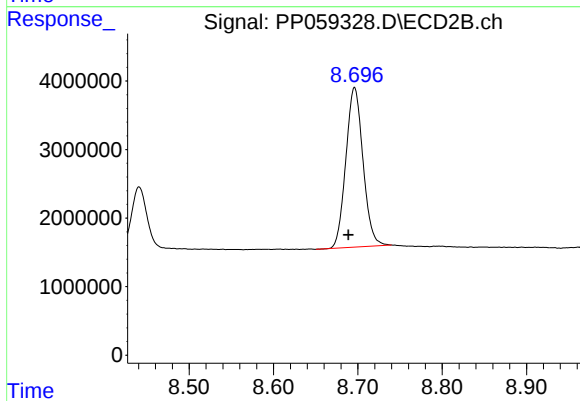

#2 Decachlorobiphenyl


R.T.: 8.696 min
Delta R.T.: 0.008 min
Response: 32914036
Conc: 23.40 ng/ml

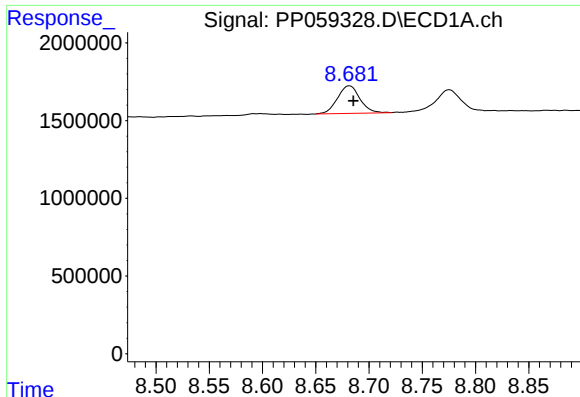

#41 AR-1268-1


R.T.: 8.682 min
Delta R.T.: -0.004 min
Response: 2607015
Conc: 22.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

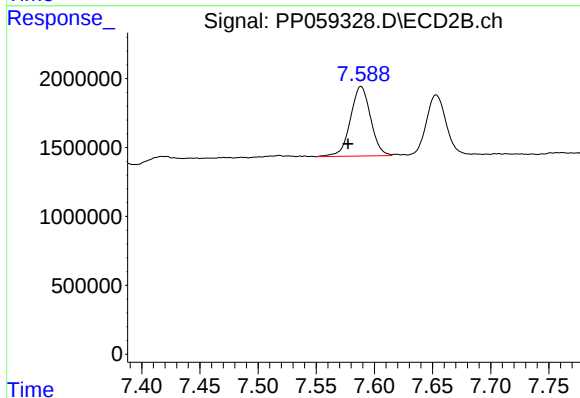


#41 AR-1268-1

R.T.: 7.589 min
Delta R.T.: 0.011 min
Response: 6108186
Conc: 25.05 ng/ml

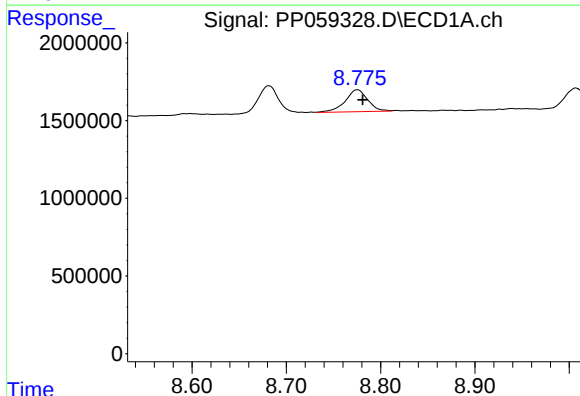


#42 AR-1268-2

R.T.: 8.776 min
Delta R.T.: -0.005 min
Response: 2349583
Conc: 23.87 ng/ml

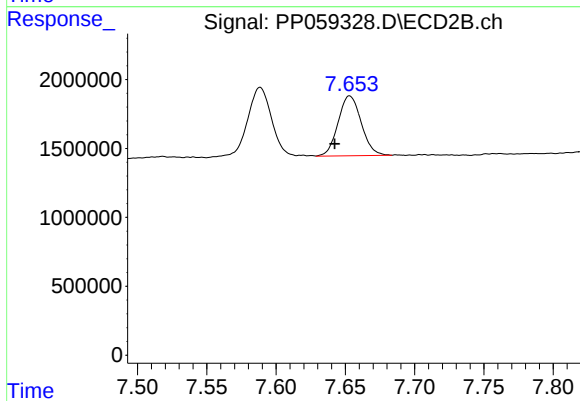

#42 AR-1268-2


R.T.: 7.653 min
Delta R.T.: 0.011 min
Response: 5063126
Conc: 23.12 ng/ml

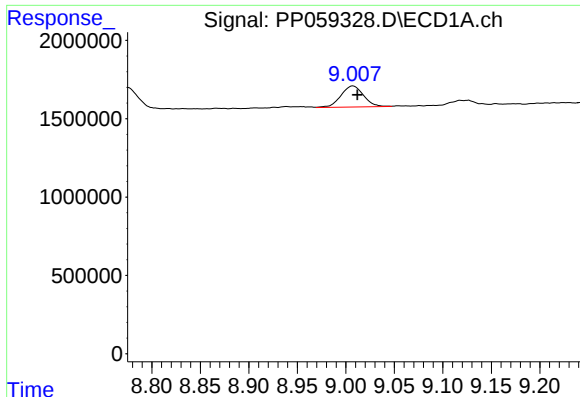

#43 AR-1268-3


R.T.: 9.007 min
Delta R.T.: -0.005 min
Response: 2177570
Conc: 23.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

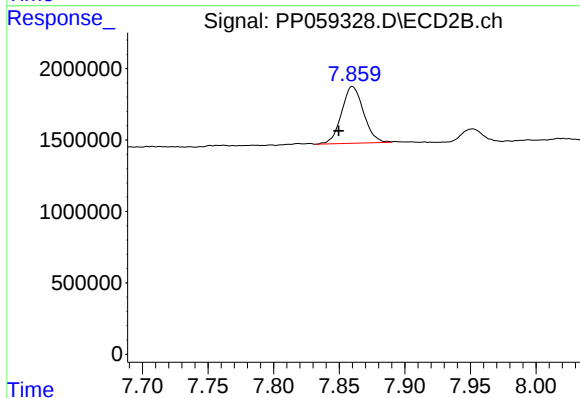


#43 AR-1268-3

R.T.: 7.860 min
Delta R.T.: 0.010 min
Response: 4637970
Conc: 23.72 ng/ml

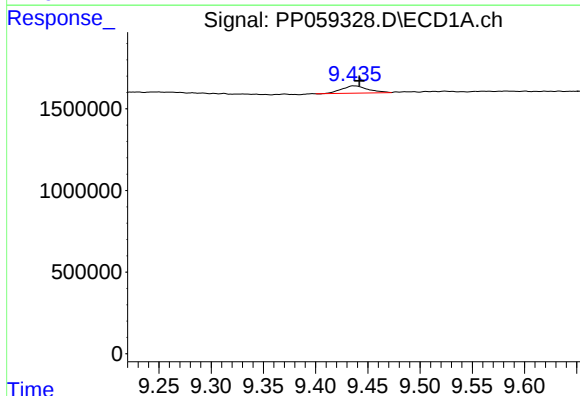


#44 AR-1268-4

R.T.: 9.436 min
Delta R.T.: -0.005 min
Response: 785378
Conc: 24.62 ng/ml

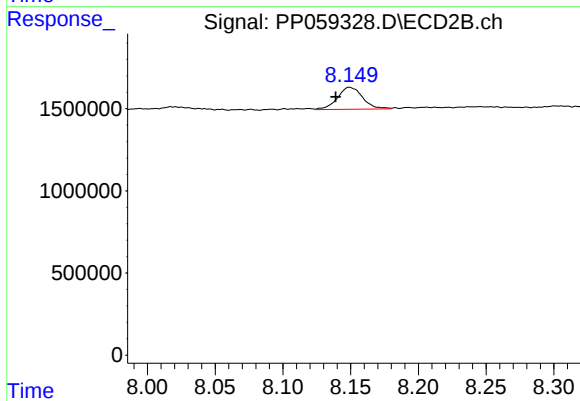

#44 AR-1268-4


R.T.: 8.149 min
Delta R.T.: 0.010 min
Response: 1739896
Conc: 25.00 ng/ml

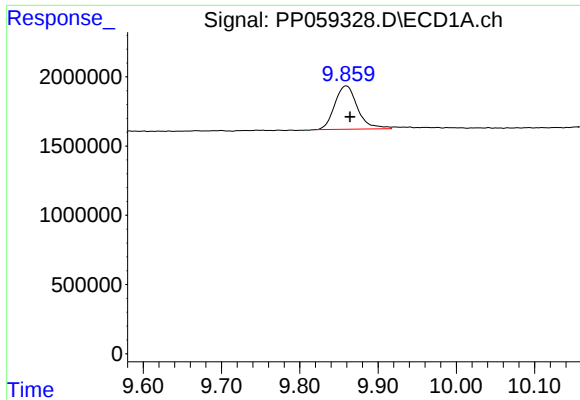

#45 AR-1268-5

R.T.: 9.860 min
Delta R.T.: -0.005 min
Response: 6353069
Conc: 23.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

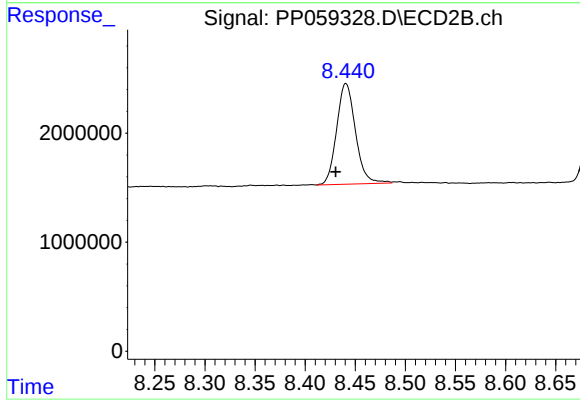

#45 AR-1268-5

R.T.: 8.441 min
Delta R.T.: 0.010 min
Response: 12096609
Conc: 23.33 ng/ml