

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090821\
 Data File : PD065617.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2021 09:57
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 07:08:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 04 01:23:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.494	4.013	19234501	167.6E6	19.627	22.867
28)	SA Decachlor...	8.238	9.085	34124777	117.5E6	19.793	22.028
Target Compounds							
15)	B Endosulfa...	0.000	6.947	0	1787412	N.D.	0.279 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090821\
Data File : PD065617.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2021 09:57
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 07:08:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
Quant Title : GC Extractables
QLast Update : Sat Sep 04 01:23:47 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

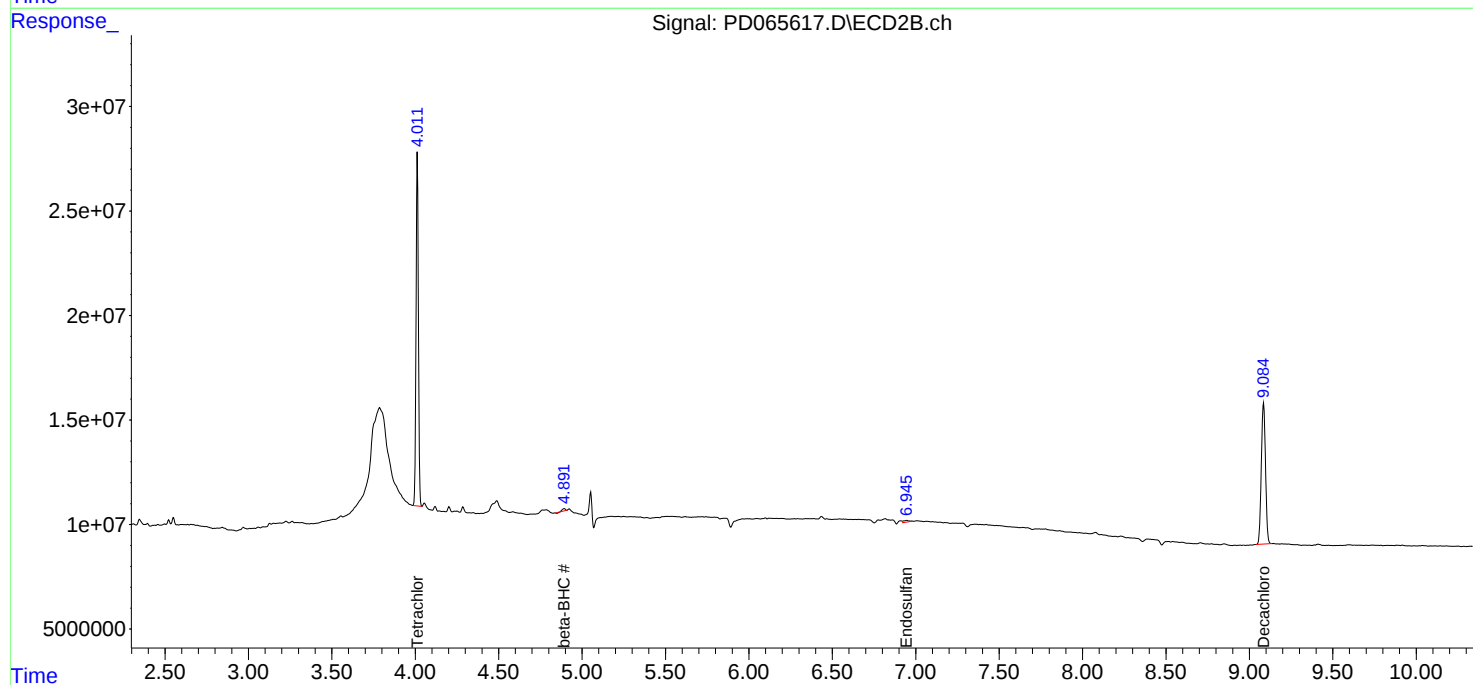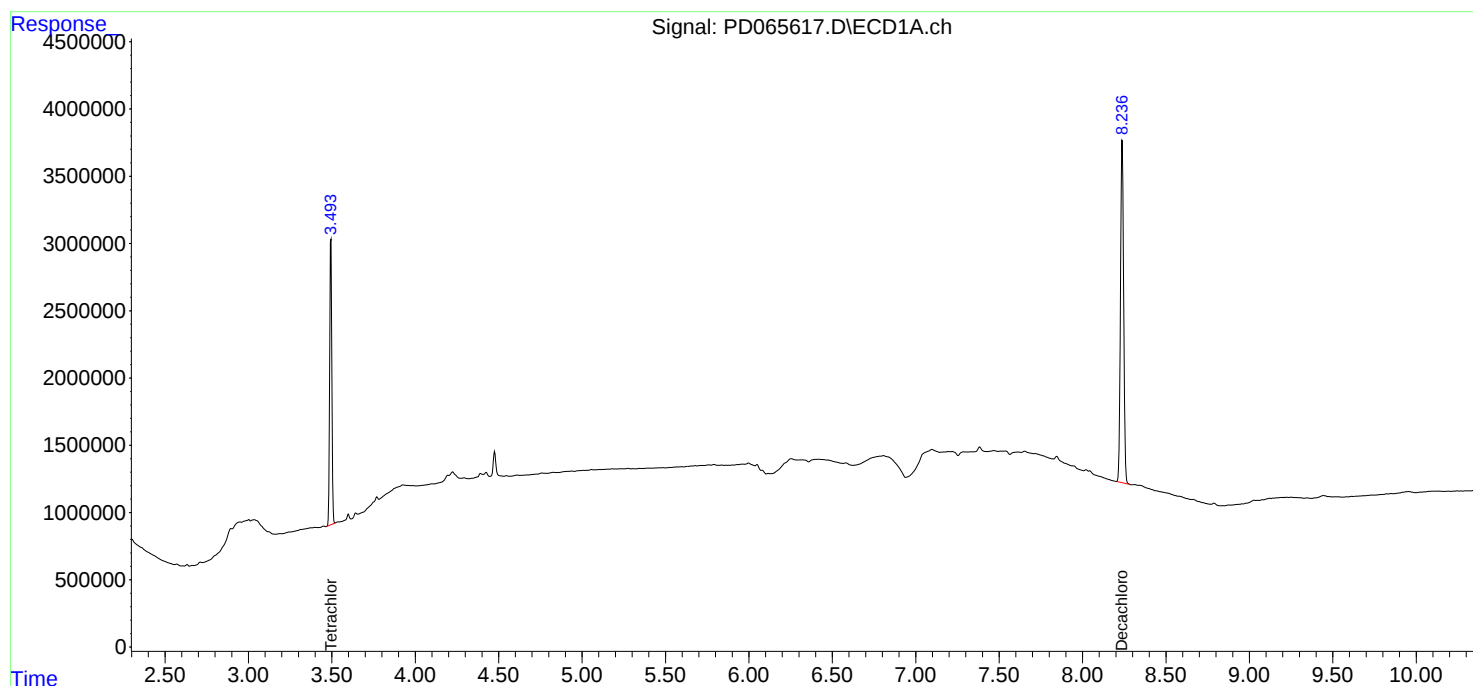


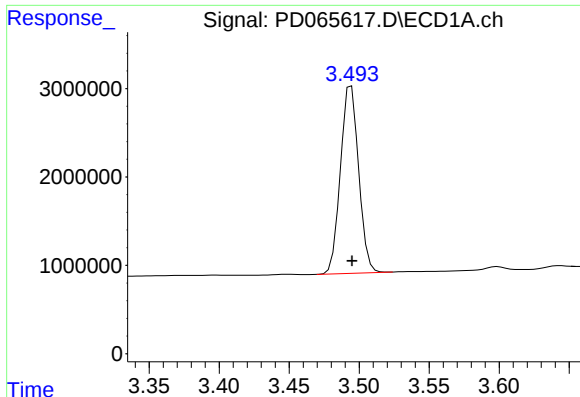

#1 Tetrachloro-m-xylene


R.T.: 3.494 min
Delta R.T.: 0.000 min
Response: 19234501
Conc: 19.63 ng/ml

Instrument :
ECD_P
ClientSampleId :

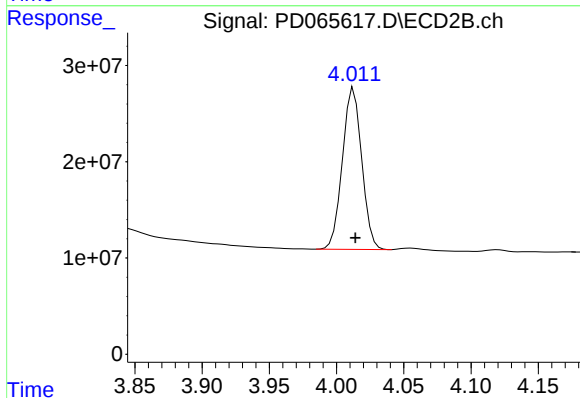


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: -0.001 min
Response: 167602967
Conc: 22.87 ng/ml

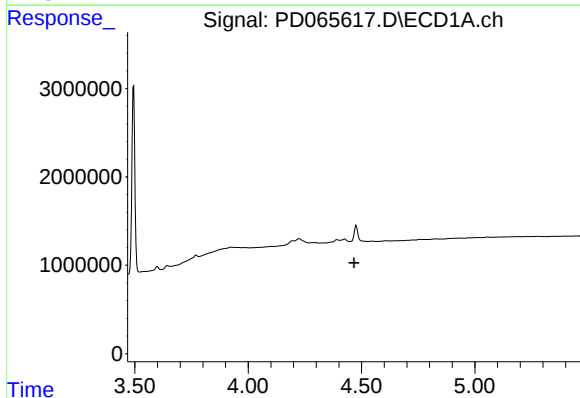


#6 beta-BHC

R.T.: 4.476 min
Delta R.T.: 0.008 min
Response: 2189617
Conc: N.D.

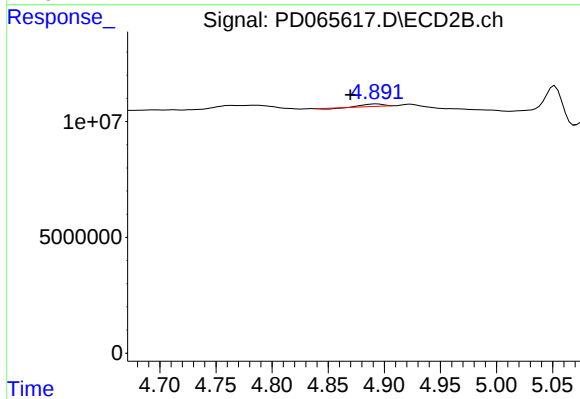

#6 beta-BHC


R.T.: 4.893 min
Delta R.T.: 0.023 min
Response: 1312030
Conc: 0.28 ng/ml

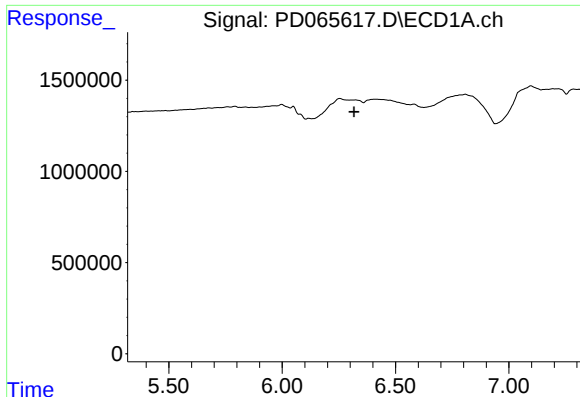

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.318 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

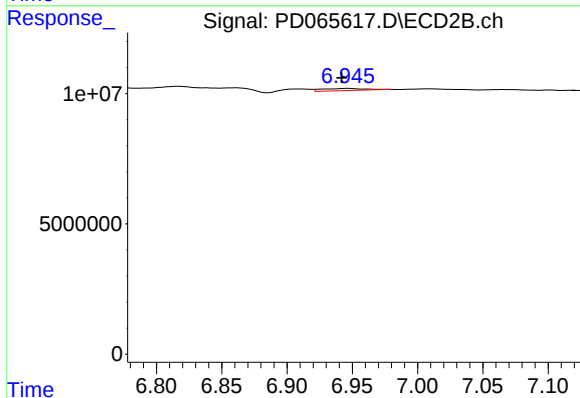


#15 Endosulfan II

R.T.: 6.947 min
Delta R.T.: 0.005 min
Response: 1787412
Conc: 0.28 ng/ml

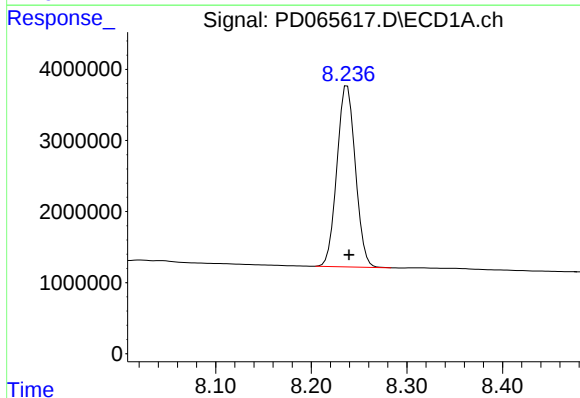

#28 Decachlorobiphenyl

R.T.: 8.238 min
Delta R.T.: -0.002 min
Response: 34124777
Conc: 19.79 ng/ml

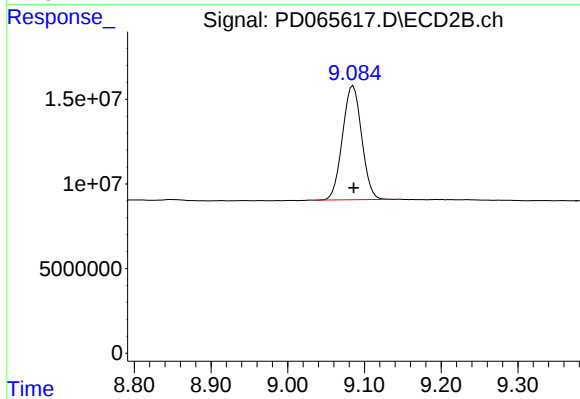

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: 0.000 min
Response: 117542450
Conc: 22.03 ng/ml