

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090821\
 Data File : PD065624.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2021 13:12
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 07:10:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 04 01:23:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.013	18196030	156.0E6	18.567	21.284
28)	SA Decachlor...	8.244	9.088	25295782	90319434	14.672	16.926
Target Compounds							
4)	MA Heptachlor	0.000	5.211	0	5394726	N.D.	0.593 #
5)	MB Aldrin	0.000	5.522f	0	969925	N.D.	0.115 #
15)	B Endosulfa...	0.000	6.932	0	10774205	N.D.	1.681 #
17)	MA 4,4'-DDT	0.000	7.158	0	5791489	N.D.	0.951 #
19)	B Endosulfa...	0.000	7.278	0	965168	N.D.	0.151 #
21)	B Endrin ke...	0.000	7.774	0	3782316	N.D.	0.500 #
22)	Mirex	7.389	0.000	507065	0	0.323	N.D. #
27)	Chlordane-5	0.000	7.000	0	2595634	N.D.	11.068 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090821\
Data File : PD065624.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2021 13:12
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 07:10:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
Quant Title : GC Extractables
QLast Update : Sat Sep 04 01:23:47 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

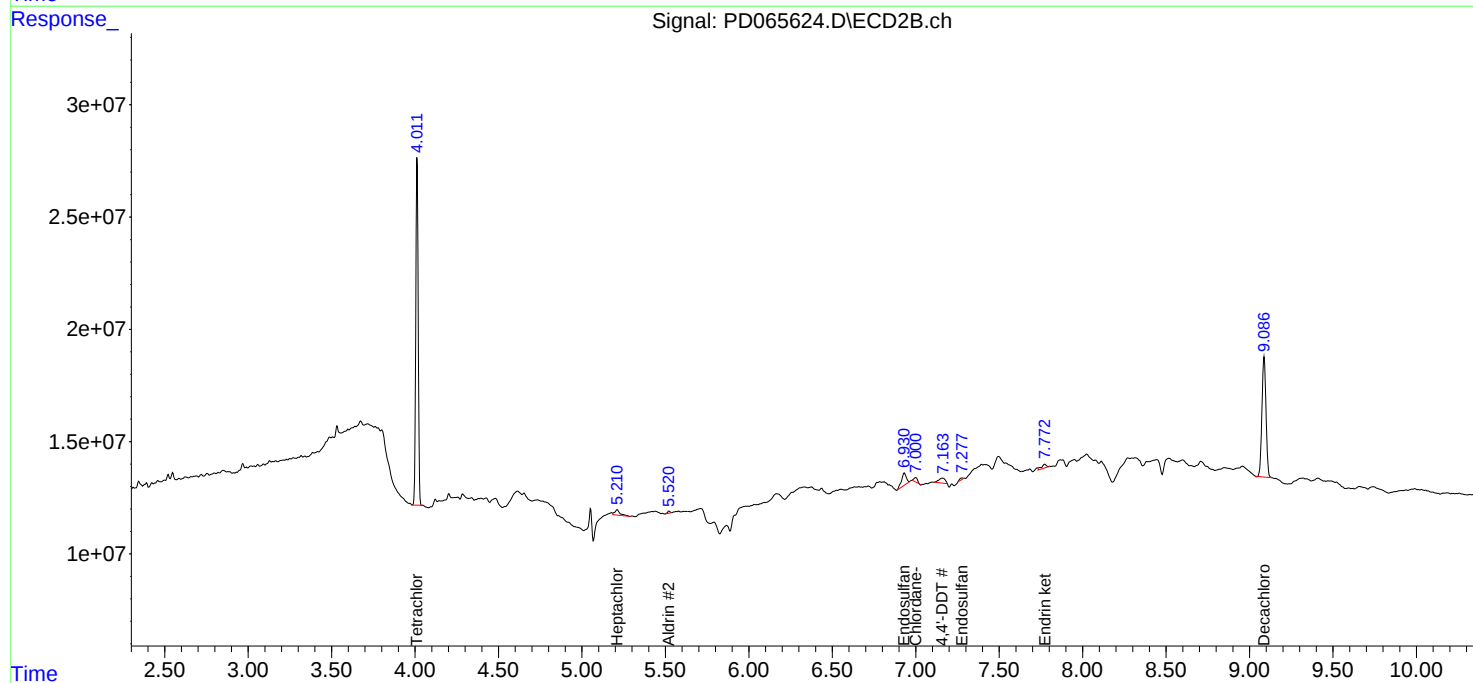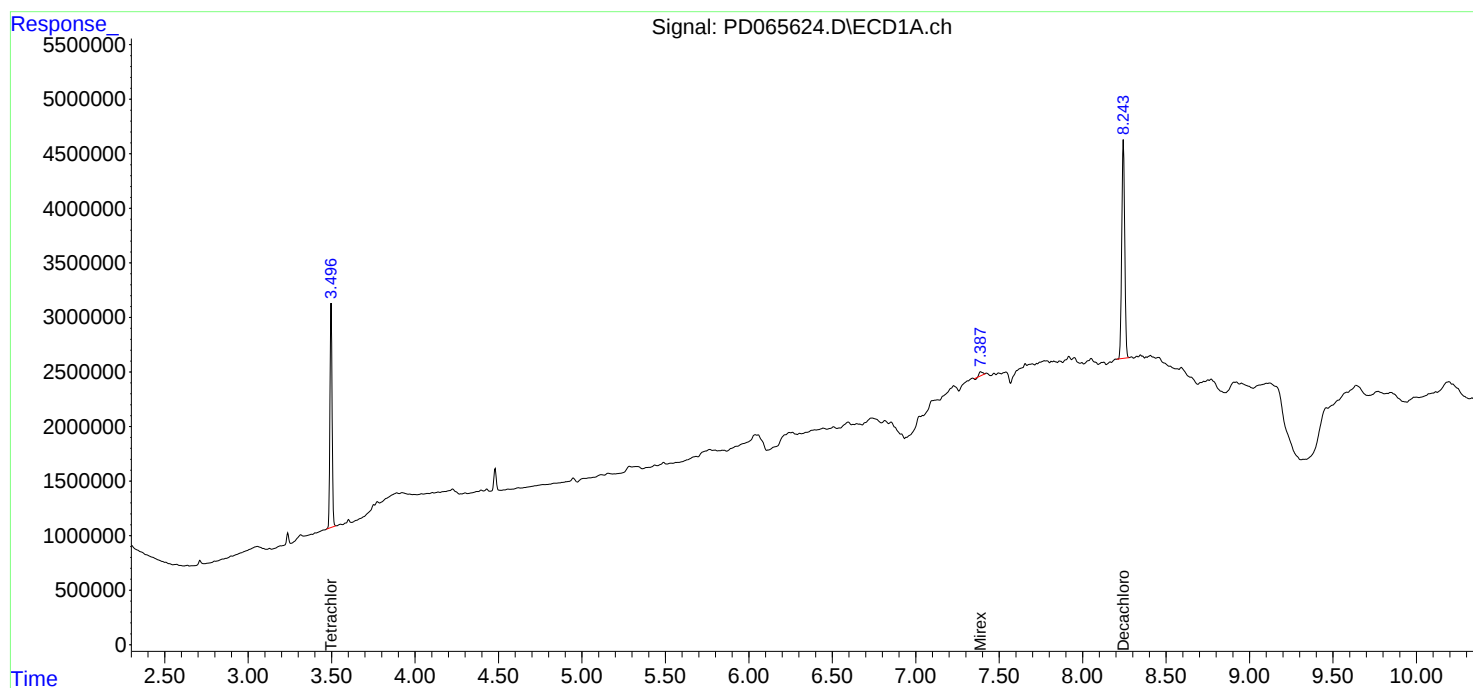


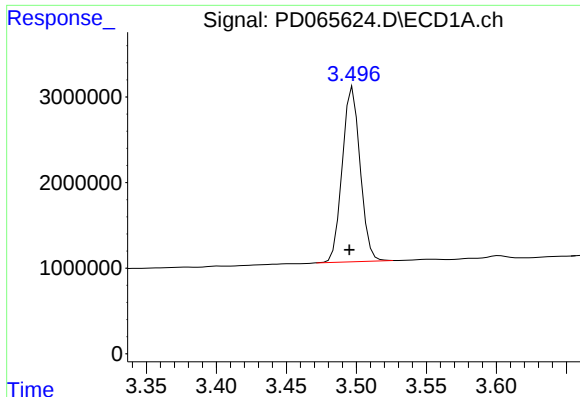

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.002 min
Response: 18196030
Conc: 18.57 ng/ml

Instrument :
ECD_P
ClientSampleId :

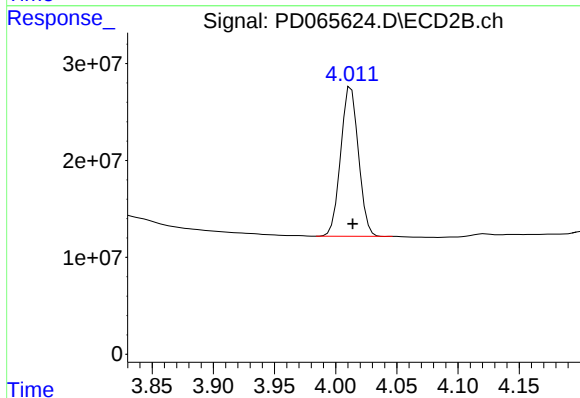


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: -0.001 min
Response: 155995726
Conc: 21.28 ng/ml

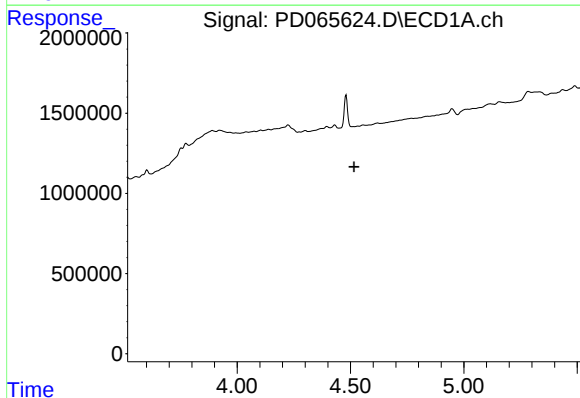


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.516 min
Response: 0
Conc: N.D.

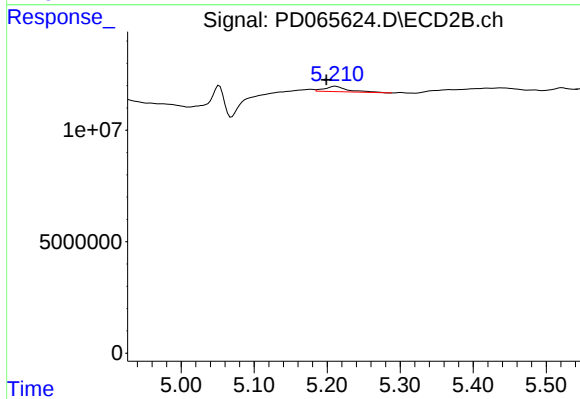

#4 Heptachlor


R.T.: 5.211 min
Delta R.T.: 0.013 min
Response: 5394726
Conc: 0.59 ng/ml

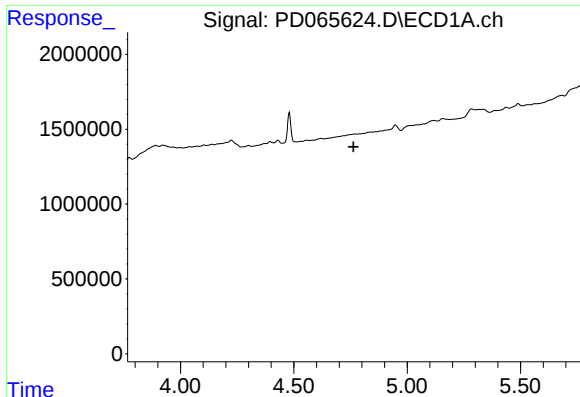

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.764 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

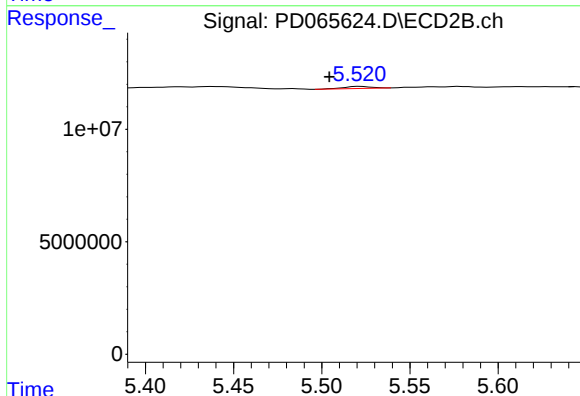


#5 Aldrin

R.T.: 5.522 min
Delta R.T.: 0.018 min
Response: 969925
Conc: 0.11 ng/ml

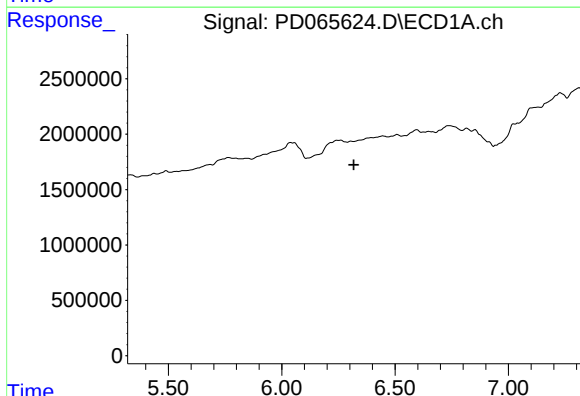


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.318 min
Response: 0
Conc: N.D.

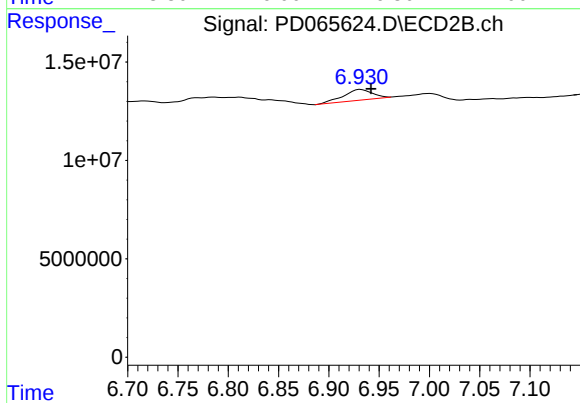

#15 Endosulfan II


R.T.: 6.932 min
Delta R.T.: -0.010 min
Response: 10774205
Conc: 1.68 ng/ml

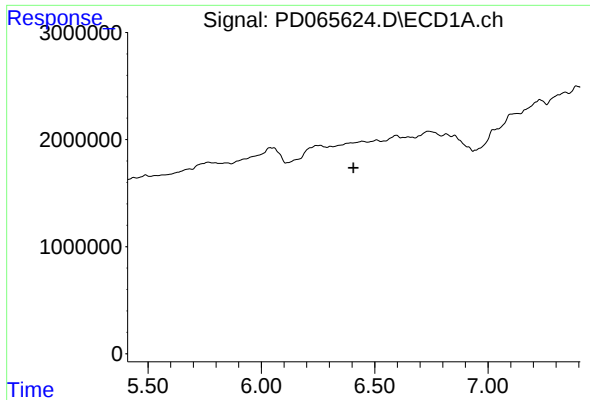

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.407 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

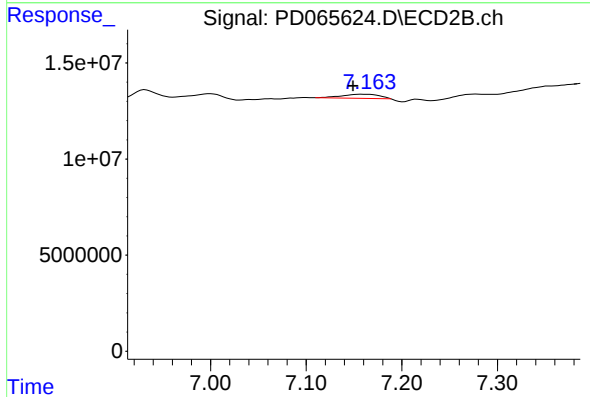


#17 4,4'-DDT

R.T.: 7.158 min
Delta R.T.: 0.008 min
Response: 5791489
Conc: 0.95 ng/ml

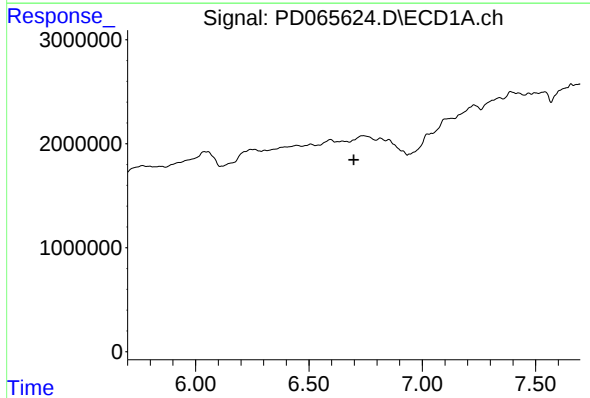


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 6.698 min
Response: 0
Conc: N.D.

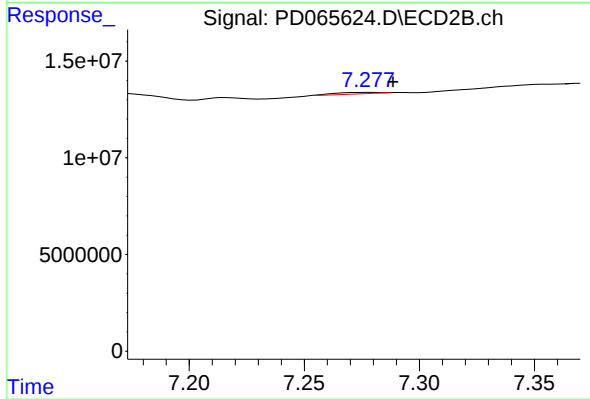

#19 Endosulfan Sulfate


R.T.: 7.278 min
Delta R.T.: -0.010 min
Response: 965168
Conc: 0.15 ng/ml

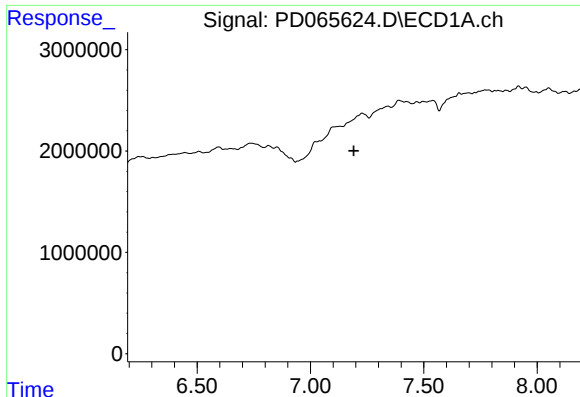

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.192 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

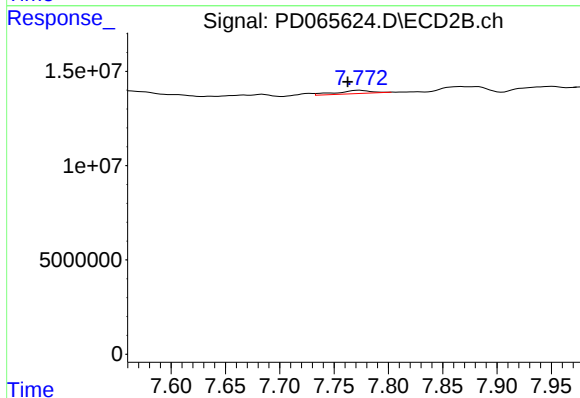


#21 Endrin ketone

R.T.: 7.774 min
Delta R.T.: 0.011 min
Response: 3782316
Conc: 0.50 ng/ml

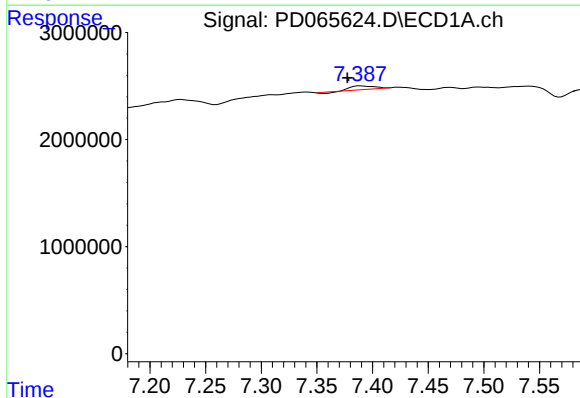


#22 Mirex

R.T.: 7.389 min
Delta R.T.: 0.012 min
Response: 507065
Conc: 0.32 ng/ml

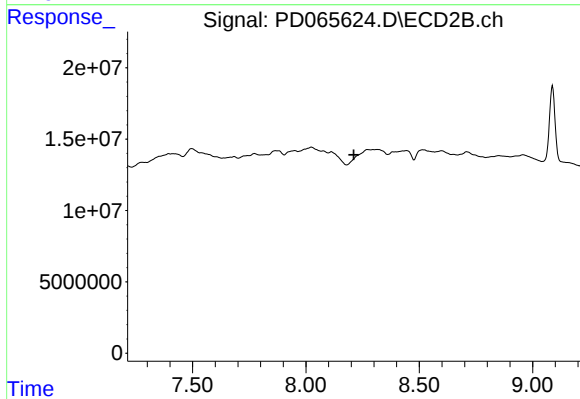

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 8.211 min
Response: 0
Conc: N.D.

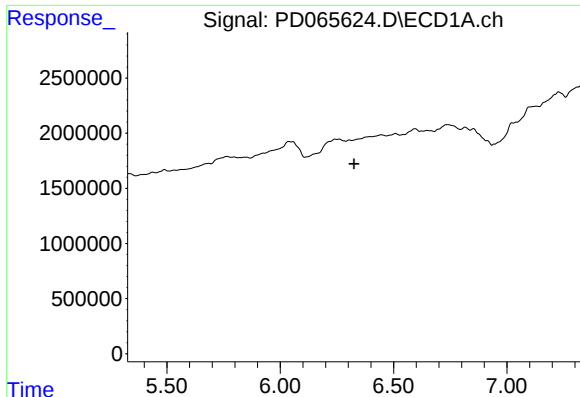

#27 Chlorodane-5


R.T.: 0.000 min
Exp R.T.: 6.326 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

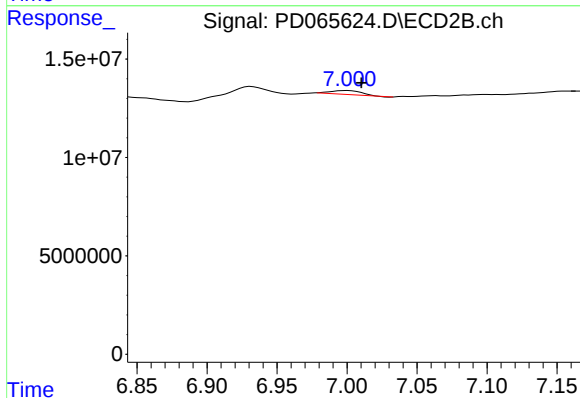


#27 Chlorodane-5

R.T.: 7.000 min
Delta R.T.: -0.010 min
Response: 2595634
Conc: 11.07 ng/ml

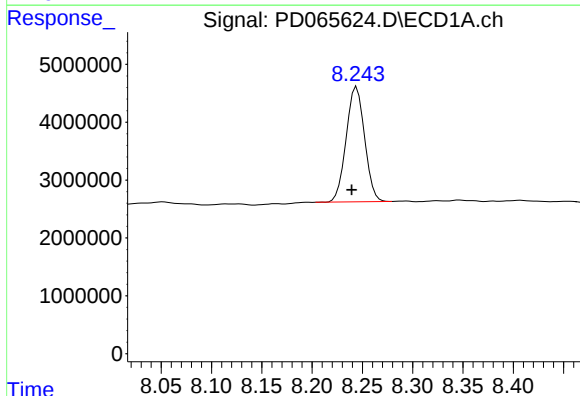

#28 Decachlorobiphenyl

R.T.: 8.244 min
Delta R.T.: 0.005 min
Response: 25295782
Conc: 14.67 ng/ml

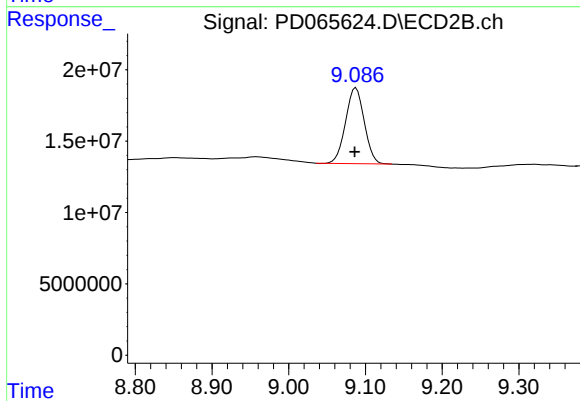

#28 Decachlorobiphenyl

R.T.: 9.088 min
Delta R.T.: 0.002 min
Response: 90319434
Conc: 16.93 ng/ml