

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090821\
 Data File : PL069763.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2021 15:14
 Operator : AR\AJ
 Sample : PIBLK203
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 08:07:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 08 10:30:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.633	5.566	8429232	27784545	19.830	20.420
27)	SA Decachlor...	10.400	11.491	28890017	48556548	37.983	41.442
Target Compounds							
2)	A alpha-BHC	5.332	0.000	3247455	0	5.565	N.D. #
4)	MA Heptachlor	0.000	7.228f	0	2365671	N.D.	1.360
6)	B beta-BHC	0.000	6.833f	0	20452186	N.D.	20.493
7)	B delta-BHC	0.000	7.084	0	531918	N.D.	0.298
8)	B Heptachlo...	0.000	8.038	0	60452	N.D.	<MDL
14)	MA Endrin	0.000	8.913f	0	228784	N.D.	0.187
15)	B Endosulfa...	8.300f	0.000	1010766	0	1.640	N.D. #
16)	A 4,4'-DDD	0.000	9.071f	0	2102259	N.D.	1.798
20)	A Methoxychlor	0.000	9.848f	0	179089	N.D.	0.285
21)	B Endrin ke...	0.000	10.092	0	758300	N.D.	0.592


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090821\
Data File : PL069763.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2021 15:14
Operator : AR\AJ
Sample : PIBLK203
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 08:07:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 08 10:30:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

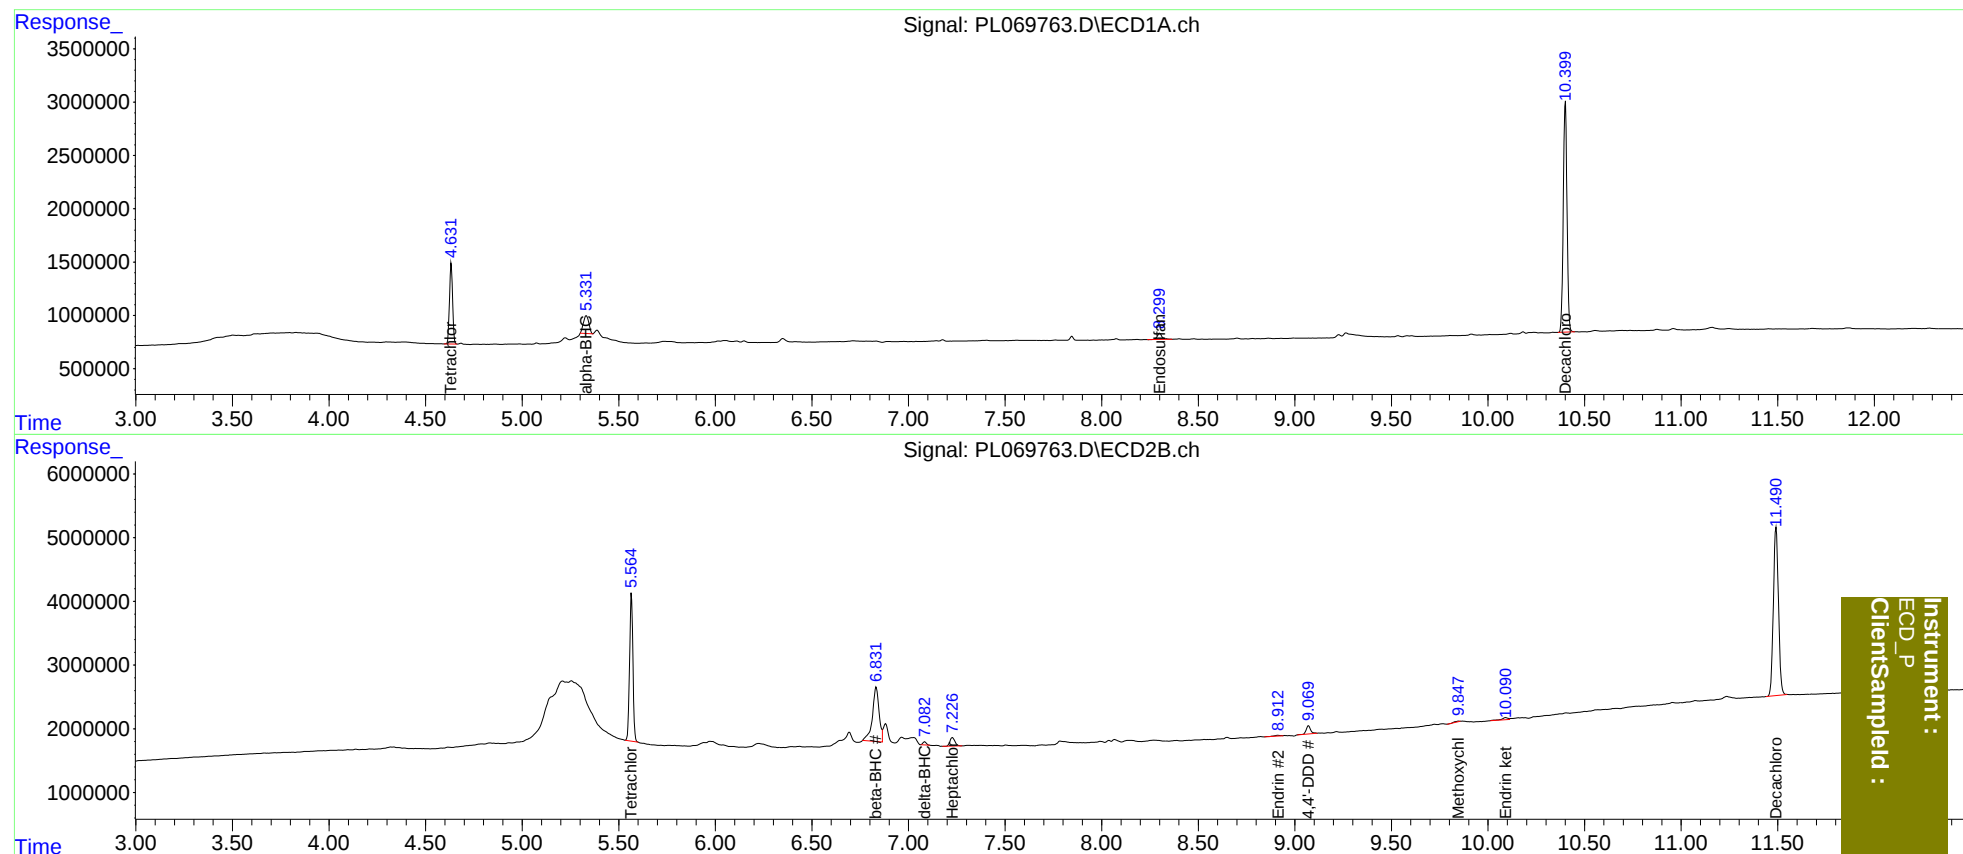


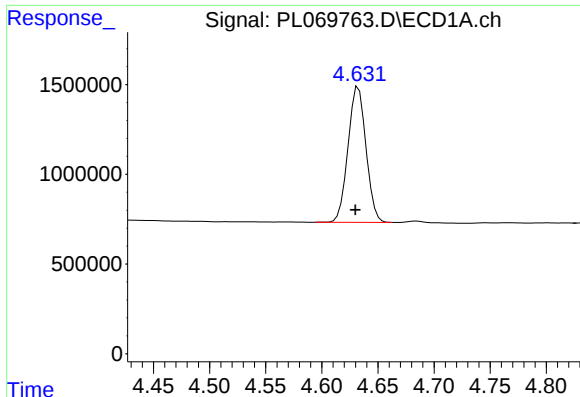

#1 Tetrachloro-m-xylene


R.T.: 4.633 min
Delta R.T.: 0.003 min
Response: 8429232
Conc: 19.83 ng/ml

Instrument :
ECD_P
ClientSampleId :

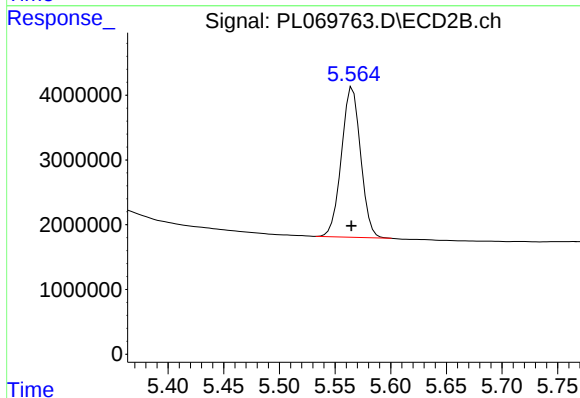


#1 Tetrachloro-m-xylene

R.T.: 5.566 min
Delta R.T.: 0.001 min
Response: 27784545
Conc: 20.42 ng/ml

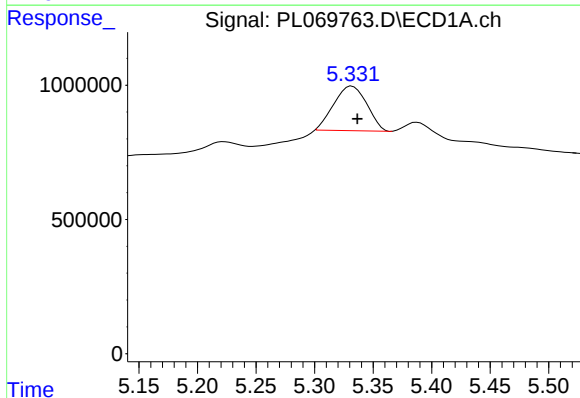


#2 alpha-BHC

R.T.: 5.332 min
Delta R.T.: -0.005 min
Response: 3247455
Conc: 5.56 ng/ml

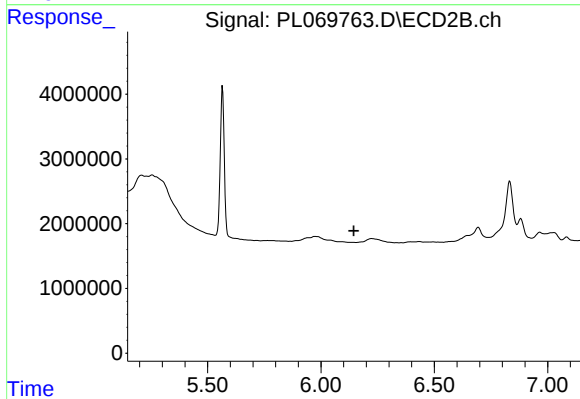

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.145 min
Response: 0
Conc: N.D.

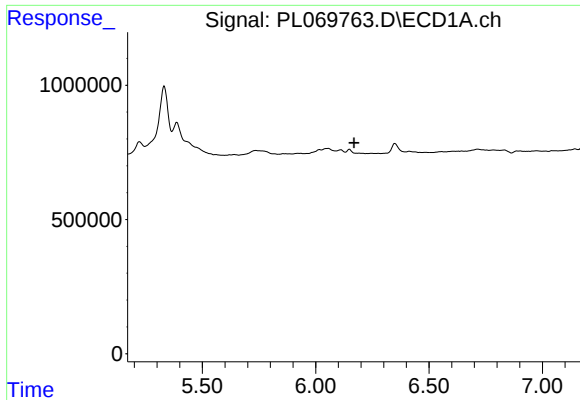

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 6.169 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

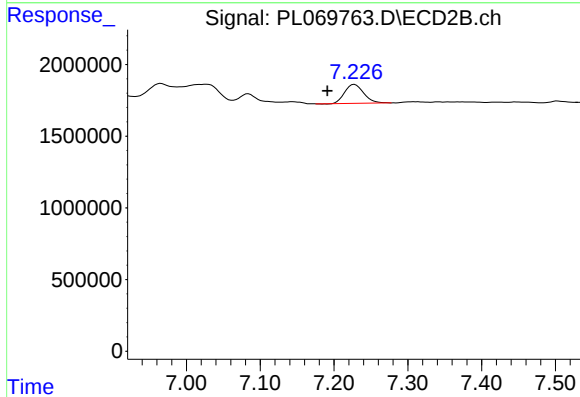


#4 Heptachlor

R.T.: 7.228 min
Delta R.T.: 0.036 min
Response: 2365671
Conc: 1.36 ng/ml

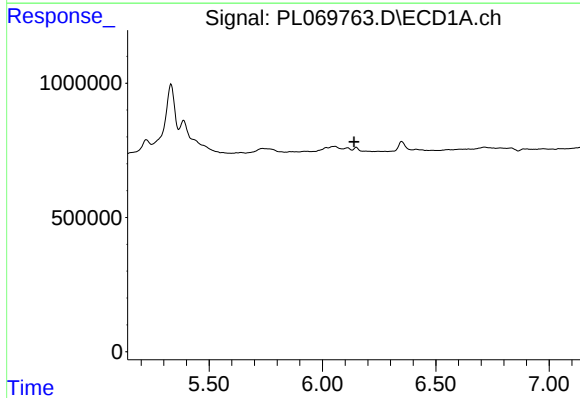


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 6.139 min
Response: 0
Conc: N.D.

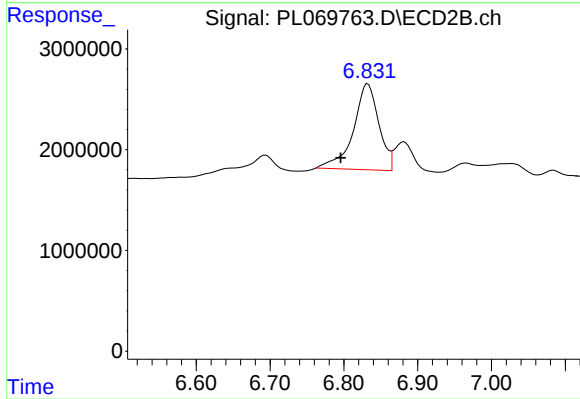

#6 beta-BHC


R.T.: 6.833 min
Delta R.T.: 0.037 min
Response: 20452186
Conc: 20.49 ng/ml

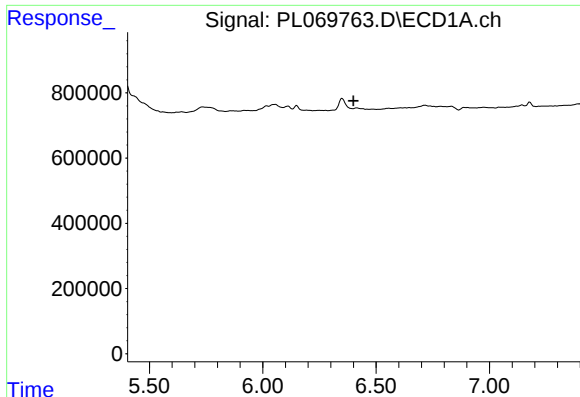

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.400 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

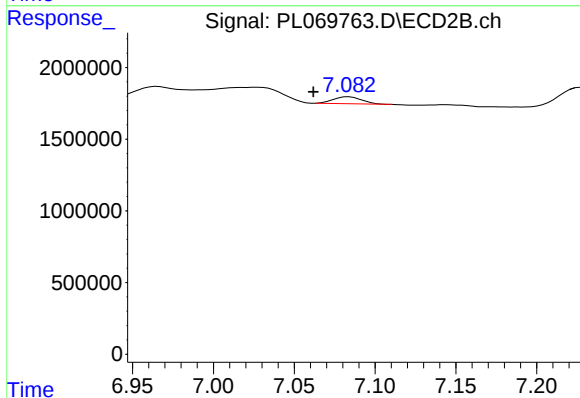


#7 delta-BHC

R.T.: 7.084 min
Delta R.T.: 0.022 min
Response: 531918
Conc: 0.30 ng/ml

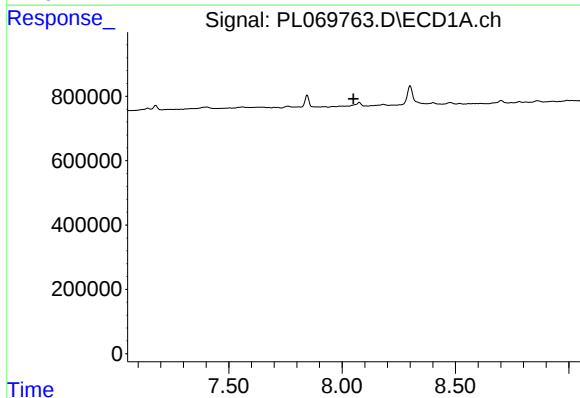


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.050 min
Response: 0
Conc: N.D.

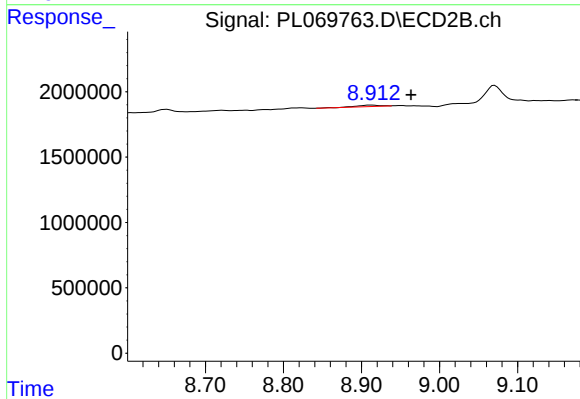

#14 Endrin


R.T.: 8.913 min
Delta R.T.: -0.050 min
Response: 228784
Conc: 0.19 ng/ml

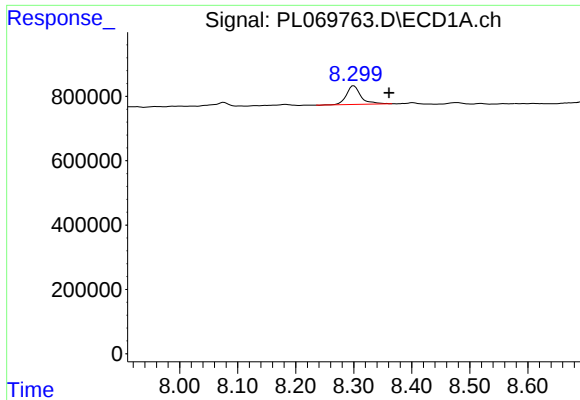

#15 Endosulfan II


R.T.: 8.300 min
Delta R.T.: -0.061 min
Response: 1010766
Conc: 1.64 ng/ml

Instrument :
ECD_P
ClientSampleId :

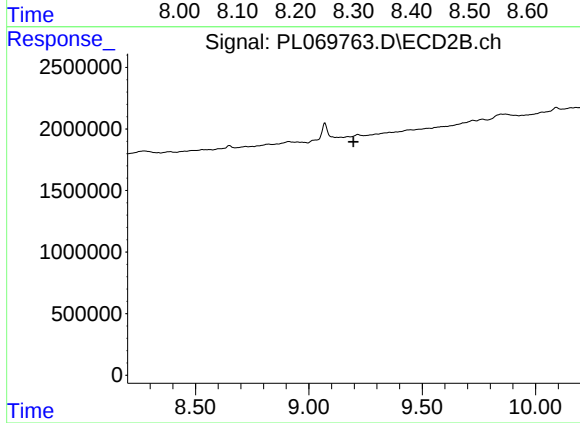


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 9.197 min
Response: 0
Conc: N.D.

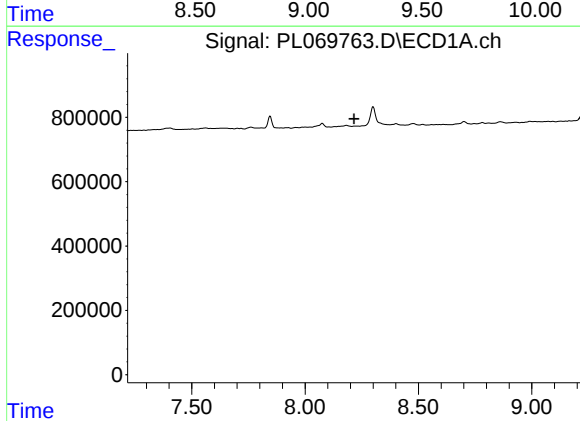


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.216 min
Response: 0
Conc: N.D.

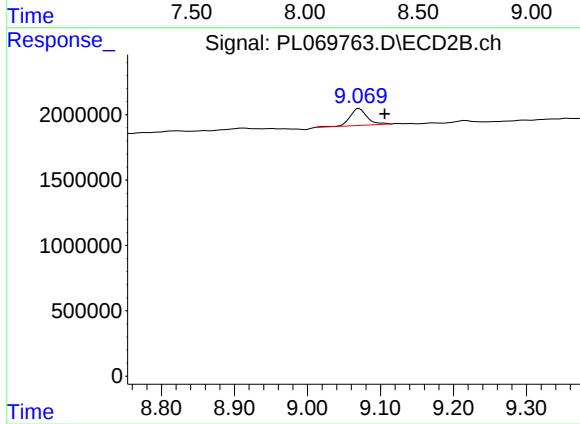

#16 4,4'-DDD


R.T.: 9.071 min
Delta R.T.: -0.035 min
Response: 2102259
Conc: 1.80 ng/ml

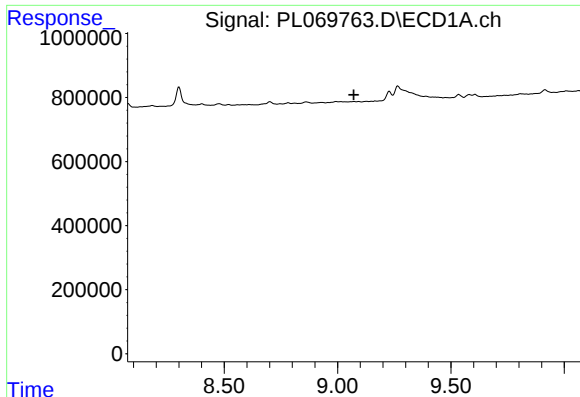

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.072 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

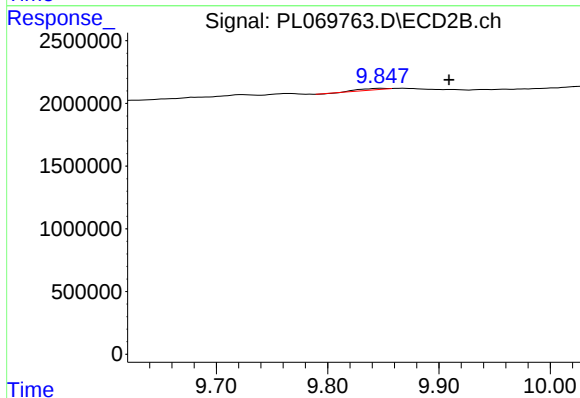


#20 Methoxychlor

R.T.: 9.848 min
Delta R.T.: -0.061 min
Response: 179089
Conc: 0.29 ng/ml

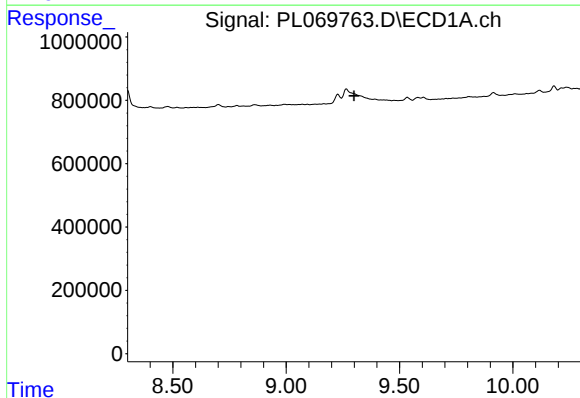


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.299 min
Response: 0
Conc: N.D.

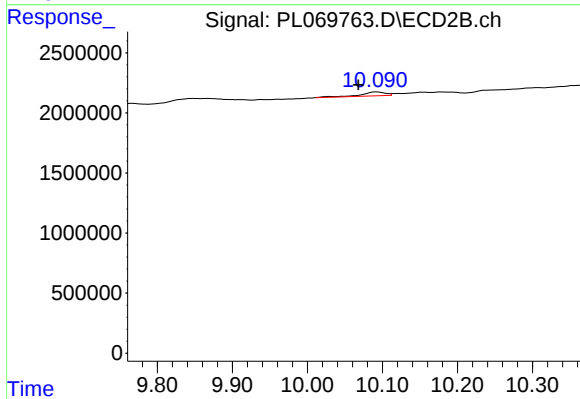

#21 Endrin ketone


R.T.: 10.092 min
Delta R.T.: 0.024 min
Response: 758300
Conc: 0.59 ng/ml

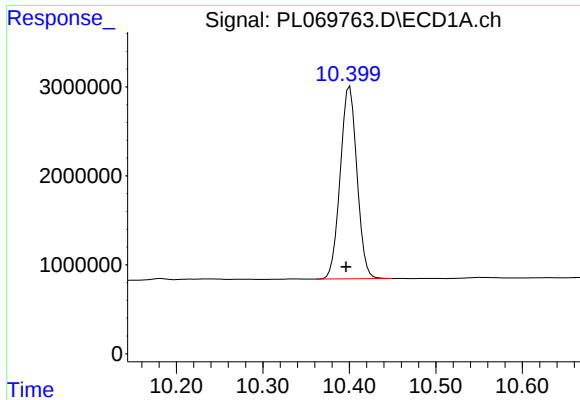

#27 Decachlorobiphenyl

R.T.: 10.400 min
Delta R.T.: 0.004 min
Response: 28890017
Conc: 37.98 ng/ml

Instrument :
ECD_P
ClientSampleId :

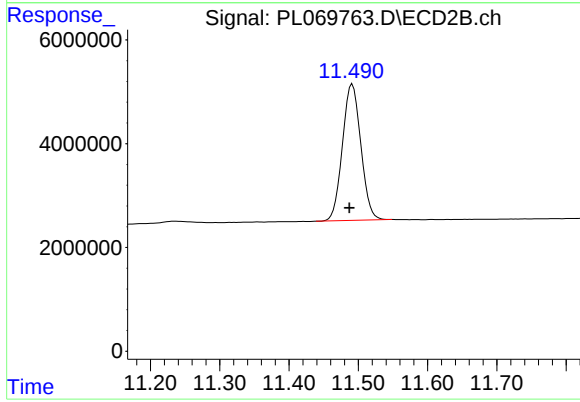

#27 Decachlorobiphenyl

R.T.: 11.491 min
Delta R.T.: 0.004 min
Response: 48556548
Conc: 41.44 ng/ml