

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090821\
 Data File : PP039244.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Sep 2021 12:08
 Operator : AJ\MA
 Sample : M3661-04RE
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 04-A-04-B-04-CRE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 06:36:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP090221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 03 04:15:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.870	3.855	1566145	737352	40.880	30.741
2) SA Decachlor...	10.834	9.106	1099048	662070	33.389	30.252

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090821\
Data File : PP039244.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Sep 2021 12:08
Operator : AJ\MA
Sample : M3661-04RE
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
04-A-04-B-04-CRE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 06:36:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP090221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 03 04:15:14 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

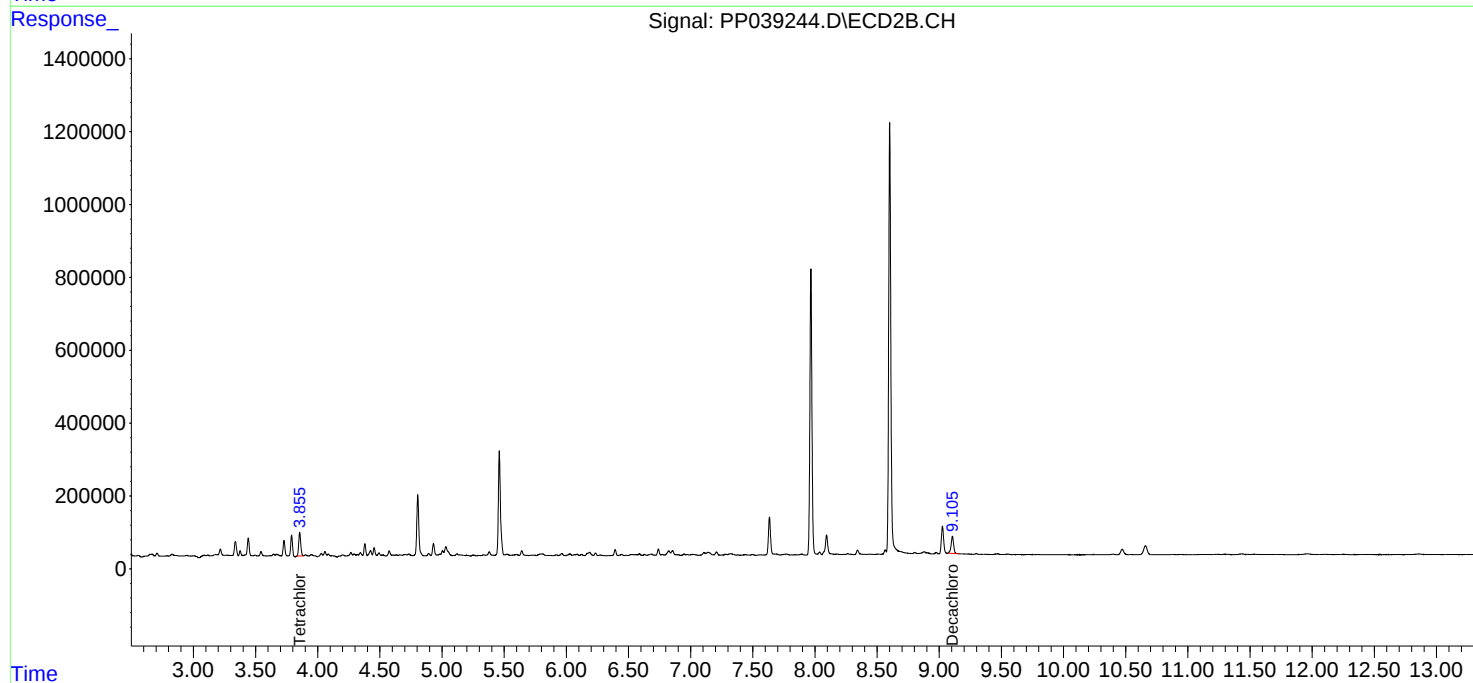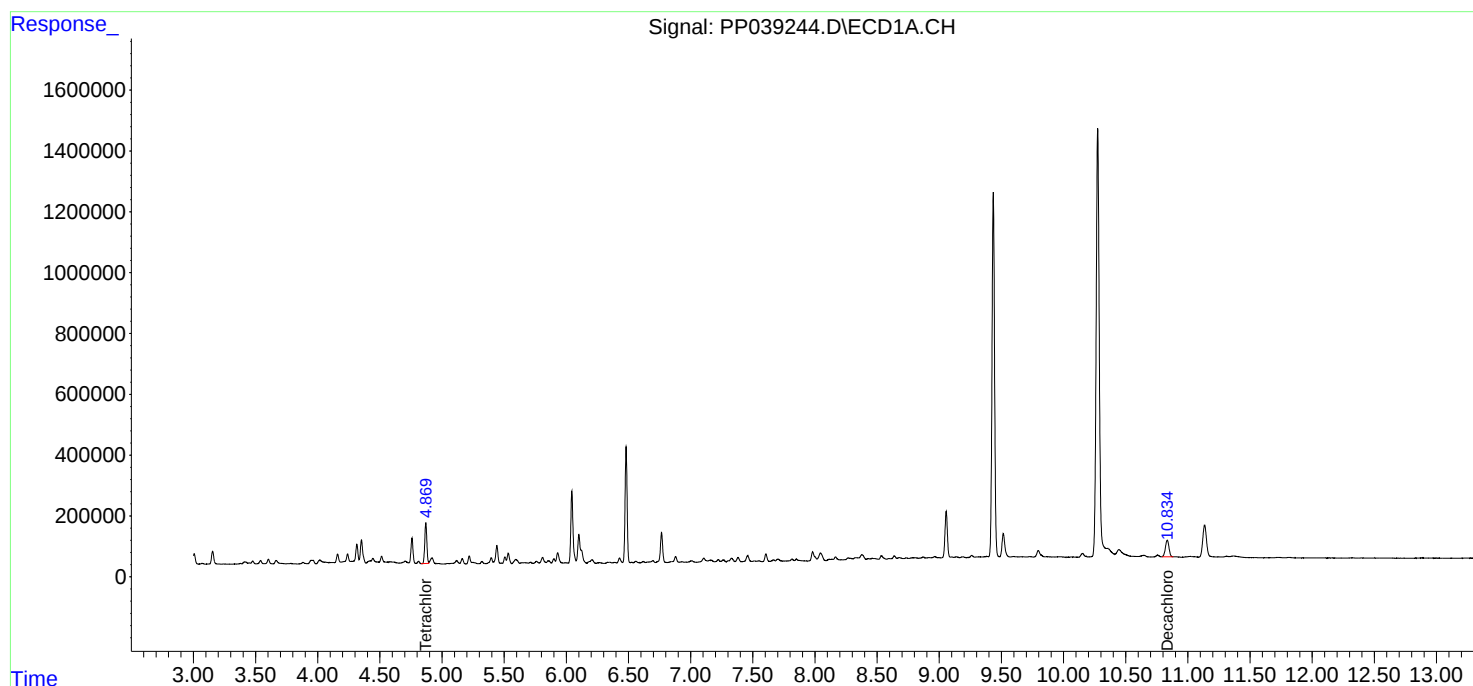


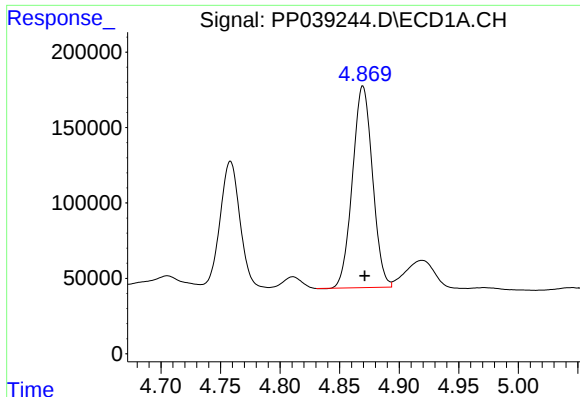

#1 Tetrachloro-m-xylene


R.T.: 4.870 min
Delta R.T.: -0.001 min
Response: 1566145
Conc: 40.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
04-A-04-B-04-CRE

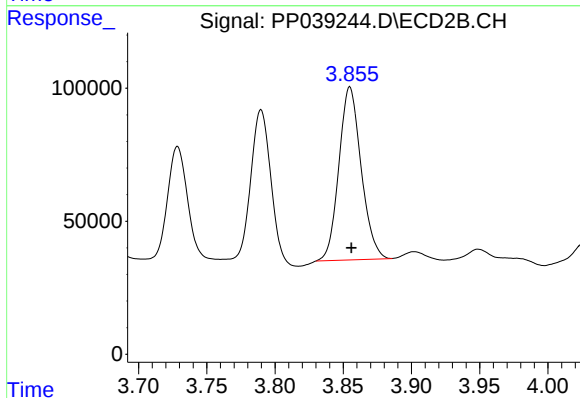


#1 Tetrachloro-m-xylene

R.T.: 3.855 min
Delta R.T.: -0.001 min
Response: 737352
Conc: 30.74 ng/ml

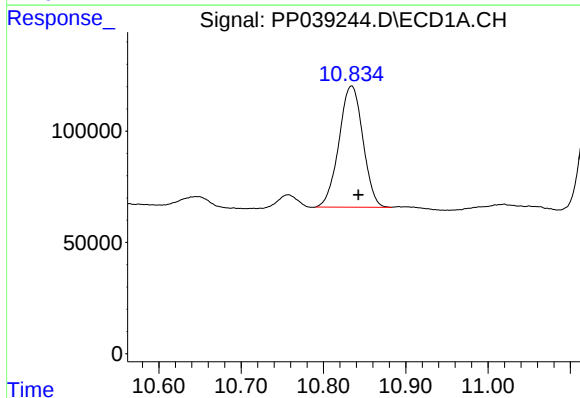

#2 Decachlorobiphenyl

R.T.: 10.834 min
Delta R.T.: -0.009 min
Response: 1099048
Conc: 33.39 ng/ml

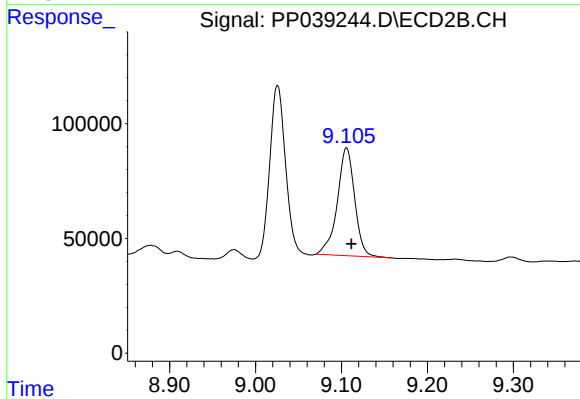

#2 Decachlorobiphenyl

R.T.: 9.106 min
Delta R.T.: -0.006 min
Response: 662070
Conc: 30.25 ng/ml