

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092223\
 Data File : PP060161.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2023 20:07
 Operator : YP\AJ
 Sample : 04574-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FRAC-TANK-A2421

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 01:05:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 19 09:22:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.509	3.666	38004310	28102067	18.269	17.252
2) SA Decachlor...	10.422	8.732	25880563	26520021	16.967	17.515

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092223\
Data File : PP060161.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2023 20:07
Operator : YP\AJ
Sample : 04574-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
FRAC-TANK-A2421

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 01:05:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091823.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 19 09:22:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

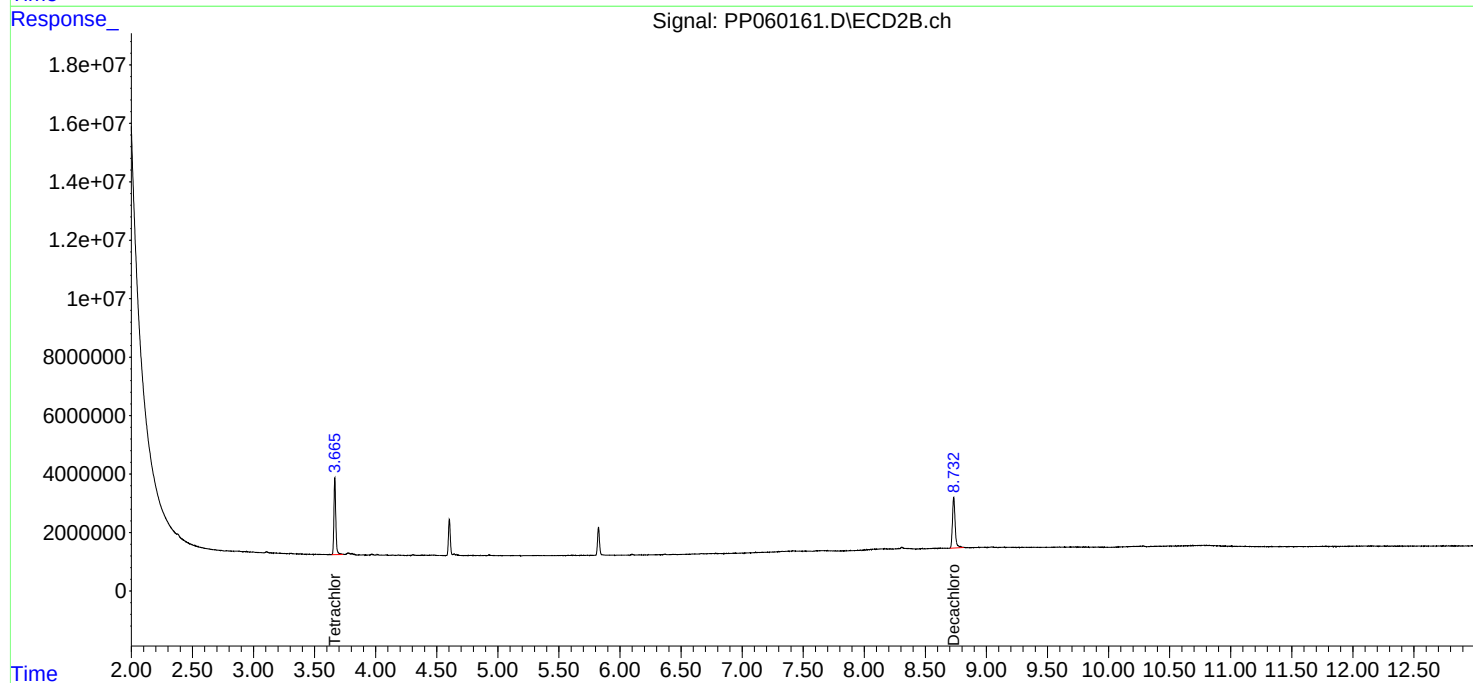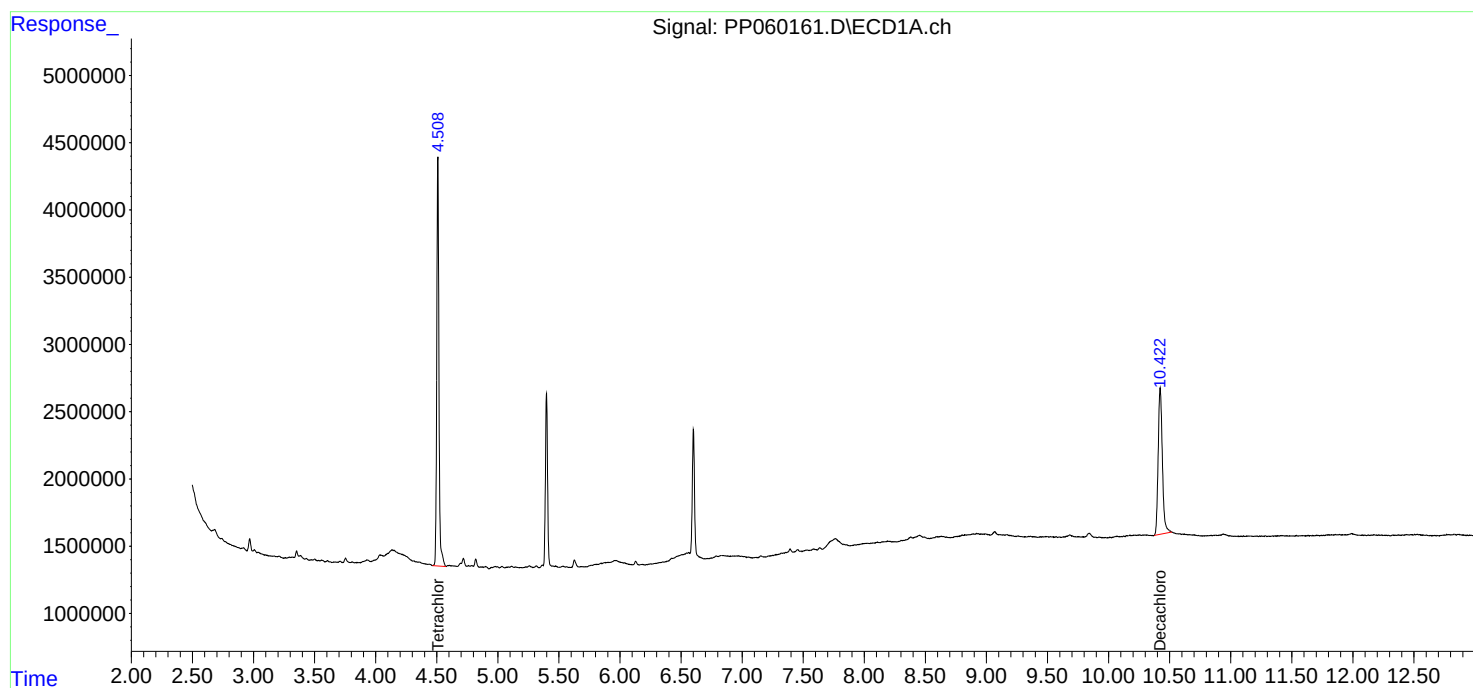


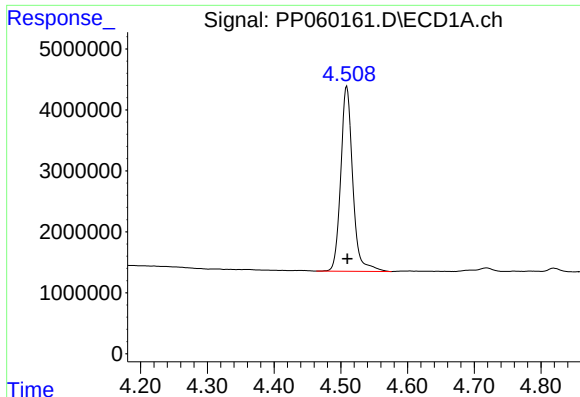

#1 Tetrachloro-m-xylene


R.T.: 4.509 min
Delta R.T.: 0.000 min
Response: 38004310
Conc: 18.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
FRAC-TANK-A2421

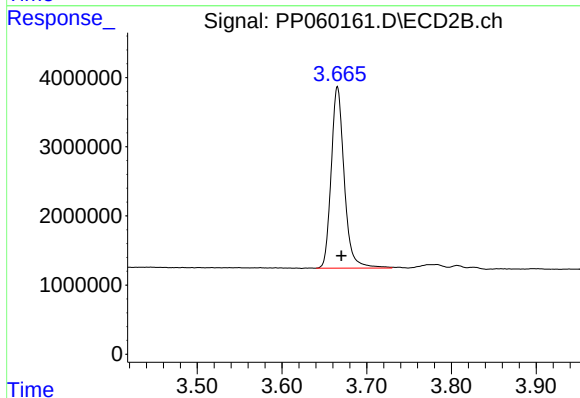


#1 Tetrachloro-m-xylene

R.T.: 3.666 min
Delta R.T.: -0.005 min
Response: 28102067
Conc: 17.25 ng/ml

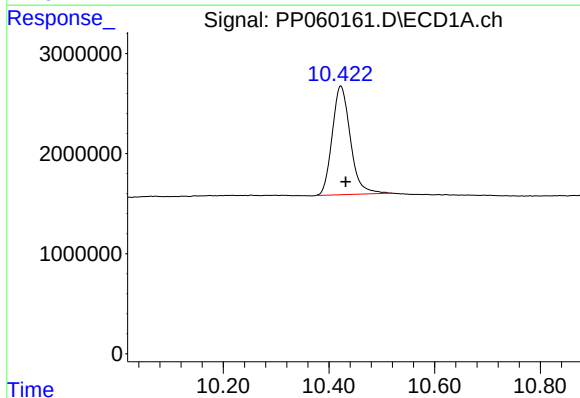

#2 Decachlorobiphenyl

R.T.: 10.422 min
Delta R.T.: -0.009 min
Response: 25880563
Conc: 16.97 ng/ml

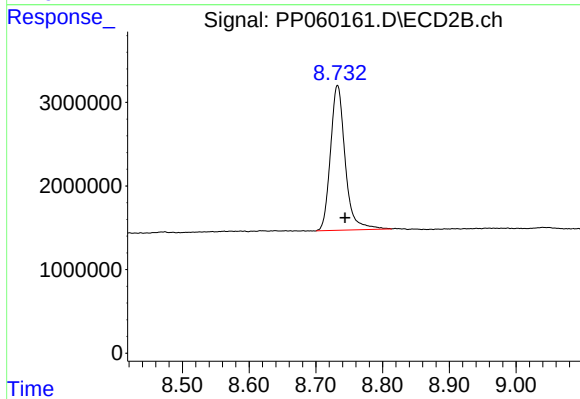

#2 Decachlorobiphenyl

R.T.: 8.732 min
Delta R.T.: -0.012 min
Response: 26520021
Conc: 17.51 ng/ml