

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092223\
 Data File : PP060167.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2023 21:45
 Operator : YP\AJ
 Sample : 04563-06 10X
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BEL-23-0005

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/25/2023
 Supervised By :Ankita Jodhani 09/25/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 01:06:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 19 09:22:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.508	3.666	3918940	3164185	1.884m	1.943
2) SA Decachlor...	10.424	8.732	5391025	5192631	3.534m	3.429

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092223\
Data File : PP060167.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2023 21:45
Operator : YP\AJ
Sample : 04563-06 10X
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BEL-23-0005


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/25/2023
Supervised By :Ankita Jodhani 09/25/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 01:06:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091823.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 19 09:22:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

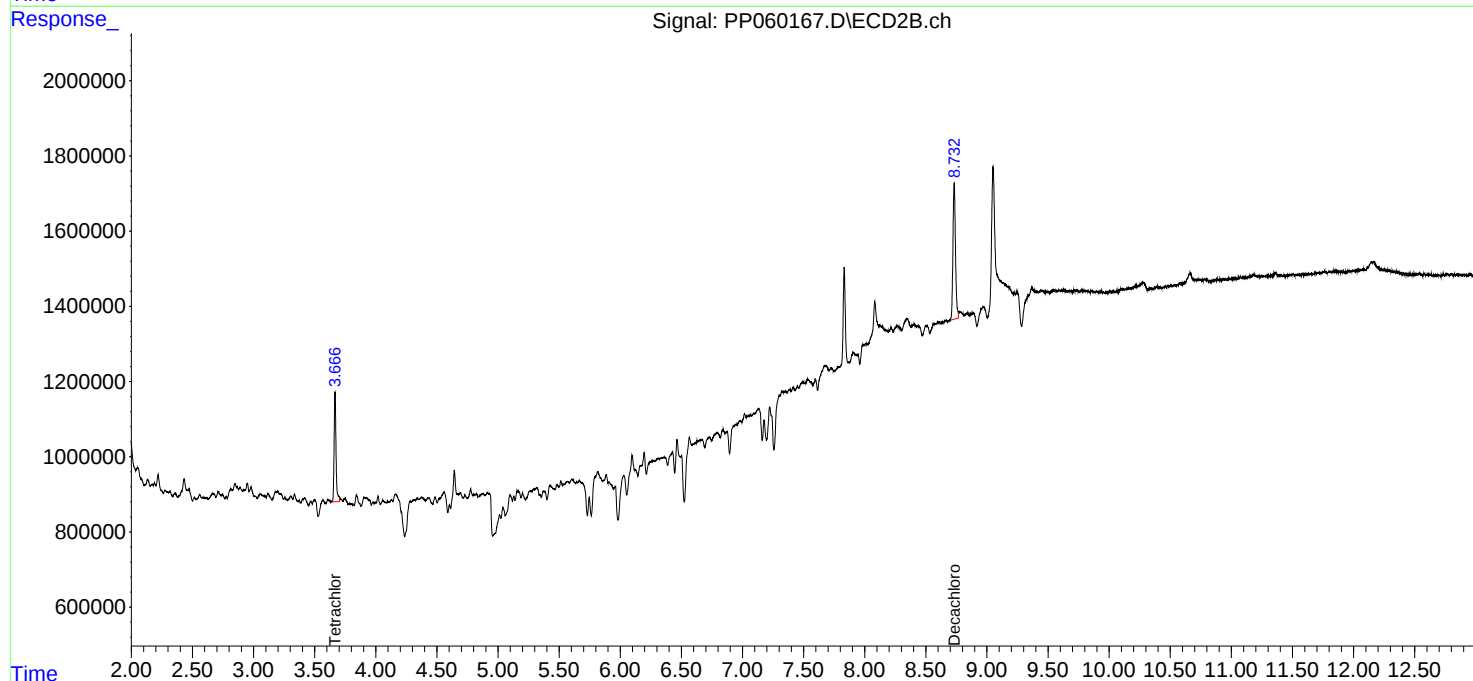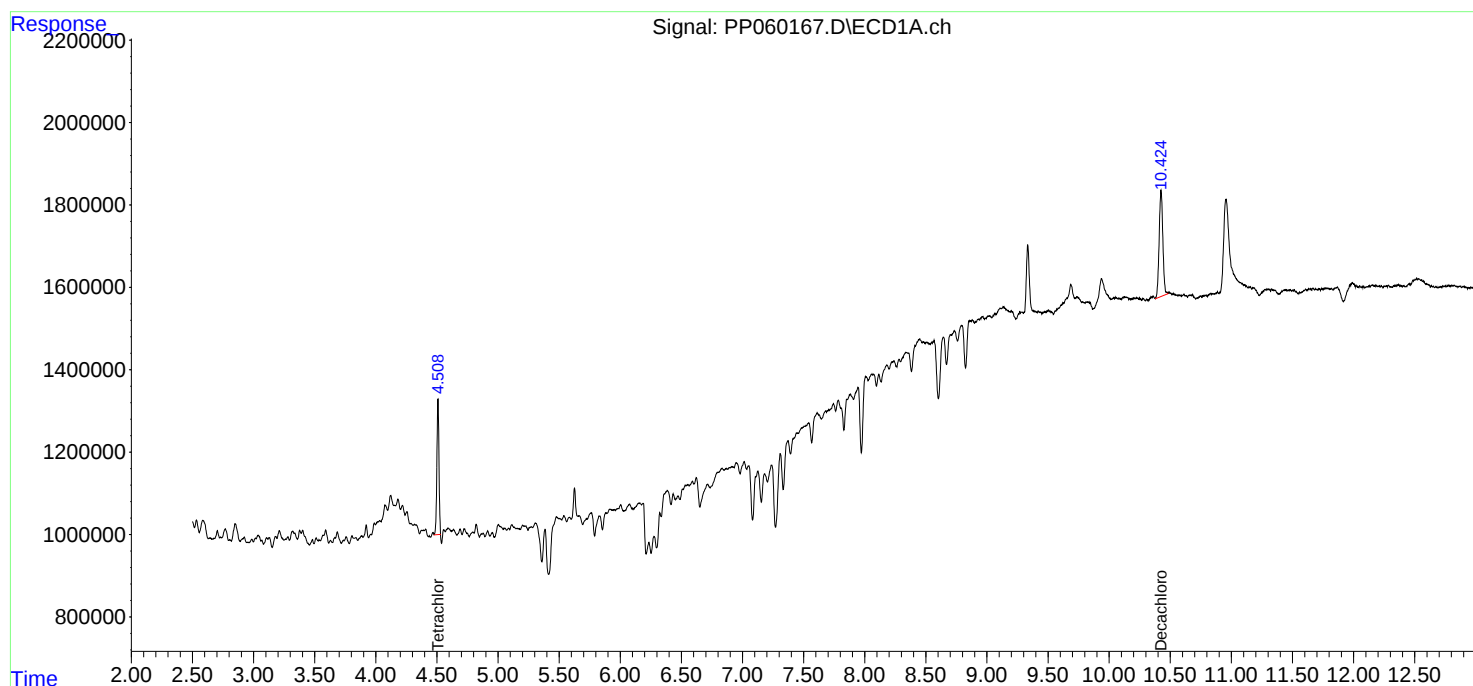

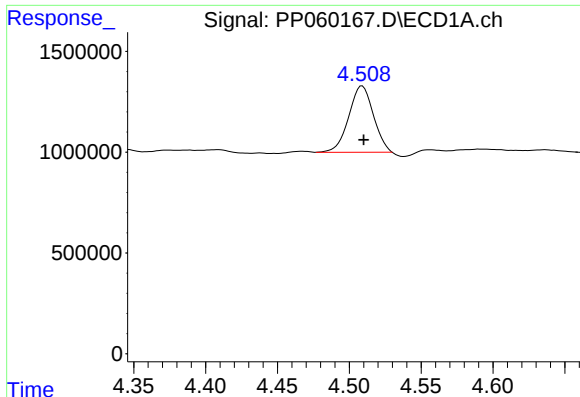


#1 Tetrachloro-m-xylene

R.T.: 4.508 min
Delta R.T.: -0.002 min
Response: 3918940
Conc: 1.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
BEL-23-0005


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/25/2023
Supervised By :Ankita Jodhani 09/25/2023

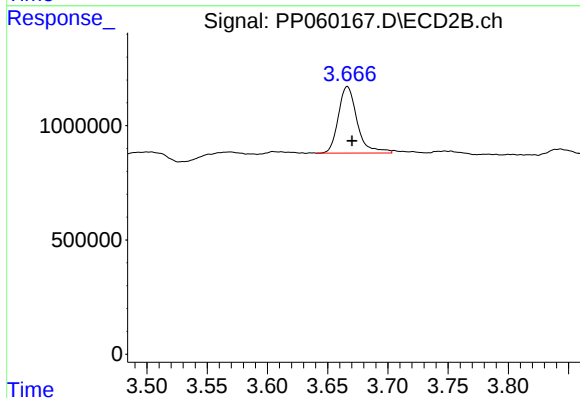


#1 Tetrachloro-m-xylene

R.T.: 3.666 min
Delta R.T.: -0.004 min
Response: 3164185
Conc: 1.94 ng/ml

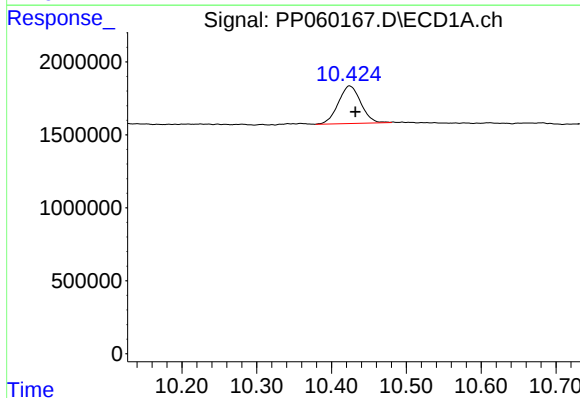

#2 Decachlorobiphenyl

R.T.: 10.424 min
Delta R.T.: -0.008 min
Response: 5391025
Conc: 3.53 ng/ml m

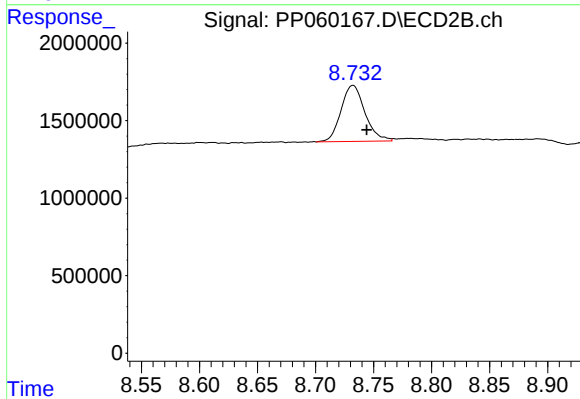

#2 Decachlorobiphenyl

R.T.: 8.732 min
Delta R.T.: -0.012 min
Response: 5192631
Conc: 3.43 ng/ml