

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100324\
 Data File : PP067460.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2024 11:03
 Operator : YP\AJ
 Sample : P4254-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MH-147-SLUDGE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 01:29:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 27 06:59:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.753	4.052	8442864	9187770	6.281	6.149
2)	SA Decachlor...	10.663	9.217	5801284	5792052	3.996	4.203
Target Compounds							
3)	L1 AR-1016-1	5.875f	5.204f	2832846	46068	59.414	0.893 #
4)	L1 AR-1016-2	5.875f	5.204	2832846	46068	40.912	0.648 #
5)	L1 AR-1016-3	0.000	5.363	0	326686	N.D.	8.209 #
6)	L1 AR-1016-4	6.087	5.401	1446018	73282	40.239	2.122 #
7)	L1 AR-1016-5	6.365	5.664f	1225190	121291	33.248	2.827 #
8)	L2 AR-1221-1	4.957	0.000	630849	0	37.683	N.D. #
9)	L2 AR-1221-2	0.000	4.361	0	238262	N.D.	16.240 #
10)	L2 AR-1221-3	0.000	4.425	0	133985	N.D.	3.090 #
11)	L3 AR-1232-1	0.000	4.425	0	133985	N.D.	3.725 #
12)	L3 AR-1232-2	5.645	5.204	681599	46068	38.293	1.391 #
13)	L3 AR-1232-3	5.875f	5.363	2832846	326686	89.611	18.184 #
14)	L3 AR-1232-4	6.087	5.476	1446018	110754	89.610	6.333 #
15)	L3 AR-1232-5	6.205	5.664f	327383	121291	24.199	6.460 #
16)	L4 AR-1242-1	5.875f	5.204f	2832846	46068	79.658	1.201 #
17)	L4 AR-1242-2	5.875f	5.204	2832846	46068	54.145	0.880 #
18)	L4 AR-1242-3	0.000	5.363	0	326686	N.D.	10.992 #
19)	L4 AR-1242-4	6.087	5.476	1446018	110754	52.724	3.442 #
20)	L4 AR-1242-5	6.833	5.992	417867	2927414	14.040	76.678 #
21)	L5 AR-1248-1	5.875f	5.204f	2832846	46068	100.331	1.504 #
22)	L5 AR-1248-2	6.205	5.401	327383	73282	7.374	1.615 #
23)	L5 AR-1248-3	6.365	5.476	1225190	110754	25.249	2.340 #
24)	L5 AR-1248-4	6.787	5.664f	2692131	121291	49.616	2.233 #
25)	L5 AR-1248-5	6.833	6.031	417867	135316	7.578	2.776 #
26)	L6 AR-1254-1	6.787	5.992	2692131	2927414	43.210	36.114
27)	L6 AR-1254-2	7.006	6.127	2223381	405179	24.504	5.524 #
28)	L6 AR-1254-3	7.355	6.544	633892	378440	6.758	3.319 #
29)	L6 AR-1254-4	7.619	6.791	1006988	138248	15.110	2.215 #
30)	L6 AR-1254-5	8.055	7.181	545655	382006	6.638	3.721 #
31)	L7 AR-1260-1	0.000	6.658	0	324151	N.D.	3.963 #
32)	L7 AR-1260-2	7.778	6.850	1629773	356206	17.881	3.792 #
33)	L7 AR-1260-3	0.000	7.013	0	207092	N.D.	2.286 #
34)	L7 AR-1260-4	8.422f	7.485	139211	468065	1.844	7.020 #
35)	L7 AR-1260-5	8.706	7.720	140561	440972	1.086	3.029 #
36)	L8 AR-1262-1	8.422f	7.216	139211	119185	1.460	1.133
37)	L8 AR-1262-2	8.706	7.485	140561	468065	0.866	4.944 #
38)	L8 AR-1262-3	0.000	8.010	0	60959	N.D.	0.831 #
39)	L8 AR-1262-4	0.000	8.072	0	105800	N.D.	0.803 #
40)	L8 AR-1262-5	0.000	8.601	0	43065	N.D.	0.709 #
41)	L9 AR-1268-1	0.000	8.010	0	60959	N.D.	0.303 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100324\
Data File : PP067460.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2024 11:03
Operator : YP\AJ
Sample : P4254-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 01:29:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092624.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 27 06:59:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	0.000	8.072	0	105800	N.D.	0.592 #
43) L9	AR-1268-3	0.000	8.291	0	438768	N.D.	2.762 #
44) L9	AR-1268-4	0.000	8.601	0	43065	N.D.	0.667 #
45) L9	AR-1268-5	0.000	8.979f	0	7232	N.D.	0.016 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100324\
Data File : PP067460.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2024 11:03
Operator : YP\AJ
Sample : P4254-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 01:29:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092624.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 27 06:59:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

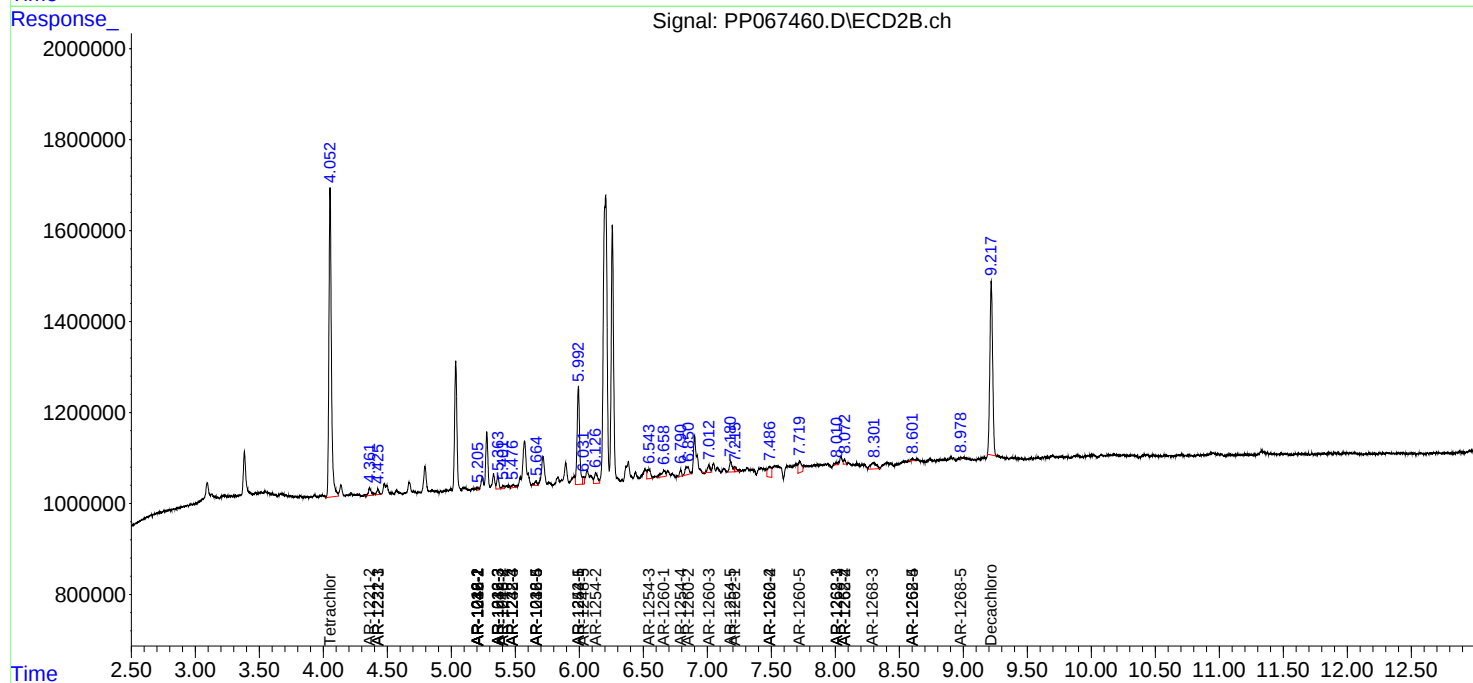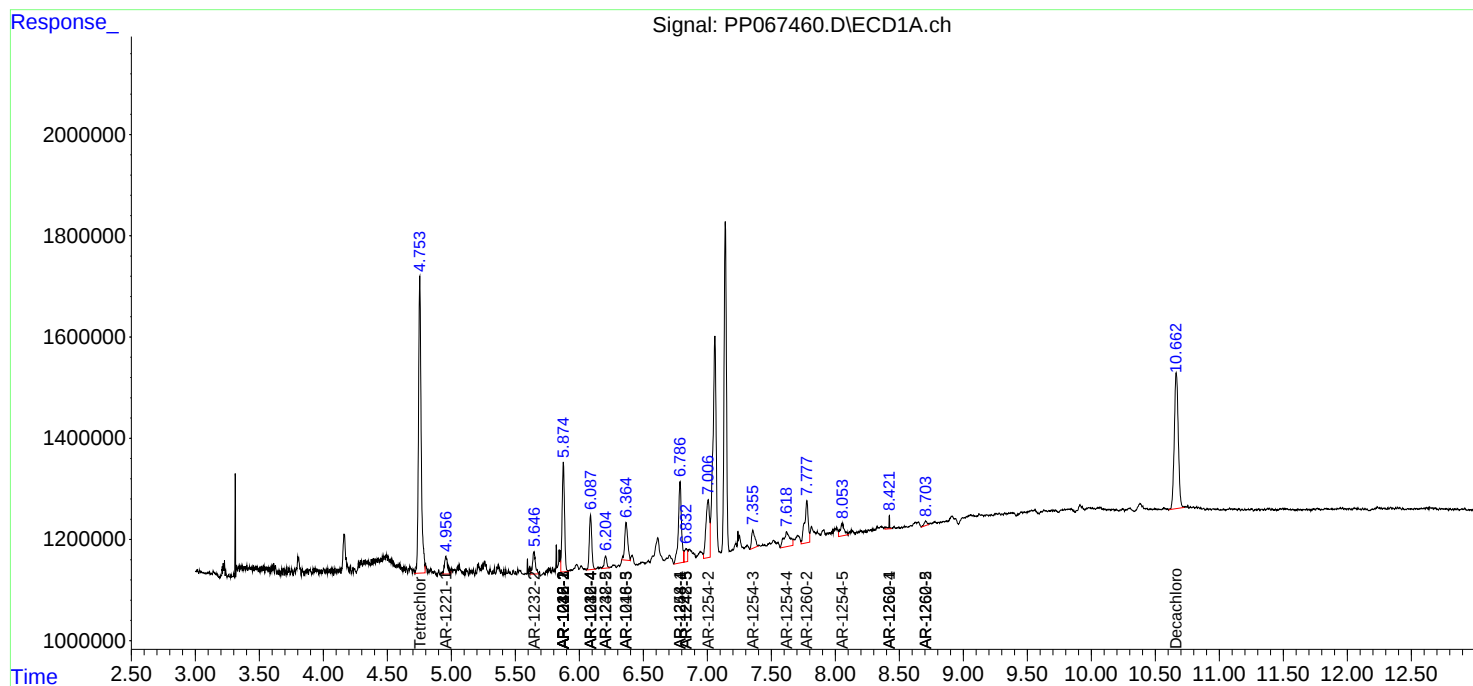


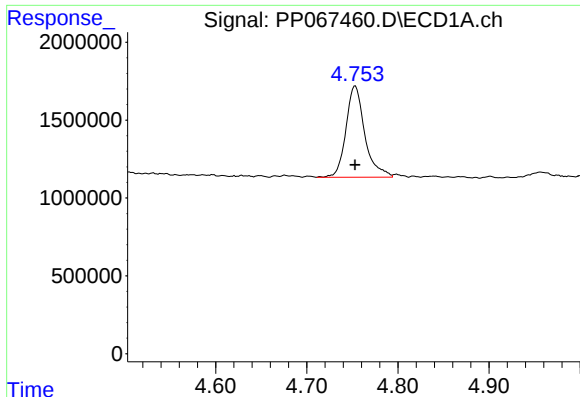

#1 Tetrachloro-m-xylene


R.T.: 4.753 min
Delta R.T.: 0.000 min
Response: 8442864
Conc: 6.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGE

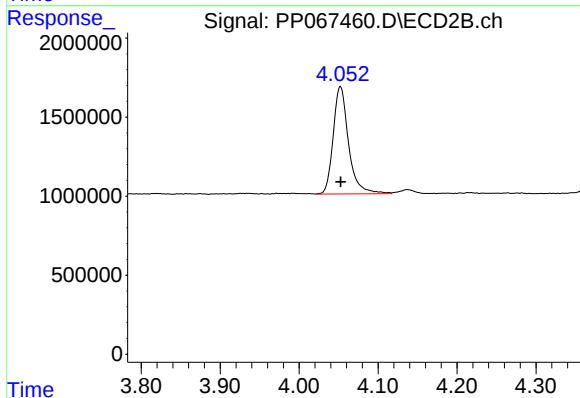


#1 Tetrachloro-m-xylene

R.T.: 4.052 min
Delta R.T.: 0.000 min
Response: 9187770
Conc: 6.15 ng/ml

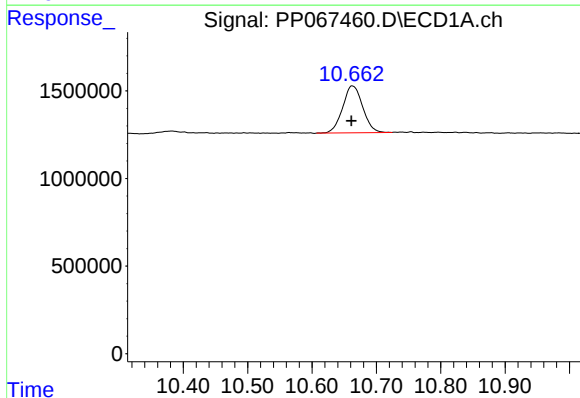


#2 Decachlorobiphenyl

R.T.: 10.663 min
Delta R.T.: 0.002 min
Response: 5801284
Conc: 4.00 ng/ml

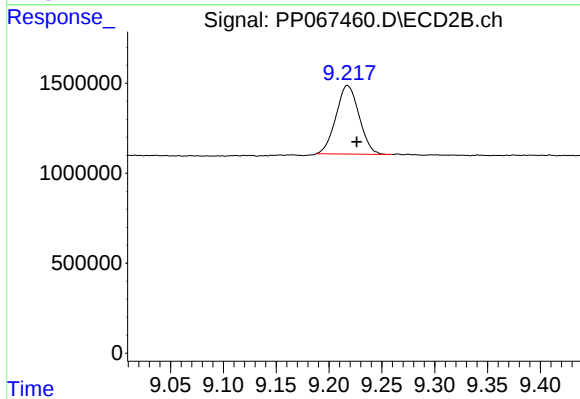

#2 Decachlorobiphenyl


R.T.: 9.217 min
Delta R.T.: -0.009 min
Response: 5792052
Conc: 4.20 ng/ml

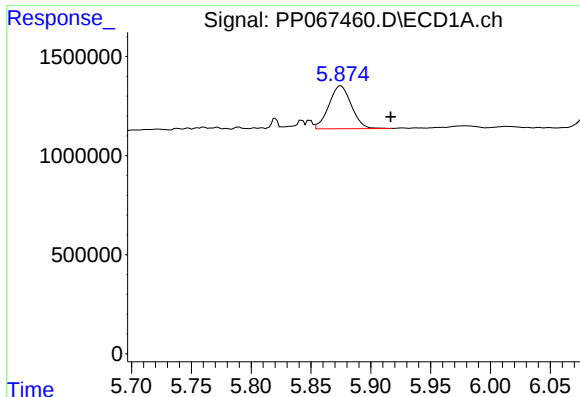

#3 AR-1016-1


R.T.: 5.875 min
Delta R.T.: -0.042 min
Response: 2832846
Conc: 59.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGE

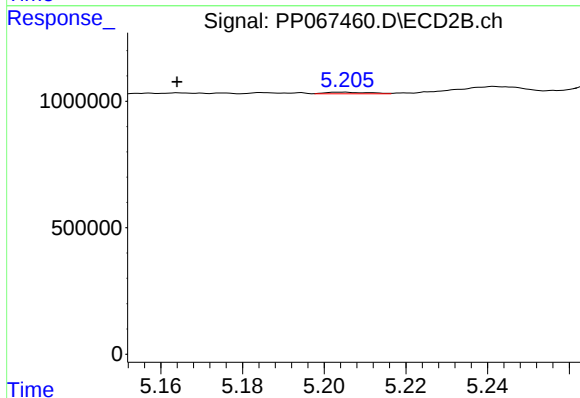


#3 AR-1016-1

R.T.: 5.204 min
Delta R.T.: 0.040 min
Response: 46068
Conc: 0.89 ng/ml

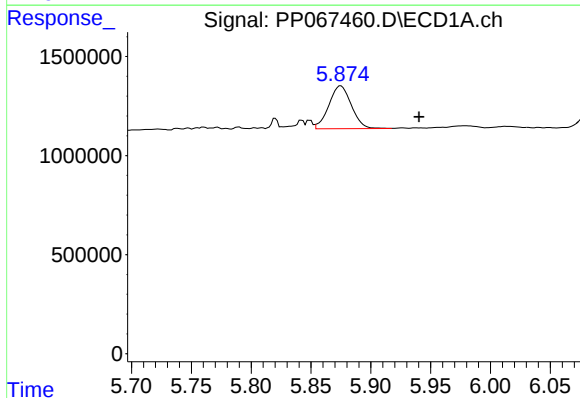


#4 AR-1016-2

R.T.: 5.875 min
Delta R.T.: -0.065 min
Response: 2832846
Conc: 40.91 ng/ml

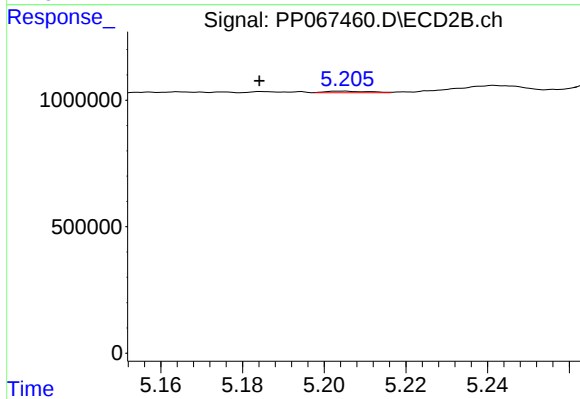

#4 AR-1016-2


R.T.: 5.204 min
Delta R.T.: 0.020 min
Response: 46068
Conc: 0.65 ng/ml

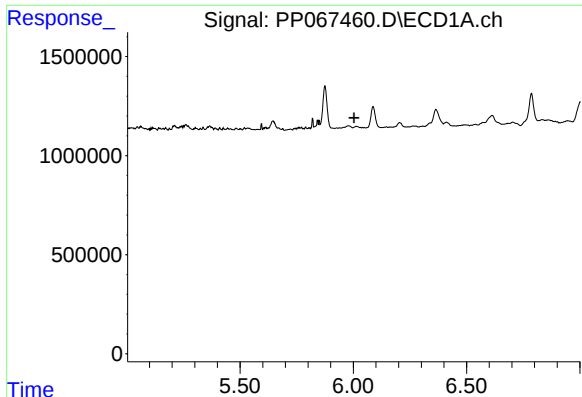

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 6.003 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGE

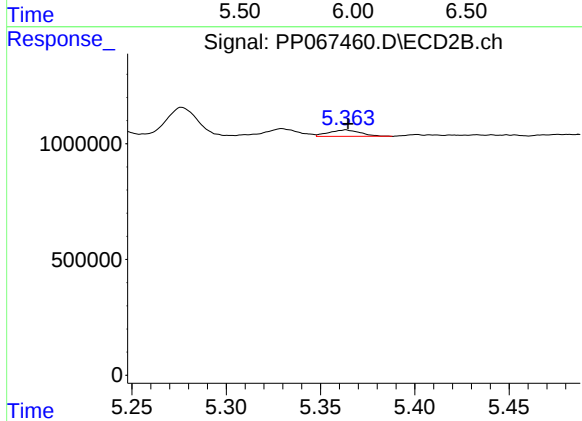


#5 AR-1016-3

R.T.: 5.363 min
Delta R.T.: -0.001 min
Response: 326686
Conc: 8.21 ng/ml

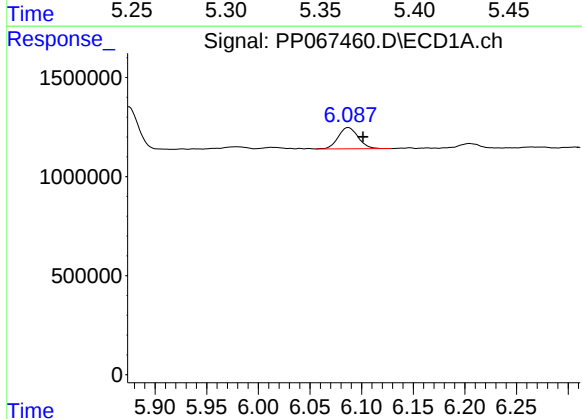


#6 AR-1016-4

R.T.: 6.087 min
Delta R.T.: -0.014 min
Response: 1446018
Conc: 40.24 ng/ml

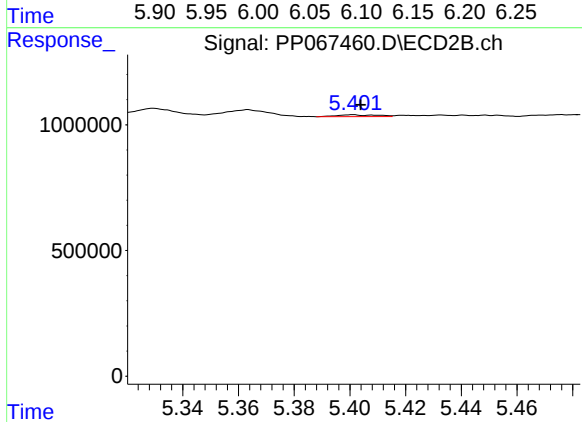

#6 AR-1016-4


R.T.: 5.401 min
Delta R.T.: -0.003 min
Response: 73282
Conc: 2.12 ng/ml

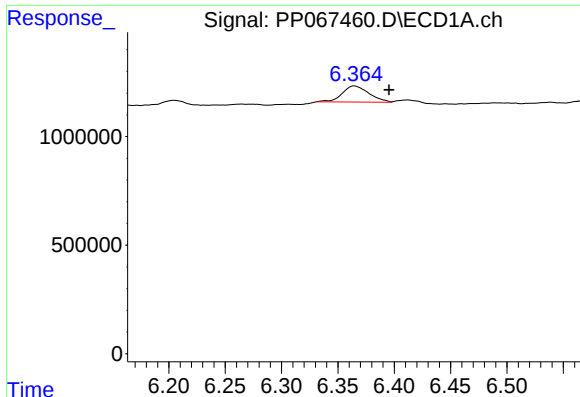

#7 AR-1016-5


R.T.: 6.365 min
Delta R.T.: -0.031 min
Response: 1225190
Conc: 33.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGE

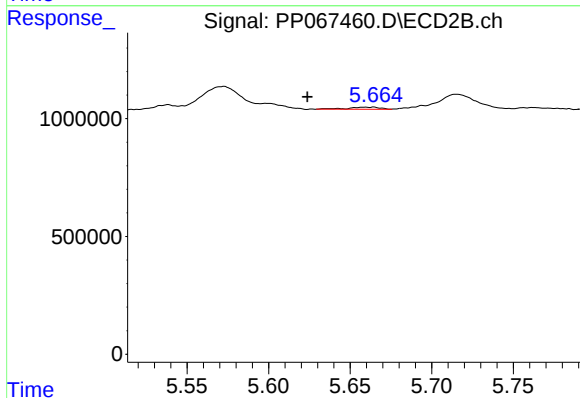


#7 AR-1016-5

R.T.: 5.664 min
Delta R.T.: 0.040 min
Response: 121291
Conc: 2.83 ng/ml

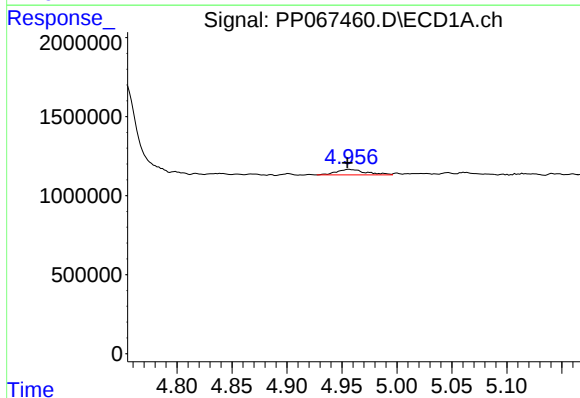


#8 AR-1221-1

R.T.: 4.957 min
Delta R.T.: 0.002 min
Response: 630849
Conc: 37.68 ng/ml

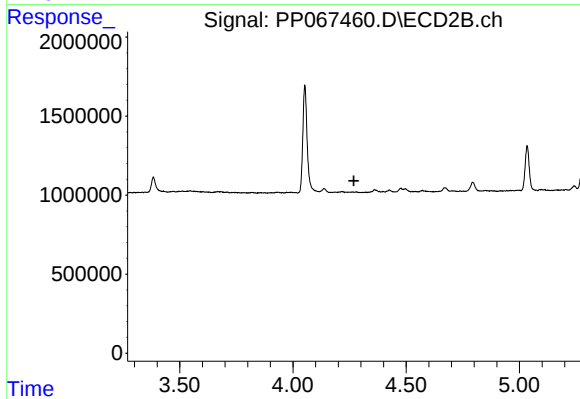

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T.: 4.269 min
Response: 0
Conc: N.D.

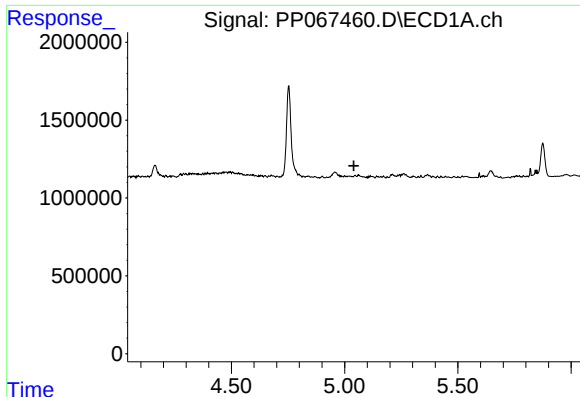

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 5.041 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGE

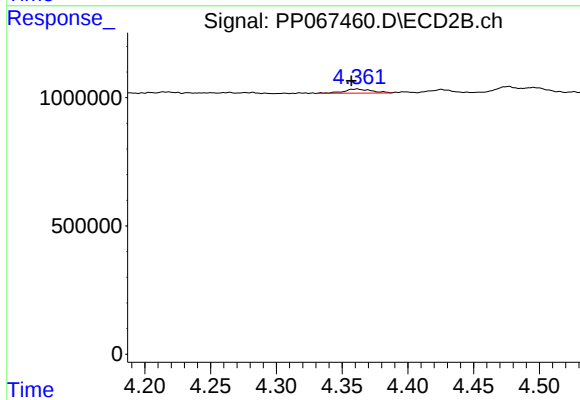


#9 AR-1221-2

R.T.: 4.361 min
Delta R.T.: 0.004 min
Response: 238262
Conc: 16.24 ng/ml

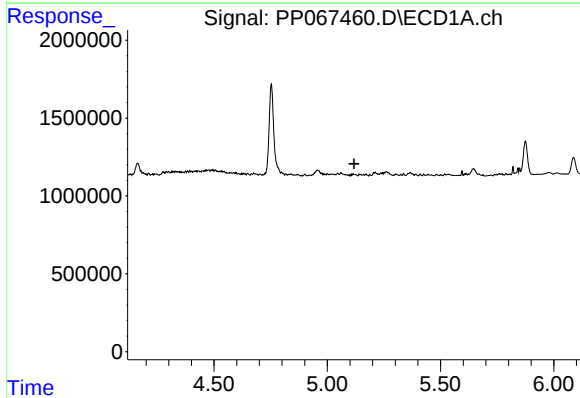


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T.: 5.118 min
Response: 0
Conc: N.D.

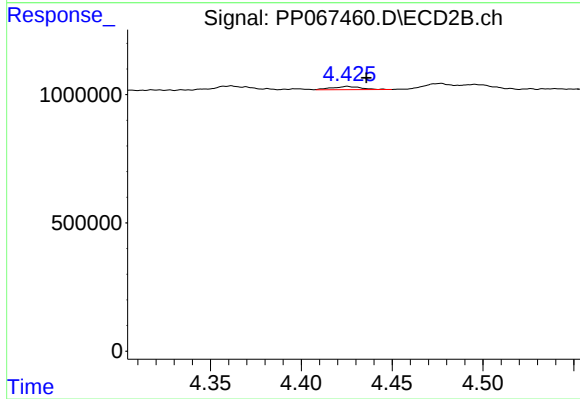

#10 AR-1221-3


R.T.: 4.425 min
Delta R.T.: -0.011 min
Response: 133985
Conc: 3.09 ng/ml

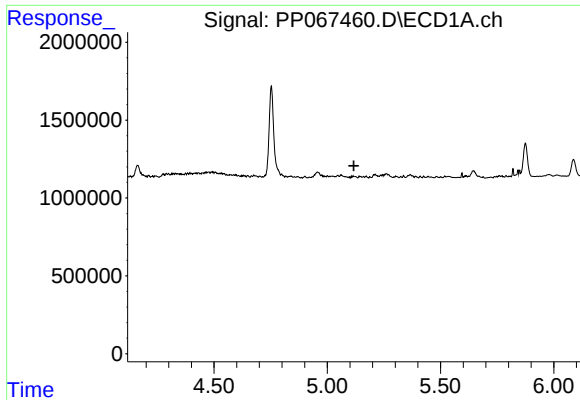

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T.: 5.118 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGE

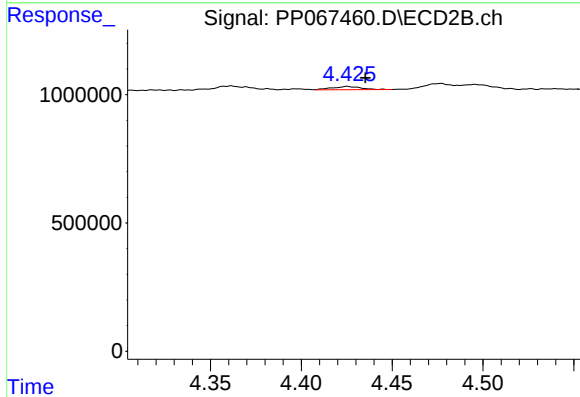


#11 AR-1232-1

R.T.: 4.425 min
Delta R.T.: -0.010 min
Response: 133985
Conc: 3.72 ng/ml

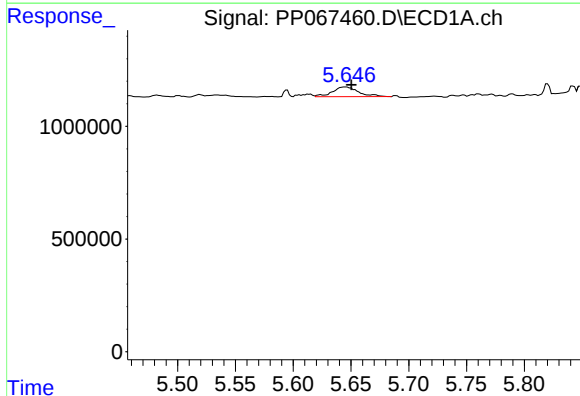


#12 AR-1232-2

R.T.: 5.645 min
Delta R.T.: -0.005 min
Response: 681599
Conc: 38.29 ng/ml

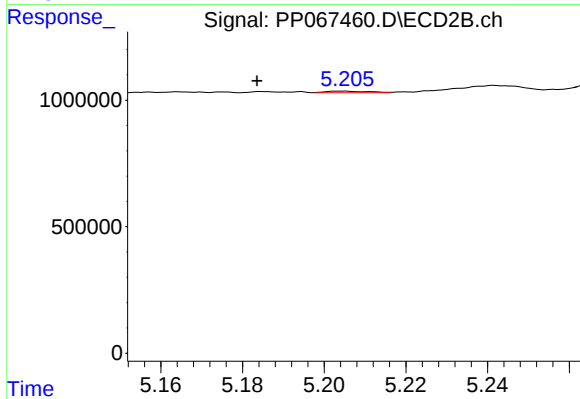

#12 AR-1232-2


R.T.: 5.204 min
Delta R.T.: 0.021 min
Response: 46068
Conc: 1.39 ng/ml

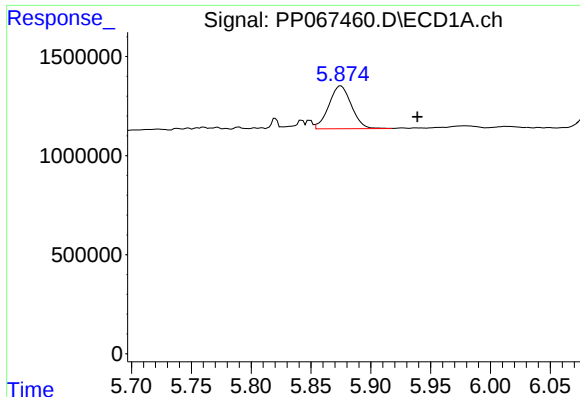

#13 AR-1232-3


R.T.: 5.875 min
Delta R.T.: -0.064 min
Response: 2832846
Conc: 89.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGE

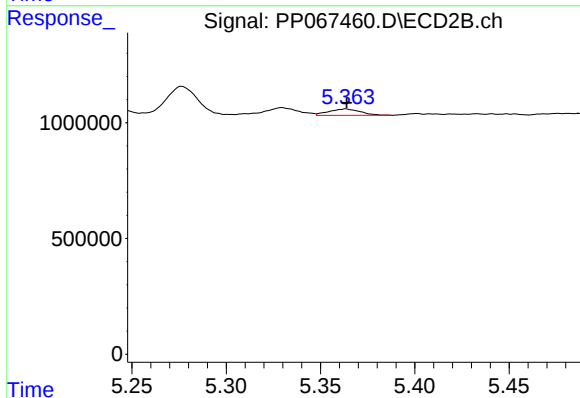


#13 AR-1232-3

R.T.: 5.363 min
Delta R.T.: 0.000 min
Response: 326686
Conc: 18.18 ng/ml

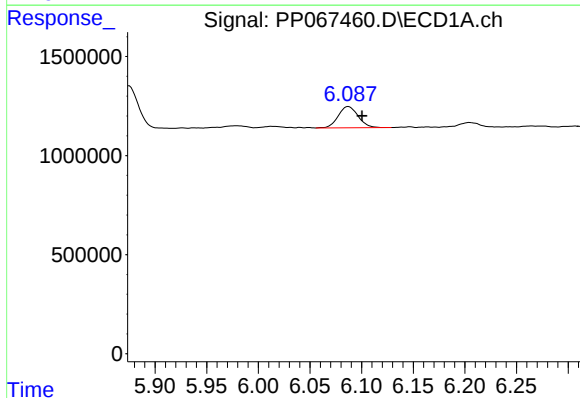


#14 AR-1232-4

R.T.: 6.087 min
Delta R.T.: -0.013 min
Response: 1446018
Conc: 89.61 ng/ml

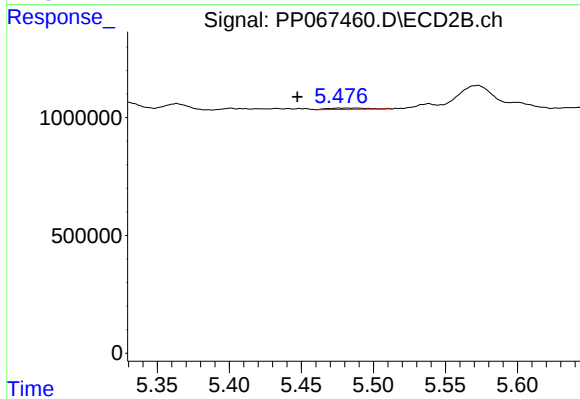

#14 AR-1232-4


R.T.: 5.476 min
Delta R.T.: 0.029 min
Response: 110754
Conc: 6.33 ng/ml

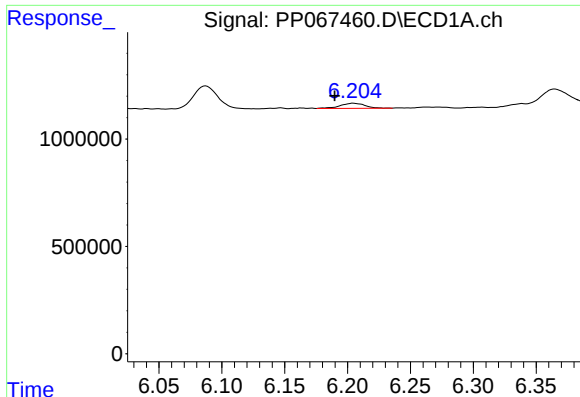

#15 AR-1232-5


R.T.: 6.205 min
Delta R.T.: 0.015 min
Response: 327383
Conc: 24.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGE

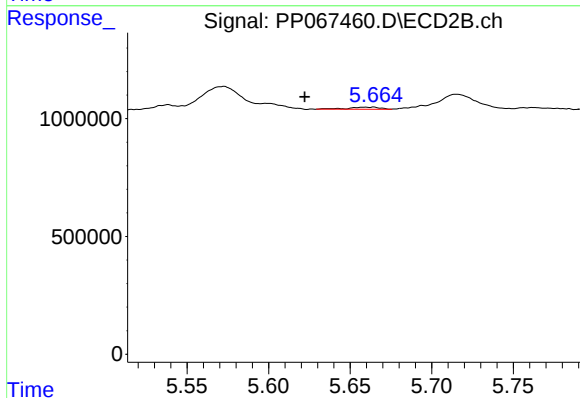


#15 AR-1232-5

R.T.: 5.664 min
Delta R.T.: 0.042 min
Response: 121291
Conc: 6.46 ng/ml

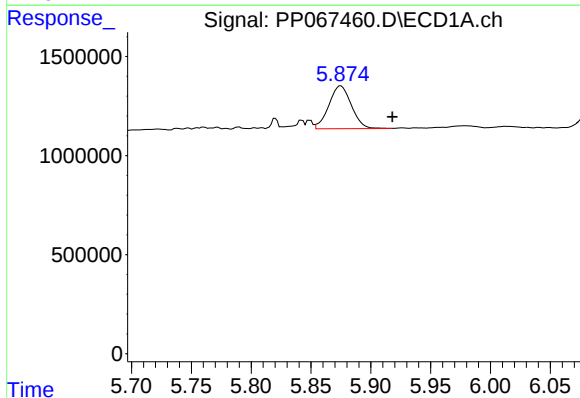


#16 AR-1242-1

R.T.: 5.875 min
Delta R.T.: -0.043 min
Response: 2832846
Conc: 79.66 ng/ml

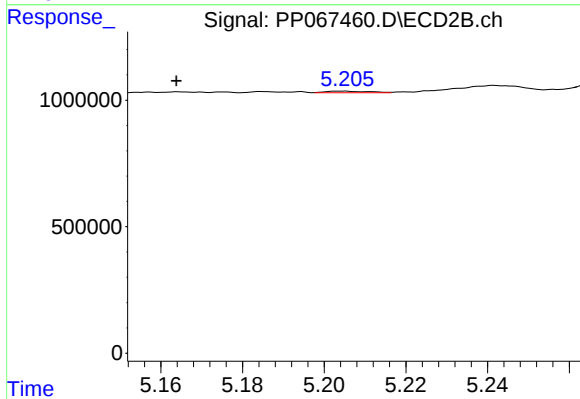

#16 AR-1242-1


R.T.: 5.204 min
Delta R.T.: 0.040 min
Response: 46068
Conc: 1.20 ng/ml

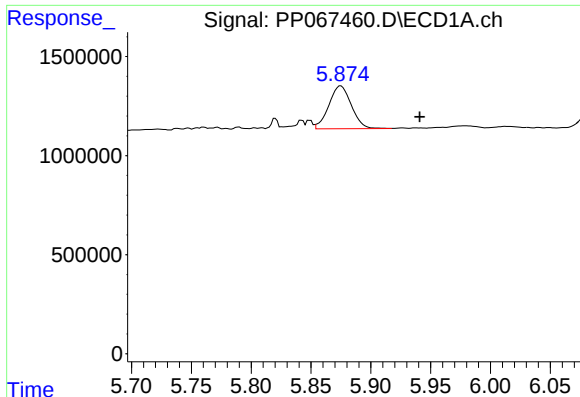

#17 AR-1242-2


R.T.: 5.875 min
Delta R.T.: -0.066 min
Response: 2832846
Conc: 54.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGE

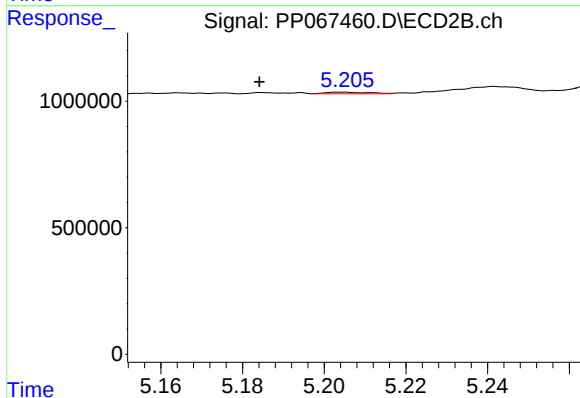


#17 AR-1242-2

R.T.: 5.204 min
Delta R.T.: 0.020 min
Response: 46068
Conc: 0.88 ng/ml

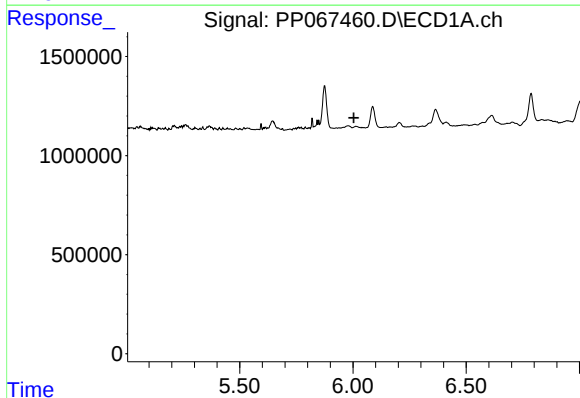


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T. : 6.004 min
Response: 0
Conc: N.D.

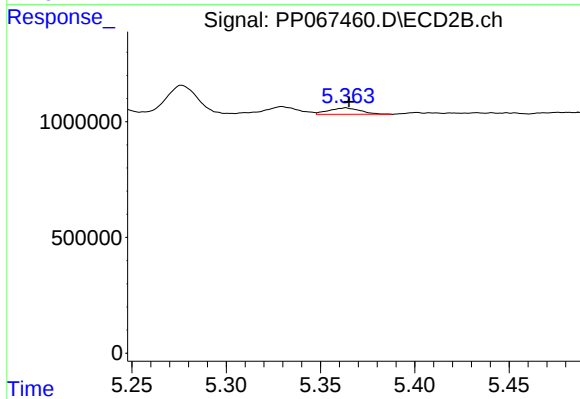

#18 AR-1242-3


R.T.: 5.363 min
Delta R.T.: -0.002 min
Response: 326686
Conc: 10.99 ng/ml

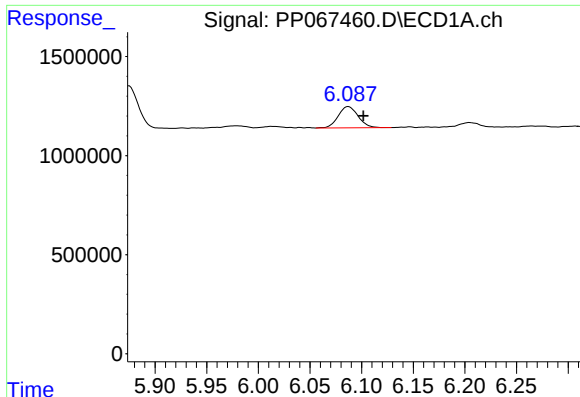

#19 AR-1242-4


R.T.: 6.087 min
Delta R.T.: -0.015 min
Response: 1446018
Conc: 52.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGE

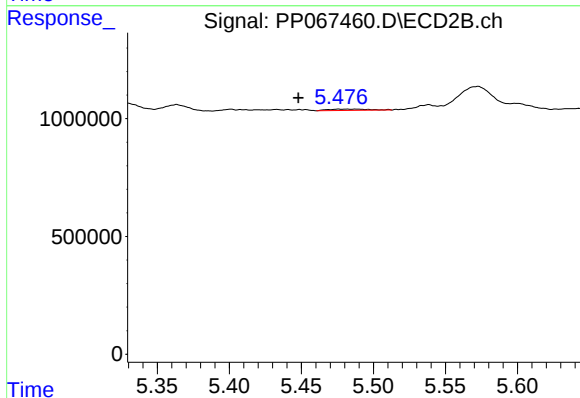


#19 AR-1242-4

R.T.: 5.476 min
Delta R.T.: 0.028 min
Response: 110754
Conc: 3.44 ng/ml

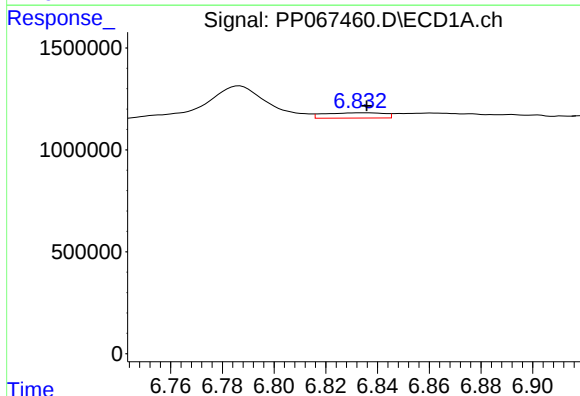


#20 AR-1242-5

R.T.: 6.833 min
Delta R.T.: -0.003 min
Response: 417867
Conc: 14.04 ng/ml

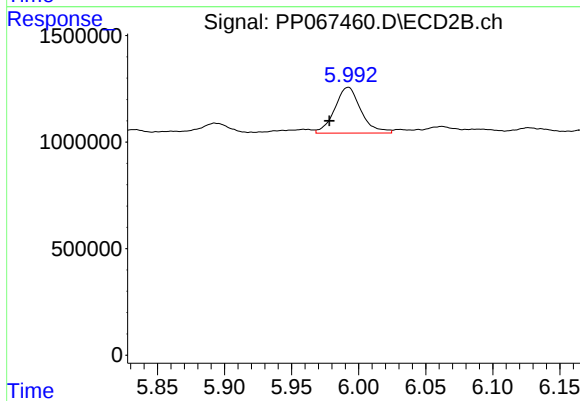

#20 AR-1242-5


R.T.: 5.992 min
Delta R.T.: 0.014 min
Response: 2927414
Conc: 76.68 ng/ml

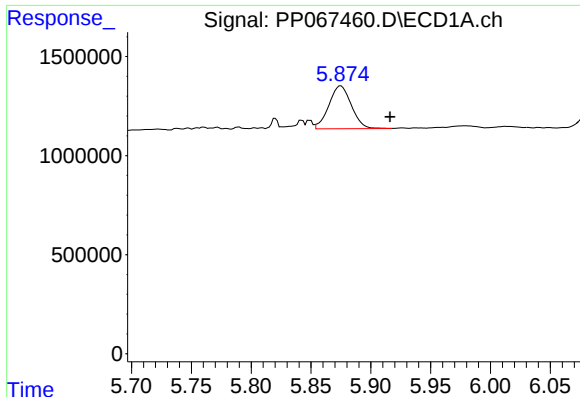

#21 AR-1248-1


R.T.: 5.875 min
Delta R.T.: -0.041 min
Response: 2832846
Conc: 100.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGE

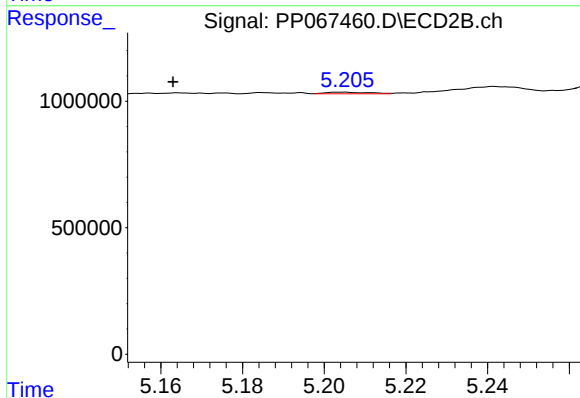


#21 AR-1248-1

R.T.: 5.204 min
Delta R.T.: 0.041 min
Response: 46068
Conc: 1.50 ng/ml

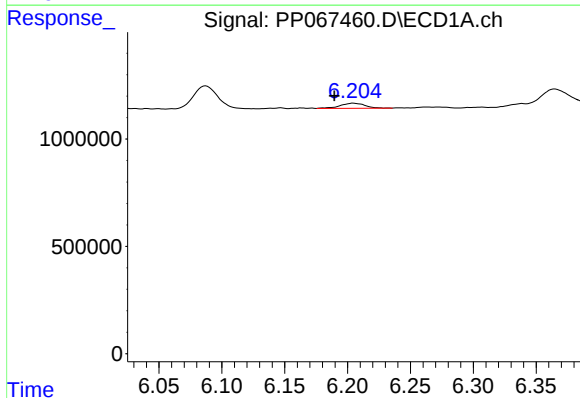


#22 AR-1248-2

R.T.: 6.205 min
Delta R.T.: 0.015 min
Response: 327383
Conc: 7.37 ng/ml

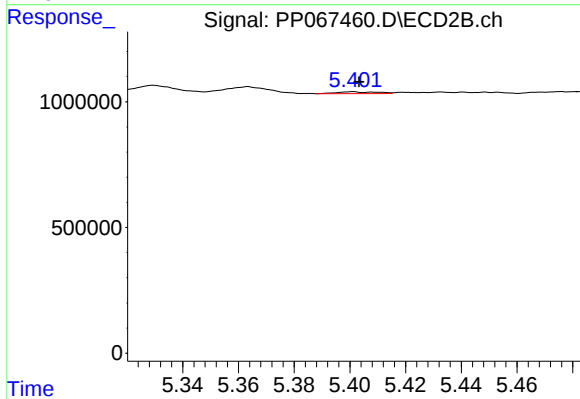

#22 AR-1248-2


R.T.: 5.401 min
Delta R.T.: -0.002 min
Response: 73282
Conc: 1.62 ng/ml

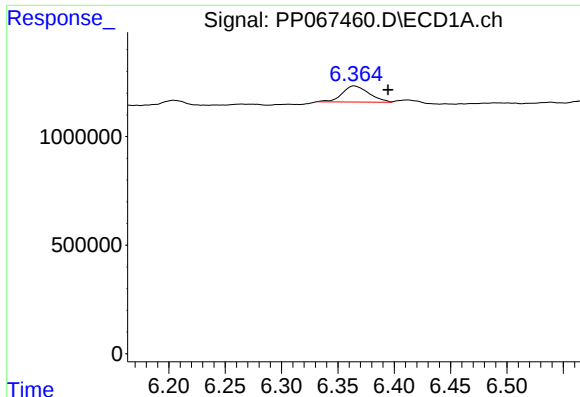

#23 AR-1248-3


R.T.: 6.365 min
Delta R.T.: -0.030 min
Response: 1225190
Conc: 25.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGE

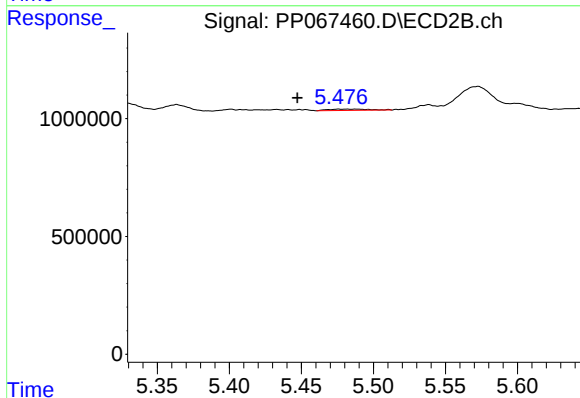


#23 AR-1248-3

R.T.: 5.476 min
Delta R.T.: 0.029 min
Response: 110754
Conc: 2.34 ng/ml

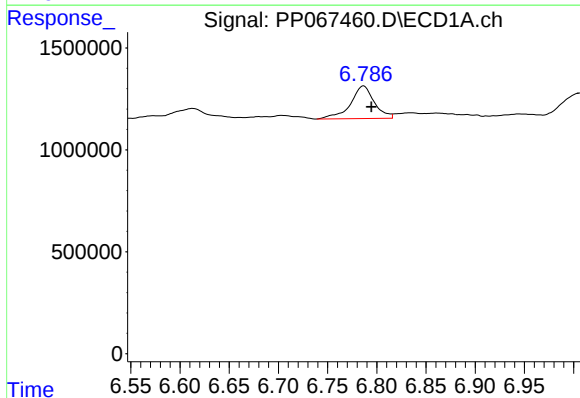


#24 AR-1248-4

R.T.: 6.787 min
Delta R.T.: -0.008 min
Response: 2692131
Conc: 49.62 ng/ml

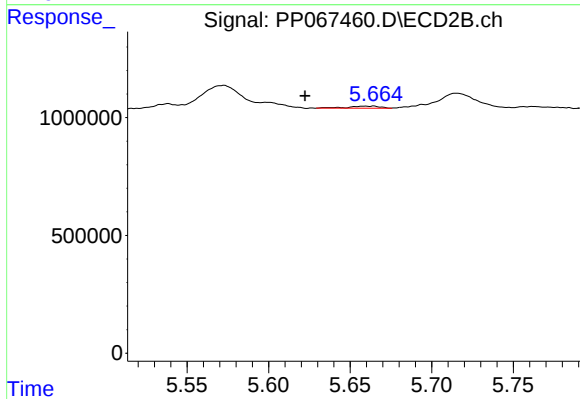

#24 AR-1248-4


R.T.: 5.664 min
Delta R.T.: 0.042 min
Response: 121291
Conc: 2.23 ng/ml

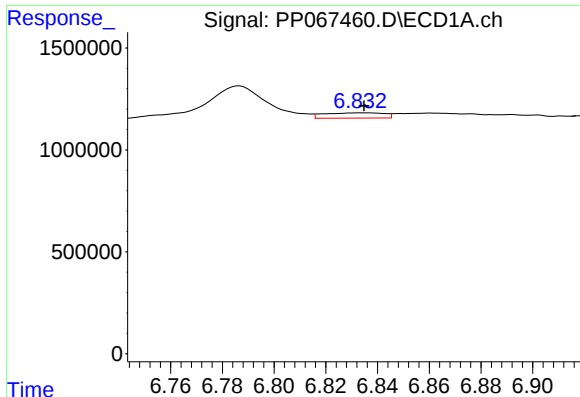

#25 AR-1248-5


R.T.: 6.833 min
Delta R.T.: -0.002 min
Response: 417867
Conc: 7.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGE

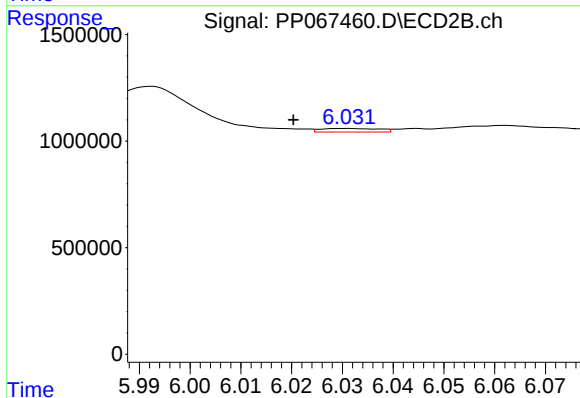


#25 AR-1248-5

R.T.: 6.031 min
Delta R.T.: 0.010 min
Response: 135316
Conc: 2.78 ng/ml

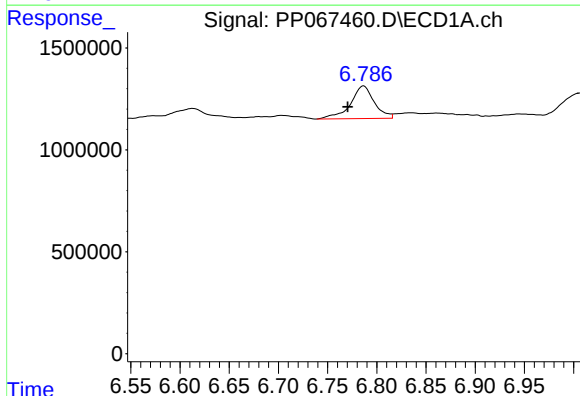


#26 AR-1254-1

R.T.: 6.787 min
Delta R.T.: 0.016 min
Response: 2692131
Conc: 43.21 ng/ml

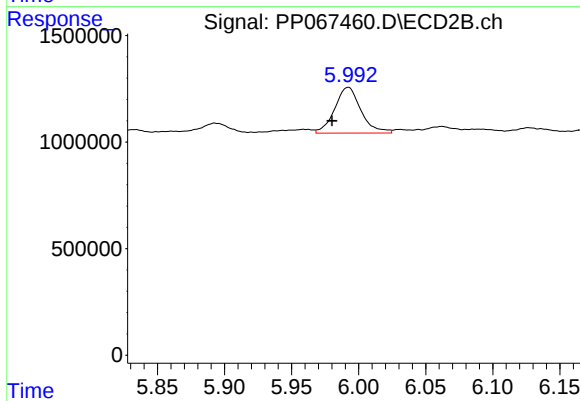

#26 AR-1254-1


R.T.: 5.992 min
Delta R.T.: 0.012 min
Response: 2927414
Conc: 36.11 ng/ml

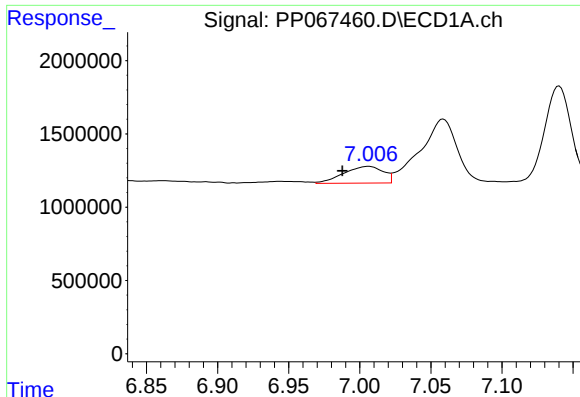

#27 AR-1254-2


R.T.: 7.006 min
Delta R.T.: 0.018 min
Response: 2223381
Conc: 24.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGE

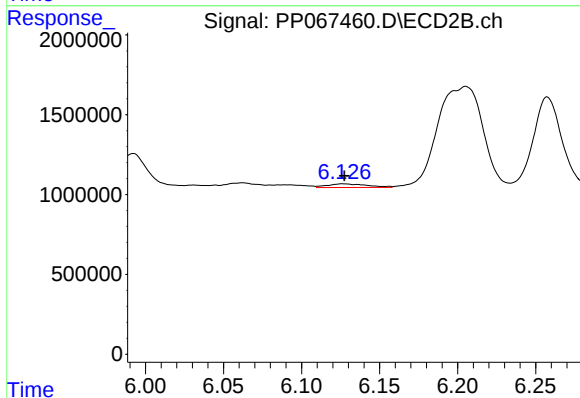


#27 AR-1254-2

R.T.: 6.127 min
Delta R.T.: 0.000 min
Response: 405179
Conc: 5.52 ng/ml

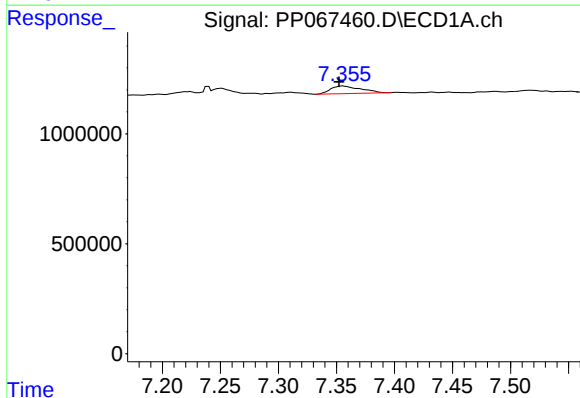


#28 AR-1254-3

R.T.: 7.355 min
Delta R.T.: 0.003 min
Response: 633892
Conc: 6.76 ng/ml

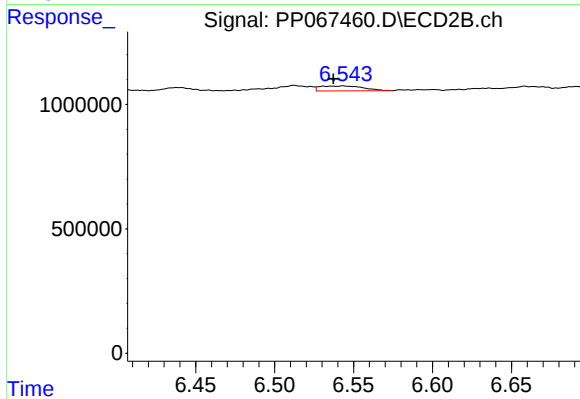

#28 AR-1254-3


R.T.: 6.544 min
Delta R.T.: 0.006 min
Response: 378440
Conc: 3.32 ng/ml

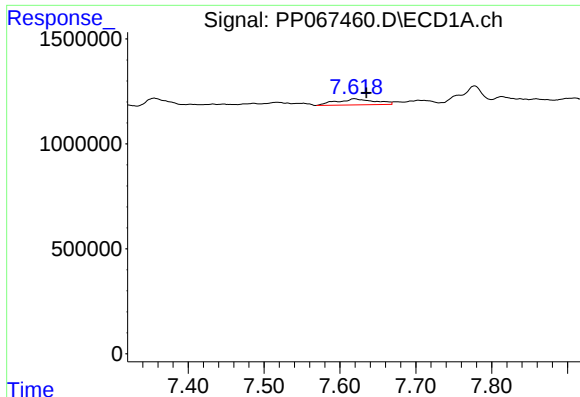

#29 AR-1254-4


R.T.: 7.619 min
Delta R.T.: -0.016 min
Response: 1006988
Conc: 15.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGE

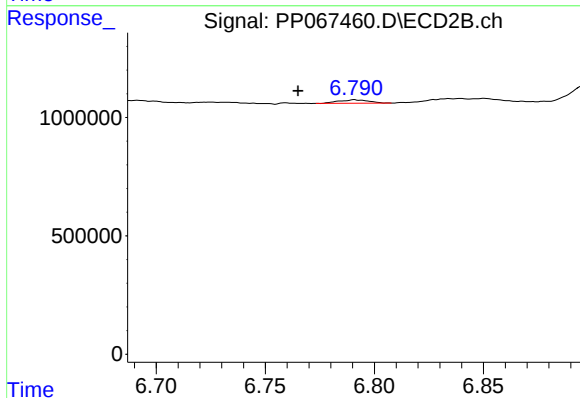


#29 AR-1254-4

R.T.: 6.791 min
Delta R.T.: 0.026 min
Response: 138248
Conc: 2.21 ng/ml

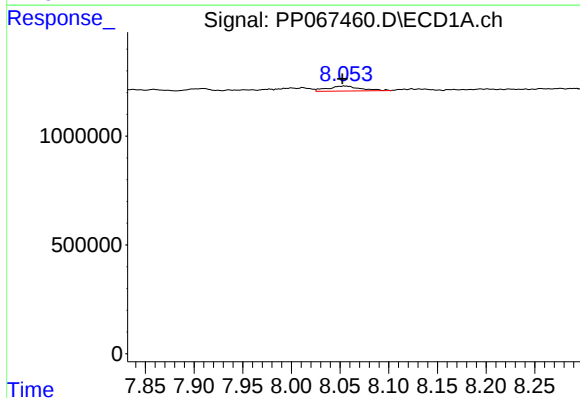


#30 AR-1254-5

R.T.: 8.055 min
Delta R.T.: 0.003 min
Response: 545655
Conc: 6.64 ng/ml

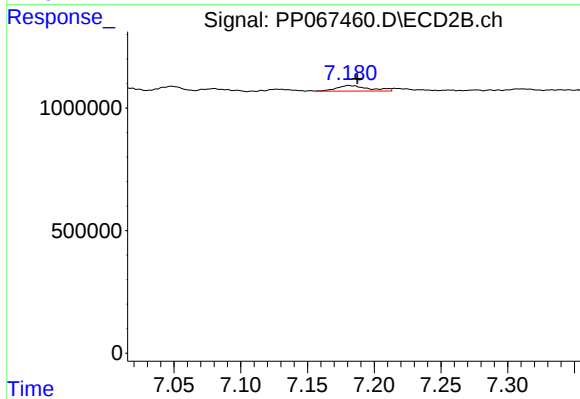

#30 AR-1254-5


R.T.: 7.181 min
Delta R.T.: -0.006 min
Response: 382006
Conc: 3.72 ng/ml

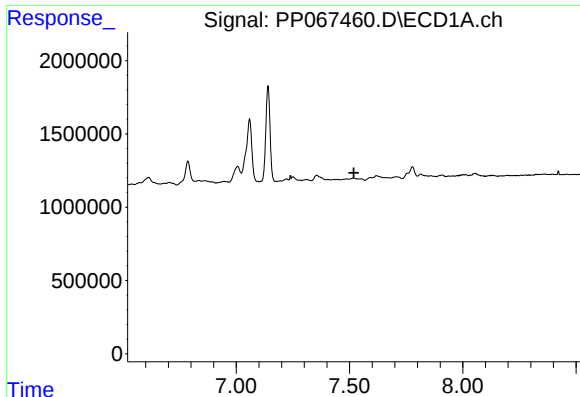

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.518 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGE

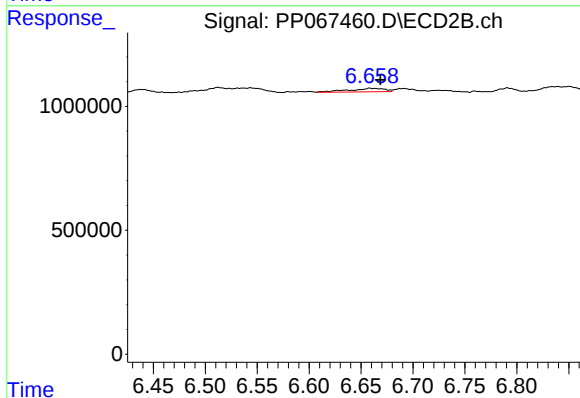


#31 AR-1260-1

R.T.: 6.658 min
Delta R.T.: -0.010 min
Response: 324151
Conc: 3.96 ng/ml

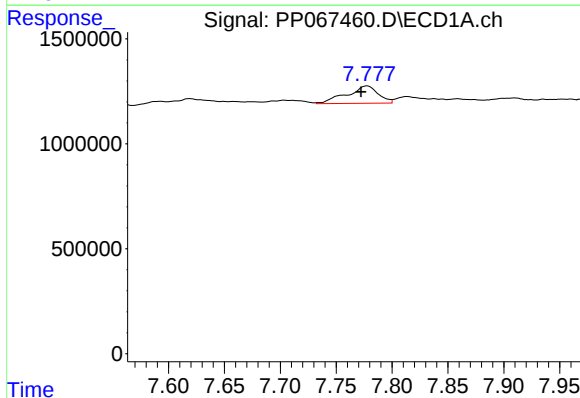


#32 AR-1260-2

R.T.: 7.778 min
Delta R.T.: 0.005 min
Response: 1629773
Conc: 17.88 ng/ml

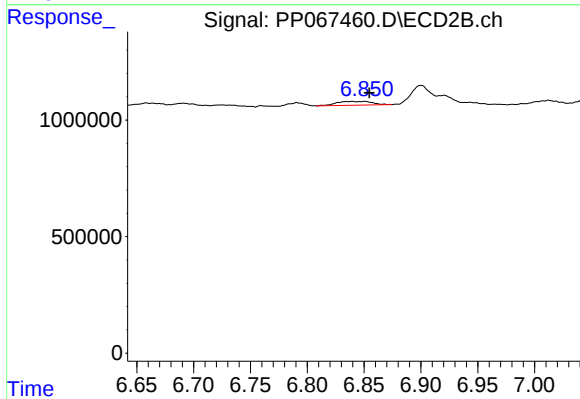

#32 AR-1260-2


R.T.: 6.850 min
Delta R.T.: -0.004 min
Response: 356206
Conc: 3.79 ng/ml

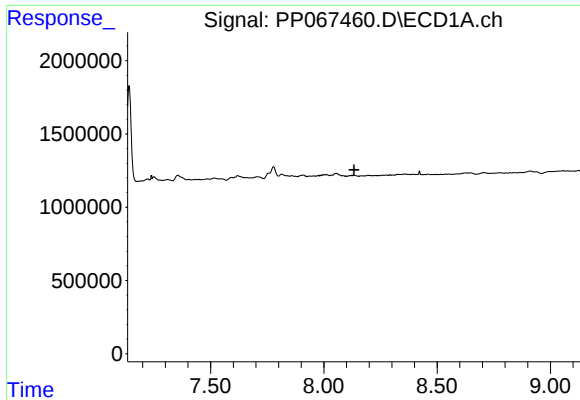

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 8.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGE

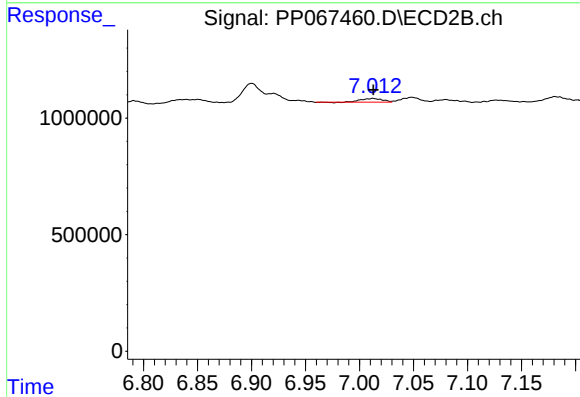


#33 AR-1260-3

R.T.: 7.013 min
Delta R.T.: 0.000 min
Response: 207092
Conc: 2.29 ng/ml

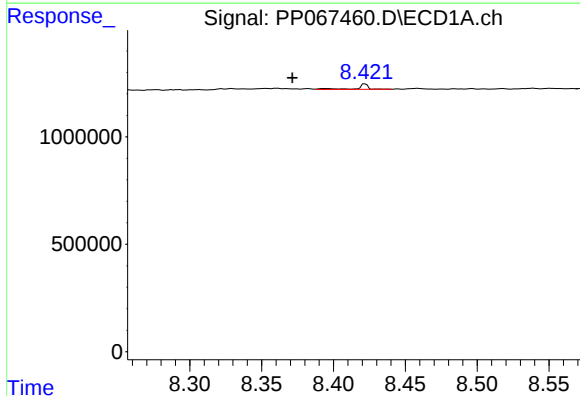


#34 AR-1260-4

R.T.: 8.422 min
Delta R.T.: 0.051 min
Response: 139211
Conc: 1.84 ng/ml

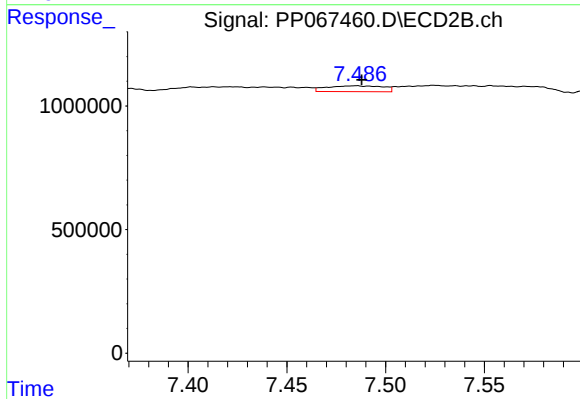

#34 AR-1260-4


R.T.: 7.485 min
Delta R.T.: -0.003 min
Response: 468065
Conc: 7.02 ng/ml

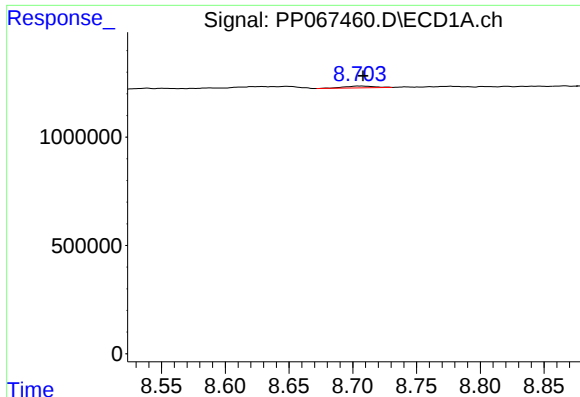

#35 AR-1260-5


R.T.: 8.706 min
Delta R.T.: -0.002 min
Response: 140561
Conc: 1.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGE

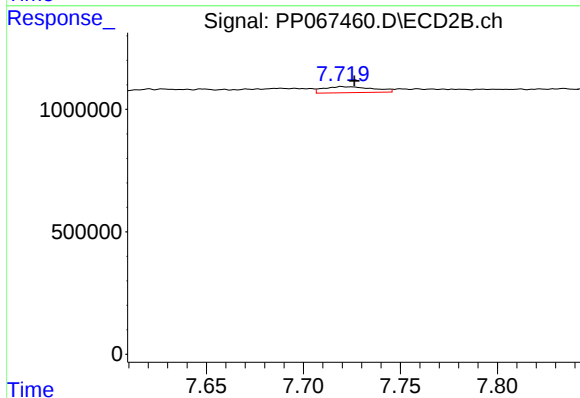


#35 AR-1260-5

R.T.: 7.720 min
Delta R.T.: -0.006 min
Response: 440972
Conc: 3.03 ng/ml

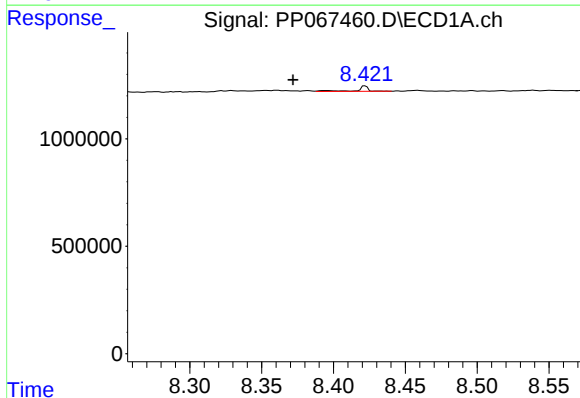


#36 AR-1262-1

R.T.: 8.422 min
Delta R.T.: 0.050 min
Response: 139211
Conc: 1.46 ng/ml

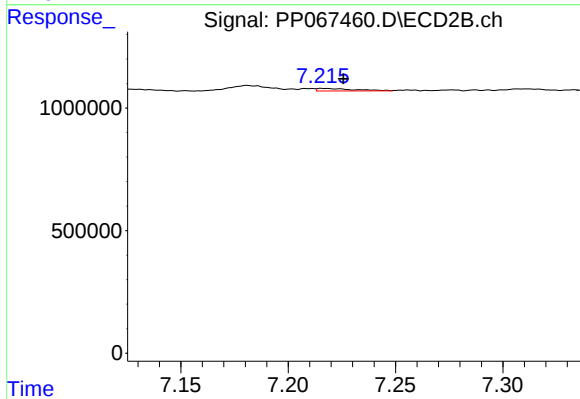

#36 AR-1262-1


R.T.: 7.216 min
Delta R.T.: -0.010 min
Response: 119185
Conc: 1.13 ng/ml

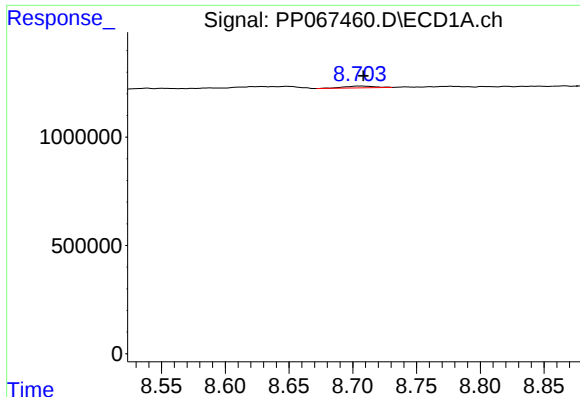

#37 AR-1262-2


R.T.: 8.706 min
Delta R.T.: -0.002 min
Response: 140561
Conc: 0.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGE

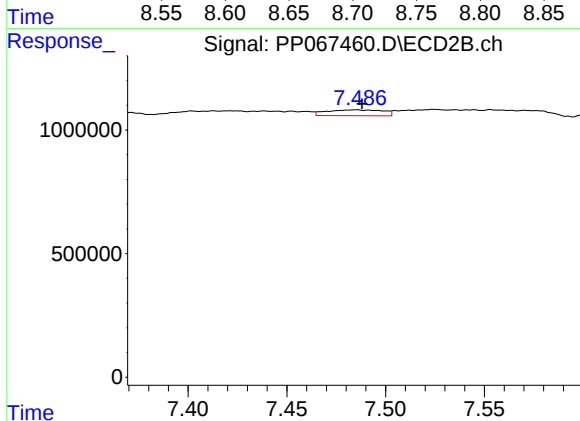


#37 AR-1262-2

R.T.: 7.485 min
Delta R.T.: -0.003 min
Response: 468065
Conc: 4.94 ng/ml

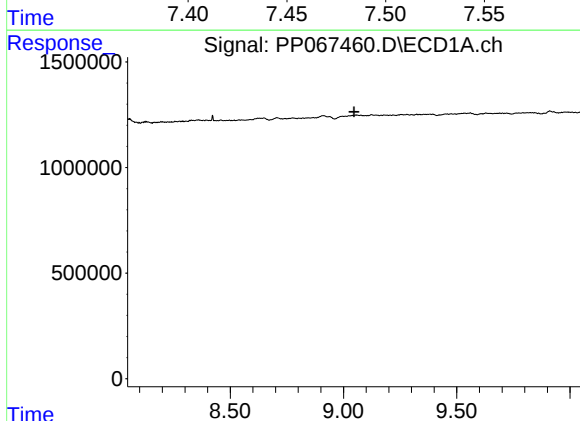


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 9.046 min
Response: 0
Conc: N.D.

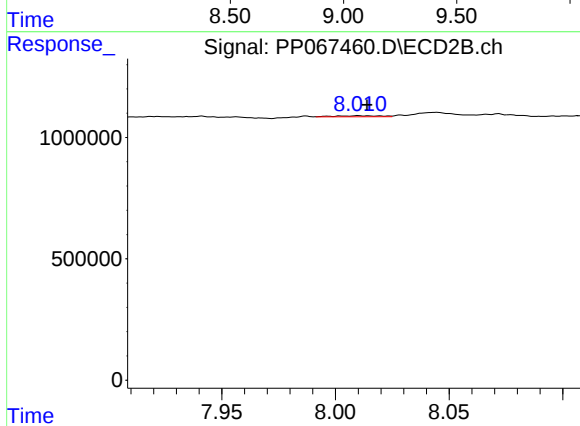

#38 AR-1262-3


R.T.: 8.010 min
Delta R.T.: -0.004 min
Response: 60959
Conc: 0.83 ng/ml

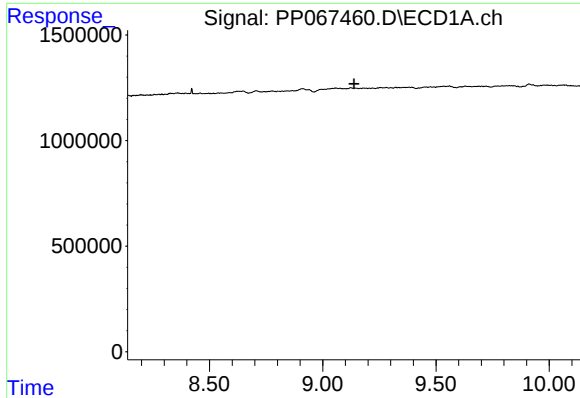

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 9.138 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGE

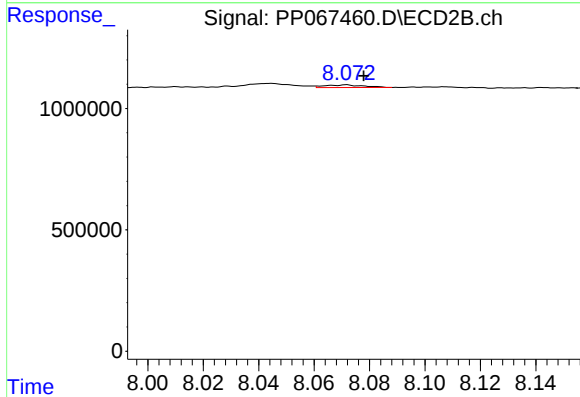


#39 AR-1262-4

R.T.: 8.072 min
Delta R.T.: -0.006 min
Response: 105800
Conc: 0.80 ng/ml

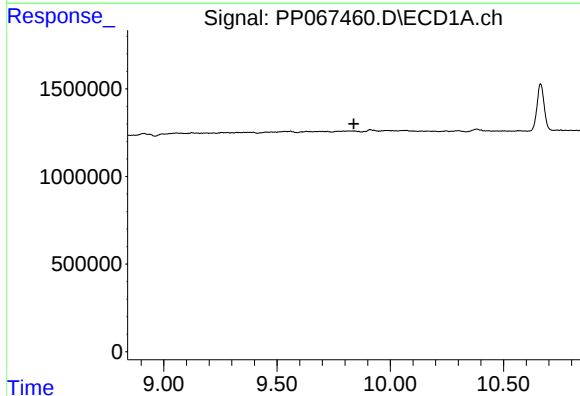


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.839 min
Response: 0
Conc: N.D.

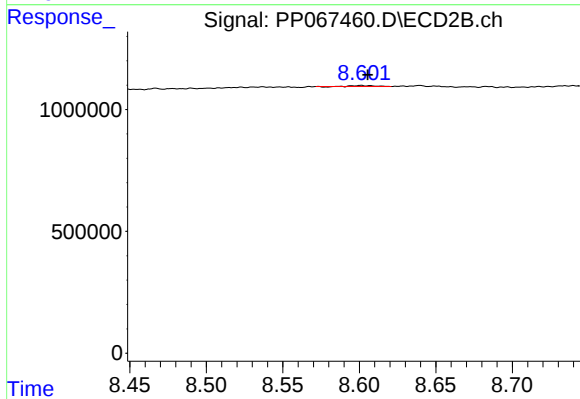

#40 AR-1262-5


R.T.: 8.601 min
Delta R.T.: -0.004 min
Response: 43065
Conc: 0.71 ng/ml

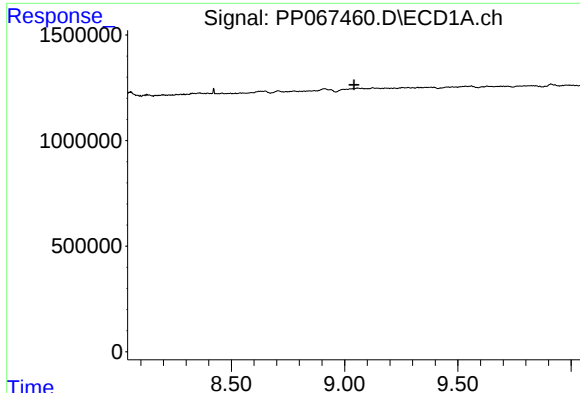

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 9.042 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGE

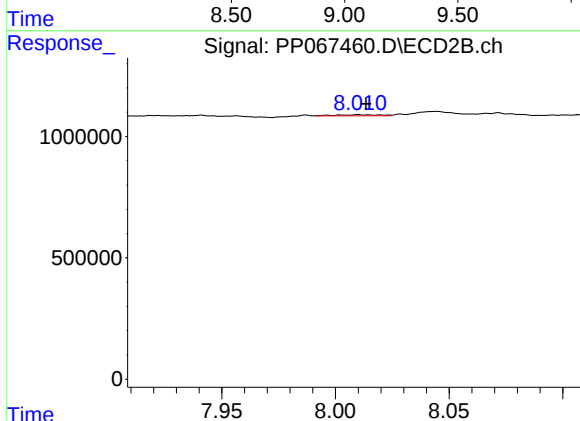


#41 AR-1268-1

R.T.: 8.010 min
Delta R.T.: -0.003 min
Response: 60959
Conc: 0.30 ng/ml

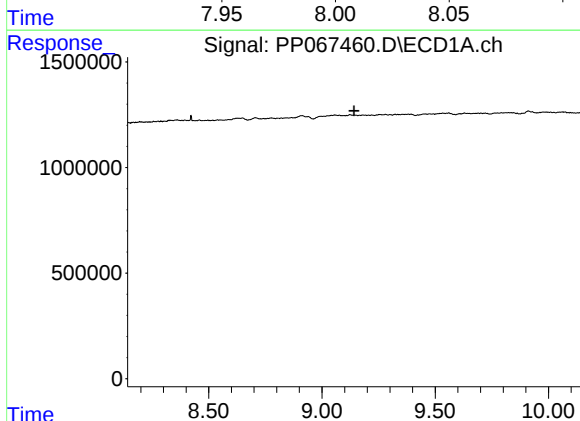


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 9.141 min
Response: 0
Conc: N.D.

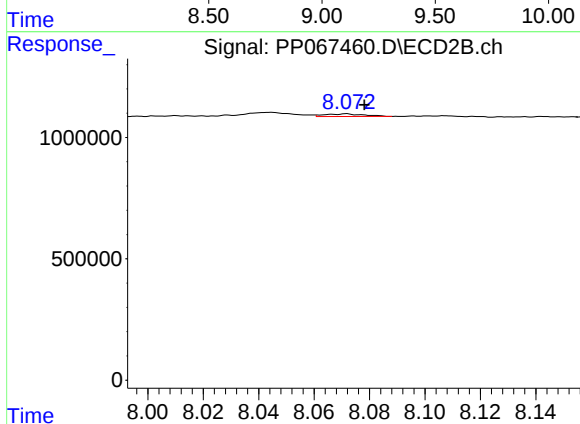

#42 AR-1268-2


R.T.: 8.072 min
Delta R.T.: -0.007 min
Response: 105800
Conc: 0.59 ng/ml

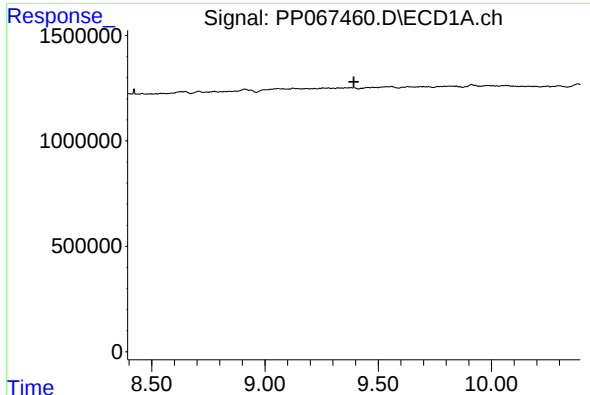

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.392 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGE

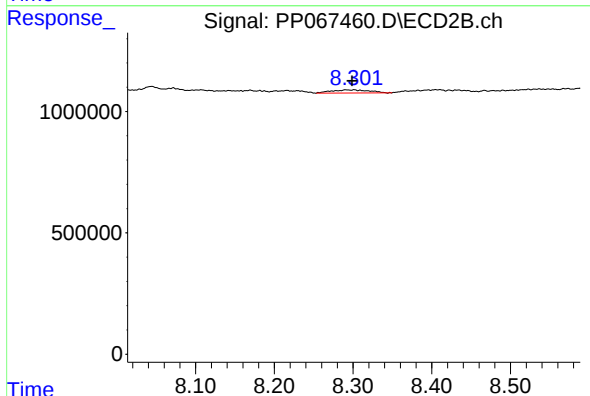


#43 AR-1268-3

R.T.: 8.291 min
Delta R.T.: -0.008 min
Response: 438768
Conc: 2.76 ng/ml

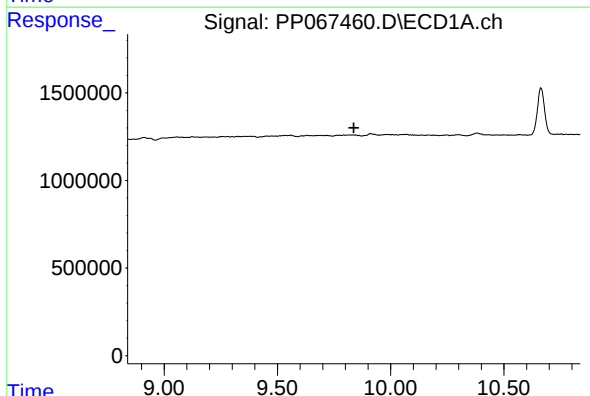


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.838 min
Response: 0
Conc: N.D.

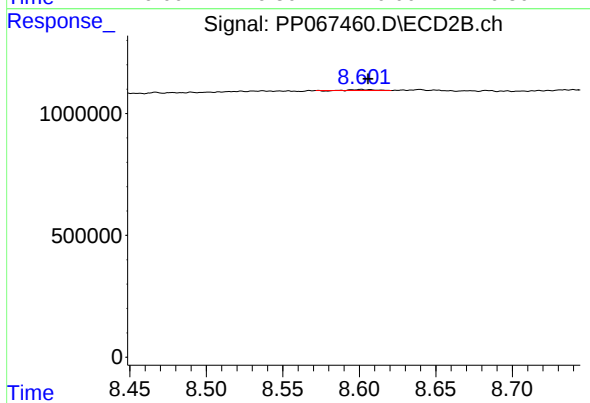

#44 AR-1268-4


R.T.: 8.601 min
Delta R.T.: -0.004 min
Response: 43065
Conc: 0.67 ng/ml

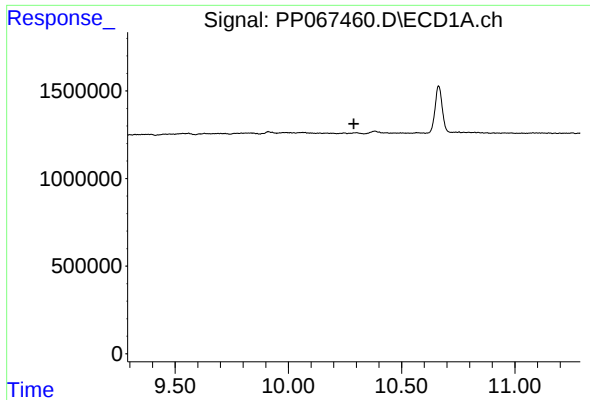

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.289 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGE

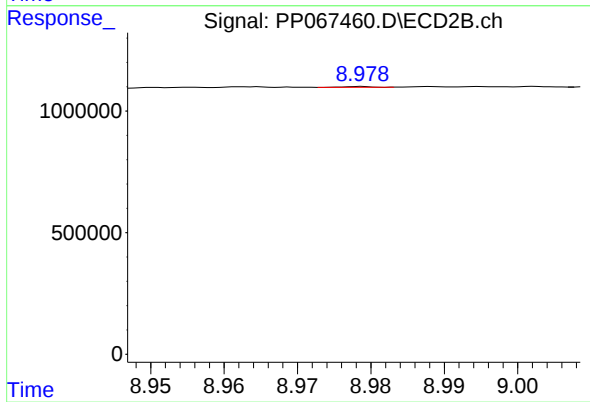

#45 AR-1268-5

R.T.: 8.979 min
Delta R.T.: 0.045 min
Response: 7232
Conc: 0.02 ng/ml