

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100324\
 Data File : PP067461.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2024 11:19
 Operator : YP\AJ
 Sample : P4254-01RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MH-147-SLUDGERE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/04/2024
 Supervised By :Ankita Jodhani 10/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 09:05:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 27 06:59:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.751	4.050	8082153	8576439	6.013m	5.740
2) SA Decachlor...	10.661	9.216	5900161	5801865	4.064	4.210
Target Compounds						
3) L1 AR-1016-1	5.874f	5.098f	2751091	495247	57.699	9.602 #
4) L1 AR-1016-2	5.979f	5.241f	241108	911523	3.482	12.820 #
5) L1 AR-1016-3	5.979	5.360	241108	583081	5.398	14.651 #
6) L1 AR-1016-4	6.086	5.404	1410595	526008	39.254	15.234 #
7) L1 AR-1016-5	6.363	5.658	1273838	102843	34.568	2.397 #
8) L2 AR-1221-1	4.957	0.000	730970	0	43.664	N.D. #
9) L2 AR-1221-2	5.055	4.358	137997	236632	10.892	16.129 #
10) L2 AR-1221-3	5.063f	4.423	87270	163961	2.255	3.781 #
11) L3 AR-1232-1	5.063f	4.423	87270	163961	2.722	4.558 #
12) L3 AR-1232-2	5.644	5.241f	503660	911523	28.296	27.516
13) L3 AR-1232-3	5.979f	5.360	241108	583081	7.627	32.455 #
14) L3 AR-1232-4	6.086	5.487f	1410595	159569	87.414	9.124 #
15) L3 AR-1232-5	6.204	5.658f	296316	102843	21.903	5.477 #
16) L4 AR-1242-1	5.874f	5.098f	2751091	495247	77.359	12.915 #
17) L4 AR-1242-2	5.979f	5.241f	241108	911523	4.608	17.406 #
18) L4 AR-1242-3	5.979	5.360	241108	583081	7.075	19.619 #
19) L4 AR-1242-4	6.086	5.487f	1410595	159569	51.433	4.959 #
20) L4 AR-1242-5	6.833	5.990	1065699	3529472	35.808	92.447 #
21) L5 AR-1248-1	5.874f	5.098f	2751091	495247	97.435	16.171 #
22) L5 AR-1248-2	6.204	5.404	296316	526008	6.675	11.594 #
23) L5 AR-1248-3	6.363	5.487f	1273838	159569	26.252	3.371 #
24) L5 AR-1248-4	6.785	5.658f	4177414	102843	76.989	1.894 #
25) L5 AR-1248-5	6.833	6.029	1065699	215057	19.326	4.412 #
26) L6 AR-1254-1	6.785	5.990	4177414	3529472	67.050	43.541 #
27) L6 AR-1254-2	7.004	6.128	3278627	777994	36.134	10.608 #
28) L6 AR-1254-3	7.352	6.541	2055225	725707	21.911	6.365 #
29) L6 AR-1254-4	7.621	6.790	1543587	155002	23.162	2.483 #
30) L6 AR-1254-5	8.051	7.181	481297	320468	5.855	3.121 #
31) L7 AR-1260-1	7.518	6.662	1308655	743305	16.611	9.086 #
32) L7 AR-1260-2	7.776	6.832	1830195	590410	20.080	6.285 #
33) L7 AR-1260-3	0.000	7.008	0	290927	N.D.	3.211 #
34) L7 AR-1260-4	0.000	7.480	0	501324	N.D.	7.518 #
35) L7 AR-1260-5	8.704	7.720	179160	522668	1.384	3.590 #
36) L8 AR-1262-1	0.000	7.210	0	165523	N.D.	1.574 #
37) L8 AR-1262-2	8.704	7.480	179160	501324	1.104	5.295 #
38) L8 AR-1262-3	0.000	8.043	0	342937	N.D.	4.675 #
39) L8 AR-1262-4	0.000	8.065	0	112427	N.D.	0.853 #
41) L9 AR-1268-1	0.000	8.043	0	342937	N.D.	1.703 #
42) L9 AR-1268-2	0.000	8.065	0	112427	N.D.	0.629 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100324\
 Data File : PP067461.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2024 11:19
 Operator : YP\AJ
 Sample : P4254-01RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MH-147-SLUDGERE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/04/2024
 Supervised By :Ankita Jodhani 10/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 09:05:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 27 06:59:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	0.000	8.290	0	495833	N.D.	3.121 #
45) L9	AR-1268-5	0.000	8.911	0	184280	N.D.	0.417 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100324\
Data File : PP067461.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2024 11:19
Operator : YP\AJ
Sample : P4254-01RE
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGERE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/04/2024
Supervised By :Ankita Jodhani 10/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 09:05:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092624.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 27 06:59:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

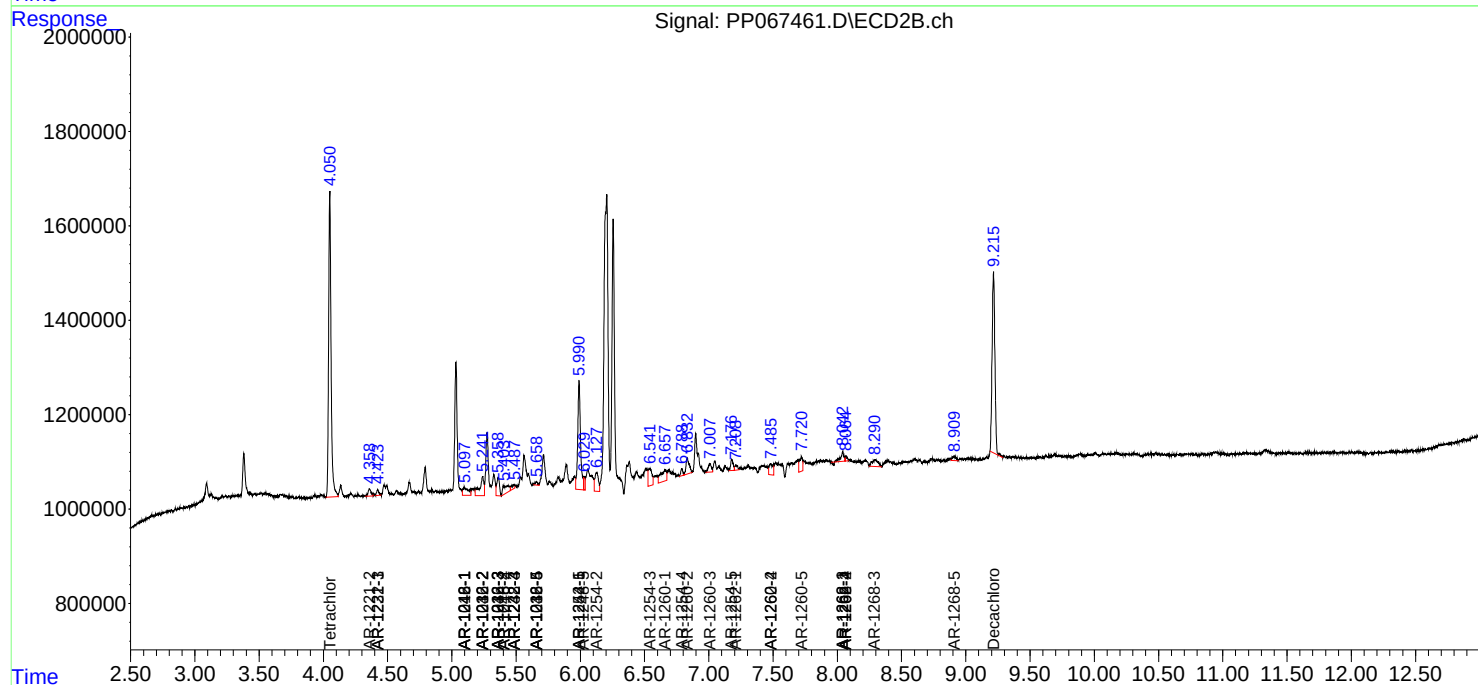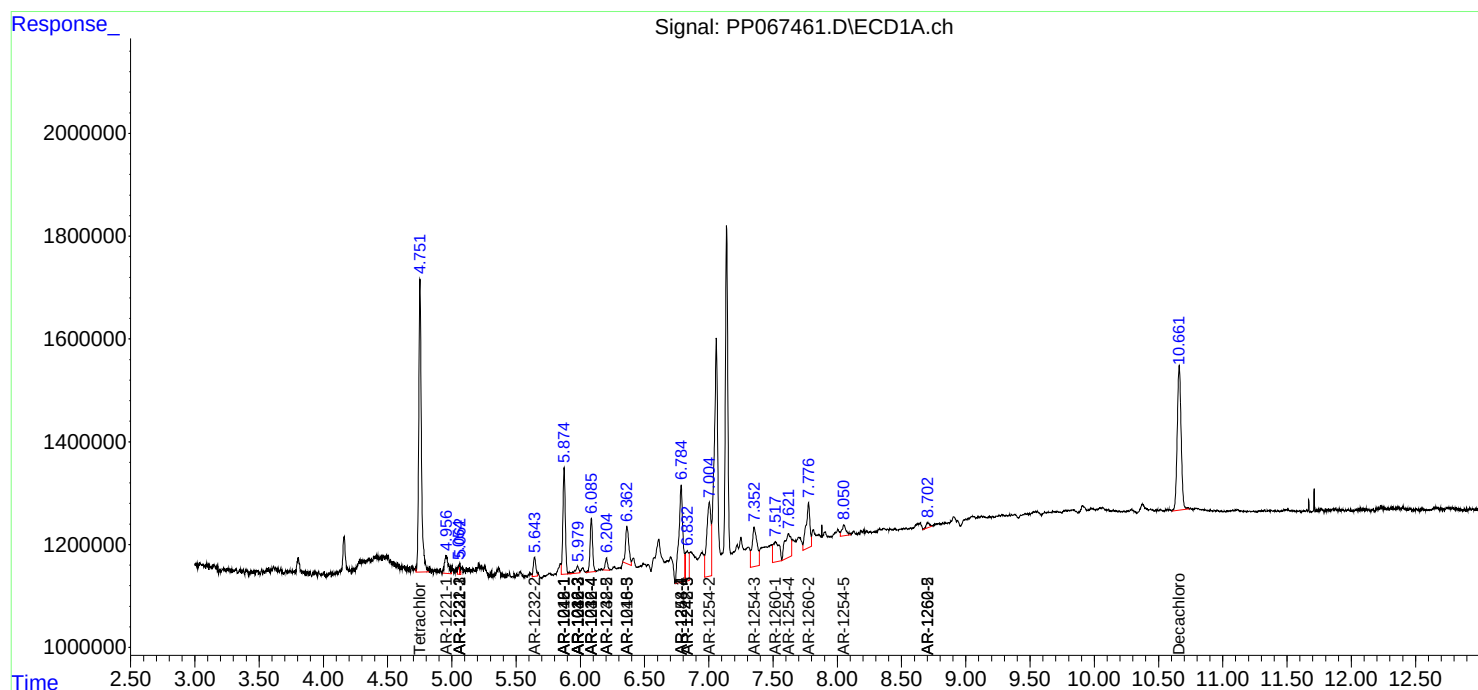

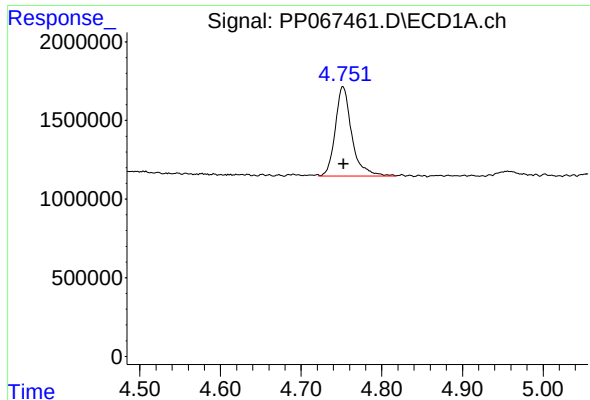


#1 Tetrachloro-m-xylene

R.T.: 4.751 min
Delta R.T.: -0.002 min
Response: 8082153
Conc: 6.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGERE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/04/2024
Supervised By :Ankita Jodhani 10/04/2024

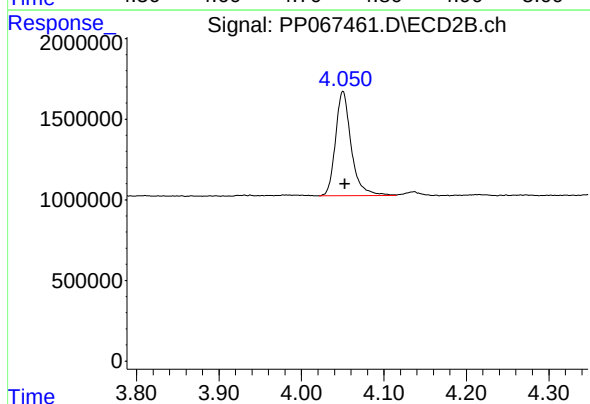


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.003 min
Response: 8576439
Conc: 5.74 ng/ml

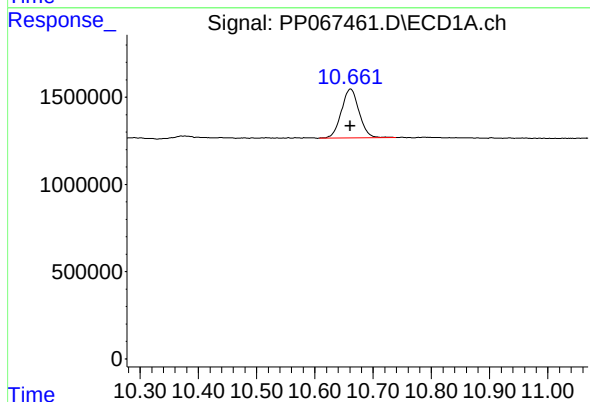


#2 Decachlorobiphenyl

R.T.: 10.661 min
Delta R.T.: 0.000 min
Response: 5900161
Conc: 4.06 ng/ml

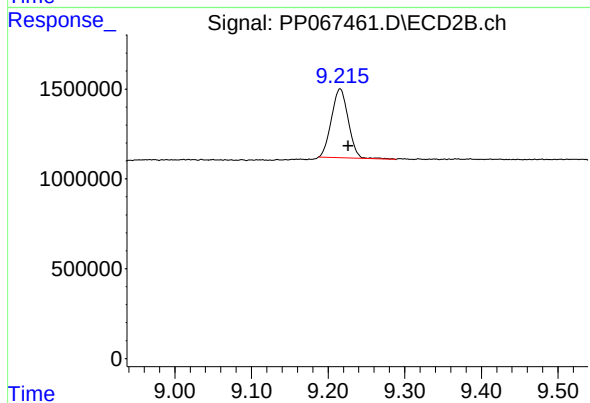

#2 Decachlorobiphenyl

R.T.: 9.216 min
Delta R.T.: -0.011 min
Response: 5801865
Conc: 4.21 ng/ml

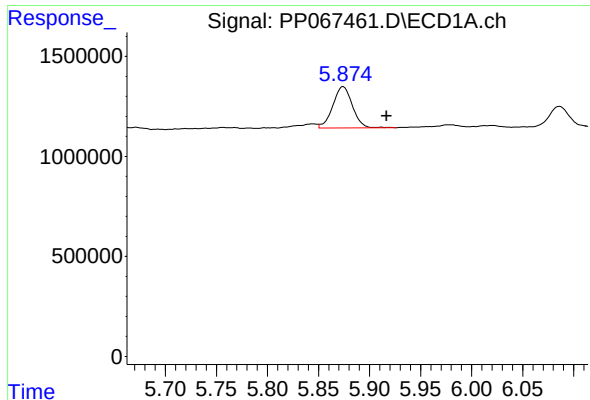


#3 AR-1016-1

R.T.: 5.874 min
Delta R.T.: -0.042 min
Response: 2751091
Conc: 57.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGERE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/04/2024
Supervised By :Ankita Jodhani 10/04/2024

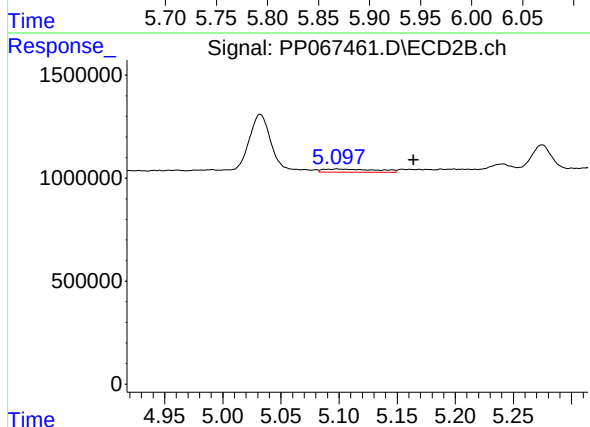


#3 AR-1016-1

R.T.: 5.098 min
Delta R.T.: -0.066 min
Response: 495247
Conc: 9.60 ng/ml

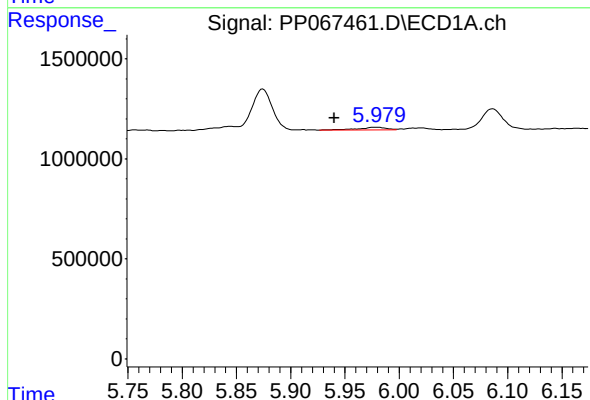


#4 AR-1016-2

R.T.: 5.979 min
Delta R.T.: 0.038 min
Response: 241108
Conc: 3.48 ng/ml

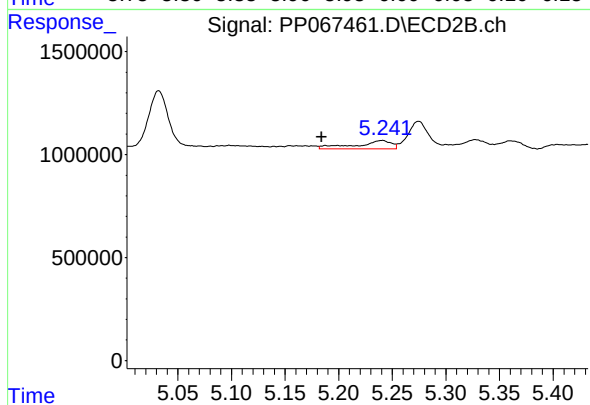

#4 AR-1016-2

R.T.: 5.241 min
Delta R.T.: 0.057 min
Response: 911523
Conc: 12.82 ng/ml

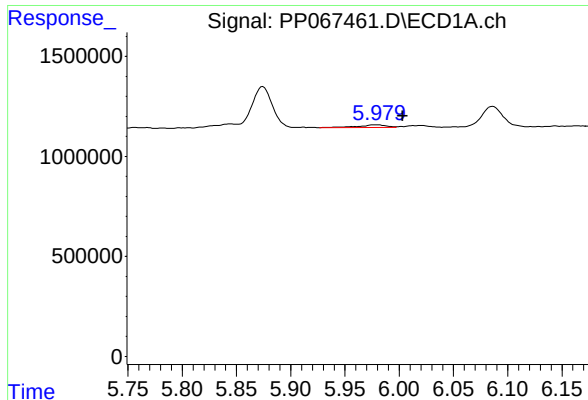


#5 AR-1016-3

R.T.: 5.979 min
Delta R.T.: -0.025 min
Response: 241108
Conc: 5.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGERE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/04/2024
Supervised By :Ankita Jodhani 10/04/2024

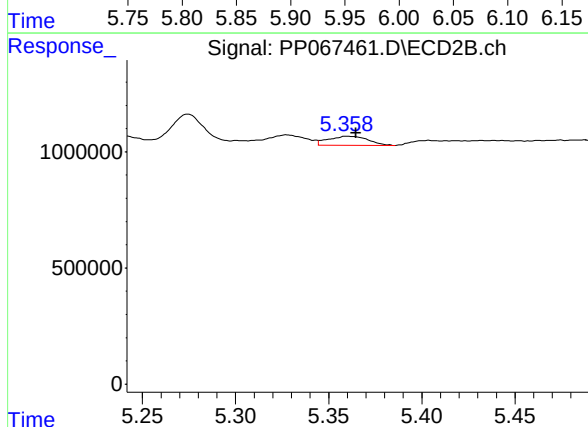


#5 AR-1016-3

R.T.: 5.360 min
Delta R.T.: -0.004 min
Response: 583081
Conc: 14.65 ng/ml

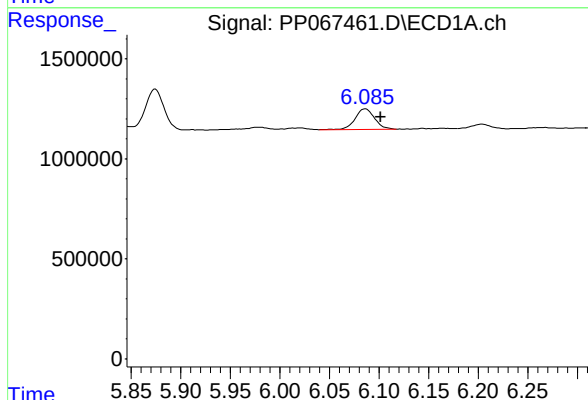


#6 AR-1016-4

R.T.: 6.086 min
Delta R.T.: -0.015 min
Response: 1410595
Conc: 39.25 ng/ml

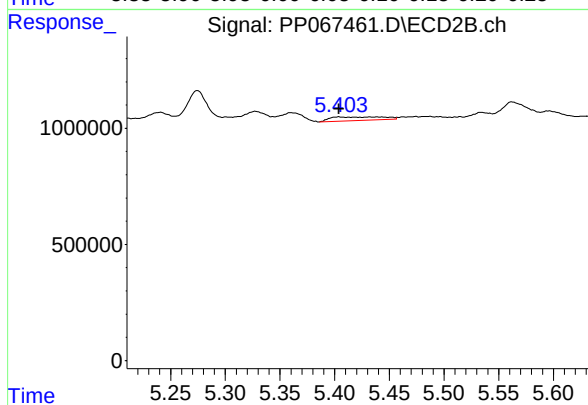

#6 AR-1016-4

R.T.: 5.404 min
Delta R.T.: 0.000 min
Response: 526008
Conc: 15.23 ng/ml

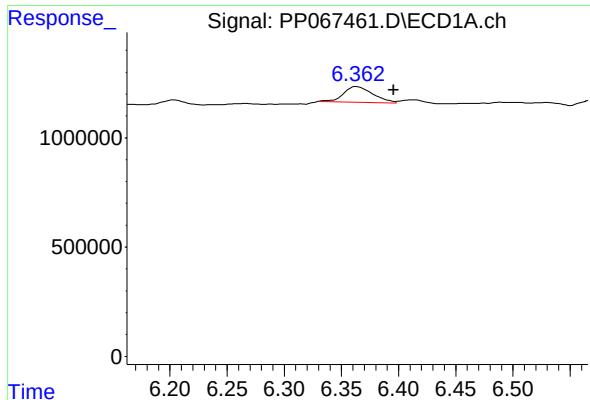


#7 AR-1016-5

R.T.: 6.363 min
Delta R.T.: -0.033 min
Response: 1273838
Conc: 34.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGERE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/04/2024
Supervised By :Ankita Jodhani 10/04/2024

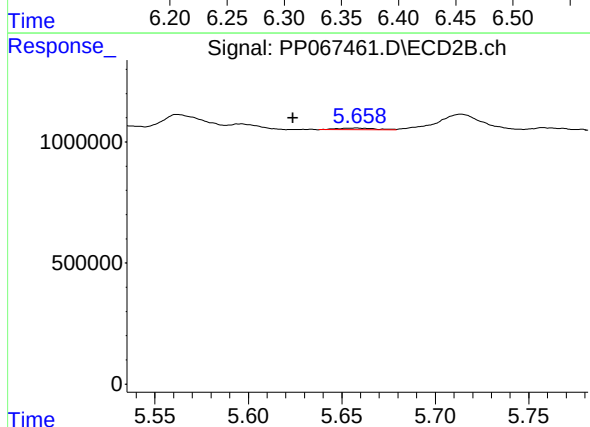


#7 AR-1016-5

R.T.: 5.658 min
Delta R.T.: 0.034 min
Response: 102843
Conc: 2.40 ng/ml

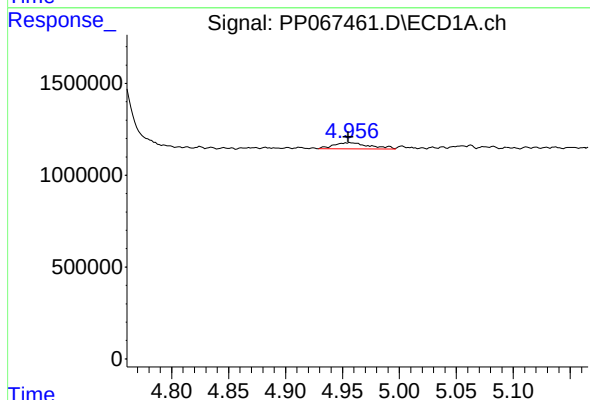


#8 AR-1221-1

R.T.: 4.957 min
Delta R.T.: 0.002 min
Response: 730970
Conc: 43.66 ng/ml

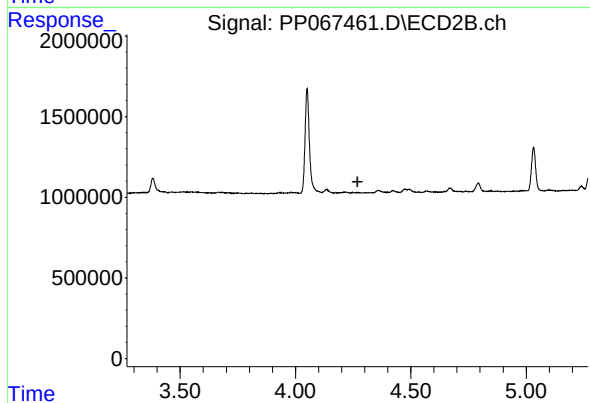

#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.269 min
Response: 0
Conc: N.D.

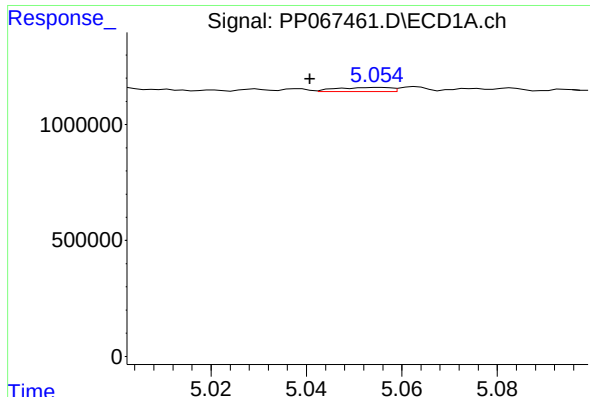


#9 AR-1221-2

R.T.: 5.055 min
Delta R.T.: 0.014 min
Response: 137997
Conc: 10.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGERE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/04/2024
Supervised By :Ankita Jodhani 10/04/2024

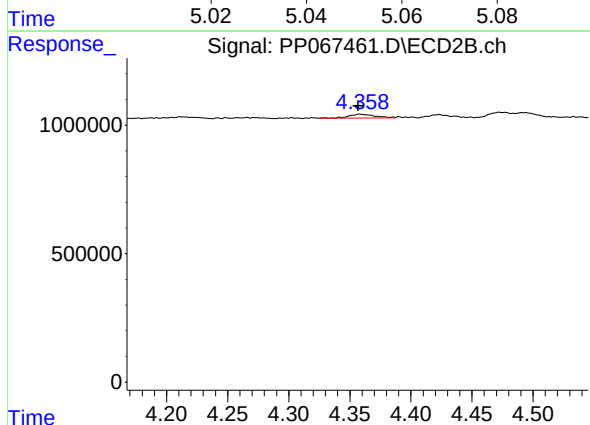


#9 AR-1221-2

R.T.: 4.358 min
Delta R.T.: 0.001 min
Response: 236632
Conc: 16.13 ng/ml

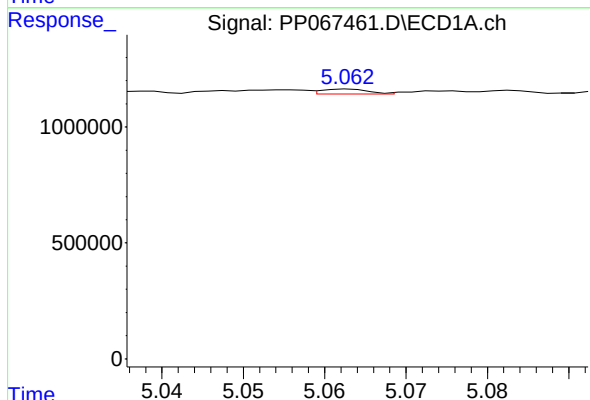


#10 AR-1221-3

R.T.: 5.063 min
Delta R.T.: -0.055 min
Response: 87270
Conc: 2.25 ng/ml

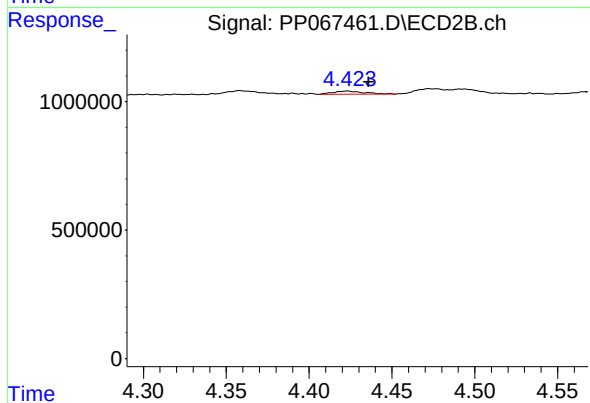

#10 AR-1221-3

R.T.: 4.423 min
Delta R.T.: -0.013 min
Response: 163961
Conc: 3.78 ng/ml

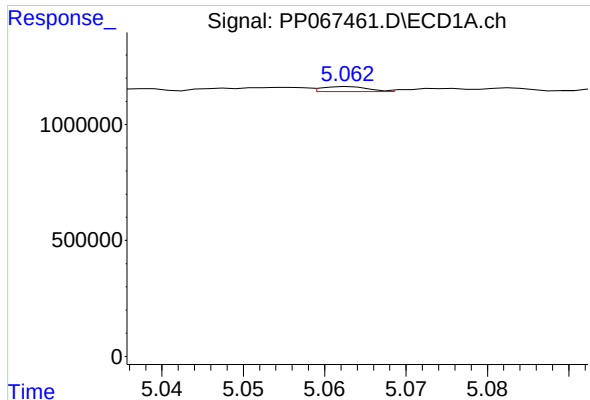


#11 AR-1232-1

R.T.: 5.063 min
Delta R.T.: -0.055 min
Response: 87270
Conc: 2.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGERE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/04/2024
Supervised By :Ankita Jodhani 10/04/2024

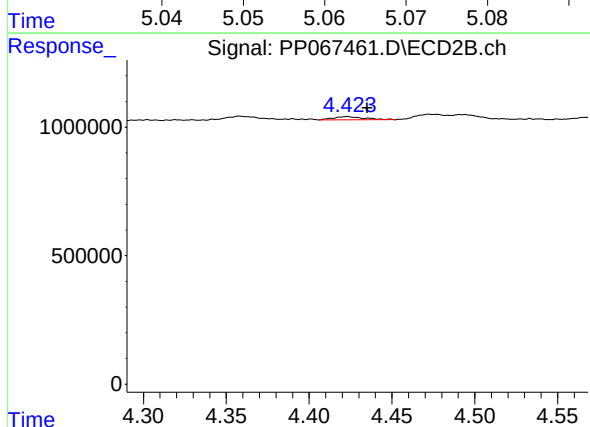


#11 AR-1232-1

R.T.: 4.423 min
Delta R.T.: -0.012 min
Response: 163961
Conc: 4.56 ng/ml

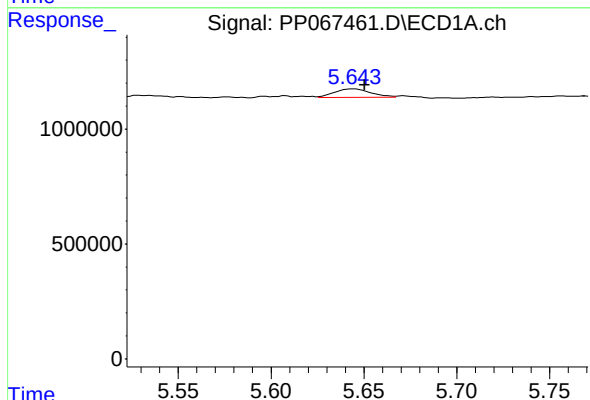


#12 AR-1232-2

R.T.: 5.644 min
Delta R.T.: -0.006 min
Response: 503660
Conc: 28.30 ng/ml

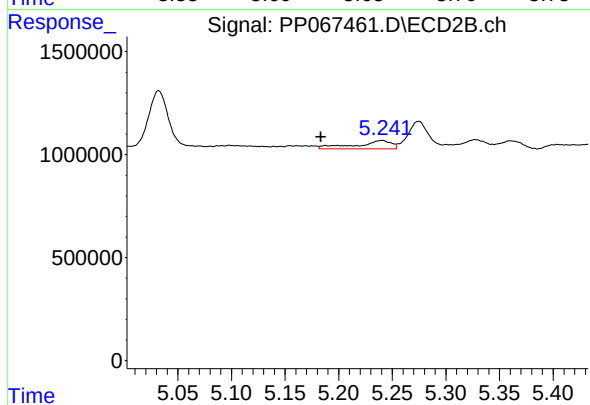

#12 AR-1232-2

R.T.: 5.241 min
Delta R.T.: 0.057 min
Response: 911523
Conc: 27.52 ng/ml

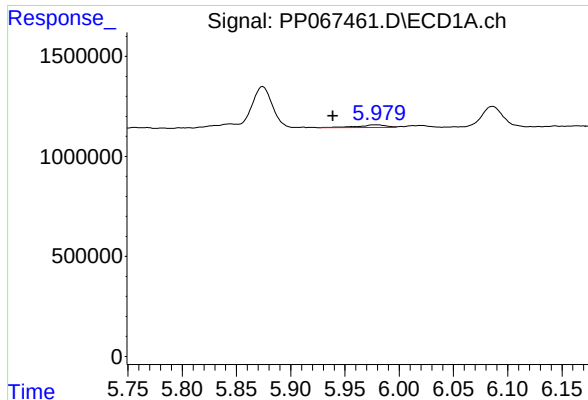


#13 AR-1232-3

R.T.: 5.979 min
Delta R.T.: 0.040 min
Response: 241108
Conc: 7.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGERE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/04/2024
Supervised By :Ankita Jodhani 10/04/2024

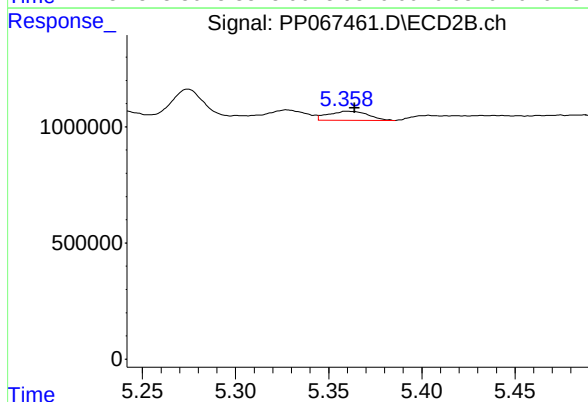


#13 AR-1232-3

R.T.: 5.360 min
Delta R.T.: -0.004 min
Response: 583081
Conc: 32.46 ng/ml

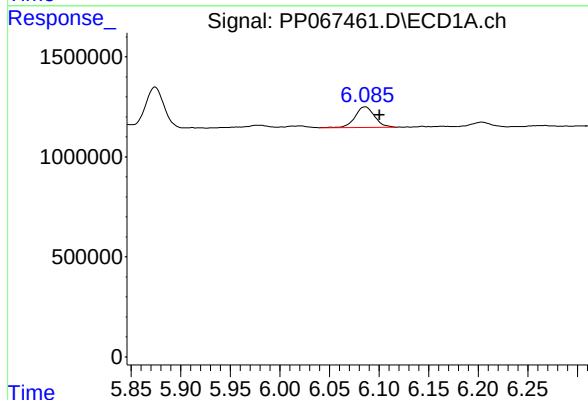


#14 AR-1232-4

R.T.: 6.086 min
Delta R.T.: -0.014 min
Response: 1410595
Conc: 87.41 ng/ml

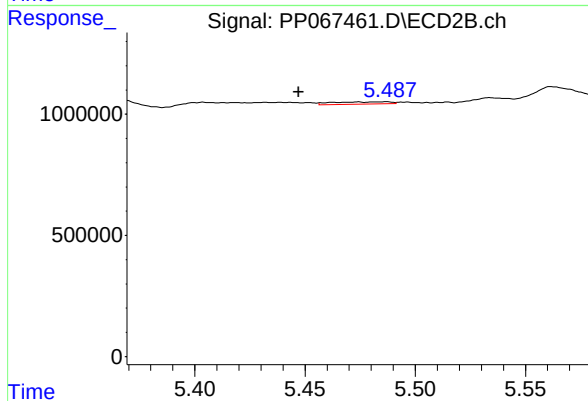

#14 AR-1232-4

R.T.: 5.487 min
Delta R.T.: 0.040 min
Response: 159569
Conc: 9.12 ng/ml

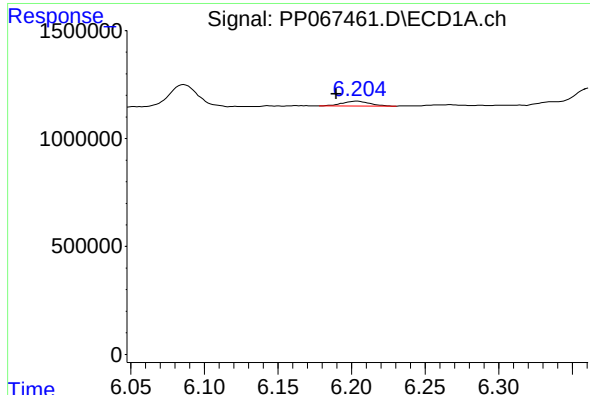


#15 AR-1232-5

R.T.: 6.204 min
Delta R.T.: 0.014 min
Response: 296316
Conc: 21.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGERE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/04/2024
Supervised By :Ankita Jodhani 10/04/2024

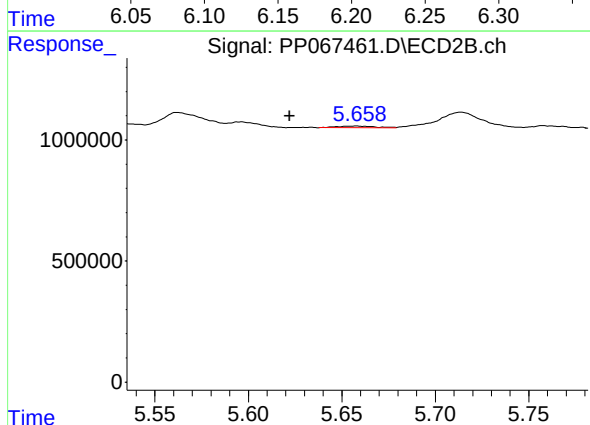


#15 AR-1232-5

R.T.: 5.658 min
Delta R.T.: 0.036 min
Response: 102843
Conc: 5.48 ng/ml

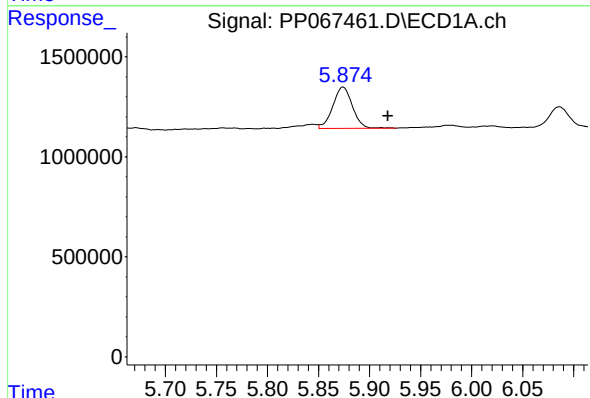


#16 AR-1242-1

R.T.: 5.874 min
Delta R.T.: -0.044 min
Response: 2751091
Conc: 77.36 ng/ml

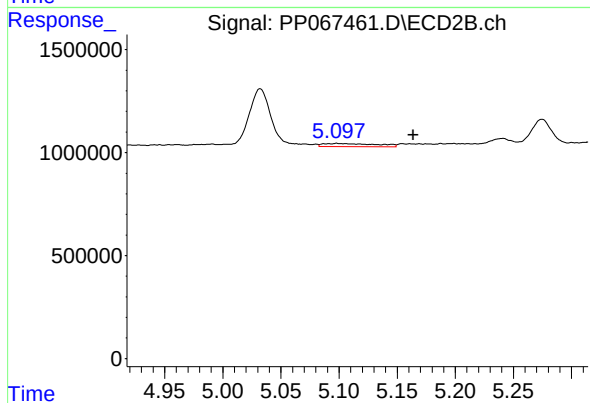

#16 AR-1242-1

R.T.: 5.098 min
Delta R.T.: -0.066 min
Response: 495247
Conc: 12.92 ng/ml

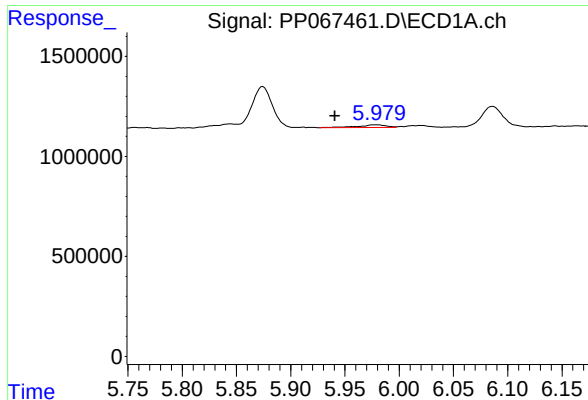


#17 AR-1242-2

R.T.: 5.979 min
Delta R.T.: 0.038 min
Response: 241108
Conc: 4.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGERE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/04/2024
Supervised By :Ankita Jodhani 10/04/2024

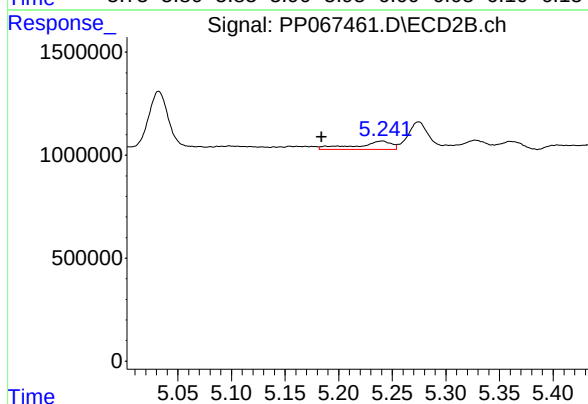


#17 AR-1242-2

R.T.: 5.241 min
Delta R.T.: 0.057 min
Response: 911523
Conc: 17.41 ng/ml

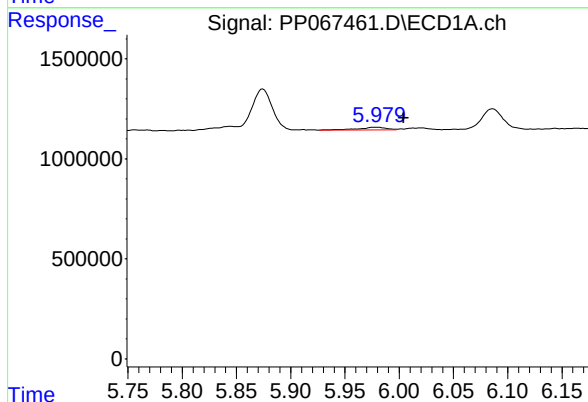


#18 AR-1242-3

R.T.: 5.979 min
Delta R.T.: -0.025 min
Response: 241108
Conc: 7.07 ng/ml

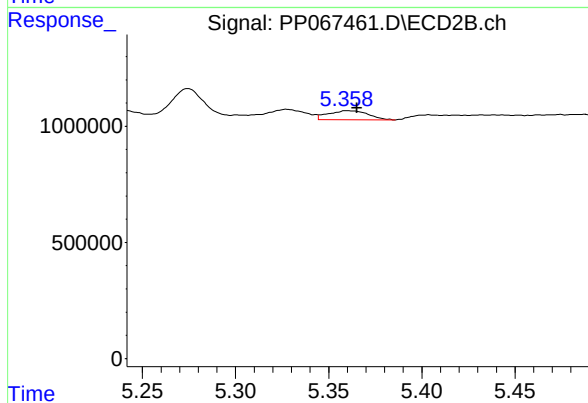

#18 AR-1242-3

R.T.: 5.360 min
Delta R.T.: -0.005 min
Response: 583081
Conc: 19.62 ng/ml

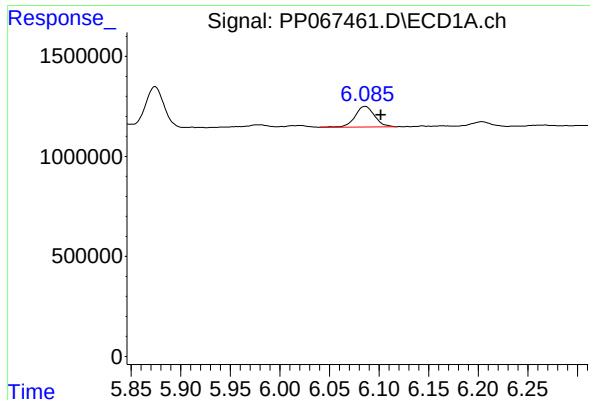


#19 AR-1242-4

R.T.: 6.086 min
Delta R.T.: -0.016 min
Response: 1410595
Conc: 51.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGERE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/04/2024
Supervised By :Ankita Jodhani 10/04/2024

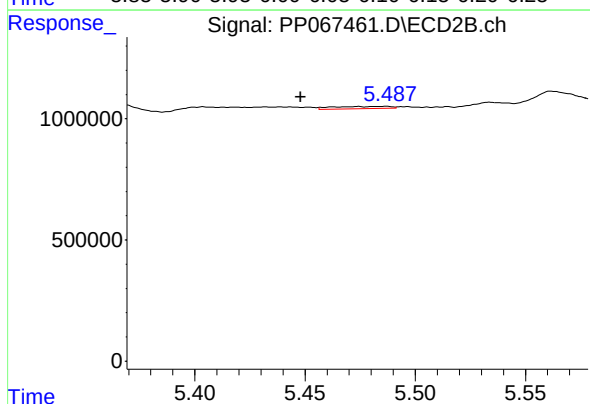


#19 AR-1242-4

R.T.: 5.487 min
Delta R.T.: 0.039 min
Response: 159569
Conc: 4.96 ng/ml

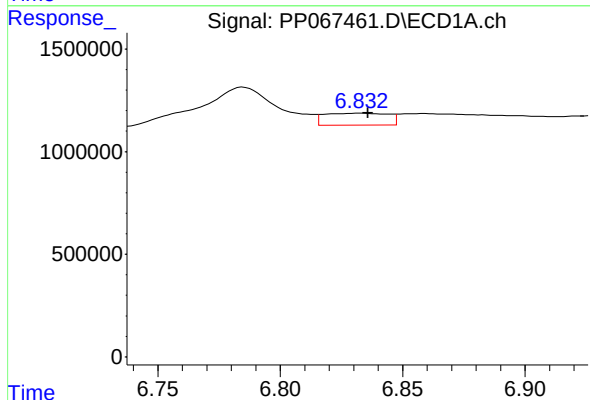


#20 AR-1242-5

R.T.: 6.833 min
Delta R.T.: -0.003 min
Response: 1065699
Conc: 35.81 ng/ml

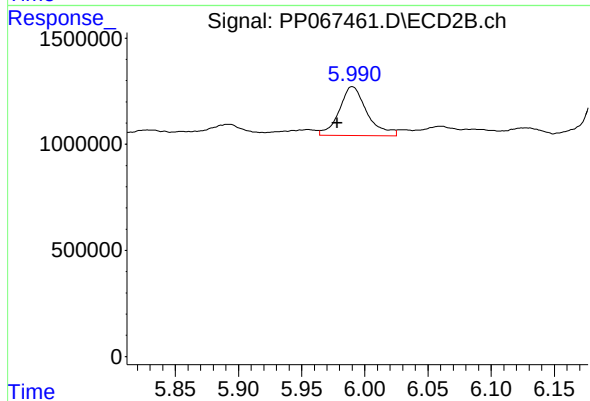

#20 AR-1242-5

R.T.: 5.990 min
Delta R.T.: 0.012 min
Response: 3529472
Conc: 92.45 ng/ml

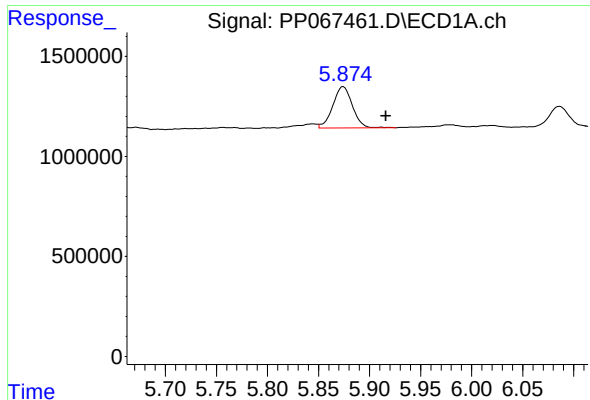


#21 AR-1248-1

R.T.: 5.874 min
Delta R.T.: -0.042 min
Response: 2751091
Conc: 97.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGERE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/04/2024
Supervised By :Ankita Jodhani 10/04/2024

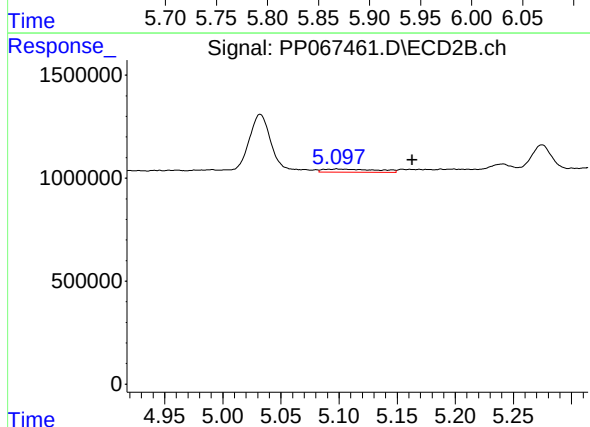


#21 AR-1248-1

R.T.: 5.098 min
Delta R.T.: -0.065 min
Response: 495247
Conc: 16.17 ng/ml

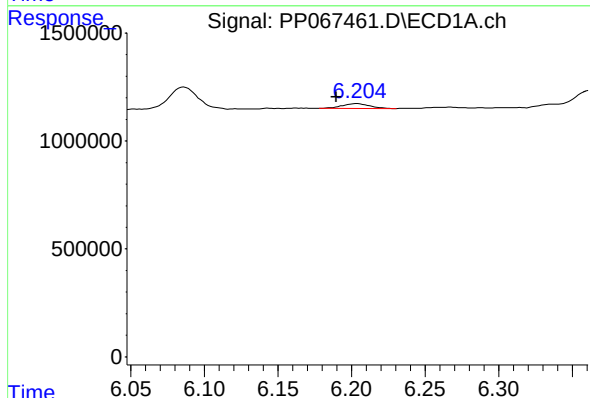


#22 AR-1248-2

R.T.: 6.204 min
Delta R.T.: 0.014 min
Response: 296316
Conc: 6.67 ng/ml

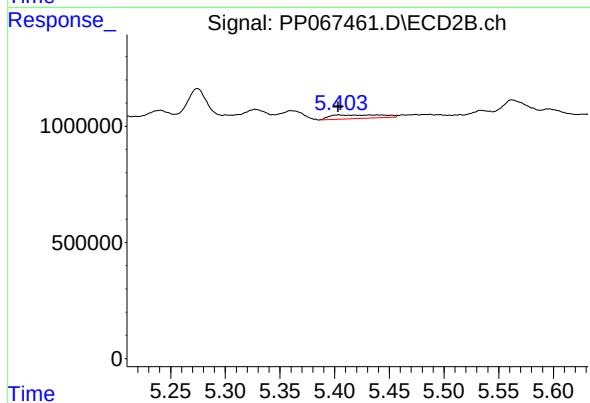

#22 AR-1248-2

R.T.: 5.404 min
Delta R.T.: 0.000 min
Response: 526008
Conc: 11.59 ng/ml

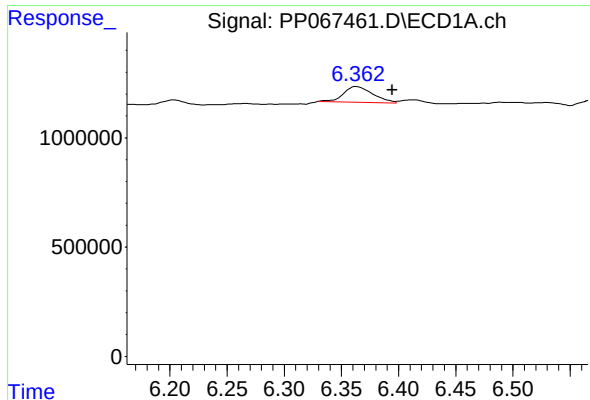


#23 AR-1248-3

R.T.: 6.363 min
Delta R.T.: -0.032 min
Response: 1273838
Conc: 26.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGERE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/04/2024
Supervised By :Ankita Jodhani 10/04/2024

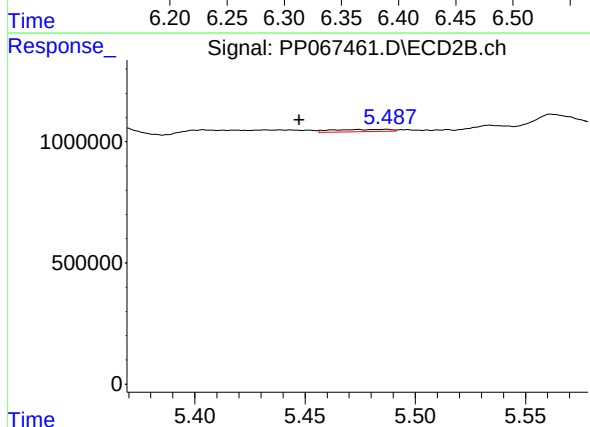


#23 AR-1248-3

R.T.: 5.487 min
Delta R.T.: 0.039 min
Response: 159569
Conc: 3.37 ng/ml

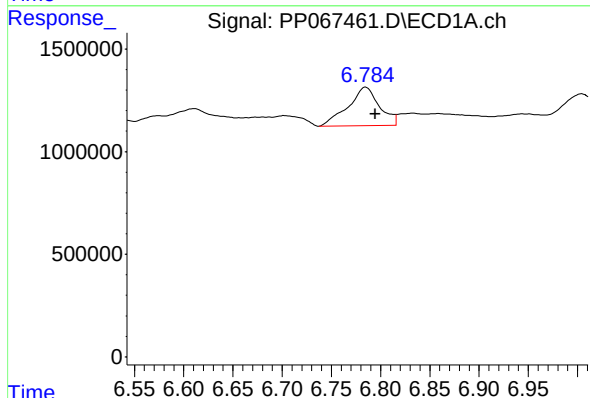


#24 AR-1248-4

R.T.: 6.785 min
Delta R.T.: -0.010 min
Response: 4177414
Conc: 76.99 ng/ml

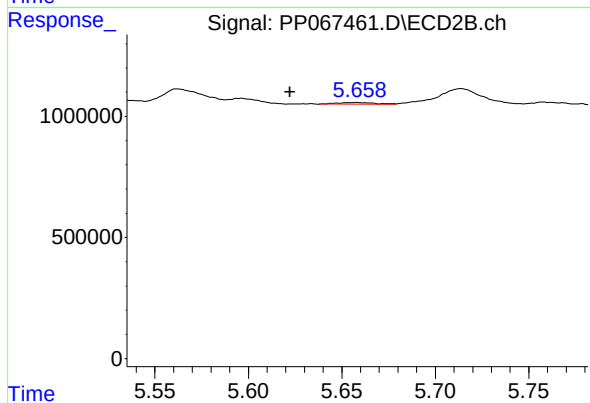

#24 AR-1248-4

R.T.: 5.658 min
Delta R.T.: 0.035 min
Response: 102843
Conc: 1.89 ng/ml

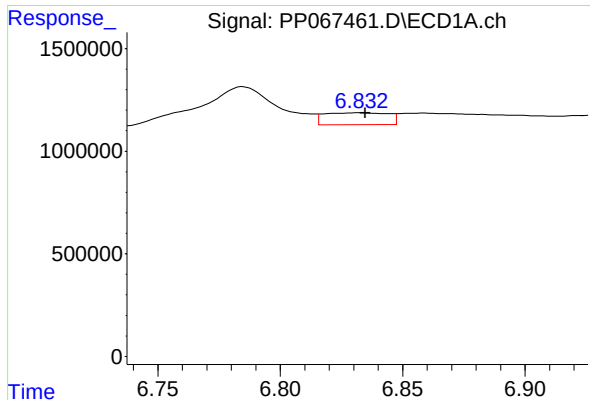


#25 AR-1248-5

R.T.: 6.833 min
Delta R.T.: -0.002 min
Response: 1065699
Conc: 19.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGERE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/04/2024
Supervised By :Ankita Jodhani 10/04/2024

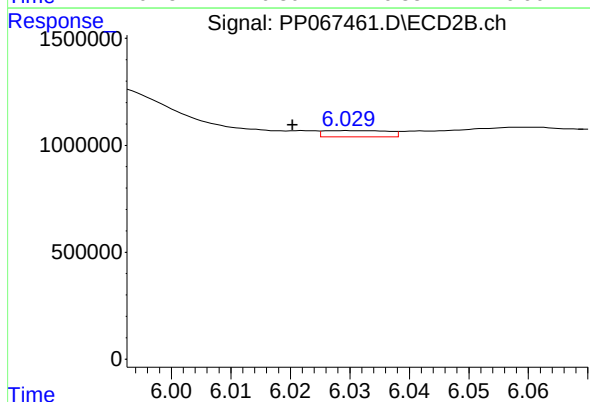


#25 AR-1248-5

R.T.: 6.029 min
Delta R.T.: 0.009 min
Response: 215057
Conc: 4.41 ng/ml

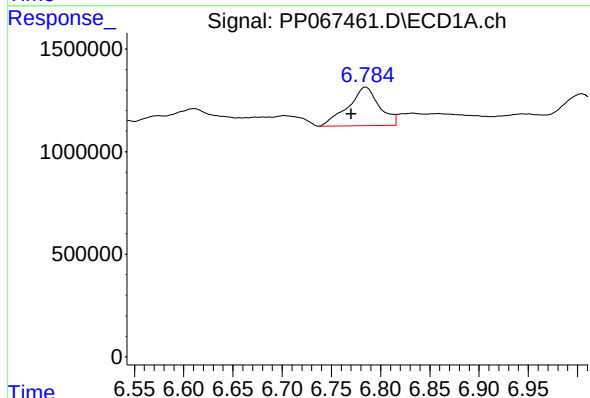


#26 AR-1254-1

R.T.: 6.785 min
Delta R.T.: 0.014 min
Response: 4177414
Conc: 67.05 ng/ml

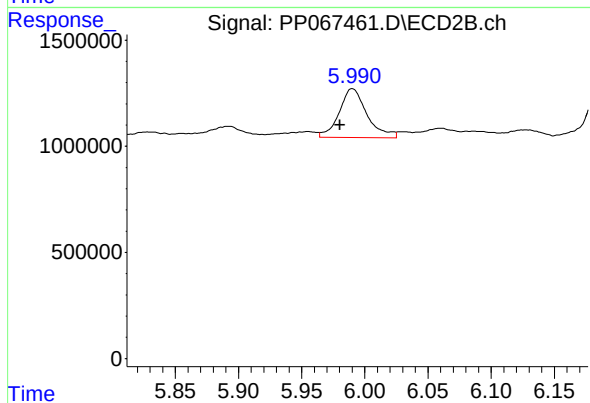

#26 AR-1254-1

R.T.: 5.990 min
Delta R.T.: 0.010 min
Response: 3529472
Conc: 43.54 ng/ml

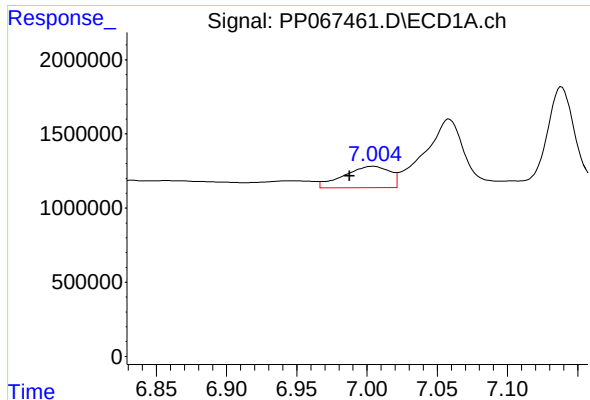


#27 AR-1254-2

R.T.: 7.004 min
Delta R.T.: 0.016 min
Response: 3278627
Conc: 36.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGERE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/04/2024
Supervised By :Ankita Jodhani 10/04/2024

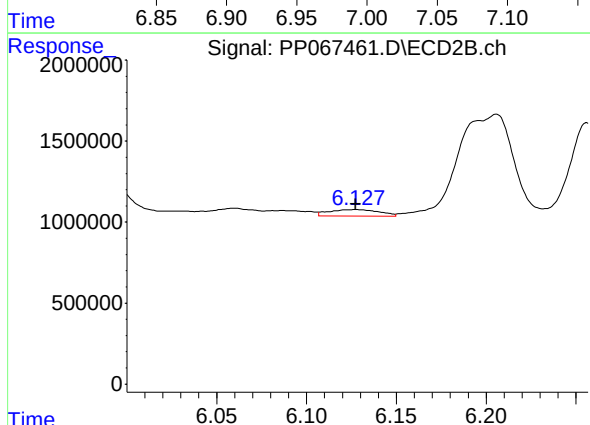


#27 AR-1254-2

R.T.: 6.128 min
Delta R.T.: 0.000 min
Response: 777994
Conc: 10.61 ng/ml

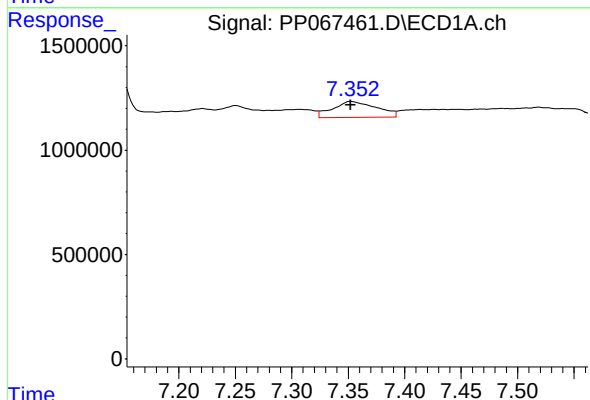


#28 AR-1254-3

R.T.: 7.352 min
Delta R.T.: 0.000 min
Response: 2055225
Conc: 21.91 ng/ml

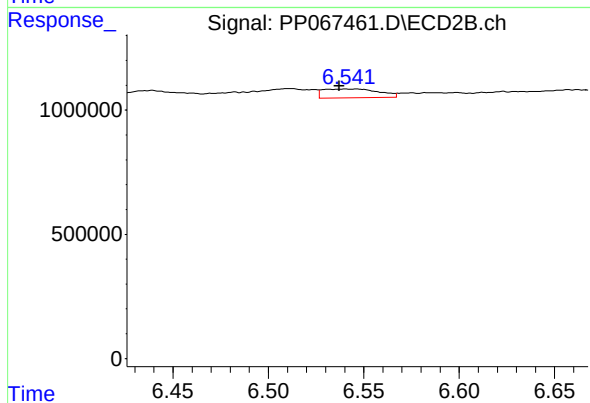

#28 AR-1254-3

R.T.: 6.541 min
Delta R.T.: 0.004 min
Response: 725707
Conc: 6.36 ng/ml

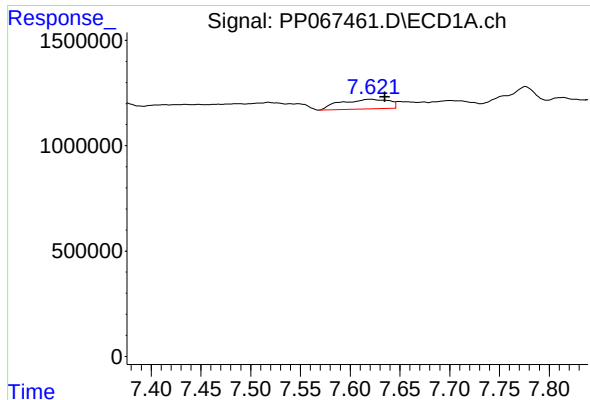


#29 AR-1254-4

R.T.: 7.621 min
Delta R.T.: -0.014 min
Response: 1543587
Conc: 23.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGERE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/04/2024
Supervised By :Ankita Jodhani 10/04/2024

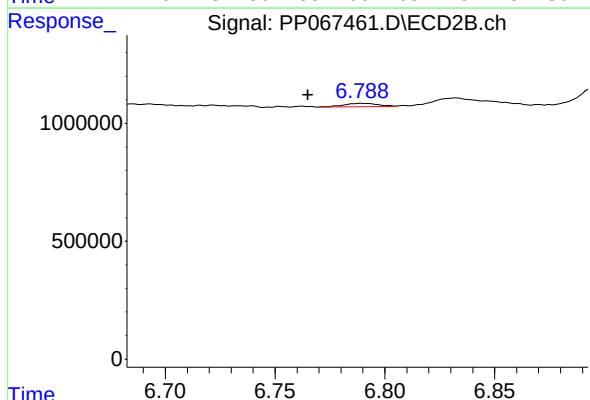


#29 AR-1254-4

R.T.: 6.790 min
Delta R.T.: 0.025 min
Response: 155002
Conc: 2.48 ng/ml

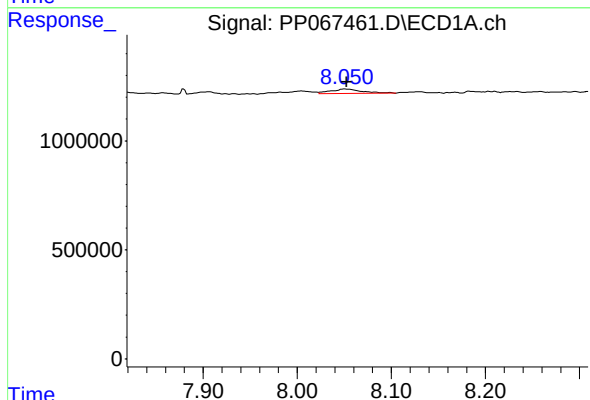


#30 AR-1254-5

R.T.: 8.051 min
Delta R.T.: -0.001 min
Response: 481297
Conc: 5.86 ng/ml

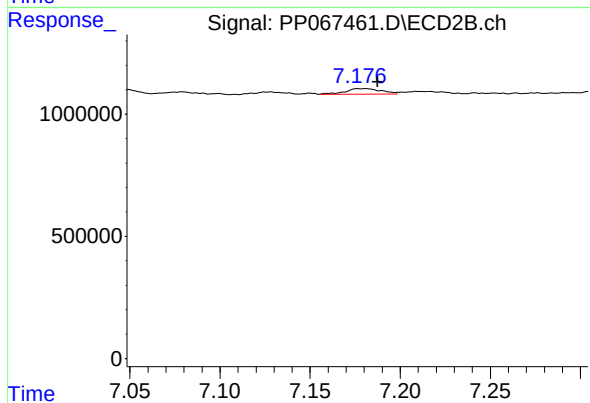

#30 AR-1254-5

R.T.: 7.181 min
Delta R.T.: -0.007 min
Response: 320468
Conc: 3.12 ng/ml

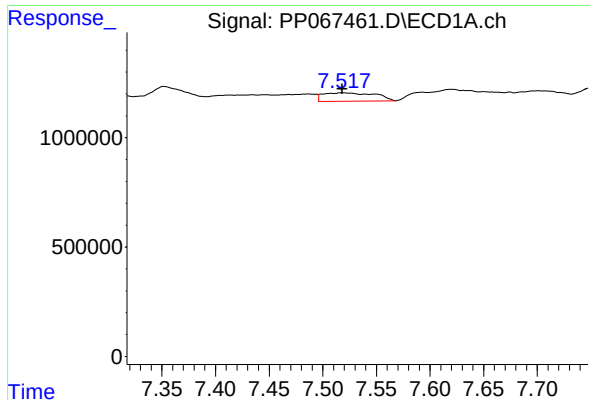


#31 AR-1260-1

R.T.: 7.518 min
Delta R.T.: 0.000 min
Response: 1308655
Conc: 16.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGERE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/04/2024
Supervised By :Ankita Jodhani 10/04/2024

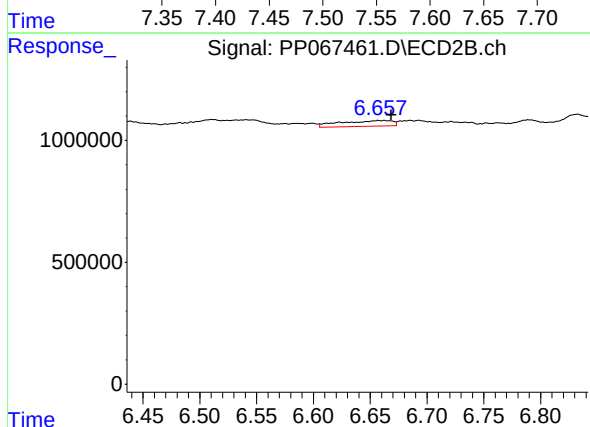


#31 AR-1260-1

R.T.: 6.662 min
Delta R.T.: -0.006 min
Response: 743305
Conc: 9.09 ng/ml

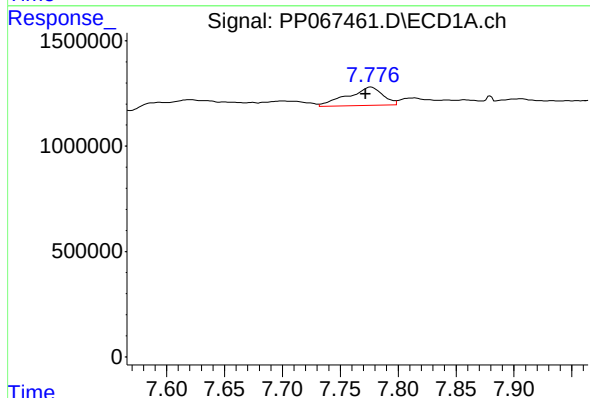


#32 AR-1260-2

R.T.: 7.776 min
Delta R.T.: 0.004 min
Response: 1830195
Conc: 20.08 ng/ml

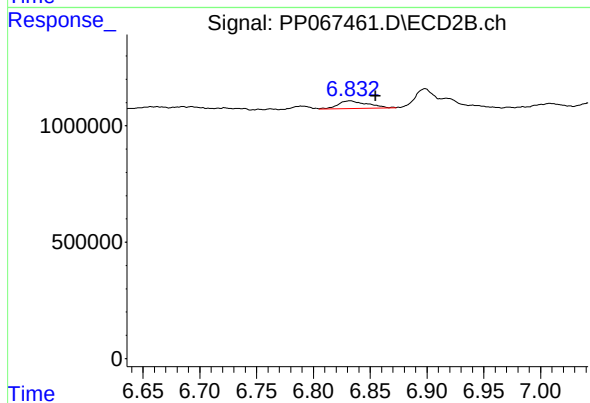

#32 AR-1260-2

R.T.: 6.832 min
Delta R.T.: -0.022 min
Response: 590410
Conc: 6.28 ng/ml

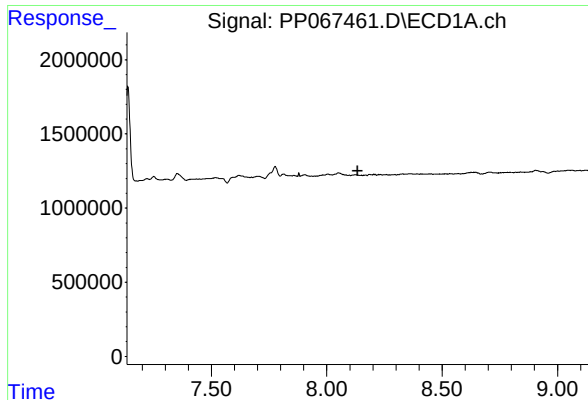


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T.: 8.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGERE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/04/2024
Supervised By :Ankita Jodhani 10/04/2024

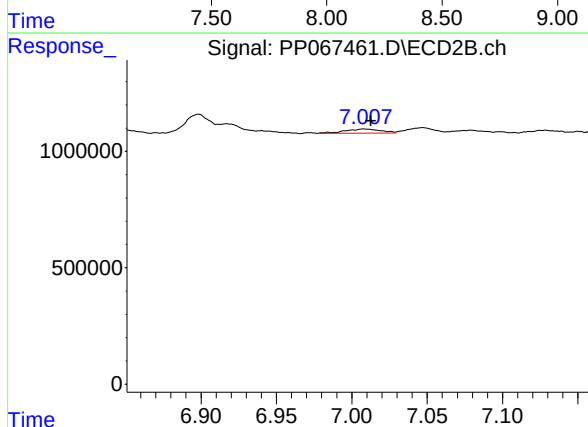


#33 AR-1260-3

R.T.: 7.008 min
Delta R.T.: -0.005 min
Response: 290927
Conc: 3.21 ng/ml

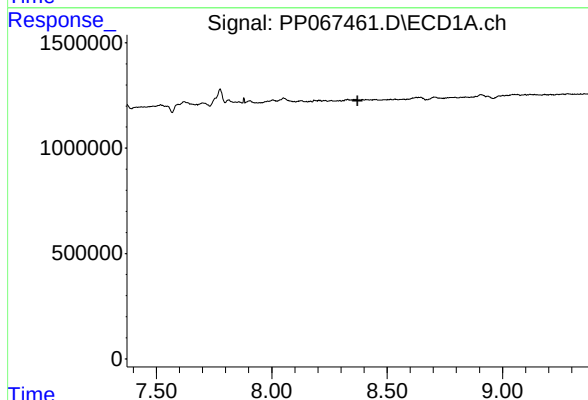


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 8.371 min
Response: 0
Conc: N.D.

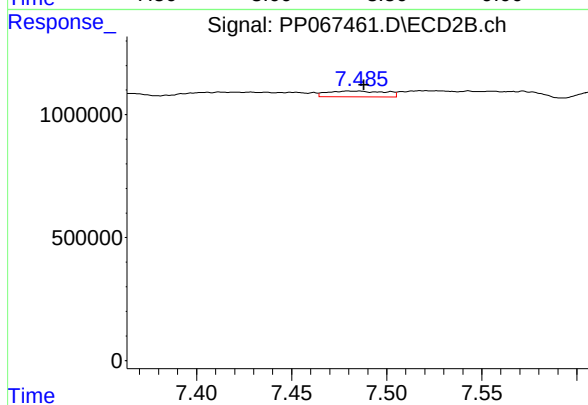

#34 AR-1260-4

R.T.: 7.480 min
Delta R.T.: -0.008 min
Response: 501324
Conc: 7.52 ng/ml

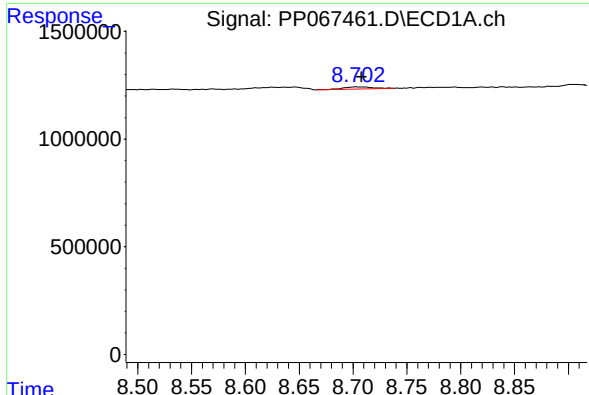


#35 AR-1260-5

R.T.: 8.704 min
Delta R.T.: -0.004 min
Response: 179160
Conc: 1.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGERE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/04/2024
Supervised By :Ankita Jodhani 10/04/2024

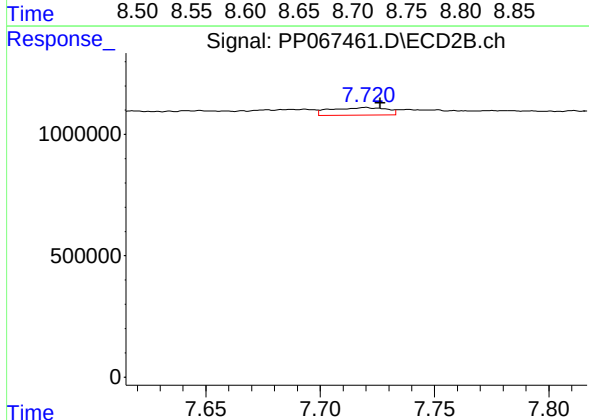


#35 AR-1260-5

R.T.: 7.720 min
Delta R.T.: -0.006 min
Response: 522668
Conc: 3.59 ng/ml

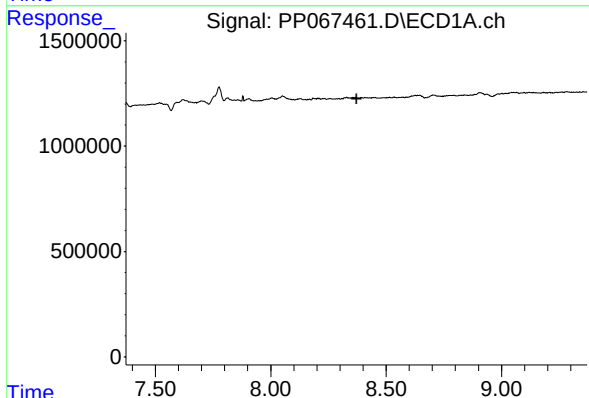


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 8.372 min
Response: 0
Conc: N.D.

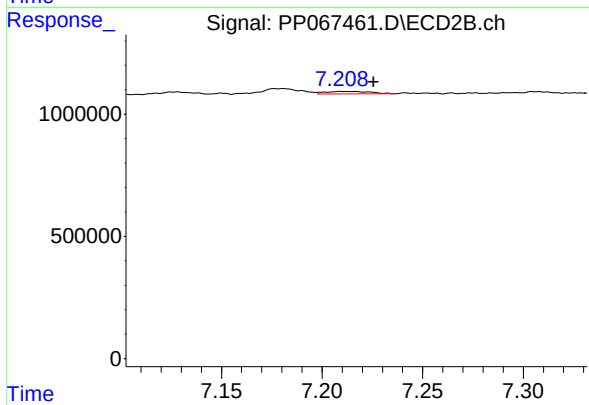

#36 AR-1262-1

R.T.: 7.210 min
Delta R.T.: -0.016 min
Response: 165523
Conc: 1.57 ng/ml

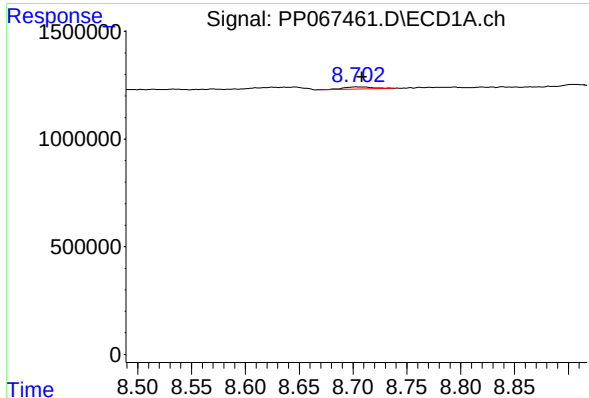


#37 AR-1262-2

R.T.: 8.704 min
Delta R.T.: -0.004 min
Response: 179160
Conc: 1.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGERE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/04/2024
Supervised By :Ankita Jodhani 10/04/2024

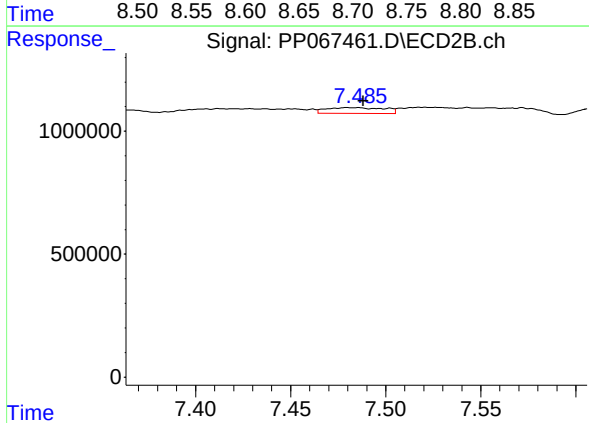


#37 AR-1262-2

R.T.: 7.480 min
Delta R.T.: -0.008 min
Response: 501324
Conc: 5.30 ng/ml

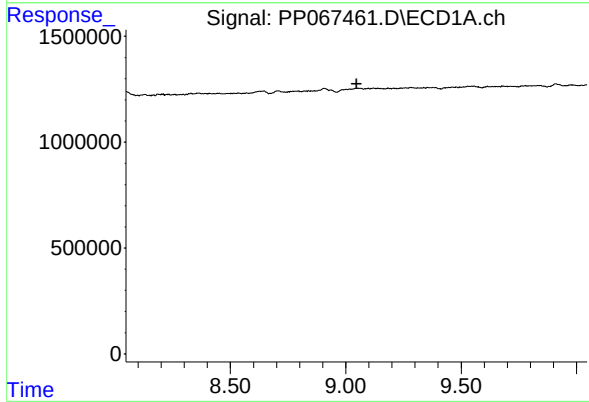


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 9.046 min
Response: 0
Conc: N.D.

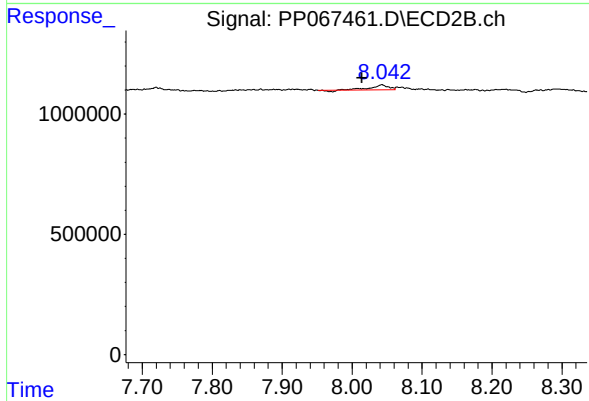

#38 AR-1262-3

R.T.: 8.043 min
Delta R.T.: 0.029 min
Response: 342937
Conc: 4.68 ng/ml

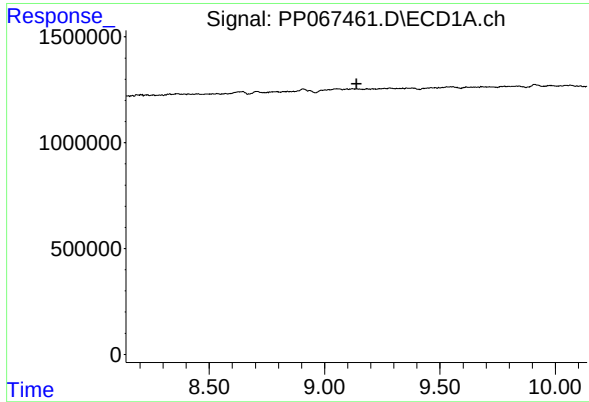


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 9.138 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGERE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/04/2024
Supervised By :Ankita Jodhani 10/04/2024

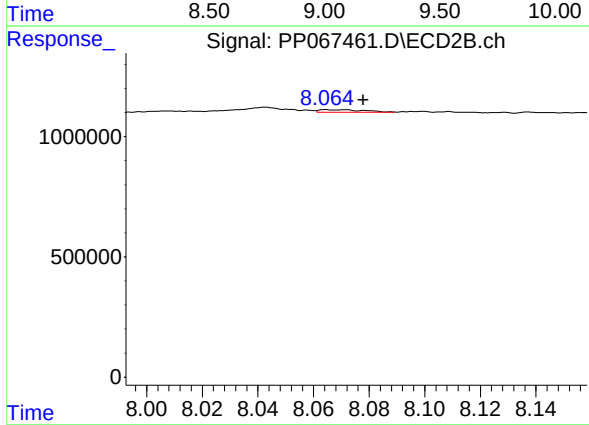


#39 AR-1262-4

R.T.: 8.065 min
Delta R.T.: -0.013 min
Response: 112427
Conc: 0.85 ng/ml

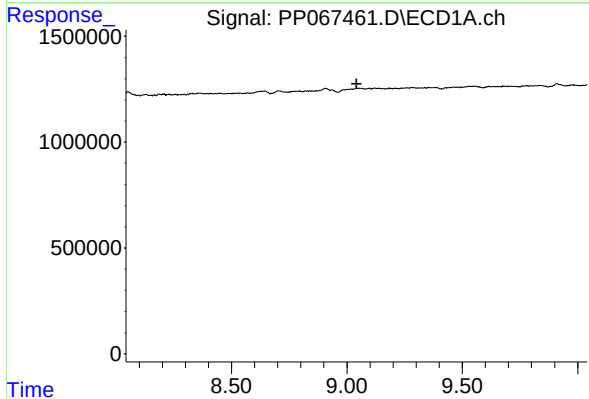


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.042 min
Response: 0
Conc: N.D.

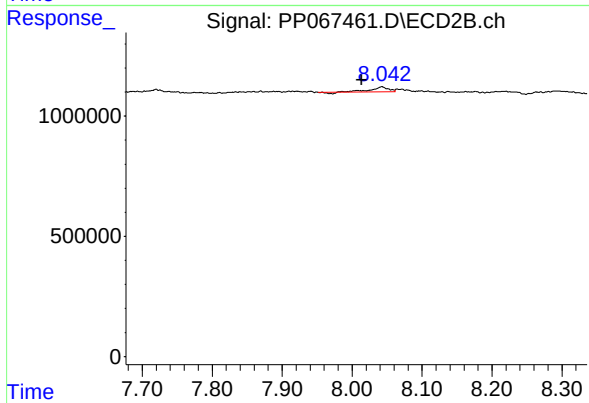

#41 AR-1268-1

R.T.: 8.043 min
Delta R.T.: 0.029 min
Response: 342937
Conc: 1.70 ng/ml

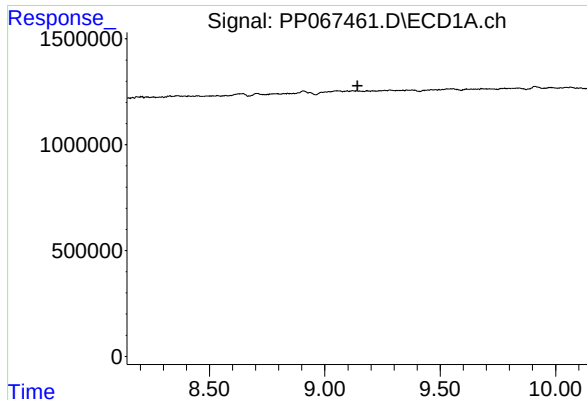


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 9.141 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGERE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/04/2024
Supervised By :Ankita Jodhani 10/04/2024

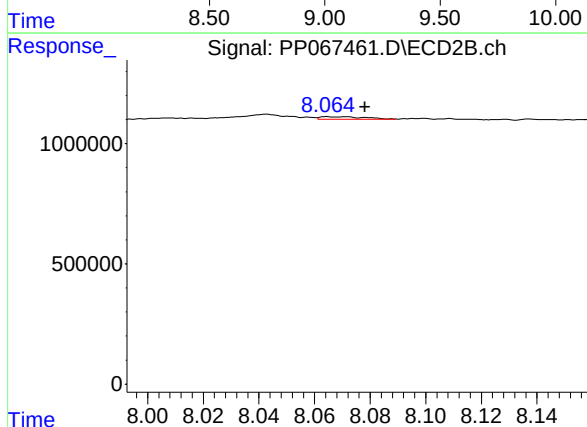


#42 AR-1268-2

R.T.: 8.065 min
Delta R.T.: -0.013 min
Response: 112427
Conc: 0.63 ng/ml

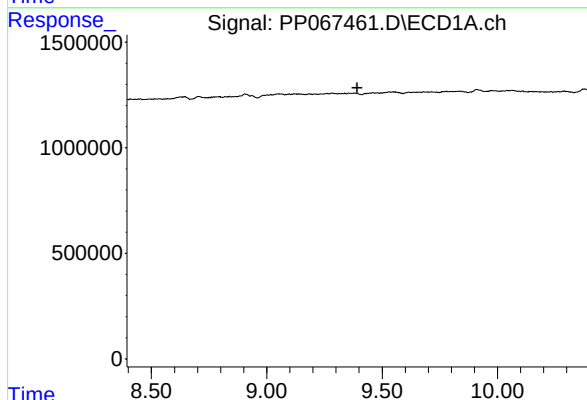


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 9.392 min
Response: 0
Conc: N.D.

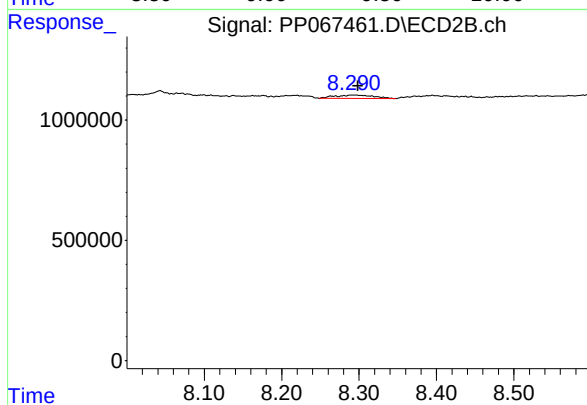

#43 AR-1268-3

R.T.: 8.290 min
Delta R.T.: -0.009 min
Response: 495833
Conc: 3.12 ng/ml

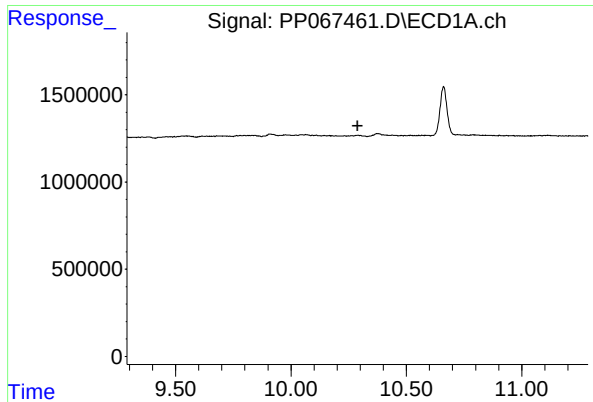


#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.289 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MH-147-SLUDGERE

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/04/2024
Supervised By :Ankita Jodhani 10/04/2024

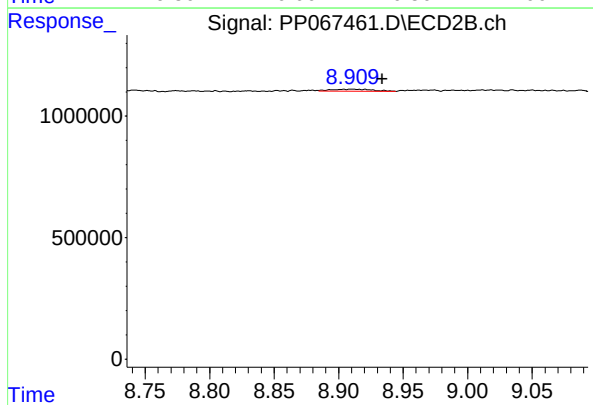

#45 AR-1268-5

R.T.: 8.911 min
Delta R.T.: -0.023 min
Response: 184280
Conc: 0.42 ng/ml