

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100324\
 Data File : PP067473.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2024 15:05
 Operator : YP\AJ
 Sample : P4275-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TRE-1300

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/04/2024
 Supervised By :Ankita Jodhani 10/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 01:32:43 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 27 06:59:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.752	4.054	19595406	15689508	14.579m	10.501 #
2) SA Decachlor...	10.677	9.233	19587127	17527593	13.492	12.719

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100324\
Data File : PP067473.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2024 15:05
Operator : YP\AJ
Sample : P4275-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TRE-1300


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/04/2024
Supervised By :Ankita Jodhani 10/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 01:32:43 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092624.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 27 06:59:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

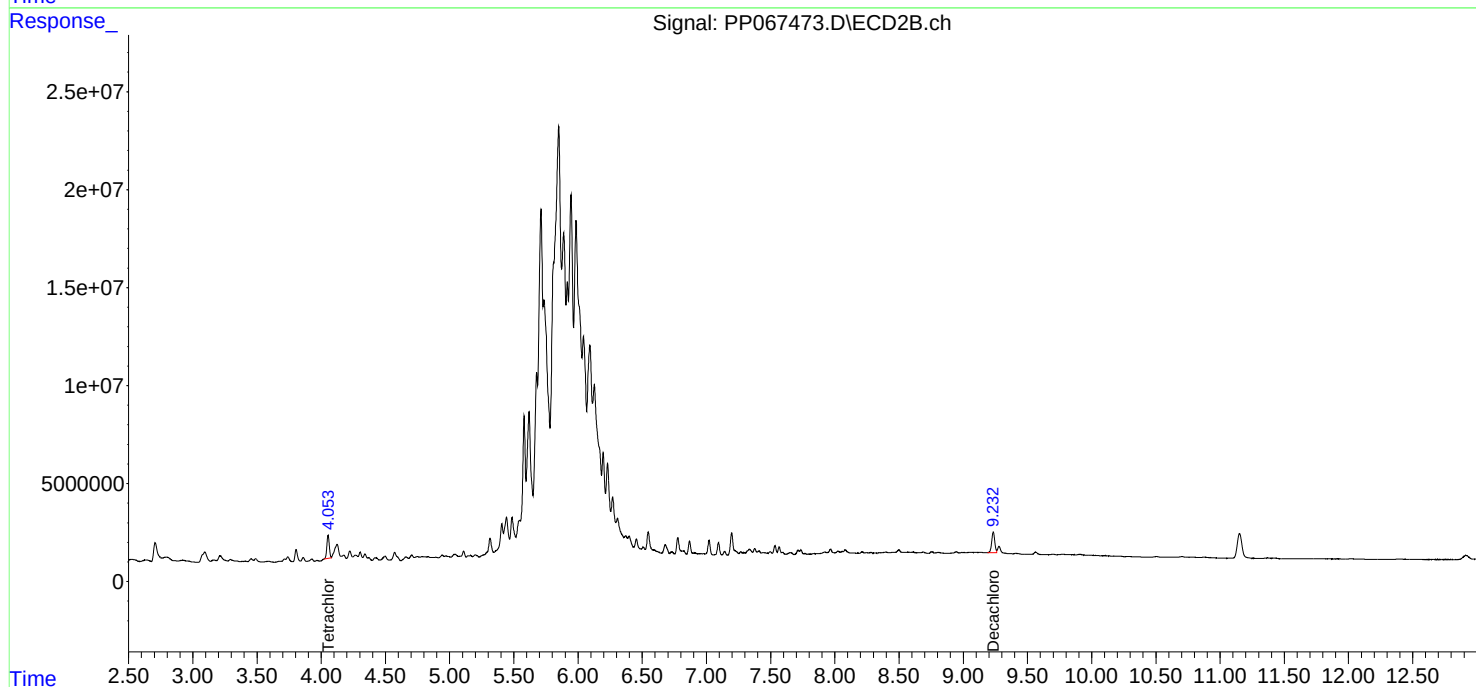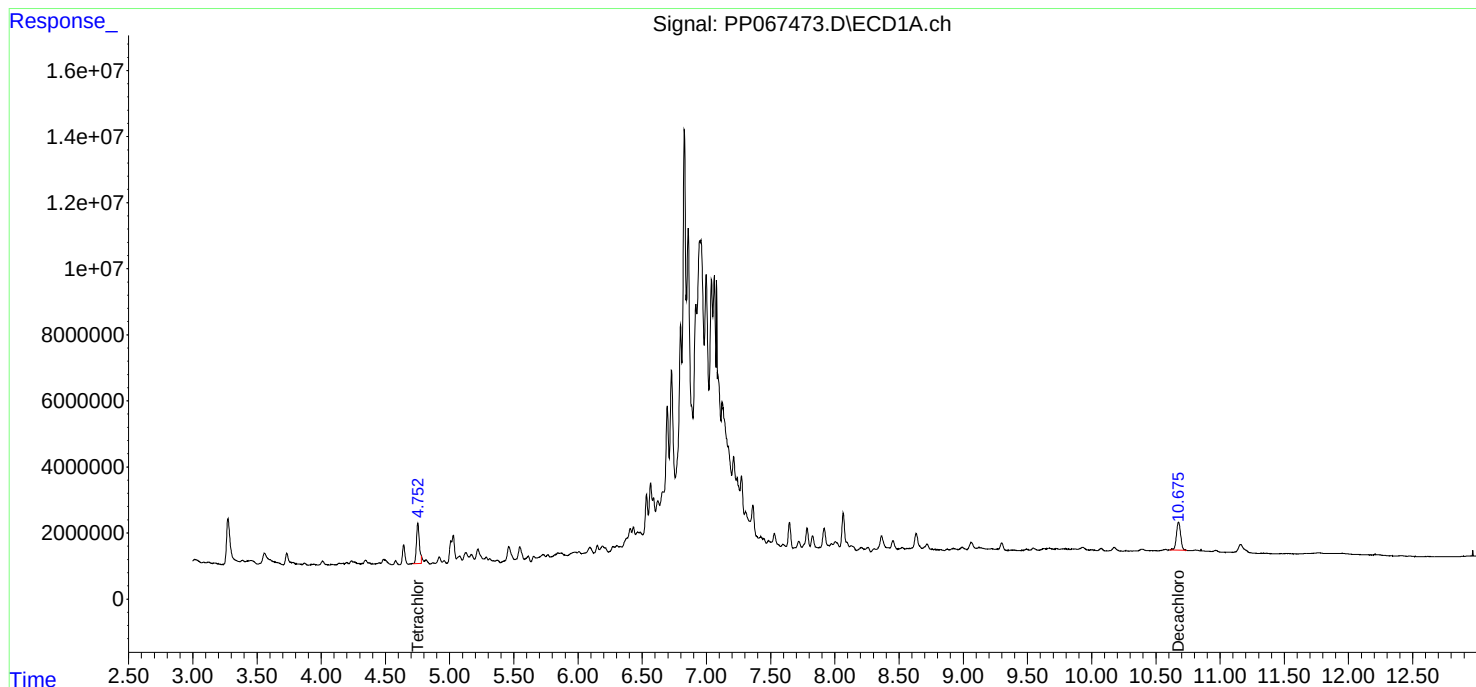

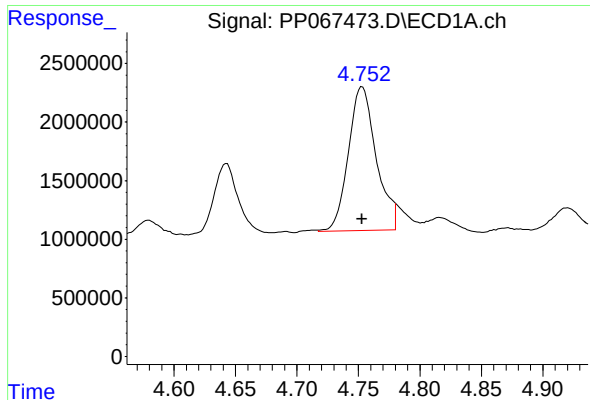


#1 Tetrachloro-m-xylene

R.T.: 4.752 min
Delta R.T.: 0.000 min
Response: 19595406
Conc: 14.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRE-1300


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/04/2024
Supervised By :Ankita Jodhani 10/04/2024

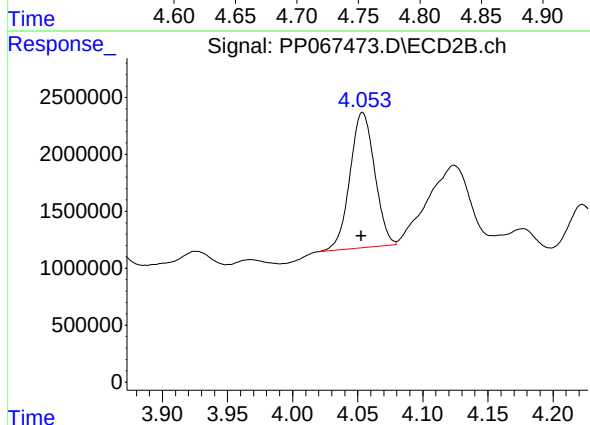


#1 Tetrachloro-m-xylene

R.T.: 4.054 min
Delta R.T.: 0.000 min
Response: 15689508
Conc: 10.50 ng/ml

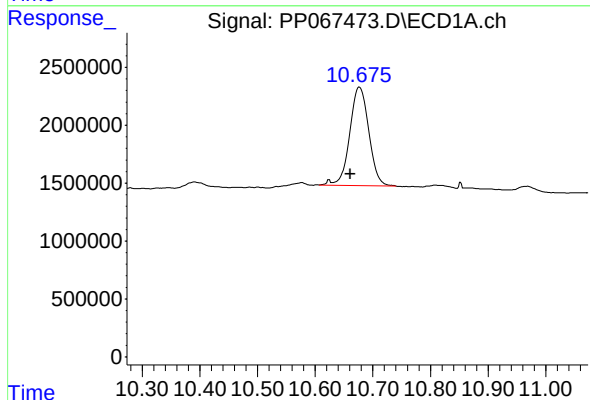

#2 Decachlorobiphenyl

R.T.: 10.677 min
Delta R.T.: 0.015 min
Response: 19587127
Conc: 13.49 ng/ml

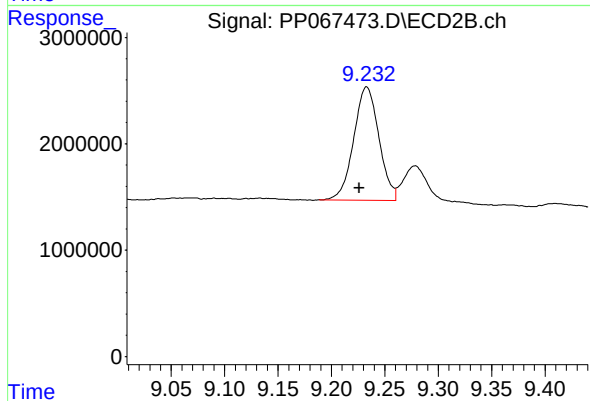

#2 Decachlorobiphenyl

R.T.: 9.233 min
Delta R.T.: 0.007 min
Response: 17527593
Conc: 12.72 ng/ml