

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102723\
 Data File : PP061280.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2023 10:31
 Operator : YP\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 18:45:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 27 18:44:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
20)	L4	AR-1242-5	6.689	0.000	297053	0	5.743 N.D. #
25)	L5	AR-1248-5	6.689	0.000	297053	0	3.503 N.D. #
27)	L6	AR-1254-2	6.829	0.000	601179	0	4.507 N.D. #
28)	L6	AR-1254-3	7.219	0.000	846220	0	6.119 N.D. #
29)	L6	AR-1254-4	7.497	0.000	648926	0	6.519 N.D. #
30)	L6	AR-1254-5	7.953f	0.000	298524	0	2.713 N.D. #
31)	L7	AR-1260-1	7.391	0.000	32292	0	0.287 N.D. #
32)	L7	AR-1260-2	7.633	0.000	367305	0	2.839 N.D. #
33)	L7	AR-1260-3	8.014	0.000	265275	0	3.123 N.D. #
36)	L8	AR-1262-1	8.014	0.000	265275	0	1.995 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102723\
Data File : PP061280.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2023 10:31
Operator : YP\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 18:45:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102723.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 27 18:44:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

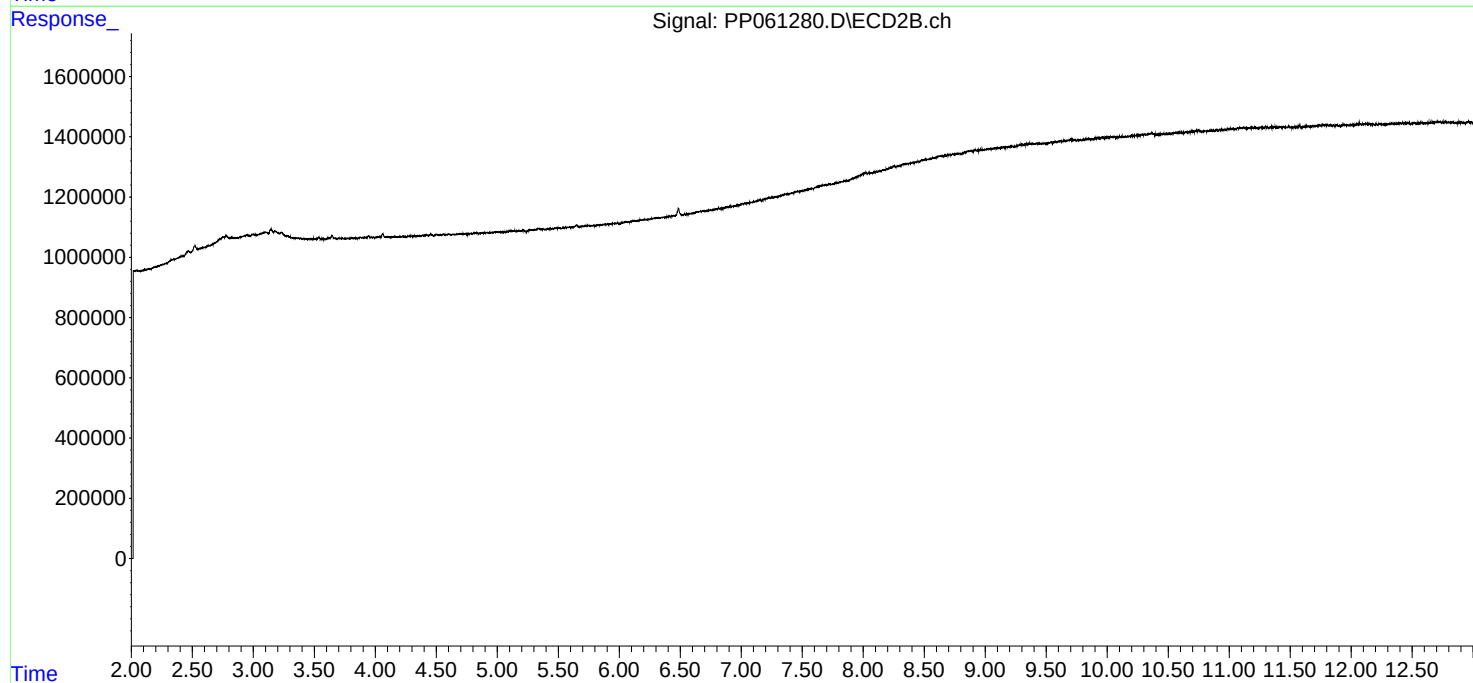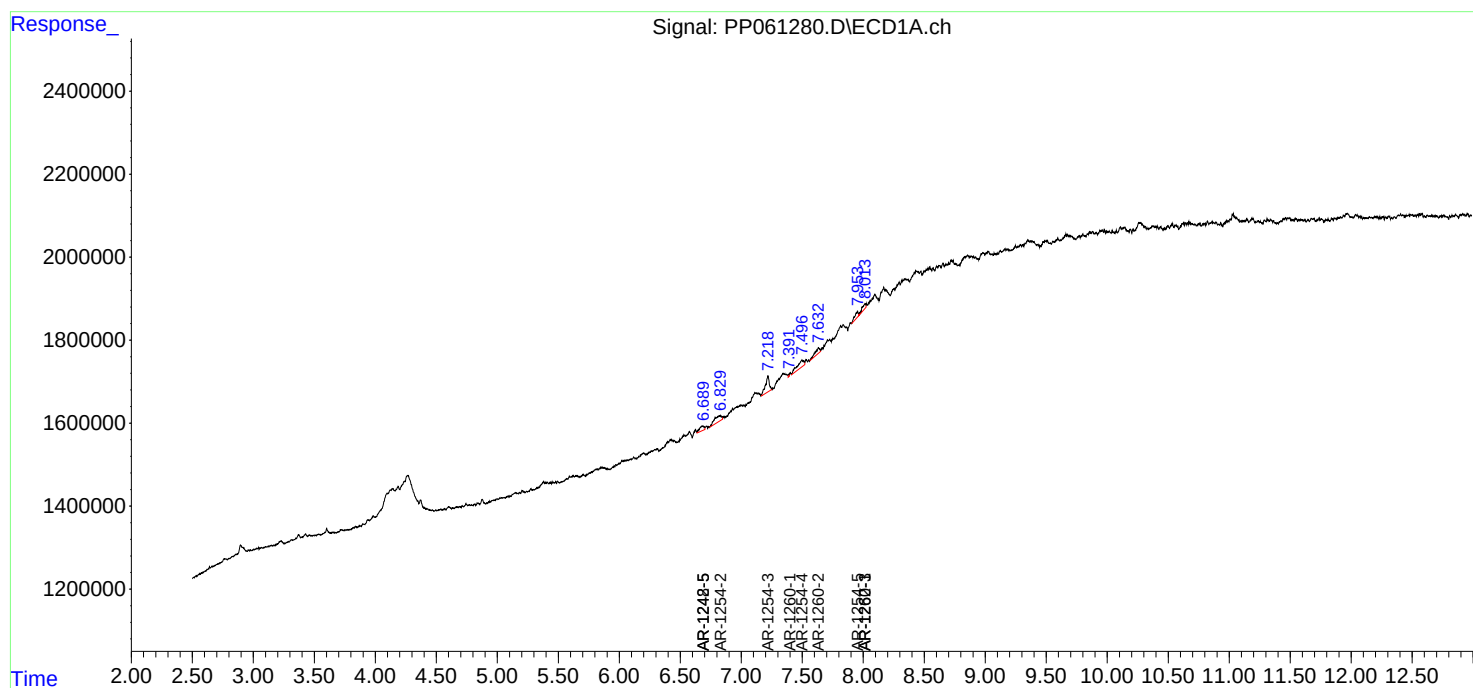

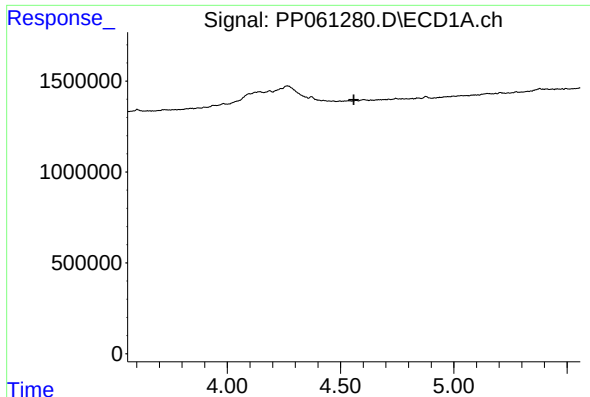

#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.559 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.694 min
Response: 0
Conc: N.D.

#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.536 min
Response: 0
Conc: N.D.

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 8.764 min
Response: 0
Conc: N.D.

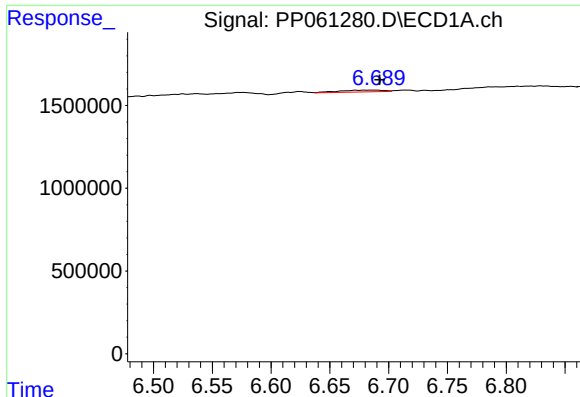

#20 AR-1242-5


R.T.: 6.689 min
Delta R.T.: -0.003 min
Response: 297053
Conc: 5.74 ng/ml

Instrument :
ECD_P
ClientSampleId :

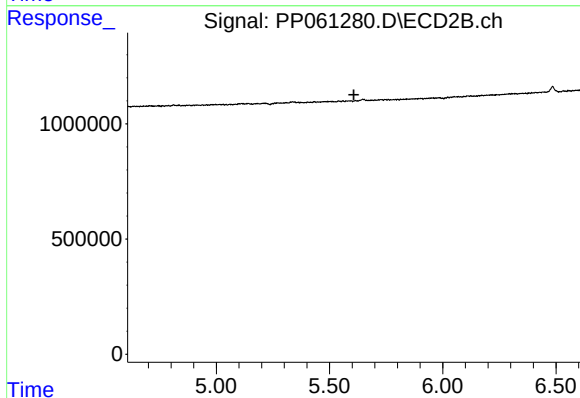


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 5.608 min
Response: 0
Conc: N.D.

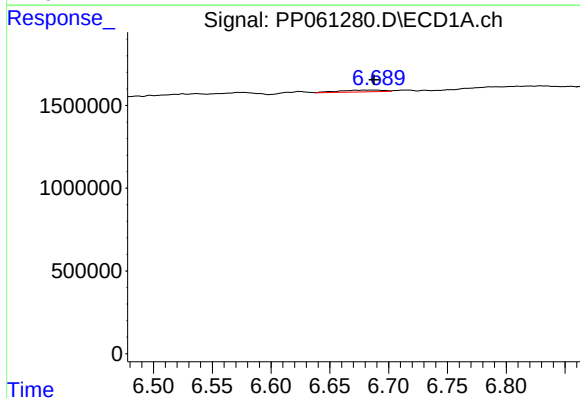


#25 AR-1248-5

R.T.: 6.689 min
Delta R.T.: 0.002 min
Response: 297053
Conc: 3.50 ng/ml

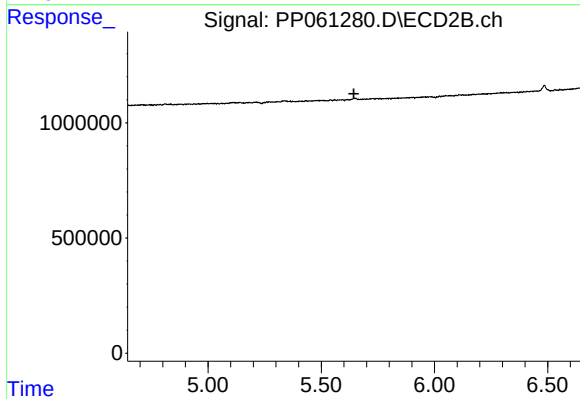

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 5.644 min
Response: 0
Conc: N.D.

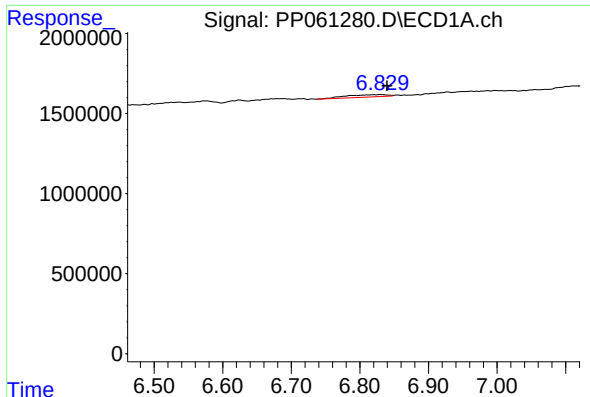

#27 AR-1254-2


R.T.: 6.829 min
Delta R.T.: -0.011 min
Response: 601179
Conc: 4.51 ng/ml

Instrument :
ECD_P
ClientSampleId :

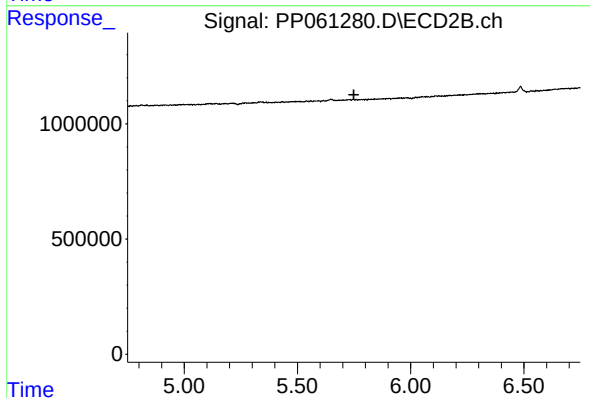


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 5.749 min
Response: 0
Conc: N.D.

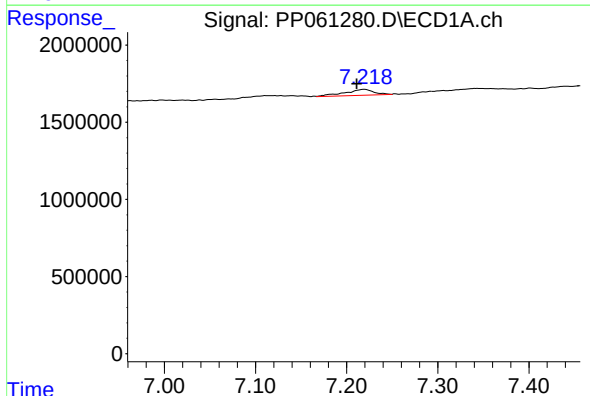


#28 AR-1254-3

R.T.: 7.219 min
Delta R.T.: 0.008 min
Response: 846220
Conc: 6.12 ng/ml

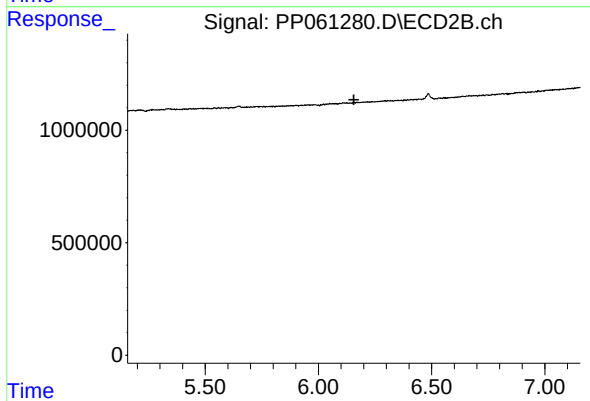

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.157 min
Response: 0
Conc: N.D.

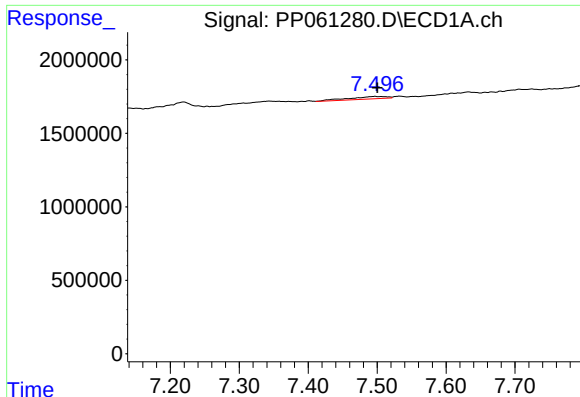

#29 AR-1254-4


R.T.: 7.497 min
Delta R.T.: -0.003 min
Response: 648926
Conc: 6.52 ng/ml

Instrument :
ECD_P
ClientSampleId :

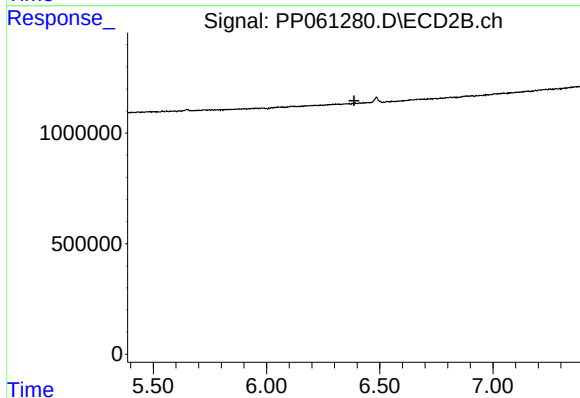


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.386 min
Response: 0
Conc: N.D.

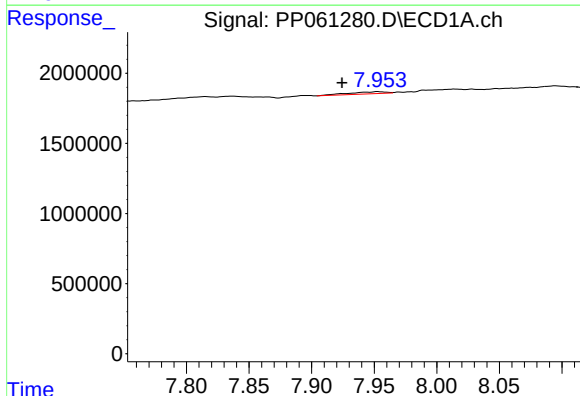


#30 AR-1254-5

R.T.: 7.953 min
Delta R.T.: 0.029 min
Response: 298524
Conc: 2.71 ng/ml

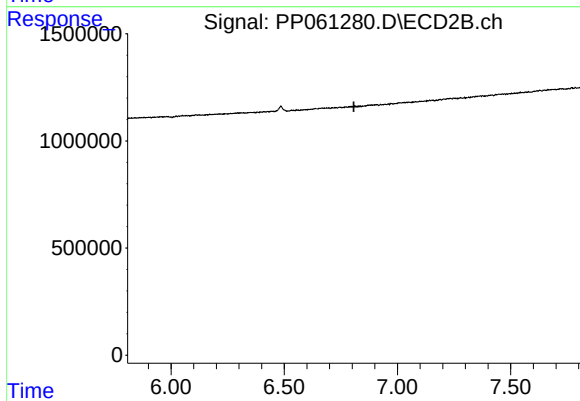

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 6.808 min
Response: 0
Conc: N.D.

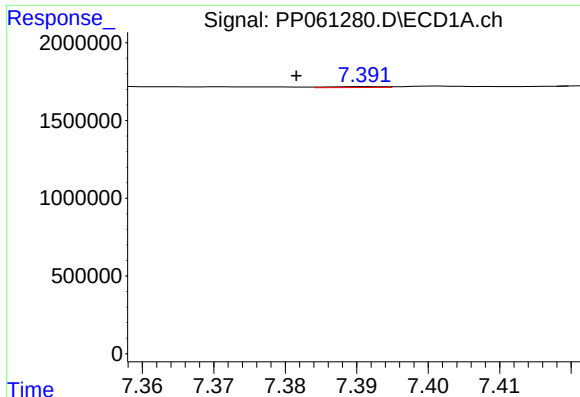

#31 AR-1260-1


R.T.: 7.391 min
Delta R.T.: 0.010 min
Response: 32292
Conc: 0.29 ng/ml

Instrument :
ECD_P
ClientSampleId :

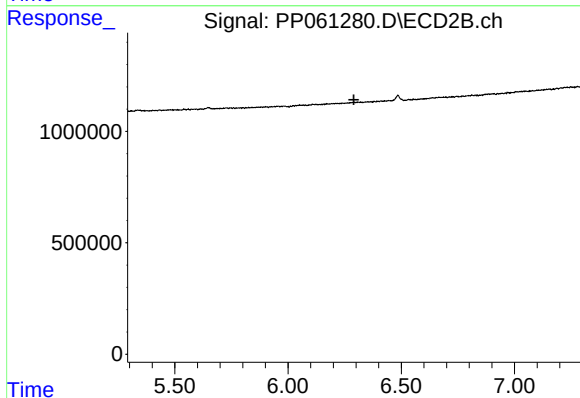


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.291 min
Response: 0
Conc: N.D.

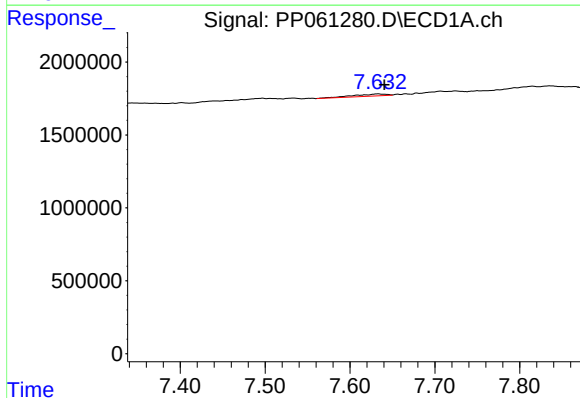


#32 AR-1260-2

R.T.: 7.633 min
Delta R.T.: -0.008 min
Response: 367305
Conc: 2.84 ng/ml

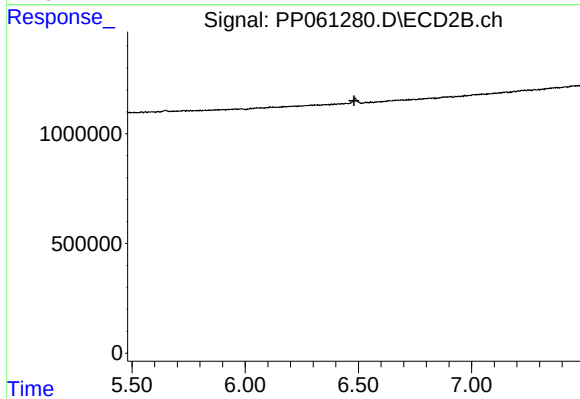

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.480 min
Response: 0
Conc: N.D.

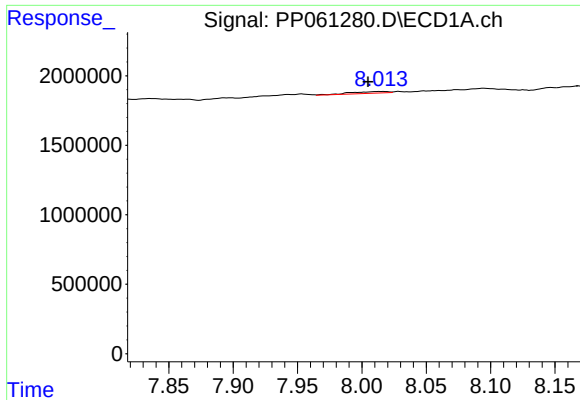

#33 AR-1260-3


R.T.: 8.014 min
Delta R.T.: 0.010 min
Response: 265275
Conc: 3.12 ng/ml

Instrument :
ECD_P
ClientSampleId :

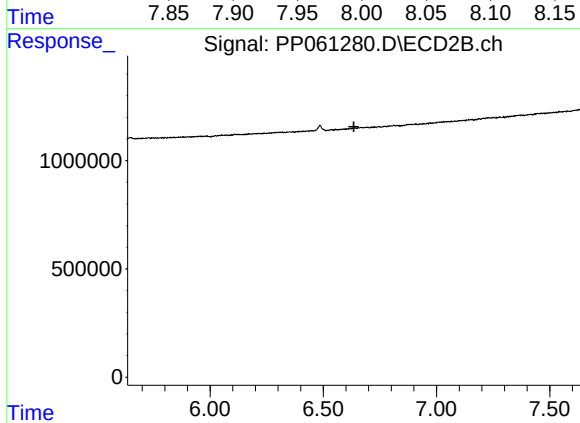


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 6.635 min
Response: 0
Conc: N.D.

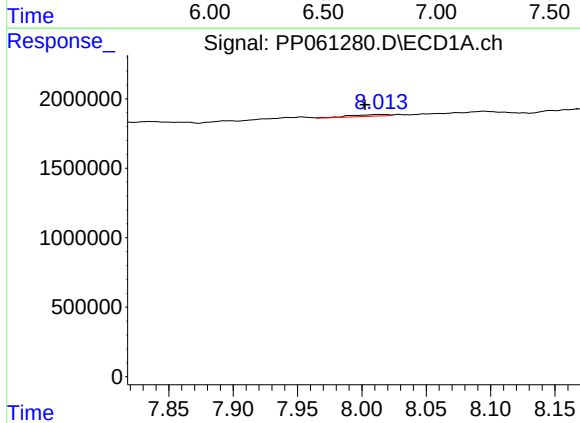

#36 AR-1262-1

R.T.: 8.014 min
Delta R.T.: 0.012 min
Response: 265275
Conc: 2.00 ng/ml

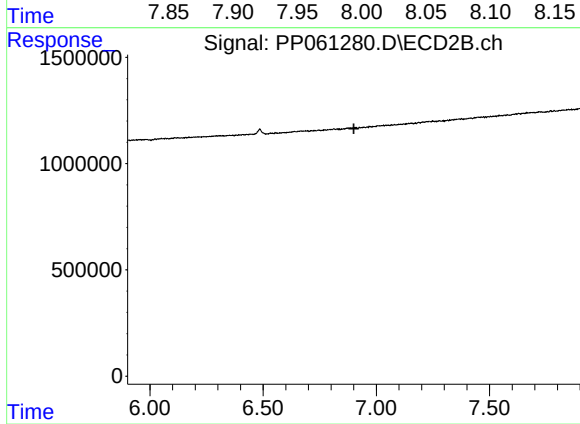

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 6.901 min
Response: 0
Conc: N.D.