

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102723\
 Data File : PP061281.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2023 10:47
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 18:46:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 27 18:44:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.561	3.695	57142004	36719096	23.133	24.570
2)	SA Decachlor...	10.539	8.767	46033019	37529469	24.412	24.438
Target Compounds							
9)	L2 AR-1221-2	4.875f	3.999	794199	482957	35.662	33.915
20)	L4 AR-1242-5	6.709f	0.000	262309	0	5.071	N.D. #
24)	L5 AR-1248-4	6.627f	0.000	181340	0	2.057	N.D. #
25)	L5 AR-1248-5	6.709f	0.000	262309	0	3.094	N.D. #
26)	L6 AR-1254-1	6.627	0.000	181340	0	2.048	N.D. #
27)	L6 AR-1254-2	6.844	0.000	155232	0	1.164	N.D. #
28)	L6 AR-1254-3	7.218	0.000	849226	0	6.140	N.D. #
29)	L6 AR-1254-4	7.515	0.000	314886	0	3.163	N.D. #
30)	L6 AR-1254-5	7.929	0.000	405612	0	3.686	N.D. #
31)	L7 AR-1260-1	7.356f	0.000	232043	0	2.063	N.D. #
32)	L7 AR-1260-2	7.654	0.000	208328	0	1.610	N.D. #
33)	L7 AR-1260-3	7.999	0.000	306687	0	3.611	N.D. #
34)	L7 AR-1260-4	8.226	0.000	155473	0	1.538	N.D. #
36)	L8 AR-1262-1	7.999	0.000	306687	0	2.306	N.D. #
45)	L9 AR-1268-5	0.000	8.503	0	204125	N.D.	0.360 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102723\
Data File : PP061281.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2023 10:47
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 18:46:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102723.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 27 18:44:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

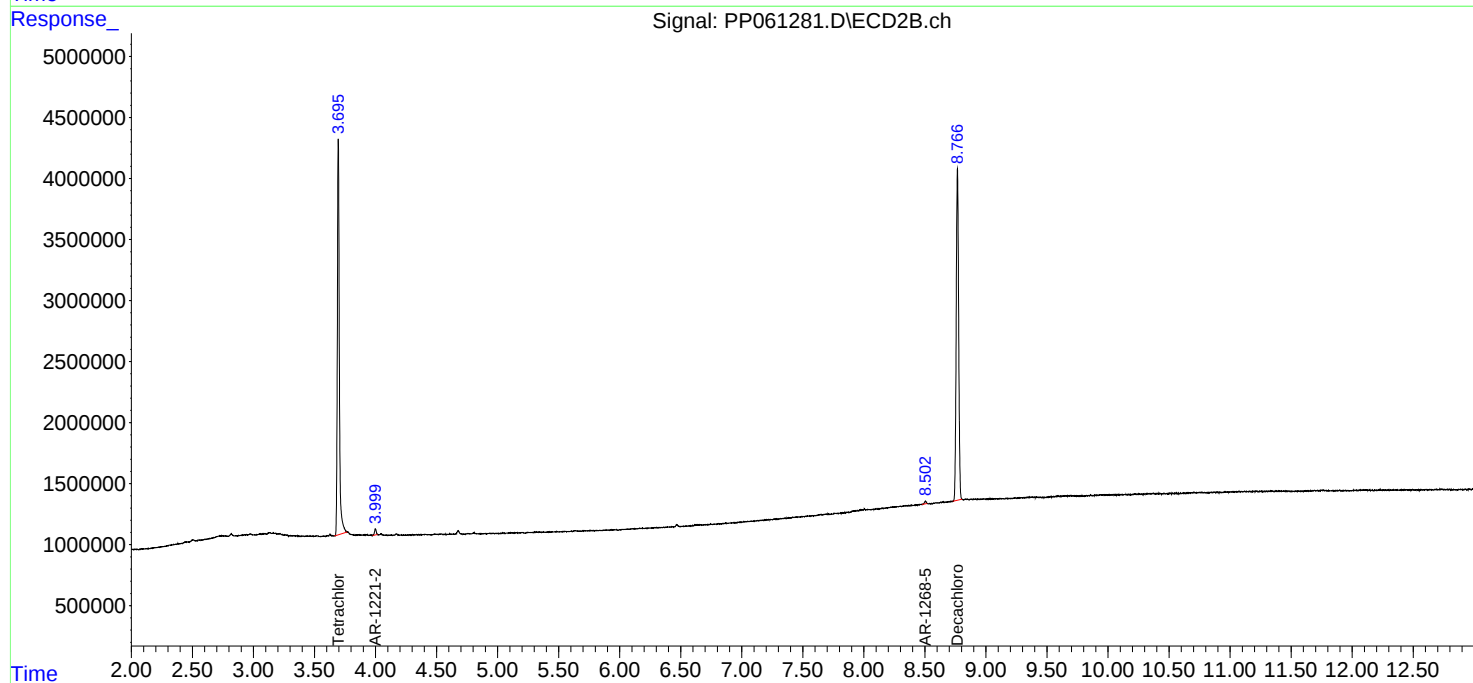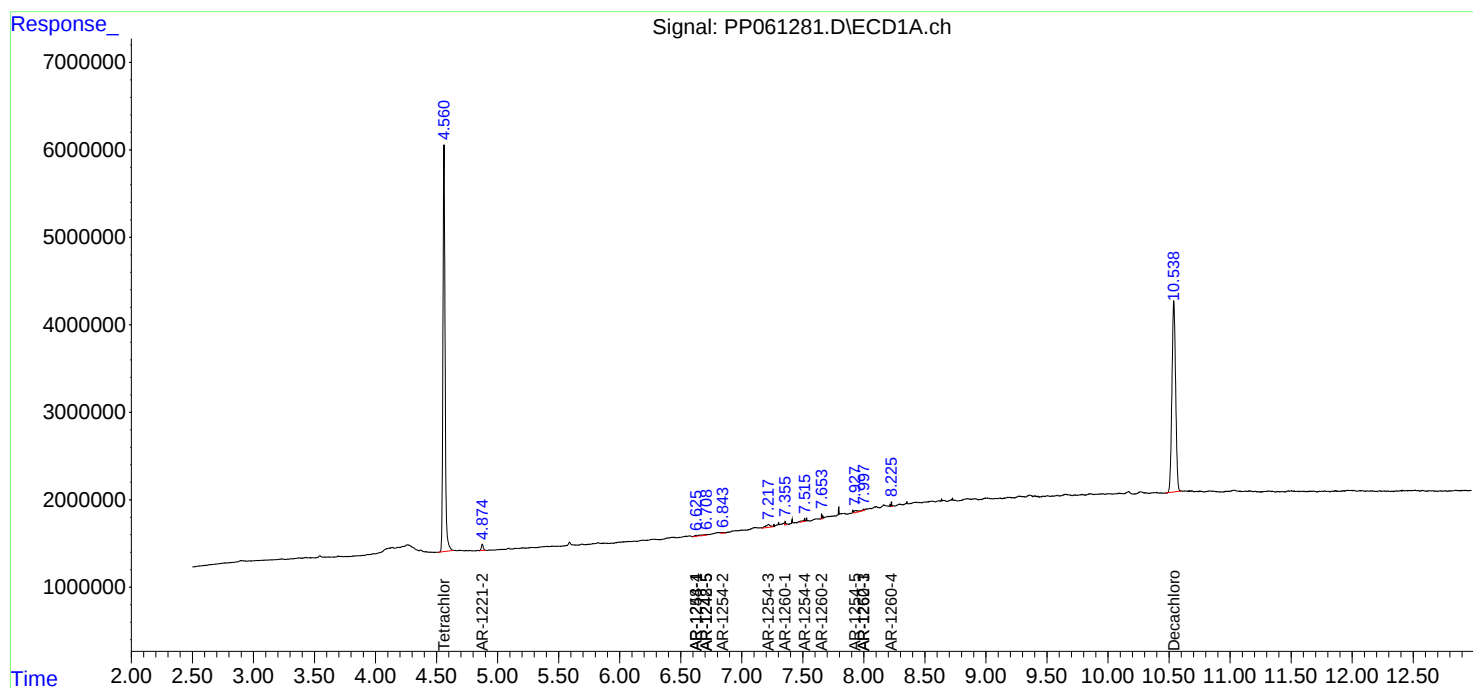


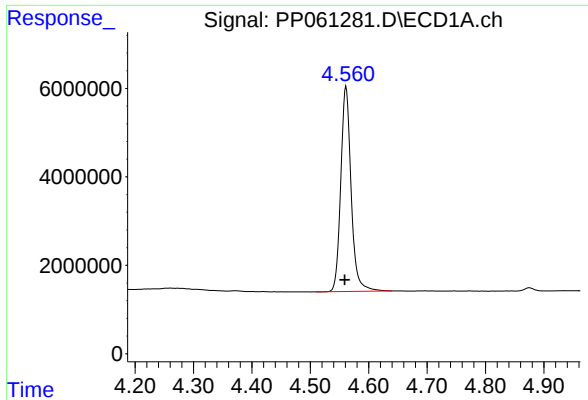

#1 Tetrachloro-m-xylene


R.T.: 4.561 min
Delta R.T.: 0.002 min
Response: 57142004
Conc: 23.13 ng/ml

Instrument :
ECD_P
ClientSampleId :

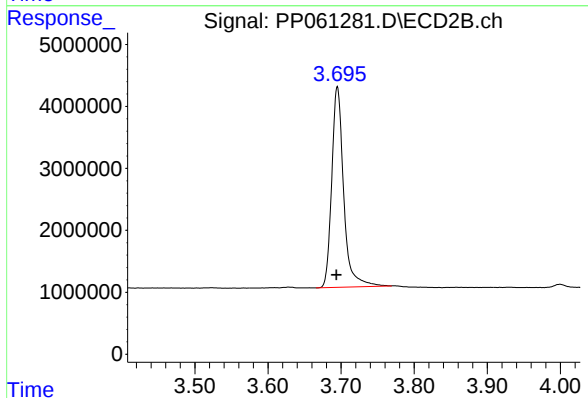


#1 Tetrachloro-m-xylene

R.T.: 3.695 min
Delta R.T.: 0.001 min
Response: 36719096
Conc: 24.57 ng/ml

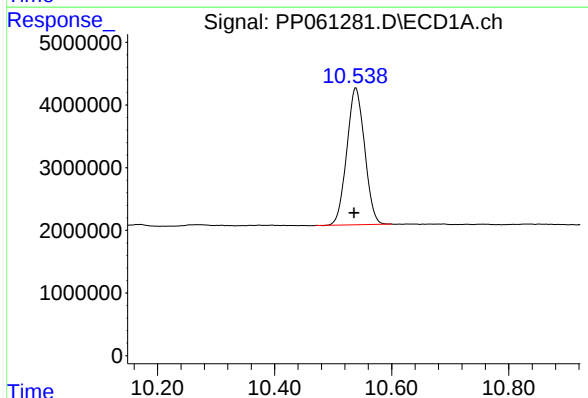


#2 Decachlorobiphenyl

R.T.: 10.539 min
Delta R.T.: 0.003 min
Response: 46033019
Conc: 24.41 ng/ml

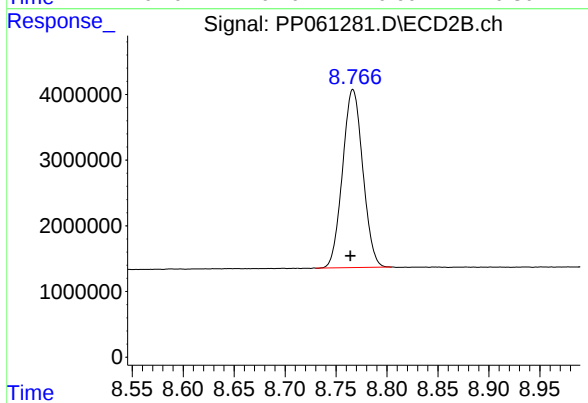

#2 Decachlorobiphenyl


R.T.: 8.767 min
Delta R.T.: 0.002 min
Response: 37529469
Conc: 24.44 ng/ml

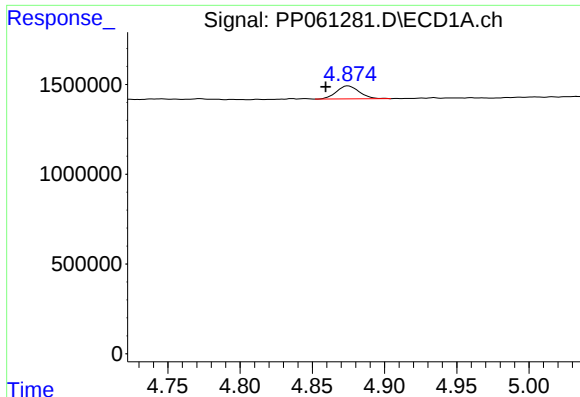

#9 AR-1221-2


R.T.: 4.875 min
Delta R.T.: 0.016 min
Response: 794199
Conc: 35.66 ng/ml

Instrument :
ECD_P
ClientSampleId :

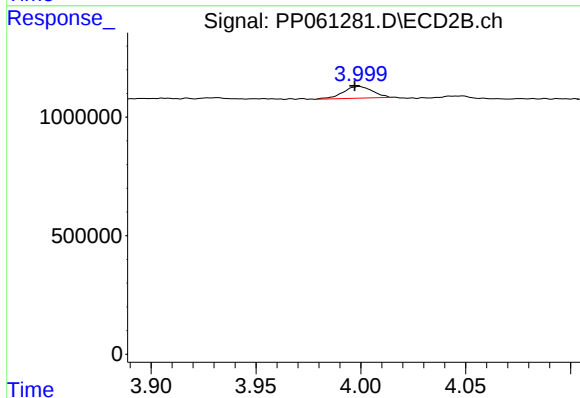


#9 AR-1221-2

R.T.: 3.999 min
Delta R.T.: 0.002 min
Response: 482957
Conc: 33.92 ng/ml

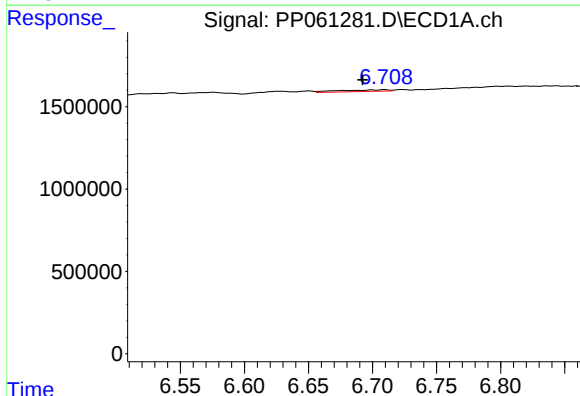


#20 AR-1242-5

R.T.: 6.709 min
Delta R.T.: 0.017 min
Response: 262309
Conc: 5.07 ng/ml

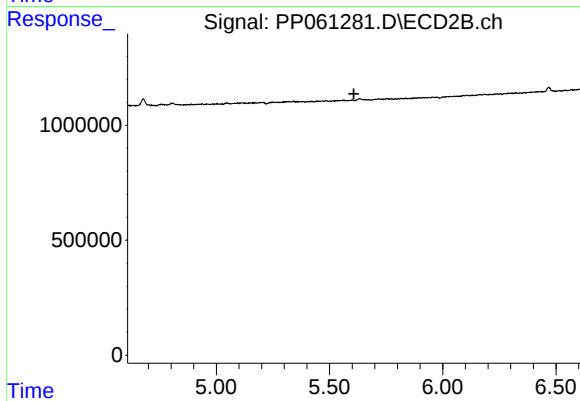

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 5.608 min
Response: 0
Conc: N.D.

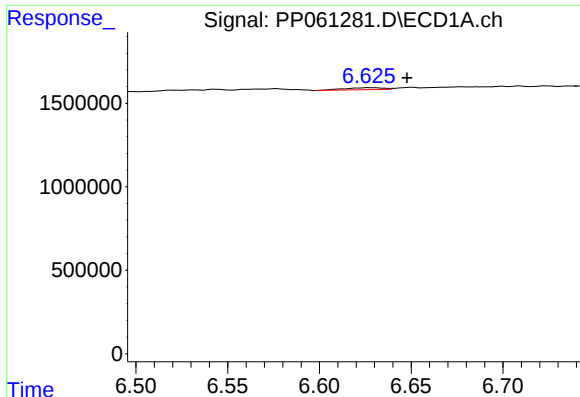

#24 AR-1248-4


R.T.: 6.627 min
Delta R.T.: -0.021 min
Response: 181340
Conc: 2.06 ng/ml

Instrument :
ECD_P
ClientSampleId :

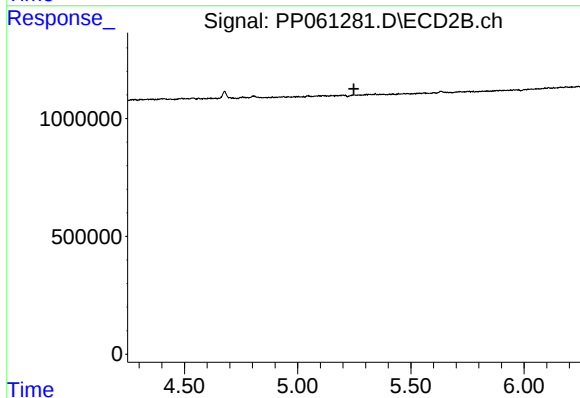


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.248 min
Response: 0
Conc: N.D.

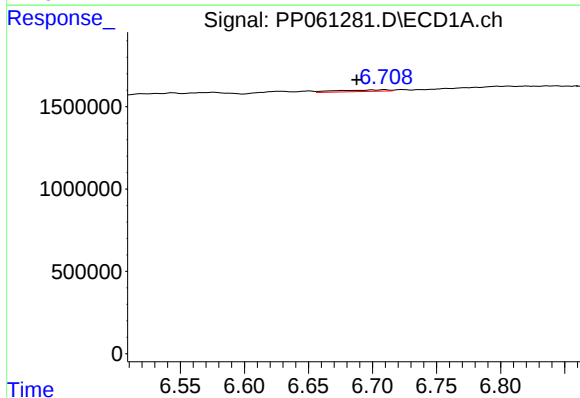


#25 AR-1248-5

R.T.: 6.709 min
Delta R.T.: 0.021 min
Response: 262309
Conc: 3.09 ng/ml

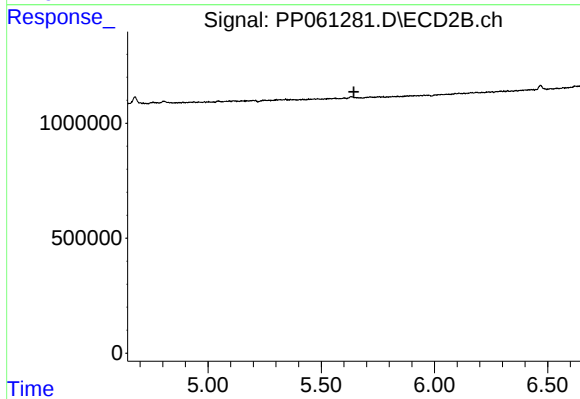

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 5.644 min
Response: 0
Conc: N.D.

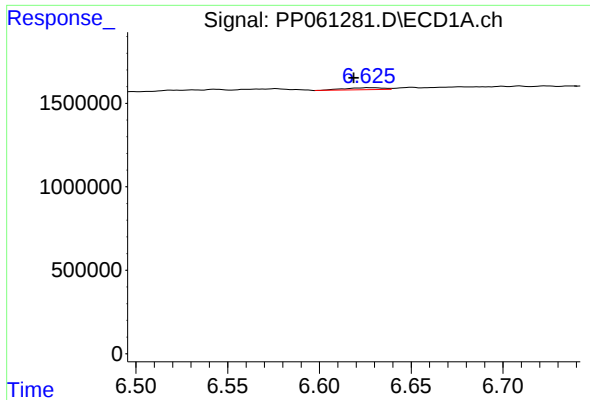

#26 AR-1254-1


R.T.: 6.627 min
Delta R.T.: 0.008 min
Response: 181340
Conc: 2.05 ng/ml

Instrument :
ECD_P
ClientSampleId :

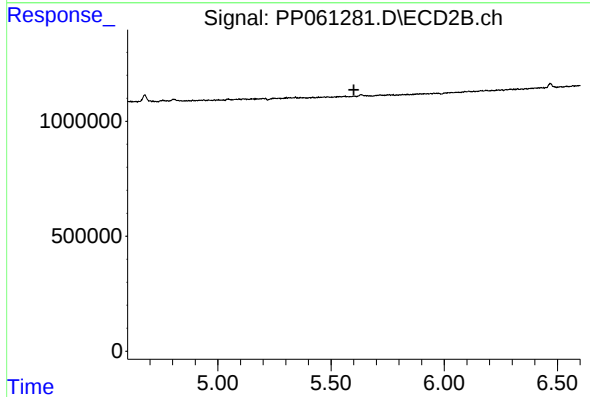


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 5.601 min
Response: 0
Conc: N.D.

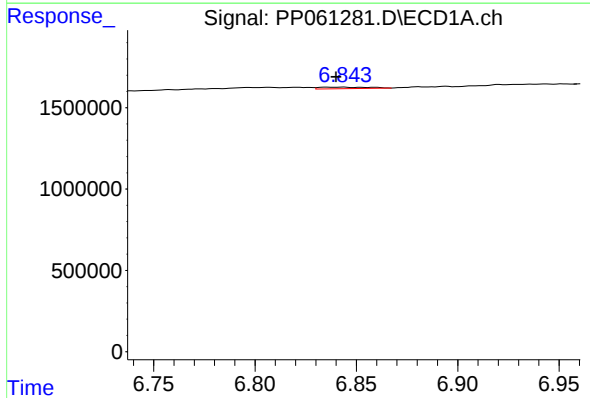


#27 AR-1254-2

R.T.: 6.844 min
Delta R.T.: 0.004 min
Response: 155232
Conc: 1.16 ng/ml

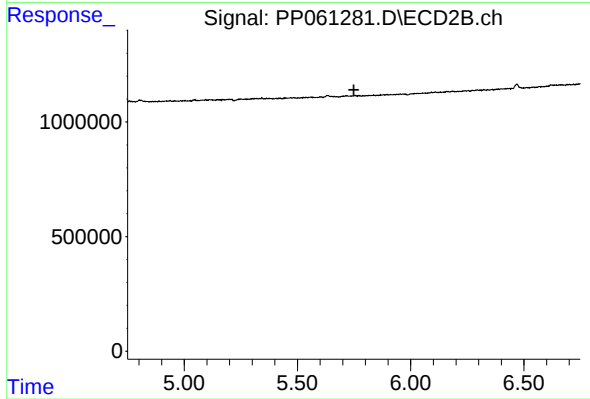

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T. : 5.749 min
Response: 0
Conc: N.D.

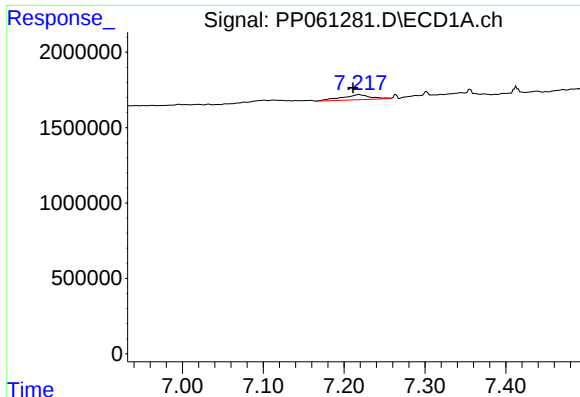

#28 AR-1254-3


R.T.: 7.218 min
Delta R.T.: 0.007 min
Response: 849226
Conc: 6.14 ng/ml

Instrument :
ECD_P
ClientSampleId :

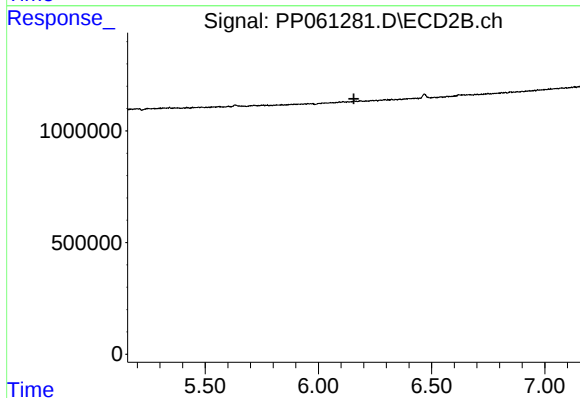


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.157 min
Response: 0
Conc: N.D.

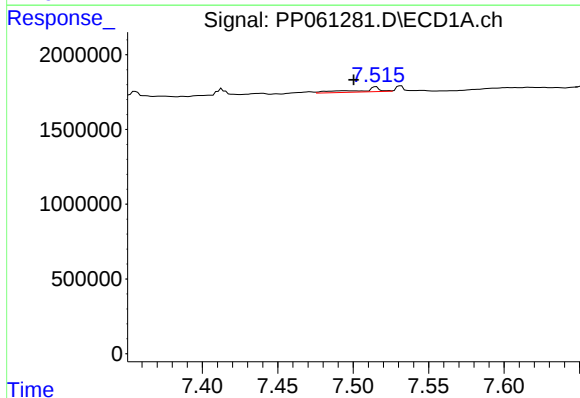


#29 AR-1254-4

R.T.: 7.515 min
Delta R.T.: 0.015 min
Response: 314886
Conc: 3.16 ng/ml

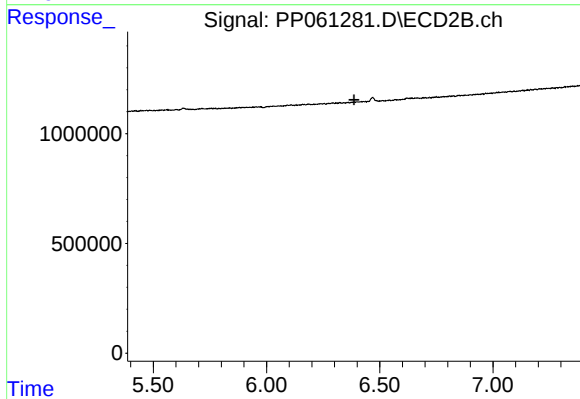

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.386 min
Response: 0
Conc: N.D.

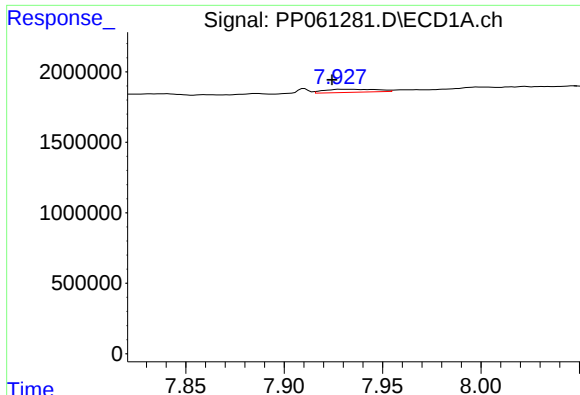

#30 AR-1254-5


R.T.: 7.929 min
Delta R.T.: 0.005 min
Response: 405612
Conc: 3.69 ng/ml

Instrument :
ECD_P
ClientSampleId :

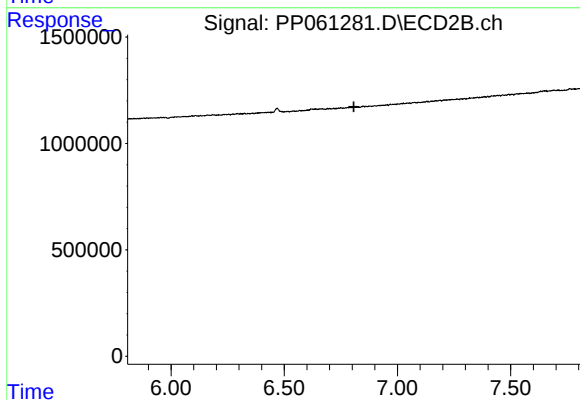


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 6.808 min
Response: 0
Conc: N.D.

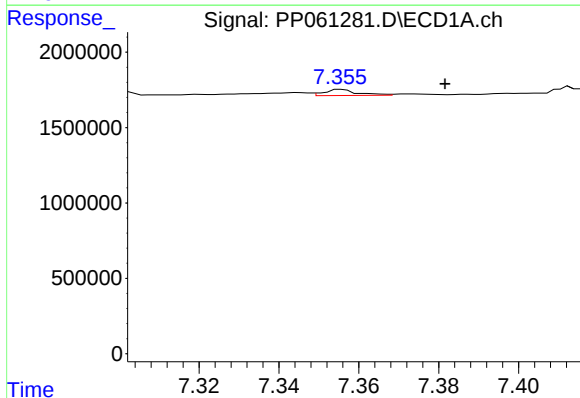


#31 AR-1260-1

R.T.: 7.356 min
Delta R.T.: -0.026 min
Response: 232043
Conc: 2.06 ng/ml

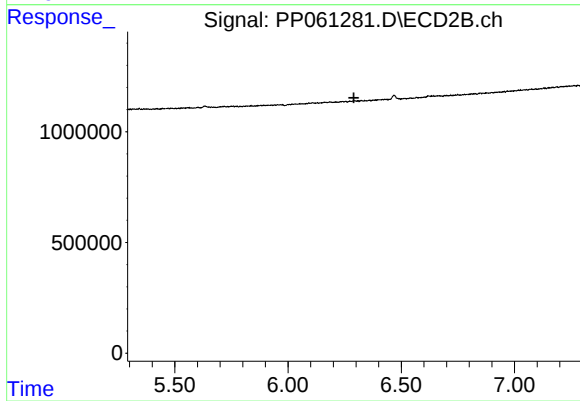

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 6.291 min
Response: 0
Conc: N.D.

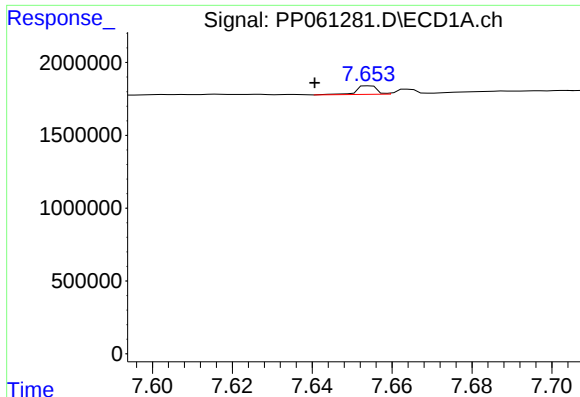

#32 AR-1260-2


R.T.: 7.654 min
Delta R.T.: 0.014 min
Response: 208328
Conc: 1.61 ng/ml

Instrument :
ECD_P
ClientSampleId :

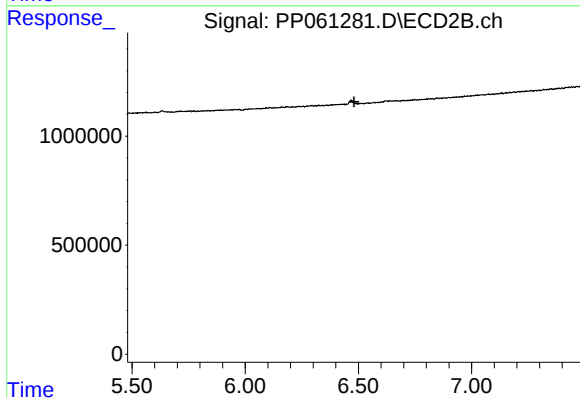


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.480 min
Response: 0
Conc: N.D.

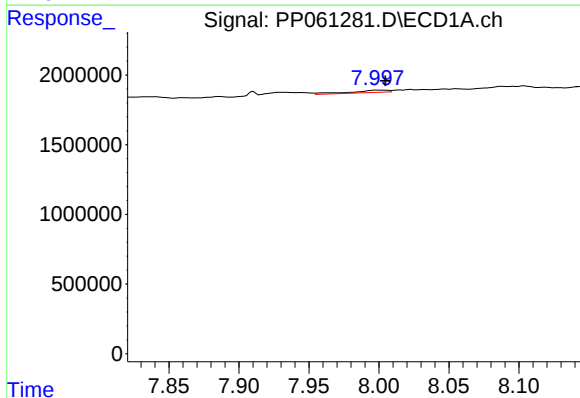


#33 AR-1260-3

R.T.: 7.999 min
Delta R.T.: -0.006 min
Response: 306687
Conc: 3.61 ng/ml

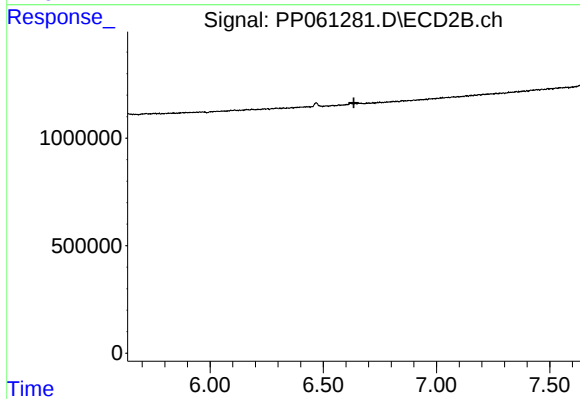

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 6.635 min
Response: 0
Conc: N.D.

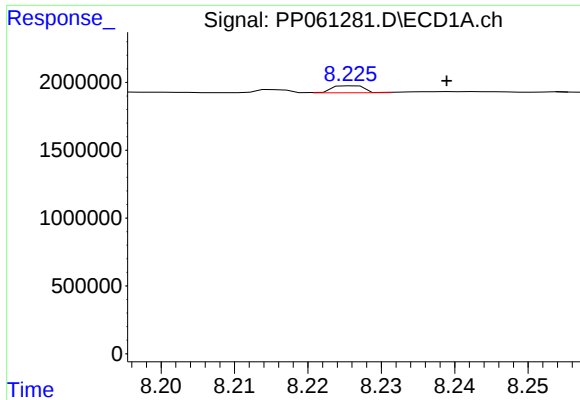

#34 AR-1260-4


R.T.: 8.226 min
Delta R.T.: -0.013 min
Response: 155473
Conc: 1.54 ng/ml

Instrument :
ECD_P
ClientSampleId :

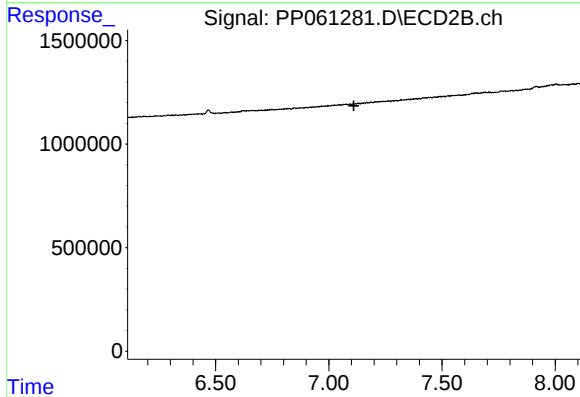


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.111 min
Response: 0
Conc: N.D.

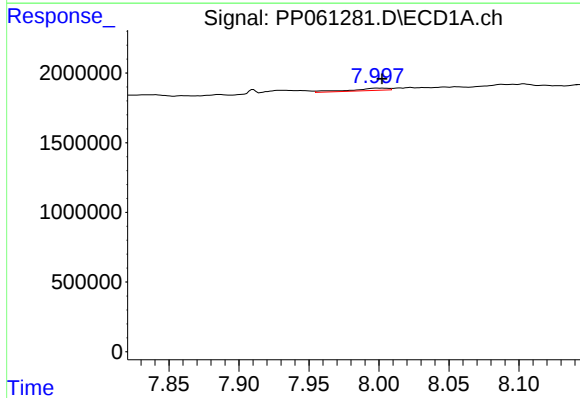


#36 AR-1262-1

R.T.: 7.999 min
Delta R.T.: -0.003 min
Response: 306687
Conc: 2.31 ng/ml

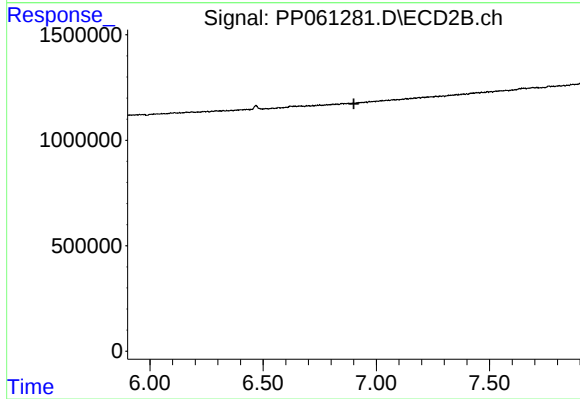

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 6.901 min
Response: 0
Conc: N.D.

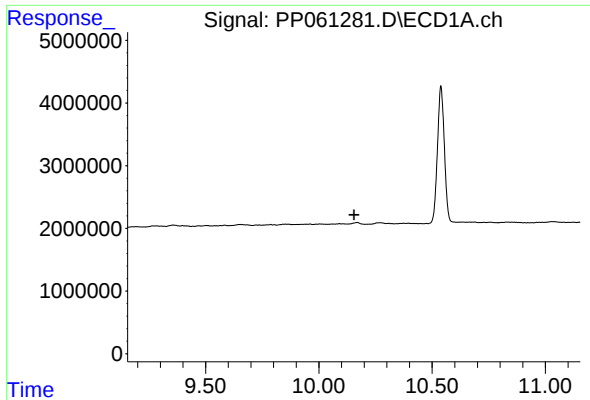

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.155 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

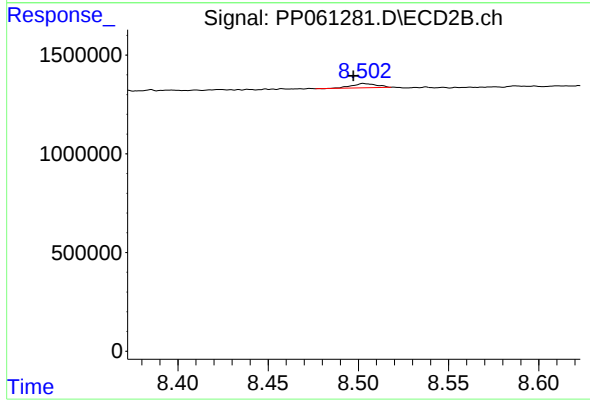

#45 AR-1268-5

R.T.: 8.503 min
Delta R.T.: 0.005 min
Response: 204125
Conc: 0.36 ng/ml