

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102723\
 Data File : PP061287.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2023 12:25
 Operator : YP\AJ
 Sample : AR1221ICC500
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1221ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 12:43:00 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 27 12:42:42 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.559	3.693	124.9E6	71698556	50.000	50.000
2) SA Decachlor...	10.533	8.765	92384320	74502321	50.000	50.000
Target Compounds						
8) L2 AR-1221-1	4.771	3.910	14851638	9777002	500.000	500.000
9) L2 AR-1221-2	4.859	3.997	11135085	7120053	500.000	500.000
10) L2 AR-1221-3	4.937	4.074	32397077	20295508	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102723\
Data File : PP061287.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2023 12:25
Operator : YP\AJ
Sample : AR1221ICC500
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1221ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 12:43:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102723.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 27 12:42:42 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

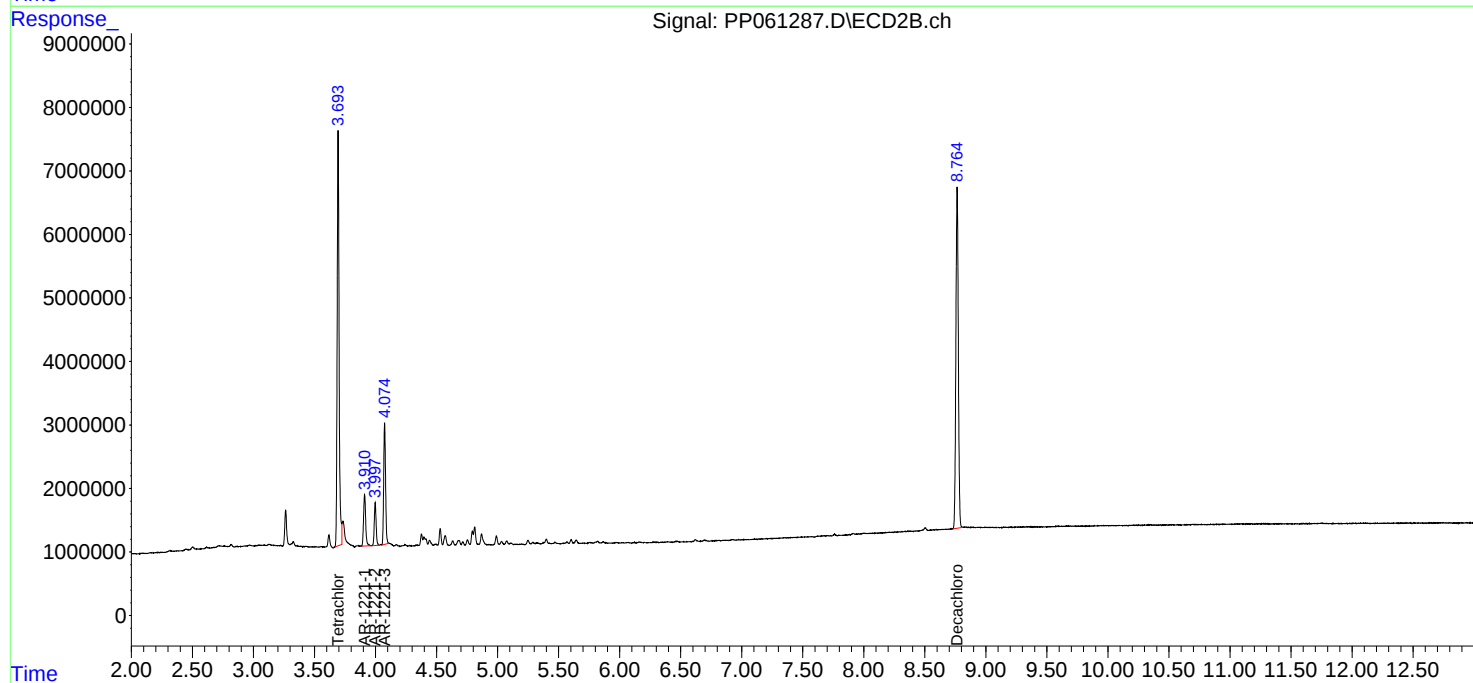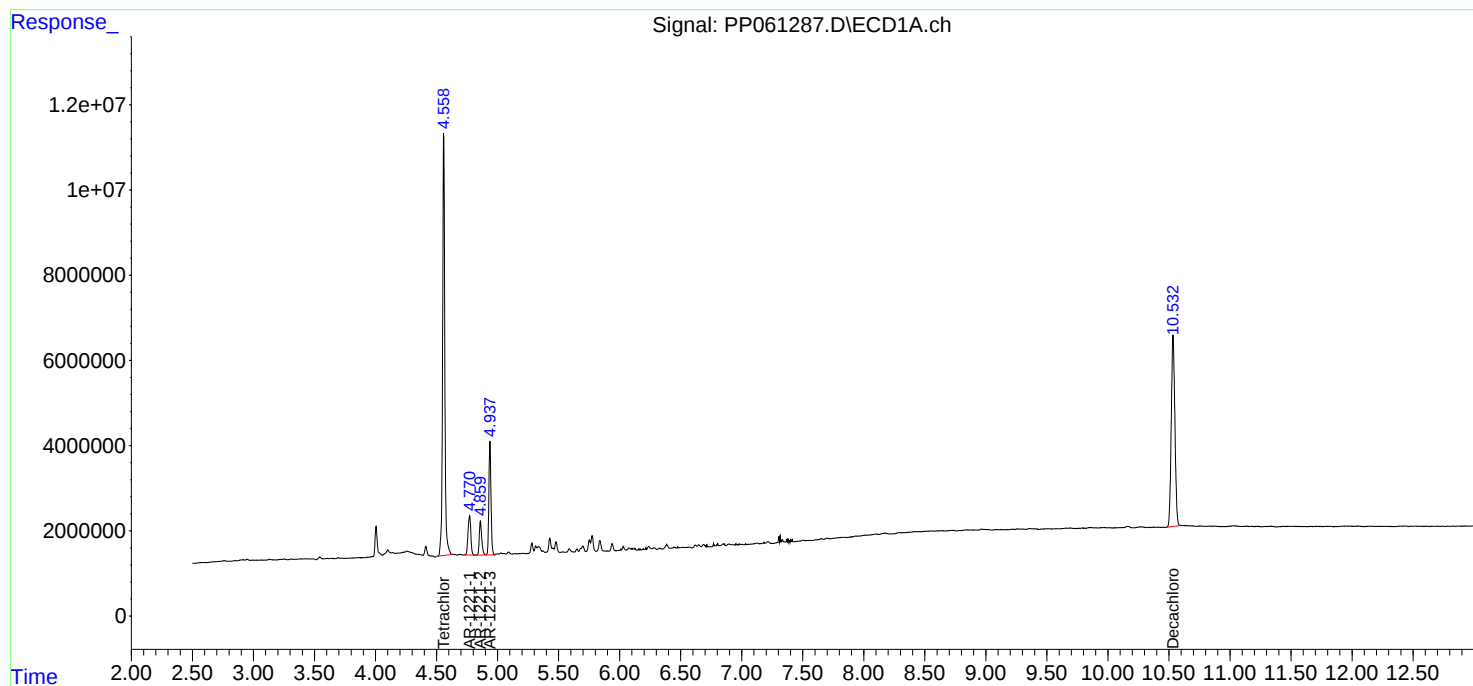


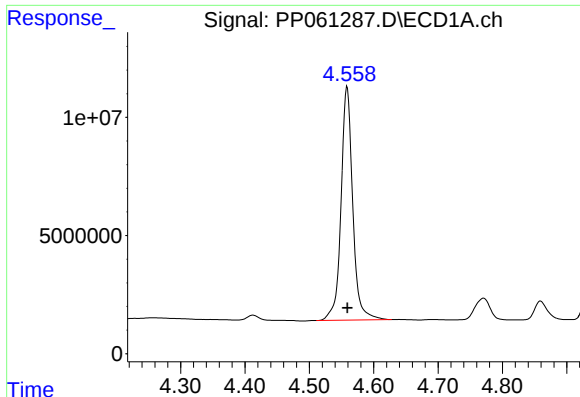

#1 Tetrachloro-m-xylene


R.T.: 4.559 min
Delta R.T.: 0.000 min
Response: 124853864
Conc: 50.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1221ICC500

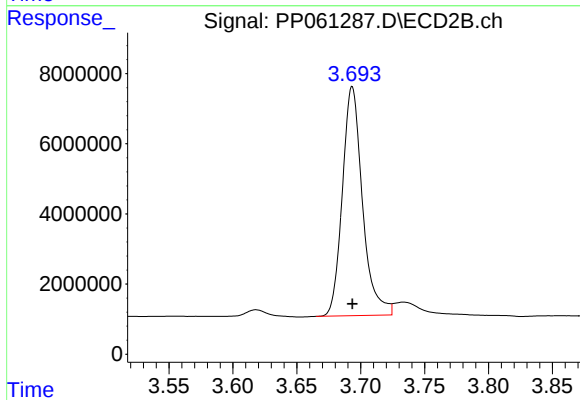


#1 Tetrachloro-m-xylene

R.T.: 3.693 min
Delta R.T.: 0.000 min
Response: 71698556
Conc: 50.00 ng/ml

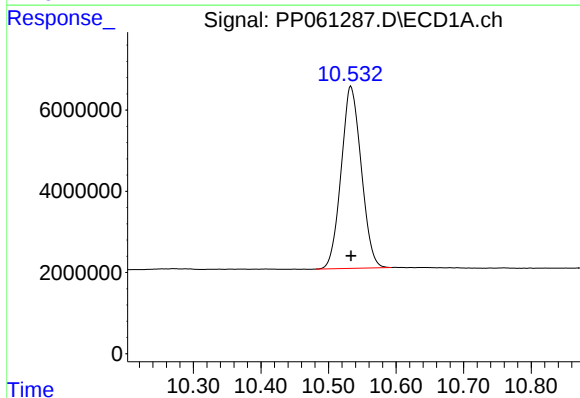


#2 Decachlorobiphenyl

R.T.: 10.533 min
Delta R.T.: 0.000 min
Response: 92384320
Conc: 50.00 ng/ml

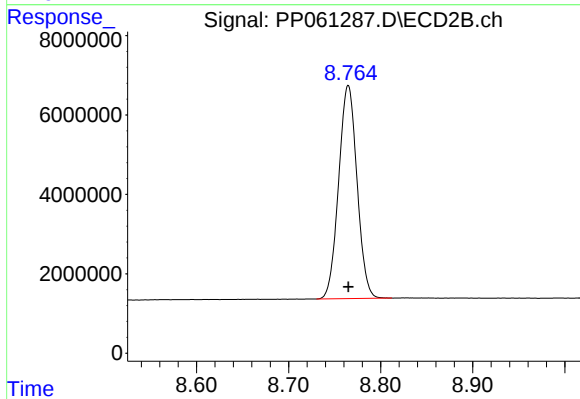

#2 Decachlorobiphenyl


R.T.: 8.765 min
Delta R.T.: 0.000 min
Response: 74502321
Conc: 50.00 ng/ml

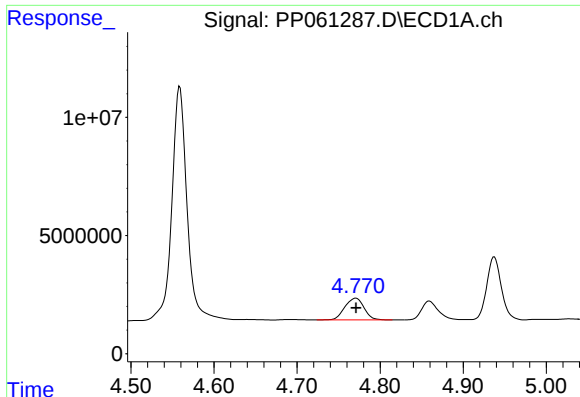

#8 AR-1221-1


R.T.: 4.771 min
Delta R.T.: 0.000 min
Response: 14851638
Conc: 500.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1221ICC500

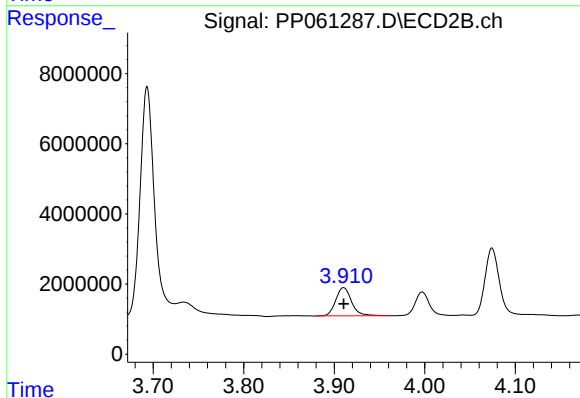


#8 AR-1221-1

R.T.: 3.910 min
Delta R.T.: 0.000 min
Response: 9777002
Conc: 500.00 ng/ml

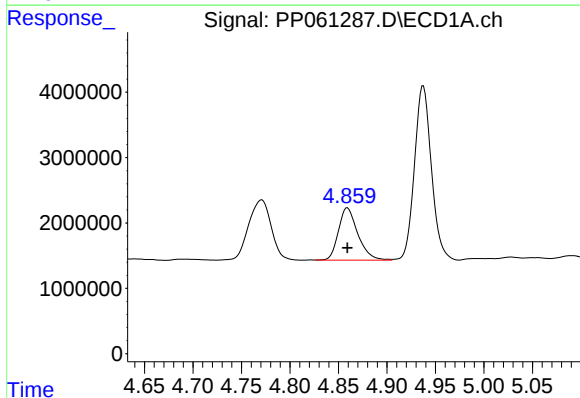


#9 AR-1221-2

R.T.: 4.859 min
Delta R.T.: 0.000 min
Response: 11135085
Conc: 500.00 ng/ml

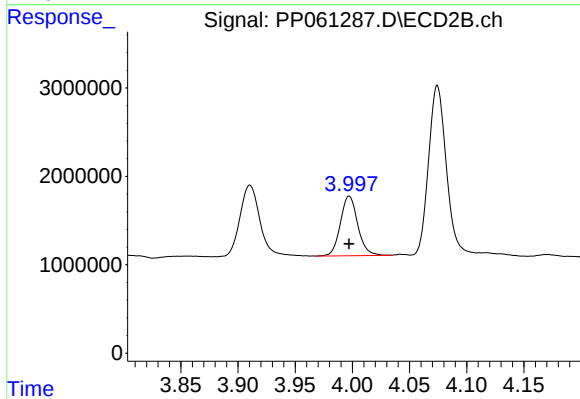

#9 AR-1221-2


R.T.: 3.997 min
Delta R.T.: 0.000 min
Response: 7120053
Conc: 500.00 ng/ml

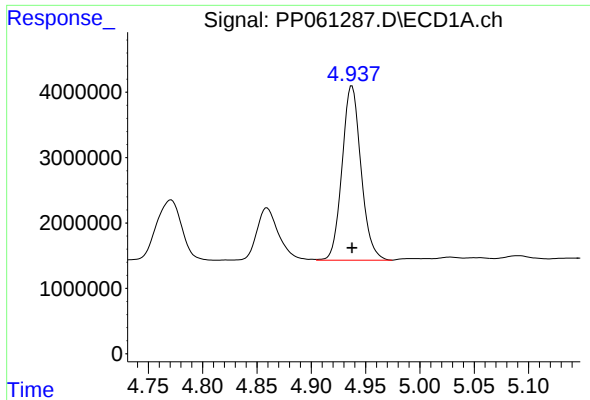

#10 AR-1221-3

R.T.: 4.937 min
Delta R.T.: 0.000 min
Response: 32397077
Conc: 500.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1221ICC500

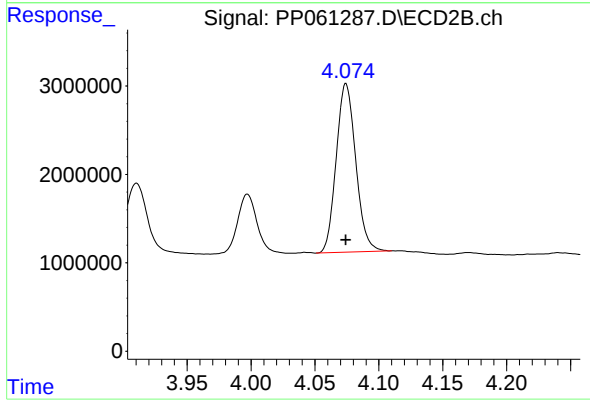

#10 AR-1221-3

R.T.: 4.074 min
Delta R.T.: 0.000 min
Response: 20295508
Conc: 500.00 ng/ml