

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ010422\
 Data File : PQ055541.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2022 22:41
 Operator : AJ\MA
 Sample : M5196-07
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 COMPOSITE-SAMPLE-4-SHALLOW

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 05:18:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ010422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 04 15:29:13 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.240	4.305	271.5E6	220.4E6	23.651	22.902
2) SA Decachlor...	11.422	9.684	311.2E6	152.7E6	20.867	20.550

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ010422\
Data File : PQ055541.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2022 22:41
Operator : AJ\MA
Sample : M5196-07
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
COMPOSITE-SAMPLE-4-SHALLOW

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 05:18:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ010422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 04 15:29:13 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

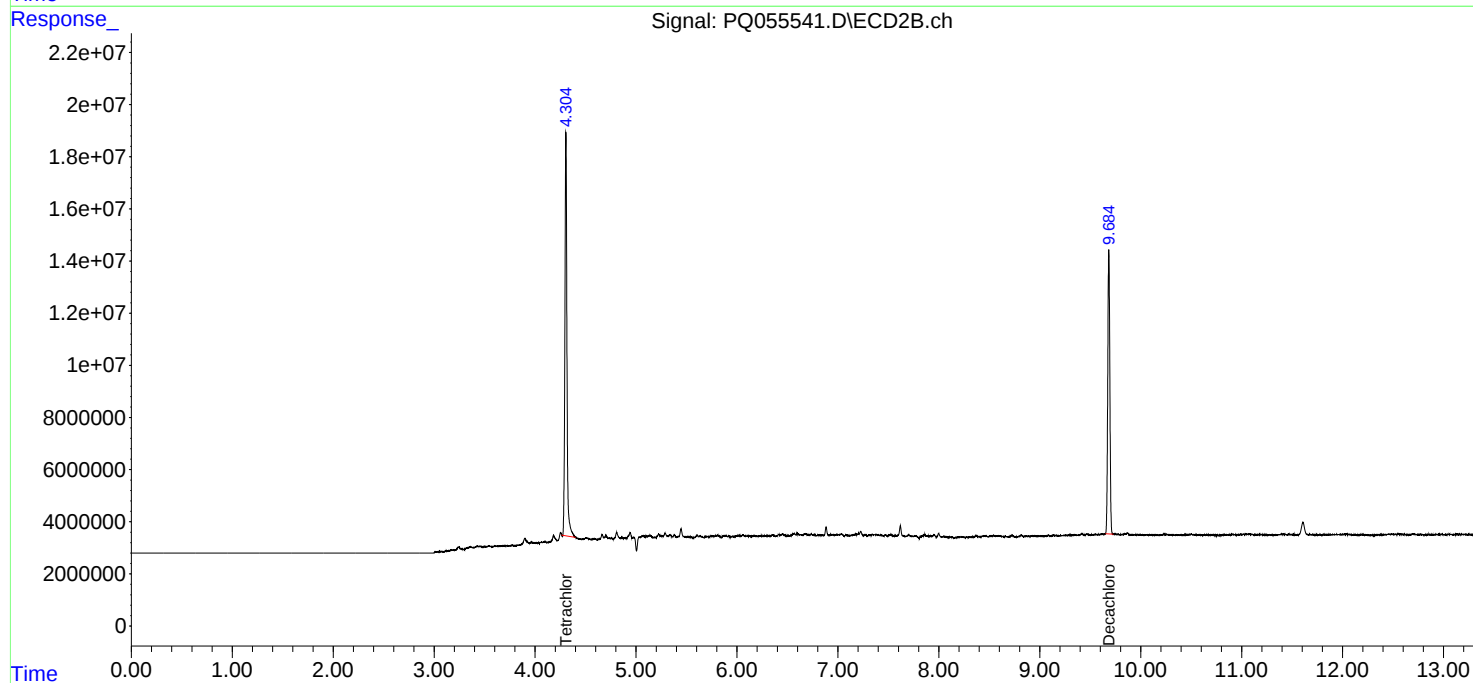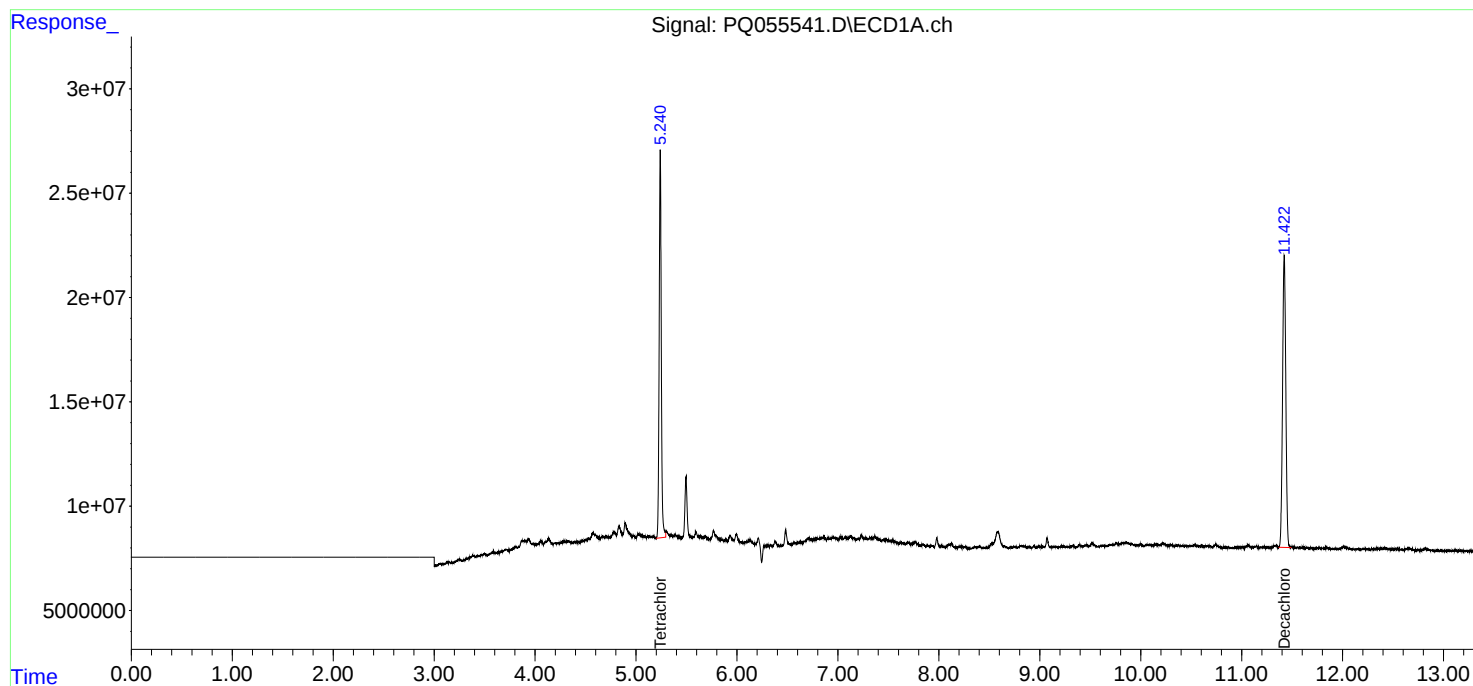


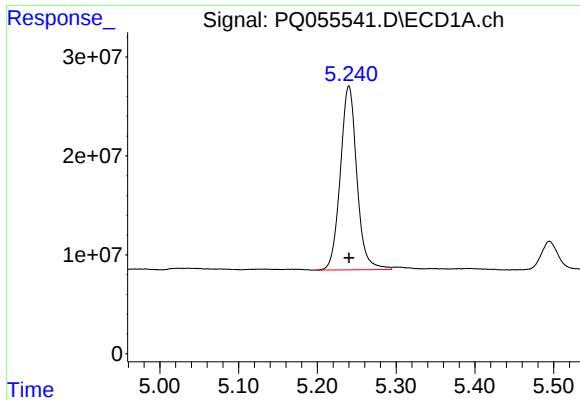

#1 Tetrachloro-m-xylene


R.T.: 5.240 min
Delta R.T.: 0.000 min
Response: 271490026
Conc: 23.65 ng/ml

Instrument :
ECD_Q
ClientSampleId :
COMPOSITE-SAMPLE-4-SHALLOW

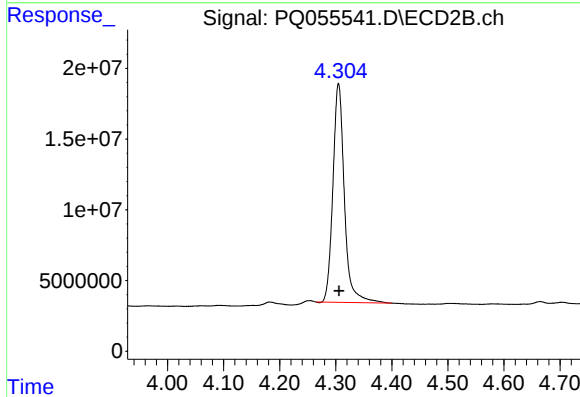


#1 Tetrachloro-m-xylene

R.T.: 4.305 min
Delta R.T.: -0.001 min
Response: 220435480
Conc: 22.90 ng/ml

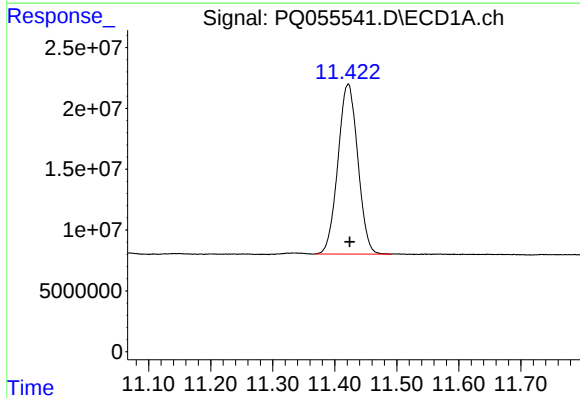

#2 Decachlorobiphenyl

R.T.: 11.422 min
Delta R.T.: -0.003 min
Response: 311202623
Conc: 20.87 ng/ml

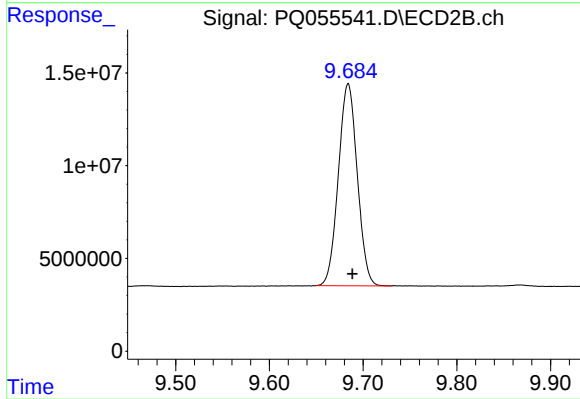

#2 Decachlorobiphenyl

R.T.: 9.684 min
Delta R.T.: -0.004 min
Response: 152721928
Conc: 20.55 ng/ml