

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ010422\
 Data File : PQ055544.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2022 23:30
 Operator : AJ\MA
 Sample : M5340-01 10X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 BAYSHORE-FILL

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/05/2022
 Supervised By :mohammad ahmed 01/05/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 05:20:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ010422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 04 15:29:13 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.240	4.306	41304551	19793298	3.598	2.056 #
2) SA Decachlor...	11.422	9.684	35228196	16076855	2.362	2.163

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ010422\
Data File : PQ055544.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2022 23:30
Operator : AJ\MA
Sample : M5340-01 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
BAYSHORE-FILL


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/05/2022
Supervised By :mohammad ahmed 01/05/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 05:20:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ010422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 04 15:29:13 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

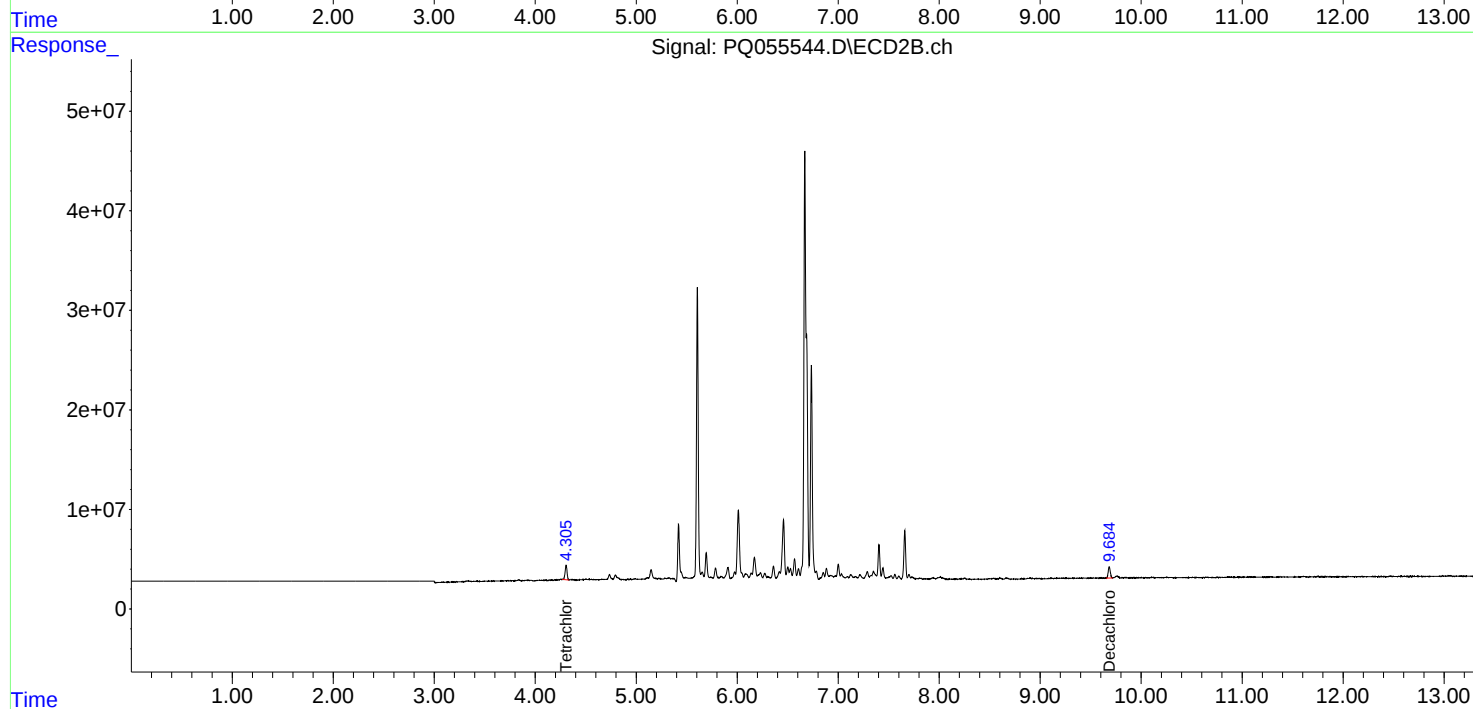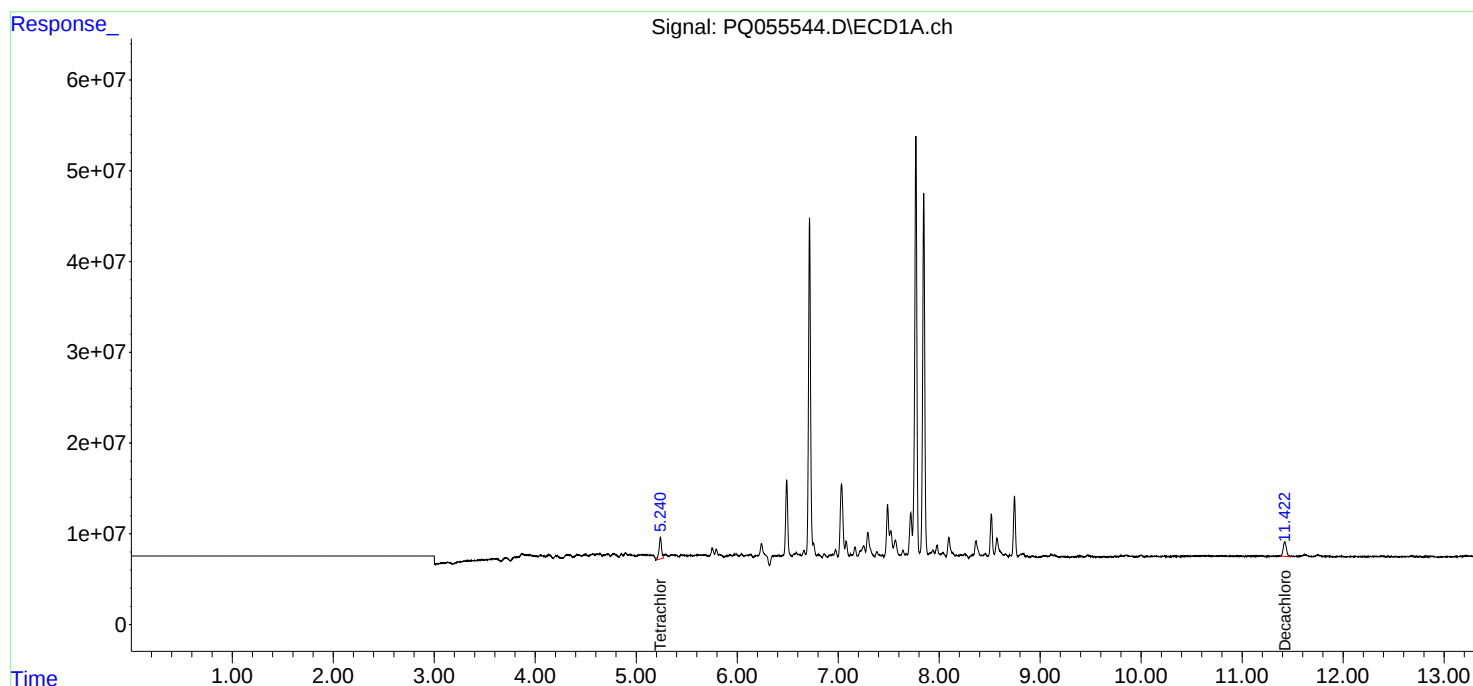

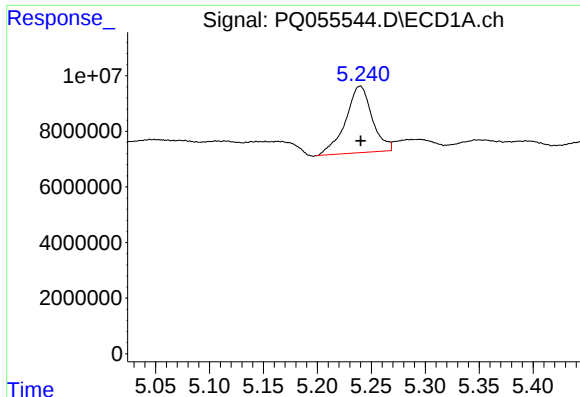


#1 Tetrachloro-m-xylene

R.T.: 5.240 min
Delta R.T.: 0.000 min
Response: 41304551
Conc: 3.60 ng/ml

Instrument :
ECD_Q
ClientSampleId :
BAYSHORE-FILL


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/05/2022
Supervised By :mohammad ahmed 01/05/2022

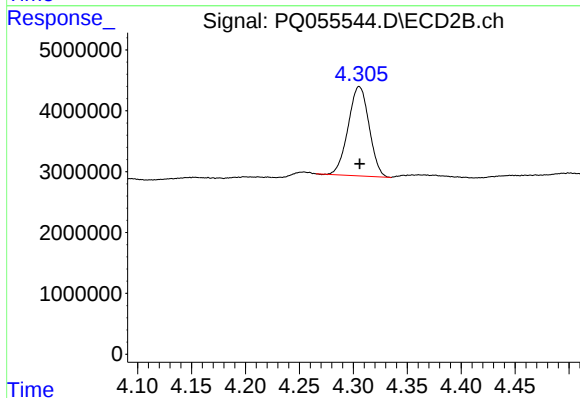


#1 Tetrachloro-m-xylene

R.T.: 4.306 min
Delta R.T.: 0.000 min
Response: 19793298
Conc: 2.06 ng/ml

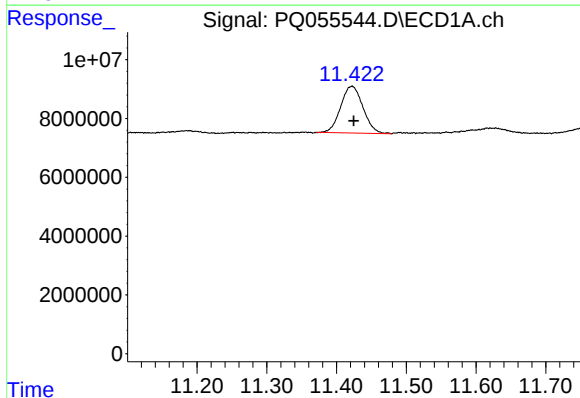

#2 Decachlorobiphenyl

R.T.: 11.422 min
Delta R.T.: -0.002 min
Response: 35228196
Conc: 2.36 ng/ml

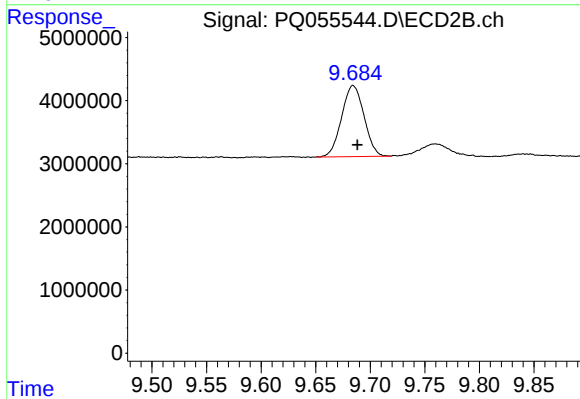

#2 Decachlorobiphenyl

R.T.: 9.684 min
Delta R.T.: -0.004 min
Response: 16076855
Conc: 2.16 ng/ml