

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ010422\
 Data File : PQ055558.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2022 08:09
 Operator : AJ\MA
 Sample : M5336-11
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 40565

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/05/2022
 Supervised By :mohammad ahmed 01/05/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 09:42:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ010422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 04 15:29:13 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.239	4.305	299.5E6	244.8E6	26.095m	25.435
2) SA Decachlor...	11.425	9.685	312.2E6	149.0E6	20.933	20.044

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ010422\
Data File : PQ055558.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2022 08:09
Operator : AJ\MA
Sample : M5336-11
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
40565


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/05/2022
Supervised By :mohammad ahmed 01/05/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 09:42:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ010422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 04 15:29:13 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

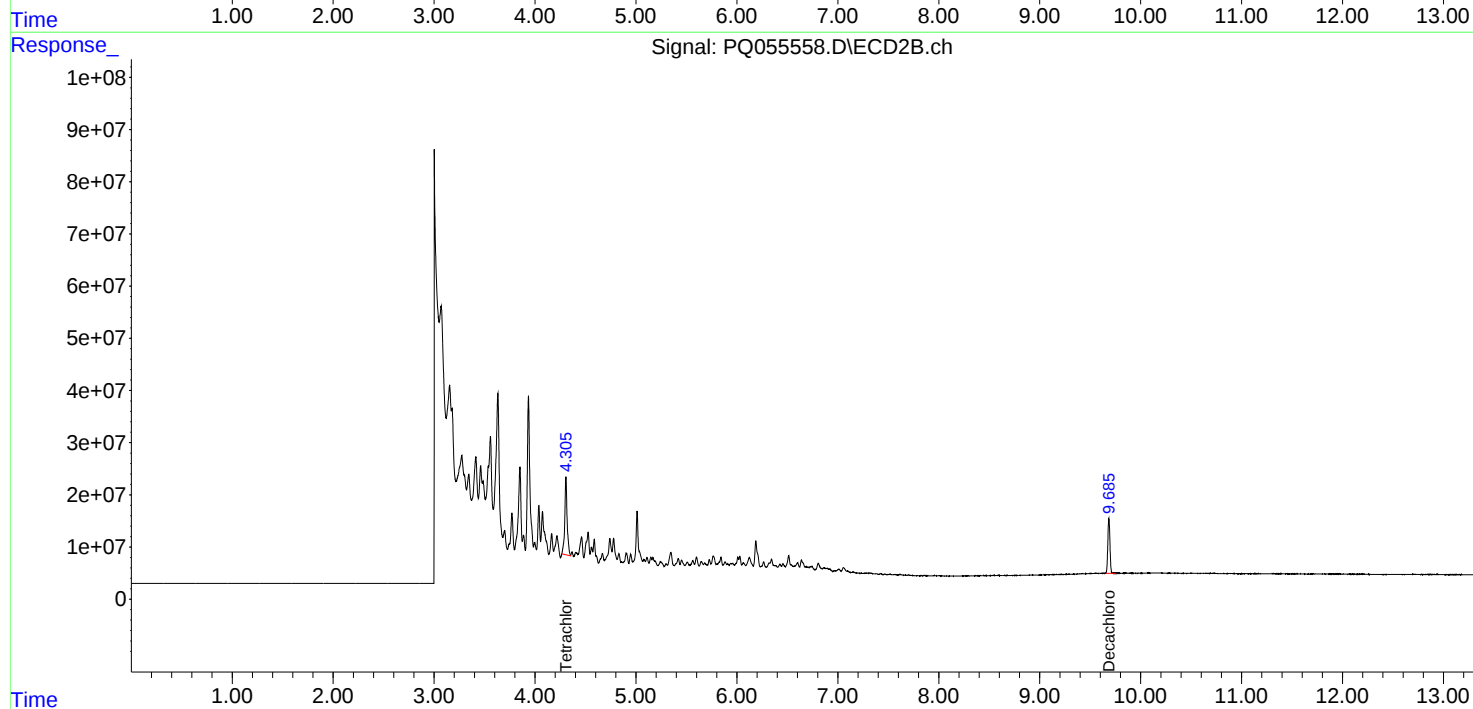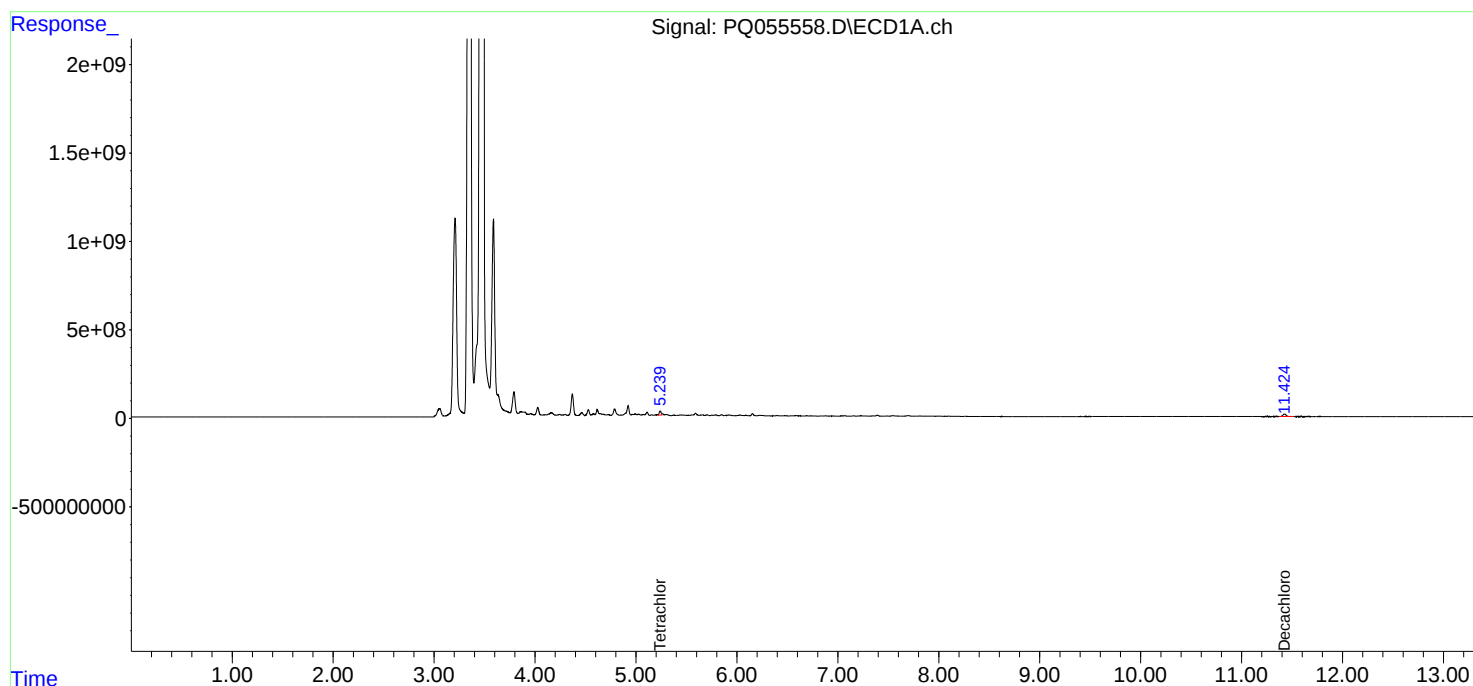

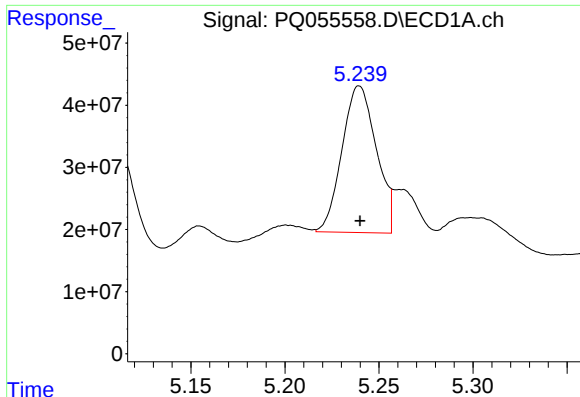


#1 Tetrachloro-m-xylene

R.T.: 5.239 min
Delta R.T.: -0.001 min
Response: 299541658
Conc: 26.09 ng/ml

Instrument :
ECD_Q
ClientSampleId :
40565


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/05/2022
Supervised By :mohammad ahmed 01/05/2022

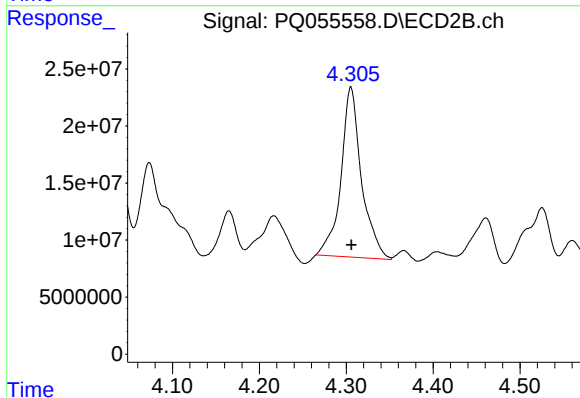


#1 Tetrachloro-m-xylene

R.T.: 4.305 min
Delta R.T.: 0.000 min
Response: 244810530
Conc: 25.43 ng/ml

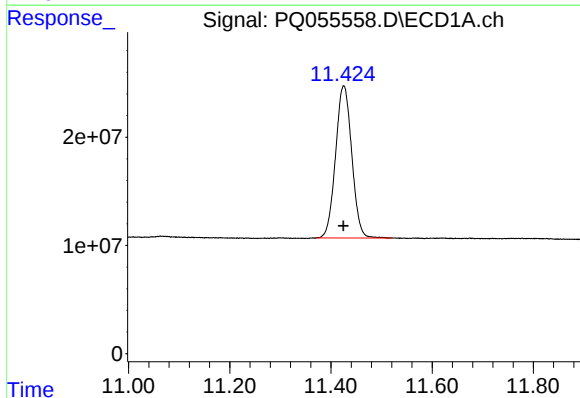

#2 Decachlorobiphenyl

R.T.: 11.425 min
Delta R.T.: 0.000 min
Response: 312185310
Conc: 20.93 ng/ml

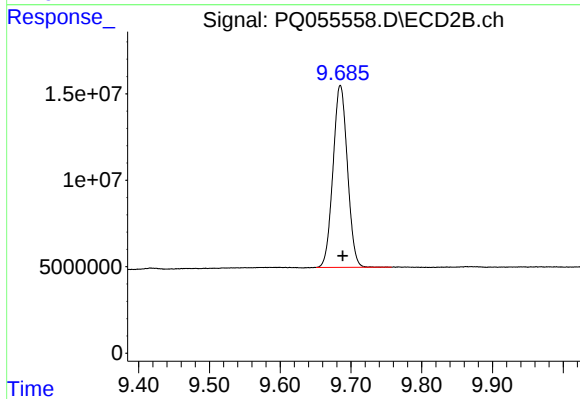

#2 Decachlorobiphenyl

R.T.: 9.685 min
Delta R.T.: -0.003 min
Response: 148961322
Conc: 20.04 ng/ml