

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ010521\
 Data File : PQ051608.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2021 14:13
 Operator : DD\AJ
 Sample : L5214-01
 Misc : AR1660 MDL 25 PPB
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 MDL-WATER-QT1-2021-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 06 09:15:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ122120CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 22 06:18:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.238	4.258	518.8E6	141.8E6	20.121	19.418
2)	SA Decachlor...	11.433	9.609	732.4E6	233.9E6	39.946	38.459
Target Compounds							
3)	L1 AR-1016-1	6.560	5.516	16539446	6728764	19.575	26.248 #
4)	L1 AR-1016-2	6.583	5.536	34638078	7547880	27.964	21.084
5)	L1 AR-1016-3	6.651	5.730	20231434	4946577	27.645	26.873
6)	L1 AR-1016-4	6.757	5.780	16570636	4190436	26.960	29.039
7)	L1 AR-1016-5	7.073	6.011	15981652	4656765	26.860	24.475
8)	L2 AR-1221-1	5.498	4.513	4657169	645893	17.546	8.380 #
9)	L2 AR-1221-2	5.592	4.614	8701993	2654298	47.643	49.633
10)	L2 AR-1221-3	5.674	4.704	11625666	3868372	18.836	21.118
11)	L3 AR-1232-1	5.674	4.704	11625666	3868372	25.255	28.298
12)	L3 AR-1232-2	6.265	5.536	16068152	7547880	65.105	53.671
13)	L3 AR-1232-3	6.583	5.730	34638078	4946577	68.447	69.125
14)	L3 AR-1232-4	6.757	5.825	16570636	4739483	66.353	77.092
15)	L3 AR-1232-5	6.852	6.011	14106236	4656765	79.512	72.592
16)	L4 AR-1242-1	6.560	5.516	16539446	6728764	23.538	32.004 #
17)	L4 AR-1242-2	6.583	5.536	34638078	7547880	33.614	25.866
18)	L4 AR-1242-3	6.651	5.730	20231434	4946577	32.904	32.784
19)	L4 AR-1242-4	6.757	5.825	16570636	4739483	32.242	32.739
20)	L4 AR-1242-5	7.542	6.390	4836377	4299875	8.773	22.504 #
21)	L5 AR-1248-1	6.560	5.516	16539446	6728764	29.236	40.041 #
22)	L5 AR-1248-2	6.852	5.780	14106236	4190436	17.534	18.502
23)	L5 AR-1248-3	7.073	5.825	15981652	4739483	17.239	20.155
24)	L5 AR-1248-4	7.500	6.011	3358027	4656765	3.165	16.940 #
25)	L5 AR-1248-5	7.542	6.433	4836377	740158	4.661	2.565 #
26)	L6 AR-1254-1	7.470	6.390	12681547	4299875	12.895	10.132
27)	L6 AR-1254-2	7.697	6.548	13841658	4330372	9.090	11.797 #
28)	L6 AR-1254-3	8.081	6.988	8922098	7450601	5.400	12.210 #
29)	L6 AR-1254-4	8.374	7.208	8224424	1047717	6.917	2.774 #
30)	L6 AR-1254-5	8.806	7.637	43354951	14148856	34.351	26.939
31)	L7 AR-1260-1	8.247	7.106	30372166	10723173	29.324	30.229
32)	L7 AR-1260-2	8.511	7.302	40627719	13314946	32.854	30.096
33)	L7 AR-1260-3	8.878	7.458	22437210	12490655	24.708	30.143
34)	L7 AR-1260-4	9.121	7.943	26648596	8081167	24.996	23.302
35)	L7 AR-1260-5	9.467	8.188	52677722	18478401	23.656	21.401
36)	L8 AR-1262-1	8.878	7.637	22437210	14148856	14.787	49.352 #
37)	L8 AR-1262-2	9.467	8.188	52677722	18478401	18.775	18.124
38)	L8 AR-1262-3	9.829	8.477	31444416	3748056	26.201	9.961 #
39)	L8 AR-1262-4	9.881	8.539	17502067	14133060	24.843	19.274
40)	L8 AR-1262-5	10.619	9.044	12156650	4168647	12.771	12.663
41)	L9 AR-1268-1	9.829	8.477	31444416	3748056	9.529	3.227 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ010521\
 Data File : PQ051608.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2021 14:13
 Operator : DD\AJ
 Sample : L5214-01
 Misc : AR1660 MDL 25 PPB
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 MDL-WATER-QT1-2021-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 06 09:15:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ122120CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 22 06:18:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	9.881	8.539	17502067	14133060	5.829	13.282 #
43) L9	AR-1268-3	10.145	8.754	2632066	1507113	1.029	1.691 #
44) L9	AR-1268-4	10.619	9.044	12156650	4168647	11.193	11.301
45) L9	AR-1268-5	11.065	9.346	9149297	3013595	1.094	1.082



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ010521\
Data File : PQ051608.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2021 14:13
Operator : DD\AJ
Sample : L5214-01
Misc : AR1660 MDL 25 PPB
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-QT1-2021-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 06 09:15:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ122120CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 22 06:18:29 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

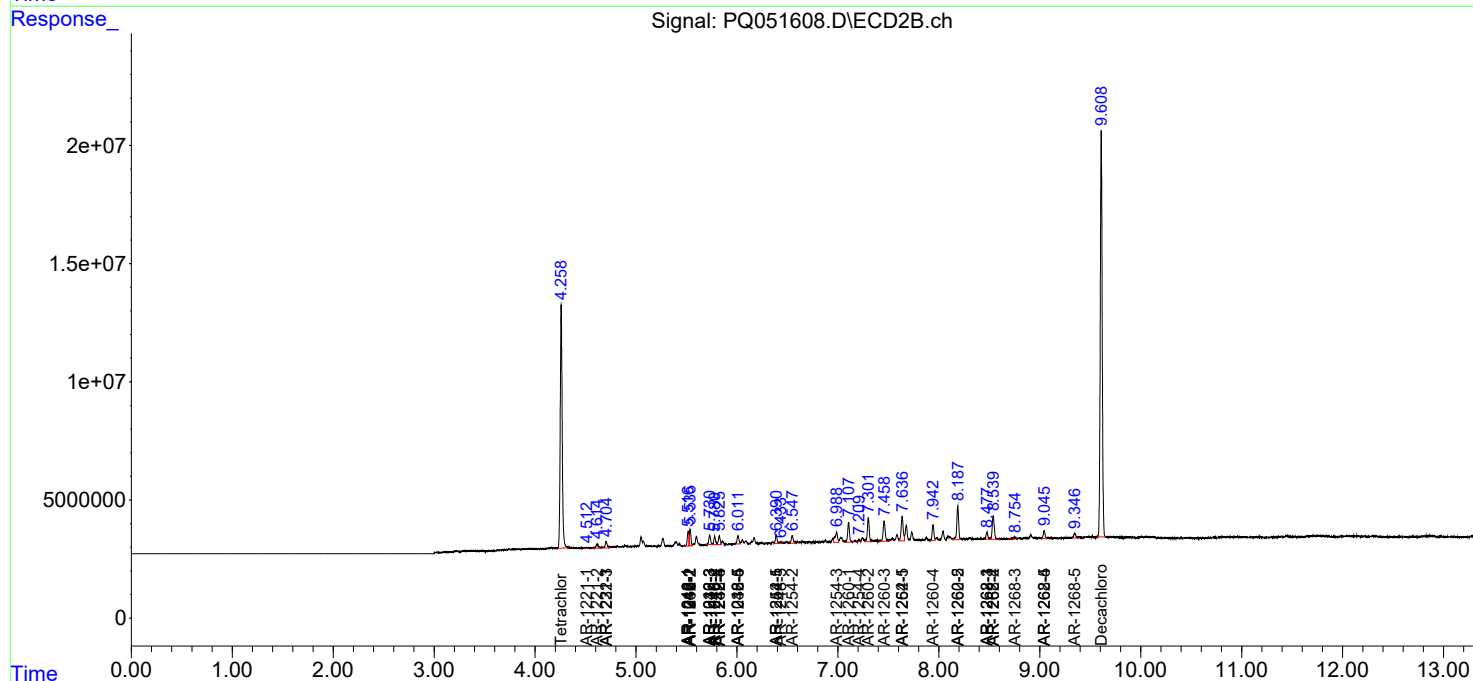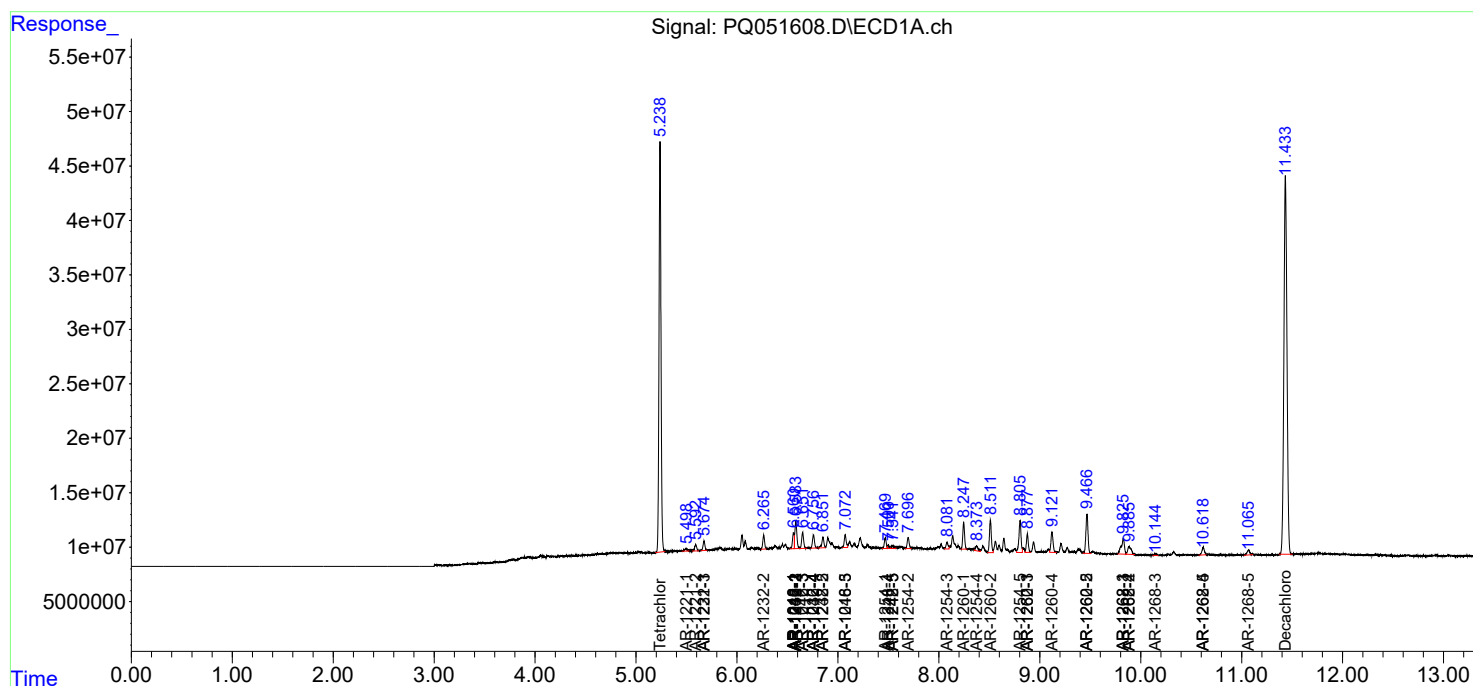


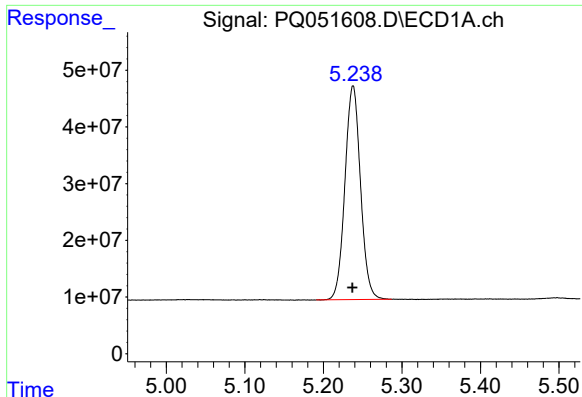

#1 Tetrachloro-m-xylene


R.T.: 5.238 min
Delta R.T.: 0.000 min
Response: 518837231
Conc: 20.12 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-QT1-2021-01

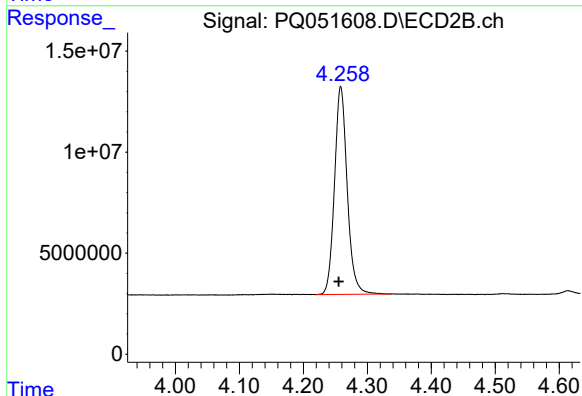


#1 Tetrachloro-m-xylene

R.T.: 4.258 min
Delta R.T.: 0.003 min
Response: 141812519
Conc: 19.42 ng/ml

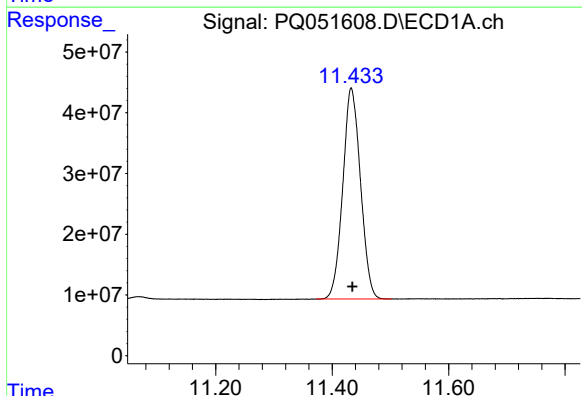


#2 Decachlorobiphenyl

R.T.: 11.433 min
Delta R.T.: -0.002 min
Response: 732385600
Conc: 39.95 ng/ml

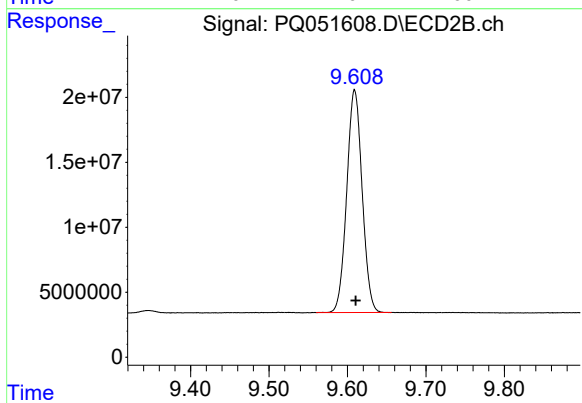

#2 Decachlorobiphenyl


R.T.: 9.609 min
Delta R.T.: -0.001 min
Response: 233896808
Conc: 38.46 ng/ml

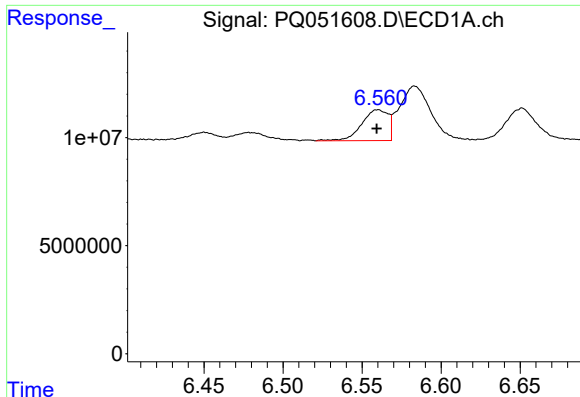

#3 AR-1016-1


R.T.: 6.560 min
Delta R.T.: 0.001 min
Response: 16539446
Conc: 19.58 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-QT1-2021-01

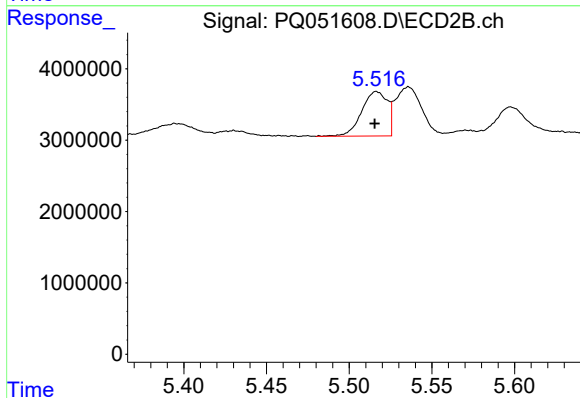


#3 AR-1016-1

R.T.: 5.516 min
Delta R.T.: 0.000 min
Response: 6728764
Conc: 26.25 ng/ml

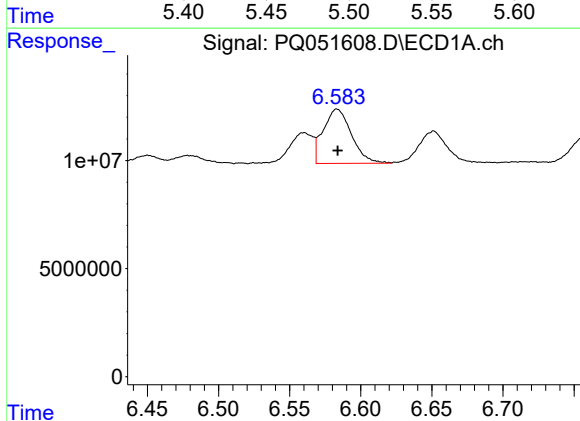


#4 AR-1016-2

R.T.: 6.583 min
Delta R.T.: 0.000 min
Response: 34638078
Conc: 27.96 ng/ml

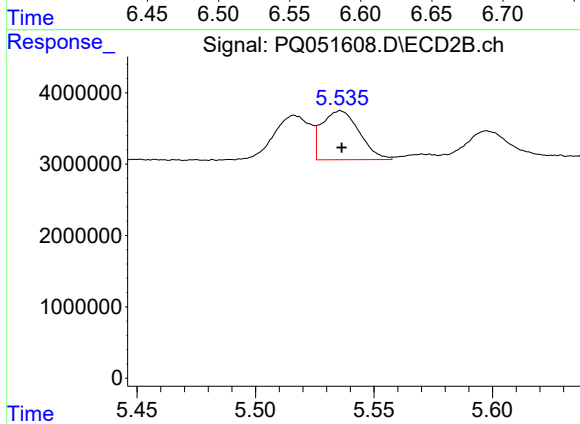

#4 AR-1016-2


R.T.: 5.536 min
Delta R.T.: 0.000 min
Response: 7547880
Conc: 21.08 ng/ml

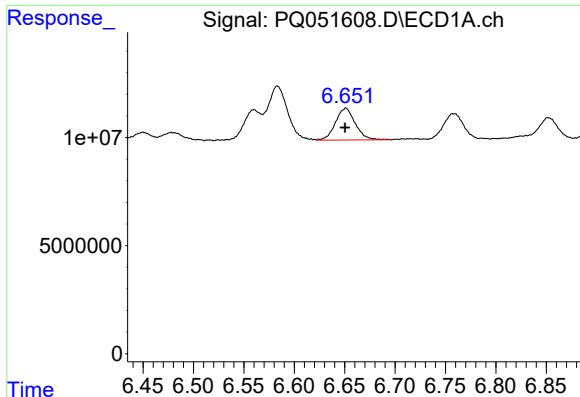

#5 AR-1016-3


R.T.: 6.651 min
Delta R.T.: 0.000 min
Response: 20231434
Conc: 27.65 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-QT1-2021-01

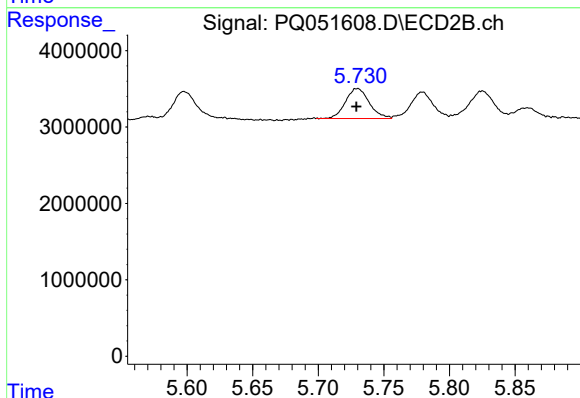


#5 AR-1016-3

R.T.: 5.730 min
Delta R.T.: 0.001 min
Response: 4946577
Conc: 26.87 ng/ml

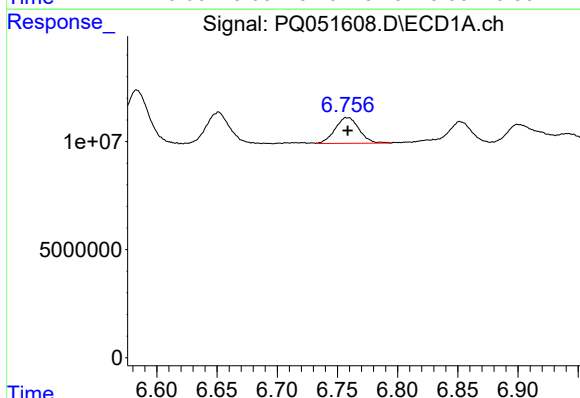


#6 AR-1016-4

R.T.: 6.757 min
Delta R.T.: -0.002 min
Response: 16570636
Conc: 26.96 ng/ml

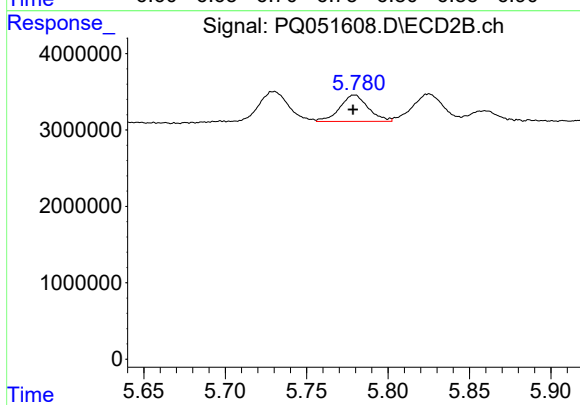

#6 AR-1016-4


R.T.: 5.780 min
Delta R.T.: 0.001 min
Response: 4190436
Conc: 29.04 ng/ml

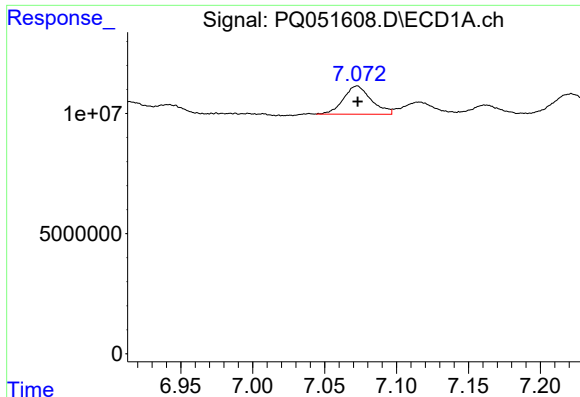

#7 AR-1016-5


R.T.: 7.073 min
Delta R.T.: 0.000 min
Response: 15981652
Conc: 26.86 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-QT1-2021-01

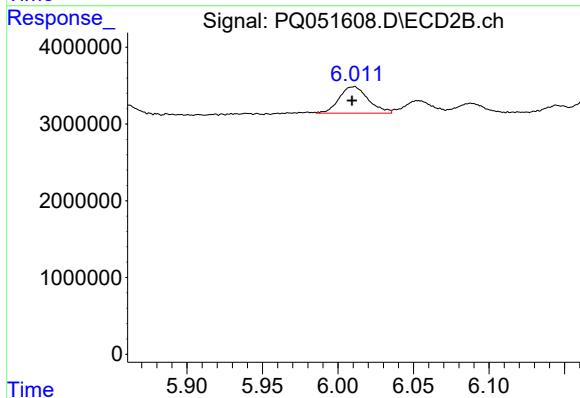


#7 AR-1016-5

R.T.: 6.011 min
Delta R.T.: 0.002 min
Response: 4656765
Conc: 24.47 ng/ml

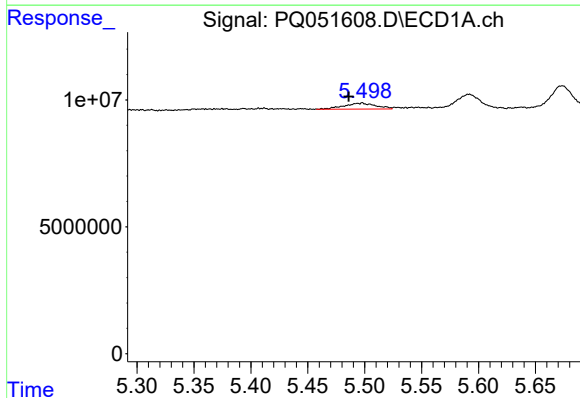


#8 AR-1221-1

R.T.: 5.498 min
Delta R.T.: 0.012 min
Response: 4657169
Conc: 17.55 ng/ml

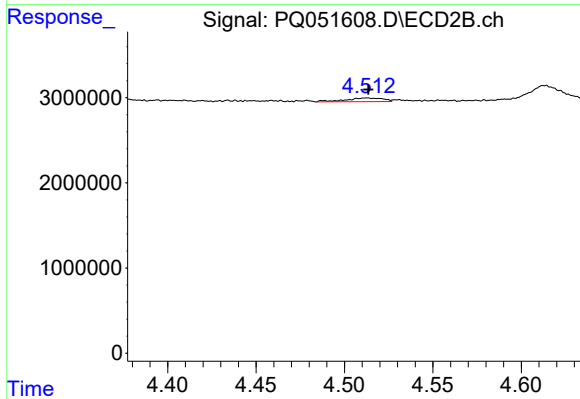

#8 AR-1221-1


R.T.: 4.513 min
Delta R.T.: 0.000 min
Response: 645893
Conc: 8.38 ng/ml

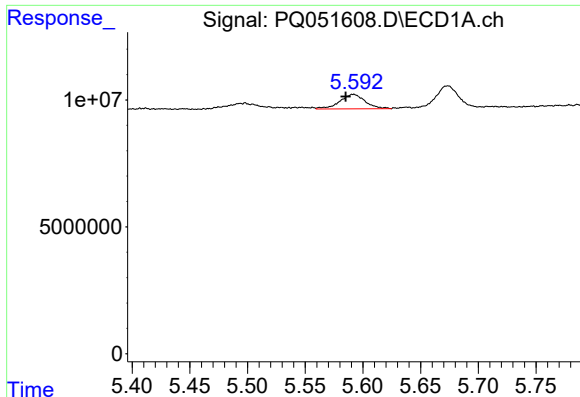

#9 AR-1221-2


R.T.: 5.592 min
Delta R.T.: 0.007 min
Response: 8701993
Conc: 47.64 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-QT1-2021-01

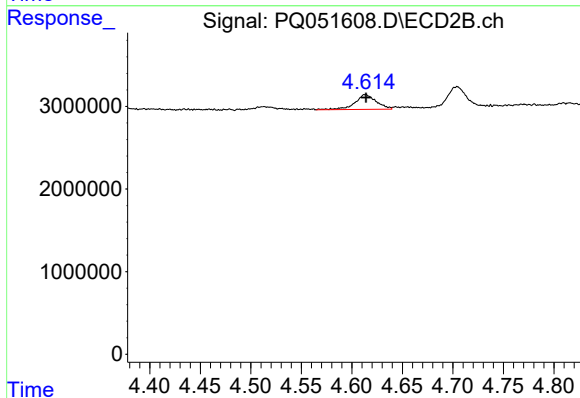


#9 AR-1221-2

R.T.: 4.614 min
Delta R.T.: 0.000 min
Response: 2654298
Conc: 49.63 ng/ml

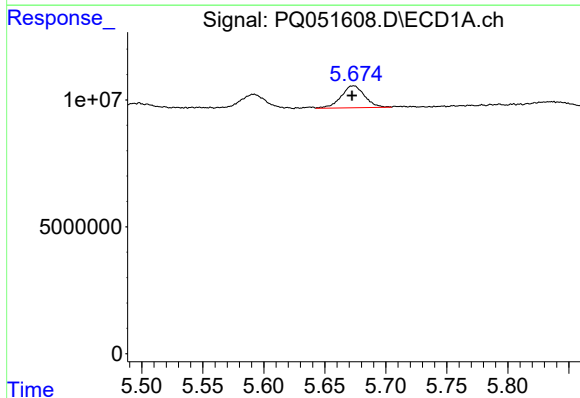


#10 AR-1221-3

R.T.: 5.674 min
Delta R.T.: 0.002 min
Response: 11625666
Conc: 18.84 ng/ml

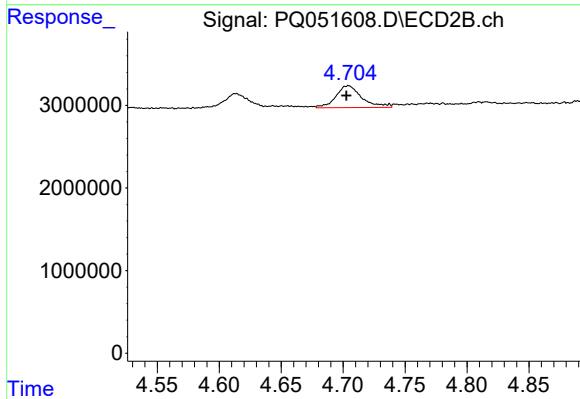

#10 AR-1221-3


R.T.: 4.704 min
Delta R.T.: 0.002 min
Response: 3868372
Conc: 21.12 ng/ml

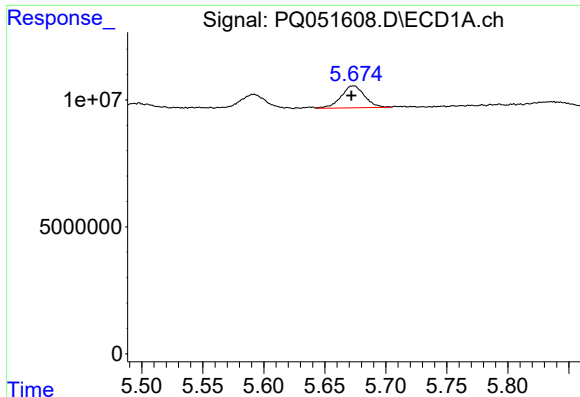

#11 AR-1232-1


R.T.: 5.674 min
Delta R.T.: 0.002 min
Response: 11625666
Conc: 25.26 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-QT1-2021-01

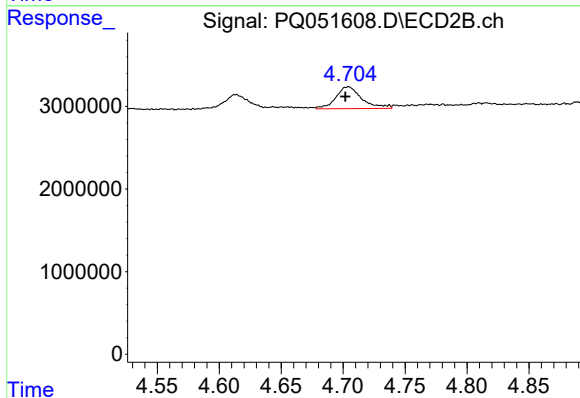


#11 AR-1232-1

R.T.: 4.704 min
Delta R.T.: 0.003 min
Response: 3868372
Conc: 28.30 ng/ml

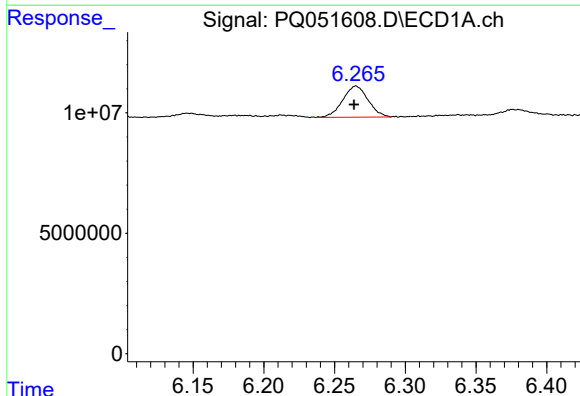


#12 AR-1232-2

R.T.: 6.265 min
Delta R.T.: 0.001 min
Response: 16068152
Conc: 65.11 ng/ml

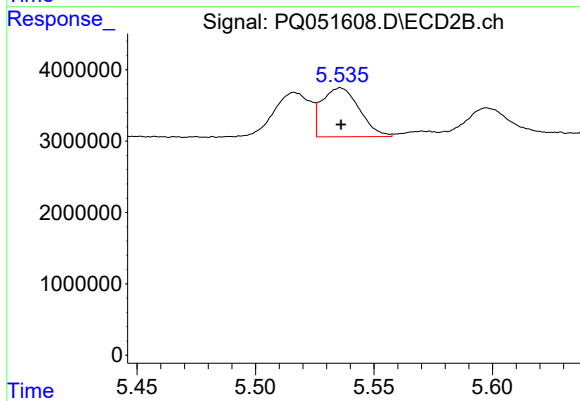

#12 AR-1232-2


R.T.: 5.536 min
Delta R.T.: 0.000 min
Response: 7547880
Conc: 53.67 ng/ml

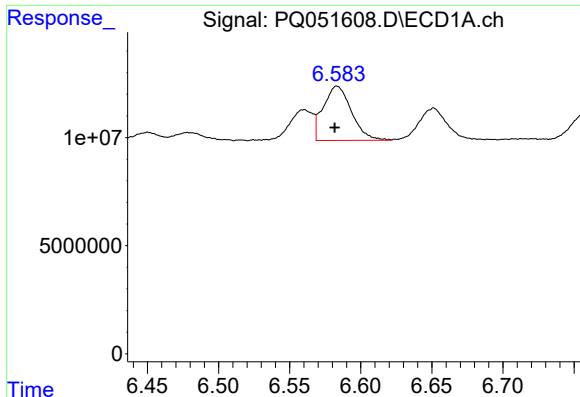

#13 AR-1232-3


R.T.: 6.583 min
Delta R.T.: 0.002 min
Response: 34638078
Conc: 68.45 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-QT1-2021-01

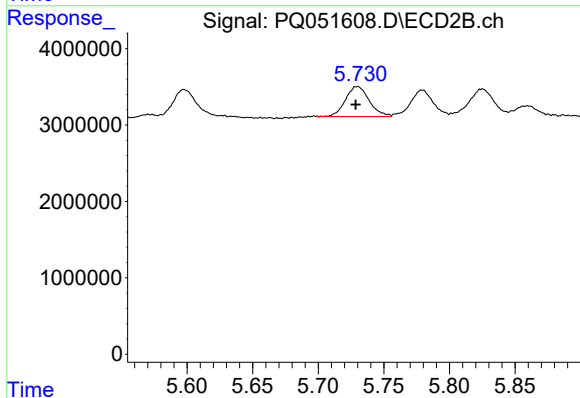


#13 AR-1232-3

R.T.: 5.730 min
Delta R.T.: 0.002 min
Response: 4946577
Conc: 69.12 ng/ml

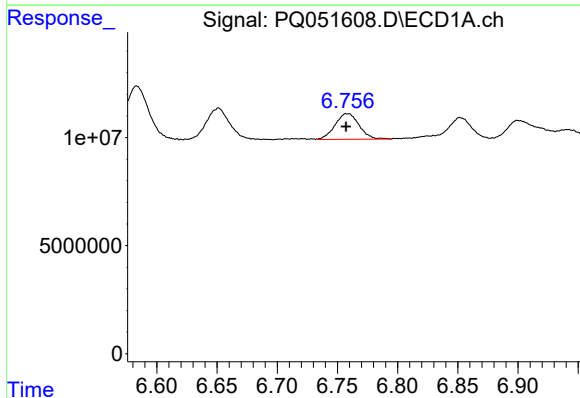


#14 AR-1232-4

R.T.: 6.757 min
Delta R.T.: 0.000 min
Response: 16570636
Conc: 66.35 ng/ml

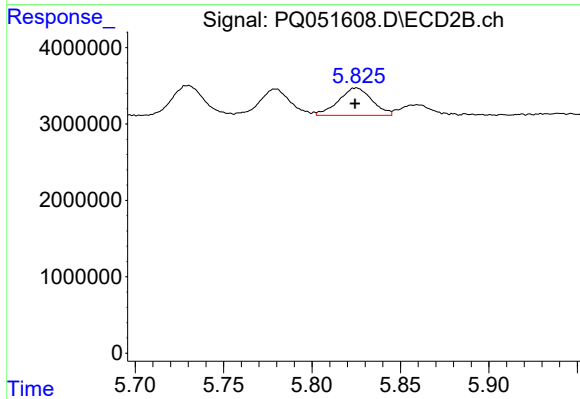

#14 AR-1232-4


R.T.: 5.825 min
Delta R.T.: 0.000 min
Response: 4739483
Conc: 77.09 ng/ml

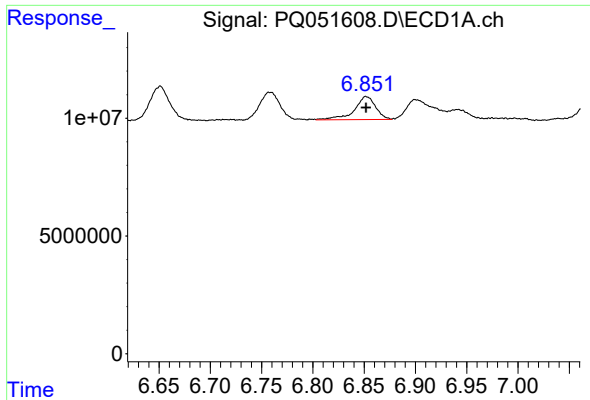

#15 AR-1232-5


R.T.: 6.852 min
Delta R.T.: 0.000 min
Response: 14106236
Conc: 79.51 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-QT1-2021-01

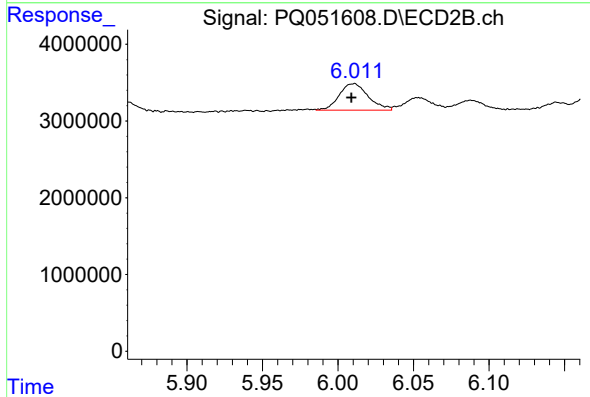


#15 AR-1232-5

R.T.: 6.011 min
Delta R.T.: 0.002 min
Response: 4656765
Conc: 72.59 ng/ml

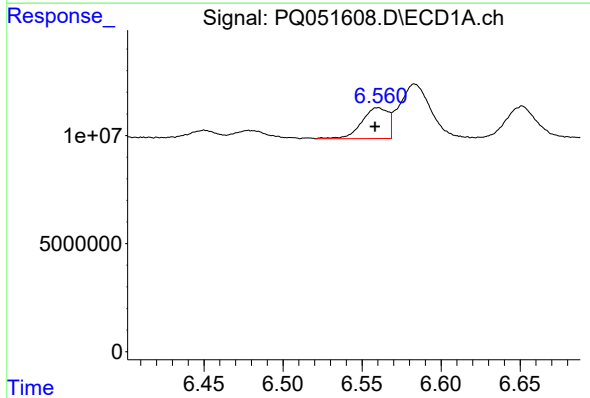


#16 AR-1242-1

R.T.: 6.560 min
Delta R.T.: 0.002 min
Response: 16539446
Conc: 23.54 ng/ml

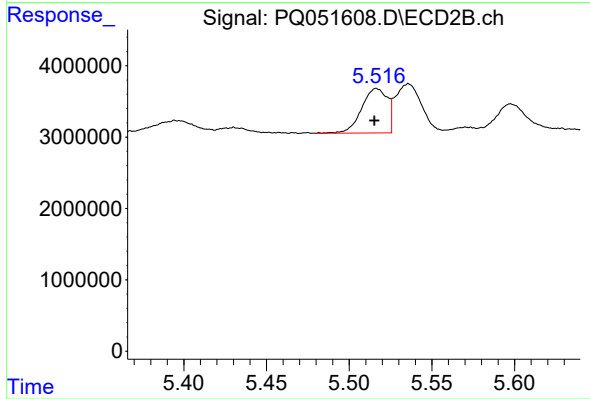

#16 AR-1242-1


R.T.: 5.516 min
Delta R.T.: 0.001 min
Response: 6728764
Conc: 32.00 ng/ml

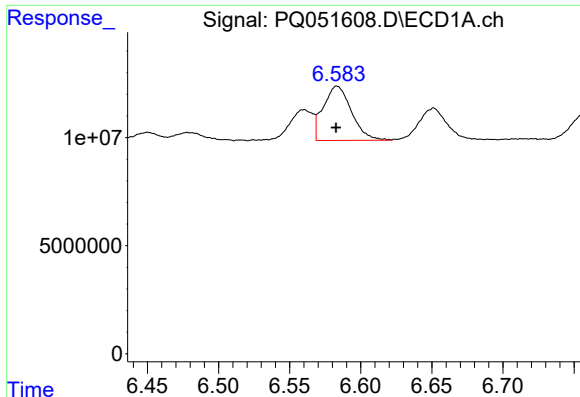

#17 AR-1242-2


R.T.: 6.583 min
Delta R.T.: 0.000 min
Response: 34638078
Conc: 33.61 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-QT1-2021-01

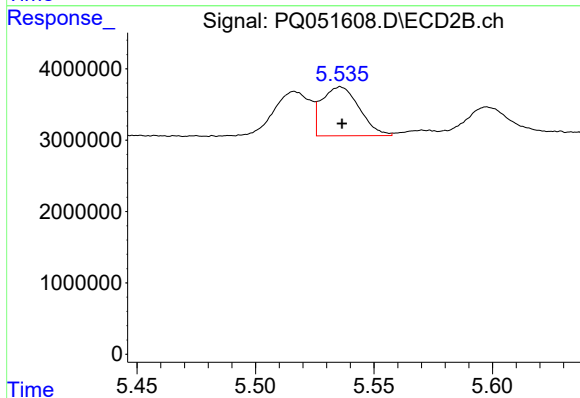


#17 AR-1242-2

R.T.: 5.536 min
Delta R.T.: 0.000 min
Response: 7547880
Conc: 25.87 ng/ml

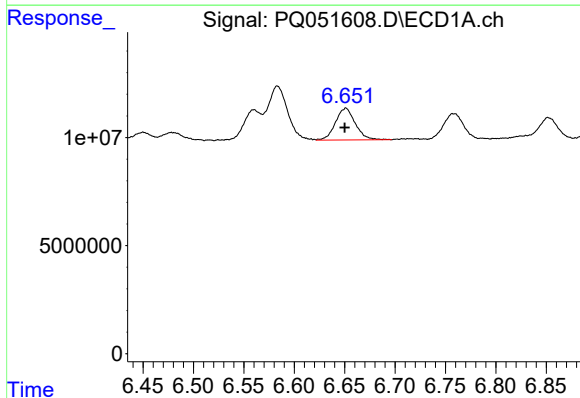


#18 AR-1242-3

R.T.: 6.651 min
Delta R.T.: 0.001 min
Response: 20231434
Conc: 32.90 ng/ml

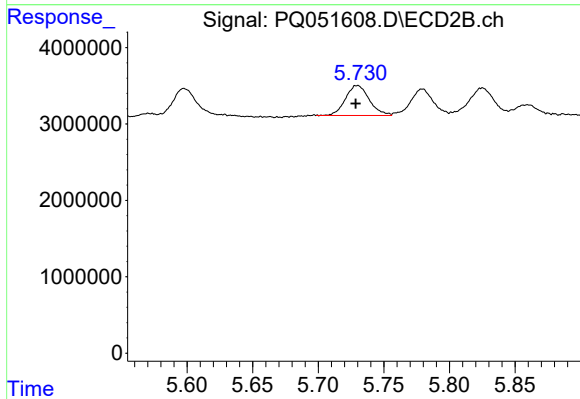

#18 AR-1242-3


R.T.: 5.730 min
Delta R.T.: 0.002 min
Response: 4946577
Conc: 32.78 ng/ml

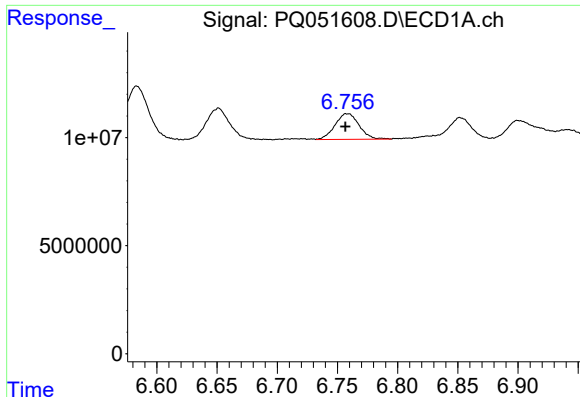

#19 AR-1242-4


R.T.: 6.757 min
Delta R.T.: 0.000 min
Response: 16570636
Conc: 32.24 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-QT1-2021-01

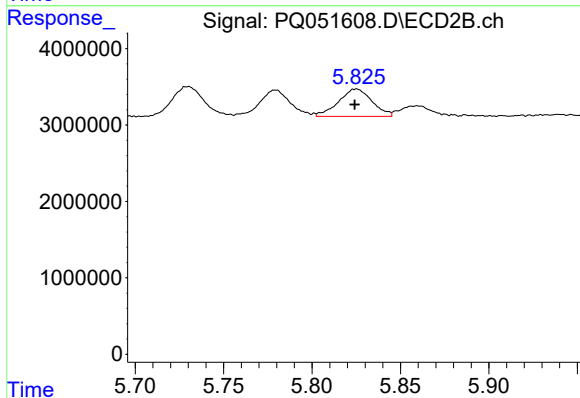


#19 AR-1242-4

R.T.: 5.825 min
Delta R.T.: 0.001 min
Response: 4739483
Conc: 32.74 ng/ml

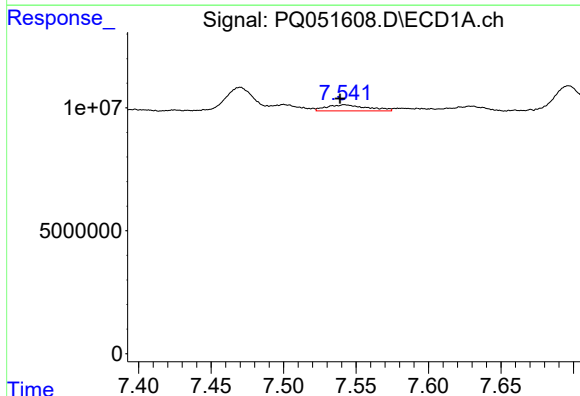


#20 AR-1242-5

R.T.: 7.542 min
Delta R.T.: 0.003 min
Response: 4836377
Conc: 8.77 ng/ml

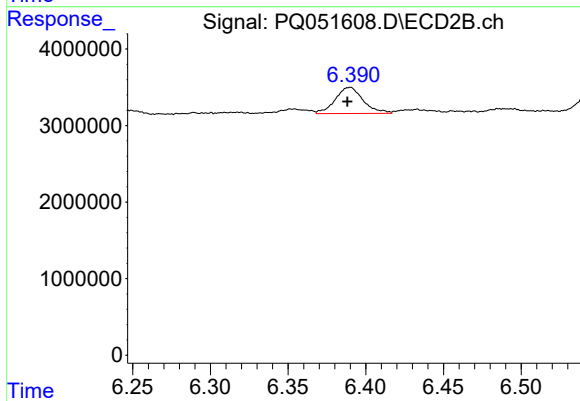

#20 AR-1242-5


R.T.: 6.390 min
Delta R.T.: 0.001 min
Response: 4299875
Conc: 22.50 ng/ml

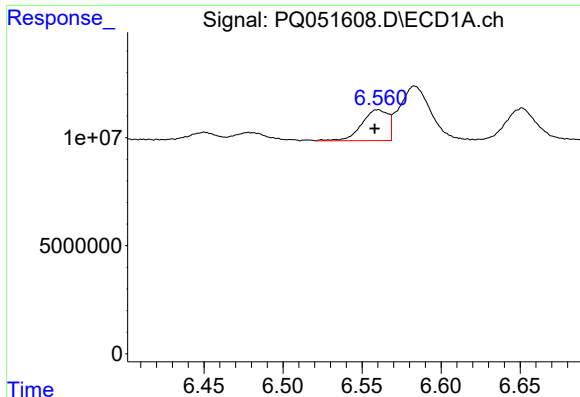

#21 AR-1248-1


R.T.: 6.560 min
Delta R.T.: 0.002 min
Response: 16539446
Conc: 29.24 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-QT1-2021-01

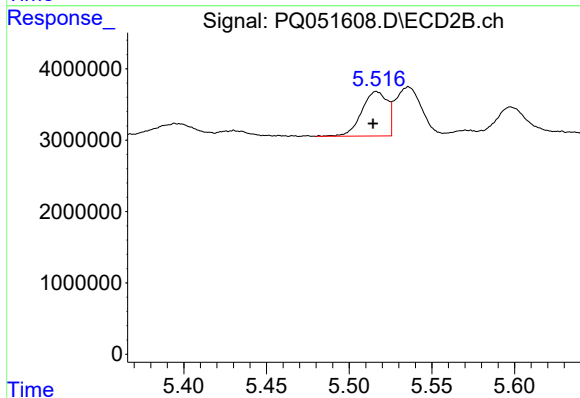


#21 AR-1248-1

R.T.: 5.516 min
Delta R.T.: 0.002 min
Response: 6728764
Conc: 40.04 ng/ml

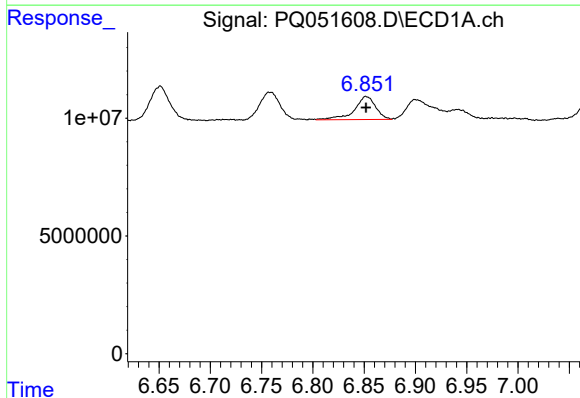


#22 AR-1248-2

R.T.: 6.852 min
Delta R.T.: 0.000 min
Response: 14106236
Conc: 17.53 ng/ml

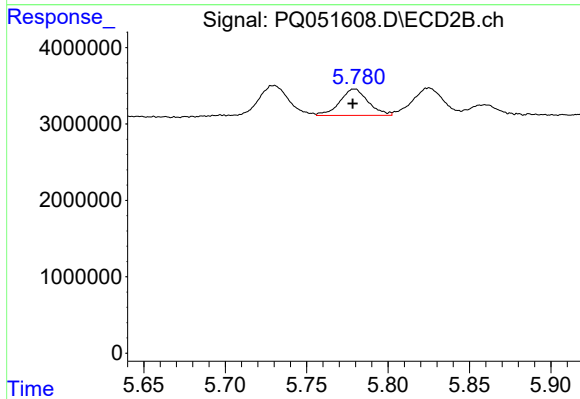

#22 AR-1248-2


R.T.: 5.780 min
Delta R.T.: 0.001 min
Response: 4190436
Conc: 18.50 ng/ml

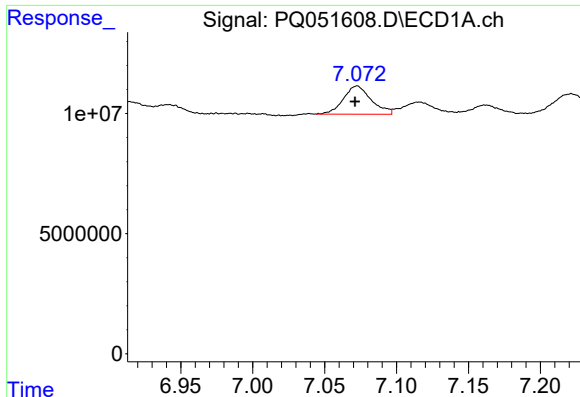

#23 AR-1248-3


R.T.: 7.073 min
Delta R.T.: 0.002 min
Response: 15981652
Conc: 17.24 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-QT1-2021-01

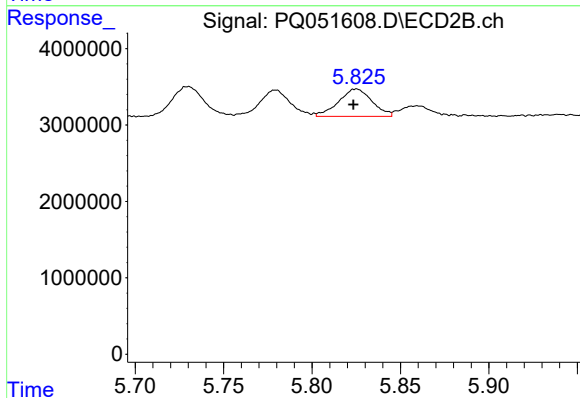


#23 AR-1248-3

R.T.: 5.825 min
Delta R.T.: 0.002 min
Response: 4739483
Conc: 20.15 ng/ml

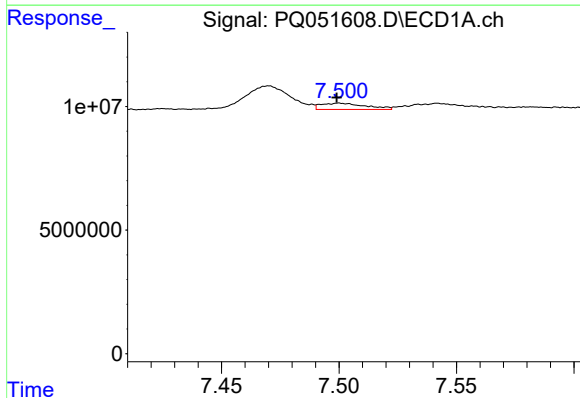


#24 AR-1248-4

R.T.: 7.500 min
Delta R.T.: 0.001 min
Response: 3358027
Conc: 3.16 ng/ml

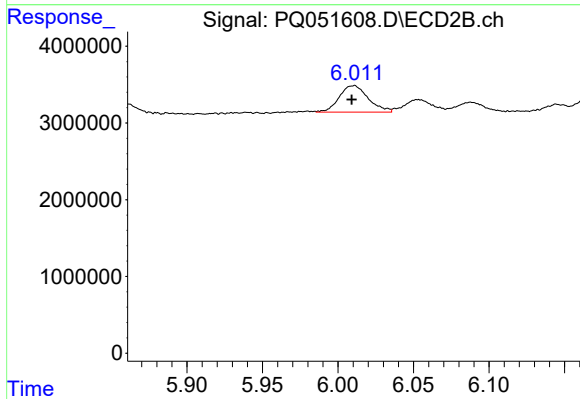

#24 AR-1248-4


R.T.: 6.011 min
Delta R.T.: 0.002 min
Response: 4656765
Conc: 16.94 ng/ml

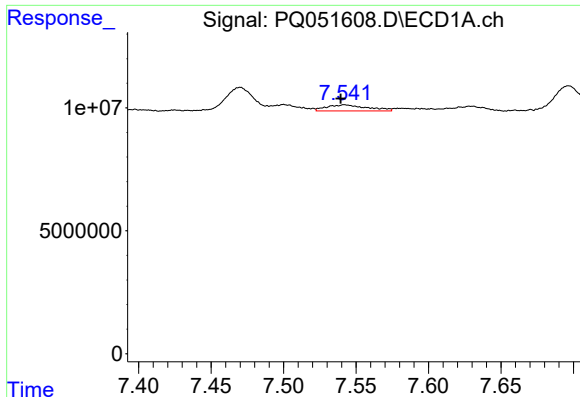

#25 AR-1248-5


R.T.: 7.542 min
Delta R.T.: 0.002 min
Response: 4836377
Conc: 4.66 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-QT1-2021-01

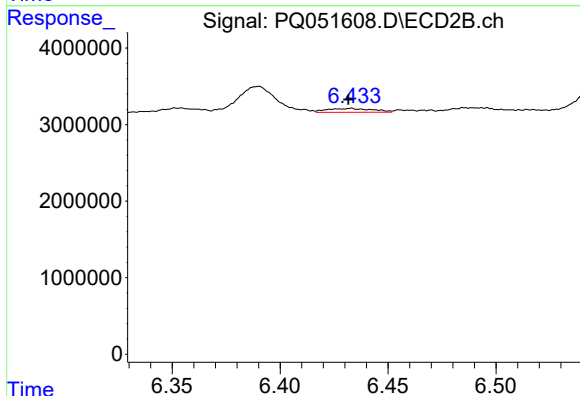


#25 AR-1248-5

R.T.: 6.433 min
Delta R.T.: 0.001 min
Response: 740158
Conc: 2.57 ng/ml

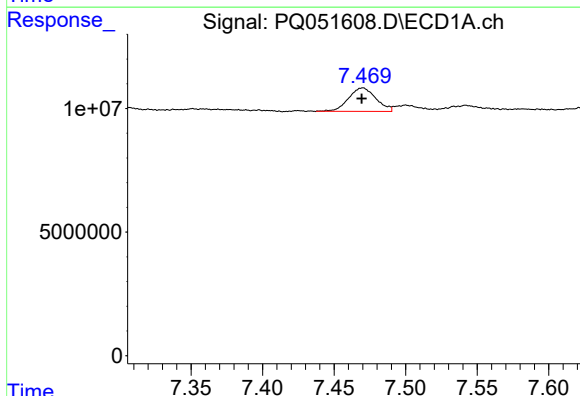


#26 AR-1254-1

R.T.: 7.470 min
Delta R.T.: 0.000 min
Response: 12681547
Conc: 12.89 ng/ml

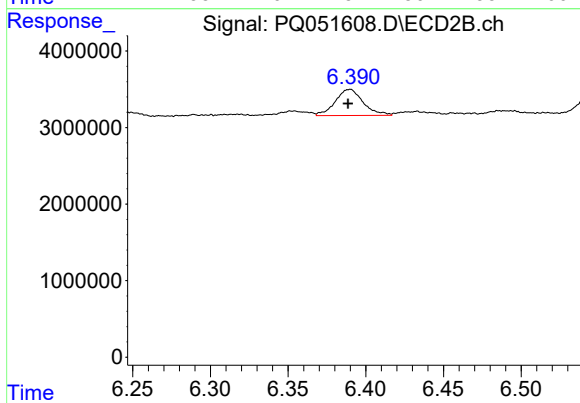

#26 AR-1254-1


R.T.: 6.390 min
Delta R.T.: 0.001 min
Response: 4299875
Conc: 10.13 ng/ml

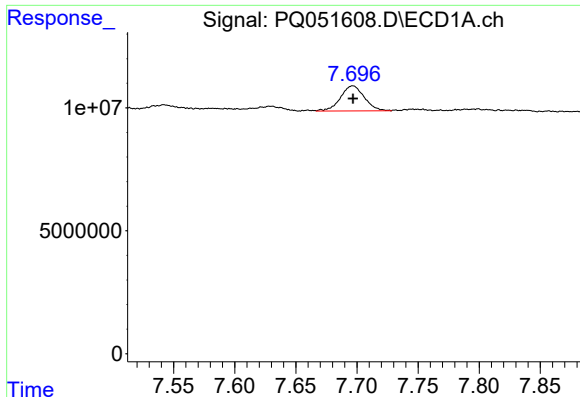

#27 AR-1254-2


R.T.: 7.697 min
Delta R.T.: 0.000 min
Response: 13841658
Conc: 9.09 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-QT1-2021-01

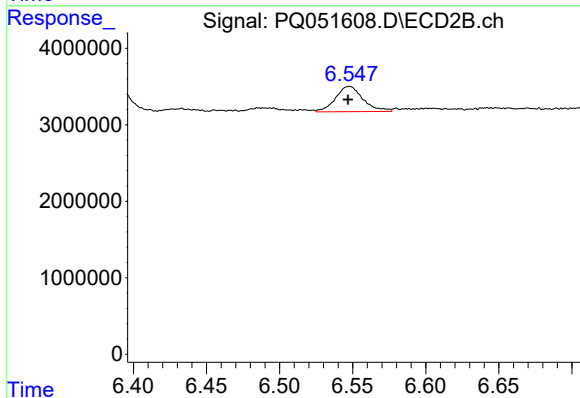


#27 AR-1254-2

R.T.: 6.548 min
Delta R.T.: 0.000 min
Response: 4330372
Conc: 11.80 ng/ml

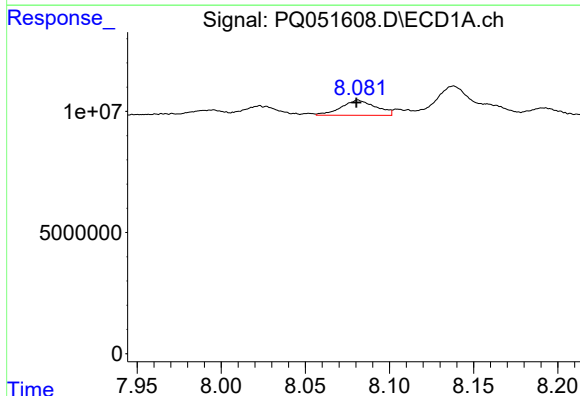


#28 AR-1254-3

R.T.: 8.081 min
Delta R.T.: 0.001 min
Response: 8922098
Conc: 5.40 ng/ml

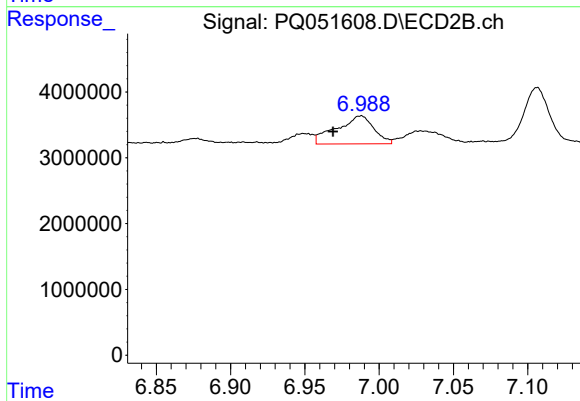

#28 AR-1254-3


R.T.: 6.988 min
Delta R.T.: 0.019 min
Response: 7450601
Conc: 12.21 ng/ml

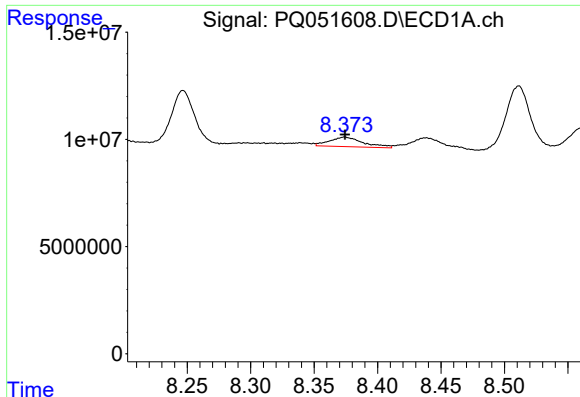

#29 AR-1254-4


R.T.: 8.374 min
Delta R.T.: 0.000 min
Response: 8224424
Conc: 6.92 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-QT1-2021-01

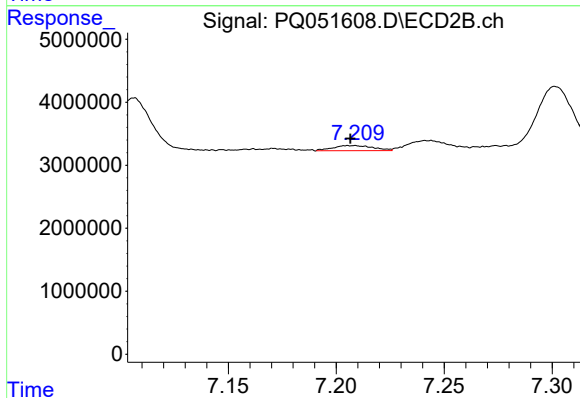


#29 AR-1254-4

R.T.: 7.208 min
Delta R.T.: 0.001 min
Response: 1047717
Conc: 2.77 ng/ml

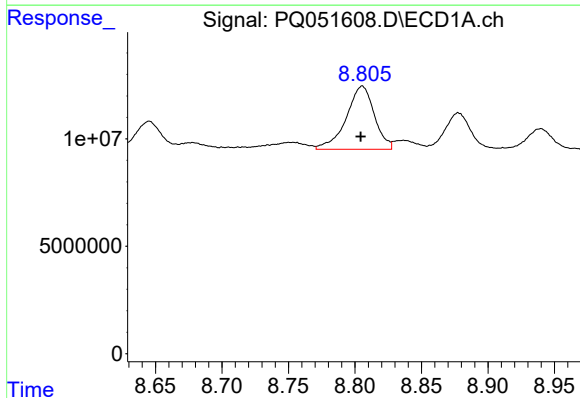


#30 AR-1254-5

R.T.: 8.806 min
Delta R.T.: 0.001 min
Response: 43354951
Conc: 34.35 ng/ml

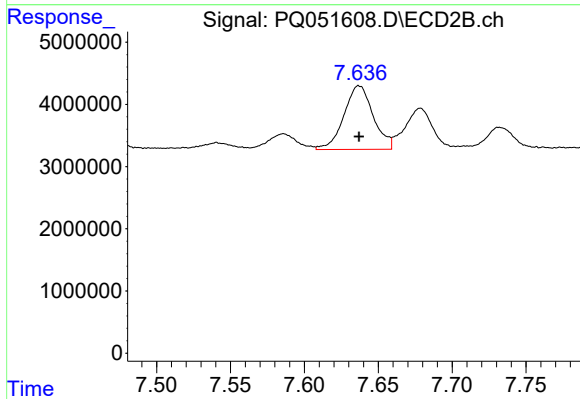

#30 AR-1254-5


R.T.: 7.637 min
Delta R.T.: 0.000 min
Response: 14148856
Conc: 26.94 ng/ml

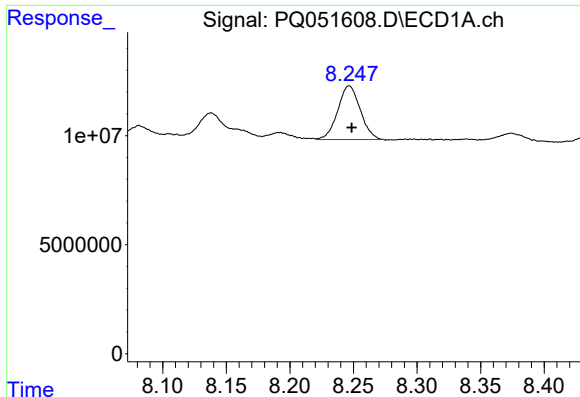

#31 AR-1260-1


R.T.: 8.247 min
Delta R.T.: -0.002 min
Response: 30372166
Conc: 29.32 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-QT1-2021-01

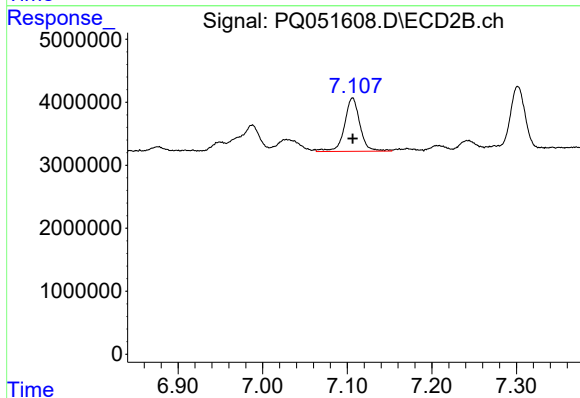


#31 AR-1260-1

R.T.: 7.106 min
Delta R.T.: 0.000 min
Response: 10723173
Conc: 30.23 ng/ml

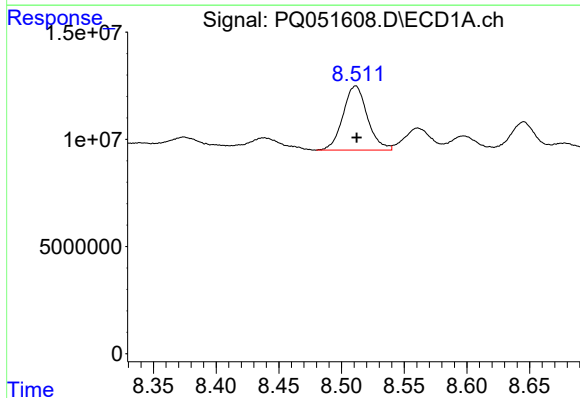


#32 AR-1260-2

R.T.: 8.511 min
Delta R.T.: 0.000 min
Response: 40627719
Conc: 32.85 ng/ml

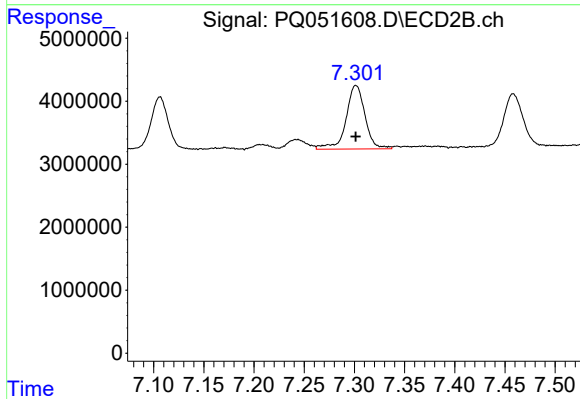

#32 AR-1260-2


R.T.: 7.302 min
Delta R.T.: 0.000 min
Response: 13314946
Conc: 30.10 ng/ml

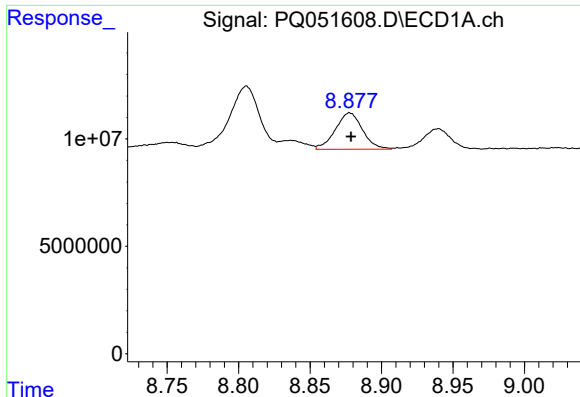

#33 AR-1260-3


R.T.: 8.878 min
Delta R.T.: -0.001 min
Response: 22437210
Conc: 24.71 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-QT1-2021-01

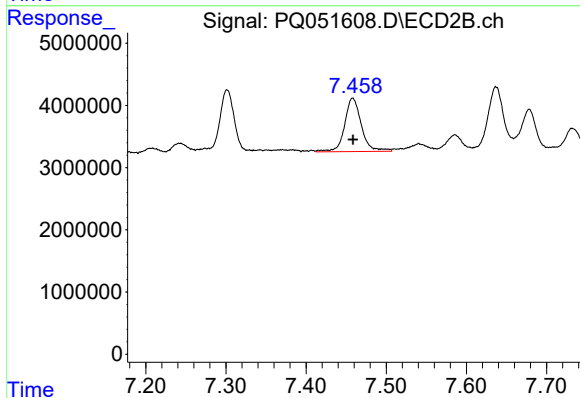


#33 AR-1260-3

R.T.: 7.458 min
Delta R.T.: 0.000 min
Response: 12490655
Conc: 30.14 ng/ml

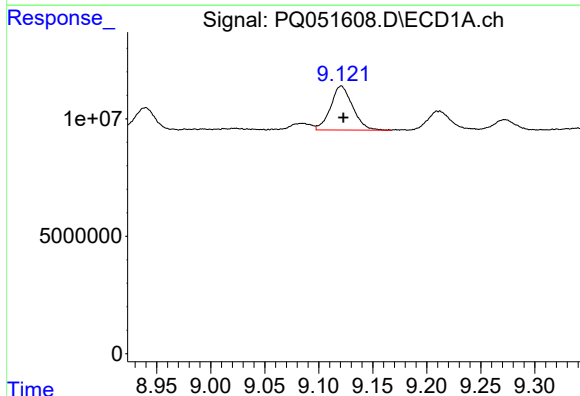


#34 AR-1260-4

R.T.: 9.121 min
Delta R.T.: -0.002 min
Response: 26648596
Conc: 25.00 ng/ml

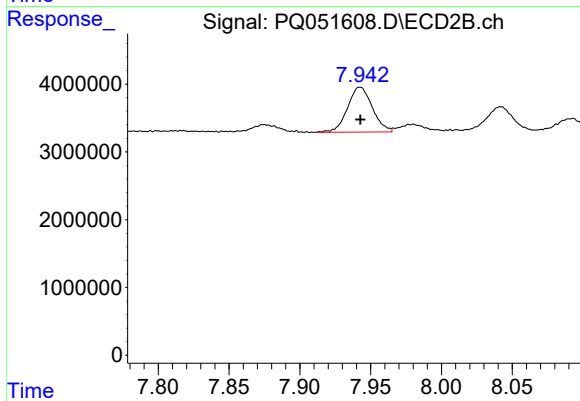

#34 AR-1260-4


R.T.: 7.943 min
Delta R.T.: 0.000 min
Response: 8081167
Conc: 23.30 ng/ml

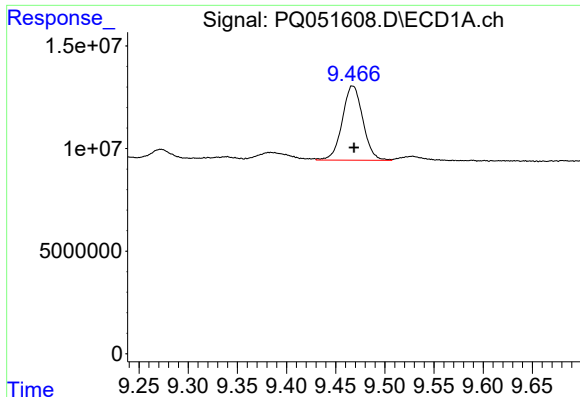

#35 AR-1260-5


R.T.: 9.467 min
Delta R.T.: -0.002 min
Response: 52677722
Conc: 23.66 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-QT1-2021-01

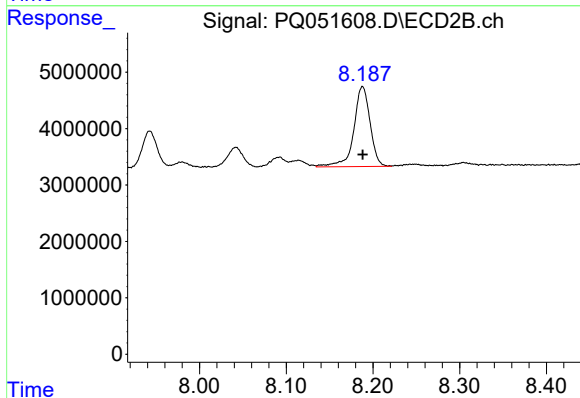


#35 AR-1260-5

R.T.: 8.188 min
Delta R.T.: 0.000 min
Response: 18478401
Conc: 21.40 ng/ml

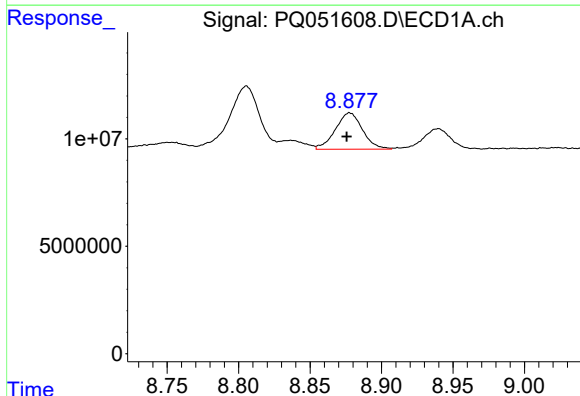


#36 AR-1262-1

R.T.: 8.878 min
Delta R.T.: 0.002 min
Response: 22437210
Conc: 14.79 ng/ml

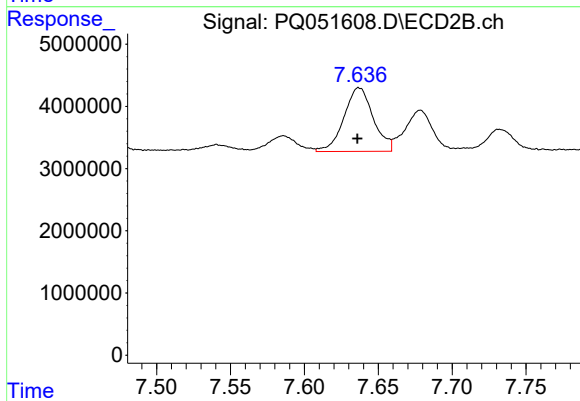

#36 AR-1262-1


R.T.: 7.637 min
Delta R.T.: 0.001 min
Response: 14148856
Conc: 49.35 ng/ml

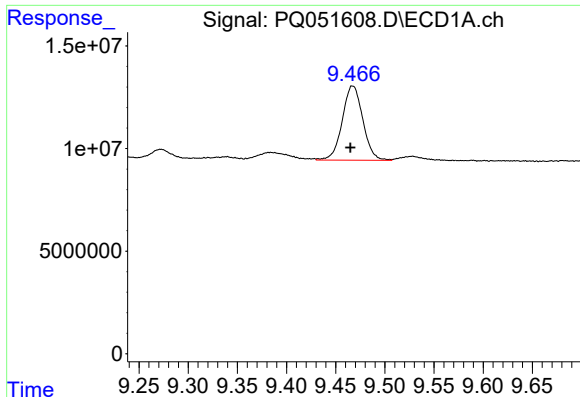

#37 AR-1262-2


R.T.: 9.467 min
Delta R.T.: 0.002 min
Response: 52677722
Conc: 18.78 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-QT1-2021-01

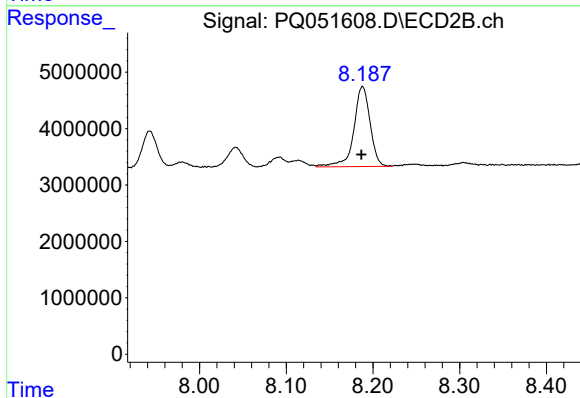


#37 AR-1262-2

R.T.: 8.188 min
Delta R.T.: 0.002 min
Response: 18478401
Conc: 18.12 ng/ml

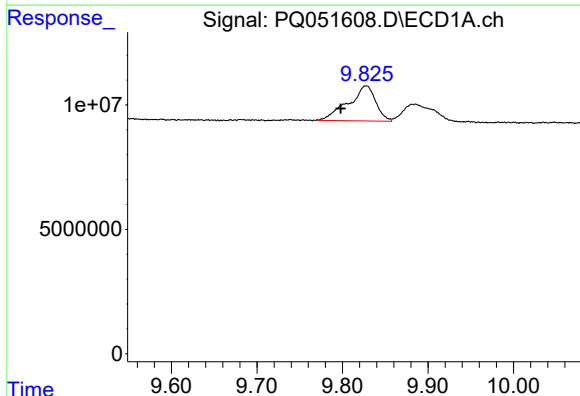


#38 AR-1262-3

R.T.: 9.829 min
Delta R.T.: 0.031 min
Response: 31444416
Conc: 26.20 ng/ml

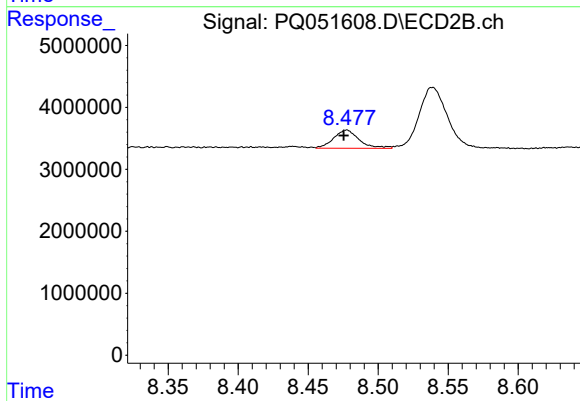

#38 AR-1262-3


R.T.: 8.477 min
Delta R.T.: 0.002 min
Response: 3748056
Conc: 9.96 ng/ml

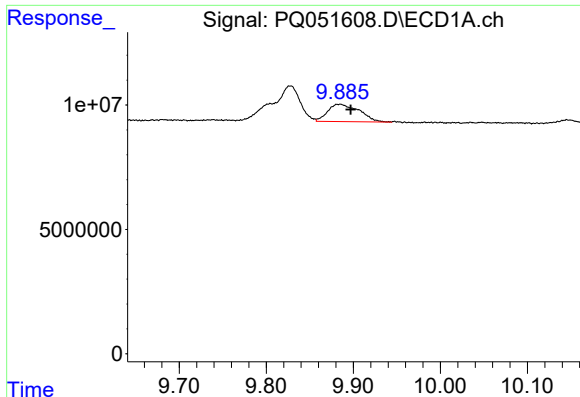

#39 AR-1262-4


R.T.: 9.881 min
Delta R.T.: -0.016 min
Response: 17502067
Conc: 24.84 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-QT1-2021-01

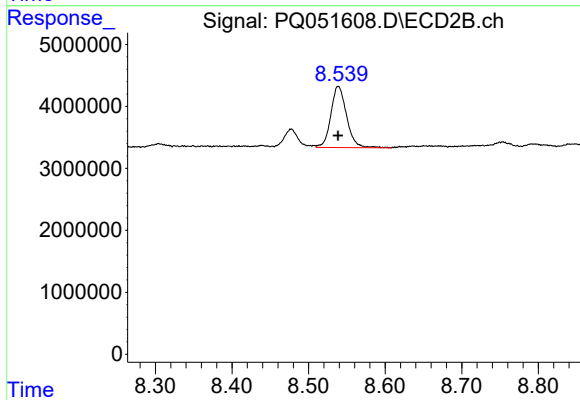


#39 AR-1262-4

R.T.: 8.539 min
Delta R.T.: 0.000 min
Response: 14133060
Conc: 19.27 ng/ml

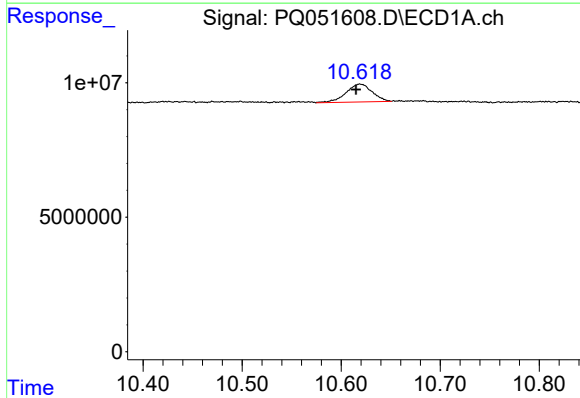


#40 AR-1262-5

R.T.: 10.619 min
Delta R.T.: 0.004 min
Response: 12156650
Conc: 12.77 ng/ml

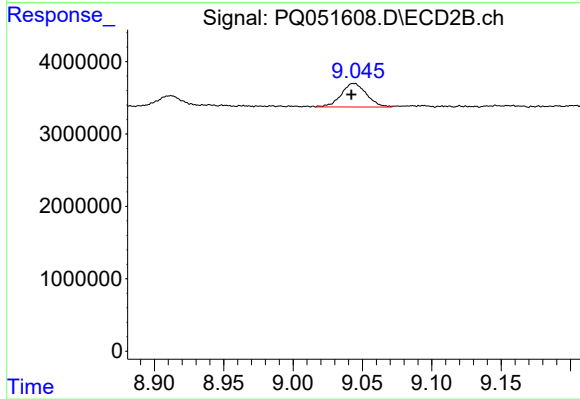

#40 AR-1262-5


R.T.: 9.044 min
Delta R.T.: 0.002 min
Response: 4168647
Conc: 12.66 ng/ml

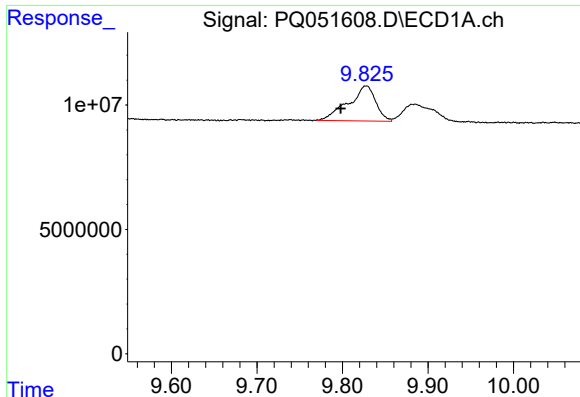

#41 AR-1268-1


R.T.: 9.829 min
Delta R.T.: 0.031 min
Response: 31444416
Conc: 9.53 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-QT1-2021-01

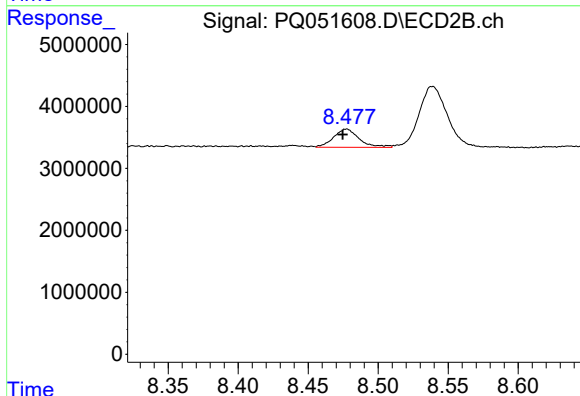


#41 AR-1268-1

R.T.: 8.477 min
Delta R.T.: 0.003 min
Response: 3748056
Conc: 3.23 ng/ml

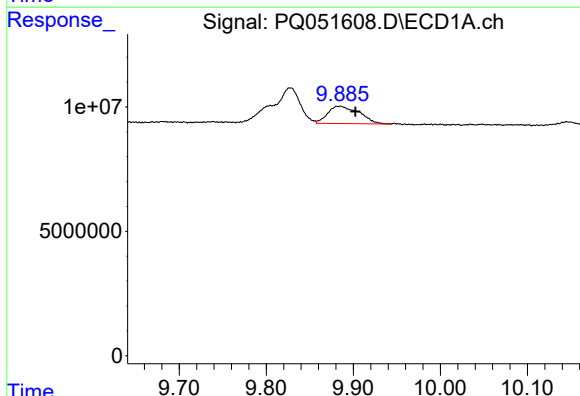


#42 AR-1268-2

R.T.: 9.881 min
Delta R.T.: -0.021 min
Response: 17502067
Conc: 5.83 ng/ml

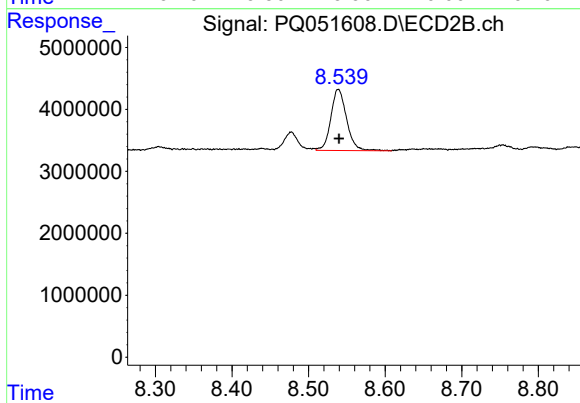

#42 AR-1268-2


R.T.: 8.539 min
Delta R.T.: -0.001 min
Response: 14133060
Conc: 13.28 ng/ml

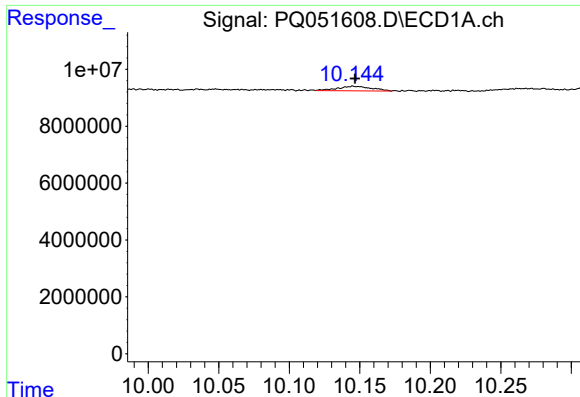

#43 AR-1268-3


R.T.: 10.145 min
Delta R.T.: -0.001 min
Response: 2632066
Conc: 1.03 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-QT1-2021-01

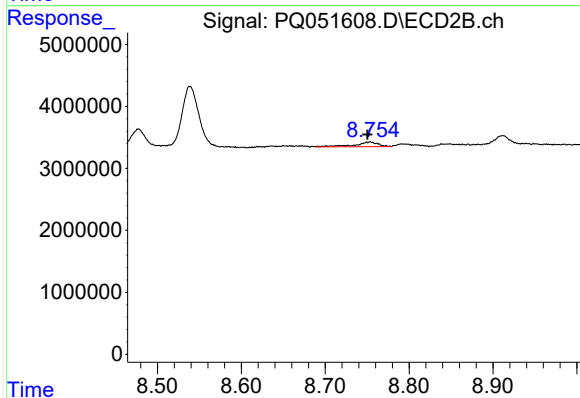


#43 AR-1268-3

R.T.: 8.754 min
Delta R.T.: 0.004 min
Response: 1507113
Conc: 1.69 ng/ml

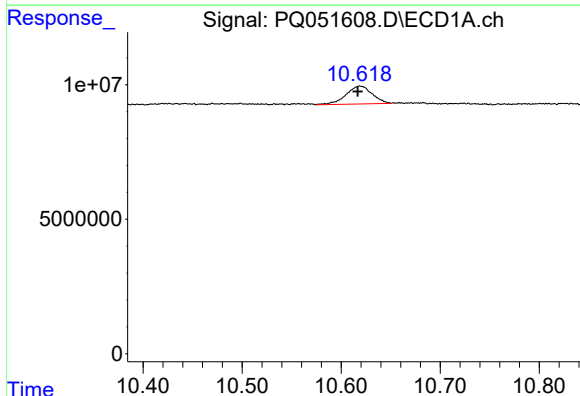


#44 AR-1268-4

R.T.: 10.619 min
Delta R.T.: 0.002 min
Response: 12156650
Conc: 11.19 ng/ml

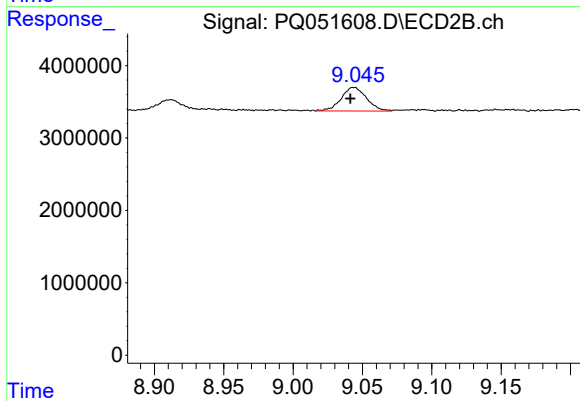

#44 AR-1268-4


R.T.: 9.044 min
Delta R.T.: 0.002 min
Response: 4168647
Conc: 11.30 ng/ml

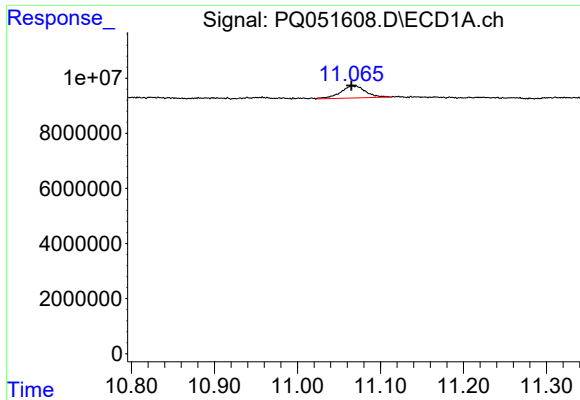

#45 AR-1268-5

R.T.: 11.065 min
Delta R.T.: 0.000 min
Response: 9149297
Conc: 1.09 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-QT1-2021-01

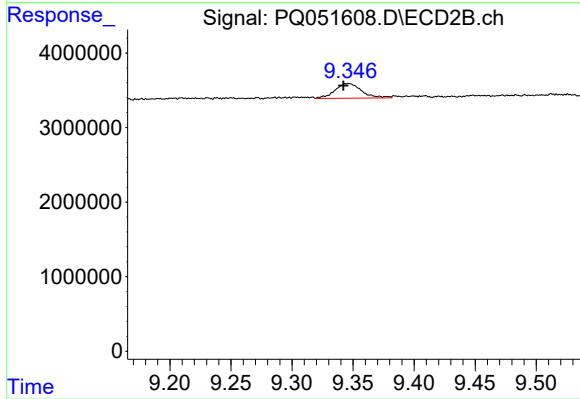

#45 AR-1268-5

R.T.: 9.346 min
Delta R.T.: 0.004 min
Response: 3013595
Conc: 1.08 ng/ml