

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ010522\
 Data File : PQ055570.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2022 11:52
 Operator : AJ\MA
 Sample : N1010-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 20211307-CAPE-1-SITE-WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 14:00:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ010422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 04 15:29:13 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.241	4.308	368.4E6	303.4E6	32.095	31.527
2) SA Decachlor...	11.425	9.684	292.2E6	133.8E6	19.591	18.009

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ010522\
Data File : PQ055570.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2022 11:52
Operator : AJ\MA
Sample : N1010-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
20211307-CAPE-1-SITE-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 14:00:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ010422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 04 15:29:13 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

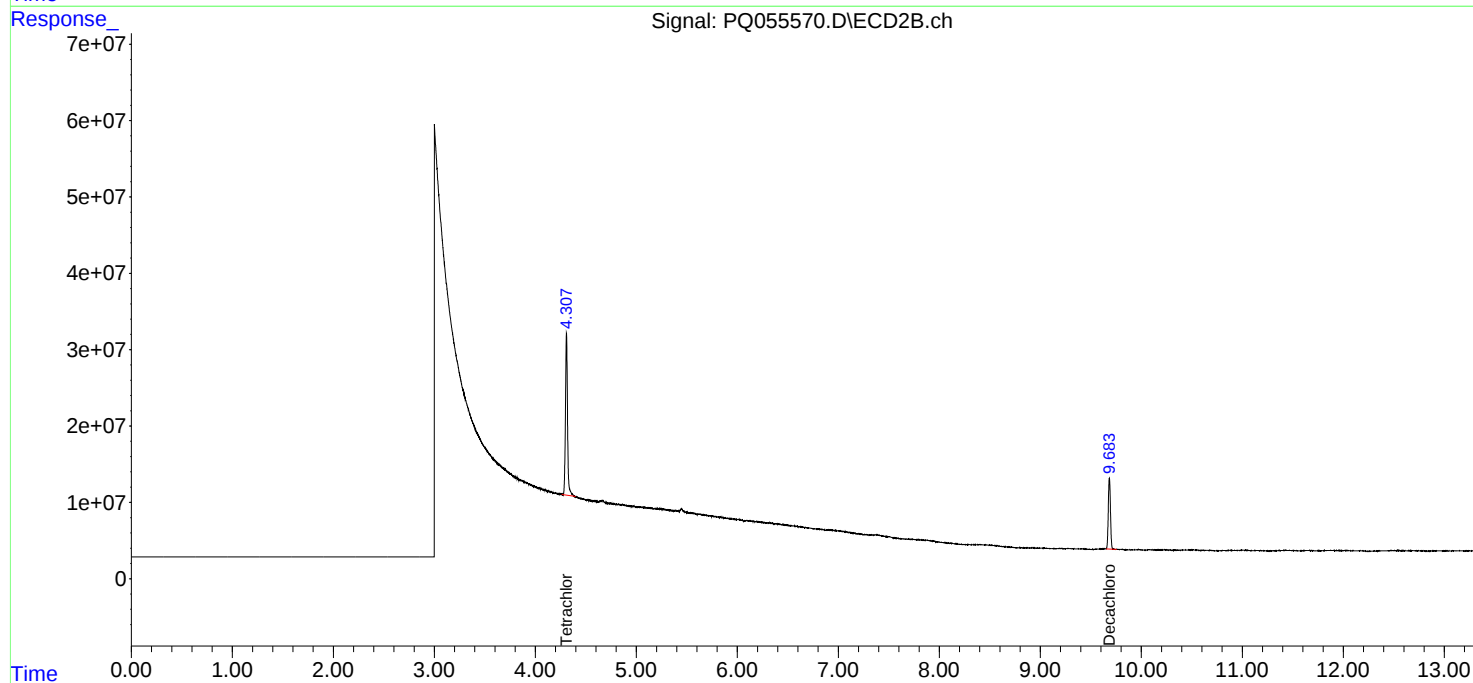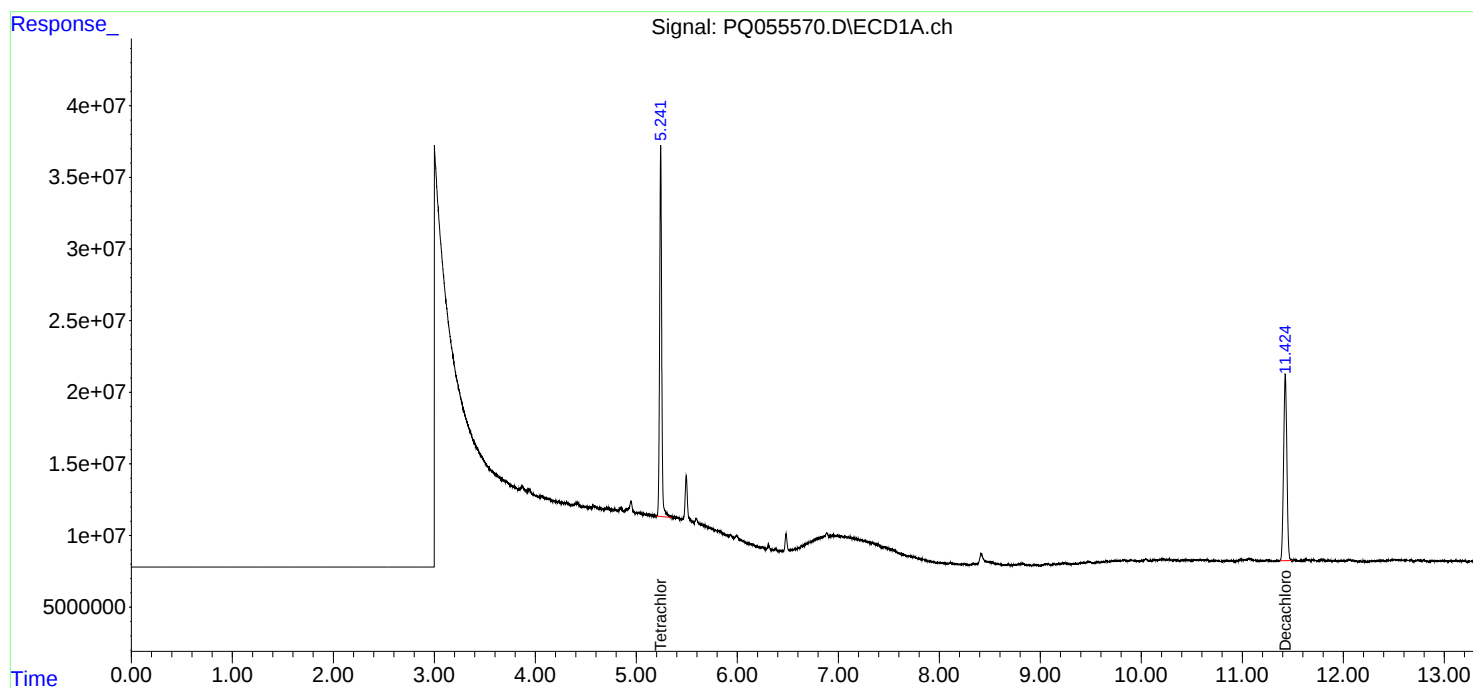


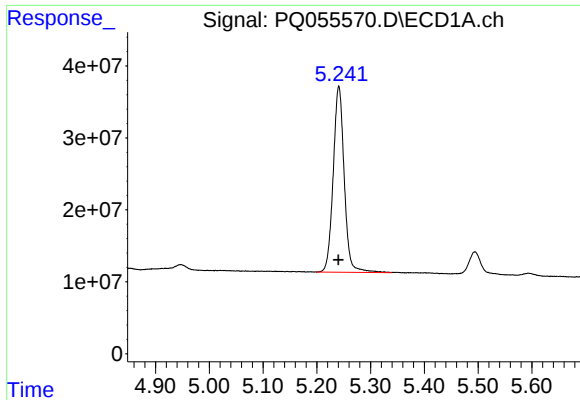

#1 Tetrachloro-m-xylene


R.T.: 5.241 min
Delta R.T.: 0.001 min
Response: 368417543
Conc: 32.09 ng/ml

Instrument :
ECD_Q
ClientSampleId :
20211307-CAPE-1-SITE-WATER

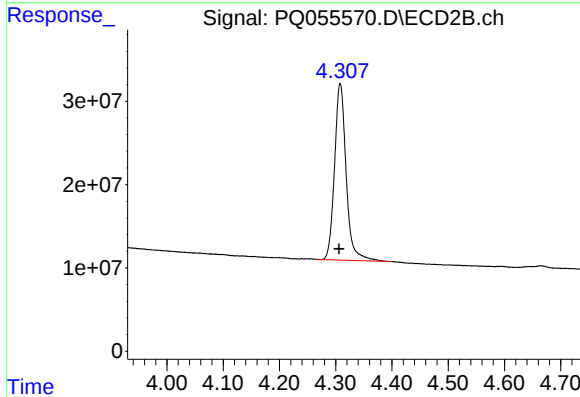


#1 Tetrachloro-m-xylene

R.T.: 4.308 min
Delta R.T.: 0.002 min
Response: 303445639
Conc: 31.53 ng/ml

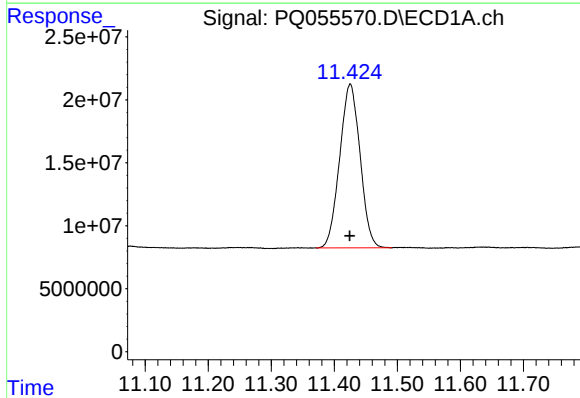

#2 Decachlorobiphenyl

R.T.: 11.425 min
Delta R.T.: 0.000 min
Response: 292168778
Conc: 19.59 ng/ml

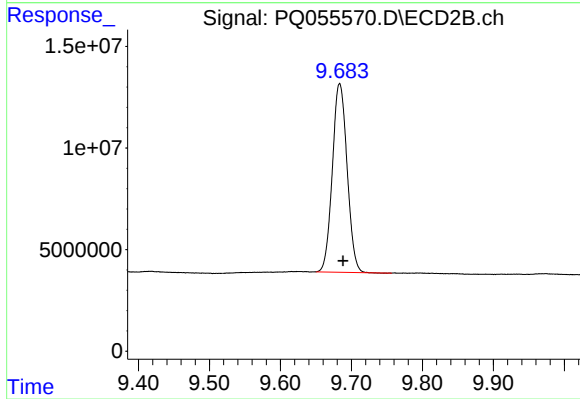

#2 Decachlorobiphenyl

R.T.: 9.684 min
Delta R.T.: -0.005 min
Response: 133837508
Conc: 18.01 ng/ml