

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ010522\
 Data File : PQ055594.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2022 19:09
 Operator : AJ\MA
 Sample : PB141843BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 PB141843BL

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/06/2022
 Supervised By :mohammad ahmed 01/06/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 06 05:14:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ010422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 04 15:29:13 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.239	4.305	267.0E6	220.9E6	23.262	22.949
2) SA Decachlor...	11.423	9.682	352.4E6	169.5E6	23.631m	22.813m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ010522\
Data File : PQ055594.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2022 19:09
Operator : AJ\MA
Sample : PB141843BL
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
PB141843BL


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/06/2022
Supervised By :mohammad ahmed 01/06/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 06 05:14:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ010422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 04 15:29:13 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

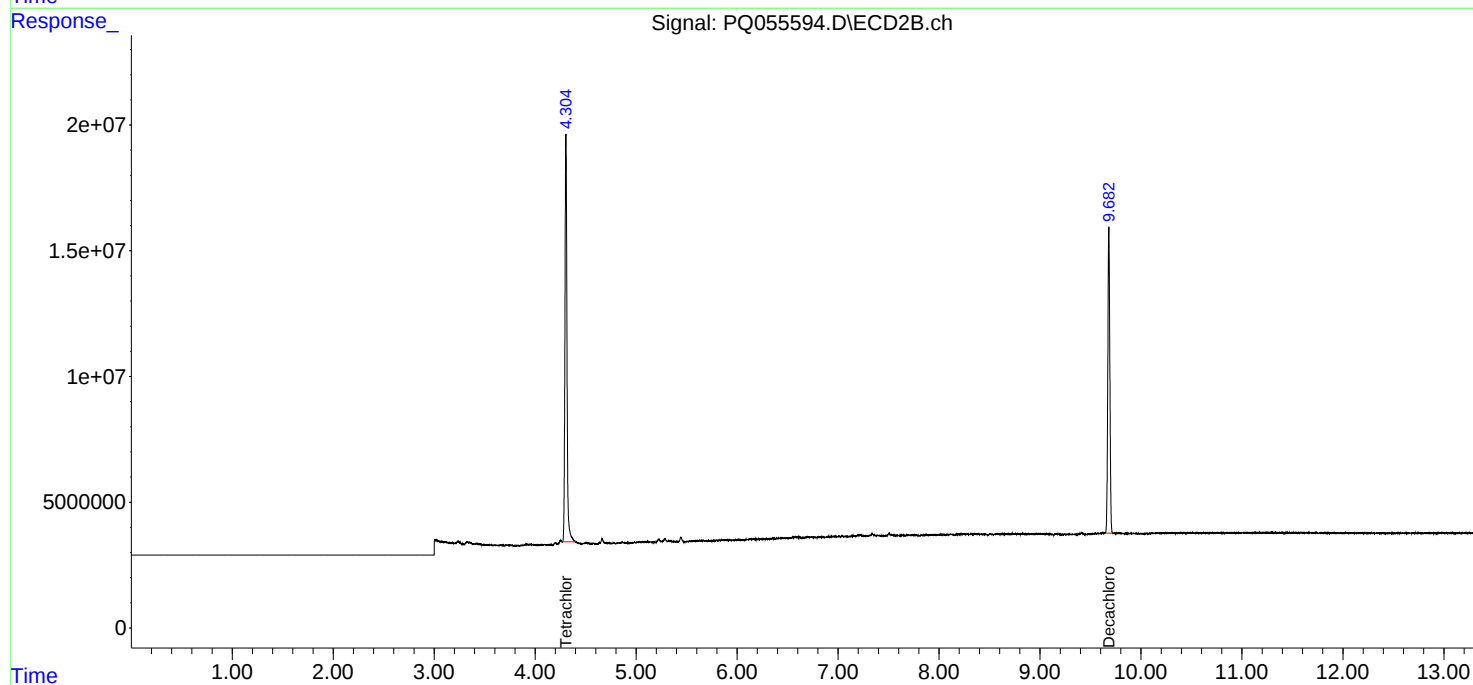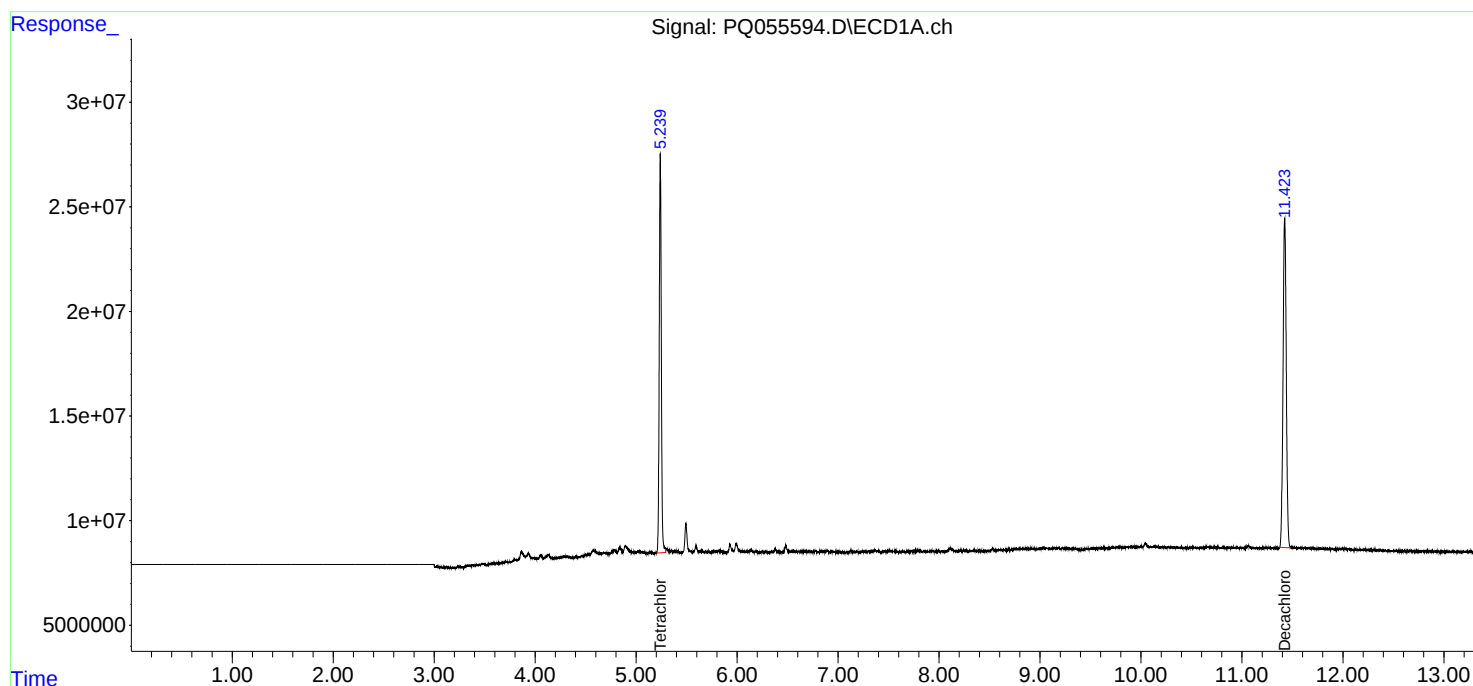

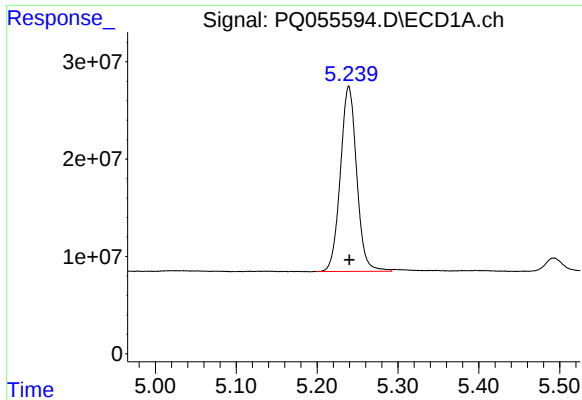


#1 Tetrachloro-m-xylene

R.T.: 5.239 min
Delta R.T.: 0.000 min
Response: 267020604
Conc: 23.26 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PB141843BL


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/06/2022
Supervised By :mohammad ahmed 01/06/2022

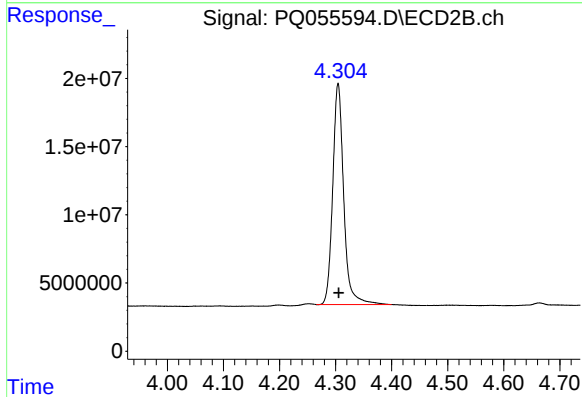


#1 Tetrachloro-m-xylene

R.T.: 4.305 min
Delta R.T.: -0.001 min
Response: 220888413
Conc: 22.95 ng/ml

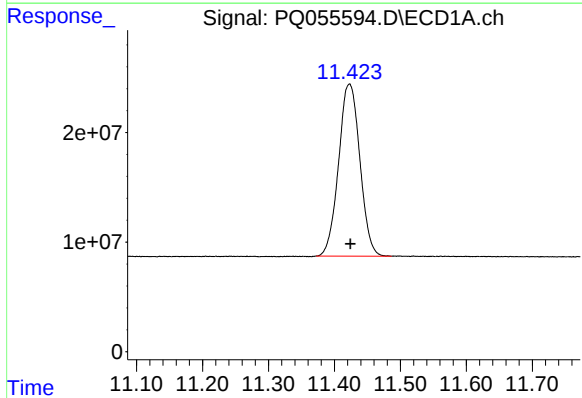

#2 Decachlorobiphenyl

R.T.: 11.423 min
Delta R.T.: -0.001 min
Response: 352418756
Conc: 23.63 ng/ml m

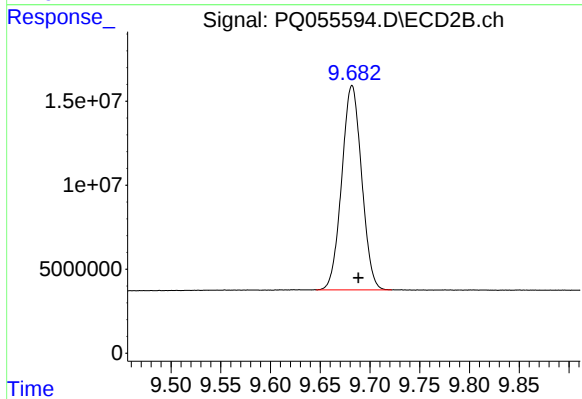

#2 Decachlorobiphenyl

R.T.: 9.682 min
Delta R.T.: -0.007 min
Response: 169533176
Conc: 22.81 ng/ml m