

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ010622\
 Data File : PQ055632.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jan 2022 20:05
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/07/2022
 Supervised By :mohammad ahmed 01/10/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 03:16:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ010422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 04 15:29:13 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.232	4.295	252.1E6	199.5E6	21.960	20.727
2) SA Decachlor...	11.418	9.673	249.2E6	132.0E6	16.712m	17.758m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ010622\
Data File : PQ055632.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jan 2022 20:05
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/07/2022
Supervised By :mohammad ahmed 01/10/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 03:16:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ010422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 04 15:29:13 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

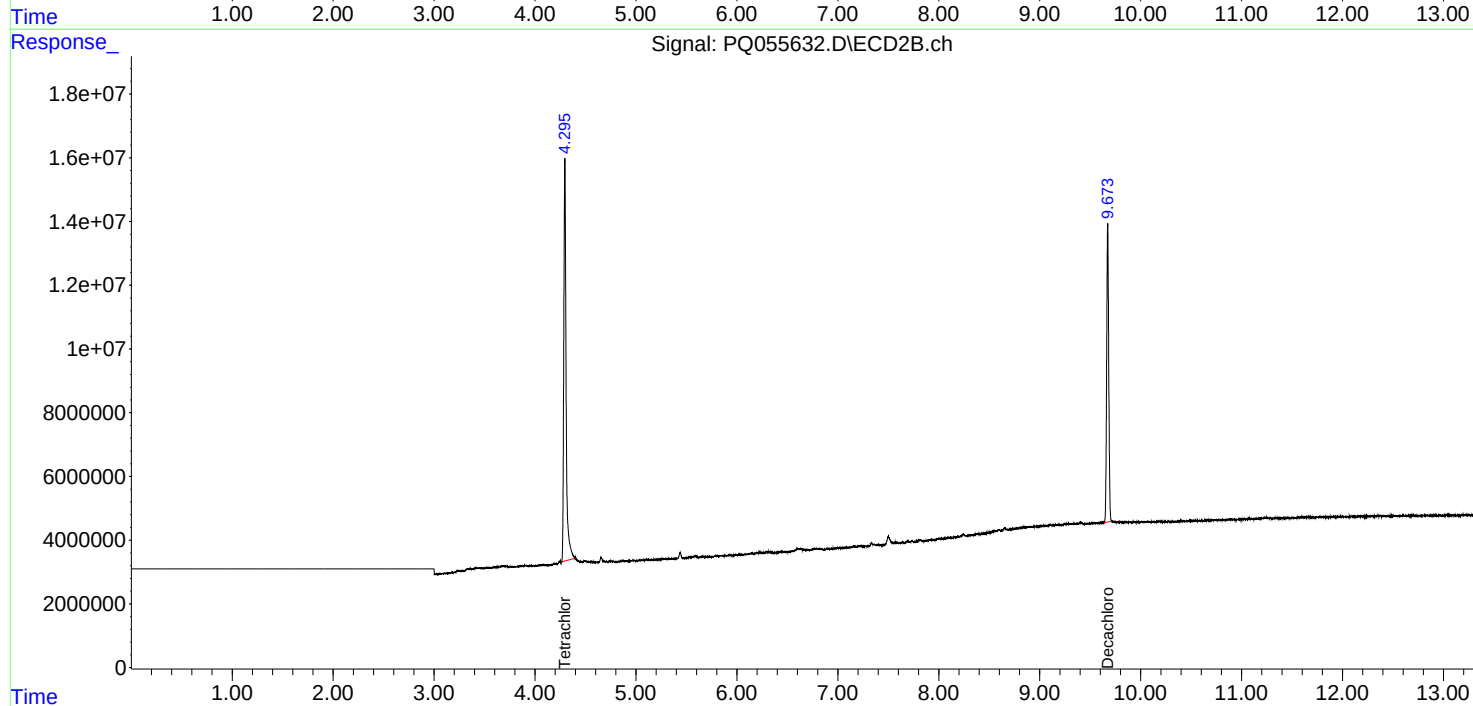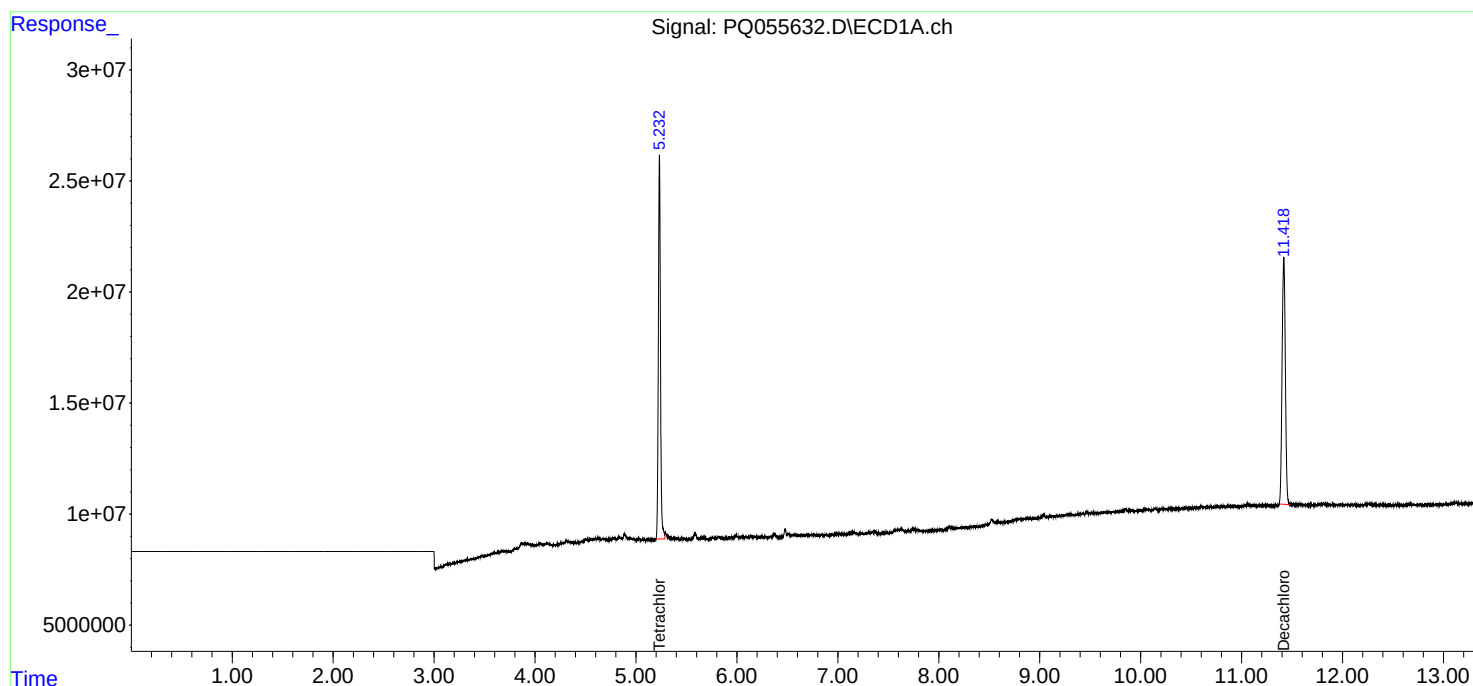

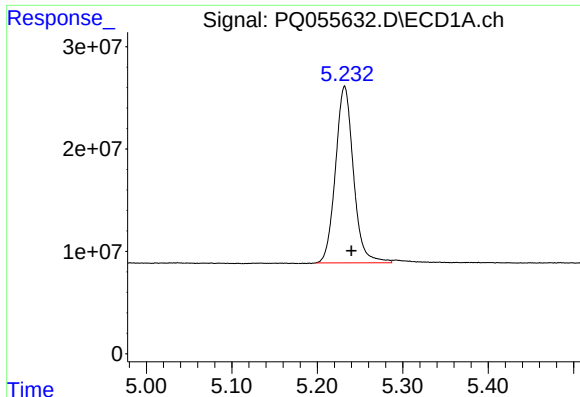


#1 Tetrachloro-m-xylene

R.T.: 5.232 min
Delta R.T.: -0.008 min
Response: 252073528
Conc: 21.96 ng/ml

Instrument :
ECD_Q
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/07/2022
Supervised By :mohammad ahmed 01/10/2022

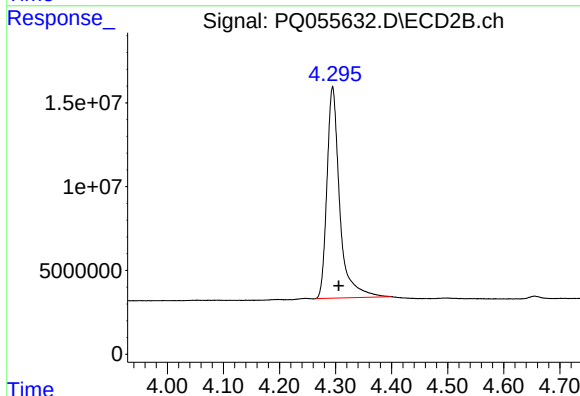


#1 Tetrachloro-m-xylene

R.T.: 4.295 min
Delta R.T.: -0.011 min
Response: 199496910
Conc: 20.73 ng/ml

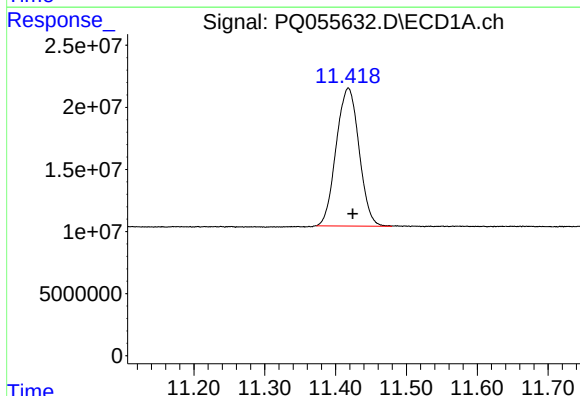

#2 Decachlorobiphenyl

R.T.: 11.418 min
Delta R.T.: -0.006 min
Response: 249231917
Conc: 16.71 ng/ml m

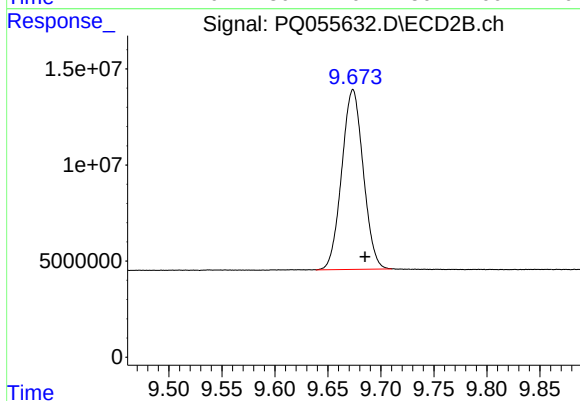

#2 Decachlorobiphenyl

R.T.: 9.673 min
Delta R.T.: -0.012 min
Response: 131972387
Conc: 17.76 ng/ml m