

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ011222\
 Data File : PQ055672.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jan 2022 21:10
 Operator : AJ\MA
 Sample : N1097-16
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 TP-3D

Manual Integrations
 APPROVED

Reviewed By :Ankita
 Jodhani

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 02:27:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ010422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 04 15:29:13 2022
 Response via : Initial Calibration
 Integrator: ChemStation

01/13/2022
 Supervised By :mohammad
 ahmed

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	01/13/2022
----------	------	------	--------	--------	-------	-------	------------

System Monitoring Compounds

1) SA Tetrachlo...	5.233	4.295	314.6E6	250.9E6	27.406m	26.064
2) SA Decachlor...	11.416	9.670	299.1E6	151.6E6	20.057	20.405

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ011222\
Data File : PQ055672.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jan 2022 21:10
Operator : AJ\MA
Sample : N1097-16
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
TP-3D



Manual Integrations
APPROVED


Reviewed By :Ankita
Jodhani

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 02:27:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ010422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 04 15:29:13 2022
Response via : Initial Calibration
Integrator: ChemStation

01/13/2022
Supervised By :mohammad
ahmed

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

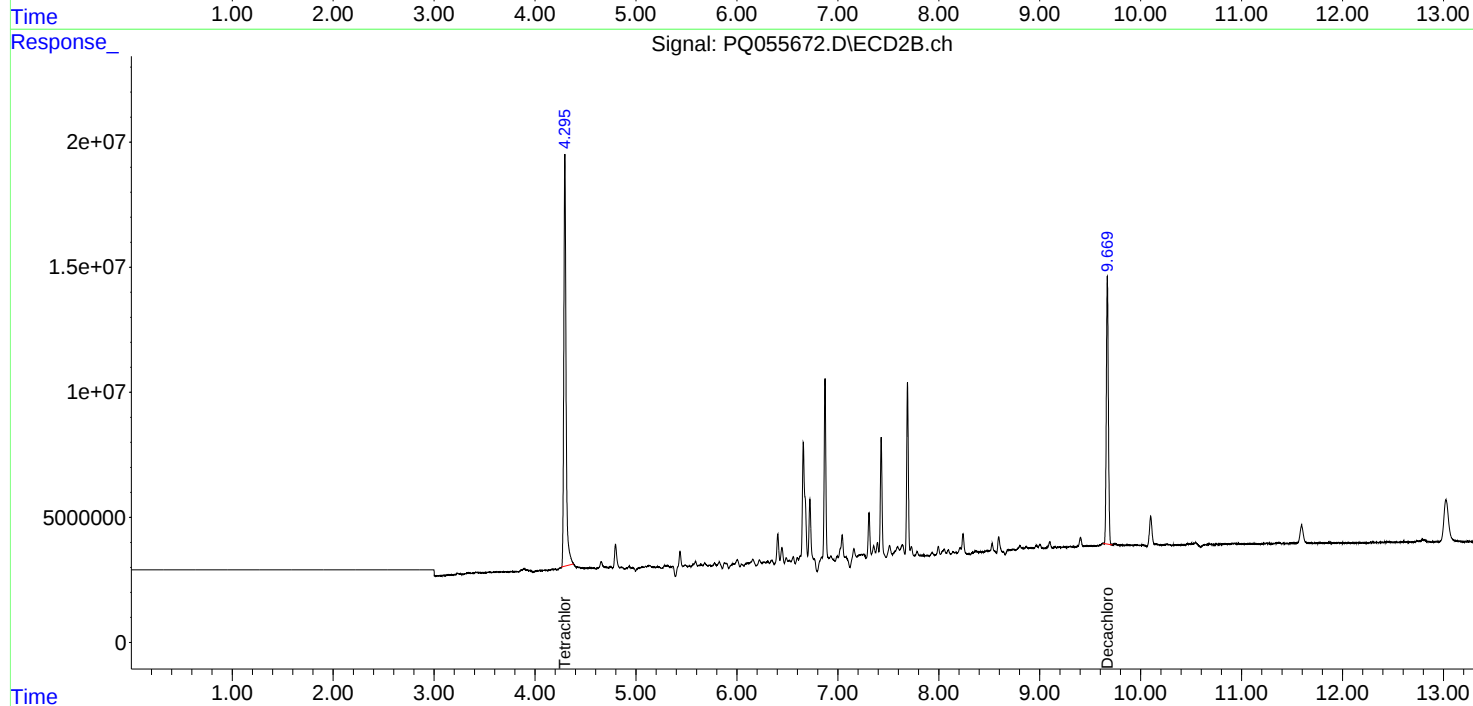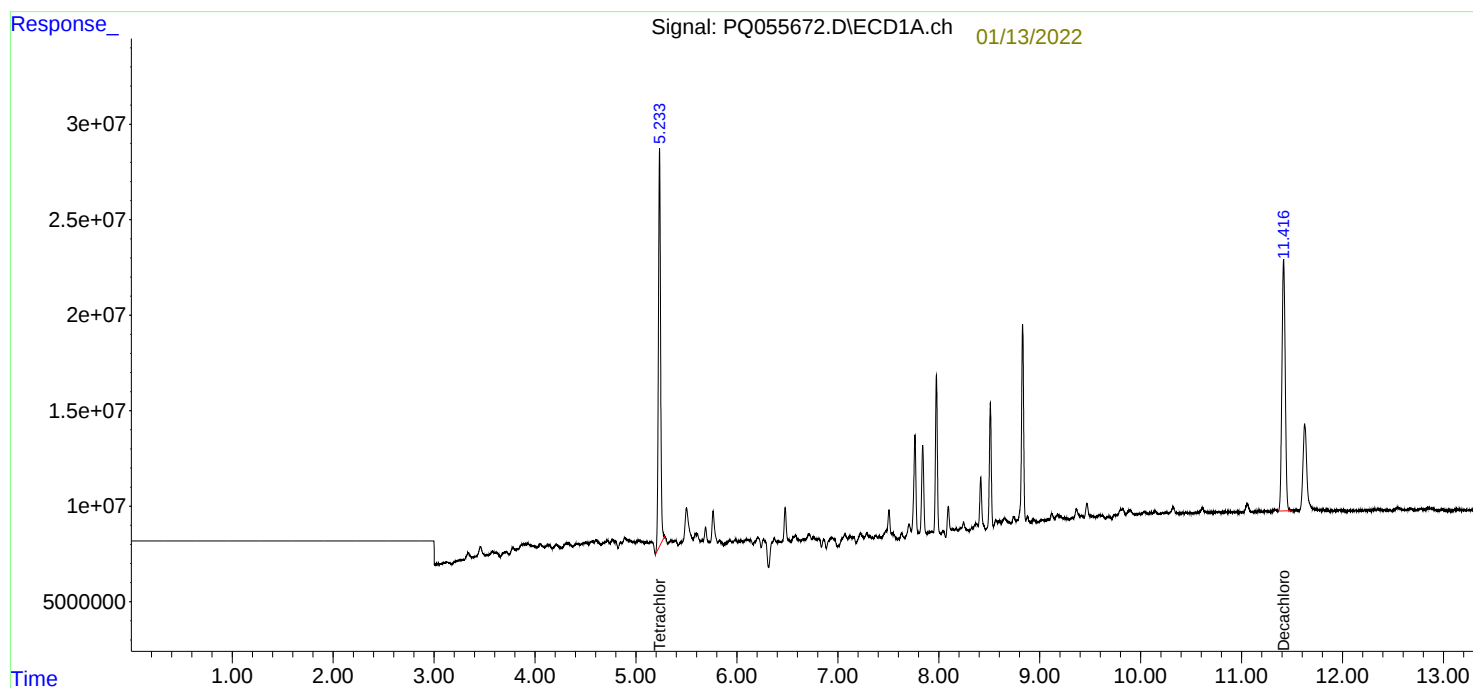

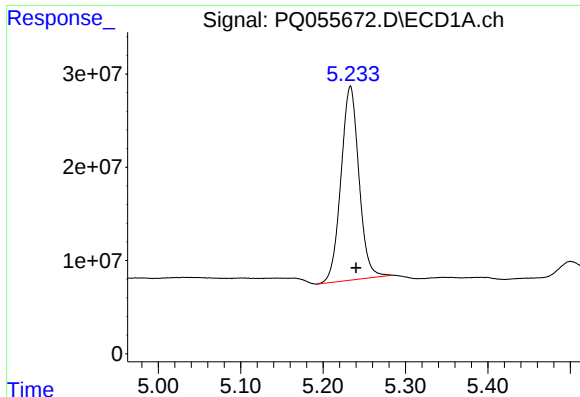


#1 Tetrachloro-m-xylene

R.T.: 5.233 min
Delta R.T.: -0.007 min
Response: 314592701
Conc: 27.41 ng/ml

Instrument :
ECD_Q
ClientSampleId :
TP-3D

Manual Integrations
APPROVED

Reviewed By :Ankita
Jodhani

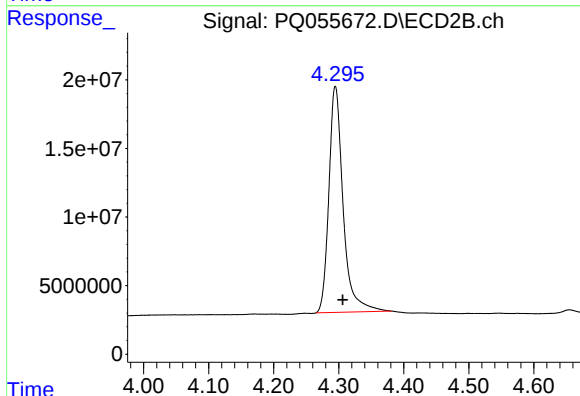


#1 Tetrachloro-m-xylene

R.T.: 4.295 min
Delta R.T.: -0.011 min
Response: 250865014
Conc: 26.06 ng/ml


01/13/2022
Supervised By :mohammad
ahmed

01/13/2022

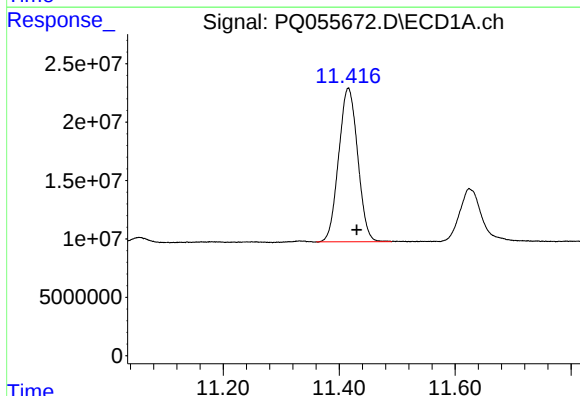

#2 Decachlorobiphenyl

R.T.: 11.416 min
Delta R.T.: -0.014 min
Response: 299112970
Conc: 20.06 ng/ml

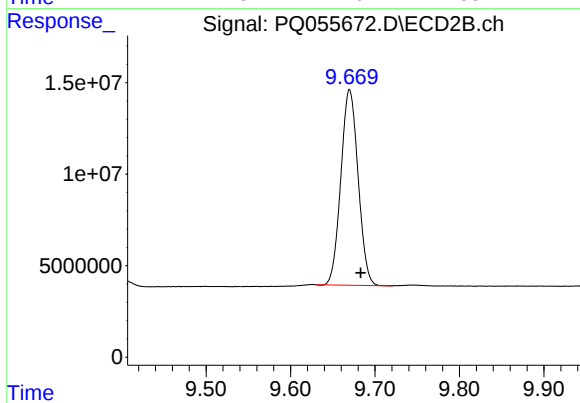

#2 Decachlorobiphenyl

R.T.: 9.670 min
Delta R.T.: -0.013 min
Response: 151640800
Conc: 20.40 ng/ml