

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ011222\
 Data File : PQ055678.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jan 2022 22:47
 Operator : AJ\MA
 Sample : N1099-05
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 VACLOT-BACKFILL-TILCON-05

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 02:30:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ010422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 04 15:29:13 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.233	4.295	303.5E6	240.6E6	26.443	25.001
2)	SA Decachlor...	11.416	9.669	239.3E6	117.7E6	16.045	15.837

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ011222\
Data File : PQ055678.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jan 2022 22:47
Operator : AJ\MA
Sample : N1099-05
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
VACLOT-BACKFILL-TILCON-05

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 02:30:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ010422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 04 15:29:13 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

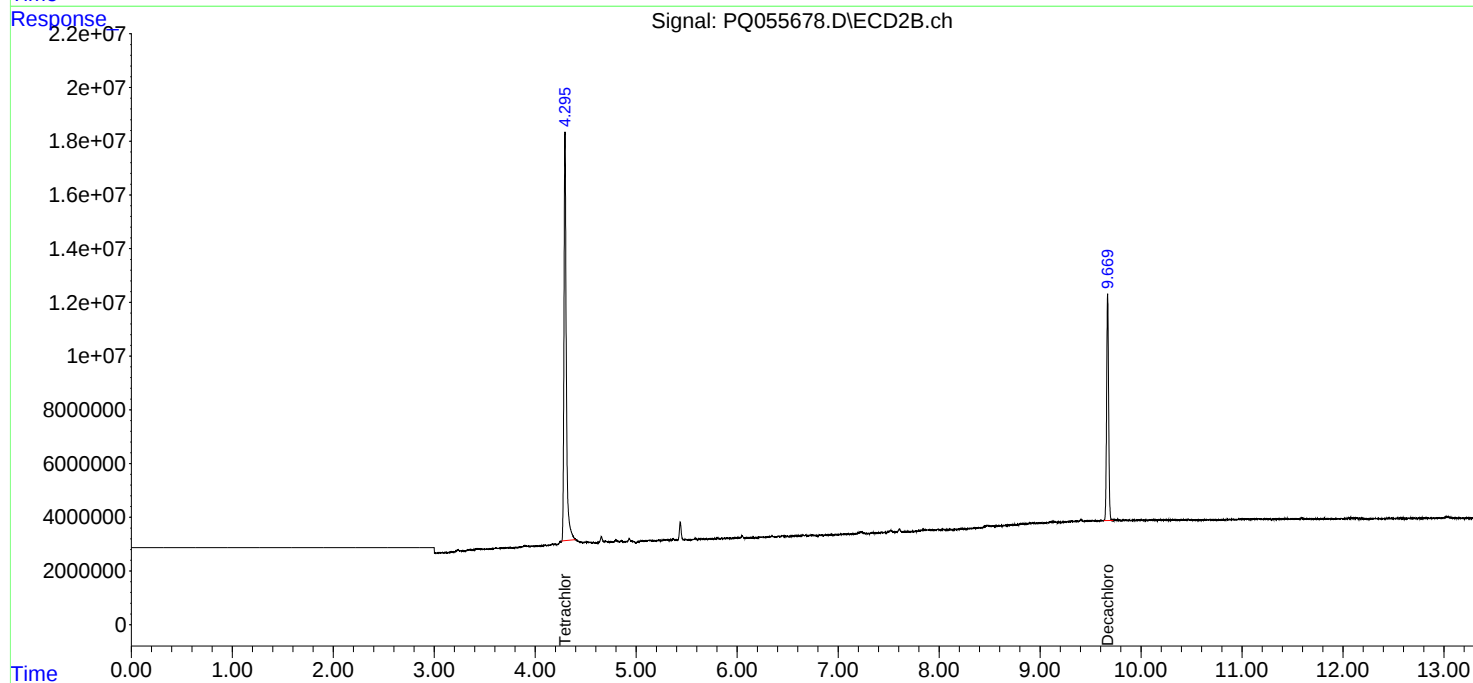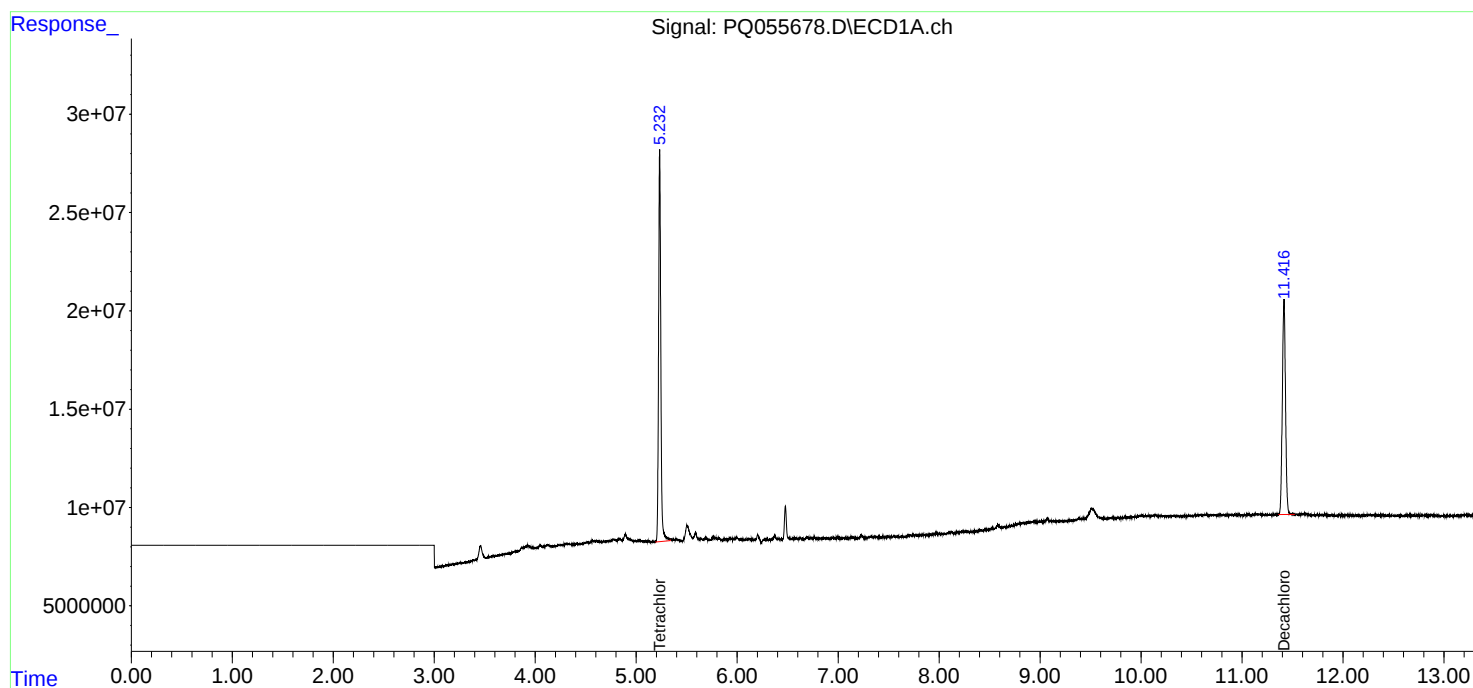


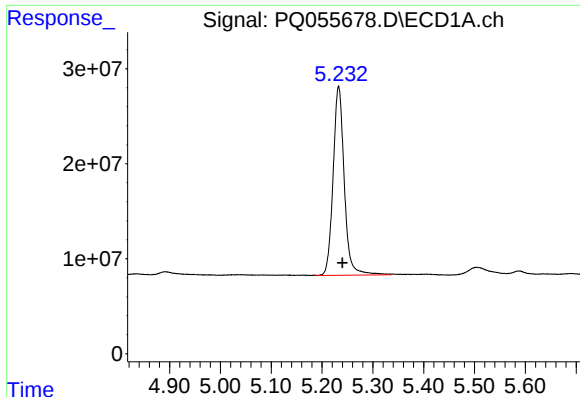

#1 Tetrachloro-m-xylene


R.T.: 5.233 min
Delta R.T.: -0.007 min
Response: 303533740
Conc: 26.44 ng/ml

Instrument :
ECD_Q
ClientSampleId :
VACLOT-BACKFILL-TILCON-05

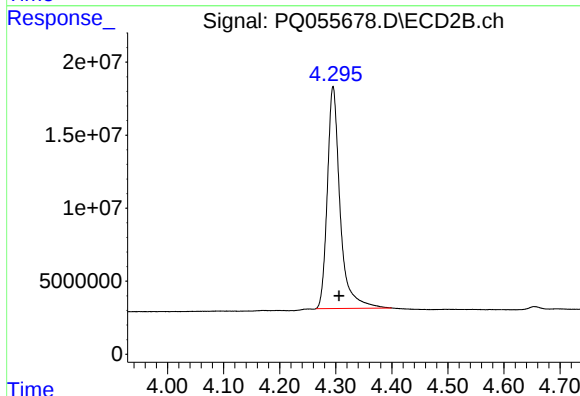


#1 Tetrachloro-m-xylene

R.T.: 4.295 min
Delta R.T.: -0.011 min
Response: 240636958
Conc: 25.00 ng/ml

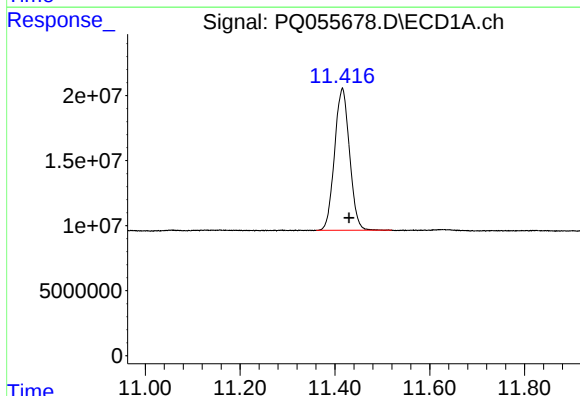

#2 Decachlorobiphenyl

R.T.: 11.416 min
Delta R.T.: -0.014 min
Response: 239286991
Conc: 16.05 ng/ml

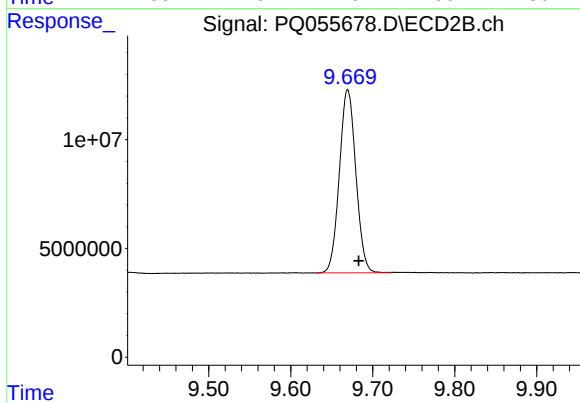

#2 Decachlorobiphenyl

R.T.: 9.669 min
Delta R.T.: -0.014 min
Response: 117696375
Conc: 15.84 ng/ml