

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ011222\
 Data File : PQ055687.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jan 2022 01:46
 Operator : AJ\MA
 Sample : N1099-09
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 VACLOT-BACKFILL-TILCON-09

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 05:07:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ010422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 04 15:29:13 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.233	4.298	298.1E6	236.5E6	25.973	24.571
2)	SA Decachlor...	11.416	9.669	331.1E6	163.6E6	22.200	22.010

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ011222\
Data File : PQ055687.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jan 2022 01:46
Operator : AJ\MA
Sample : N1099-09
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
VACLOT-BACKFILL-TILCON-09

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 05:07:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ010422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 04 15:29:13 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

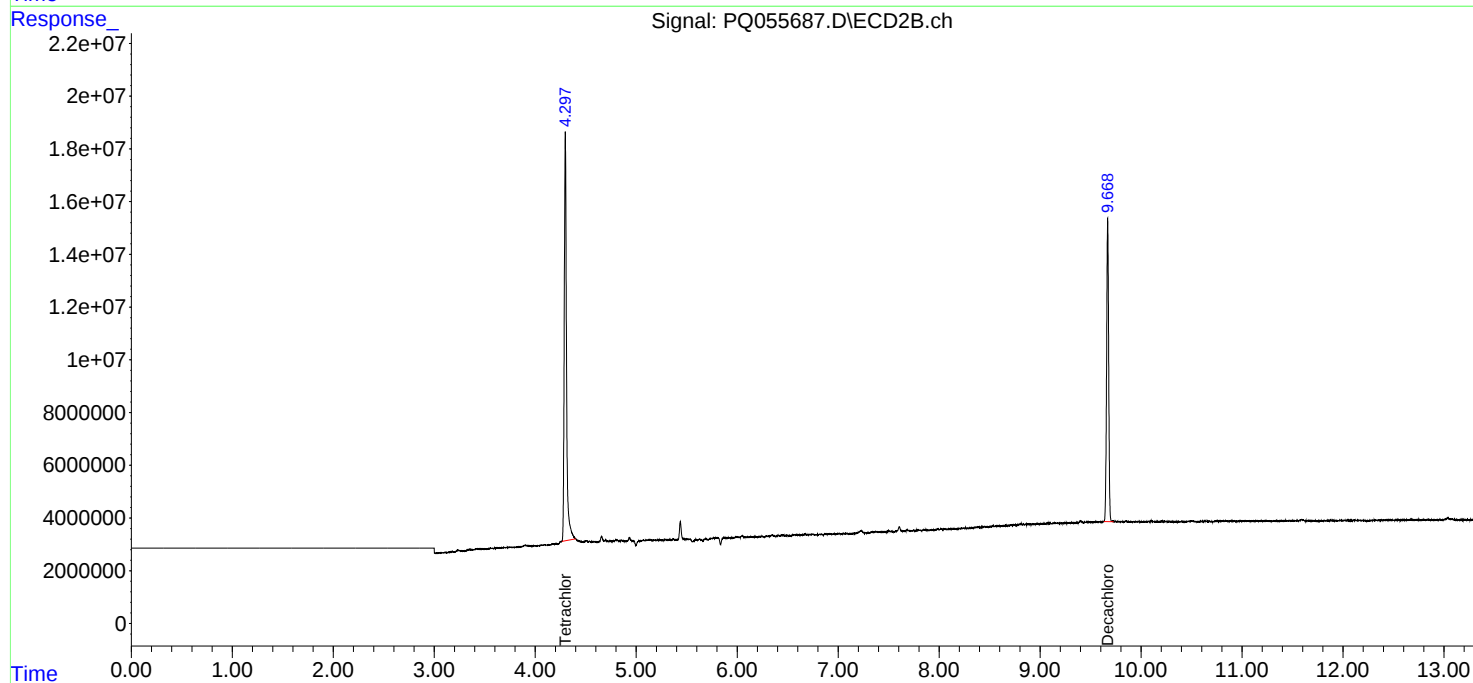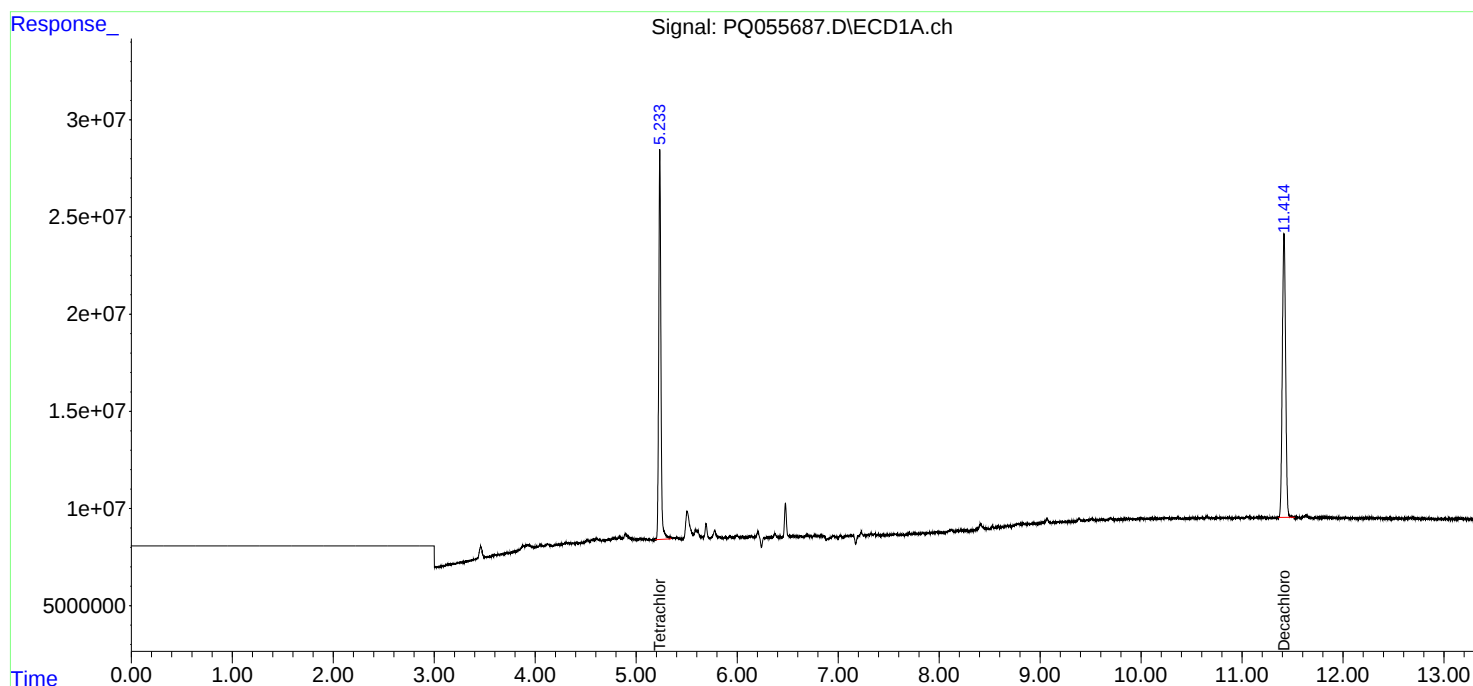


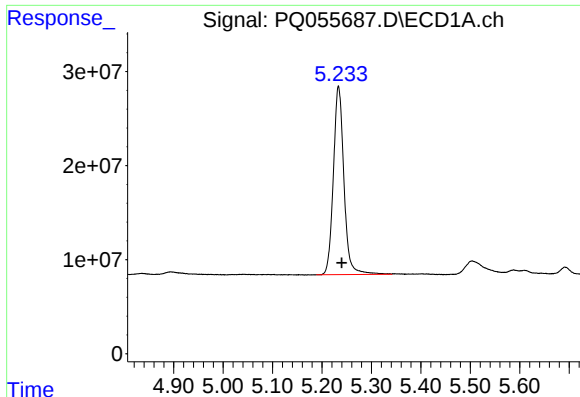

#1 Tetrachloro-m-xylene


R.T.: 5.233 min
Delta R.T.: -0.007 min
Response: 298139289
Conc: 25.97 ng/ml

Instrument :
ECD_Q
ClientSampleId :
VACLOT-BACKFILL-TILCON-09

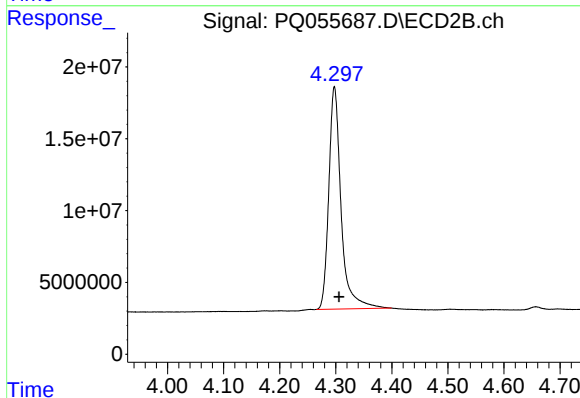


#1 Tetrachloro-m-xylene

R.T.: 4.298 min
Delta R.T.: -0.008 min
Response: 236496849
Conc: 24.57 ng/ml

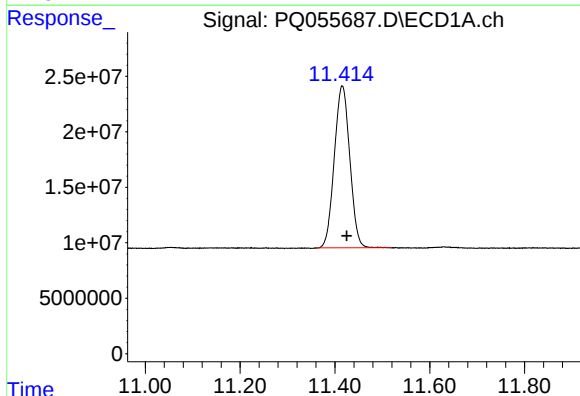

#2 Decachlorobiphenyl

R.T.: 11.416 min
Delta R.T.: -0.010 min
Response: 331077312
Conc: 22.20 ng/ml

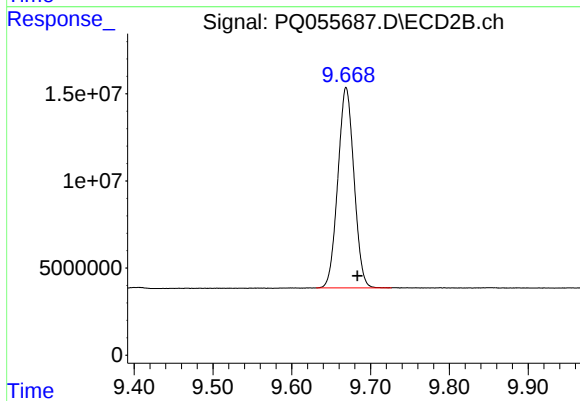

#2 Decachlorobiphenyl

R.T.: 9.669 min
Delta R.T.: -0.014 min
Response: 163570261
Conc: 22.01 ng/ml