

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ011822\
 Data File : PQ055770.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2022 12:51
 Operator : AJ\MA
 Sample : N1162-29 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 MMO-16-2022-B

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/19/2022
 Supervised By :Ankita Jodhani 01/19/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 00:29:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ010422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 04 15:29:13 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.234	4.300	23564550	15201444	2.053m	1.579
2) SA Decachlor...	11.415	9.667	23080556	10650374	1.548m	1.433m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ011822\
Data File : PQ055770.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2022 12:51
Operator : AJ\MA
Sample : N1162-29 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
MMO-16-2022-B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/19/2022
Supervised By :Ankita Jodhani 01/19/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 00:29:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ010422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 04 15:29:13 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

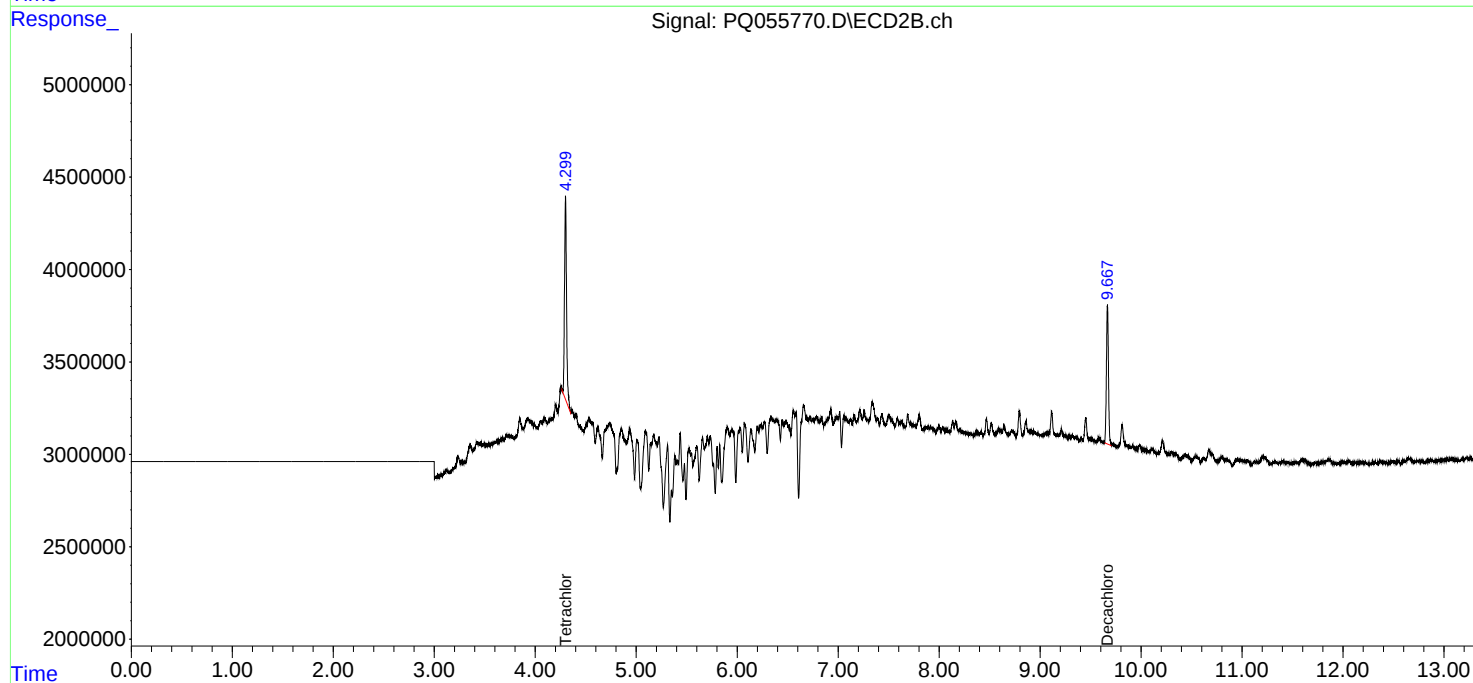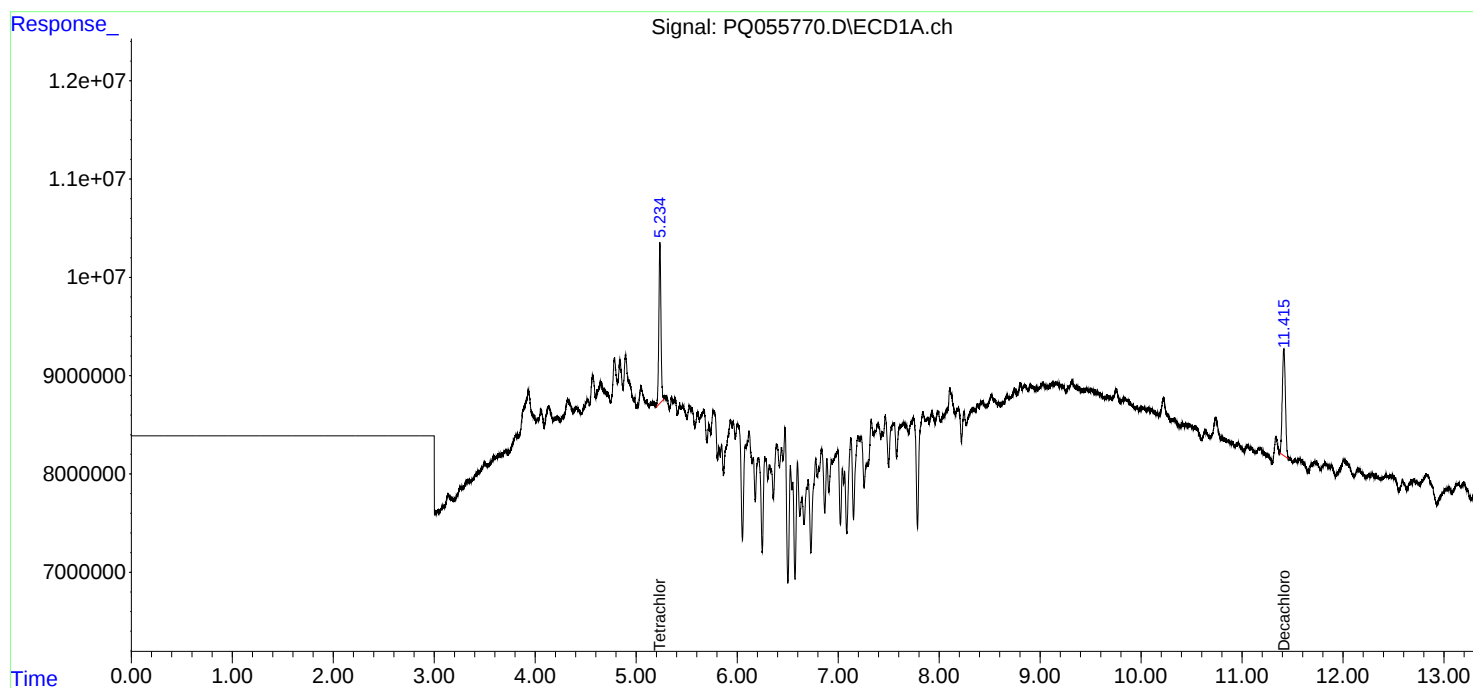

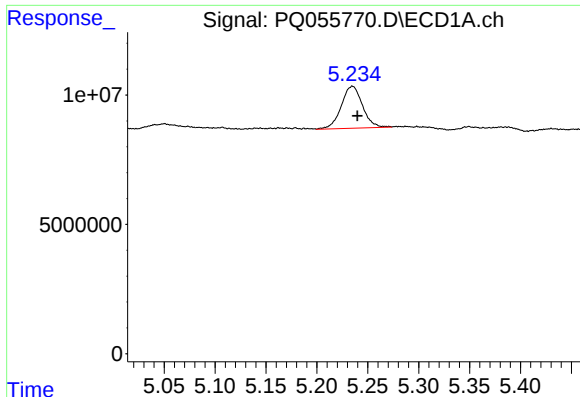


#1 Tetrachloro-m-xylene

R.T.: 5.234 min
Delta R.T.: -0.006 min
Response: 23564550
Conc: 2.05 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MMO-16-2022-B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/19/2022
Supervised By :Ankita Jodhani 01/19/2022

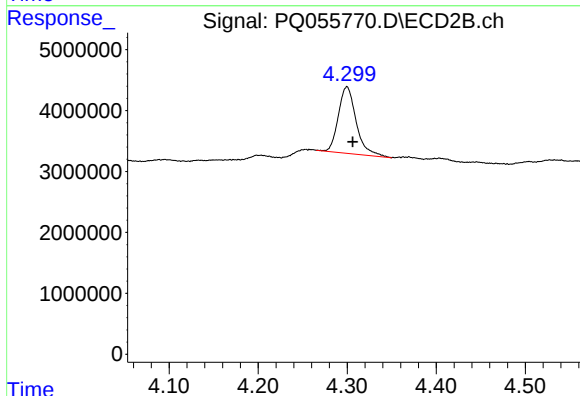


#1 Tetrachloro-m-xylene

R.T.: 4.300 min
Delta R.T.: -0.006 min
Response: 15201444
Conc: 1.58 ng/ml

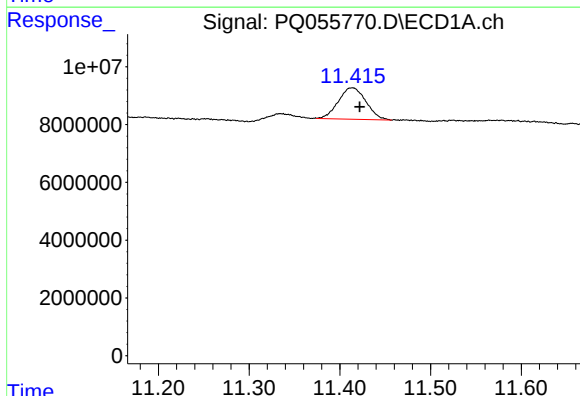

#2 Decachlorobiphenyl

R.T.: 11.415 min
Delta R.T.: -0.007 min
Response: 23080556
Conc: 1.55 ng/ml m

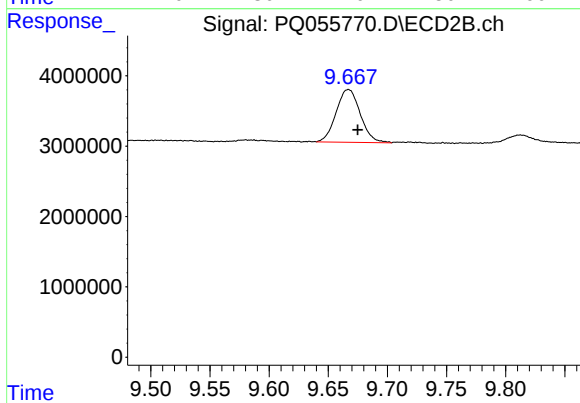

#2 Decachlorobiphenyl

R.T.: 9.667 min
Delta R.T.: -0.008 min
Response: 10650374
Conc: 1.43 ng/ml m