

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ012022\
 Data File : PQ055816.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2022 10:04
 Operator : AJ\MA
 Sample : N1099-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 VACLOT-BACKFILL-TILCON-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 01:50:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ011922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 20 13:18:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.238	4.298	291.1E6	231.7E6	21.495	20.608
2)	SA Decachlor...	11.420	9.663	316.6E6	162.5E6	21.687	20.375

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ012022\
Data File : PQ055816.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2022 10:04
Operator : AJ\MA
Sample : N1099-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
VACLOT-BACKFILL-TILCON-03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 01:50:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ011922.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 20 13:18:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

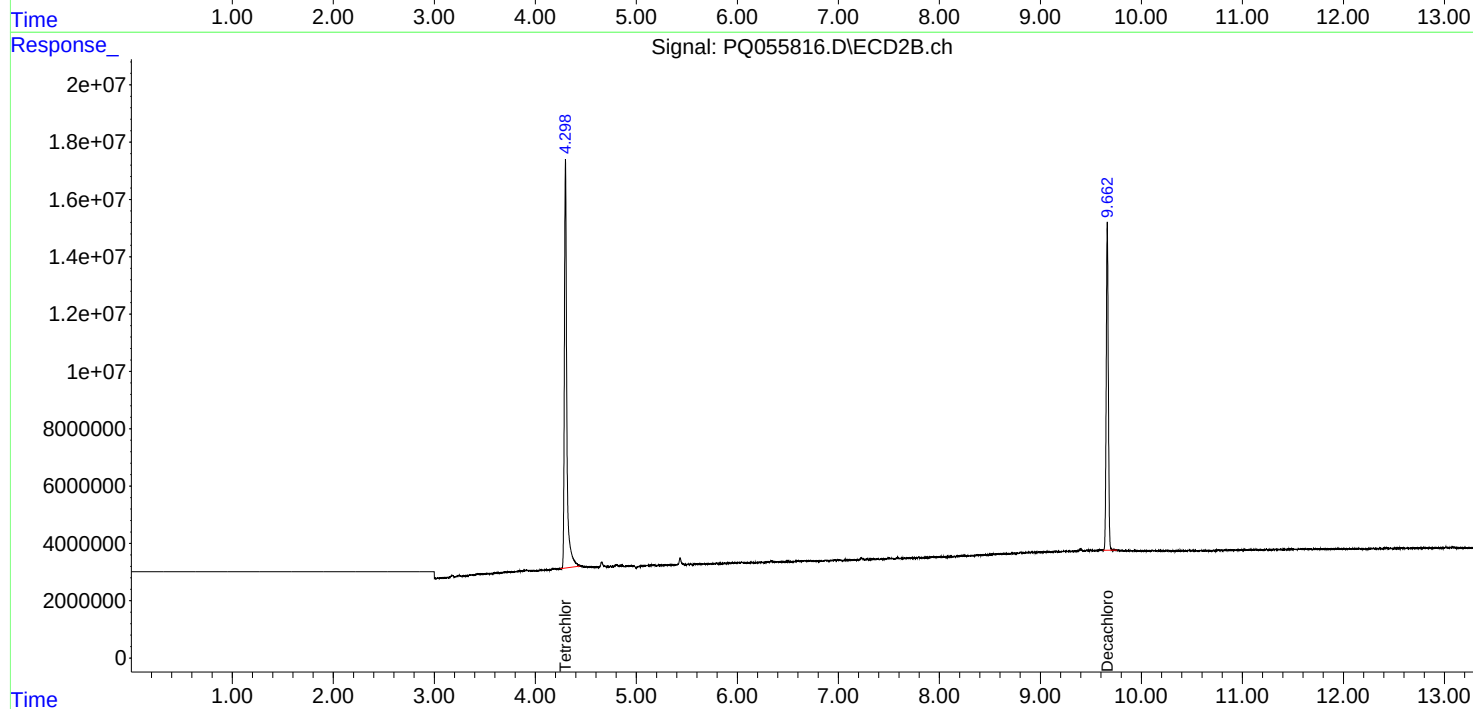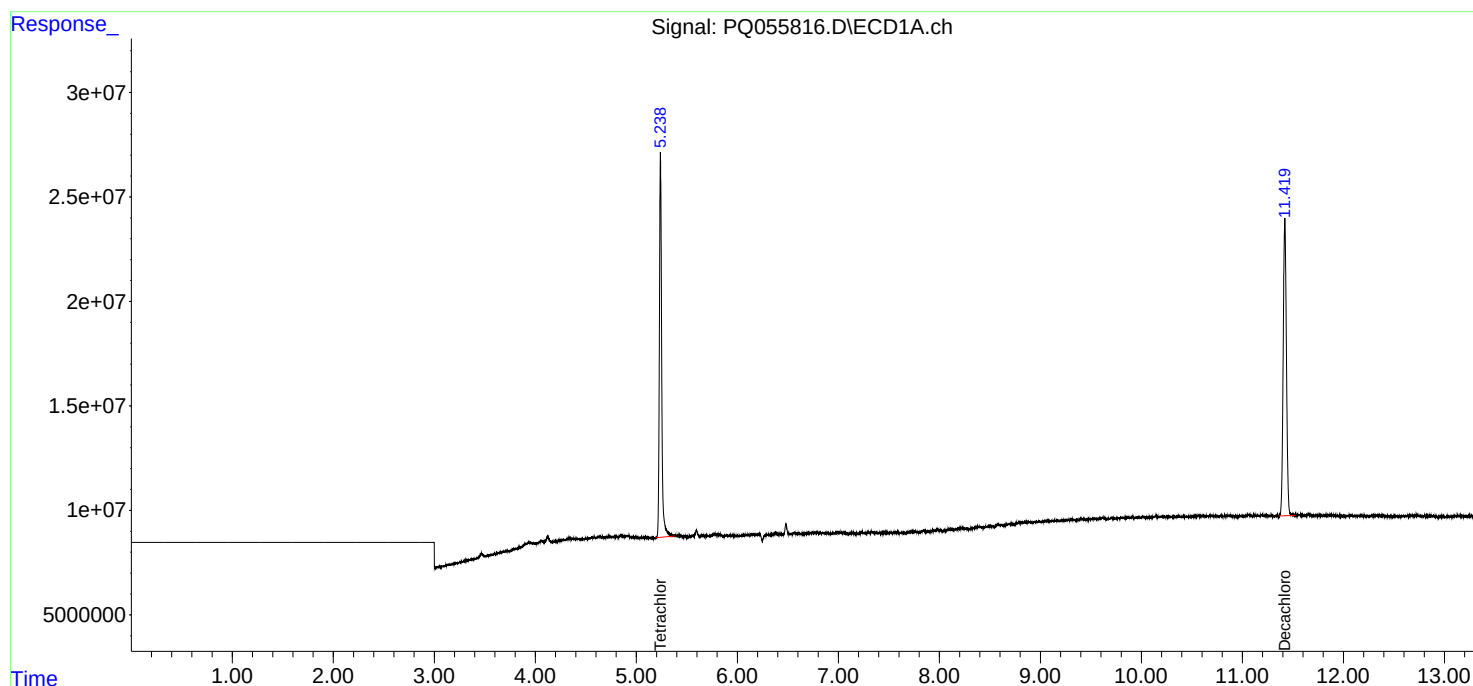


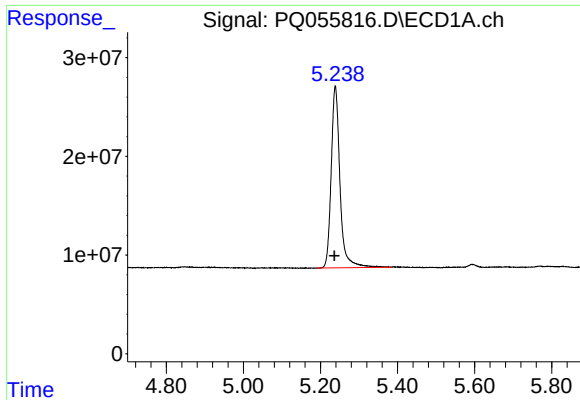

#1 Tetrachloro-m-xylene


R.T.: 5.238 min
Delta R.T.: 0.002 min
Response: 291122995
Conc: 21.49 ng/ml

Instrument :
ECD_Q
ClientSampleId :
VACLOT-BACKFILL-TILCON-03

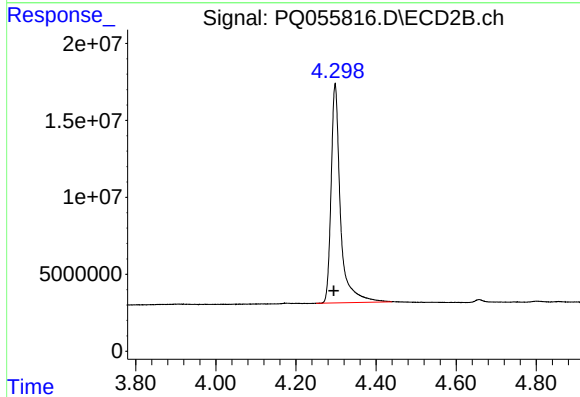


#1 Tetrachloro-m-xylene

R.T.: 4.298 min
Delta R.T.: 0.004 min
Response: 231715951
Conc: 20.61 ng/ml

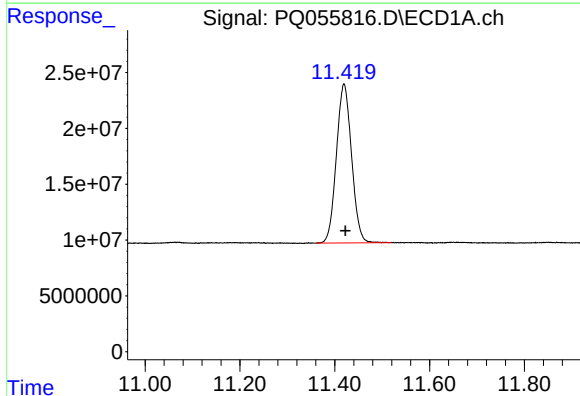

#2 Decachlorobiphenyl

R.T.: 11.420 min
Delta R.T.: -0.002 min
Response: 316607952
Conc: 21.69 ng/ml

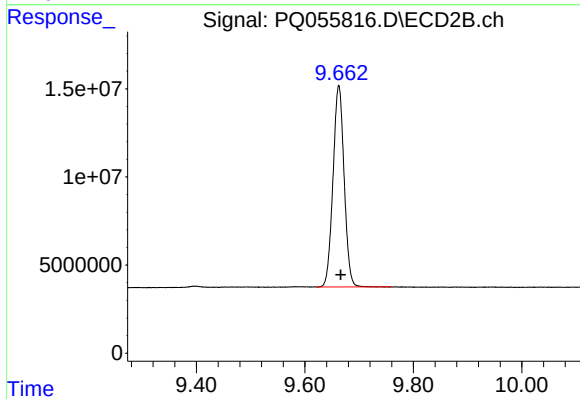

#2 Decachlorobiphenyl

R.T.: 9.663 min
Delta R.T.: -0.004 min
Response: 162496498
Conc: 20.38 ng/ml